A-A-51848A
21 February 1989
SUPERSEDING
A-A-0051848(DM)
12 March 1977

COMMERCIAL ITEM DESCRIPTION

FORCEPS, ELECTROCOAGULATION, BIPOLAR, 6 INCH (Malis)

The General Services Administration has authorized the use of this commercial item description.

This commercial item description covers a bipolar coagulation forceps of the Malis design used in microsurgical procedures involving cauterization of blood vessels through application of an electric current.

Salient characteristics:

General. The forceps shall be either a Type I (fine tip 0.5 mm wide) or Type II (extra fine tip 0.25 mm wide) forceps with tips which tapers to a fine rounded point. The handles shall have serrations to aid fingertip control. The proximal end shall have two prongs separated by an insulating material and shall be compatible with a power cord which connects the forceps to the power supply (See Note 2). The forceps shall be usable under irrigation fluids and in a bloody surgical field.

Material. The tips and handles shall be Ti6Al4 titanium in accordance with ASTM Designation B348, Grade 5. The base insulator shall be rigid plastic or epoxy.

Style, design and dimensions. The forceps shall be in accordance with Figure 1.

Finish. The metal portion of the forceps shall have a blue anodized finish over a base matte finish. The matte finish shall exhibit a uniform nondirectional surface texture equivalent to that produced by lightly glass bead-blasting the prepared surface with fine abrasives under pressure.

AMSC N/A FSC 6515

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:02Z
Check the source to verify that this is the current version before use.

Corrosion resistance. The forceps shall show no evidence of corrosion when repeatedly steam sterilized.

Performance. The tips shall meet exactly under visual or microscopic examination. The forceps including the base, shall be capable of repeated steam sterilization. The forceps shall be tested for continuity from connection prong to tip and for resistance from pin to pin and from pin to outside of insulator.

Identification marking and labeling. The forceps shall bear the contractor's name or registered trademark and the word "titanium". Forceps of foreign manufacture shall bear the name of the country of manufacture.

Workmanship. Forceps shall be processed in such a manner as to be uniform and free from cracks, pits, burrs, sharp edges, scale, rough areas, corrosion, grind or tool marks, and dirt or polishing materials.

Visual and dimensional examination. Forceps shall be examined to verify that design, construction and workmanship are in accordance with applicable requirements.

Materials. The supplier shall be responsible for performing tests to assure that materials are in accordance with requirements.

Unit. Each (EA). One forceps, as specified, constitutes one unit.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:02Z
Check the source to verify that this is the current version before use.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Sampling for examination. Sampling for examination shall be conducted in accordance with MIL-STD-105 and as specified herein. Unit of product for examination purposes shall be one forceps. Unit shall be level II with an and AQL of 1.0.

Examination. Examination shall be conducted to determine compliance with specification requirements.

Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and as specified herein. Unit of product for test purposes shall be one forceps. Sampling shall be level S-2 with an AQL of 1.0.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more test characteristics.

Contractor certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Metric products. Products manufactured to metric dimensions will be considered on an equal basis with those manufactured using inch-pound units, providing they fall within the tolerances specified using conversion tables contained in the latest revision of Federal Standard No. 376, and all other requirements of this document are met.

Source: https://assist.dla.mil -- Downloaded: 202610-26T09:02Z
Check the source to verify that this is the current version before use.

If a product is manufactured to metric dimensions and those dimensions exceed the tolerances specified in the inch/pound units, a request should be made to the contracting officer to determine if the product is acceptable.

The contracting officer has the option of accepting or rejecting the product.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Public Law 94-580, as amended, and as implemented by Federal Acquisition Regulation Subpart 23.4 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

NOTE1: The following National Stock Numbers are covered by this document:

NSN	TYPE	ITEM IDENTIFICATION
6515-01-139-7943	I	Forceps, Coagulation, Titanium, Fine Tip, Bipolar, Malis, 6 Inch
6515-01-139-7944	II	Forceps, Coagulation, Malis, Bipolar, Titanium, 6 Inch Long, Extra Fine Tip

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:02Z
Check the source to verify that this is the current version before use.

NOTE 2: The forceps are compatible with Cord, Coagulator, Bipolar, Malis, 144 inch, NSN 6515-01-139-7942, which is purportedly similar to Codman and Shurtleff Part Number 30-1536. This cord is a component of Coagulator, Microsurgical Unit, 110 volt, NSN 6515-01-210-9495 which, purportedly similar to Codman and Shurtleff Part Number 80-1114.

Ordering data (Intermediate/exterior package quantities, labeling, and marking must be specified in the contract and/or order).

MILITARY INTERESTS:

Custodians:

Army - MD
Navy - MS
Air Force - 03

PREPARING ACTIVITY:

DoD - MB

Agent:


DLA-DM

CIVIL AGENCY COORDINATING ACTIVITIES:

VA-OSS
PHS
PDA-MPQAS

Project No. 6515-4436

Source: https://assist.dla.mil -- Downloaded: 202640-26T09:02Z
Check the source to verify that this is the currentversion before use.

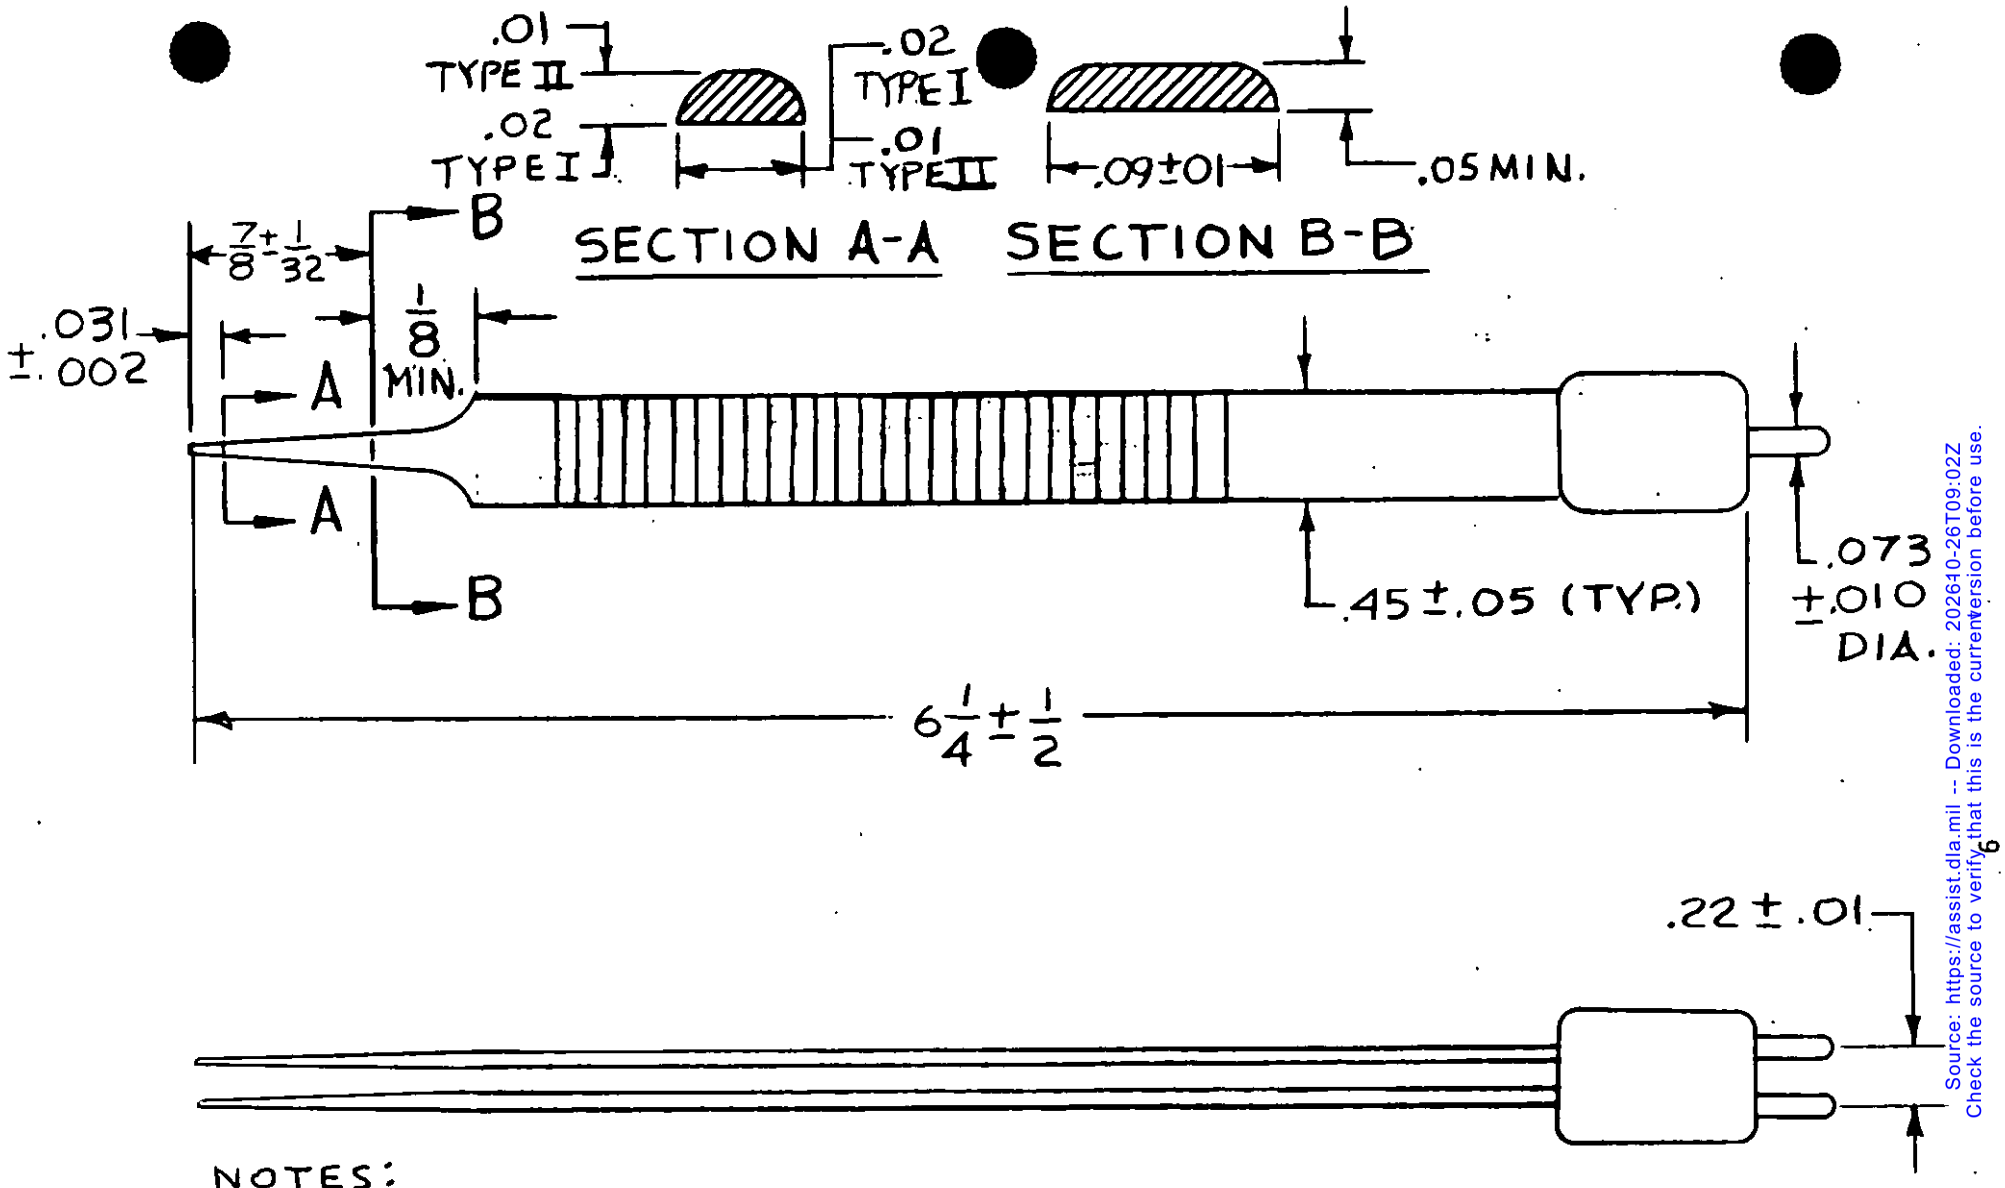

NOTES:

1. WIDTH OF ONE TIP SHALL BE WITHIN .001 OF THE OTHER
2. TIP SEPARATION .59 TO .69 IN FULLY OPEN POSITION.
3. ALL DIMENSIONS ARE INCHES.
4. DO NOT SCALE.

A-A-51848A

FIGURE 1 FORCEPS, COAGULATION, MALIS, 6 INCH

Source: https://assist.dla.mil -- Downloaded: 2026-02-26T09:02Z
Check the source to verify that this is the current version before use.