A-A-51863A
2 May 1989
SUPERSEDING
A-A-0051863(DM)
6 APRIL 1987

COMMERCIAL ITEM DESCRIPTION

HOOK, DURA (Dandy)

The General Services Administration has authorized the use of this commercial item description.

This commercial item description covers one size of a nerve hook of the Dandy design suitable for use in neurosurgical procedures.

Salient characteristics:

Classification. Hooks shall be of the following types, as specified:

Type I	-	Hook left
Type II	-	Straight
Type III	-	Hook right

Material. Hooks shall be manufactured from martensitic corrosion-resistant steel in accordance with American Society for Testing and Materials (ASTM) Designation F899.

Hardness. Hooks shall have a Rockwell Hardness C scale (HRC) of 48 to 53. As an alternate, hooks manufactured from material with a carbon content of less than 0.22% shall have a Rockwell Hardness C scale (HRC) of 45 minimum. The hardness shall be tested in accordance with ASTM Designation E18 or E92 whichever is applicable. Conversion of hardness values shall be tested in accordance with ASTM Designation E140.

Style and design. Hooks shall be in accordance with Figure 1 for the type specified. Hook tips shall be smoothly rounded.

Passivation. Hooks shall be properly passivated.

AMSC N/A FSC 6515

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:02Z
Check the source to verify that this is the current version before use.

Finish. The finish of the hooks shall be mirror or satin. The finish shall be uniform and free from burrs, chips, pits, rough areas, and grind or tool marks.

Identification markings. Hooks shall be permanently marked with the contractor's name or registered trademark and the word "stainless." In addition, hooks of foreign manufacture shall bear the name of the country of manufacture.

Corrosion resistance. Hooks shall show no signs of corrosion or copper plating when tested in accordance with ASTM Designation F1089.

Workmanship. The hooks shall be processed in such a manner as to be uniform and free from defects which affect life, utility, or appearance.

Product Quality Level

Visual and dimensional examination. Shall be examined to verify that design, construction and workmanship are in accordance with applicable requirements.

Materials. The supplier shall be responsible for performing tests to assure that materials are in accordance with requirements specified.

Unit. Each (EA). One hook of the type specified, constitutes one unit.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Source: https://assist.dla.mil -- Downloaded: 202640-26T09:02Z
Check the source to verify that this is the currentversion before use.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Examination. The hooks shall be examined to determine compliance with all requirements contained in this specification.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more test characteristics.

Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and as specified herein. The unit of product for test purposes shall be one hook. Sampling shall be level S-1, AQL 1.0.

Contractor certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producers' own drawings, specification, standard, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Metric products. Products manufactured to metric dimensions will be considered on an equal basis with those manufactured using inch-pound units, providing they fall within the tolerances specified using conversion tables contained in the latest revision of Federal Standard No. 376, and all other requirements of this document are met.

If a product is manufactured to metric dimensions and those dimensions exceed the tolerances specified in the inch/pound units, a request should be made to the contracting officer to determine if the product is acceptable.

The contracting officer has the option of accepting or rejecting the product.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:02Z
Check the source to verify that this is the current version before use.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Public Law 94-580, as amended and as implemented by Federal Acquisition Regulation Subpart 23.4 the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

NOTE: The following National Stock Numbers are covered by this document:

NSN	ITEM IDENTIFICATION	SPECIFICATION TYPE
6515-01-113-7147	HOOK, DURA, Dandy, Left, 8 Inch (20.32 cm)	I
6515-01-117-3900	HOOK, DURA, Dandy, Straight, 8 Inch (20.32 cm)	II
6515-01-117-7157	HOOK, DURA, Dandy, Right 8 Inch (20.32 cm)	III

Ordering data (Intermediate/exterior package quantities and labeling and marking must be specified in the contract and/or order).

Source: https://assist.dla.mil -- Downloaded: 202610-26T09:02Z
Check the source to verify that this is the current version before use.

MILITARY INTERESTS:

Custodians:

Army - MD
Navy - MS
Air Force - 03

Preparing Activity:

DoD-MB

Agent:

DLA-DM

CIVIL AGENCY COORDINATING ACTIVITIES:

VA-OSS
PHS
FDA-MPQAS

Project No. 6515-4588

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:02Z
Check the source to verify that this is the current version before use.

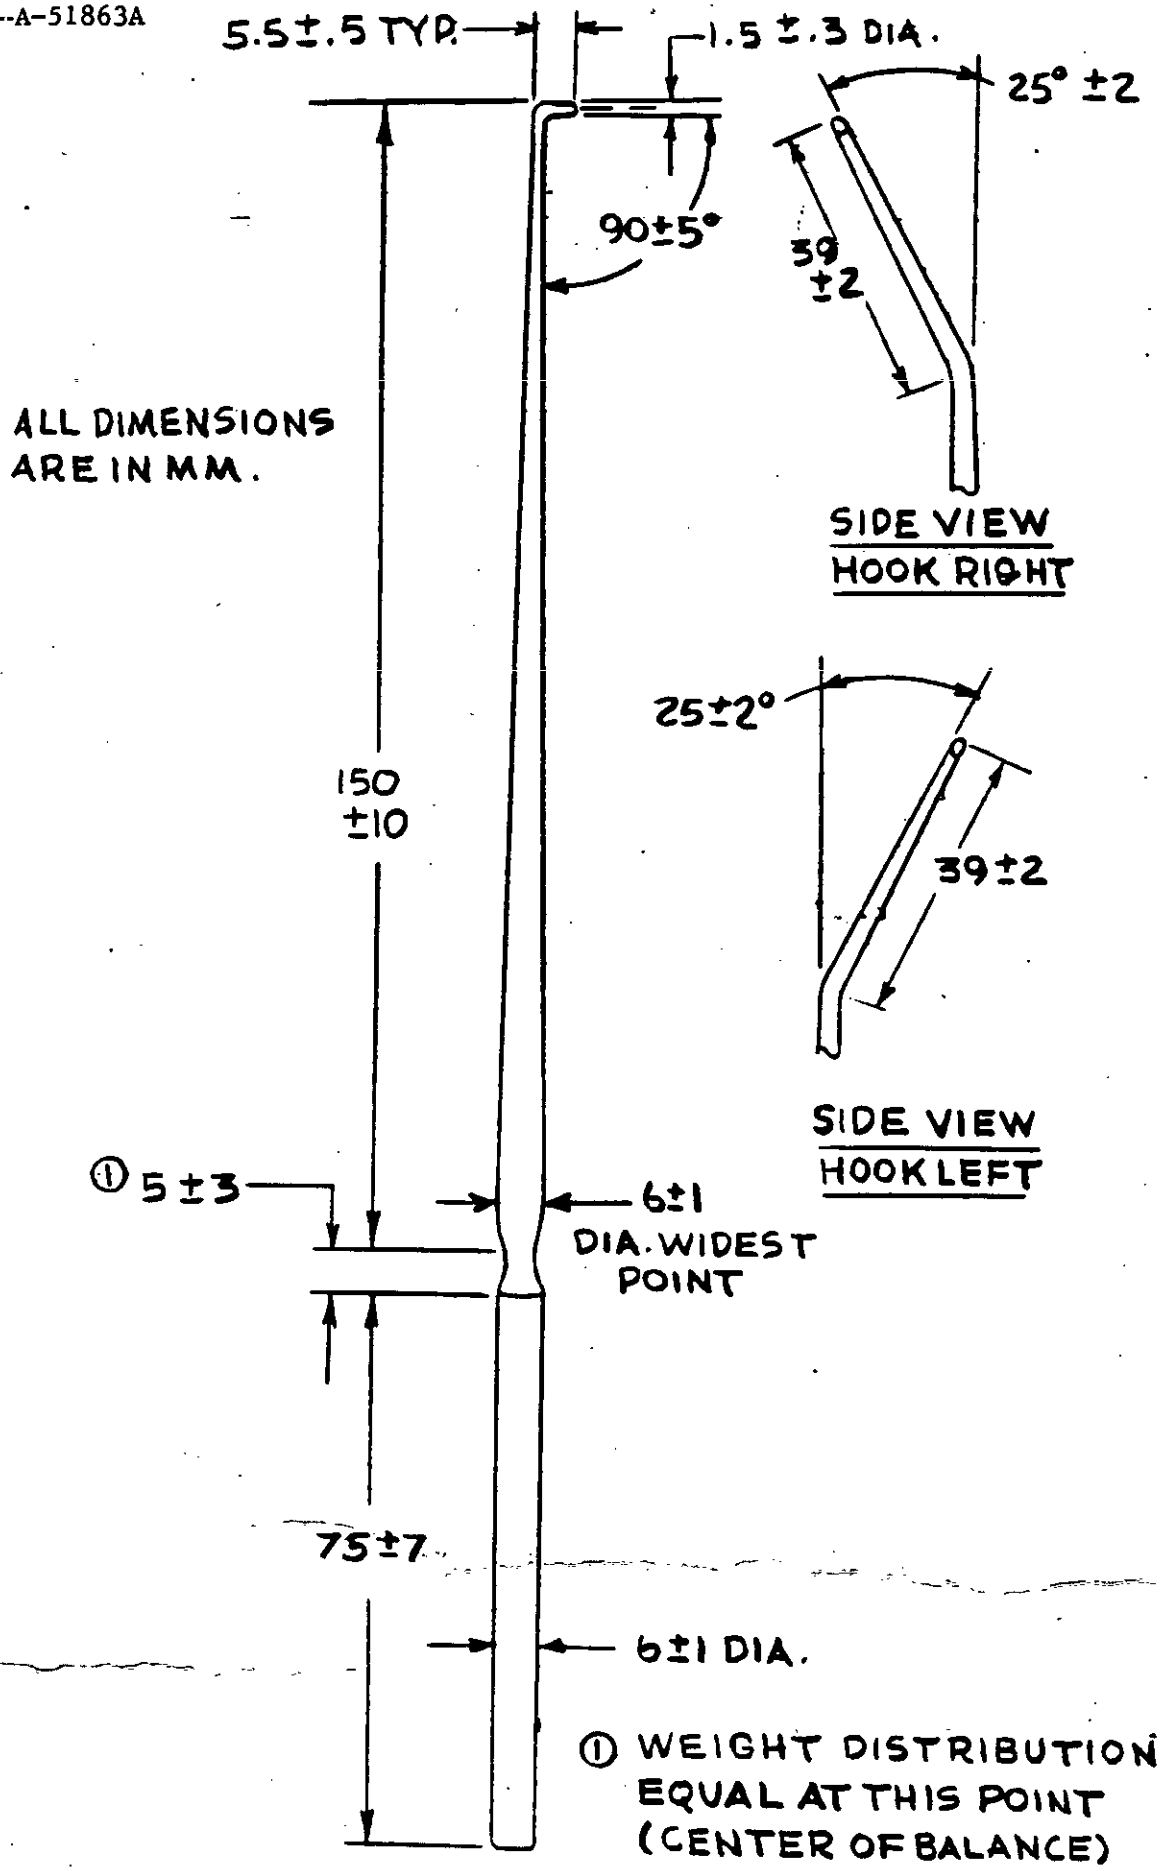


FIGURE 1. HOOK, DURA-DANDY

Source: https://assist.dla.mil -- Downloaded: 2026-01-26T09:02Z
Check the source to verify that this is the current version before use.