A-A-51881A
10 July 1989
SUPERSEDING
A-A-0051881(DM)
27 APRIL 1987

COMMERCIAL ITEM DESCRIPTION

HOLDER, SUTURE NEEDLE (Troutman)

The General Services Administration has authorized the use of this commercial item description.

This commercial item description covers a suture needle holder of the Troutman design suitable for use in mircosurgery.

Salient characteristics:

Style and design. Suture needle holder shall be without lock and have curved miniature jaws with flat tips. Cross-section of the handles shall be semi-circular. Suture needle holder shall have dimensions as specified in Figure 1.

Material. Suture needle holder shall be fabricated of a martensitic corrosion-resistant steel in accordance with ASTM Designation F899.

Hardness. Suture needle holder shall have a Rockwell Hardness C scale (HRC) of 40 to 48 when tested in accordance with ASTM Designation E18 or E92 whichever is applicable. Conversion of hardness values shall be in accordance with ASTM Designation E140.

Corrosion-resistance. Suture needle holder shall show no signs of corrosion or copper plating when tested in accordance with ASTM Designation F1089.

Passivation. Suture needle holder shall be properly passivated.

Finish. Suture needle holder shall have a mirror or satin finish.

Identification marking and labeling. Suture needle holder shall bear the contractor's name or registered trademark and the word "stainless". Holders of foreign manufacture shall bear the name of the country of manufacture.

AMSC N/A FSC 6515

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:02Z
Check the source to verify that this is the current version before use.

Workmanship. The suture needle holder shall be processed in such a manner as to be uniform and free from defects which affect life, utility, or appearance.

PRODUCT QUALITY LEVEL.

Visual and dimensional examination. Shall be examined to verify that design, construction and workmanship are in accordance with applicable requirements.

Materials. The supplier shall be responsible for performing tests to assure that materials are in accordance with requirements specified.

Unit. Each (EA). One suture needle holder, as specified, constitutes one unit.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Source: https://assist.dla.mil -- Downloaded: 202640-26T09:02Z
Check the source to verify that this is the current version before use.

Certificate of quality. Certificate of quality supplied by the manufacturer of the steel may be furnished in lieu of actual performance of composition testing by the contractor, provided lot indentity has been maintained and can be demonstrated to the Government. The certificate shall include the name of the contractor, the contact number, the name of the manufacturer or supplier, the National Stock Number, the item indentification, the lot number, the lot size, the sample size, the date of testing, the test method, indivdual test results, and the specification requirements.

Tests. Tests shall be conducted to determine compliance with specification requirements and as specified herein. Where feasible, the same sample shall be used for the determination of two or more test characteristics.

Sampling for examination. Sampling for examination shall be conducted in accordance with MIL-STD-105 with an AQL of 1.0 (percent defective) and an Inspection level of II. Unit of product for examination purposes shall be one suture needle holder. Defects shall be those listed below.

Defects

Suture needle holder not free from cracks, pits, burs, sharp edges, scale, rough areas or corrosion.

Finish of the holder not as specified.

Style, design and dimensions not as specified.

Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and as specified herein. The unit of product for test purposes shall be one suture needle holder. Sampling shall be S-1 and 1.0% AQL, except chemical composition for which acceptance number shall be zero.

Contractor certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:02Z
Check the source to verify that this is the current version before use.

Metric products. Products manufactured to metric dimensions will be considered on an equal basis with those manufactured using inch-pound units, providing they fall within the tolerances specified using conversion tables contained in the latest revision of Federal Standard No. 376, and all other requirements of this document are met.

If a product is manufactured to metric dimensions and those dimensions exceed the tolerances specified in the inch/pound units, a request should be made to the contracting officer to determine if the product is acceptable.

The contracting officer has the option of accepting or rejecting the product.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Public Law 94-580, as amended, and as implemented by Federal Acquisition Regulation Subpart 23.4 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:02Z
Check the source to verify that this is the current version before use.

NOTE: The following National Stock Number is covered by this document:

NSN	ITEM IDENTIFICATION
6515-01-120-5016	HOLDER, SUTURE NEEDLE (Troutman)

Ordering data (Intermediate/exterior package quantities and labeling and marking must be specified in the contract and/or order).

MILITARY INTERESTS:

Custodians:

Army - MD
Navy - MS
Air Force - 03

Preparing Activity:

DoD-MB

Agent:


DLA-DM

CIVIL AGENCY COORDINATING ACTIVITIES:

VA-OSS
PBS
FDA-MPQAS

Project No. 6515-4590

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:02Z
Check the source to verify that this is the current version before use.

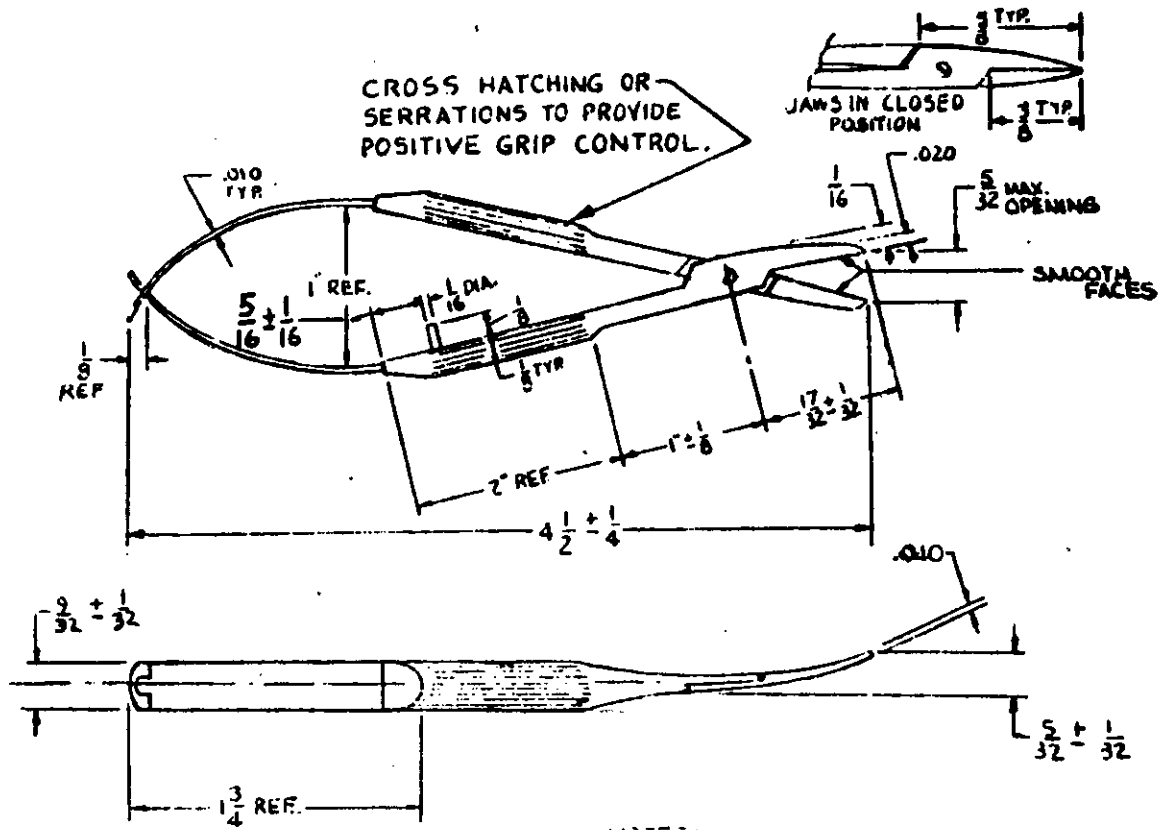

UNLESS OTHERWISE SPECIFIED DIMENSIONS ARE IN INCHES		
TOLERANCES ON		
FRACTIONS	DECIMALS	ANGLES
±1/64	± .005	±

NOTES:

1. TOLERANCES INDICATED ARE INTENDED TO PERMIT VARIATION IN DESIGN AND ARE NOT INTENDED TO PERMIT VARIANCES WITHIN A SINGLE INSTRUMENT WHICH WOULD SACRIFICE QUALITY, FUNCTION, OR WORKMANSHIP.
2. FORCEPS BLADE EDGES AND DISTAL TIPS SHALL BE UNIFORM AND MATCH EXACTLY WITHIN A SINGLE INSTRUMENT.

FIGURE 1 **HOLDER**, SUTURE NEEDLE, TROUTMAN (4½ INCH)

Source: https://assist.dla.mil -- Downloaded: 2026-02-26T09:02Z
Check the source to verify that this is the current version before use.