METRIC

A-A-54198A
27 March 1992
SUPERSEDING
A-A-54198
17 July 1990

COMMERCIAL ITEM DESCRIPTION

AIRWAY, PHARYNGEAL (BERMAN)

The General Services Administration has authorized the use of this commercial item description.

This commercial item description covers a Berman type airway suitable for use during anesthesia procedures

Salient characteristics:

General. The airway shall be clean, opaque and non-toxic, constructed of disposable plastic, and conform to American National Standards Institute (ANSI) Standard Z79.3 for Anesthetic Equipment - Oropharyngeal and Nasopharyngeal Airways. The airway shall be contoured for the patient's oropharynx. The flanged end shall fit between the teeth or gums at the lips. The pharyngeal end shall be inserted into the patient's oropharynx.

Material. The airway shall have a Shore Durometer Hardness of A80 to A90 when tested in accordance with ASTM Designation D2240.

Style, design, and dimensions. The airway shall be in accordance with figures 1 and 2.

Certificate of biocompatibility. A certificate of compliance, stipulating that offered items meet the biocompatibility test, shall be acceptable, provided that the contractor has supplied acceptable items to the Government within the past three years and that there have been no changes to material formulation and method of processing since the actual testing was performed. The certificate shall include the date the testing was performed, the test method and results, the name and title of the person evaluating the results, the current contract number and National Stock Number (NSN), a statement certifying that material

AMSC N/A FSC 6515
DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:30Z
Check the source to verify that this is the current version before use.

processing and formulation have not changed since the time that biocompatibility was performed and the signature and title of the person making the certification.

Workmanship. The airway shall be free from defects which defect from its appearance or impair its serviceability.

Unit. Package (PG). One package containing either 10 or 12 individually packaged airways of one size only, as specified, constitutes one unit. Each clean, ready for use airway shall be individually packaged in a sealed, peel-open/tear-open container capable of maintaining cleanliness of contents unless the container is damaged or opened.

QUALITY ASSURANCE PROVISIONS.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set orth in the specifications where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory applicances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more test characteristics.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:30Z
Check the source to verify that this is the current version before use.

Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and as specified herein. Inspection shall be conducted at Inspection level II and an Acceptable Quality Level (AQL) of 1.0 percent. The unit of product for test purposes shall be one airway.

Metric products. Products manufactured to metric dimensions will be considered on an equal basis with those manufactured using inch-pound units, providing they fall within the tolerance specified using conversion tables contained in the lastest revision of Federal Standard No. 376, and all other requirements of this document are met.

If a product is manufactured to metric dimensions and those dimensions exceed the tolerances specified in the inch-pound units, a request should be made to the contracting officer to determine if the products is acceptable.

The contracting officer has the option of accepting or rejecting the product.

Contractor certification. The contractor shall certify and maintain substantiating evidence that the product offered meets the salient characteristics of this Commercial Item Description, and that the product conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Regulatory requirements.

Federal Food, Drug, and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction , the offeror/contractor shall comply , and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Federal Acquisition Regulation Subpart 23.4 to the maximum extent practical.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:30Z
Check the source to verify that this is the current version before use.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and /or order.

Ordering data. Intermediate/exterior package quantities and labeling and marking must be specified in the contract and/or order.

NOTE: The following National Stock Numbers are covered by this document:

NATIONAL STOCK NUMBER	ITEM IDENTIFICATION
6515-00-068-5028	AIRWAY, PHARYNGEAL, Berman, Plastic, Disposable, Infant, 43 mm, 12's
6515-00-687-8052	AIRWAY, PHARYGNEAL, Berman, Plastic, Disposable, Large Adult, 100 mm, 12's
6515-00-958-2232	AIRWAY, PHARYNGEAL, Berman, Plastic, Disposable, Child, 80 mm, 12's
6515-01-240-3851	AIRWAY, PHARYNGEAL, Berman, Plastic, Disposable, Medium Adult, 90 mm, 10's

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:30Z
Check the source to verify that this is the current version before use.

A-A-54198A

MILITARY INTERESTS:

Custodians:

Army-MD
Navy-MS
Air Force-03

PREPARING ACTIVITY:

DoD-MB

Agent:


DLA-DM


CIVIL AGENCY COORDINATING ACTIVITIES:

VA-OSS
USPHS
FDA-MPQAS


Project No. 6515-5174
Location: c:\word\seto\airway


Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:30Z
Check the source to verify that this is the current version before use.

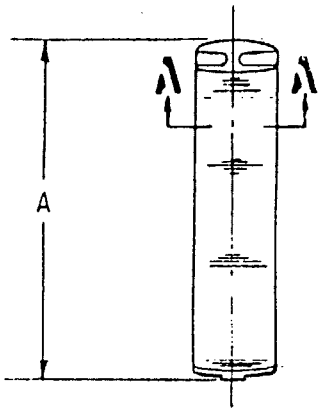

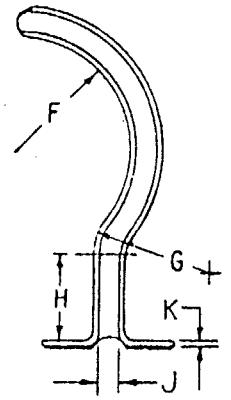

NOTES:
1. UNLESS OTHERWISE SPECIFIED TOLERANCES SHALL BE AS FOLLOWS:
   DIMS. UP TO AND INCLUDING 1mm ±0.1mm.
   DIMS. ABOVE 1mm UP TO AND INCL 10mm ±0.5mm
   DIMS. ABOVE 10mm UP TO AND INCL 50mm ± 1mm
   DIMS. ABOVE 50mm UP TO AND INCL 100mm ± 2mm.
2. REMOVE ALL SHARP EDGES AND FLASHING.



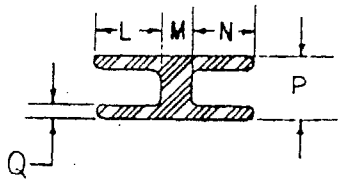

SEC A A
SCALE 2:1

UNLESS OTHERWISE SPECIFIED DIMENSIONS ARE IN MILLIMETERS.


NSN	A	B	C	D	E	F RAD.	G RAD.	H	J	K	L	M	N	P	Q
6515-00-068-5078 INFANT	43	10.0	22	8.0	3.0	12	11	8.0	3.0	1.5	4.0	2.5	4.0	5.0	0.8
6515-00-068-2232 CHILD	80	18	40	11	5.0	25	12	21	6.0	2.0	7.0	4.0	7.0	8.0	1.5
6515-00-687-6052 LARGE ADULT	100	23	54	16	6.0	32	14	27	7.0	2.0	9.0	6.0	9.0	10.0	2.0
6515-00-240-3851 MEDIUM ADULT	90	22	46	15	3.5	29	13	25	5.2	1.8	9.0	3.0	8.5	8.5	1.8

FIGURE 1 AIRWAY, PHARYNGEAL, BERMAN

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:30Z
Check the source to verify that this is the current version before use.

NOTES:

1. UNLESS OTHERWISE SPECIFIED TOLERANCES SHALL BE AS FOLLOWS:
   DIMS. UP TO AND INCLUDING 1MM ___ ±0.1 MM
   DIMS. ABOVE 1MM UP TO AND INCL 10 MM ___ ±0.5 MM
   DIMS. ABOVE 10 MM UP TO AND INCL 50 MM ±1 MM
   DIMS. ABOVE 50 MM UP TO AND INCL 100 MM ___ ±2 MM
2. REMOVE ALL SHARP EDGES AND FLASHING.

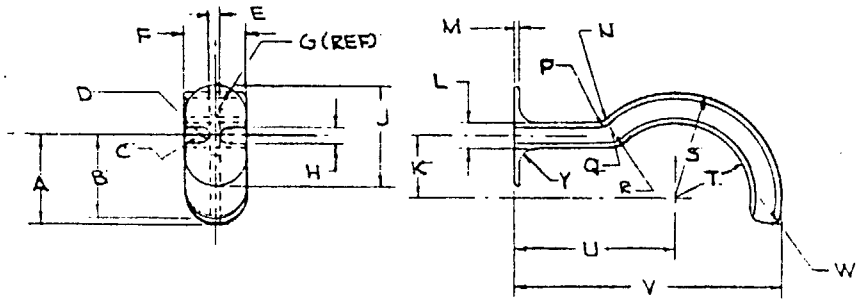

ALTERNATE

UNLESS OTHERWISE SPECIFIED DIMENSIONS ARE IN MILLIMETERS.

NSN	INCHES / MM	A	B	C	D	E	F	G	H	J	K	L	M	N	P	Q	R	S	T	U	V	W	Y
6515-00-068-5028 INFANT	INCHES	.45	.41	.02	.06	.12	.41	.20	.12	.67	.35	.20	.08	.06	.10	.12	.16	.63	.43	1.02	1.65	.04	.12
	MM	11	10.0	0.50	2.0	3.0	10.0	5.0	3.0	17	9.0	5.0	2.0	2.0	3.0	3.0	4.0	16	11	26	42	1.0	3.0
6515-00-958-2232 CHILD	INCHES	1.08	1.02	.02	.09	.08	.71	.35	.18	1.22	.75	.31	.08	.24	.29	.35	.41	1.26	.94	1.81	3.07	.07	.20
	MM	27	26	0.50	2.0	2.0	18	9.0	5.0	31	19	8.0	2.0	6.0	7.0	9.0	10	32	24	46	78	2.0	5.0
6515-00-687-6052 LARGE ADULT	INCHES	1.34	1.24	.04	.12	.16	.91	.45	.24	1.50	.93	.39	.08	.31	.37	.41	.47	1.57	1.18	2.36	3.94	.12	.24
	MM	34	31	1.0	3.0	4.0	23	11	6.0	38	24	10.0	2.0	8.0	9.0	10.0	12	40	30	60	100	10.0	6.0

FIGURE 2 AIRWAY, PHARYNGEAL, BERMAN

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:30Z
Check the source to verify that this is the current version before use.