A-A-54206
31 August 1990

COMMERCIAL ITEM DESCRIPTION

CATHETER, CARDIOVASCULAR (Occlusion)

The General Services Administration has authorized the use of this commercial item description as a replacement for Military Specification MIL-C-42041(DM), which is cancelled.

This commercial item description covers a Fogarty cardiovascular catheter suitable for blood vessel tamponade or occlusion procedures.

Salient characteristics:

General. The catheter shall be a cardiovascular catheter of the Fogarty design with a flexible, atraumatic semi-pointed tip and an inflatable latex rubber balloon. The balloon shall be securely affixed by epoxied sutures. The proximal end shall have a gate valve with a female Luer lock hub in accordance with ANSI/HIMA MD70.1. Catheter shall be in accordance with Figure 1.

Material. The catheter shall be fabricated of polyvinylchloride which meets the requirements of the USP for Class IV plastics. The catheter shall be furnished with a stylet which traverses the length of the catheter. The stylet shall be fabricated of Type 304 stainless steel in accordance with ASTM Designation F899. Except for the balloon and insertion depth markings, the catheter body shall be radiopaque in accordance with commercial practice.

Sterility, pyrogencity and toxicity. The catheter shall be non-pyrogenic and non-toxic in accordance with the USP. The catheter shall be sterile in accordance with USP or AAMI guidelines. Sterility Assurance level shall be 0.000001.

Saline resistance. The catheter and balloon shall be tested for intravenous fluid compatibility by submersion in 5% USP saline solution at 37 $\pm$ 1°C for 72 hours. Afterward, the balloon shall be fully inflated and deflated once every 20 minutes for 8 hours.

AMSC N/A FSC 6515

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:30Z
Check the source to verify that this is the current version before use.

Shelf life. The shelf life date must be printed on the package label and at least 24 months shelf life shall remain at the time of delivery to the Government.

Markings. The catheter shall be legibly marked every 10 centimeters to indicate depth of penetration.

Workmanship. The catheter shall be free from defects which affect life, utility or appearance.

PRODUCT QUALITY LEVEL.

Visual and dimensional examination. Shall be examined to verify that design, construction and workmanship are in accordance with applicable requirements.

Materials. The supplier shall be responsible for performing tests to assure that materials are in accordance with requirements specified.

Unit. Each (EA). Each catheter packaged in a rigid plastic tray, as specified, constitutes one unit. The rigid plastic tray shall have a rigid plastic lid designed to avoid crushing of the catheter. The balloon shall be provided with a protector for protection from the atmosphere. The tray shall be further packaged in a sealed, peel-open type bag capable of maintaining sterility of the contents unless the bag is damaged or opened. The bag shall be constructed of tyvek having a clear plastic backing. As an alternate, each catheter may be packed in a rigid tube designed to protect the balloon from the atmosphere.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:30Z
Check the source to verify that this is the current version before use.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Examination. The catheter shall be examined to determine compliance with specification requirements.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more test characteristics.

Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 as specified herein. The unit of product for test purposes shall be one catheter. Sampling shall be S-1, AQL 1.0.

Contractor certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Metric products. Products manufactured to metric dimensions will be considered on an equal basis with those manufactured using inch-pound units, providing they fall within the tolerances specified using conversion tables contained in the latest revision of Federal Standard No. 376, and all other requirements of this document are met.

If a product is manufactured to metric dimensions and those dimensions exceed the tolerances specified in the inch/pound units, a request should be made to the contracting officer to determine if the product is acceptable.

The contracting officer has the option of accepting or rejecting the product.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:30Z
Check the source to verify that this is the current version before use.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Federal Acquisition Regulation Subpart 23.4 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

NOTE: The following National Stock Number is covered by this document:

NSN	ITEM IDENTIFICATION
6515-01-115-1724	CATHETER, CARDIOVASCULAR, Fogarty, Occlusion, Plastic, 8 French

Ordering data (Intermediate/exterior package quantities, labeling, and marking must be specified in the contract and/or order).

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:30Z
Check the source to verify that this is the current version before use.

MILITARY INTERESTS:

Custodians:

Army - MD
Navy - MS
Air Force - 03

PREPARING ACTIVITY:

DoD - MB

Agent:


DLA-DM

CIVIL AGENCY COORDINATING ACTIVITIES:

VA-OSS
PHS
FDA-MPQAS

Project No. 6515-4424

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:30Z
Check the source to verify that this is the current version before use.

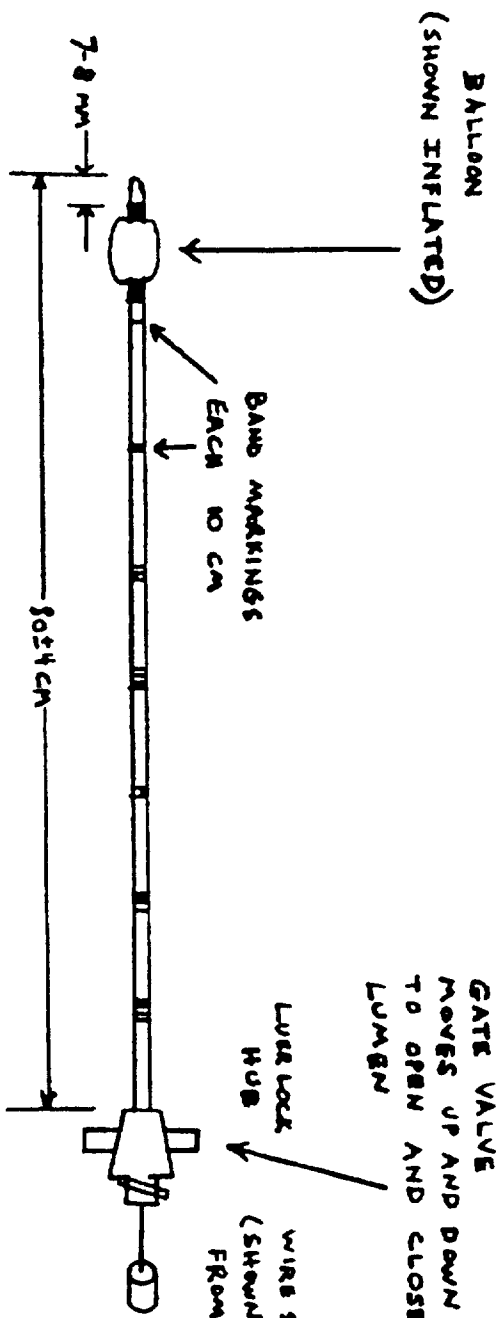

CATHETER SIZE	CATHETER COLOR	DIAMETER DEFLATED BALLOON	DIAMETER INFLATED BALLOON	BALLOON VOLUME	STYLET THICKNESS
8 Fr	BROWN	14 Fr	28MM	20 ML GAS 10 ML LIQUID	0.5±.005MM

FIGURE 1

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:30Z
Check the source to verify that this is the current version before use.

INSTRUCTIONS: In a continuing effort to make our standardization documents better, the DoD provides this form for use in submitting comments and suggestions for improvements. All users of military standardization documents are invited to provide suggestions. This form may be detached, folded along the lines indicated, taped along the loose edge *(DO NOT STAPLE)*, and filed. In block 5, be as specific as possible about particular problem areas such as wording which required interpretation, was too rigid, restrictive, loose, ambiguous, or was incompatible, and give proposed wording changes which would alleviate the problems. Enter in block 6 any remarks not related to a specific paragraph of the document. If block 7 is filled out, an acknowledgement will be mailed to you within 30 days to let you know that your comments were received and are being considered.

NOTE: This form may not be used to request copies of documents, nor to request waivers, deviations, or clarification of specification requirements on current contracts. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements.

(Fold along this line)

(Fold along this line)

NO POSTAGE NECESSARY IF MAILED IN THE UNITED STATES

OFFICIAL BUSINESS
PENALTY FOR PRIVATE USE $300

BUSINESS REPLY MAIL
FIRST CLASS PERMIT NO 4966 Alexandria, VA

POSTAGE WILL BE PAID BY

Commander
Defense Personnel Support Center
ATTN: DPSC-RSTF
2800 South 20th Street
Philadelphia, Pennsylvania 19101-8419

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:30Z
Check the source to verify that this is the current version before use.

(TO DETACH THIS FORM, CUT ALONG THIS LINE.)

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

(See Instructions – Reverse Side)

1. DOCUMENT NUMBER	2. DOCUMENT TITLE
A-A-54206	CATHETER, CARDIOVASCULAR (Occlusion)

3a. NAME OF SUBMITTING ORGANIZATION

b. ADDRESS *(Street, City, State, ZIP Code)*

4. TYPE OF ORGANIZATION *(Mark one)*

- ☐ VENDOR
- ☐ USER
- ☐ MANUFACTURER
- ☐ OTHER *(Specify)*: _____

5. PROBLEM AREAS

a. Paragraph Number and Wording

b. Recommended Wording

c. Reason/Rationale for Recommendation

6. REMARKS

7a. NAME OF SUBMITTER *(Last, First, MI)* – Optional	b. WORK TELEPHONE NUMBER *(Include Area Code)* – Optional
c. MAILING ADDRESS *(Street, City, State, ZIP Code)* – Optional	8. DATE OF SUBMISSION *(YYMMDD)*

DD FORM 1426 PREVIOUS EDITION IS OBSOLETE

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:30Z
Check the source to verify that this is the current version before use.