FEDERAL SPECIFICATION

SCREEN, BEDSIDE

This specification was approved by the Commissioner, Federal Supply Service, General Services Administration, for the use of all Federal agencies.

1. SCOPE AND CLASSIFICATION

1.1 Scope.—This specification covers an aluminum, folding, bedside screen.

1.2 Classification.

1.2.1 *Grade and type.*—Bedside screens furnished under this specification shall be one grade and one type.

2. APPLICABLE SPECIFICATIONS AND STANDARDS

2.1 Specifications.—The following specifications, of the issues in effect on date of invitation for bids, form a part of this specification:

Federal Specifications:

FF–C–86—Casters; Truck.
QQ–M–151—Metals; General Specification for Inspection of.
WW–T–789—Tubing, Aluminum Alloy 61S, Round, Square, Rectangular and Other Shapes, Seamless, Drawn.

Military Specifications:

MIL–C–5541—Chemical Films for Aluminum and Aluminum Alloys.

(Activities outside the Federal Government may obtain copies of Federal Specifications and Standards as outlined under General Information in the Index of Federal Specifications and Standards, and at the prices indicated in the Index. The Index, which includes cumulative monthly supplements as issued, is for sale on a subscription basis by the Superintendent of Documents, U. S. Government Printing Office, Washington 25, D. C.

(Single copies of this specification and other product specifications required by activities outside the Federal Government for bidding purposes are available without charge at the General Services Administration Regional Offices in Boston, New York, Atlanta, Chicago, Kansas City, Mo., Dallas, Denver, San Francisco, Los Angeles, Seattle, and Washington, D. C.

(Federal Government activities may obtain copies of Federal Specifications and Standards and the Index of Federal Specifications and Standards from established distribution points in their agencies.

(Copies of Military Specifications required by contractors in connection with specific procurement functions should be obtained from the procuring agency or as directed by the contracting officer.)

2.2 Specifications and standard applicable only to individual departments are listed in section 7.

3. REQUIREMENTS

3.1 Material.—Material shall be high quality throughout, and suitable in all respects for the purpose intended.

3.1.1 *Aluminum.*—Frame and base shall be of square aluminum tubing in accordance with type II of Federal Specification WW–T–789 with 0.065-inch wall. Commercial tolerances shall apply.

3.1.2 *Screws, lockwashers, and nuts.*—Screws, lockwashers, and nuts shall be of steel, zinc plated.

3.1.3 *Continuous hinges.*—Continuous hinges shall be steel or brass chromium plated, corrosion-resisting steel, or anodized aluminum. Hinges shall have an open width of $1\frac{1}{16}$ inches and a metal thickness of 0.036 inch minimum.

3.2 Construction. — Construction shall conform to the requirements specified herein, and as shown on figure 1. Unit shall be a three-panel, folding bedside screen, approximately 70 inches high and 95 inches wide, constructed of

Source: https://assist.dla.mil -- Downloaded: 202610-26T11:39Z
Check the source to verify that this is the currentversion before use.

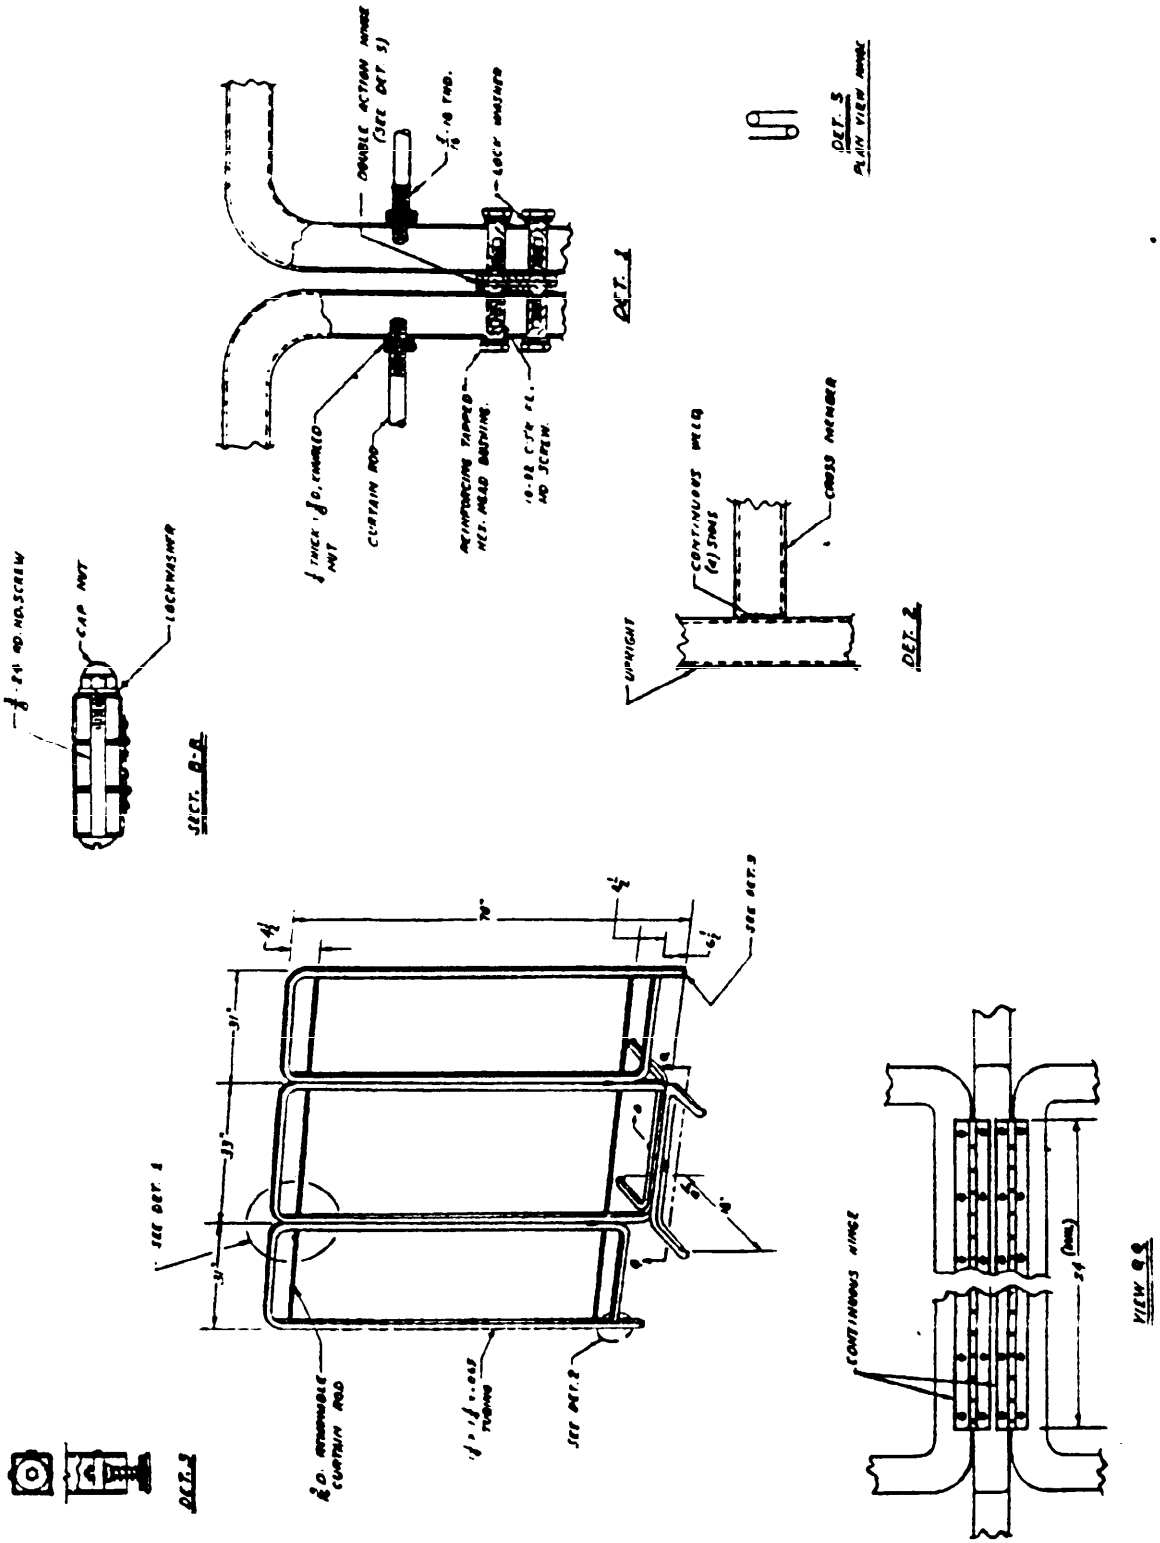


FIGURE 1.—Screen, bedside, Aluminum.

Source: https://assist.dla.mil -- Downloaded: 202610-26T11:39Z
Check the source to verify that this is the current version before use.

square tubing. Center panel shall be mounted on a base consisting of formed tubular legs hinged and bolted perpendicular to the panel and fitted with fixed glides. Corners of frame shall have a radius of approximately 2½ inches. Continuous hinges shall be held in place by sheet metal screws as shown on view QQ of figure 1, or shall be welded in place in a manner suitable for the purpose intended. The hole for the central bolt shall be drilled after assembly of the legs to the center panel to insure that the bolt can readily be inserted into the tubular section of the screen.

3.2.1 *Glides.*—Unless otherwise specified, all legs shall be fitted with conventional 1¼-inch diameter nickel or chromium-plated glides.

3.2.1.1 *Center panel glides.*—The four center panel glides shall be removable type held in place by means of rubber expanding adapters.

3.2.1.2 *End panel glides.* — The two end panel glides shall be spring-actuated and self-adjusting, held in place by means of setscrews. Style, location, and method of fastening shall be as shown on detail 3 of figure 1.

3.2.1.3 *Casters.*—Casters, when specified in lieu of glides, shall be ball bearing, swivel type, 2-inch-diameter wheels of hard-rubber composition with soft-rubber tread, in accordance with Federal Specification FF–C–86.

3.2.2 *Hinges.*—End panels shall be attached to center panel by means of double-action hinges. Hinges shall be fastened by flathead countersunk screws, fitting into reinforcing, tapped, hexagonal head, brass bushings with lockwashers, as shown on detail 1 of figure 1. Fittings shall be brass, chromium plated. Hinges may be brass or steel, chromium plated.

3.2.3 *Curtains.* — Curtains shall not be supplied.

3.2.4 *Curtain rod.* — Curtain rod shall be 5/16-inch diameter, brass, chromium-plated rod. Rods shall be removable and shall be threaded and fitted with knurled nuts for fastening, as shown on detail 1 of figure 1.

3.2.5 *Tolerances.* — All tolerances shall be kept to a minimum. Commercial tolerances on gage sizes are acceptable. In no instance shall tolerance exceed ¼ inch for any one dimension shown on figure 1.

3.2.6 *Stability.* — Screen shall be so constructed as to permit ready movement and adjustment of unit in use, and shall be sturdy and sufficiently stable to prevent toppling due to accidental bump or blow in normal use.

3.3 Finish. — Tubing shall be chemically treated in accordance with Military Specification MIL–C–5541 to form a suitable base for subsequent paint finishes. Chemical treatment of tubing shall be followed by a coat of aluminum pigmented vinyl and a finishing coat of clear vinyl lacquer. Finishes shall be suitable for use on aluminum, shall be applied in accordance with the paint manufacturer's recommendations, and shall level out to produce a clear, nonyellowing, uniform tough finish having good adhesion properties, and excellent resistance to cleaning soaps and to weather. The finished coating shall have a minimum average dry film thickness of 0.8 mils with no part of the film being less than 0.5 mils in thickness. Finish shall be free of deep orangepeel, seed, and foreign matter; and shall have sufficient gloss to give the desired eye appeal.

3.4 Identification marking. — Each screen shall be fitted in an inconspicuous location with a nameplate of metal similar to that portion of the screen where the nameplate is affixed. The nameplate shall contain the stock number and manufacturer's name or registered trademark. In addition, each screen shall be clearly tagged with instructions for inserting bolt, lockwasher, and capnut in erecting screen.

3.5 Workmanship.—Workmanship shall be first class throughout. The screens shall be free from defects which detract from their appearance or may impair their serviceability. Forming shall be neatly done without scratches or tears.

3.5.1 *Welding.* — Screens shall be welded as shown on figure 1. Welds shall be sound, well-fused, and free from blisters or blowholes, de-

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:39Z
Check the source to verify that this is the current version before use.

veloping strength equal to the part welded. Welding rod shall be of similar chemical composition to part welded. Rod shall be 5 percent silicon aluminum welding rod. All welds shall be cleaned and free from twists or strains; all exposed welds shall be ground smooth to eliminate pitmarks and seams, and shall be polished to blend with the color of the adjacent surfaces. All surfaces shall be free from sharp edges. All tubing shall be properly bent or formed to correct radii without ripples or dents. All welding of side panels and base shall be continuous.

4. SAMPLING, INSPECTION, AND TEST PROCEDURES

4.1 Sampling.—Representative samples shall be taken at random from each delivery of bedside screens to determine compliance with the requirements of this specification.

4.2 Inspection.—Samples shall be inspected for material, construction, identification marking and workmanship.

4.3 Tests.

4.3.1 *Tests on finish.* — The manufacturer shall supply ten 4- by 6-inch aluminum alloy test panels finished in exactly the same manner as the screen. These test panels shall be subjected to the following tests:

4.3.1.1 *Humidity test.*—The finish shall not blister after being subjected to 100 percent relative humidity at 100°F., for a period of 48 hours.

4.3.1.2 *Salt-spray test.*—The panel shall be prepared for test by scribing each panel along two diagonals for a distance of 5 inches, using a razor blade. The scribe marks shall penetrate through the coating to the base metal. The panel shall be exposed for 48 hours to a salt-spray test given in accordance with the applicable requirements of Federal Specification QQ–M–151 and shall show no evidence of corrosion, peeling, or undercoating of the coating at points other than within ⅛ inch distance of the scribe marks.

4.3.1.3 *Chemical spot tests.* — Finish shall show no deterioration when subjected to the following reagents at room temperature, confined under a watchglass for the specified time:

Reagent	
20 percent Sodium Hydroxide Solution	24 Hours.
50 percent Sulfuric Acid	24 Hours.
95 percent Ethyl Alcohol	30 Minutes.

4.3.1.4 *Water-immersion test.*—Finish shall show no blistering after panel is immersed in water for 24 hours at room temperature.

4.3.1.5 *Grease-resistance test.* — The finish shall not permanently soften when smeared with equal parts c.p. Oleic acid and lard oil, and stored at room temperature for a period of 5 days.

5. PREPARATION FOR DELIVERY

5.1 Packaging.—Unless otherwise specified, each screen shall be packaged in accordance with accepted commercial practice.

5.2 Packing.—The subject commodity shall be prepared for shipment to permit acceptance by carrier for transportation at the lowest applicable rate, and to afford maximum protection from normal hazards of transportation.

5.3 Marking.

5.3.1 *Packages.*—Unless otherwise specified, packages shall be marked with the name and size of the commodity, the quantity contained therein, and the name of the manufacturer and contractor.

5.3.2 *Shipping containers.*—Unless otherwise specified, shipping containers shall be marked with the name and size of the commodity as defined by the contract or order under which the shipment is made, the quantity contained therein, the name of the contractor, the number of the contract or order, the name and address of the consignee, and the gross weight.

6. NOTES

6.1 Purchasers should exercise any desired options offered herein. (See 3.2.1, 5.1, 5.3, 7.2.2, 7.2.3, and 7.2.4.)

6.2 This specification covers the following item appearing in the Armed Services Medical Stock List:

6530–707–7975 Screen, Bedside, Aluminum.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:39Z
Check the source to verify that this is the current version before use.

6.3 It is believed that this specification adequately describes the characteristics necessary to secure the desired material, and that normally no samples will be necessary prior to award to determine conformance to the requirements of this specification. If, for any particular purpose, samples with bids are necessary, they should be specifically asked for in the invitation for bids, and the particular purpose to be served by the bid sample should be definitely stated, the specification to apply in all other respects.

6.4 Federal specifications do not include all types, classes, grades, sizes, etc., of the commodities indicated by the titles of the specifications, or which are commercially available, but are intended to cover the types, etc., which are suitable for Federal Government requirements.

6.5 Transportation description.—Transportation description applicable to this item is:

Screens, floor, not otherwise indexed by name.
Carload minimum weights:
In cars 40′9″ or less in length, inside measurements, 10,000; 12,000; 15,000; 18,000; 22,000; 30,000 pounds.
In cars exceeding 40′9″ in length, inside measurements, 16,000; 18,000; 21,000; 24,000; 30,000; 40,000 pounds.
Truckload minimum weight 12,000 pounds.

Patent notice.—When Government drawings, specifications, or other data are used for any purpose other than in connection with a definitely related Government procurement operation, the United States Government thereby incurs no responsibility nor any obligation whatsoever; and the fact that the Government may have formulated, furnished, or in any way supplied the said drawings, specifications, or other data, is not to be regarded by implication or otherwise as in any manner licensing the holder or any other person or corporation, or conveying any rights or permission to manufacture, use, or sell any patented invention that may in any way be related thereto.

7. DEPARTMENTAL REQUIREMENTS

7.1 The following specifications and standard, of the issues in effect on date of invitation for bids, and special requirements, form a part of this specification for purchases made under this specification by the respective departments.

7.2 Army, Navy and Air Force.

7.2.1 *Applicable specifications and standard.*

Federal Specifications:

NN–B–621—Boxes, Wood, Nailed and Lock-Corner.

LLL–B–631—Boxes; Fiber Corrugated (for Domestic Shipment).

PPP–B–601 — Boxes, Wood, Cleated-Plywood.

Military Specifications:

JAN–P–106—Packaging and Packing for Overseas Shipment—Boxes; Wood, Nailed.

JAN–P–108—Packaging and Packing for Overseas Shipment — Boxes, Fiberboard (V-Board and W-Board), Exterior and Interior.

MIL–B–10377—Box, Wood, Cleated, Veneer, Paper Overlaid.

Military Standard:

MIL–STD–129—Marking for Shipment and Storage.

(Copies of specifications, standards, and drawings required by contractors in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.)

7.2.2 *Packaging.*

7.2.2.1 *Unit of issue.*—One screen, as specified, constitutes one unit.

7.2.2.2 *Level A—Military package.*—Screen shall be in a closed position. Legs shall be folded flat. Care shall be exercised to see that the glide button of the outer frame is in a closed position and resting against the top edge of the leg frame. Sections of the screen and legs shall be secured in position by tying with cord or cotton tape. Bolt, nut, and washer shall be packaged in a cloth bag of suitable size and design. Exterior surfaces of the unit shall be protected by wrapping in kraft paper or other suitable material. Work shall be accomplished in such manner as to prevent scratching or marring of the unit.

7.2.2.3 *Level B—Limited Military package.*—Package shall be as specified in 7.2.2.2.

Source: https://assist.dla.mil -- Downloaded: 202610-26T11:39Z
Check the source to verify that this is the current version before use.

7.2.2.4 *Level C—Minimum Military package.*—Package shall be as specified in 5.1.

7.2.3 *Packing.*

7.2.3.1 *Level A—Military pack.*—Each unit shall be overpacked in an exterior container constructed in accordance with the requirements of one of the following specifications:

Military Specification JAN-P-106 — Boxes, Wood, Nailed.

Military Specification JAN-P-108 — Boxes, Fiberboard (V-Board and W-Board); type SF, grade 2, style FOL, compliance symbol V2s.

Federal Specification PPP-B-601 — Boxes, Wood, Cleated-Plywood. Box shall comply with table II. Plywood shall be type III, class 1.

Military Specification MIL-B-10377—Boxes, Wood, Cleated, Veneer, Paper Overlaid. Box shall comply with table II.

Closure and strapping shall comply with appendix of applicable specification. Container design shall include suitable interior fittings or braces to prevent shifting of, or damage to, the contents.

7.2.3.2 *Level B—Limited Military pack.*—Each unit shall be overpacked in an exterior container constructed in accordance with the requirements of one of the following specifications:

Federal Specification NN-B-621 — Boxes, Wood, Nailed and Lock-Corner.

Federal Specification LLL-B-631 — Boxes; Fiber Corrugated. Box shall be style OLC, overlap slotted box. Fiberboard shall be double wallboard and shall have bursting strength of not less than 500 pounds Mullen test.

Federal Specification PPP-B-601 — Boxes, Wood, Cleated-Plywood. Box shall comply with table I. Plywood shall be type III, class 1.

Military Specification MIL-B-10377—Boxes, Wood, Cleated, Veneer, Paper Overlaid. Box shall comply with table I.

Container design shall include suitable interior fittings or braces to prevent shifting or damage to contents.

7.2.3.3 *Level C—Minimum Military pack.*—Pack shall be specified in 5.2.

7.2.4 *Marking.*

7.2.4.1 *Level A—Military marking.*—Shipping container shall be marked in accordance with Military Standard MIL-STD-129. Service color marking and symbol are not required on containers for level A packs when addressed to domestic establishments for the Medical Services of the Armed Forces.

7.2.4.2 *Level B—Limited Military marking.*—Shipping container shall be marked in accordance with Military Standard MIL-STD-129.

7.2.4.3 *Level C—Minimum Military marking.*—Marking shall be as specified in 5.3.2.

7.2.5 *Ordering data.*—Requests, requisitions, schedules, and contracts or orders should specify the desired level of protection. (See 7.2.2, 7.2.3, and 7.2.4.)

MILITARY INTEREST:

Army—M
Navy—Md
Air Force.

Copies of this specification may be purchased for 10 cents each.

Source: https://assist.dla.mil -- Downloaded: 202610-26T11:39Z
Check the source to verify that this is the current version before use.