AA-S-75A
September 8, 1975
SUPERSEDING
AA-S-75
April 29, 1959

FEDERAL SPECIFICATION

SAFE, DENTAL X-RAY FILM PROTECTIVE

This specification was approved by the Commissioner, Federal Supply Service, General Services Administration, for the use of all Federal agencies.

1. SCOPE

1.1 This specification covers a two-compartment dental x-ray film protecting safe designed for the protective storage and convenient dispensing of dental x-ray films.

2. APPLICABLE DOCUMENTS

2.1 The following documents of the issue in effect on date of invitation for bids or request for proposals, form a part of this specification to the extent specified herein:

Federal Specifications:

L-F-310	-	Film, Dental Radiographic, Film, Photofluorographic, Medical, Film, Radiographic, Medical.
PPP-B-585	-	Boxes, Wood, Wirebound.
PPP-B-601	-	Boxes, Wood, Cleated-Plywood.
PPP-B-621	-	Boxes, Wood, Nailed and Lock-Corner.
PPP-B-636	-	Boxes, Shipping, Fiberboard.

Federal Standards:

Fed. Std. No. 123 - Marking for Shipment (Civil Agencies).

FSC 6525

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:38Z
Check the source to verify that this is the current version before use.

(Activities outside the Federal Government may obtain copies of Federal Specification, Standards, and Handbooks as outlined under General Information in the Index of Federal Specifications and Standards and at the prices indicated in the Index. The Index, which includes cumulative monthly supplements as issued, is for sale on a subscription basis by the Superintendent of Documents, U.S. Government Printing Office, Washington, D.C. 20402.

(Single copies of this specification and other Federal Specifications required by activities outside the Federal Government for bidding purposes are available without charge from Business Service Centers at the General Services Administration Regional Offices in Boston, New York, Washington, DC, Atlanta, Chicago, Kansas City, MO, Fort Worth, Denver, San Francisco, Los Angeles, and Seattle, WA.

(Federal Government activities may obtain copies of Federal Specifications, Standards, and Handbooks and the Index of Federal Specifications and Standards from established distribution points in their agencies.)

Military Specification:

MIL-L-10547 - Liners, Case, and Sheet, Overwrap, Water-Vaporproof or Water proof, Flexible.

Military Standards:

MIL-STD-105 - Sampling Procedures and Tables for Inspection by Attributes.
MIL-STD-129 - Marking for Shipment and Storage.

(Copies of Military Specifications, and Standards required by suppliers in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.)

3. REQUIREMENTS

3.1 Material. The dental x-ray film protective safe shall be fabricated of case grey iron suitable in all respects for the purpose intended.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:38Z
Check the source to verify that this is the current version before use.

3.2 Design and construction. The dental safe shall be in the shape of an inverted "T" as shown in figure 1. Shall consist of a cast body, with doors and dispensing mechanism. Shall be furnished with accessories, as required, for wall and cabinet mounting. The body of the safe shall be a one-piece grey-iron casting containing two separate compartments. The upper compartment shall be for storage of exposed film. Dimensions shall be nominally 2 inches wide by 2 inches deep. The upper compartment shall have a slot on the top for insertion of the film and shall accommodate no less than 16 packets of exposed dental x-ray film, 1-1/4 by 1-5/8 inches. The lower compartment shall be nominally 2 inches wide and 1-1/2 inches deep and shall accommodate at least 150 packets of standard 1-1/4 inch by 1-5/8 inch unexposed periapical dental x-ray film. The body shall have provisions for both wall and dental cabinet mounting.

3.2.1 Doors. The two compartments of the body shall be provided with separate doors. The doors shall be held tightly closed by either gravity or a spring device. The doors shall also be provided with locking devices capable of securing the doors. The doors when closed, shall fit tightly with the body. The lower compartment shall be provided with a hand-operated dispensing mechanism which shall satisfactorily dispense standard size periapical dental film, one at a time, without clogging or jamming the film or mechanism. Dispensing mechanism shall be adjustable in order to properly dispense all thicknesses of the 1-1/4 inch by 1-5/8-inch periapical dental X-ray film packets. The maximum overall dimensions across any part of the unit shall not be greater than 16 inches high, 7 inches wide, and 5-1/2 inches deep (see fig. 1).

3.4 Performance. The safe shall protect dental x-ray film from x-ray radiation. No detectable fog shall be produced on the film while in the safe when the safe is exposed to x-rays as specified in 4.4.1. When developed, density of such "exposed" film shall meet the original requirements of the film.

3.5 Finish. All metal parts except corrosion-resisting steel parts shall have a protective finish. Grey-iron castings shall be given a baked enamel paint finish. Other metal parts shall have either a baked enamel or an electro-plated finish. Protective plating shall be zinc, or chromium, or an anodic conversion coating. Enamel, when used, shall be applied over primer, and final baking shall be performed at 250°F. for 45 minutes or at a temperature as recommended by the paint manufacturer.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:38Z
Check the source to verify that this is the current version before use.

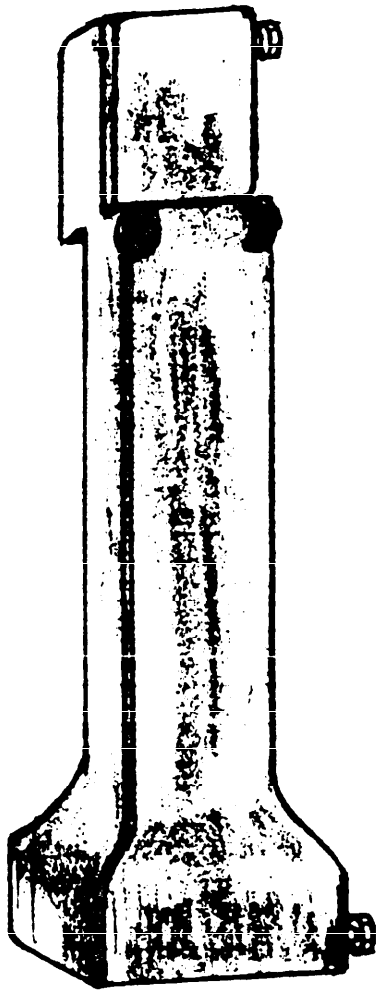


Figure 1. Safe, dental, x-ray film protective

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:38Z
Check the source to verify that this is the current version before use.

3.6 Service data. The contractor shall enclose with each unit, two copies of instructions for installation and maintenance. Instructions shall be complete with directions for adjustment of the dispensing mechanism to accommodate different thicknesses of film packets.

3.7 Identification marking. Each dental X-ray film protective safe shall be permanently and legibly marked in a conspicuous location with the manufacturer's name or registered trademark. Marking shall be accomplished by stamping, or by means of a metal nameplate permanently affixed. Nameplate shall be a size such as required for easy readability and identification.

3.8 Workmanship. Workmanship shall be first class throughout. Dental X-ray film protective safes shall be free from defects which detract from their appearance or may impair their serviceability.

4. QUALITY ASSURANCE PROVISIONS

4.1 Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the supplier is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or order, the supplier may use his own or any other facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure that supplies and services conform to prescribed requirements.

4.1.1 Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government, upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of 2 years after delivery of the supplies to which such records relate.

4.1.2 Certificates of quality. Certificates of quality, supplied by the manufacturer of the component or material may be furnished in lieu of actual performance of such testing by the contractor, provided lot identity has been maintained and can be demonstrated to the Government. The Certificate shall include the name of the contractor, the contract number, the name of the manufacturer or supplier, the NSN, the Item Identification, the name of the component/material, the lot number, the lot size, the sample size, the date of testing, the test method, individual test results, and the specification requirements.

Source: https://assist.dla.mil -- Downloaded: 202610-26T11:38Z
Check the source to verify that this is the currentversion before use.

the film while in the safe when the safe is exposed to x-rays

4.1.3 Inspection. Inspection, as used in this specification, is defined as both examination (such as visual, and auditory, investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

4.2 Sampling.

4.2.1 For examination. Sampling for examination shall be conducted in accordance with MIL-STD-105, and table I.

TABLE I. Sampling for examination

	Inspection level	AQL (defects per hundred units)
For visual examination		
Major defects	S-4	1.0
Minor defects	S-4	4.0
For dimensional examination	S-1	2.5

4.2.2 For tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 for an inspection level of S-2. Acceptance number shall be 0.

4.3 Examination. The tables shall be examined to determine compliance with all requirements contained in this specification.

4.3.1 Classification of defects. Examination shall be conducted in accordance with the following classification of defects, as shown in table II.

TABLE II. Classification of defects

Categories	Defects 1/
Major:	
101	Safe not free of cracks, burs, sharp edges.
102	Safe not complete with all component parts.
103	Safe does not accommodate number of films required in each compartment.
104	Holes for wall or dental cabinet mounting not provided.
105	Safe doors do not close and align properly with body.
106	Locking devices do not secure doors.
107	Dispensing mechanism does not operate smoothly, without jamming.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:38Z
Check the source to verify that this is the current version before use.

TABLE II. Classification of defects (Con.)

Categories	Defects 1/
Major:	
108	Dispensing mechanism does not deliver only one film packet per operation.
109	Dispensing mechanism not adjustable for various film packet thicknesses.
110	Castings not sound, not free of porosity, or flash.
Minor:	
201	Finish not as specified, not free of chipped out areas.
202	Instructions regarding adjustment of dispensing mechanism not complete.
203	Identification marking not present, not permanent, not complete.

1/ Inspection shall not be restricted to the classified possible defects listed above.

4.4 Tests.

4.4.1 X-ray test. Two each of type I, class B, size 1, X-ray dental film packets as specified in L-F-310 shall be placed in the upper and lower compartments. The doors of the safe shall be closed. The safe shall be exposed to the useful X-ray beam incident in any direction on the safe, including the bottom of the safe, except within 70° of vertical from the top edges. At least four X-ray exposures shall be taken. The X-rays shall be produced utilizing the following technical factors: 70 KVP, 1000 MAS, and 36-inch distance from safe. The exposed dental film shall then be compared with at least two samples of unexposed X-ray dental film from the same lot. The exposed and unexposed dental X-ray films shall be checked for density and fog in accordance with the requirements of L-F-310, and shall meet the requirements of 3.4 of this specification.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:38Z
Check the source to verify that this is the current version before use.

4.5 Examination for preparation for delivery. An examination shall be made to determine whether the packaging, packing, and marking comply with the requirements of section 5. Defects shall be scored as specified in table III. Sampling shall be in accordance with MIL-STD-105. The sample unit shall be one container fully prepared for delivery. The lot shall be the number of containers offered for inspection at one time. The inspection level shall be S-2 and the acceptable quality level shall be 4.0 defects per hundred units

TABLE III. Examination for preparation for delivery

Examination	Defect
Containers	Not as specified.
Quantity	Quantity in interior packages and shipping containers not as specified.
Packaging and packing materials	Any component missing or damaged.
Workmanship	Inadequate application of components, such as incomplete closure of container flaps, tape improperly applied, or containers distorted.
Markings	Omitted, incorrect, illegible, improper size, location, sequence, or method of application.

5. PREPARATION FOR DELIVERY

5.1 Packaging. Packaging shall be Level A or C as specified (see 6.2).

5.1.1 Unit of issue. One safe, as specified, constitutes one unit of issue.

5.1.2 Packaging quantities. The number of units of issue indicated in table IV shall be packaged in each unit, intermediate, and exterior container, as applicable, for the required level of protection specified in the procurement document.

TABLE IV. Packaging quantities

Unit package	Intermediate package	Exterior container
1 unit	Not required	12 units

Source: https://assist.dla.mil -- Downloaded: 202610-26T11:38Z
Check the source to verify that this is the currentversion before use.

5.1.2.1 Packing variation permitted. If the required number of units in the entire shipment is less than the number of units specified to be overpacked in an exterior container, such units shall be packed in an exterior container of suitable size and design, acceptable to a common carrier, which shall insure safe delivery to destination.

5.1.3 Level A.

5.1.3.1 Unit package. Unit package shall be a box of appropriate size and design constructed in accordance with PPP-B-636, type CF, class domestic. Box shall be designed with suitable interior fittings or shall contain sufficient cushioning material to insure against shifting of, or damage to, the contents. Closure shall be adequate to prevent accidental opening under normal handling.

5.1.4 Level C. Units shall be packaged in standard commercial containers of the size and kind commonly used, which will afford the degree of protection required for shipment and use of the product for its intended purpose.

5.2 Packing. Packing shall be Level A, B or C as specified (see 6.2).

5.2.1 Level A.

5.2.1.1 Exterior container. Exterior container shall be designed for a type 2 load and constructed in accordance with PPP-B-585, class 3, style 3; PPP-B-601, overseas type; PPP-B-621, class 2; or PPP-B-636, class weather-resistant, grade V3c. Closure and strapping shall be as specified in the appendix of the applicable box specification.

5.2.1.2 Case liner. Each Level A wood box shall be lined with a waterproof case liner conforming to MIL-L-10547. Closure and sealing shall conform to applicable paragraphs of appendix thereto. Case liner shall not be required for fiberboard boxes. Fiberboard boxes shall be waterproof in accordance with 30.4 of PPP-B-636.

5.2.2 Level B.

5.2.2.1 Exterior container. Exterior container shall be designed for a type 2 load and constructed in accordance with PPP-B-585, class 1, style 3; PPP-B-601, domestic type; PPP-B-621, class 1; or PPP-B-636, class domestic. Closure shall be as specified in the appendix of the applicable box specification. Fiberboard box shall be closed by method II of PPP-B-636.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:38Z
Check the source to verify that this is the current version before use.

5.2.3 Level C. The subject commodity shall be packed in substantial commercial containers of the type, size, and kind commonly used for the purpose, so constructed as to insure acceptance and safe delivery by common or other carriers, at the lowest rate, to point of delivery called for in the contract or purchase order.

5.3 Marking.

5.3.1 Civil agencies. Marking for shipment shall be in accordance with FED-STD-123.

5.3.2 Military.

5.3.2.1 Interior package. Each unit package shall be marked in accordance with MIL-STD-129. Contract or purchase order number and name of contractor shall be shown.

5.3.2.2 Exterior container. Exterior container shall be marked in accordance with MIL-STD-129.

6. NOTES

6.1 Intended use. The safe is intended for protection of exposed and unexposed x-ray film from fogging due to inadvertent irradiation of x-rays.

6.2 Ordering data. Purchasers should select the preferred options permitted herein and include the following information in procurement documents.

a. Title, number, and date of this specification.

b. Selection of applicable levels of packaging and packing (see 5.1 and 5.2).

6.3 This specification covers the following item listed in the Federal Supply Catalog.

NSN	Item Identification
6525-00-612-7650	SAFE, DENTAL X-RAY FILM PROTECTIVE

6.4 This specification does not cover all types, classes, grades, or sizes of the commodity indicated by the title of this specification, or those which are commercially available, but is intended to cover the types which are normally procured to meet requirements.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:38Z
Check the source to verify that this is the current version before use.

Custodians:

Army - MD
Navy - MS
Air Force - 03

Civil Agency Coordinating Activity:

GSA-FSS

Preparing activity:

DSA-DM

Project No. 6525-1116

Orders for this publication are to be placed with General Services Administration, acting as an agent for the Superintendent of Documents. See section 2 of this specification to obtain extra copies and other documents referenced herein. Price 35 cents each.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:38Z
Check the source to verify that this is the current version before use.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:38Z
Check the source to verify that this is the current version before use.

FOLD

DEFENSE PERSONNEL SUPPORT CENTER
2800 South 20th Street
Philadelphia, PA 19101

POSTAGE AND FEES PAID
DEFENSE SUPPLY AGENCY
DoD - 304

OFFICIAL BUSINESS
PENALTY FOR PRIVATE USE $300

HEADQUARTERS, DEFENSE PERSONNEL SUPPORT CENTER
ATTN: DIRECTORATE OF MEDICAL MATERIEL, CODE ATT
2800 SOUTH 20TH STREET
PHILADELPHIA, PA 19101

FOLD

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:38Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

OMB Approval
No. 22-R255

INSTRUCTIONS: The purpose of this form is to solicit beneficial comments which will help achieve procurement of suitable products at reasonable cost and minimum delay, or will otherwise enhance use of the document. DoD contractors, government activities, or manufacturers/vendors who are prospective suppliers of the product are invited to submit comments to the government. Fold on lines on reverse side, staple in corner, and send to preparing activity. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements. Attach any pertinent data which may be of use in improving this document. If there are additional papers, attach to form and place both in an envelope addressed to preparing activity.

DOCUMENT IDENTIFIER AND TITLE

AA-S-75A SAFE, DENTAL X-RAY FILM PROTECTIVE

NAME OF ORGANIZATION AND ADDRESS

CONTRACT NUMBER

MATERIAL PROCURED UNDER A

☐ DIRECT GOVERNMENT CONTRACT ☐ SUBCONTRACT

1. HAS ANY PART OF THE DOCUMENT CREATED PROBLEMS OR REQUIRED INTERPRETATION IN PROCUREMENT USE?

A. GIVE PARAGRAPH NUMBER AND WORDING.

B. RECOMMENDATIONS FOR CORRECTING THE DEFICIENCIES

2. COMMENTS ON ANY DOCUMENT REQUIREMENT CONSIDERED TOO RIGID

3. IS THE DOCUMENT RESTRICTIVE?

☐ YES ☐ NO *(If "Yes", in what way?)*

4. REMARKS

SUBMITTED BY *(Printed or typed name and address - Optional)*

TELEPHONE NO.

DATE

DD FORM 1 JAN 72 1426 REPLACES EDITION OF 1 JAN 66 WHICH MAY BE USED

☆ GPO 1974 – 603-680/6126 2-1

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:38Z
Check the source to verify that this is the current version before use.