AA-T-0041E (DSA-DM)
4 June 1975
SUPERSEDING
Revision of
Int. Fed. Spec.
AA-T-0041d
October 2, 1969

INTERIM FEDERAL SPECIFICATION

TABLE, ANESTHETIST'S

This interim Federal specification was developed by the Defense Personnel Support Center, 2800 South 20th Street, Philadelphia, Pennsylvania 19101, based upon currently available technical information. It is recommended that Federal agencies use it in procurement and forward recommendations for changes to the preparing activity at the address shown above.

1. SCOPE

1.1 This specification covers corrosion-resisting steel anesthetists' tables with two removable trays and one drawer under the lower tray, suitable for use in hospitals and doctors' offices.

2. APPLICABLE DOCUMENTS

2.1 The following documents of the issue in effect on date of invitation for bids or request for proposal, form a part of this specification to the extent specified herein.

SPECIFICATIONS

Federal

FF-C-77	Casters, Institutional Duty
PPP-B-585	Box, Wood, Wirebound.
PPP-B-601	Box, Wood, Cleated-Plywood.
PPP-B-621	Box, Wood, Nailed and Lock-Corner.
PPP-B-640	Box, Fiberboard, Corrugated, Triple-wall.

FSC 6530

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:38Z
Check the source to verify that this is the current version before use.

STANDARDS

Federal

FED-STD-66	Steel Chemical Composition and Hardenability
FED-STD-123	Marking for Domestic Shipment (Civilian Agencies).
FED-STD-151	Metals, Test Methods

(Activities outside the Federal Government may obtain copies of Federal Specifications and Standards as outlined under General Information in the Index of Federal Specifications and Standards and at the prices indicated in the Index. The Index, which includes cumulative monthly supplements as issued, is for sale on a subscription basis by the Superintendent of Documents, U.S. Government Printing Office, Washington, DC 20402.

(Single copies of this specification and other product specifications required by activities outside the Federal Government for bidding purposes are available without charge at the General Services Administration Regional Offices in Boston, New York, Atlanta, Chicago, Kansas City, MO., Dallas, Denver, San Francisco, Los Angeles, Seattle, and Washington, DC.

(Federal Government activities may obtain copies of Federal Specifications and standards and the Index of Federal Specifications and Standards from established distribution points in their agencies.)

SPECIFICATIONS

Military

MIL-L-10547	Liners, Case, and Sheet, Overwrap; Water-Vaporproof, or Waterproof, Flexible.

STANDARDS

Military

MIL-STD-105	Sampling Procedures and Tables for Inspection by Attributes.
MIL-STD-129	Marking for Shipment and Storage.

(Copies of Military specifications, standards, and drawings required by suppliers in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.)

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:38Z
Check the source to verify that this is the current version before use.

2.2 Other publications. The following documents form a part of this specification to the extent specified herein. Unless otherwise indicated, the issue in effect on date of invitation for bids shall apply.

AMERICAN WELDING SOCIETY

Welders Handbook, 6th Edition

(Application for copies should be addressed to the American Welding Society, Inc., 345 East 47th Street, New York, NY 10017.)

NATIONAL FIRE PROTECTION ASSOCIATION (NFPA)
No. 56A Code for the use of Flammable Anesthetics.

(Application for copies should be addressed to the National Fire Protection Association, 60 Batterymarch Street, Boston, MA 02110).

3. REQUIREMENTS

3.1 Material. Tables shall be constructed of corrosion-resisting steel, conforming to class 302, finish 4, of FED-STD-66, except the frame which shall be class 304, finish 4 and shall meet the requirements for chemical composition specified therein when tested as specified in 4.4.2. Thicknesses of material shall be as shown in Table I. Commercial tolerances on gages shall apply.

Table I. Thickness of material

Section	Thickness	
	Gage	Inches
Leg	No. 16 Birmingham Wire	0.065
Drawer body	No. 24 U. S. Standard	.025
Drawer front	No. 16 U. S. Standard	.062
Drawer channels	No. 16 U. S. Standard	.062
Frames	No. 11 U. S. Standard	.125
Trays	No. 20 U. S. Standard	.037

3.2 Design and construction. The unit shall consist of a table, complete with two trays as shown in Figure 2 and a drawer, as shown on Figures 1 or 3. When tested as specified in 4.4.1, the assembled table shall comply with the requirements of National Fire Protection Association (NFPA) No. 56A.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:38Z
Check the source to verify that this is the current version before use.

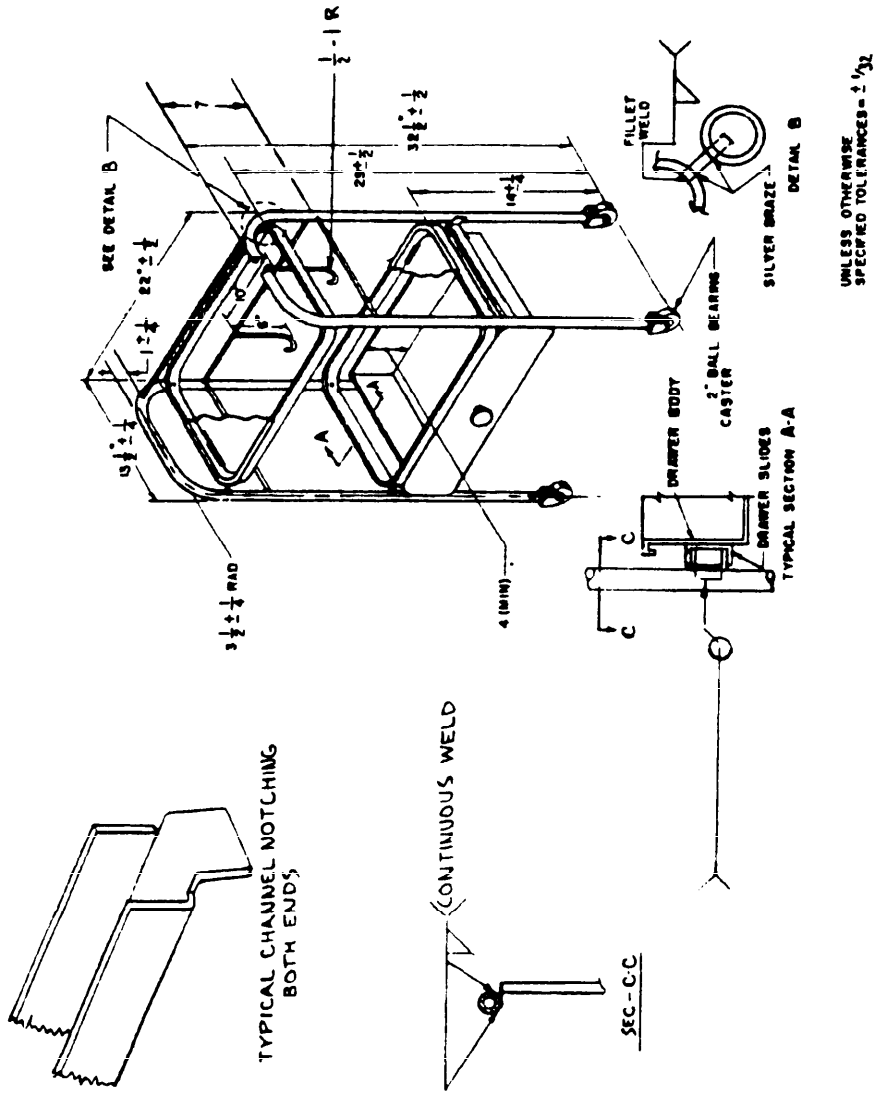


FIG. 1

FIGURE 1
Anesthetist's Table DIMENSIONS ARE IN INCHES

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:38Z
Check the source to verify that this is the current version before use.

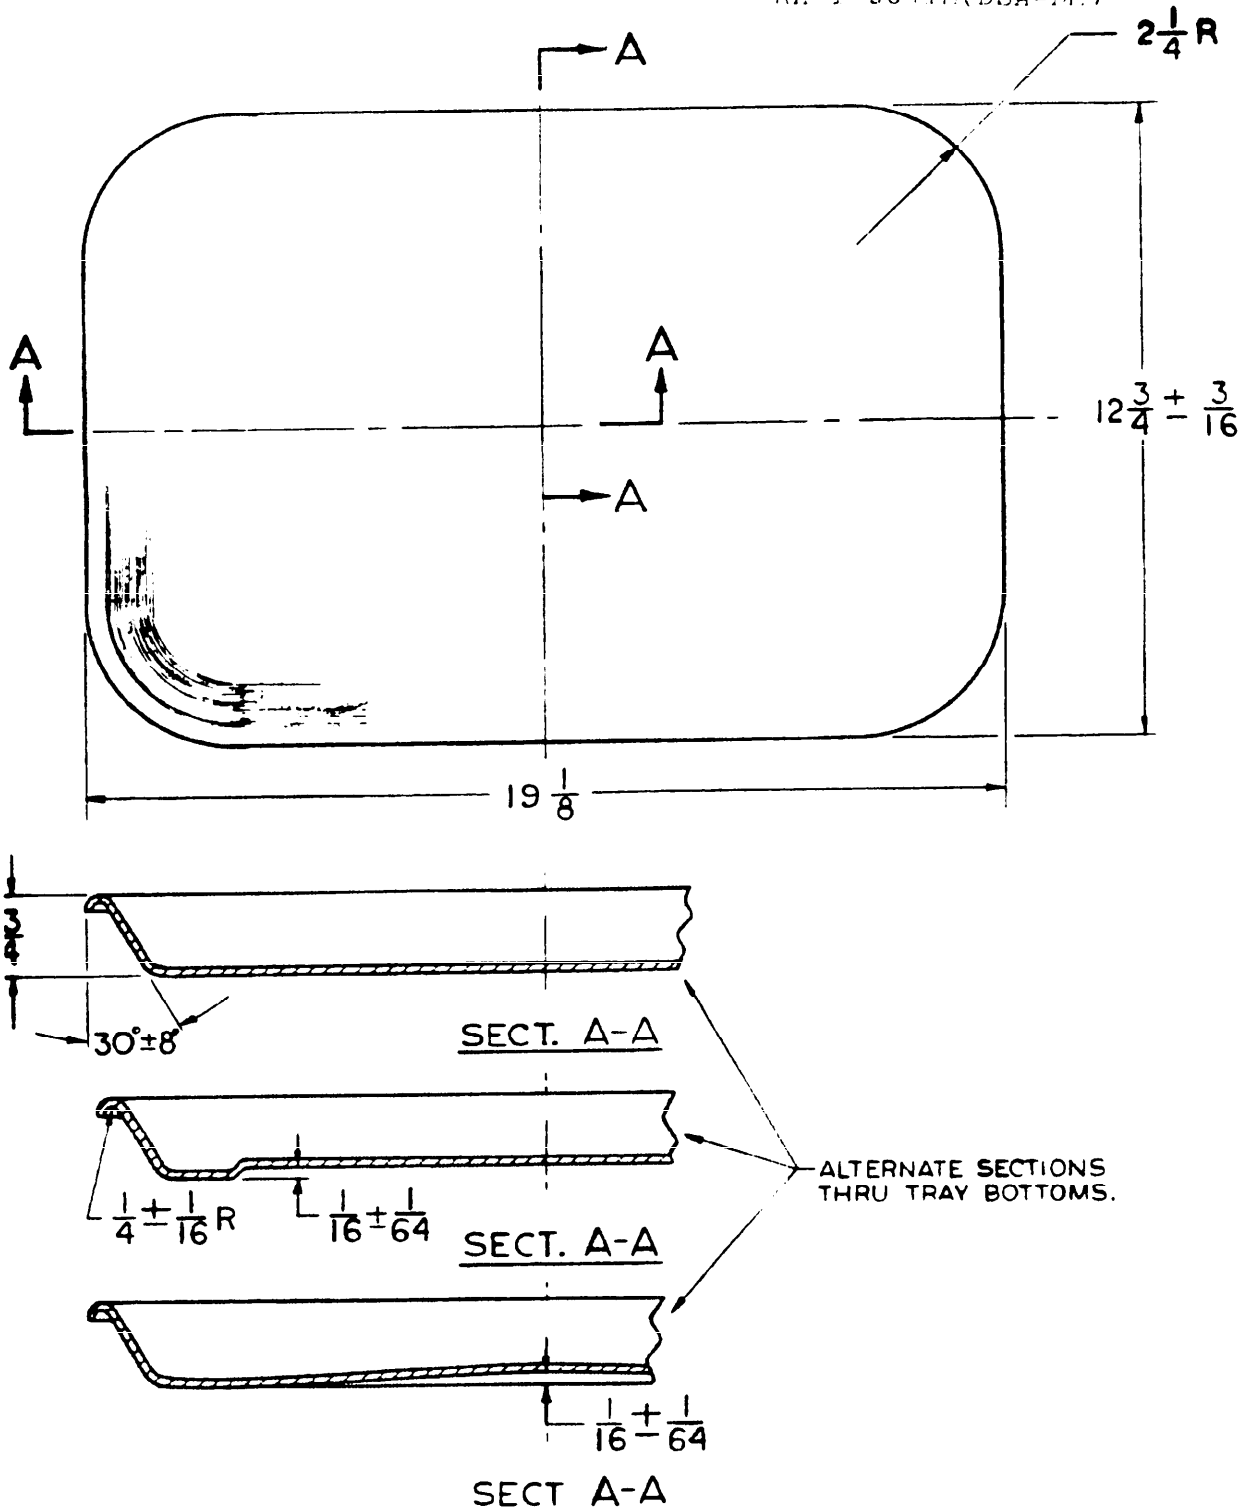


FIGURE 2

-Trays

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:38Z
Check the source to verify that this is the current version before use.

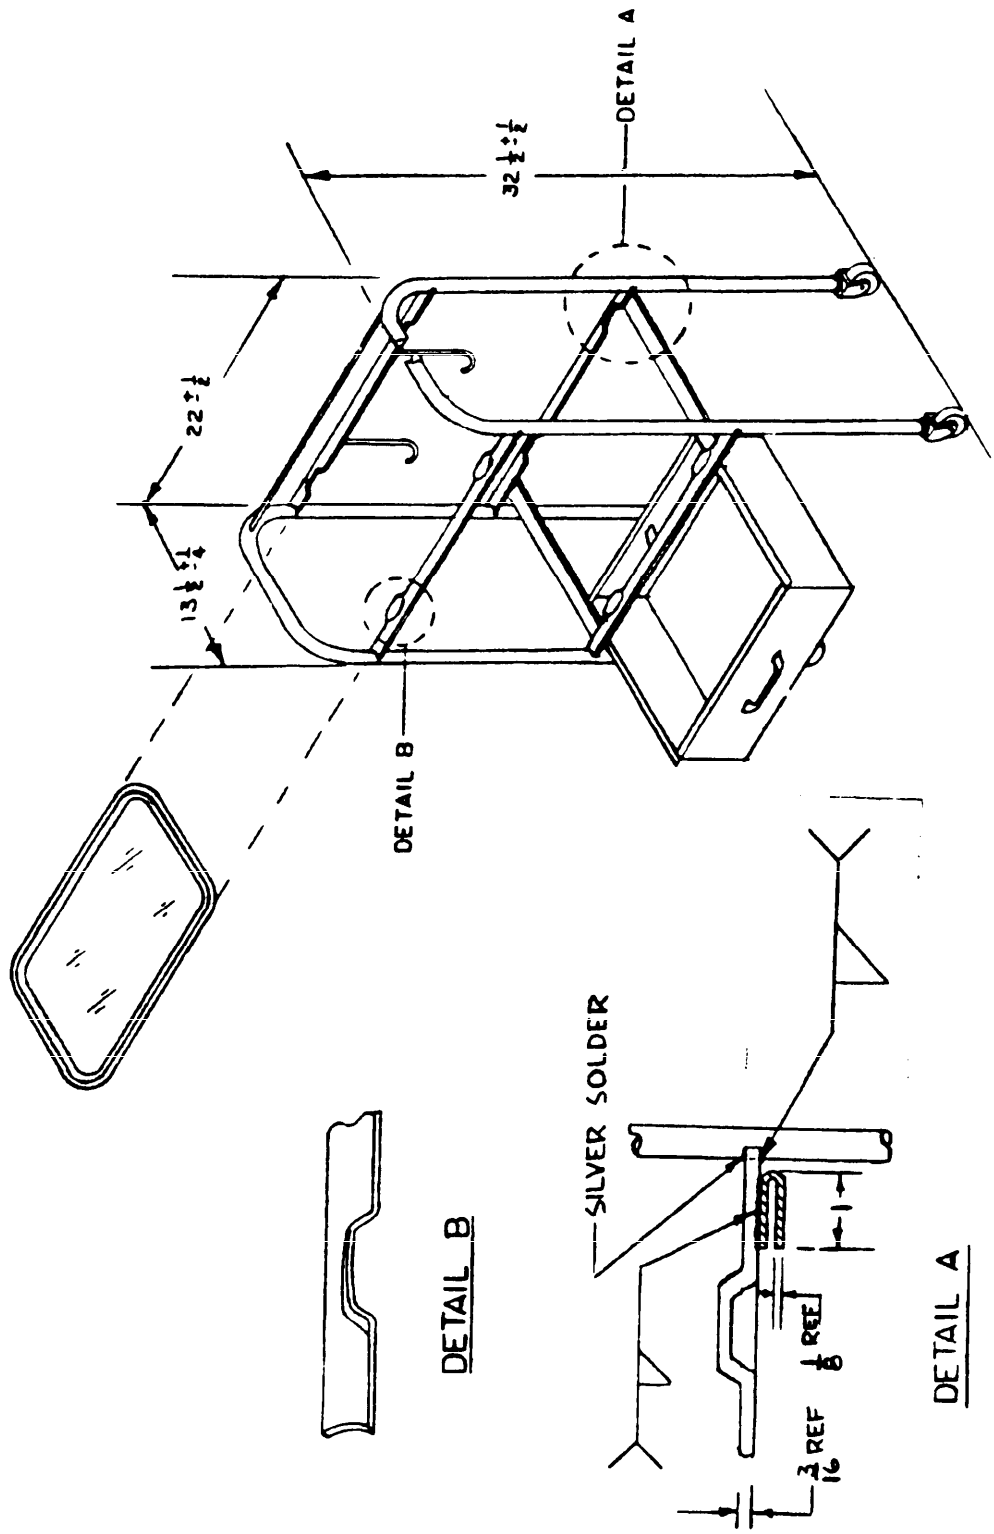


FIGURE 3

Alternate Construction to Anesthetist's Table

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:38Z
Check the source to verify that this is the current version before use.

3.2.1 Uprights. The uprights shall form the legs and shall consist of two inverted U-shaped, round, 1-inch outside-diameter tubes. Each leg shall be equipped with a caster. The tubing shall not be flattened at the bends. The legs on the assembled table shall be straight from the end of the bend to the floor end.

3.2.2 Casters. The tables shall be mounted on four 2-inch diameter ball bearing casters which conform to Type II, Class B, style b or c, Mounting A requirements of FF-C-77. All exposed metal parts of the casters shall be bright zinc or cadmium plated.

3.2.3 Tray frames. Two tray frames shall be joined to the uprights with 1/4 inch corrosion-resisting steel rod as shown in Figure 1. The frames shall be constructed of 1/8 inch by 1 inch strip having dimensions as indicated in Figure 1, and curved corners for accomodating the rim of the tray. As an alternate to the above construction, a 1/8 inch by 1 inch flat corrosion-resisting steel bar, having raised sections and welded as shown in Figure 3, may be used. Each tray frame shall have opposite sides parallel to each other within ± 1/16 inch for both the horizontal and vertical axes.

3.2.4 Braces and guardrail. For tables constructed as shown in Figure 1, two 3/8 inch diameter corrosion-resisting steel rods shall be welded between the two back legs, and similar rods shall be welded on both sides between the legs. The side braces shall be fillet welded on both ends. Tables constructed using the alternate construction (figure 3) shall only have a 3/8 inch diameter corrosion-resisting steel rod welded as shown for the guardrail. Hooks shall be either 3/8 inch steel diameter rod or 1/8 by 3/4 inch steel round edge flat stock welded as shown in figures 1 and 3.

3.2.5 Trays. Two trays, as shown in figure 2, shall be provided, which shall properly fit on the frames. The corners shall be slightly rounded. Trays shall be formed from a single piece of corrosion-resisting steel not less than 0.0375 inch thick.

3.2.6 Drawer. Below the lower shelf shall be a drawer not less than 4 inches deep inside, hemmed on back and two sides, which shall occupy the full width between the frames. A one-piece drawer is acceptable. The drawer shall operate on channel suspension slides, spot welded to the side of the drawer. Drawer shall be suspended on channel suspension slides welded to the table legs so that drawer assembly is rigidly positioned. Alternate drawer suspension is shown in figure 3. The drawer shall have a positive metal stop to prevent inadvertent removal of the drawer, but shall be so designed as to permit removal of the drawer for cleaning purposes. Positive means shall be provided to keep the drawer in the closed position while the stand is being wheeled. The drawer front shall extend the full width between the front legs.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:38Z
Check the source to verify that this is the current version before use.

* 3.2.6.1 Drawer pull. The pull may be of brass, bronze, steel corrosion-resisting steel, or anodized aluminum. Where brass or bronze pulls are furnished, they shall be plated with chromium over nickel. Where steel pulls are furnished, they shall be plated over chromium over nickel over copper. The pull shall be secured in the center of the outside surface of the front of the drawer in a manner which shall prevent the knob from turning after attachment.

3.3 Dimensions. Dimensions shall be as shown on figures 1, 2 and 3.

* 3.4 Finish.

3.4.1 Table and tray. The entire inside and outside surfaces of the table and tray shall be furnished with a No. 4 commercial finish after all surface imperfections have been removed by previous grinding. Tubing shall be turned, ground and polished to match the adjacent finish of the table. The last grinding shall produce a uniform finished surface with all imperfections and marks of previous grind removed. The thickness of the sheet shall not be reduced below 0.033 inch by grinding to remove surface imperfections.

3.4.2 Tray.

3.4.2.1 Alternate finish. As an alternate, the interior and/or exterior of the tray may be finished by electropolishing. The electropolishing shall result in a uniform, bright, shiny surface which can be readily cleaned.

3.4.2.2 Cleaning. As a final operation, the trays shall be thoroughly cleaned to remove foreign particles such as dirt, grease, graphite, and metal.

* 3.5 Identification marking.

3.5.1 Table. Each table shall be permanently and legibly marked by stamping or by a metal nameplate securely attached thereto by welding or riveting. The marking shall include national stock number, manufacturer's name or registered trademark, and contract or purchase order number. If a nameplate is used on the table, it shall be located in an inconspicuous place.

3.5.2 Tray. Each tray shall have impressed on the underside the name or registered trademark of the manufacturer of the tray. All impressions shall be made at even pressure so as not to penetrate the inside surface of the tray. Markings secured by adhesives shall not be used.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:38Z
Check the source to verify that this is the current version before use.

* 3.6 Stability.

3.6.1 Uprights. The tables shall be tested as specified in 4.4.3.1 for rock in either lateral axis. Distance between the bottom of any of the caster wheels and the floor surface shall not exceed 1/16 inch.

3.6.2 Trays. A maximum of 1/8 inch wobble shall be allowed in a side to side motion when the tray is placed on the tray frame when tested in accordance with 4.4.3.2.

* 3.7 Workmanship. The tables and trays shall be smoothly and properly finished, and shall be free from defects which detract from their appearance or which may impair their serviceability.

3.7.1 Welding. Welding shall be durable, sound in every detail and in accordance with latest practices recommended by the American Welding Society. All welds shall be produced by qualified welding operators with satisfactory welding equipment using satisfactory filler metal and electrode where applicable to provide the best possible weld. Surfaces to be welded shall be free from grease, oil, oxides or any other foreign matter. Any cleaning method which will remove these substances and leave the surface clean is satisfactory. All weld joints shall blend into the adjacent metal in gradual, smooth curves. Beads shall be smooth and free of slag, excessive undercut, or excessive spatter. Sufficient metal shall be added to provide a suitable fillet or reinforcement unless otherwise specified. Fusion through the full thickness of the base metal, in areas other than those where 100 percent penetration is a requirement of joint design, is not acceptable when welding materials over 0.050 inches in thickness. Welds shall not be oxidized. All welds shall be continuous with no visible voids, pin holes, or cracks which affect the quality, and have more strength than required for the purpose intended. Any crevices which result during the fabrication of the tables shall be filled with a high quality silver solution. All the mating surfaces between the parts being welded are closed by welds without any breaks or voids. Grinding wheels used to remove excess weld material and to prepare weld surfaces for subsequent polishing operations shall be of a suitable grit free of metal filings or other materials such as iron oxides which would tend to cut into the parent metal surfaces and allow for rusting at a later date.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:38Z
Check the source to verify that this is the current version before use.

* 3.8 Tolerances. Tolerances on dimensions are for design purposes only and are not production tolerances. The manufacturer of the item required herein shall control fabrication to within + 1/32 inch of the manufacturer's design dimension. Where tolerances prescribed could cumulatively result in improper design the manufacturer shall provide a product with dimensions within the tolerances prescribed on the drawing to insure proper function fit, assembly and operation of the item.

* 4. QUALITY ASSURANCE PROVISIONS

4.1 Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the supplier is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or order, the supplier may use his own or any other facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements

4.1.1 Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government, upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of 3 years after delivery of the supplies to which such records relate.

4.1.2 Inspection. Inspection, as used in this specification, is defined as both examination (such as visual, and auditory, investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

4.1.3 Certificates of quality. Certificates of quality, supplied by the manufacturer of the tables may be furnished in lieu of actual performance of such testing by the contractor, provided lot identity has been maintained and can be demonstrated to the Government. The Certificate shall include the name of the contractor, the contract number, the name of the manufacturer or supplier, the NSN, the Item Identification, the name of the component/material, the lot number, the lot size, the sample size, the date of testing, the test method, individual test results, and the specification requirements.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:38Z
Check the source to verify that this is the current version before use.

4.2 Sampling.

4.2.1 For visual examination. Sampling procedures for visual examination shall be conducted in accordance with MIL-STD-105 and Table I.

Table I. Sampling for Visual Examination

	Inspection level	AQL (percent defective)	Minimum sample size
For visual examination:			
Major defects ------	II	1.0	--
Total (Major and minor combined) defects	II	4.0	--
For dimensional examination	S-4	2.5	3

4.2.2 For tests. Sample sizes for tests shall be as indicated for inspection level S-2 in MIL-STD-105, except that the acceptance number shall be zero for all sample sizes, and a minimum of three (3) samples shall be taken.

4.3 Examination. The tables and trays shall be examined to determine compliance with all requirements contained in this specification.

4.3.1 Classification of defects. Examination shall be conducted in accordance with the classification of defects listed in Table II.

Table II. Classification of Defects

Categories and defects	
Major	
101	Unit not complete with all required parts.
102	Components and mating parts not properly aligned or fitted.
103	Metal components not free of cracks, tears, ruptures, or deformed surfaces.
104	Edges, corners, or surfaces not free of burs, sharpness, or sharp projections.
105	Drawer slides not functioning smoothly and easily.
106	Casters do not move freely without binding.
Minor	
201	Identification marking not complete, not legible, or not permanently attached on table or trays.
202	Drawer not provided with positive metal stop to prevent inadvertent removal of the drawer.

cont'd

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:38Z
Check the source to verify that this is the current version before use.

Classification of Defects* (Cont'd)

Minor

203	Drawer not prevented from opening when table is rolled.
204	Drawer pull not secured to prevent knob from turning.
205	Drawer not removable for cleaning.
206	Finish not uniform or not free of coarse grind marks or scratched areas.
207	Welds (tack, fillet, and spot) not sound or not free of pits, flux, splatter, and discoloration.
208	Unit not clean or free of foreign matter.
209	Bends of uprights not smoothly and uniformly accomplished

* Examination shall not be restricted to the classified possible defects listed above.

4.3.2 Dimensional examination. The table and trays shall be examined for defects in dimensions. Any dimension not within the tolerances specified herein shall be classified as a defect.

4.4 Tests. Tests shall be conducted, as necessary, to determine compliance with specification requirements.

4.4.1 Conductivity of Table. Test for electrical conductivity shall be conducted on table as described in section 469 of National Fire Protection Association, NFPA No. 56A.

4.4.2 Chemical composition. Tests for chemical analysis shall be conducted in accordance with method 111.2 or 112.2 of FED-STD-15 In lieu of the above, a certificate of quality, may be furnished, showing results of tests performed to indicate that material is as specified in 3.1.

* 4.4.3 Stability.

* 4.4.3.1 Uprights. The table shall be placed on a level surface and examined for rocking conditions in both lateral directions. The distance between the bottom of the caster wheels and the floor surface shall be recorded for any caster wheel not resting on the floor surface.

* 4.4.3.2 Trays. Each tray shall be placed in a tray frame and examined for improper fit or wobbling. Trays which will not seat flush in the frame or wobble more than 1/8 inch in either lateral axis when placed on the tray frame are classified as defect

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:38Z
Check the source to verify that this is the current version before use.

4.5 Examination for preparation for delivery. An examination shall be made to determine whether the packaging, packing, and marking comply with the requirements of Section 5. Defects shall be scored as specified in Table III. Sampling shall be in accordance with MIL-STD-105. The sample unit shall be one container fully prepared for delivery. The lot shall be the number of containers offered for inspection at one time. The inspection level shall be S-2 and the acceptable quality level shall be 4.0 defects per hundred units.

Table III. Examination for Preparation for Delivery

Examination	Defect
Containers	Not as specified.
Quantity	Quantity in interior packages and shipping containers not as specified.
Packaging and Packing Materials	Any component missing or damaged.
Workmanship	Inadequate application of components, such as incomplete closure of container flaps, tape improperly applied, or containers distorted.
Markings	Omitted, incorrect, illegible, improper size, location, sequence, or method of application.

5. PREPARATION FOR DELIVERY

5.1 Packaging. Packaging shall be level A or C as specified, (see 6.1).

5.1.1 Level A.

5.1.1.1 Unit preparation. Casters shall be removed, packaged in a bag of suitable size and design, and secured to the unit. Trays shall be wrapped in noncorrosive paper and the package secured in such manner as to prevent shifting or damage. Each unit shall be further protected by wrapping with noncorrosive paper or other suitable material. Cushioning shall be interposed between points of contact of the container and wrapped unit. The required wrapping and cushioning material shall be secured in position.

5.1.3 Level C. Unit shall be packaged in standard commercial containers of the size and kind commonly used, which will afford the degree of protection required for shipment and use of the product for its intended purpose.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:38Z
Check the source to verify that this is the current version before use.

5.2 Packing. Packing shall be level A, B, or C as specified (see 6.1).

* 5.2.1 Level A. Each table shall be packed in an exterior container designed for a type 3 load and constructed in accordance with PPP-B-585, Class 3, style 3; PPP-B-601, overseas type; PPP-B-621, class 2; or PPP-B-640, class 2, style E. Container shall be designed with suitable interior fittings or shall contain sufficient cushioning material to prevent shifting of or damage to the unit. Closure and strapping shall be as specified in the applicable box specification.

* 5.2.1.1 Case liner. Each Level A wood box shall be lined with a waterproof case liner conforming to MIL-L-10547. Closure and sealing shall conform to applicable paragraphs of appendix thereto. Case liner shall not be required for fiberboard boxes. Each fiberboard box shall be sealed as specified in PPP-B-640.

* 5.2.2 Level B. Table unit shall be packed in an exterior container designed for a type 3 load and constructed in accordance with PPP-B-585, class 1, style 3; PPP-B-601, domestic type; PPP-B-621, class 1; or PPP-B-640, class 2, style E. Container shall be designed with suitable interior fittings or shall contain sufficient cushioning material to insure against shifting of or damage to the contents. Closure shall be as specified in the applicable box specification.

5.2.3 Level C. The subject commodity shall be packed in substantial commercial containers of the type, size, and kind commonly used for the purpose, so constructed as to insure acceptance and safe delivery by common or other carriers, at the lowest rate, to point of delivery called for in the contract or purchase order.

5.3 Marking.

5.3.1 Civil Agencies. In addition to any special marking specified in the contract or order, shipping containers shall be marked in accordance with FED-STD-123.

5.3.2 Military agencies. Shipping containers shall be marked in accordance with MIL-STD-129.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:38Z
Check the source to verify that this is the current version before use.

6. NOTES

6.1 Ordering data. Procurement documents should specify the following:

(a) Title, number, and date of this specification.
(b) Selection of applicable levels of packaging and packing (see 5.1 and 5.2).

6.2 This specification covers the following item appearing in the Federal Supply Catalog:

National Stock No.	Item Identification
6530-00-708-8425	TABLE, ANESTHETIST'S, Corrosion-Resisting Steel

6.3 This specification does not cover all types, classes, grades, or sizes of the commodity indicated by the title of this specification, or those which are commercially available, but is intended to cover the types which are normally procured to meet requirements.

6.4 The margins of this specification are marked with an asterisk to indicate where changes (additions, modifications, corrections, deletions) from the previous issue were made. This was done as a convenience only and the Government assumes no liability whatsoever for any inaccuracies in these notations. Bidders and contractors are cautioned to evaluate the requirements of this document based on the entire content irrespective of the marginal notations and relationship to the last previous issue.

Custodians:
Army - MD
Navy - MS
Air Force - 03

Preparing activity:
Defense Supply Agency - DM

Project No. 6530-1353
is

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:38Z
Check the source to verify that this is the current version before use.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:38Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

OMB Approval
No. 22-R255

INSTRUCTIONS: The purpose of this form is to solicit beneficial comments which will help achieve procurement of suitable products at reasonable cost and minimum delay, or will otherwise enhance use of the document. DoD contractors, government activities, or manufacturers/ vendors who are prospective suppliers of the product are invited to submit comments to the government. Fold on lines on reverse side, staple in corner, and send to preparing activity. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements. Attach any pertinent data which may be of use in improving this document. If there are additional papers, attach to form and place both in an envelope addressed to preparing activity.

DOCUMENT IDENTIFIER AND TITLE
AA-T-0041E(DSA-DM) TABLE, ANESTHETIST'S

NAME OF ORGANIZATION AND ADDRESS

CONTRACT NUMBER

MATERIAL PROCURED UNDER A
☐ DIRECT GOVERNMENT CONTRACT ☐ SUBCONTRACT

1. HAS ANY PART OF THE DOCUMENT CREATED PROBLEMS OR REQUIRED INTERPRETATION IN PROCUREMENT USE?
   A. GIVE PARAGRAPH NUMBER AND WORDING.

   B. RECOMMENDATIONS FOR CORRECTING THE DEFICIENCIES

2. COMMENTS ON ANY DOCUMENT REQUIREMENT CONSIDERED TOO RIGID

3. IS THE DOCUMENT RESTRICTIVE?
   ☐ YES ☐ NO *(If "Yes", in what way?)*

4. REMARKS

SUBMITTED BY *(Printed or typed name and address - Optional)*

TELEPHONE NO.

DATE

DD FORM 1 JAN 72 1426 REPLACES EDITION OF 1 JAN 66 WHICH MAY BE USED

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:38Z
Check the source to verify that this is the current version before use.

FOLD

DEFENSE PERSONNEL SUPPORT CENTER
2800 South 20th Street
Philadelphia, PA 19101

POSTAGE AND FEES PAID
DEFENSE SUPPLY AGENCY
DoD - 304

U.S. MAIL

OFFICIAL BUSINESS
PENALTY FOR PRIVATE USE $300

HEADQUARTERS, DEFENSE PERSONNEL SUPPORT CENTER
ATTN: DIRECTORATE OF MEDICAL MATERIEL, CODE ATT
2800 SOUTH 20TH STREET
PHILADELPHIA, PA 19101

FOLD

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:38Z
Check the source to verify that this is the current version before use.