AA-T-41c
SEPTEMBER 20, 1960
SUPERSEDING
Fed. Spec. AA-T-41b
August 21, 1958

FEDERAL SPECIFICATION

TABLE, ANESTHETIST'S

This specification was approved by the Commissioner, Federal Supply Service, General Services Administration, for the use of all Federal agencies.

1. SCOPE

1.1 This specification covers corrosion-resisting steel anesthetist tables with two removable trays and one drawer under the lower tray, suitable for use in hospitals and doctors offices.

2. APPLICABLE SPECIFICATIONS, STANDARDS, AND OTHER PUBLICATIONS

2.1 **Specifications and standards.**—The following specifications and standards, of the issues in effect on date of invitation for bids, form a part of this specification:

Federal Specifications:

QQ–S–766 — Steel Plates, Sheets, and Strip Corrosion Resisting.
UU–P–271 — Paper, Wrapping, Water-Proofed Kraft.
PPP–B–585—Boxes, Wood, Wirebound.
PPP–B–601 — Boxes, Wood, Cleated-Plywood.
PPP–B–621 — Boxes, Wood, Nailed and Lock-Corner.
PPP–B–640—Boxes, Corrugated, Triple Wall, 350-Pound Maximum Weight.
PPP–T–76 — Tape, Pressure Sensitive Adhesive Paper, Water Resistant.

Federal Standards:

Fed. Std. No. 102 — Preservation, Packaging, and Packing Levels.
Fed. Std. No. 123 — Marking for Domestic Shipment (Civilian Agencies).
Fed. Test Method Std. No. 151—Metals; Test Methods.

(Activities outside the Federal Government may obtain copies of Federal Specifications, Standards, and Handbooks as outlined under General Information in the Index of Federal Specifications, Standards, and Handbooks and at the prices indicated in the Index. The Index, which includes cumulative monthly supplements as issued, is for sale on a subscription basis by the Superintendent of Documents, U. S. Government Printing Office, Washington 25, D. C.

(Single copies of this specification and other product specifications required by activities outside the Federal Government for bidding purposes are available without charge at the General Services Administration Regional Offices in Boston, New York, Atlanta, Chicago, Kansas City, Mo., Dallas, Denver, San Francisco, Los Angeles, Seattle, and Washington, D. C.

(Federal Government activities may obtain copies of Federal Specifications, Standards, and Handbooks and the Index of Federal Specifications, Standards, and Handbooks from established distribution points in their agencies.)

Military Specifications:

MIL–A–101 — Adhesive, Water-Resistant, for Sealing Fiberboard Boxes.
MIL–B–10377 — Box, Wood, Cleated, Veneer, Paper Overlaid.

Military Standards:

MIL–STD–105 — Sampling Procedures and Tables for Inspection by Attributes.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:38Z
Check the source to verify that this is the current version before use.

MIL–STD–129 — Marking for Shipment and Storage.

(Copies of Military Specifications and Standards required by contractors in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.)

2.2 Other publications. — The following document forms a part of this specification. Unless otherwise indicated, the issues in effect on date of invitation for bids shall apply.

National Board of Fire Underwriters:

NBFU — No. 56 — Standards of the National Board of Fire Underwriters for the Use of Flammable Anesthetics as recommended by the National Fire Protection Association.

(Application for copies should be addressed to the National Board of Fire Underwriters, 85 John St., New York 38, N. Y.; 222 West Adams Street, Chicago 6, Ill.; and 465 California St., San Francisco 4, Calif.)

3. REQUIREMENTS

3.1 Material.—Tables shall be constructed of corrosion-resisting steel, conforming to class 302, finish 4, of Federal Specification QQ–S–766, and shall meet the requirements for chemical composition specified therein when tested as specified in 4.3.3. Thicknesses of material shall be as shown in table I. Commercial tolerances on gages shall apply.

TABLE I.—*Thickness of material*

Section	Thickness	
	Gage	*Inch*
Leg	No. 16 Birmingham Wire	0.065
Drawer body	No. 24 U. S. Standard	.025
Drawer front	No. 16 U. S. Standard	.062
Drawer channels	No. 18 U. S. Standard	.050
Drawer hanger	No. 12 U. S. Standard	.109
Frames	No. 11 U. S. Standard	.125
Trays	No. 20 U. S. Standard	.037

3.2 Design and construction. — The unit shall consist of a table, complete with two trays and a drawer, as shown on figures 1 and 2.

3.2.1 *Uprights.*—The uprights shall form the legs and shall consist of two inverted U-shaped, round, 1-inch-outside-diameter tubes. Each leg shall be equipped with a caster.

3.2.2 *Casters.*—The casters shall be ball-bearing with metal-expanding stems, having a 2-inch molded-type wheel, with a 0.75-inch tread. The wheels shall consist of electrically conductive rubber, so compounded and molded as to result in a hard, strong core or body, and a soft, resilient, live tread securely vulcanized to the core. All exposed metal parts of the casters shall be bright zinc or cadmium plated. Casters shll pass the conductivity test specified in 4.3.1.


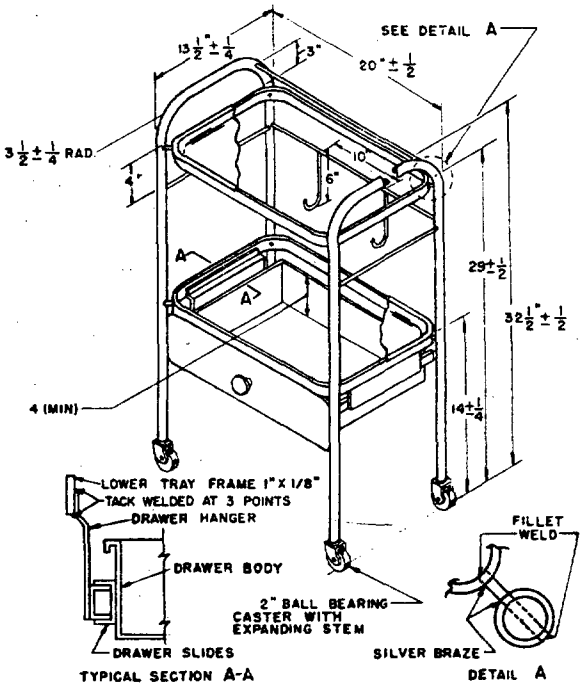


FIGURE 1.

3.2.3 *Tray frames.*—Two tray frames shall be joined to the uprights as shown on figure 1. The frames shall be constructed of ⅛- by 1¼-inch strap, and shall be 18⅜ ± 1/16 inches long by 12⅜ ± 1/16 inches wide, with curved corners to accommodate the rim of the tray.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:38Z
Check the source to verify that this is the current version before use.

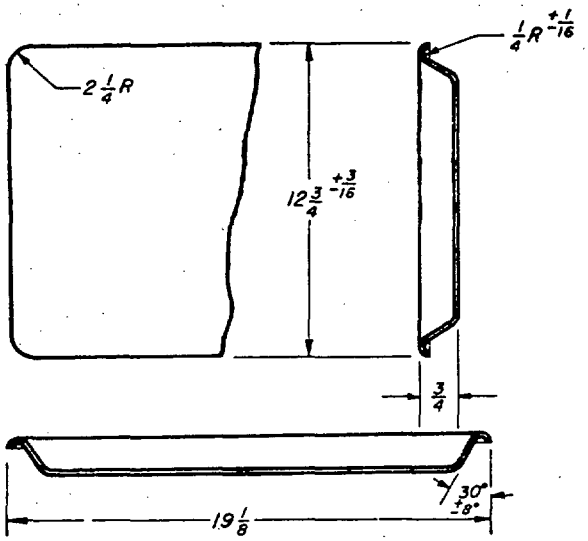

Note.—Tol. ±1/8 unless otherwise specified

FIGURE 2.

3.2.4 *Braces.* — A 3/8-inch-diameter rod shall be welded between the two back legs, and similar rods shall be welded on both sides between the legs. Two 6-inch ± 1/8 steel hooks, made of 3/8-inch-diameter rod, or 1/8- by 3/4-inch round edge flat stock, shall be welded to the back rod. Hooks shall have a radius of 1/2 to 1 inch.

3.2.5 *Guardrail.* — A guardrail, formed from 3/8-inch-diameter rod, shall be welded between the two back legs.

3.2.6 *Trays.* — Two trays, as shown on figure 1, shall be provided, which shall properly fit on the frames. The corners shall be slightly rounded. Trays shall be formed from a single piece of corrosion-resisting steel not less than 0.0375 inch thick.

3.2.7 *Drawer.* — Below the lower shelf shall be a drawer not less than 4 inches deep inside, hemmed on back and two sides, which shall occupy the full width between the frames. The drawer shall operate on channel suspension slides, spotwelded to the side of the drawer. The hangers shall be tackwelded to the side members of the lower frame. Drawer shall be suspended on channel suspension slides welded to drawer hangers so that drawer assembly is rigidly positioned. The drawer shall have a positive metal stop to prevent inadvertent removal of the drawer, but shall be so designed as to permit removal of the drawer for cleaning purposes. Suitable means shall be provided to keep the drawer in closed position while stand is being wheeled.

3.2.7.1 *Drawer pull.*—The drawer pull shall be round, plain, 1-inch-diameter, single-knob type, with threaded pommel base. The pull may be of brass, bronze, steel, corrosion-resisting steel, or anodized aluminum. Where brass or bronze pulls are furnished, they shall be plated with chromium over nickel. Where steel pulls are furnished, they shall be plated with chromium over nickel over copper. The pull shall be secured in the center of the outside surface of the front of the drawer by a special washer and machine screw which shall prevent the knob from turning after attachment.

3.3 Dimensions. — Dimensions shall be as shown on figures 1 and 2.

3.4 Finish.

3.4.1 *Table and tray.*—The entire inside and outside surfaces of the table and tray shall be finished with a No. 4 commercial finish after all surface imperfections have been removed by previous grinding. The last grinding shall produce a uniform finished surface with all imperfections and marks of previous grinds removed. The thickness of the sheet shall not be reduced below 0.033 inch by grinding to remove surface imperfections.

3.4.2 *Tray.*

3.4.2.1 *Alternate interior finish.* — As an alternate, the interior of the tray only may be finished by electropolishing. The electropolishing shall result in a uniform, bright, shiny surface which can be readily cleaned.

3.4.2.2 *Cleaning.*—As a final operation, the

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:38Z
Check the source to verify that this is the current version before use.

trays shall be thoroughly cleaned to remove foreign particles such as dirt, grease, graphite, and metal.

3.4.2.3 *Corrosion resistance.* — Finished trays shall be subjected to the salt-spray test specified in 4.3.2. Slight surface corrosion of the specimen which can be washed off shall not be considered cause for rejection, but if the specimen should rust or show continuous bleeding from pits, it shall be considered as having failed to pass the test.

3.5 **Identification marking.** — Each table and tray shall be permanently marked with the following information:

Stock number.

Manufacturer's name or registered trademark.

Contract or order number.

U.S.

A metal nameplate, permanently attached in an inconspicuous place, may be used on the table. Markings shall be impressed on each tray. All impressions shall be made at even pressure so as not to penetrate the inside surface of the tray. Marking secured by adhesives shall not be used.

3.6 **Workmanship.**—The tables and trays shall be smoothly and properly finished, and shall be free from defects which detract from their appearance or which may impair their serviceability.

3.6.1 *Welding.*—Welding rod shall be of material similar in composition to the welded members. Welds shall be thorough, nonporous, free of pits, cracks, or other imperfections. All welds shall be cleaned and all surfaces shall be free from sharp edges. All exposed welds shall be ground and finished smooth to match adjoining surfaces.

4. SAMPLING, INSPECTION AND TEST PROCEDURES

4.1 Sampling.

4.1.1 *For visual examination.* — Sampling procedures for visual examination shall be conducted in accordance with the procedures set forth in Military Standard MIL–STD–105.

	Inspection level	*AQL (percent defective)*	*Minimum sample size*
For visual examination:			
Major defects -----	II	1.0	--
Total (major and minor combined) defects ----------	II	4.0	--
For dimensional examination ----------	L5	2.5	2

4.1.2 *For tests.* — Sample sizes for tests shall be as indicated for inspection level L–2 in Military Standard MIL–STD–105, except that the acceptance number shall be zero for all sample sizes, and a minimum of three (3) samples shall be taken.

4.2 **Examination.** — The tables and trays shall be examined to determine compliance with all requirements contained in this specification.

4.2.1 *Classification of defects.* — Examination shall be conducted in accordance with the following classification of defects:

*Categories and defects**

Major

101. Unit not complete with all required parts.
102. Components and mating parts not properly aligned or fitted.
103. Metal components not free of cracks, tears, ruptures, and deformed surfaces.
104. Exposed or accesible edges, corners, and surfaces not free of burs, sharpness, or sharp projections.
105. Telescoping drawer slides do not function smoothly and easily.
106. Tray frames do not satisfactorily accommodate trays.

Minor

201. Casters not in accordance with 3.2.2.
202. Identification marking not complete, not legible, and not permanently attached on table and trays.
203. Drawer pull not provided with positive metal stop.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:38Z
Check the source to verify that this is the current version before use.

204. Drawer pull not secured to prevent knob from turning.
205. Drawer not removable for cleaning.
206. Stainless steel finish not uniform and not free of coarse grind marks and scratched areas.
207. Welds (tack, filet, and spot) not sound and not free of pits, flux, splatter, and discoloration.
208. Unit not clean and free of foreign matter.
209. Bends of uprights not smoothly and uniformly accomplished.

* Examination shall not be restricted to the classified possible defects listed above.

4.2.2 *Dimensional examination.* — The table and trays shall be examined for defects in dimensions. Any dimension not within the tolerances specified herein shall be classified as a defect.

4.3 **Tests.**—Tests shall be conducted, as necessary, to determine compliance with specification requirements.

4.3.1 *Conductivity of rubber caster wheels.* — Test for electrical conductivity shall be conducted using equipment described in section 2522 (c) of National Board of Fire Underwriters, NBFU No. 56.

4.3.2 *Salt-spray test.* — Sample trays selected at random shall be tested for a period of 48 hours in accordance with method 811.1 of Federal Test Method Standard No. 151.

4.3.3 *Chemical composition.* — Tests for chemical analysis shall be conducted in accordance with method 111.1 or 112.1 of Federal Test Method Standard No. 151. In lieu of the above, a certificate of quality, showing results of tests performed to indicate that material is as specified in 3.1, may be furnished.

4.4 **Supplier responsibilities for inspection.** —The supplier is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified, the supplier may utilize his own or any other inspection facilities and services acceptable to the Government. Inspection records of the examination and tests shall be kept complete and available to the Government as specified in the contract or order. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

4.4.1 Inspection, as used in this specification, is defined as both examination (such as visual, auditory, etc., investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

5. PREPARATION FOR DELIVERY

Levels of preservation, packaging and packing protection used are defined in Federal Standard No. 102 (for civil agencies only).

5.1 **Packaging.**

5.1.1 *Unit of issue.*—One table, as specified, constitutes one unit.

5.1.2 *Packaging quantities.*—The number of units of issue indicated in table II shall be packaged in each unit, intermediate, and exterior container, as applicable, for the required level of protection specified in the procurement document.

TABLE II. — *Packaging quantities*

Federal stock number	Unit package	Intermediate package	Shipping container
6530–708–8425	1 unit	Not required	1 unit

5.1.3 *Level A.*

5.1.3.1 *Unit package.*—Casters shall be removed, packaged in a bag of suitable size and design, and secured to the unit. Trays shall be wrapped in kraft paper and the package

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:38Z
Check the source to verify that this is the current version before use.

secured in such manner as to prevent shifting or damage. Each unit shall be further protected by wrapping with kraft paper or other suitable material. Cushioning shall be interposed between points of contact of the container and wrapped unit. The required wrapping and cushioning material shall be secured in position.

5.1.4 *Level C.*—Unit shall be packaged in standard commercial containers of the size and kind commonly used, which will afford the degree of protection required for shipment and use of the product for its intended purpose within the continental limits of the United States of America.

5.2 Packing.

5.2.1 *Level A.* — Each unit shall be overpacked in an exterior container designed for type 3 load, and constructed in accordance with Federal Specification PPP–B–585; style 3, for class 3 use; PPP–B–601, table II, using type III, class 1 plywood, PPP–B–621, table IV; or Military Specification MIL–B–10377, table II. Container design shall include suitable interior fittings to prevent shifting or damage to the unit. Each unit shall be protected with a shroud fabricated of material conforming to Federal Specification UU–P–271. Closure of box shall comply with appendix of applicable specification. Strapping will not be required for shipments forwarded to a receiving activity within the continental limits of the United States for storage. As an alternate, exterior container may be a box conforming to the requirements of Federal Specification PPP–B–640. Box shall conform to class 2, style E, regular slotted. Container design shall include suitable interior fittings to prevent shifting or damage to the unit. Shroud will not be required. Top and bottom flaps shall be securely closed with a water-resistant adhesive conforming to the requirements of Military Specification MIL–A–101. The adhesive shall be applied to the entire area of contact between the flaps. Center seams shall be closed by means of tape conforming to the requirements of Federal Specification PPP–T–76. The tape shall be not less than 3 inches wide and shall extend at least 2 inches onto each of the end panels. When exterior containers are furnished in accordance with Federal Specification PPP–B–640, strapping shall be applied in accordance with 30.2.2 thereof.

5.2.2 *Level C.* — The subject commodity shall be packed in substantial commercial containers of the type, size, and kind commonly used for the purpose, so constructed as to insure acceptance and safe delivery by common or other carriers, at the lowest rate, to point of delivery called for in the contract or purchase order.

5.3 Marking.

5.3.1 *Civilian Agencies.* — In addition to any special marking specified in the contract or order shipping containers shall be marked in accordance with Federal Standard No. 123.

5.3.2 *Military agencies.* — Shipping containers shall be marked in accordance with Military Standard MIL–STD–129. Service color and service symbol markings are required only on direct shipments from the contractor's plant to overseas activities.

6. NOTES

6.1 Ordering data.—Purchasers should exercise any desired options offered herein, and procurement documents should specify the following:

(*a*) Title, number, and date of this specification.

(*b*) Selection of applicable levels of packaging and packing (see 5.1 and 5.2).

6.2 It is believed that this specification adequately describes the characteristics necessary to secure the desired material, and that normally no samples will be necessary prior to award to determine compliance with this specification. If, for any particular pur-

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:38Z
Check the source to verify that this is the current version before use.

pose, samples with bids are necessary, they should be specifically asked for in the invitation for bids, and the particular purpose to be served by the bid sample should be definitely stated, the specification to apply in all other respects.

6.3 Transportation description. — Transportation descriptions and minimum weights applicable to this commodity are:

Rail:

Tables, NOIBN, Steel. (Specify set-up or knocked-down).

Carload minimum weights:

In cars 40′9″ or less in length, inside measurements, 10,000, 12,000, 15,000, 18,000, 22,000 and 30,000 pounds.

In cars exceeding 40′9″ in length, inside measurements, 16,000, 18,000, 21,000, 24,000, 30,000 and 40,000 pounds.

Motor:

Tables, NOI, Steel. (Specify set-up or knocked-down).

Truckload minimum weights:

(W)10.6, (W)12.6, (W)15.6, (W)18.6, (W)22.6, and (W)30.6 pounds, (W) subject to Rule 34, National Motor Freight Classification.

Notice. — When Government drawings, specifications, or other data are used for any purpose other than in connection with a definitely related Government procurement operation, the United States Government thereby incurs no responsibility nor any obligation whatsoever; and the fact that the Government may have formulated, furnished, or in any way supplied the said drawings, specifications, or other data, is not to be regarded, by implication or otherwise as in any manner licensing the holder or any other person or corporation, or conveying any rights or permission to manufacture, use, or sell any patented invention that may in any way be related thereto.

MILITARY INTEREST:
Army—M
Navy—Md
Air Force.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:38Z
Check the source to verify that this is the current version before use.