AA-T-50D
January 28, 1976
SUPERSEDING
AA-T-0050C (DSA-DM)
March 24, 1971 and
AA-T-50a
July 19, 1957

FEDERAL SPECIFICATION

TABLE, EXAMINING

This specification was approved by the Commissioner, Federal Supply Service, General Services Administration, for the use of all Federal agencies.

1. SCOPE

1.1 Scope. This specification covers one type of corrosion-resisting steel table with adjustable top extension suitable for use in the general medical examinations of patients.

2. APPLICABLE DOCUMENTS

2.1 The following documents, of the issue in effect on date of invitation for bids or request for proposal, form a part of the specification to the extent specified herein.

Federal Specifications:

PPP-B-585	-	Boxes, Wood, Wirebound.
PPP-B-601	-	Boxes, Wood, Cleated-Plywood.
PPP-B-640	-	Boxes, Fiberboard, Corrugated, Triple-wall.
PPP-B-1055	-	Barrier Material, Waterproofed, Flexible.

Federal Standards:

Fed. Std. No. 66	-	Steel; Chemical Composition and Hardenability.
Fed. Std. No. 123	-	Marking for Shipment (Civil Agencies).
Fed. Test Method Std. No. 151	-	Metals; Test Methods.

FSC 6530

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:38Z
Check the source to verify that this is the current version before use.

(Activities outside the Federal Government may obtain copies of Federal Specifications, Standards, and Handbooks as outlined under General Information in the Index of Federal Specifications and Standards and at the prices indicated in the Index. The Index, which includes cumulative monthly supplements as issued, is for sale on a subscription basis by the Superintendent of Documents, U.S. Government Printing Office, Washington, DC 20402.

(Single copies of this specification and other Federal Specifications required by activities outside the Federal Government for bidding purposes are available without charge from Business Service Centers at the General Services Administration Regional Offices in Boston, New York, Washington, DC, Atlanta, Chicago, Kansas City, MO, Fort Worth, Denver, San Francisco, Los Angeles, and Seattle, WA.

(Federal Government activities may obtain copies of Federal Specifications, Standards, and Handbooks and the Index of Federal Specifications and Standards from established distribution points in their agencies.

Military Specifications:

MIL-W-530 - Webbing, Textile, Cotton, General Purpose, Natural or in colors.

Military Standards:

MIL-STD-105 - Sampling Procedures and Tables for Inspection by Attributes.
MIL-STD-129 - Marking for Shipment and Storage.

(Copies of Military Specifications and Standards required by suppliers in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.)

2.2 Other publications. The following document forms a part of this specification to the extent specified herein. Unless otherwise indicated, the issue in effect on date of invitation for bids or request for proposal shall apply:

National Fire Protection Association (NFPA) Standard:

No. 56A - Standard for the Use of Inhalation Anesthetics.

(Application for copies should be addressed to the National Fire Protection Association, 60 Batterymarch Street, Boston, MA 02110.)

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:38Z
Check the source to verify that this is the current version before use.

3. REQUIREMENTS

3.1 Preproduction sample. Unless otherwise specified (see 6.2), before production is commenced, a sample of the finished commodity on contract and each component part thereof shall be submitted or made ready for the contracting officer or his authorized representative to examine and test to determine compliance with this document. Approval of the preproduction sample authorizes the commencement of production but does not relieve the contractor of responsibility for compliance with all other provisions of this document. Production units shall not vary from the preproduction sample in design or construction without written approval by the contracting officer.

3.2 Material.

3.2.1 Sheets, strips, angles, tubes, bars, rods, and hardware. Sheets, strips, angles, tubes, bars, rods, and hardware, used in the fabrication of the patient examining table, shall be corrosion-resisting steel conforming to AISI 302 or 304 of Fed. Std. No. 66 and shall comply with the chemical requirements specified herein, when tested as specified in 4.4.1.

3.2.2 Webbing. The material used in the fabrication of the leg holder straps shall be 1 inch wide white webbing conforming to type IIa, class 2 of MIL-W-530.

3.3 Design and construction. Shall be fabricated from corrosion-resisting steel, and shall be constructed in accordance with figures 1 and 2, and as specified herein. Commercial tolerances on the thickness dimensions of corrosion-resisting steel shall be acceptable. Except for specified bends, bowing or deviation from straightness of any tubular member shall not exceed 1/8 inch over the total length of the member. Tolerances on other dimensions shall be as specified in figures 1 and 2.

3.3.1 Tabletop. The tabletop shall be fabricated from corrosion-resisting sheet steel formed around a rectangular butt-welded frame of corrosion-resisting steel bars. Four holes shall be provided in the tabletop for the leg holder rods. These holes shall be fashioned so that the sheet metal flares downward into the top of the leg tubing. The holes shall be smoothly finished. The adjusting mechanism shall secure the tabletop extension at the horizontal position, at least two positions above and at least four positions below the horizontal.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:38Z
Check the source to verify that this is the current version before use.

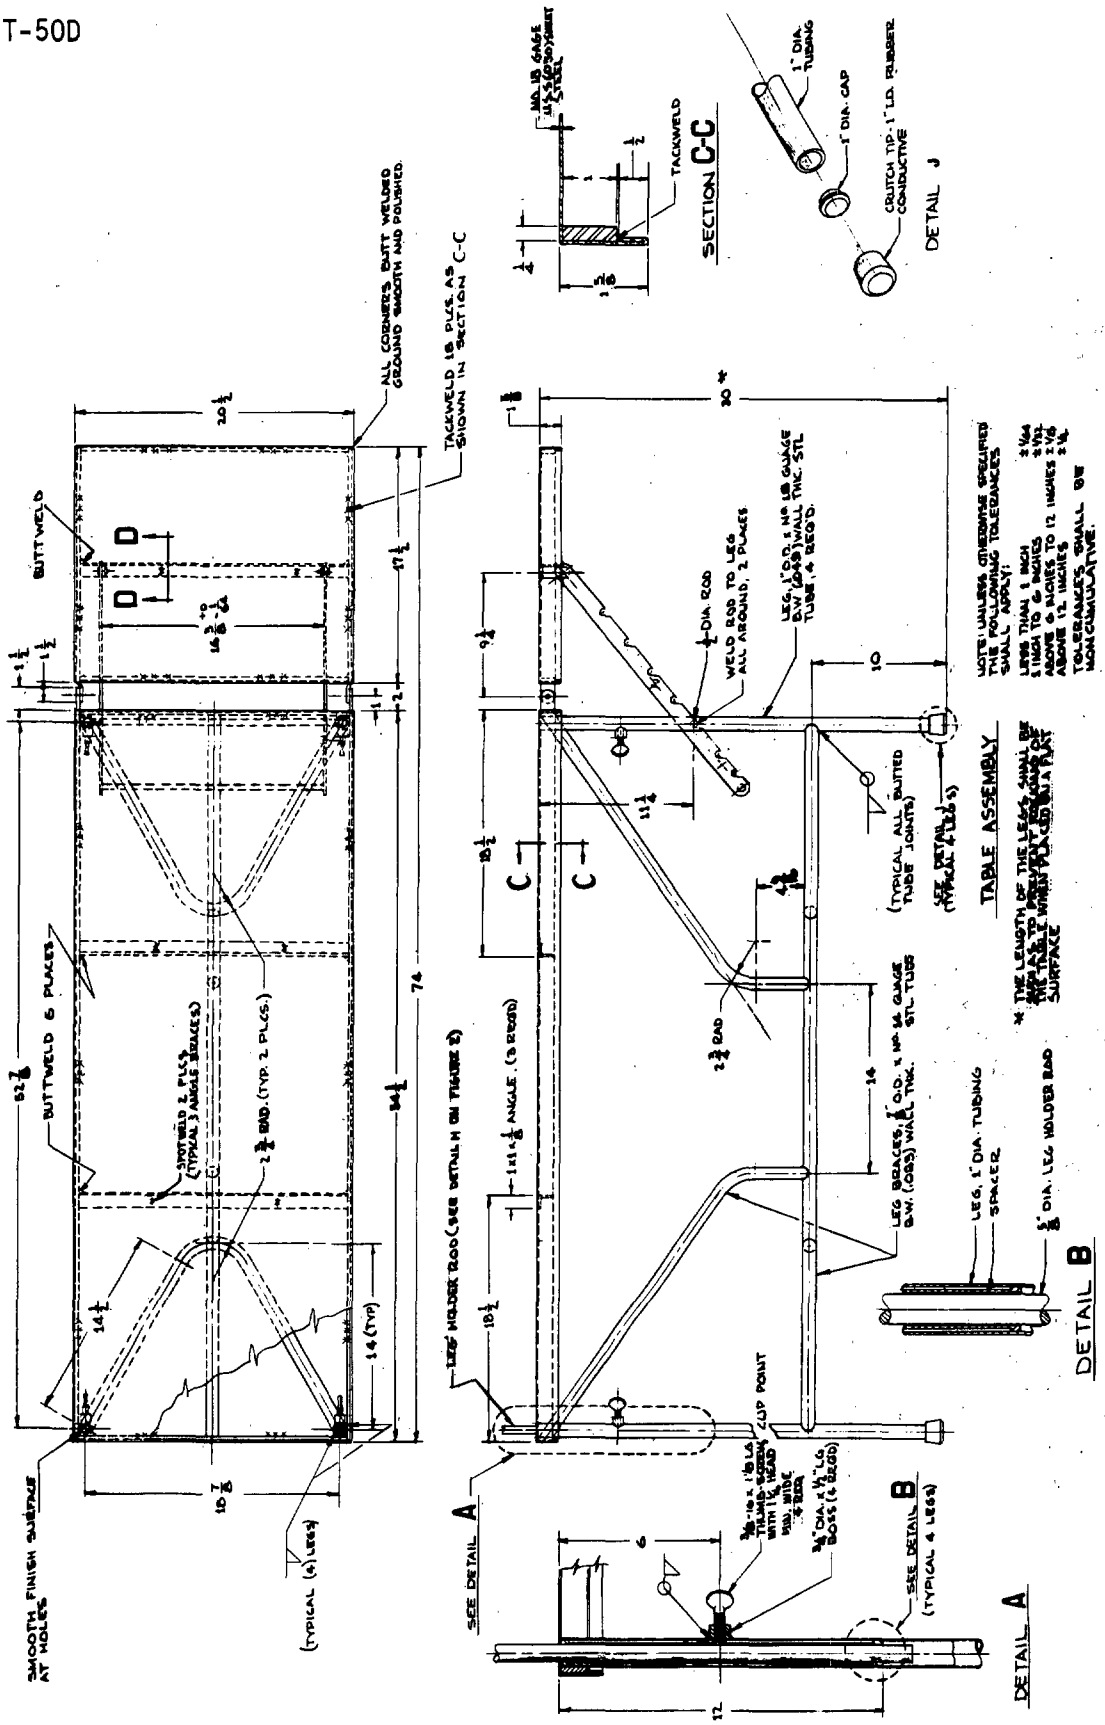


Figure 1. Examining table.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:38Z
Check the source to verify that this is the current version before use.

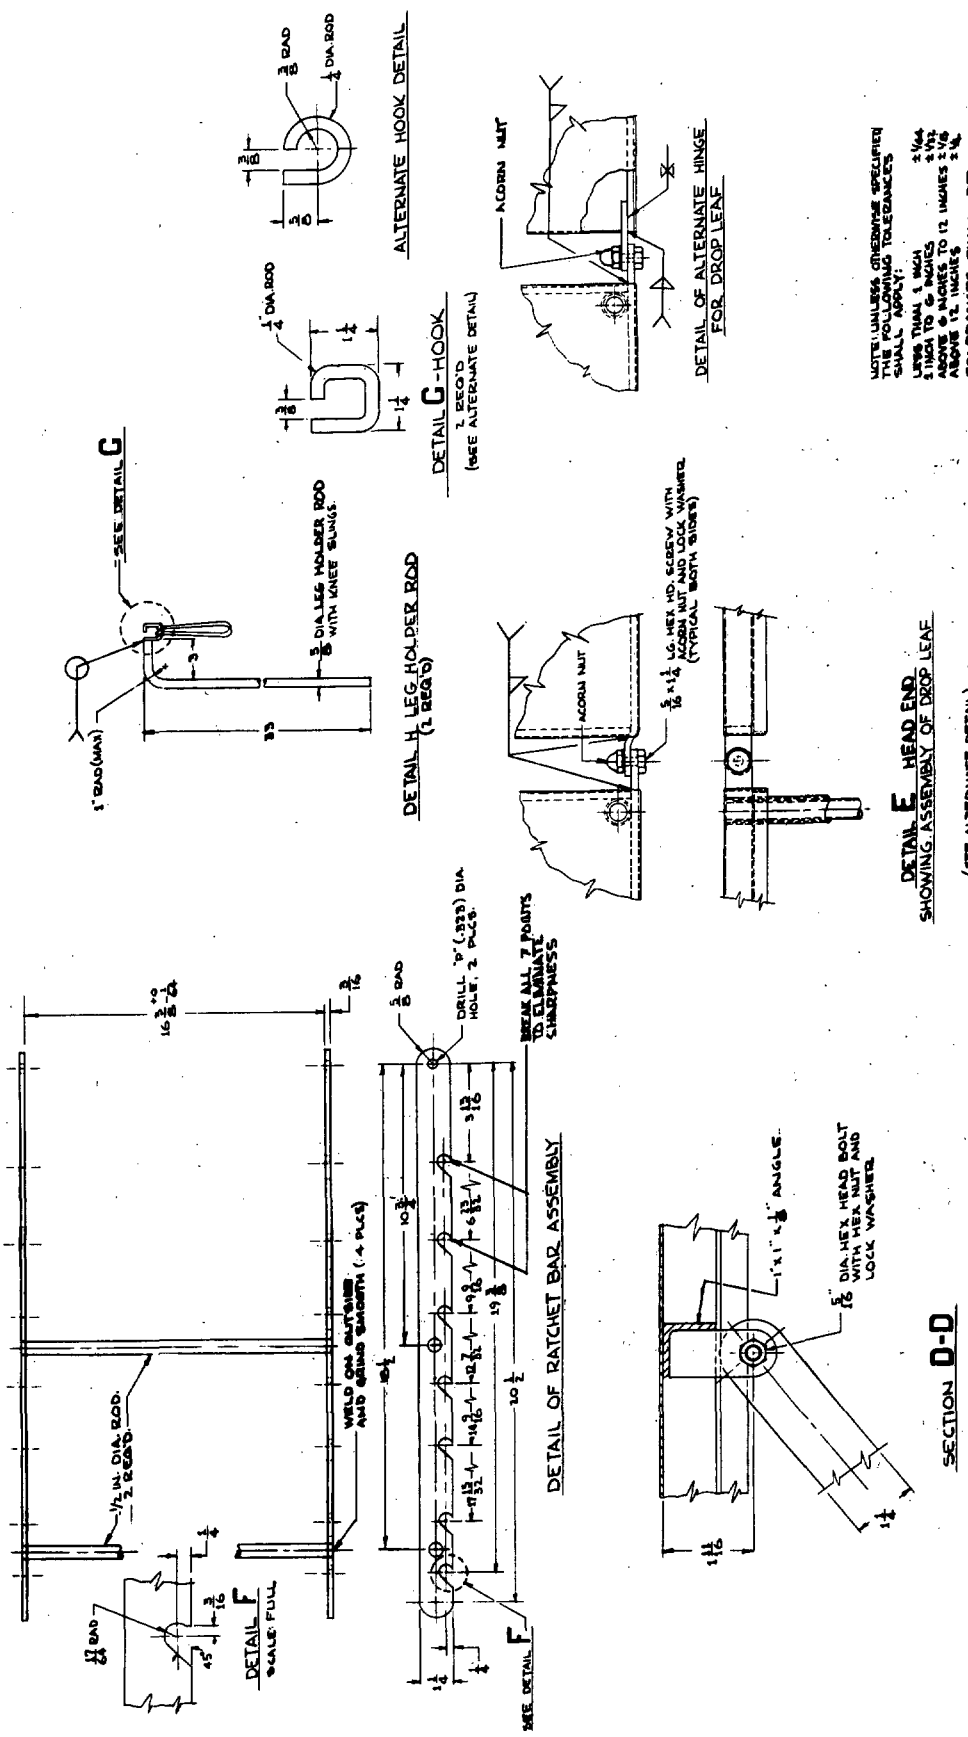


Figure 2. Examining table, detail.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:38Z
Check the source to verify that this is the current version before use.

3.3.2 Legs. A leg shall be securely welded to each corner of the fixed tabletop. Each leg shall be provided with an insert liner, as specified in 3.3.2.1, and a securely welded embossment, threaded with a thumbscrew capable of applying sufficient pressure to hold the leg holder rod (see 3.3.3) in any desired position. The floor end of each leg shall be provided with a leakproof cap, smoothly ground and polished, which is retained securely in place, but which may be removed for cleaning and readily replaced, and an electrically conductive rubber tip, meeting the requirements of NFPA No. 56A when tested as specified in 4.4.2.

3.3.2.1 Leg insert. Insert liners, consisting of an inner and outer liner fabricated of 0.050 inch thick (No. 18, B.W. Gage) corrosion-resisting steel tubing, shall be welded in the top of each leg. The outer liner shall have a 7/8 inch outside diameter and the inner liner shall have a 3/4 inch outside diameter. As an alternate to the outer liner, a corrosion-resisting steel bushing, of such size as to provide a tight fit between the inner insert and the inside of the tubular leg, shall be provided at the upper and lower ends of the inner liner. The inside diameter of the inner insert shall be such as to allow a total clearance of 1/32 inch to 1/16 inch between the leg holder rod and the inner insert liner.

3.3.3 Leg holder rods and straps. The table shall be furnished with two corrosion-resisting steel leg holder rods suitable for insertion into any of the four tubular legs. A suspension hook shall be provided on each leg holder rod to hold the rings of the leg holder strap. The leg holder straps shall be fabricated of webbing (see 3.2.2) and shall be furnished with suitable corrosion-resisting steel, nickel or chromium plated brass "D" rings securely stitched in place by cross-box stitching, backstitched at least 1/2 inch at all ends and breaks. The overall length of each strap with rings shall be 22 inches $\pm$ 1/2 inch.

3.4 Finish. All exposed surfaces shall be finished to a Commercial Standard No. 4 finish. All other surfaces shall be finished in accordance with good commercial practice. All edges shall be free of burs or sharpness.

3.5 Performance under load.

3.5.1 Tabletop. With the top extension secured at the horizontal position, the table shall support an evenly distributed load of 300 pounds without failure or deformation of any component. The tabletop shall be tested for performance under load as specified in 4.4.3.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:38Z
Check the source to verify that this is the current version before use.

3.5.2 Tabletop extension. When elevated to the 55° position above the horizontal, the extension top shall support a weight of 60 pounds, evenly distributed along the end of the extension, without failure or deformation of any component. The extension shall be tested for performance under load as specified in 4.4.4.

3.6 Welding. The welding shall be durable and sound in every detail. The welding rods shall be of a composition similar to that of the welded members. Component members shall be carefully and properly aligned prior to welding into a permanent position as a straight, rigid, and level assembly. All exposed welds shall be ground smooth to eliminate traces of pit marks and seams, and shall be polished to blend with adjacent surface. Welds shall be free of undercutting, slag, or burned areas.

3.7 Workmanship. Workmanship shall be first class throughout. Examining table shall be free from defects which detract from its appearance or may impair its serviceability. Metal parts shall be free of cracks, tears, ruptures, and deformed areas.

4. QUALITY ASSURANCE PROVISIONS

4.1 Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the supplier is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or order, the supplier may use his own or any other facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

4.1.1 Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government, upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

4.1.2 Inspection. Inspection, as used in this specification, is defined as both examination (such as visual and auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:38Z
Check the source to verify that this is the current version before use.

4.1.3 Certificates of quality. Certificates of quality, supplied by the manufacturer of the steel for the tables or webbing, may be furnished in lieu of acutal performance of such testing by the contractor, provided lot identity has been maintained and can be demonstrated to the Government. The certificate shall include the name of the contractor, the contract number, the name of the manufacturer or supplier, the NSN, the Item Identification, the name of the component or material, the lot number, the lot size, the sample size, the date of testing, the test method, individual test results, and the specification requirements.

4.2 Sampling.

4.2.1 For examination. Sampling for examination shall be conducted in accordance with MIL-STD-105, and table I.

TABLE I.

	Inspection level	AQL (defects per hundred units)
For visual examination		
Major defects	II	1.0
Minor defects	II	4.0
For dimensional examination	S-3	2.5

4.2.2 For tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and table II. The acceptance number shall be zero for all sample sizes.

TABLE II.

Component	Characteristic	Requirement	Test procedure	Inspection level
Metal	Chemical composition	3.2.1	4.4.1	(See 4.4.1)
Table	Electrical conductivity	3.3.2	4.4.2	100%
	Unit load bearing capability	3.5.1	4.4.3	S-1
	Extension load bearing capability	3.5.2	4.4.4	S-1

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:38Z
Check the source to verify that this is the current version before use.

4.3 Examination. The tables shall be examined to determine compliance with all requirements contained in this specification.

4.3.1 Classification of defects. Examination shall be conducted in accordance with the following classification of defects as shown in table III. Examination shall not be restricted to the classified possible defects listed below.

TABLE III.

Categories	Defects
Major	
101	Any component part not supplied, not useable.
102	Components not properly aligned or fitted.
103	Metal parts not free of cracks, tears, ruptures and deformed areas.
104	Welds not free of cracks, breaks, and undercutting.
105	Exposed or accessible edges not free of burrs and sharpness.
106	Welds not sound, not free of slag, burned areas.
107	Extension does not operate smoothly through required range, or does not lock firmly in all required positions.
108	Leg holder rods cannot be secured in any desired position.
109	Table does not rest evenly on a level surface without rocking.
Minor	
201	Finish not uniform, not free of scratches and coarse grind marks.
202	Any weld not continuous, not clean, not free of pitmarks, splatter, discoloration.
203	Unit not free of oil, grease, and imbedded foreign particles.

4.3.2 Dimensional examination. The tables shall be examined for defects in dimensions. Any dimension not within the tolerances specified herein shall be classified as a defect.

4.4 Tests. Tests shall be conducted, as necessary, to determine compliance with specification requirements.

4.4.1 Chemical composition. A sufficient quantity of metal used in the tables shall be tested for chemical composition in accordance with method 111 or 112 of Fed. Test Method Std. No. 151.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:38Z
Check the source to verify that this is the current version before use.

4.4.2 Electrical conductivity. The tables, complete with rubber tips, shall be tested as described in NFPA No. 56A.

4.4.3 Unit load bearing capability. With the tabletop extension secured at the horizontal position, an evenly distributed load of 300 pounds shall be placed on the load bearing surface.

4.4.4 Extension load bearing capability. With table extension elevated to the 55° position above the horizontal, a uniformly distributed load of 60 pounds shall be placed straight down along the extreme end of the extension.

4.5 Examination of preparation for delivery. An examination shall be made to determine compliance with the packaging, packing and marking requirements of section 5. Defects shall be scored as specified in table IV. Sampling shall be in accordance with MIL-STD-105. The sample unit shall be one container fully prepared for delivery. The lot shall be the number of containers offered for inspection at one time. The inspection level shall be S-2 with AQL of 4.0 expressed in terms of percent defective.

TABLE IV.

Examine	Defect
Contents	Not as specified.
Container	Not as specified.
Marking	Omitted; incorrect; illegible; improper size, location, sequence or method of application.
Material	Component missing or damaged.
Workmanship	Bulging or distoration of containers.

4.5.1 Examination of closure, waterproofing and banding of container. When the shipping container is required to comply with PPP-B-636, the examination for defects in closure, waterproofing or banding shall be in accordance with the appendix of the box specification.

5. PREPARATION FOR DELIVERY

5.1 Packaging. Packaging shall be level A or C as specified (see 6.2).

5.1.1 Level A.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:38Z
Check the source to verify that this is the current version before use.

5.1.1.1 Unit preparation. The tabletop extension shall be lowered to its lowest position and secured with tape or cord. The leg holder rods shall be lowered to their lowest position and secured. Leg straps shall be wrapped in kraft paper or other suitable material and secured to the table leg brace with tape or cord. All exterior finished surfaces shall be protected by wrapping with kraft paper and cushioned with corrugated fiberboard or other suitable material. Wrapping and cushioning shall be accomplished in such a manner to insure against damage to the unit.

5.1.2 Level C. Each table shall be protected by standard commercial methods commonly used for the purpose, which will afford the degree of protection required for shipment and use of the end product for its intended purpose. Work shall be accomplished in such a manner as to insure against marking, scratching, or damage to the unit.

5.2 Packing. Packing shall be level A, B or C as specified (see 6.2).

5.2.1 Level A. Each table shall be packed in an exterior container designed for a type 3 load and constructed in accordance with PPP-B-585, class 3, style 3; PPP-B-601, overseas type; or PPP-B-640, class 2. The table shall be blocked, braced or cushioned within the exterior container in such a manner to insure against shifting or damage. Wood boxes shall have all box panels, except the base, lined with a waterproof barrier material conforming to PPP-B-1055, class L-2. Fiberboard boxes shall be sealed against entry of water as specified in the appendix of PPP-B-640. Closure and strapping of exterior containers shall be as specified in the appendix of the applicable box specification except that the use of steel strapping is not authorized for fiberboard boxes.

5.2.2 Level B. Each table shall be packed as specified in 5.2.1 except that the boxes shall conform to PPP-B-585, class 1, style 3; PPP-B-601 domestic type; or PPP-B-640, class 1. Waterproofing shall not be required. Strapping shall not be required for wood boxes.

5.2.3 Level C. Each table shall be packed in substantial commercial containers of the type, size, and kind, commonly used for the purpose, so constructed as to insure acceptance and safe delivery by common or other carriers, at the lowest rate, to point of delivery called for in the contract or purchase order.

5.3 Marking.

5.3.1 Civil agencies. Marking for shipment shall be in accordance with Fed. Std. No. 123.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:38Z
Check the source to verify that this is the current version before use.

5.3.2 Military activities.

5.3.2.1 Interior packages. Each container shall be marked to identify contents.

5.3.2.2 Exterior container. Exterior container shall be marked in accordance with MIL-STD-129.

6. NOTES

6.1 Intended use. General use in medical examination of patients in medical treatment facilities.

6.2 Ordering data. Purchasers should select the preferred options permitted herein and include the following information in procurement documents.

(a) Title, number and date of this specification.
(b) Selection of applicable levels of packaging and packing (see 5.1 and 5.2).
(c) When preproduction sample is not required (see 3.1); all Department of Defense (DOD) activities see 6.3.
(d) When specific test facilities are required (see 4.1).

6.3 First Article instructions for DOD activities. The Armed Services Procurement Regulations (ASPR) Section No. 1, Part No. 9 and Section VII relate to First Article approval. The paragraphs within this specification shall be deleted by DOD activities and the requirements of the ASPR included in the contract or purchase order.

6.4 This specification covers the following item appearing in the Federal Supply Catalog:

National Stock Number	Item Identification
6530-00-709-3000	TABLE, EXAMINING, corrosion-resisting steel

6.5 This specification does not include all types, classes, styles or sizes of the commodity indicated by the title of this specification, or which are commercially available, but is itended to cover the items, which are normally procured to meet requirements.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:38Z
Check the source to verify that this is the current version before use.

MILITARY CUSTODIANS:
Army - MD
Navy - MS
Air Force - 03

Preparing activity:
DSA-DM

Civil Agency Coordinating Activity:
GSA-FSS

Project No. 6530-1350

Orders for this publication are to be placed with General Services Administration, acting as an agent for the Superintendent of Documents. See section 2 of this specification to obtain extra copies and other documents referenced herein. Price 40 cents each.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:38Z
Check the source to verify that this is the current version before use.

FOLD

DEFENSE PERSONNEL SUPPORT CENTER
2800 South 20th Street
Philadelphia, PA 19101

POSTAGE AND FEES PAID
DEFENSE SUPPLY AGENCY
DoD - 304

U.S.MAIL

OFFICIAL BUSINESS
PENALTY FOR PRIVATE USE $300

HEADQUARTERS, DEFENSE PERSONNEL SUPPORT CENTER
ATTN: DIRECTORATE OF MEDICAL MATERIEL, CODE ATT
2800 SOUTH 20TH STREET
PHILADELPHIA, PA 19101

FOLD

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:38Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

OMB Approval
No. 22-R255

•INSTRUCTIONS: The purpose of this form is to solicit beneficial comments which will help achieve procurement of suitable products at reasonable cost and minimum delay, or will otherwise enhance use of the document. DoD contractors, government activities, or manufacturers/ vendors who are prospective suppliers of the product are invited to submit comments to the government. Fold on lines on reverse side, staple in corner, and send to preparing activity. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements. Attach any pertinent data which may be of use in improving this document. If there are additional papers, attach to form and place both in an envelope addressed to preparing activity.

DOCUMENT IDENTIFIER AND TITLE

AA-T-50D - Table, Examining

NAME OF ORGANIZATION AND ADDRESS

CONTRACT NUMBER

MATERIAL PROCURED UNDER A

☐ DIRECT GOVERNMENT CONTRACT ☐ SUBCONTRACT

1. HAS ANY PART OF THE DOCUMENT CREATED PROBLEMS OR REQUIRED INTERPRETATION IN PROCUREMENT USE?

A. GIVE PARAGRAPH NUMBER AND WORDING.

B. RECOMMENDATIONS FOR CORRECTING THE DEFICIENCIES

2. COMMENTS ON ANY DOCUMENT REQUIREMENT CONSIDERED TOO RIGID

3. IS THE DOCUMENT RESTRICTIVE?

☐ YES ☐ NO *(If "Yes", in what way?)*

4. REMARKS

SUBMITTED BY *(Printed or typed name and address - Optional)*

TELEPHONE NO.

DATE

DD FORM 1 JAN 72 1426

REPLACES EDITION OF 1 JAN 66 WHICH MAY BE USED

S/N 0102-014-1802

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:38Z
Check the source to verify that this is the current version before use.