AA-T-55B
September 3, 1975
SUPERSEDING
Int. Fed. Spec. AA-T-0055a(DM)
November 2, 1964 and
Fed. Spec. AA-T-55
June 27, 1949

# FEDERAL SPECIFICATION

## TABLES, SURGICAL INSTRUMENT AND SURGICAL DRESSING (MOBILE)

This specification was approved by the Commissioner, Federal Supply Service, General Services Administration, for the use of all Federal agencies.

## 1. SCOPE AND CLASSIFICATION

1.1 Scope. This specification covers two types of mobile, surgical instrument and dressing tables (see 6.2 and 6.3).

1.2 Classification.

1.2.1 Types. The instrument and dressing tables shall be of the following types, as specified:

Type I - Angular-top.

Type II - Straight-top.

## 2. APPLICABLE DOCUMENTS

2.1 The following documents, of the issue in effect on date of invitations for bids or request for proposal, form a part of this specification to the extent specified herein:

Federal Specifications:

| | | |
|---|---|---|
| FF-C-77 | - | Casters, Rigid and Swivel (Institutional Duty). |
| PPP-B-585 | - | Boxes, Wood, Wirebound. |
| PPP-B-601 | - | Boxes, Wood, Cleated-Plywood. |
| PPP-B-621 | - | Boxes, Wood, Nailed and Lock-Corner. |
| PPP-B-636 | - | Boxes, Shipping, Fiberboard. |

FSC 6530

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:38Z
Check the source to verify that this is the current version before use.

Federal Specifications:

Fed. Std. No. 66 - Steel: Chemical Composition and Hardenability.
Fed. Test Method Std. No. 151 - Metals; Test Methods.

(Activities outside the Federal Government may obtain copies of Federal Specifications, Standards, and Handbooks as outlined under General Information in the Index of Federal Specifications and Standards and at the prices indicate indicated in the Index. The Index, which includes cumulative monthly supplements as issued, is for sale on a subscription basis by the Superintendent of Documents, US Government Printing Office, Washington, DC 20402.

(Single copies of this specification and other Federal Specifications required by activities outside the Federal Government for bidding purposes are available without charge from Business Service Centers at the General Services Administration Regional Offices in Boston, New York, Washington, DC, Atlanta, Chicago, Kansas City, MO, Fort Worth, Denver, San Francisco, Los Angeles, and Seattle, WA.

(Federal Government activities may obtain copies of Federal Specifications, Standards, and Handbooks and the Index of Federal Specifications and Standards from established distribution points in their agencies.

Military Specifications:

MIL-P-116 - Preservation-Packaging, Methods of.
MIL-L-10547 - Liners, Case, and Sheet, Overwrap, Water-Vaporproof or Waterproof, Flexible.

Military Standards:

MIL-STD-105 - Sampling Procedures and Tables for Inspection by Attributes.
MIL-STD-129 - Marking for Shipment and Storage.

(Copies of Military Specifications and Standards required by suppliers in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.)



Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:38Z
Check the source to verify that this is the current version before use.

2.2 Other publications. The following documents form a part of this specification to the extent specified herein. Unless a specific issue is identified, the issue in effect on date of invitation for bids or request for proposal shall apply.

National Fire Protection Association (NFPA):

56A - Standards for the Use of Inhalation Anesthetics.

(Application for copies should be addressed to the National Fire Protection Association, 60 Batterymarch Street, Boston, MA 02210.)

3. REQUIREMENTS

3.1 Material.

3.1.1 Corrosion-resisting steel. Corrosion-resisting steel used in the construction of instrument and dressing table shall be cold-rolled or drawn, and shall conform to type AISI 302 or 304 of Fed. Std. No. 66.

3.2 Construction.

3.2.1 Type I, angular-top table. Type I table shall be constructed as shown in figure 1.


3.2.1.1 Top. The top shall consist of Corrosion-resisting steel sheet, 0.0625 inch thick (No. 16, United States Standard (U.S.S.) gage), fabricated as shown in figure 1.

3.2.1.2 Framework. The table top shall be closely fitted over a similarly shaped framework shown in figure 1. The framework shall consist of reinforcing top frame, cross-braces and uprights (see 3.2.1.3). Top frame shall consist of five equally-spaced members. The top frame shall be constructed of 1 inch wide by 0.078 inch thick (No. 14 U.S.S. gage) corrosion-resisting steel.

3.2.1.3 Uprights. The table shall be supported by uprights located one at each corner of the table, and one each at front and back center. The legs shall be made of 1 inch outside diameter tubing. The tubing shall be corrosion-resisting steel, 0.065 inch thick (No. 16, Birmingham Wire (B.W.) gage). The uprights shall be reinforced by 3/4 inch-outside-diameter corrosion-resisting steel tubing, 0.049 inch thick(No. 18, B.W. gage), as shown in figure 2.



Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:38Z
Check the source to verify that this is the current version before use.

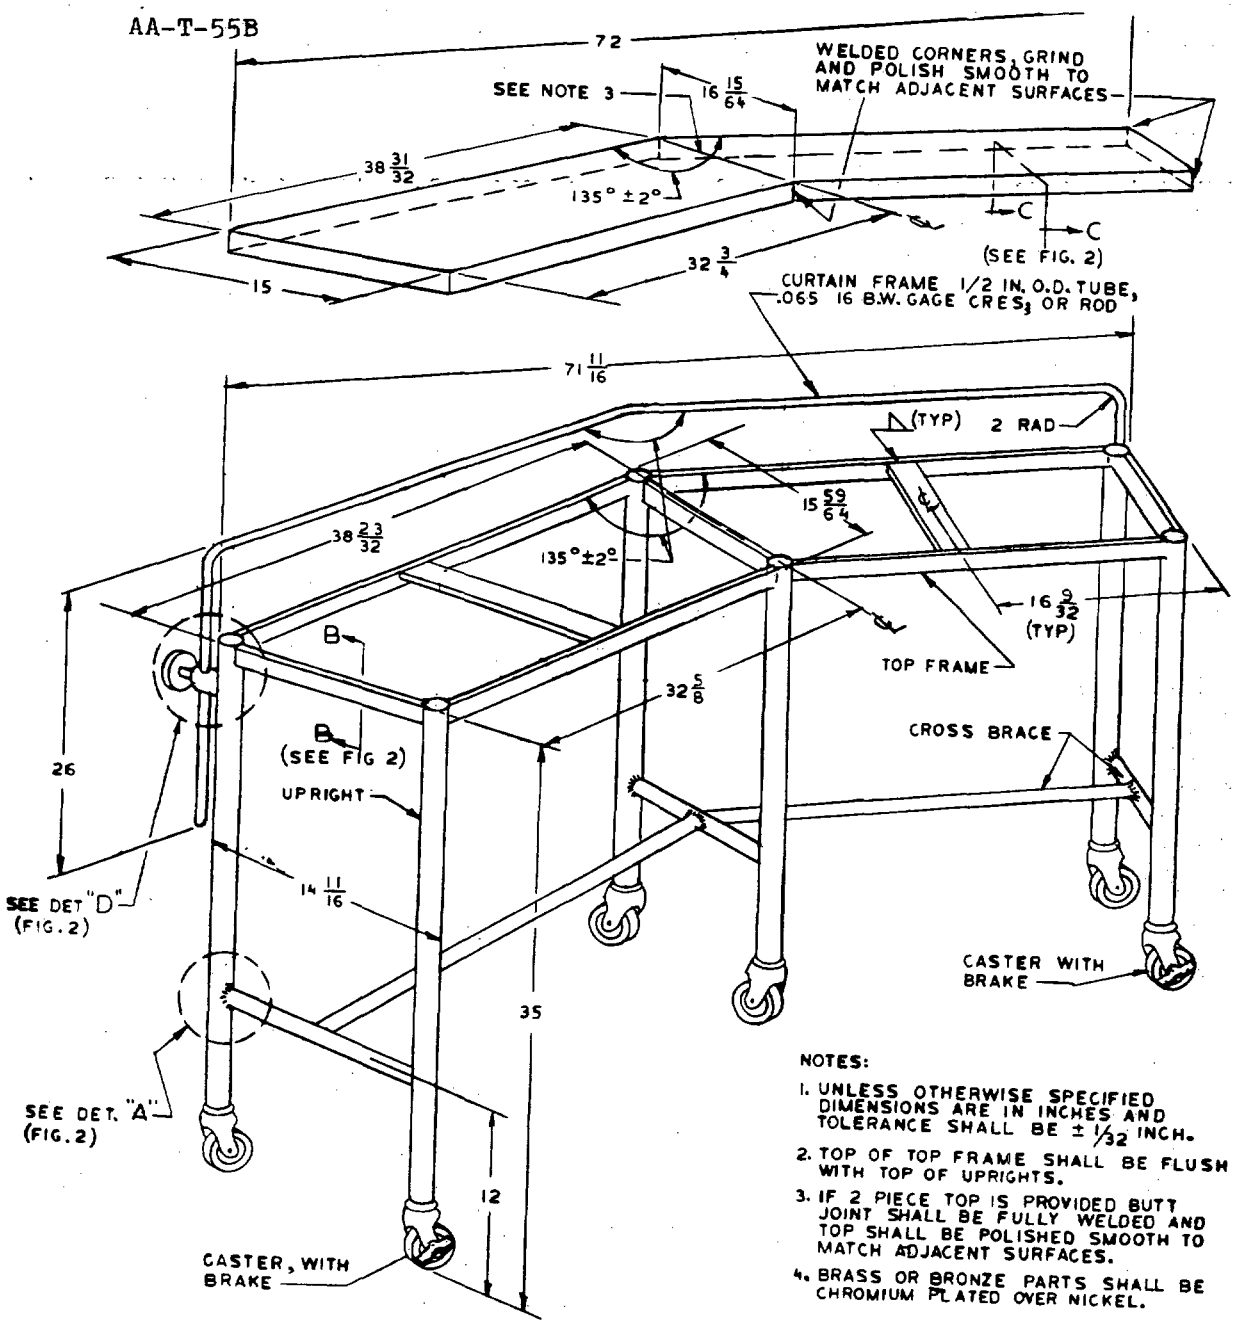



NOTES:


1. UNLESS OTHERWISE SPECIFIED DIMENSIONS ARE IN INCHES AND TOLERANCE SHALL BE ± 1/32 INCH.
2. TOP OF TOP FRAME SHALL BE FLUSH WITH TOP OF UPRIGHTS.
3. IF 2 PIECE TOP IS PROVIDED BUTT JOINT SHALL BE FULLY WELDED AND TOP SHALL BE POLISHED SMOOTH TO MATCH ADJACENT SURFACES.
4. BRASS OR BRONZE PARTS SHALL BE CHROMIUM PLATED OVER NICKEL.


Figure 1. Type I, angular-top

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:38Z
Check the source to verify that this is the current version before use.

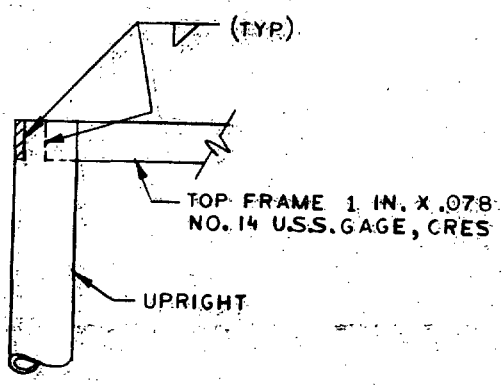



SECTION B-B

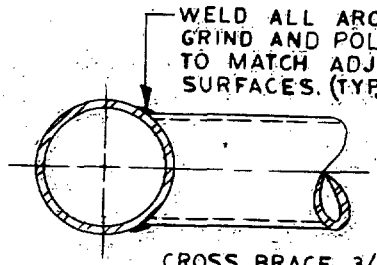


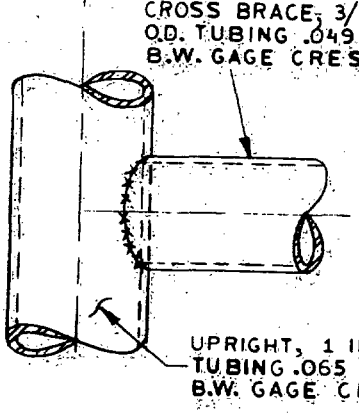
DETAIL "A"

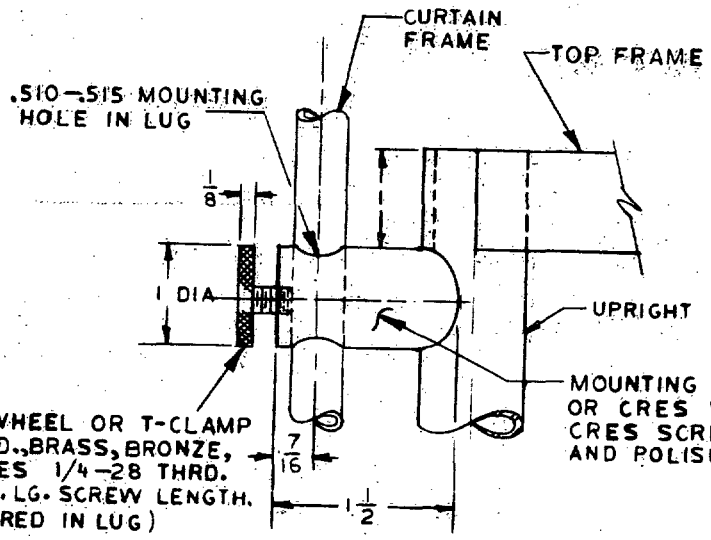


DETAIL "D"

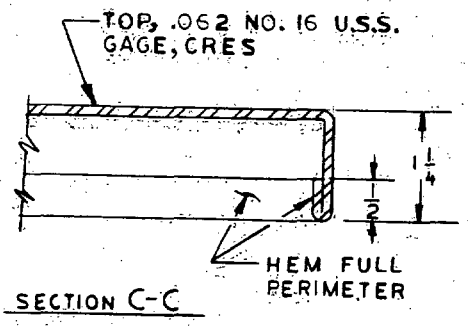


SECTION C-C

NOTE: 3/8 IN. TACK WELD, TOP TO FRAME (2 EACH END, 8 EACH SIDE) EQUALLY SPACED.

Figure 2. Type I, Angular-top, details



Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:38Z
Check the source to verify that this is the current version before use.

3.2.1.4 Mounting lugs. The two rear, corner, legs shall have mounting lugs directly below the tabletop apron. The mounting lugs shall be of brass, bronze, or corrosion-resisting steel, and shall be cast or machined from bar stock. The lugs shall be drilled through to accept the curtain frame (3.2.1.5). Each lug shall be fitted with a corrosion-resisting steel setscrew, having a cast brass, bronze or corrosion-resisting steel handwheel or "T" clamp for tightening against the curtain frame. Mounting lugs and handwheels, if made of brass or bronze, shall be chromium plated over nickel.

3.2.1.5 Curtain frame. The adjustable curtain frame shall be constructed from a continuous piece of 1/2 inch diameter corrosion-resisting steel tubing, 0.065 inch thick, (No. 16 B.W. gage), or rod.

3.2.1.6 Casters. The table legs shall be fitted with six electrically-conductive swivel casters (see 3.3) conforming to type II, class A, size 3, style b, mounting A or FF-C-77. The electrical conductivity requirement of FF-C-77 shall not apply, (see 3.3). Two casters shall have brakes. Casters shall also conform to the National Sanitation Foundation (NSF) requirements in FF-C-77.

3.2.2 Type II, straight-top table. Type II table shall be constructed as shown in figure 3.

3.2.2.1 Top and shelf. The top and shelf shall be made of corrosion-resisting steel sheets, 0.0625 inch thick (No. 16 United States Standard gage). All edges of the top and shelf shall be flanged downward and hemmed. Corners shall be notched to fit the contours of the uprights. The top shall be located 30 inches above the floor and the shelf 15 inches above the floor, as shown in figure 3.

3.2.2.2 Uprights. The table shall be supported by four uprights made from tubing 1 inch in outside diameter. The tubing shall be 0.049 inch thick (No. 18 (B.W.) gage) corrosion-resisting steel. The uprights shall extend 2 inches above the plane of the table (see 3.2.2.3).

3.2.2.3 Guardrail. The guardrail shall be 3/8 inch diameter corrosion-resisting steel rod or tubing, 0.049 inch thick, (No. 18 B.W. gage).



Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:38Z
Check the source to verify that this is the current version before use.

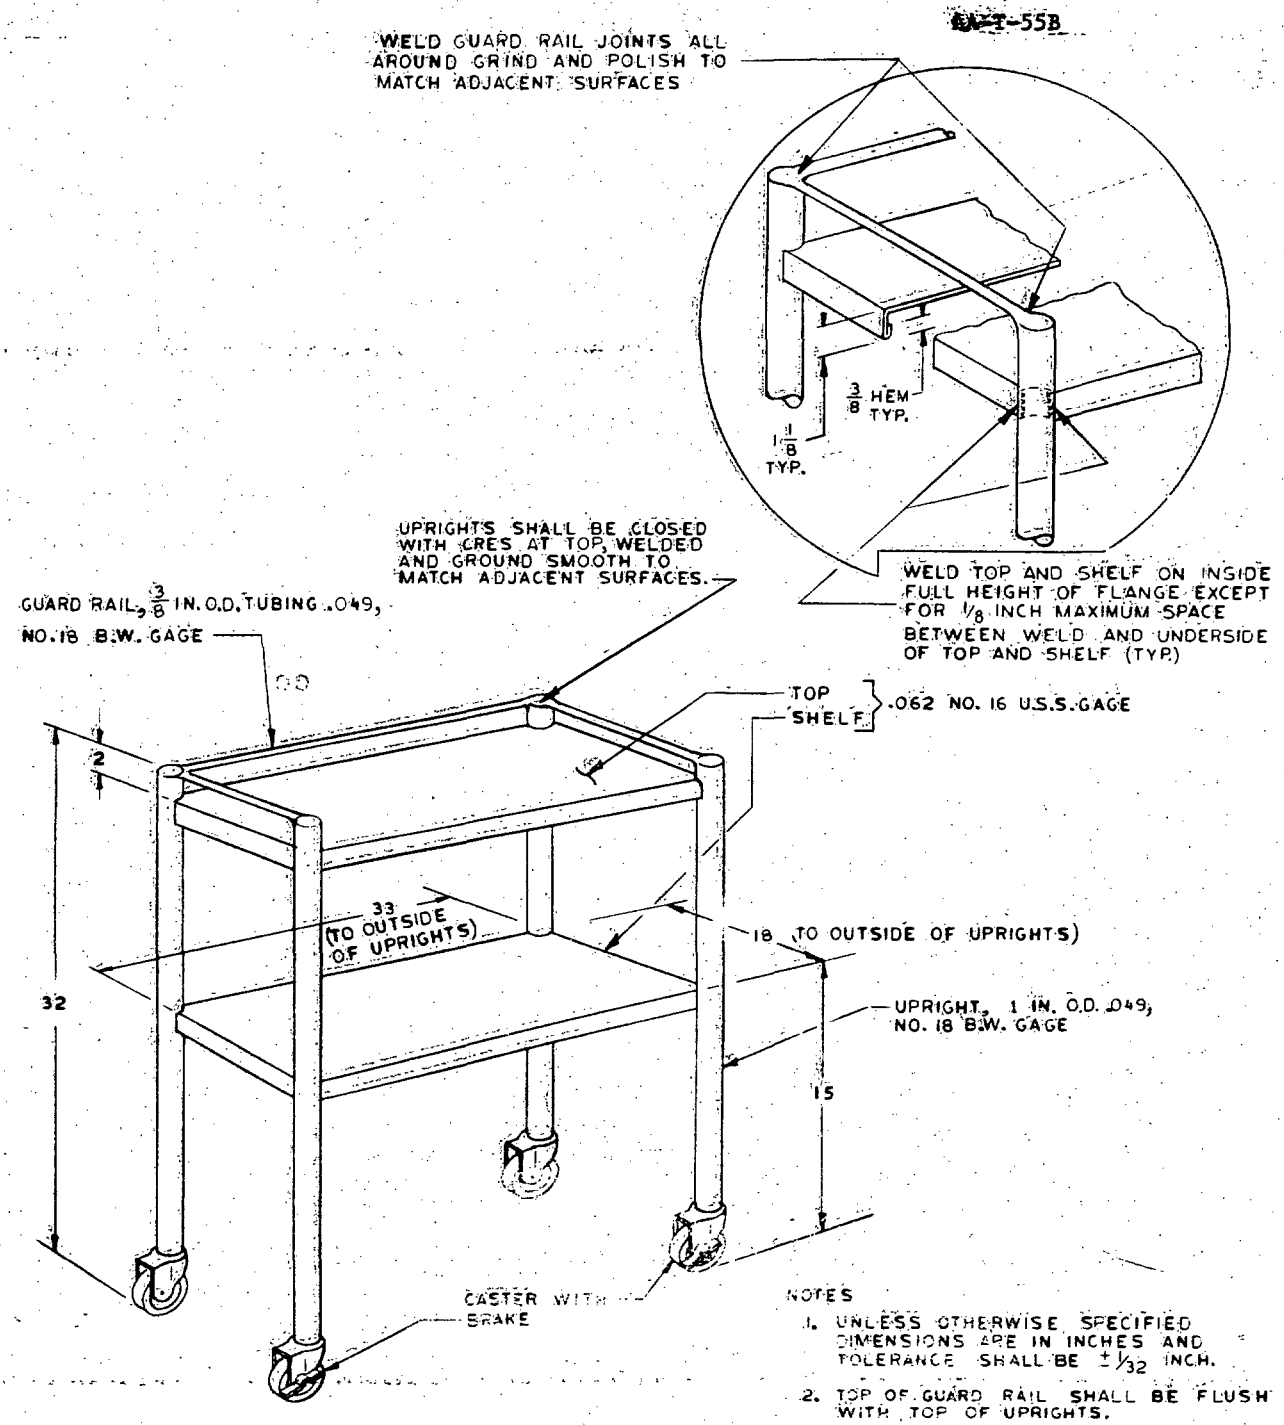



Figure 3. Type II, straight top



Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:38Z
Check the source to verify that this is the current version before use.

3.2.2.4 Casters. The table shall be mounted on four electrically conductive (see 3.3) swivel casters conforming to type II, class A, style b, mounting A of FF-C-77; except the diameter shall be 2 inches with a tread width of 3/4 inch. Two casters shall have brakes. Casters shall conform to the NSF requirements in FF-C-77. Caster shall have a nominal load rating of 75 pounds. The electrical conductivity requirement of FF-C-77 shall not apply (see 3.3).

3.3 Electrical conductivity. The assembled tables shall meet the requirements of NFPA 56A.

3.4 Identification marking. Each table shall be provided with a clear and permanent nameplate of corrosion-resisting steel bearing the following information:

National stock number.
Name or registered trademark of the manufacturer.
Contract or purchase order number.

As an alternate, marking may be stamped on the front of a vertical flange of the table top.

Marking secured by adhesive shall not be used.

3.5 Finish. All exposed corrosion-resisting steel surfaces shall have a No. 4 commercial finish.

3.6 Welding. Welding shall be of the heliarc type and shall be durable, sound in every detail and in accordance with latest practices recommended by the American Welding Society. All welds shall be produced by qualified welding operators with satisfactory welding equipment using satisfactory filler metal or electrode where applicable to provide the best possible weld. Surfaces to be welded shall be free from grease, oil, oxides or any other foreign matter. Any cleaning method which will remove these substances and leave the surface clean is satisfactory. All weld joints shall blend into the adjacent metal in gradual, smooth curves. Beads shall be smooth and free of slag, excessive undercut, or excessive spatter. Sufficient metal shall be added to provide a suitable fillet or reinforcement unless otherwise specified. Fusion through the full thickness of the base metal, in areas other than those where 100 percent penetration is a requirement of joint design, is not acceptable when welding materials over 0.050 inch in thickness. Welds shall not be oxidized. All welds shall be continuous with no vislble voids, pin holes, or cracks which affect the quality, and have more strength than required for purpose intended.



Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:38Z
Check the source to verify that this is the current version before use.

3.7 Workmanship. Workmanship, finish, and associated parts shall be first class throughout. Tables shall be free from defects which detract from their appearance or which may impair their function or serviceability. All exposed corners and edges shall be broken, rounded, or otherwise treated to eliminate sharp edges.

4. QUALITY ASSURANCE PROVISIONS

4.1 Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the supplier is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified, the supplier may utilize his own facilities or any commercial laboratory acceptable to the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure that supplies and services conform to prescribed requirements.

4.1.1 Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government, upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of 3 years after delivery of the supplies to which such records relate.

4.1.2 Inspection. Inspection, as used in this specification, is defined as both examination (such as visual and auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

4.1.3 Certificates of quality. Certificates of quality, supplied by the manufacturer of the metals may be furnished in lieu of actual performance of such testing by the contractor, provided lot identity has been maintained and can be demonstrated to the Government. The Certificate shall include the name of the contractor, the contract number, the name of the manufacturer or supplier, the NSN, the Item Identification, the name of the component/material, the lot number, the lot size, the sample size, the date of testing, the test method, individual test results, and the specification requirements.



Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:38Z
Check the source to verify that this is the current version before use.

4.2 Sampling.

4.2.1 For examination. Sampling for examination shall be conducted in accordance with MIL-STD-105 and table I.

TABLE I.

| | Inspection level | AQL (percent defective) |
|---|---|---|
| For visual examination Major defects | II | 1.0 |
| Total (major and minor combined) defects | II | 4.0 |
| For dimensional examination | S-3 | 2.5 |

4.2.2 For tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and table II.

TABLE II.

| Characteristic | Requirements | Test procedure | Inspection level |
|---|---|---|---|
| Electrical conductivity | 3.3 | 4.4.2 | 100% |

Acceptance number shall be zero.

4.2.3 Raw materials. Four ounces of each lot of each metal used in the construction of the tables shall be selected for chemical analysis.

4.3 Examination. The tables shall be examined to determine compliance with all requirements contained in this specification.

4.3.1 Classification of defects. Examination shall be conducted in accordance with classification of defects found in table III.



Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:38Z
Check the source to verify that this is the current version before use.

TABLE III.

| Categories and defects 1/ | |
|---|---|
| Major: | |
| 101 | Unit not complete with all required parts, subassemblies, and materials. |
| 102 | Component and parts not free of cracks, tears, ruptures, and deformed surfaces. |
| 103 | Components, mating parts, loose or not properly aligned and fitted. |
| 104 | Burn holes, cracks or fractures in welds, not fused. |
| Minor: | |
| 201 | Any exposed or accessible edge, corner, or surface not free of burrs, sharpness, and sharp projections. |
| 202 | Finish not uniform; not free of coarse grind marks and scratched areas. |
| 203 | Any weld not continuous, not clean, not free of pitting, splatter, and discoloration. |
| 204 | Exposed weld not ground smooth to blend with adjacent surfaces. |
| 205 | Unit not clean. |
| 206 | Identification marking missing, incomplete, illegible, or not permanently attached. |
| 207 | Unit does not rest evenly on flat surface within tolerances specified herein. |
| 208 | Casters no not function properly. |

1/ Examination shall not be restricted to the classified possible defects listed above.

4.3.2 Dimensional examination. The tables shall be examined for defects in dimensions. Any dimension not within the tolerances specified herein shall be classified as a defect.

4.4 Tests. Tests shall be conducted to determine compliance with specification requirements.

4.4.1 Chemical composition. Tests for chemical analysis shall be conducted in accordance with method 111.2 or 112.2 of FED-STD-151.

4.4.2 Electrical conductivity. The assembled table, complete with casters, shall be tested as specified in NFPA 56A.



Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:38Z
Check the source to verify that this is the current version before use.

4.5 Examination for preparation for delivery. An examination shall be made to determine whether the packaging, packing, and marking comply with the requirements of Section 5. Defects shall be scored as specified in Table IV. Sampling shall be in accordance with MIL-STD-105. The sample unit shall be one container fully prepared for delivery. The lot shall be the number of containers offered for inspection at one time. The inspection level shall be S-2 and the acceptable quality level shall be 4.0 defects per hundred units.

TABLE IV.

| Examination | Defect |
|---|---|
| Containers | Not as specified. |
| Quantity | Quantity in interior packages and shipping containers not as specified. |
| Packaging and packing materials | Any component missing or damaged. |
| Workmanship | Inadequate application of components, such as incomplete closure of container flaps, tape improperly applied, or containers distorted. |
| Markings | Omitted, incorrect, illegible, improper size, location, sequence, or method of application. |

5. PREPARATION FOR DELIVERY

5.1 Packaging.

5.1.1 Unit of issue. One table of the type specified, constitutes one unit of issue.

5.1.2 Level A. The casters shall be removed, packaged in a cloth bag and secured to the table. Each table shall be further packaged in accordance with MIL-P-116, method III.

5.1.3 Level C. Unit shall be packaged in standard commercial containers of the size and kind commonly used, which will afford the degree of protection required for shipment and use of the product for its intended purpose within the continental limits of the United States of America.



Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:38Z
Check the source to verify that this is the current version before use.

5.2 Packing.

5.2.1 Level A. Each unit shall be overboxed in an exterior container designed for a type 2 load and constructed in accordance with PPP-B-585, class 3, style 3; PPP-B-601, overseas type; PPP-B-621, class 2; or PPP-B-636, type CF, class weather-resistant, variety DW. Containers shall be designed with suitable interior fittings and shall contain sufficient cushioning material to insure against shifting of or damage to the unit. In addition, fiberboard boxes shall not be utilized for type I tables. Closure and strapping shall be as specified in the appendix of the applicable box specification.

5.2.1.1 Case liner. Each Level A wood box shall be lined with a waterproof case liner conforming to MIL-L-10547. Closure and sealing shall conform to applicable paragraphs of appendix thereto. Case liner shall not be required for fiberboard boxes. Each fiberboard box shall be waterproofed as specified in 30.4 of PPP-B-636.

5.2.2 Level B. Each unit shall be overboxed in an exterior container designed for a type 2 load and constructed in accordance with PPP-B-585, class 1, style 3; PPP-B-601, domestic type; PPP-B-621, class 1; or PPP-B-636, class domestic, variety DW. Containers shall be designed with suitable interior fitting and shall contain sufficient cushioning material to insure against shifting of or damage to the unit. Fiberboard boxes shall not be utilized for type I tables. Closure shall be as specified in the appendix of the applicable box specification. Closure of fiberboard boxes shall conform to method II as specified in PPP-B-636.

5.2.3 Level C. The subject commodity shall be packed in substantial commercial containers of the type, size, and kind commonly used for the purpose, so constructed as to insure acceptance and safe delivery by common or other carriers, at the lowest rate, to point of delivery for in the contract or purchase order.

5.3 Marking. Marking shall be as specified in MIL-STD-129.

6. NOTES

6.1 Intended use. The tables covered by this specification are intended for use in the surgical service of hospitals, and for general use in dispensaries.



Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:38Z
Check the source to verify that this is the current version before use.

6.2 Ordering data. Purchasers should select the preferred options permitted herein and include the following information in procurement documents.

(a) Title, number and date of this specification.
(b) Type table required (see 1.2.1).
(c) Selection of applicable levels of packaging and packing (see 5.1 and 5.2).

6.3 This specification covers the following items appearing in the Federal Supply Catalog:

| National Stock No. | Item Identification | Specification Designation |
|---|---|---|
| 6530-00-709-3960 | Table, Surgical Instrument and Surgical Dressing, Corrosion-Resisting Steel Angular, 72 by 15 by 35 inches | Type I |
| 6530-00-709-4010 | Table, Surgical Instrument and Surgical Dressing, Corrosion-Resisting Steel, 33 by 18 by 32 inches | Type II |

6.4 This specification does not cover all types, classes, grades, or sizes of the commodity indicated by the title of this specification, or those which are commercially available, but is intended to cover the types which are normally procured to meet requirements.

MILITARY CUSTODIANS:

Army - MD
Navy - MS
Air Force - 03

Civil Agency Coordinating Activity:

GSA - FSS

Preparing activity:

DSA - DM

Project No. 6530-1311

Orders for this publication are to be placed with General Services Administration, acting as an agent for the Superintendent of Documents. See section 2 of this specification to obtain extra copies and other documents referenced herein. **Price 40 cents each.**



Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:38Z
Check the source to verify that this is the current version before use.

FOLD

DEFENSE PERSONNEL SUPPORT CENTER
2800 South 20th Street
Philadelphia, Pa. 19101

OFFICIAL BUSINESS
PENALTY FOR PRIVATE USE $300

POSTAGE AND FEES PAID
DEFENSE SUPPLY AGENCY
DoD - 304




HEADQUARTERS, DEFENSE PERSONNEL SUPPORT CENTER
ATTN: DIRECTORATE OF MEDICAL MATERIEL, CODE ATT
2800 SOUTH 20TH STREET
PHILADELPHIA, PA. 19101

FOLD

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:38Z
Check the source to verify that this is the current version before use.

# STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

OMB Approval
No. 22-R255

INSTRUCTIONS: The purpose of this form is to solicit beneficial comments which will help achieve procurement of suitable products at reasonable cost and minimum delay or will otherwise enhance use of the document. DoD contractors, government activities, or manufacturers/vendors who are prospective suppliers of the product are invited to submit comments to the government. Fold on lines on reverse side, staple in corner, and send to preparing activity. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements. Attach any pertinent data which may be of use in improving this document. If there are additional papers, attach to form and place both in an envelope addressed to preparing activity.

DOCUMENT IDENTIFIER AND TITLE

AA-T-55B- Tables, Surgical Instrument and Surgical Dressing (Mobile)

NAME OF ORGANIZATION AND ADDRESS

CONTRACT NUMBER

MATERIAL PROCURED UNDER A

☐ DIRECT GOVERNMENT CONTRACT ☐ SUBCONTRACT

1. HAS ANY PART OF THE DOCUMENT CREATED PROBLEMS OR REQUIRED INTERPRETATION IN PROCUREMENT USE?

A. GIVE PARAGRAPH NUMBER AND WORDING.

B. RECOMMENDATIONS FOR CORRECTING THE DEFICIENCIES

2. COMMENTS ON ANY DOCUMENT REQUIREMENT CONSIDERED TOO RIGID

3. IS THE DOCUMENT RESTRICTIVE?

☐ YES ☐ NO *(If "Yes", in what way?)*

4. REMARKS

SUBMITTED BY *(Printed or typed name and address - Optional)*

TELEPHONE NO.

DATE

DD FORM 1 JAN 72 1426

REPLACES EDITION OF 1 JAN 66 WHICH MAY BE USED

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:38Z
Check the source to verify that this is the current version before use.