GGG-M-125/4B
September 20, 1982
SUPERSEDING
GGG-M-125/4A
August 22, 1978

FEDERAL SPECIFICATION

RESPIRATOR ASSEMBLY: HALF MASK, AIR FILTERING (CHEMICAL CARTRIDGE)

This specification was approved by the Commissioner, Federal Supply Service, General Services Administration, for the use of all Federal agencies.

The complete requirements for procuring the respirators described herein shall consist of this document and the issue in effect of GGG-M-125/GEN.

1. SCOPE AND CLASSIFICATION

1.1 Scope. This specification covers the specific requirements for half-mask respirators with air filtering chemical cartridges for removal of low concentrations of organic vapors.

1.2 Classification. Half-mask respirators covered by this specification shall be of the following types as specified (see 6.2):

Type I - Half-mask, air-purifying respirator with provisions to replace the air-purifying element(s) (reusable).
Type II - Half-mask air-purifying respirator where the air-purifying element(s) is/are not intended to be replaceable (disposable).

2. APPLICABLE DOCUMENTS

Latest issue of GGG-M-125/GEN and documents referenced therein.

3. REQUIREMENTS

3.1 Approval and certification. (See GGG-M-125/GEN).

3.2 Design. Respirator mask (see figures 1 and 2) shall cover the wearer's nose and mouth leaving the eyes uncovered, and shall provide protection against low concentrations of organic vapors. The lower part of the half-mask facepiece shall make facial contact under the chin. The design shall provide a gas-tight seal with the face, when worn.

3.3 Principal parts. Respirators shall consist of the following parts where required:

a. Half-mask facepiece.
b. Chemical cartridge(s) (see 3.3.1).
c. Head harness (see 3.3.2).
d. Exhalation valve(s) (see 3.3.3).
e. Inhalation valve(s) (see 3.3.4).

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:37Z
Check the source to verify that this is the current version before use.

3.3.1 Chemical cartridge(s). Chemical cartridges shall provide protection against concentration of organic vapors specified in 30 CFR, part 11.

3.3.1.1 Chemical cartridge(s) for type I respirator. Unless otherwise specified (see 6.2), 50 cartridges shall be furnished with each type I respirator having a single receptacle mask and 100 cartridges shall be furnished with each type I respirator having a dual mask.

3.3.2 Head harness. The head harness shall be adjustable and secure the respirator facepiece to the wearer's head.

3.3.3 Exhalation valve(s). The exhalation valve(s) shall be securely mounted on the facepiece, and shall permit passage of the exhaled air from the respirator and prevent entrance of ambient air into the respirator during inhalation.

3.3.4 Inhalation valve(s). The inhalation valve(s) shall prevent the passage of exhaled air into the air-purifying element(s).

3.4 Cleaning and sanitization. Type I respirators shall conform to the cleaning and sanitizing requirements specified in GGG-M-125/GEN.

3.5 Spare parts. When specified (see 6.2), spare parts shall be furnished with each respirator.

3.6 Interchangeability. Requirements in accordance with GGG-M-125/GEN.

3.7 Instructions. Requirements in accordance with GGG-M-125/GEN.

3.8 Marking. Requirements in accordance with GGG-M-125/GEN.

3.9 Workmanship. Requirements in accordance with GGG-M-125/GEN.

4. QUALITY ASSURANCE PROVISIONS

4.1 Quality assurance provisions shall be in accordance with the requirements of GGG-M-125/GEN and the additional requirements specified herein.

4.2 Examination. Respirator samples selected in accordance with GGG-M-125/GEN shall be examined for the defects listed in table I.

TABLE I. Classification of defects.

Categories	Defects
Major:	
101	Type not as specified.
102	Respirator not in accordance with NIOSH/MSHA requirements.
103	Principal parts missing.
104	Chemical cartridge not as specified.
105	Quantity of extra cartridges not as specified.
106	Spare parts missing when specified.
107	Instructions missing.
108	Markings not as required.
109	Poor workmanship.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:37Z
Check the source to verify that this is the current version before use.

4.3 Tests. Respirator assemblies sampled in accordance with GGG-M-125/GEN shall be subjected to the following test:

a. Cleaning and sanitization test type I only (see GGG-M-125/GEN).

5. PREPARATION FOR DELIVERY (In accordance with GGG-M-125/GEN).

6. NOTES

6.1 Intended use. Half-mask respirators covered by this specification are intended to give protection to the respiratory organs of the wearer from organic vapors in concentrations that are not immediately dangerous to life or health. Component parts of respirators are not interchangeable between manufacturers nor are they always interchangeable on different models produced by the same manufacturer.

6.2 Ordering data. Purchasers shall select the preferred options offered herein and include the following data in procurement documents:

a. Title, number, and date of this specification.
b. Title and date of general specification GGG-M-125/GEN.
c. Type of respirator required (see 1.2).
d. If different quantity of cartridges is required (see 3.3.1.1).
e. Specify if spare parts are required and list quantity of each type of spare part required (see 3.5).
f. Specify level of packaging and level of packing required (see GGG-M-125/GEN).

6.3 Cross reference of classifications. The following respirators were previously classified as indicated:

New	Old
GGG-M-125/4B Type I	GGG-M-125/4A

MILITARY INTEREST:

Custodians

Army - EA
Navy - YD
Air Force - 99

Review Activities

Army - MD, ME
DLA - GS

User Activities

Navy - SH. _CG, _MC

CIVIL AGENCY COORDINATING ACTIVITY:

GSA - FSS
TVA -
DCG

PREPARING ACTIVITY:

Navy - YD


Project No. 4240-0505

Orders for this publication are to be placed with General Services Administration, acting as an agent for the Superintendent of Documents. See section 2 of this specification to obtain extra copies and other documents referenced herein.

Source: https://assist.dla.mil -- Downloaded: 202640-26T12:37Z
Check the source to verify that this is the current version before use.



Dual chemical cartridge respirator.

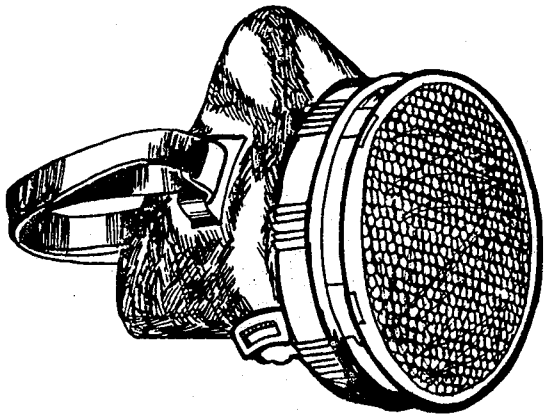

Single chemical cartridge respirator.

Figure 1. Type I half-mask respirator assemblies.
(For illustrative purposes only.)

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:37Z
Check the source to verify that this is the current version before use.

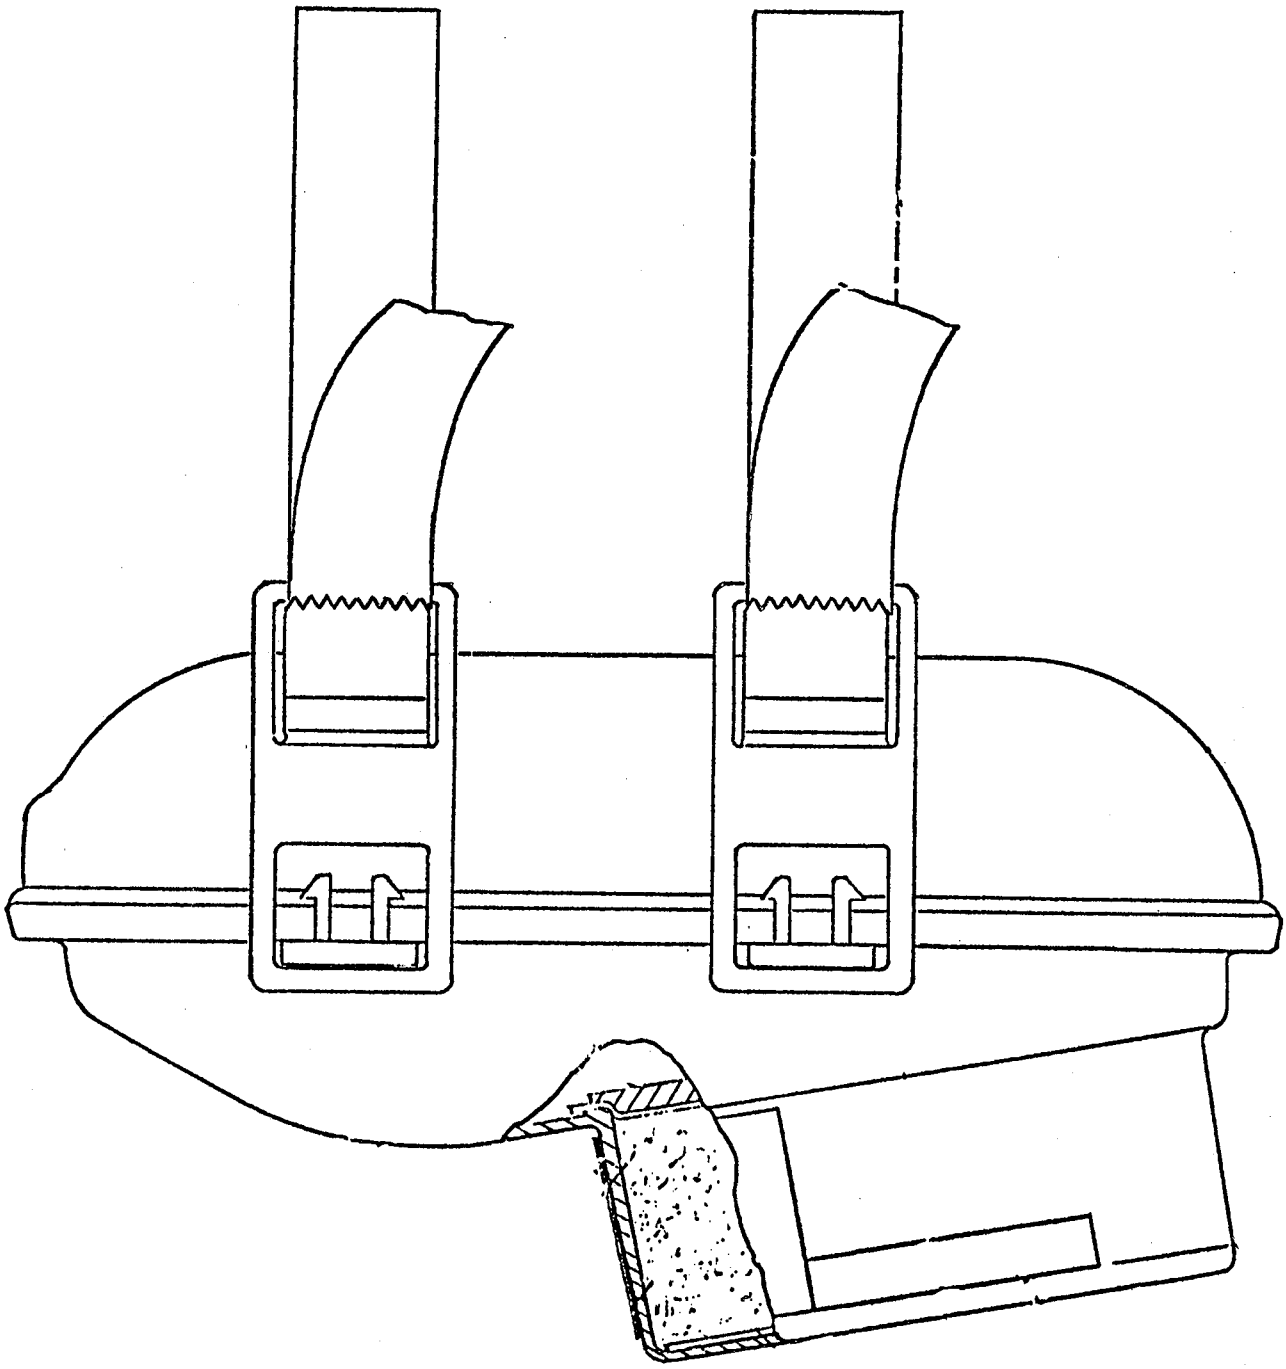


Figure 2. Type II half-mask respirator assembly.
(For illustrative purposes only.)

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:37Z
Check the source to verify that this is the current version before use.