MILITARY SPECIFICATION

# FORCEPS, HEMOSTATIC, STRAIGHT ROCHESTER-OCHSNER

This specification is approved for use by all Departments and Agencies of the Department of Defense.

## 1. SCOPE

1.1 This specification covers a hemostatic forceps of the Rochester-Ochsner design, suitable for use during surgical procedures.

1.2 Classification

1.2.1 Sizes. The forceps shall be of two sizes, as specified in the invitation for bids:

| | |
|---|---|
| Size I | 6-1/4 inch |
| Size II | 7-1/4 inch |

## 2. APPLICABLE DOCUMENTS

2.1 The following documents of the issue in effect on date of invitation for bids or request for proposals, form a part of this specification to the extent specified herein:

SPECIFICATIONS

Federal

| | |
|---|---|
| GG-I-526 | Instruments, Dental and Surgical; General Specifications. |
| MMM-A-250 | Adhesive, Water-Resistant, (For sealing Fiberboard Boxes). |
| PPP-B-566 | Boxes, Folding, Paperboard. |
| PPP-B-585 | Boxes, Wood, Wirebound. |
| PPP-B-601 | Boxes, Wood, Cleated-Plywood. |
| PPP-B-621 | Boxes, Wood, Nailed and Lock-Corner. |
| PPP-B-636 | Box, Fiberboard. |
| PPP-T-76 | Tape, Pressure-Sensitive Adhesive Paper (For Carton Sealing). |



Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:37Z
Check the source to verify that this is the current version before use.

Military

| | |
|---|---|
| MIL-P-116 | Preservation, Methods of. |
| MIL-L-10547 | Liners, Case, and Sheet Overwrap; Water-Vaporproof or Waterproof, Flexible. |

STANDARDS

Military

| | |
|---|---|
| MIL-STD-105 | Sampling Procedures and Tables for Inspection by Attributes. |
| MIL-STD-129 | Marking for Shipment and Storage. |

(Copies of specifications and standards, required by suppliers in connection with specific procurement functions should be obtained from the preparing activity or as directed by the contracting officer.)

3. REQUIREMENTS

3.1 General Requirements. The forceps shall be in accordance with the applicable requirements of GG-I-526 and the following option exercises under that specification:

3.2 Material. The forceps shall be fabricated from Class 4, Type 420 or 420F material. As an alternate, shall be type 410.

3.3 Hardness. After proper stress relieving, the forceps shall have a Rockwell hardness of C40 to C45, with the exception of the screw or pin.

3.4 Style, design and dimensions. The forceps shall be of the Rochester-Ochsner with straight tip, suitable for use as a hemostatic forceps during surgical procedures. Shall be in accordance with Figure 1.

3.4.1 Locks. Shall be box type lock.

3.5 Finish. Finish shall be mirror or mirror and satin. Locks and ratchets shall be smooth and shall be polished but need not be buffed to a mirror finish.

3.6 Lock stiffness. Forceps of box lock construction shall have shanks tested for lock stiffness in accordance with GG-I-526.

3.7 Identification marking. In addition to GG-I-526 requirements, forceps of foreign manufacture shall also be marked "stainless".



Source: https://assist.dla.mil -- Downloaded: 202640-21T09:37Z
Check the source to verify that this is the currentversion before use.

3.8 Jaw and ratchet operation. When tested as specified in 4.4.1, the jaw tips shall close first and progressively tighten with each ratchet position. Each ratchet position shall hold firmly and release instantly.

4. QUALITY ASSURANCE PROVISIONS

4.1 Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the supplier is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or order, the supplier may use his own or any other facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and servies conform to prescribed requirements.

4.1.1 Inspection. Inspection shall be in accordance with GG-I-526.

4.1.2 Records. Records of examination and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government, upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of 3 years after delivery of the supplies to which such records relate.


4.1.3 Certificates of quality. Certificates of quality supplied by the manufacturer of the corrosion resisting steel, may be furnished in lieu of actual performance of such testing by the contractor, provided lot identity has been maintained and can be demonstrated to the Government. The certificates shall include the name of the contractor, the contract number, the name of the manufacturer or supplier, the FSN, the Item Identification, the name of the material, the lot number, the lot size, the sample size, the date of testing, the test method, the individual test results, and the specification requirements.

4.2 Sampling.

4.2.1 For examination. Sampling for examination shall be conducted in accordance with MIL-STD-105 and as indicated in Table I. The unit of product for examination purposes shall be one hemostatic forceps.



Source: https://assist.dla.mil -- Downloaded: 202610-21T09:37Z
Check the source to verify that this is the current version before use.

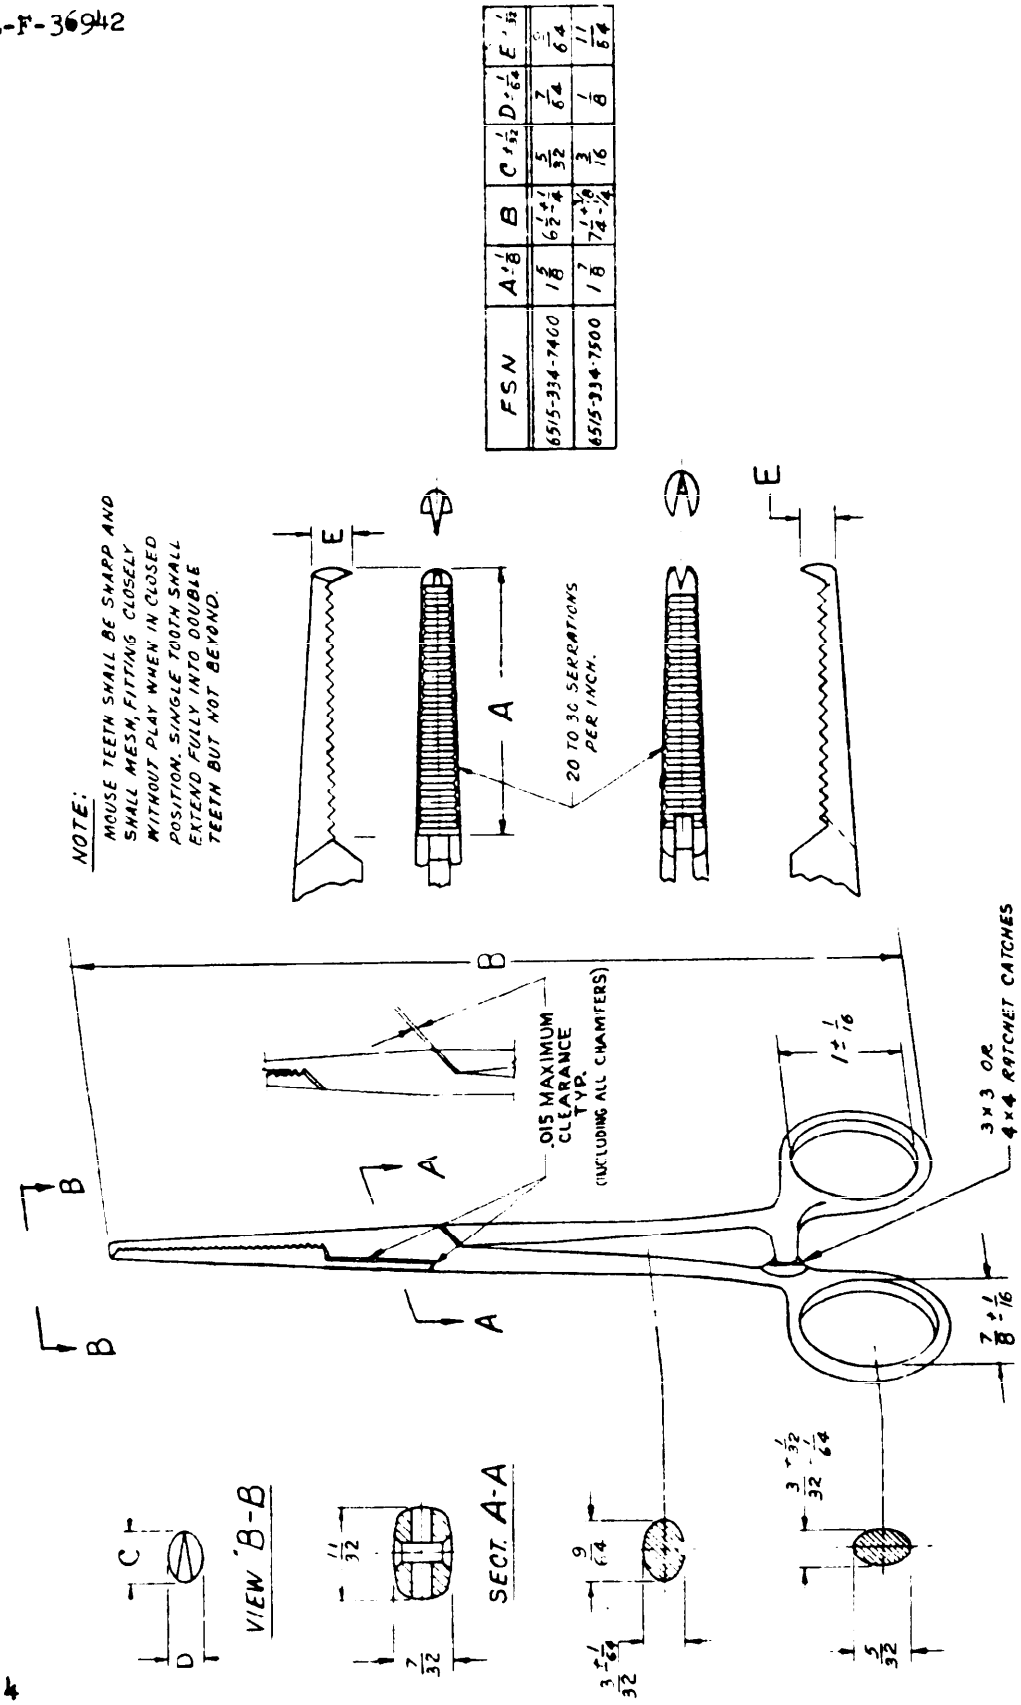


| FSN | A ±1/8 | B | C ±1/32 | D ±1/64 | E ±1/32 |
|---|---|---|---|---|---|
| 6515-334-7460 | 1 5/8 | 6 1/2 +1/4 | 5/32 | 7/64 | 5/64 |
| 6515-334-7500 | 1 7/8 | 7 1/4 +1/8 -1/4 | 3/16 | 1/8 | 11/64 |

UNLESS OTHERWISE SPECIFIED TOLERANCES ON FRACTION ± 1/32

FIGURE 1



Source: https://assist.dla.mil -- Downloaded: 202610-21T09:37Z
Check the source to verify that this is the current version before use.

Table I. Sampling Criteria for Examination

| Type of defect | Inspection level | AQL (Percent defective) |
|---|---|---|
| Major | II | 1.0 |
| Minor | II | 2.5 |

4.2.2 For tests. Sampling for tests shall be conducted in accordance with MIL-STD-105, and as indicated in Table II. Unit of product for test purposes shall be one forceps.

Table II. Sampling Criteria for Tests

| Component | Characteristic | Requirement | Test procedure | Inspection level | AQL |
|---|---|---|---|---|---|
| 1-Forceps | Composition analysis | 3.2 and GG-I-526 | GG-I-526 | ** | * |
| | Hardness | 3.3 and GG-I-526 | GG-I-526 | S-2 | * |
| | Dimensions | 3.4 | -------- | S-2 | 4.0 |
| | Boil test | GG-I-526 | GG-I-526 | S-2 | * |
| | Copper sulfate | GG-I-526 | GG-I-526 | S-2 | * |
| | Box lock stiffness | 3.6 | GG-I-526 | II | 6.5 |
| | Distortion test | GG-I-526 | GG-I-526 | S-2 | * |
| | Jaw and Ratchet operation test | 3.8 | 4.4.1 | S-2 | 1.0 |

* Acceptance number shall be zero for all sample sizes.
** Four ounces of each lot or metal used in the construction of the forceps shall be selected for chemical analysis. Wherever feasible, the same sample unit shall be used for the determination of two or more test characteristics.

4.3 Examination. The forceps shall be examined to determine compliance with all requirements contained in this specification. Examination shall be conducted as specified in Table I and III. Examination however, shall not be restricted to defects listed in Table III. Any forceps in the sample containing one or more defects shall be rejected, and if the number of defective items in any sample exceeds the acceptance number for test sample, the lot represented by the sample shall be rejected.



Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:37Z
Check the source to verify that this is the current version before use.

Table III. Classification of Defects

| Categories | Defects |
|---|---|
| Critical | None defined. |
| Major | |
| 101 | Style and design not as specified. |
| 102 | Forceps not free from cracks, pits, dents, nicks, sharp edges and burrs. |
| 103 | Serrations not as specified. |
| 104 | Ratchet teeth not uniform, or function poorly. |
| 105 | Forceps not of box lock design. |
| 106 | Forceps not free from excessive play in box lock area. |
| Minor | |
| 201 | Finish not mirror, or mirror plus satin. |
| 202 | Identification marking not present, correct, complete or legible. |

4.4 Tests. Tests shall be conducted to determine compliance with specification requirements.

4.4.1 Jaw and operation test. The forceps shall be positioned to the first ratchet position, but not locked. Forceps with jaw tips not touching shall be rejected. Forceps that do not progressively tighten with each ratchet advance shall be rejected.

5. PREPARATION FOR DELIVERY

5.1 Packaging. Packaging shall be level A or C as specified (see 6.2).

5.1.1 Unit of issue. One forceps as specified, constitutes one unit of issue.

5.1.2 Packaging quantities. The number of units of issue indicated in Table IV shall be packaged in each unit, intermediate, and exterior container as applicable, for the required level of protection specified in the procurement document.



Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:37Z
Check the source to verify that this is the current version before use.

Table IV. Packaging Quantities

| Unit package | Intermediate package | Exterior container |
|---|---|---|
| 1 unit | 12 units | 288 units |

5.1.2.1 Packing variation permitted. If the required number of units in the entire shipment is less than the number of units specified to be overpacked in an exterior container, such units shall be packed in an exterior container of suitable size and design, acceptable to a common carrier, which shall insure safe delivery to destination.

5.1.3 Level A.

5.1.3.1 Cleaning and drying. Each unit shall be thoroughly cleaned and dried in accordance with the applicable method as outlined in MIL-P-116.

5.1.3.2 Preservative. None.

5.1.3.3 Intimate wrap. Each unit shall be wrapped in neutral tissue or other suitable anticorrosive material.

5.1.3.4 Unit package. Each unit shall be packaged in accordance with MIL-P-116, method IC-1.

5.1.3.5 Intermediate package. Intermediate package shall be a box of appropriate size and design constructed in accordance with PPP-B-636, type CF, class weather-resistant. Boxes shall be closed by taping the top and bottom flaps with 2 inch wide tape conforming to PPP-T-76. Closing of bottom flap with adhesive conforming to MMM-A-250 or metal stitches is permitted.

5.1.4 Level C. Units shall be packaged in standard commercial containers of the size and kind commonly used, which will afford the degree of protection required for shipment and use of the product for its intended purpose.

5.2 Packing. Packing shall be Level A, B or C as specified (see 6.2).

5.2.1 Level A.

5.2.1.1 Exterior container. Exterior container shall be designed for a type 2 load and constructed in accordance with PPP-B-585, class 3, style 3; PPP-B-601, overseas type; PPP-B-621, class 2; or PPP-B-636, class weather-resistant, grade V3c. Closure and strapping shall be as specified in the appendix of the applicable box specification. Special requirements of applicable table shall apply for PPP-B-636.



Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:37Z
Check the source to verify that this is the current version before use.

5.2.2 Level B.

5.2.2.1 Exterior container. Exterior container shall be designed for a type 2 load and constructed in accordance with PPP-B-585, class 1, style 3; PPP-B-601, domestic type; PPP-B-621, class 1; or PPP-B-636, class domestic. Closure shall be as specified in the appendix of the applicable box specification. Closure of fiberboard boxes shall conform to method II as specified in PPP-B-636. In addition, fiberboard boxes shall conform to the special requirements as specified in PPP-B-636.

5.2.3 Level C. The subject commodity shall be packed in substantial commercial containers of the type, size, and kind commonly used for the purpose, so constructed as to insure acceptance and safe delivery by common or other carriers, at the lowest rate, to point of delivery called for in the contract or purchase order.

5.3 Marking.

5.3.1 Interior packages. Each unit package and each intermediate package shall be marked in accordance with MIL-STD-129. When labels are utilized, waterproofing shall be required only when applicable carton is fabricated of water-resistant material. Contract or purchase order number and name of contractor shall be shown.

5.3.2 Exterior container. Exterior container shall be marked in accordance with MIL-STD-129.

6. NOTES

6.1 Intended use. The hemostatic forceps are to be used for clamping blood vessels to control bleeding during surgical procedures.

6.2 Ordering data. Procurement documents should specify the following:

(a) Number, title and date of this specification.
(b) Selection of applicable level of packaging and packing required (see 5.1 and 5.2).



Source: https://assist.dla.mil -- Downloaded: 202640-21T09:37Z
Check the source to verify that this is the current version before use.

6.3 Federal Stock Number (FSN) coverage. This specification covers the following items listed in the Federal Supply Catalog:

| Federal Stock Number | Item Identification | Size |
|---|---|---|
| 6515-334-7400 | FORCEPS, HEMOSTATIC, Straight, Rochester-Ochsner, 6-1/4 inch | I |
| 6515-334-7500 | FORCEPS, HEMOSTATIC, Straight, Rochester-Ochsner, 7-1/4 inch | II |

It does not include all types or sizes as indicated by the title nor all types which are commercially available.

6.4 Supersession data. This specification includes the requirements of Purchase Description No. 7, dated 5 July 1968 for FSN 6515-334-7400 FORCEPS, HEMOSTATIC, Straight, Rochester-Ochsner, 6-1/4 inch and FSN 6515-334-7500 FORCEPS, HEMOSTATIC, Straight, Rochester-Ochsner, 7-1/4 inch.

Custodians:
Army - MD
Navy - MS
Air Force - 03

Review activities:
Army - MD
Navy - MS
Air Force - 03

Preparing activity:
Defense Supply Agency - DM

Project No. 6515-1695

Review information is current as of the date of this document. For future coordination of changes to this document, draft circulation should be based on the information in the current DODISS.



Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:37Z
Check the source to verify that this is the current version before use.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:37Z
Check the source to verify that this is the current version before use.

# STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

OMB Approval No. 22-R255

INSTRUCTIONS. The purpose of this form is to solicit beneficial comments which will help achieve procurement of suitable products at reasonable cost and minimum delay, or will otherwise enhance use of the document. DoD contractors, government activities, or manufacturers/vendors who are prospective suppliers of the product are invited to submit comments to the government. Fold on lines on reverse side, staple in corner, and send to preparing activity. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements. Attach any pertinent data which may be of use in improving this document. If there are additional papers, attach to form and place both in an envelope addressed to preparing activity.

DOCUMENT IDENTIFIER AND TITLE: MIL-F-36942

NAME OF ORGANIZATION AND ADDRESS

CONTRACT NUMBER

MATERIAL PROCURED UNDER A

☐ DIRECT GOVERNMENT CONTRACT ☐ SUBCONTRACT

1. HAS ANY PART OF THE DOCUMENT CREATED PROBLEMS OR REQUIRED INTERPRETATION IN PROCUREMENT USE?

A. GIVE PARAGRAPH NUMBER AND WORDING.

B. RECOMMENDATIONS FOR CORRECTING THE DEFICIENCIES

2. COMMENTS ON ANY DOCUMENT REQUIREMENT CONSIDERED TOO RIGID

3. IS THE DOCUMENT RESTRICTIVE?

☐ YES ☐ NO *(If "Yes", in what way?)*

4. REMARKS

SUBMITTED BY *(Printed or typed name and address - Optional)*

TELEPHONE NO.

DATE

**DD FORM 1 JAN 72 1426** REPLACES EDITION OF 1 JAN 66 WHICH MAY BE USED

Source: https://assist.dla.mil -- Downloaded: 202610-21T09:37Z
Check the source to verify that this is the current version before use.

FOLD

DEFENSE PERSONNEL SUPPORT CENTER
2800 South 20th Street
Philadelphia, Pa. 19101

POSTAGE AND FEES PAID
DEFENSE SUPPLY AGENCY
DoD - 304

U.S. MAIL

OFFICIAL BUSINESS
PENALTY FOR PRIVATE USE $300

HEADQUARTERS, DEFENSE PERSONNEL SUPPORT CENTER
ATTN: DIRECTORATE OF MEDICAL MATERIEL, CODE ATT
2800 SOUTH 20TH STREET
PHILADELPHIA, PA. 19101

FOLD

Source: https://assist.dla.mil -- Downloaded: 202640-21T09:37Z
Check the source to verify that this is the currentversion before use.