MILITARY SPECIFICATION

GUIDE, OCCLUSAL PLANE, FOX

This specification is approved for use by all Departments and Agencies of the Department of Defense.

1. SCOPE

1.1 This specification covers an occlusal plane guide of Fox design, suitable for use in establishing the proper occlusal plane in constructing artificial dentures.

2. APPLICABLE DOCUMENTS

2.1 The following documents of the issue in effect on date of invitation for bids or request for proposal, form a part of the specification to the extent specified herein:

SPECIFICATIONS

Federal

QQ-A-250/11	Aluminum Alloy 6061, Plate and Sheet.
PPP-B-566	Boxes, Folding, Paperboard.
PPP-B-585	Boxes, Wood, Wirebound.
PPP-B-601	Boxes, Wood, Cleated-plywood.
PPP-B-621	Boxes, Wood, Nailed and Lock-corner.
PPP-B-636	Box, Fiberboard.
PPP-B-676	Boxes, Setup.

Military

MIL-L-10547	Liners, Case, and Sheet, Overwrap; Water-vaporproof or Waterproof, Flexible.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:35Z
Check the source to verify that this is the current version before use.

STANDARDS

Military

MIL-STD-105	Sampling Procedures and Tables for Inspection by Attributes.
MIL-STD-129	Marking for Shipment and Storage.

(Copies of specifications and standards required by suppliers in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.)

3. REQUIREMENTS

3.1 Material. The occlusal plane guide shall be fabricated of 15 or 16 gauge Aluminum Association Alloy No. 6061-T6 aluminum sheet conforming to QQ-A-250/11.

3.2 Style, design, and dimensions. The occlusal plane guide shall be suitable for use in establishing the proper occlusal plane in constructing artificial dentures. The plane guide shall conform to figure 1 for style, design, and dimensions. The occlusal plane guide shall be of Fox design.

3.3 Finish. The occlusal plane guide shall have a smooth or brushed finish.


3.4 Instructions for use. Instructions for use shall accompany each occlusal plane guide and shall be found on the envelope containing the guide or as a separate sheet. Instructions shall include method of marking the face and inserting the plane guide into the mouth.

3.5 Workmanship. Workmanship shall be first class throughout. Occlusal plane guide shall have all edges rounded and shall be free from defects which may detract from its appearance or may impair its serviceability.

4. QUALITY ASSURANCE PROVISIONS

4.1 Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the supplier is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or order, the supplier may use his own or any other facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in this specification where such inspections are deemed necessary to assure that supplies and services conform to prescribed requirements.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:35Z
Check the source to verify that this is the current version before use.

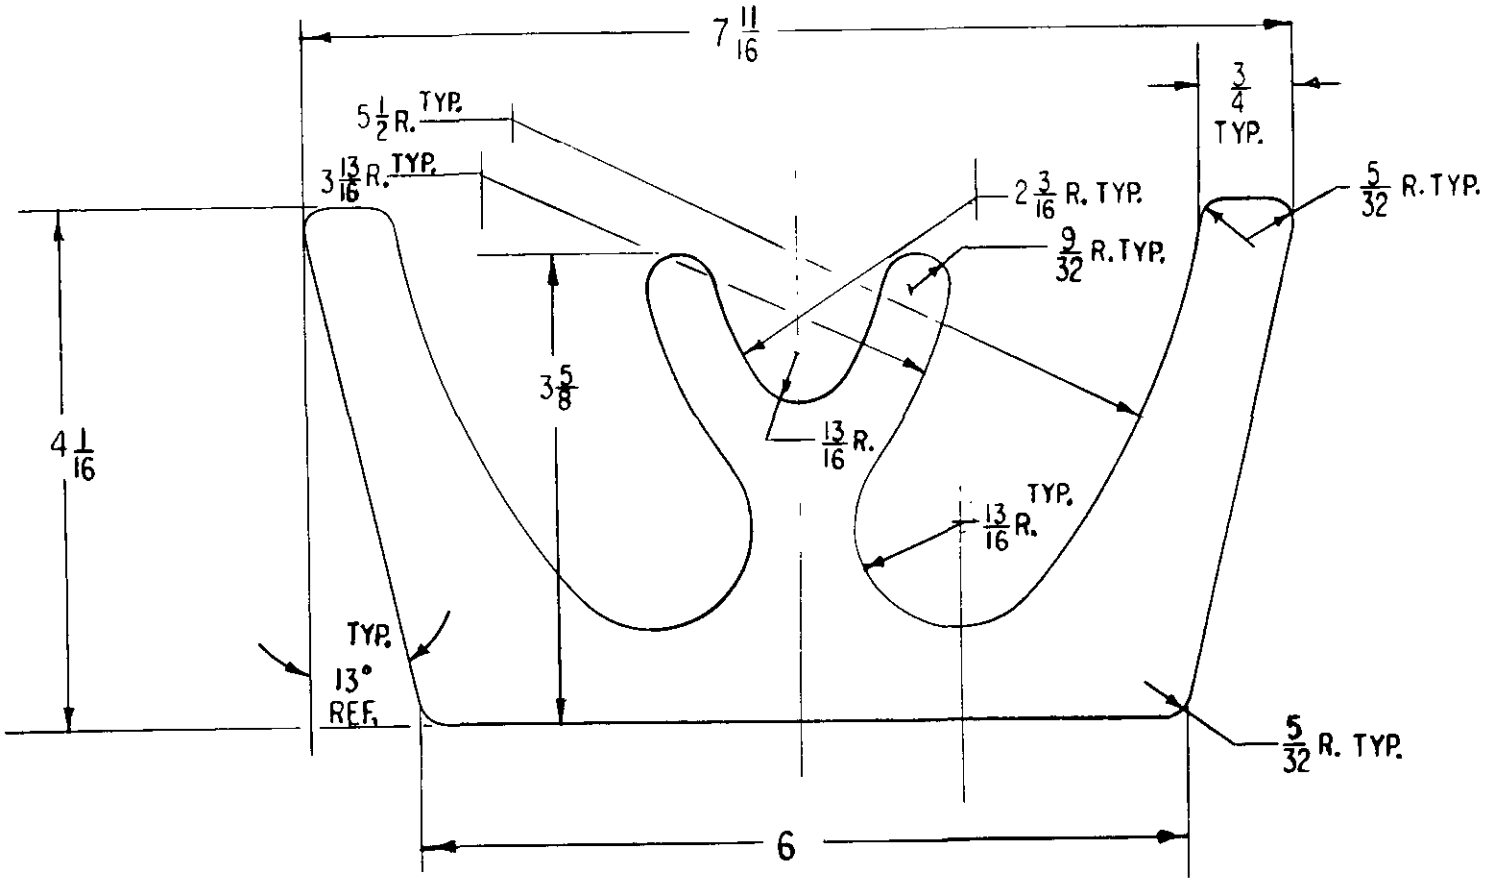

ALL DIMENSIONS ARE IN INCHES

DIMENSIONS UNDER 3 INCHES	± 1/32
DIMENSIONS OVER 3 INCHES	± 1/16

FIGURE 1

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:35Z
Check the source to verify that this is the current version before use.

4.1.1 Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government, upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of 3 years after delivery of the supplies to which such records relate.

4.1.2 Inspection. Inspection, as used in this specification, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

4.1.3 Certificates of quality. Certificates of quality, supplied by the manufacturer of the raw materials and packaging materials, may be furnished in lieu of actual performance of such testing by the contractor, provided lot identity has been maintained and can be demonstrated to the Government. The Certificate shall include the name of the contractor, the contract number, the name of the manufacturer or supplier, the FSN, the Item Identification, the name of the material, the lot number, the lot size, the sample size, the date of testing, the test method, individual test results, and the specification requirements.

4.2 Quality conformance inspection. The examinations and tests required to assure conformance of those items or lots of items to be offered for acceptance are classified as specified in tables I and II (see 4.2.1 and 4.3) and 4.2.2.

4.2.1 Sampling for examination. Sampling for examination shall be conducted in accordance with MIL-STD-105. The inspection levels and acceptable quality levels (AQL's) shall be as indicated in table I. Unit of product for examination purposes shall be one occlusal guide (unit of issue).

Table I. Sampling for examination

Type defect	Inspection level	AQL (Percent defective)
Major	II	1.0
Minor A	II	2.5
Minor B	S-2	4.0

4.2.2 Sampling for tests. Unless otherwise specified in subsidiary specifications, testing shall be conducted as indicated for inspection level S-1 in MIL-STD-105. Any failure shall be cause for rejection.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:35Z
Check the source to verify that this is the current version before use.

4.3 Examination. The guide shall be examined for defects including, but not limited to, those listed in table II.

Table II. Classification of Defects

Categories	Defects
Major:	
101	Surface of guide not free from corrosion, discoloration, or deep pits.
102	Instructions for use not as specified, or instructions missing.
103	Style and design not in accordance with figure 1.
Minor A:	
201	Finish not smooth or brushed.
202	Finish not free from coarse grind marks.
203	Guide not free from dirt, oil, or other foreign matter.
204	Packaging and packing not as specified.
205	Marking on packaging and packing illegible, incomplete, improper or missing altogether.
Minor B:	
251	Any dimension not as shown in figure 1.

4.4 Tests. Tests shall be conducted to determine compliance with specification requirements.

5. PREPARATION FOR DELIVERY

5.1 Packaging. Packaging shall be Level A or C as specified (see 6.1).

5.1.1 Unit of issue. One guide, as specified, constitutes one unit of issue.

5.1.2 Packaging quantities. The number of units of issue indicated in Table III shall be packaged in each unit, intermediate, and exterior container, as applicable, for the required level of protection specified in the procurement document.

Table III. Packaging Quantities

Unit package	Intermediate package	Exterior container
1 unit	12 units	432 units

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:35Z
Check the source to verify that this is the current version before use.

5.1.2.1 Packing variation permitted. If the required number of units in the entire shipment is less than the number of units specified to be overpacked in an exterior container, such units may be packed in an exterior container of suitable size and design, acceptable to a common carrier, which shall insure safe delivery to destination.

5.1.3 Level A.

5.1.3.1 Unit package. Each unit shall be packaged in an envelope of suitable size and strength. Envelope shall be adequate to prevent accidental opening.

5.1.3.2 Intermediate package. Intermediate package shall be a box of appropriate size and design constructed in accordance with PPP-B-566 or PPP-B-676, except commercial colors will be acceptable, or PPP-B-636, type CF, class domestic. Closure shall be adequate to prevent accidental opening under normal handling.

5.1.4 Level C. Units shall be packaged in standard commercial containers of the size and kind commonly used, which will afford the degree of protection required for shipment and use of the product for its intended purpose.

5.2 Packing. Packing shall be Level A, B or C as specified (see 6.1).

5.2.1 Level A.

5.2.1.1 Exterior container. Exterior shall be designed for a type 2 load and constructed in accordance with PPP-B-585, class 3, style 3; PPP-B-601, overseas type; PPP-B-621, class 2; or PPP-B-636, class weather-resistant, grade V3c. Closure and strapping shall be as specified in the appendix of the applicable box specification. Special requirements of applicable Table shall apply for PPP-B-636 Box.

5.2.1.2 Case liner. Each Level A wood box shall be lined with a waterproof case liner conforming to MIL-L-10547. Closure and sealing shall conform to applicable paragraphs of appendix thereto. Case liner shall not be required for fiberboard boxes.

5.2.2 Level B.

5.2.2.1 Exterior container. Exterior container shall be designed for a type 2 load and constructed in accordance with PPP-B-585, class 1, style 3; PPP-B-601, domestic type; PPP-B-621, class 1; or PPP-B-636, class domestic. Closure shall be as specified in the appendix of the applicable box specification. Fiberboard box shall be closed by method II of PPP-B-636. Special requirements of applicable Table shall apply for PPP-B-636 Box.

5.2.3 Level C. The subject commodity shall be packed in substantial commercial containers of the type, size, and kind commonly used for the purpose, so constructed as to insure acceptance and safe delivery by common or other carriers, at the lowest rate, to point of delivery called for in the contract or purchase order.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:35Z
Check the source to verify that this is the current version before use.

5.3 Marking.

5.3.1 Interior packages. Each unit package and each intermediate package shall be marked in accordance with MIL-STD-129. When labels are utilized, waterproofing shall be required only when applicable carton is fabricated of water-resistant material. Contract or purchase order number and name of contractor shall be shown.

5.3.2 Exterior container. Exterior container shall be marked in accordance with MIL-STD-129.

6. NOTES

6.1 Ordering data. Procurement documents should specify the following:

(a) Title, number, and date of this specification.

(b) Selection of applicable levels of packaging and packing (see 5.1 and 5.2).

6.2 Supersession data. This specification includes the requirements of Purchase Description Number 3, dated 19 September 1961.

6.3 Federal Stock Number (FSN) coverage. This specification covers the following item appearing in the Federal Supply Catalog.

Stock Number	Item Identification
6520-534-5500	GUIDE, OCCLUSAL PLANE, Fox

6.4 Limitations. This specification does not cover all types, classes, grades, styles, or sizes of the commodity indicated by the title of this specification, or those which are commercially available, but is intended to cover those items which are normally procured to meet Military requirements.

Custodians:
Army - MD
Navy - MS
Air Force - 03

Review activities:
Army - MD
Navy - MS
Air Force - 03

Preparing activity:
Defense Supply Agency - DM

Project No. 6520-1341

Review information is current as of the date of this document. For future coordination of changes to this document, draft circulation should be based on the information in the current DODISS.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:35Z
Check the source to verify that this is the current version before use.

FOLD

DEFENSE PERSONNEL SUPPORT CENTER
2800 South 20th Street
Philadelphia, Pa. 19101

Defense Supply Agency

OFFICIAL BUSINESS
PENALTY FOR PRIVATE USE $300

POSTAGE AND FEES PAID
DEFENSE SUPPLY AGENCY
DoD - 304

U.S.MAIL

HEADQUARTERS, DEFENSE PERSONNEL SUPPORT CENTER
ATTN: DIRECTORATE OF MEDICAL MATERIEL, CODE ATT
2800 SOUTH 20TH STREET
PHILADELPHIA, PA. 19101

FOLD

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:35Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

OMB Approval
No. 22-R255

INSTRUCTIONS: The purpose of this form is to solicit beneficial comments which will help achieve procurement of suitable products at reasonable cost and minimum delay, or will otherwise enhance use of the document. DoD contractors, government activities, or manufacturers/ vendors who are prospective suppliers of the product are invited to submit comments to the government. Fold on lines on reverse side, staple in corner, and send to preparing activity. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements. Attach any pertinent data which may be of use in improving this document. If there are additional papers, attach to form and place both in an envelope addressed to preparing activity.

DOCUMENT IDENTIFIER AND TITLE

MIL-G-36928

NAME OF ORGANIZATION AND ADDRESS

CONTRACT NUMBER

MATERIAL PROCURED UNDER A

☐ DIRECT GOVERNMENT CONTRACT ☐ SUBCONTRACT

1. HAS ANY PART OF THE DOCUMENT CREATED PROBLEMS OR REQUIRED INTERPRETATION IN PROCUREMENT USE?

A. GIVE PARAGRAPH NUMBER AND WORDING.

B. RECOMMENDATIONS FOR CORRECTING THE DEFICIENCIES

2. COMMENTS ON ANY DOCUMENT REQUIREMENT CONSIDERED TOO RIGID

3. IS THE DOCUMENT RESTRICTIVE?

☐ YES ☐ NO *(If "Yes", in what way?)*

4. REMARKS

SUBMITTED BY *(Printed or typed name and address - Optional)*

TELEPHONE NO.

DATE

DD FORM 1 JAN 72 1426 REPLACES EDITION OF 1 JAN 66 WHICH MAY BE USED

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:35Z
Check the source to verify that this is the current version before use.