MIL-N-36930
6 December 1972

MILITARY SPECIFICATION

NEEDLE, BIOPSY, Disposable

This specification is approved for use by all Departments and Agencies of the Department of Defense.

1. SCOPE

1.1 Scope. This specification covers sterile, disposable, axially reciprocating biopsy needles with a 20 mm specimen notch in the obturator. A semi-transparent plastic protective sheath is used to protect the stainless steel cannula and obturator. The biopsy needles shall be suitable for obtaining biopsy samples.

1.2 Classification. Needles shall be of the following types and sizes as specified (see 6.3):

Size 1 - 4½ inches
Size 2 - 6 inches

2. APPLICABLE DOCUMENTS

2.1 The following documents of the issue in effect on date of invitation for bids or request for proposals, form a part of the specification to the extent specified herein:

SPECIFICATIONS

Federal

GG-I-526	Instruments, Dental and Surgical; General Specifications.
PPP-B-585	Boxes, Wood, Wirebound.
PPP-B-601	Boxes, Wood, Cleated-Plywood.
PPP-B-621	Boxes, Wood, Nailed and Lock-Corner.
PPP-B-636	Box, Fiberboard.
PPP-B-676	Box, Setup.

FSC 6515

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:36Z
Check the source to verify that this is the current version before use.

Military

MIL-L-10547	Liners, Case, and Sheet, Overwrap; Water-Vaporproof or Waterproof, Flexible.
MIL-S-36586	Sterilization Strip Test, Bacterial Spore.

STANDARDS

Federal

FED-STD-151	Metal, Test Methods.

Military

MIL-STD-105	Sampling Procedures and Tables for Inspection by Attributes.
MIL-STD-129	Marking for Shipment and Storage.

(Copies of specifications and standards required by suppliers in connection with specific procurement functions should be obtained from the procurement activity or as directed by the procurement officer.)

2.2 Other publications. The following documents form a part of this specification to the extent specified herein. Unless otherwise indicated, the issue in effect on date of invitation for bids or request for proposals shall apply:

THE UNITED STATES PHARMACOPEIAL CONVENTION, INC.

The Pharmacopeia of the United States of America (U.S.P.)

(Application for copies shall be addressed to the Mack Publishing Company, Easton, Pennsylvania 18042.)

U.S. DEPARTMENT OF HEALTH EDUCATION AND WELFARE:

FOOD AND DRUG ADMINISTRATION - Federal Food, Drug, and Cosmetic Act and General Regulations for Its Enforcement.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:36Z
Check the source to verify that this is the current version before use.

(Applications for copies should be sent to Food and Drug Administration, U.S. Department of Health, Education and Welfare, Washington, D.C. 20203.)

3. REQUIREMENTS

3.1 Materials.

3.1.1 Cannula. The cannula shall be fabricated from either seamless drawn or welded and drawn stainless steel tubing AISI type 304. Material shall be tested for composition as specified in 4.4.1.

3.1.2 Obturator. The obturator shall be fabricated from hard drawn AISI type 304 stainless steel. Its composition shall be tested as indicated in 4.4.1.

3.1.3 Hubs. The cannula hub and the obturator hub shall be made of suitable rigid plastic.

3.1.4 Adhesive. A suitable epoxy adhesive shall be used to secure the cannula and obturator to their respective hubs.

3.1.5 Protective sheath. A length of tubing to protect the biopsy needle shall be fabricated from a suitable flexible plastic. It shall be semi-transparent.

3.2 Style, design and construction. Shall be a sterile, pyrogen-free, non-toxic, disposable, biopsy needle. The biopsy needle shall consist of an obturator, cannula and protective sheath. The dimensions shall be in accordance with Figs. 1 & 2.

3.2.1 Cannula. The cannula shall be a 14-gauge needle with a bevel tip and attached hub as shown in Figs. 1 and 2.

3.2.2 Obturator and hubs. The obturator shall be a 16-gauge solid needle to fit and reciprocate within the cannula. The relative position of the bevel tip of the obturator and the cannula bevel tip, and the length of stroke shall be controlled by the design and fit of the hubs. The obturator shall have a 20 mm section removed from it near its distal end. The removed section constitutes the specimen notch. The dimensions, hub, point, and specimen notch shall be as shown in Figs. 1 and 2.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:36Z
Check the source to verify that this is the current version before use.

3.2.3 Protective sheath. The protective sheath shall have dimensions as shown in Fig. 1. In use it is applied over the needle-cannula assembly and as shown in Fig. 1 and shall be long enough to protect the obturator whether in the fully inserted or retracted position.

3.3 Sterility. The biopsy needles shall be sterile when tested with a biological indicator as specified in 4.4.2.

3.3.1 Certificate of sterility. A certificate of sterility, stating that samples from each sterilizer lot have been tested and found to be sterile, shall be submitted to the procuring activity. The certificate of sterility shall include:

a. Item identification.
b. Federal stock number.
c. Contract or purchase order number.
d. Sterility lot or control number.
e. Date of sterilization.
f. Quantity of product in sterilizer lot.
g. Type of sterilization (gas, radiation, heat, steam, etc.).
h. Form of biological indicator (i.e., inoculated paper spore strip or carrier, inoculated product, or inoculated simulated product).
i. Test organism(s) and population density used.
j. Test medium, incubation temperature, incubation time, and dates of tests.
k. Number of test units.
l. Statement that samples comply with sterility tests.
m. Signature of head of laboratory or a designated qualified alternate.

When inspection is made at destination, the certificate of sterility shall be submitted by the contractor to the Directorate of Medical Materiel, ATTN: DPSC-ATQ, Defense Personnel Support Center, 2800 South 20th Street, Philadelphia, Pa., 19101, and a copy forwarded with each shipment to the consignee. When inspection is made at source, certificate of sterility shall be furnished to the cognizant Government Quality Assurance Representative for submission to the procuring activity.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:36Z
Check the source to verify that this is the current version before use.

3.3.2 Sterility lot. A sterility lot is that single quantity of product subjected to the same manufacturing operation and simultaneously sterilized in the same sterilizer chamber. Each unit package shall be clearly marked with a sterility lot (control) number and date of sterilization as specified in 5.3.1. Each sterility lot shall be traceable to the pertinent manufacturing lot(s).

3.4 Freedom from pyrogens. When tested as specified in 4.4.3, biopsy needles shall comply with the pyrogen test requirements of the USP.

3.5 Safety (Non-toxicity). When tested as specified in 4.4.4, biopsy needles shall comply with the safety test requirements of the USP.

3.6 Certificates. For destination inspection only, certificates of sterility, freedom from pyrogens, and safety, as specified below, shall be submitted by the contractor to Defense Personnel Support Center, Directorate of Medical Materiel, 2800 South 20th Street, Philadelphia, Pennsylvania, 19101, and one copy of each shall be forwarded with each shipment to the consignee.

3.6.1 Certificates of safety (non-toxicity). A certificate of safety, listing all lot or control numbers, shall state that samples from each lot or control have been tested for safety as specified in 3.5 and 4.4.4, and were found to comply with such requirements. The certificate shall reference the method used in determining safety.

3.6.2 Certificate of freedom from pyrogens. A certificate of freedom from pyrogens, listing all lot or control numbers, shall state that samples from each lot or control have been tested for pyrogens as specified in 3.4 and 4.4.3, and were found to comply with such requirements. The certificate shall reference the method used in determining freedom from pyrogens.

3.6.3 Certificate of sterility. A certificate of sterility, listing all sterility lot or control numbers, shall state that samples from each sterility lot or control have been tested for sterility, as required in 3.3 and 4.4.2, and have been found to be sterile. The certificate shall reference the method used in determining sterility.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:36Z
Check the source to verify that this is the current version before use.

3.7 Corrosion resistance. The stainless steel cannula and obturator shall comply with the boil test as specified in 4.4.5.

3.8 Instructions. Each biopsy needle shall be provided with instructions describing the proper technique for use.

3.9 Workmanship. Workmanship shall be first class throughout. Biopsy needles shall be free from defects which detract from their appearance or impair their serviceability.

4. QUALITY ASSURANCE PROVISIONS

4.1 Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the supplier is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or order, the supplier may use his own or any other facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

4.1.1 Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government, upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of 3 years after delivery of the supplies to which such records relate.

4.1.2 Inspection. Inspection, as used in this specification, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

4.1.3 Certificates of quality. Certificates of quality supplied by the manufacturer of the components or materials may be furnished in lieu of actual performance of such testing by the contractor, provided lot identity has been maintained and can be demonstrated to the Government. The certificate shall include the name of the contractor, the contract number, the name of the manufacturer or supplier, the FSN, the item identification, the name of the component/material, the lot number, the lot size, the sample size, the date of testing, the test method, individual test results, and the specification requirements.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:36Z
Check the source to verify that this is the current version before use.

4.2 Sampling.

4.2.1 For examination. Sampling for examination shall be conducted in accordance with MIL-STD-105. The inspection levels and acceptable quality levels shall be as indicated in Table I. The unit of product for examination shall be one biopsy needle complete with protective sheath.

Table I. Sampling for Examination

Type of defect	Inspection level	AQL (percent defective)*
Major	S-2	1.0
Minor	S-1	2.5

*If acceptance number is not exceeded, lot shall be accepted. If rejection number is equaled or exceeded, inspection at Level II shall be performed to determine final acceptance or rejection.

4.2.2 For tests. Sampling for tests shall be in accordance with MIL-STD-105 and as shown in Table II.

Table II. Sampling Criteria for Tests

Characteristic	Requirement	Test procedure	Inspection level	AQL (percent defective)
Composition	3.1.1 and 3.1.2	4.4.1	S-1	2.5
Sterility	3.3	4.4.2	S-2	*
Freedom from pyrogens	3.4	4.4.3	S-1	*
Safety	3.5	4.4.4	S-1	*
Corrosion resistance	3.7	4.4.5	S-1	1.5

*Acceptance number shall be zero for all sample sizes.

4.2.3 Test samples. Where feasible, the same sample shall be used for the determination of two or more test characteristics.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:36Z
Check the source to verify that this is the current version before use.

4.3 Examination. The biopsy needles shall be examined to determine compliance with all requirements contained in the specification. Examination shall be conducted as specified in Tables I and III. Examination, however, shall not be restricted to the defects listed in Table III.

Table III. Classification of Defects

Categories	Defects
Major	
101	Biopsy needle not free from foreign matter.
102	Obturator not free from burs.
103	Cannula bevel not free from burs.
104	Obturator action not smooth through entire range of stroke.
105	Specimen notch of obturator does not have sharp edges.
106	Bevels of cannula and obturator not in proper relative position to each other and to hubs.
Minor	
201	Protective sheath not properly attached to projection from cannula hub.
202	Length of stroke does not go beyond each end of the specimen notch.
203	Cannula and obturator hubs not precisely mated to control obturator stroke.

4.4 Tests. Tests shall be conducted to determine compliance with specification requirements.

4.4.1 Composition. The chemical analysis of the stainless steel cannula and obturator shall be performed in accordance with Method 111.2 of Federal Test Method Standard No. 151.

4.4.2 Sterility test. The biopsy needles shall be tested for sterility in accordance with the method specified in the USP for parenteral devices using inoculated product, inoculated simulated product, or paper spore

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:36Z
Check the source to verify that this is the current version before use.

strip (carrier). Product containing a biological indicator shall be marked or labeled so that it clearly differentiates from product intended for distribution. The incubation medium and minimum time in each case shall be soybean casein digest for 7 days for inoculated product, inoculated simulated product, or paper spore strip (carrier). The incubation temperature shall be as indicated in paragraph 4.4.2.1. The minimum number of test units, regardless of lot size, shall be 10, except for inoculated carrier which shall be 20 for Type I Sterilization and 30 for Type II Sterilization including inoculated carrier and product test units. The inspection level shall be as indicated in Table II, Sampling Criteria for Tests.

4.4.2.1 Inoculated product or simulated product. For each type of sterilization, the organism used shall be as listed below:

Type of Sterilization	Organism	Incubation Temperature
Steam	B. stearothermophilus	55° - 65°C
Dry Heat	B. stearothermophilus, or	55° - 65°C
	B. subtilis var. niger (or globigii)	30° - 35°C
Gas	B. subtilis var. niger (or globigii)	30° - 35°C
Radiation	B. pumilus	30° - 35°C

The number of viable cells shall be sufficient to provide assurance that the product has been sterilized.

4.4.2.2 Inoculated carrier. Inoculated carriers (paper spore strips) if used shall be in accordance with MIL-S-36586. Other paper carriers shall be inoculated to be of equivalent resistance. The method of incubation and number of test units shall be as indicated in 4.4.2 Sterility test and 4.4.2.1 Inoculated product or simulated product. The method of sterilization will control the organism in the spore strip to be tested for as shown in 4.4.2.1. NOTE: When an inoculated carrier is chosen, product samples must also be tested as required by the USP.

4.4.2.3 Alternate method. Suppliers conducting sterility tests or designating lots in a manner other than that indicated herein shall submit proof that the alternate method provides equal assurance concerning the sterility of the product. However, all sterility tests shall be conducted using biological indicators. Requests for approval of any alternate method of testing for sterility shall be made to the Contracting Officer, and approval obtained before employment of the alternate method on a government contract.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:36Z
Check the source to verify that this is the current version before use.

4.4.2.4 Product testing. Testing for sterility of the product after receipt by the government shall be without a biological indicator and in accordance with the USP.

4.4.3 Freedom from pyrogens. The pyrogen test shall be performed as described in the current edition of the USP for Transfusion and Infusion Assemblies, except that the cannula and obturator shall be immersed for four minutes in the same 40 ml of saline test solution. Immersion shall be up to 1/8 inch of the hubs and the obturator and cannula shall be disassembled during the immersion.

4.4.4 Safety (Non-toxicity). The safety test shall be performed as described in the current edition of the USP in Transfusion and Infusion Assemblies, except that the cannula and obturator shall be disassembled from each other and placed in a borosilicate glass test tube or other cylindrical vessel containing the saline solution and immersed to within 1/8 inch of the hubs.

4.4.5 Corrosion resistance. The boil test shall be performed in accordance with requirements of GG-I-526.

5. PREPARATION FOR DELIVERY

5.1 Packaging.

5.1.1 Unit of issue. One biopsy needle, as specified, constitutes one unit of issue.

5.1.2 Packaging quantities. The number of units of issue indicated in Table IV shall be packaged in each unit, intermediate, and exterior container, as applicable, for the required level of protection specified in the procurement document.

Table IV. Packaging Quantities

Unit package	Intermediate package	Exterior container
1 unit	12 units	72 units

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:36Z
Check the source to verify that this is the current version before use.

5.1.2.1 Packing variation permitted. If the required number of units to be shipped is less than the number of units specified to be overpacked in an exterior container, such units may be packed in an exterior container of suitable size and design, acceptable to a common carrier, which shall insure safe delivery to destination.

5.1.3 Level A.

5.1.3.1 Unit package. Each biopsy needle shall be packaged in a sealed tamper-proof container of an appropriate size and shall be capable of maintaining sterility of contents unless damaged or opened. The container shall be a combination clear polyethylene and paperback or clear rigid plastic and paperback. The container shall be a peel type and designed with tabs to facilitate dispensing. The needle shall be held securely in place in such a manner so that the point cannot be damaged by contact with any part of the container.

5.1.3.2 Intermediate package. Intermediate package shall be a box of appropriate size constructed in accordance with PPP-B-636, type CF, class domestic or PPP-B-676 except that commercial colors are acceptable. Closure shall be adequate to prevent spilling of contents under normal handling.

5.1.4 Level C. Units shall be packaged in standard commercial containers of the size and kind commonly used, which will afford the degree of protection required for shipment and use of the product for its intended purpose.

5.2 Packing.

5.2.1 Level A.

5.2.1.1 Exterior container. Exterior container shall be designed for a type 2 load and constructed in accordance with PPP-B-585, class 3, style 3; PPP-B-601, overseas type; PPP-B-621, class 2; or PPP-B-636, class weather-resistant. Fiberboard boxes shall conform to the special requirements specified in Table II of PPP-B-636.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:36Z
Check the source to verify that this is the current version before use.

5.2.1.2 Case liner. Each level A wood box shall be lined with a waterproof case liner conforming to MIL-L-10547. Closure and sealing shall conform to applicable paragraphs of appendix thereto. Case liner shall not be required for fiberboard boxes.

5.2.1.3 Closure. Closure of wood boxes shall be in accordance with appendix of applicable box specification. Closure of each fiberboard box shall be as specified in the appendix, and waterproofing shall conform with 30.4 of PPP-B-636.

5.2.1.4 Strapping. Strapping, when required, shall be in accordance with appendix of applicable box specification.

NOTE: Strapping shall not be required for shipments forwarded to a receiving activity within the continental limits of the United States for storage and redistribution.

5.2.2 Level B.

5.2.2.1 Exterior container. Exterior container shall be designed for a type 2 load and constructed in accordance with PPP-B-585, class 1, style 3; PPP-B-601, domestic type; PPP-B-621, class 1; or PPP-B-636, class domestic. Closure shall be as specified in the appendix of the applicable box specification. Fiberboard box shall be closed by method II of PPP-B-636. Fiberboard boxes shall conform to special requirements specified in Table I of PPP-B-636.

5.2.3 Level C. The subject commodity shall be packed in substantial commercial containers of the type, size, and kind commonly used for the purpose, so constructed as to insure acceptance and safe delivery by common or other carriers, at the lowest rate, to point of delivery called for in the contract or purchase order.

5.3 Marking.

5.3.1 Unit package. In addition to any commercial markings, each unit package shall be marked in accordance with MIL-STD-129 and the requirements of the Federal Food, Drug and Cosmetic Act. Sterility lot (control) number, contract or purchase order number and name of contractor shall be shown. The method of sterilization (G-Gas, R-Radiation, C-Cold, S-Steam,

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:36Z
Check the source to verify that this is the current version before use.

D-Dry Heat Sterilization) shall be shown following the level of packaging and date of packaging. Example: "A-12/72-G". Final sterilization shall be on or after indicated packaging date. In addition, marking shall include the legend: "STERILITY GUARANTEED UNLESS PACKAGE IS DAMAGED OR OPENED" or similar statement. Marking shall be placed on the container or on an insert placed within the container in such a manner as to permit ready identification.

5.3.2 Intermediate package. Each intermediate package shall be marked in accordance with MIL-STD-129. Sterility lot (control) number, contract, or purchase order number and name of contractor shall be shown. The method of sterilization as specified in 5.3.1 shall also be shown.

5.3.3 Exterior container. Exterior container shall be marked in accordance with MIL-STD-129. Sterility lot (control) number and the method of sterilization as specified in 5.3.1 shall be shown.

6. NOTES

6.1 Intended use. The biopsy needles are intended generally for prostatic and renal biopsies.

6.2 This specification is intended to cover the following items appearing in the Federal Supply Catalog:

FSN	Item Identification
6515-104-8390	NEEDLE, BIOPSY, Disposable, 14 Gage, 6 Inch, Sterile, Each
6515-487-9782	NEEDLE, BIOPSY, Disposable, 14 Gage, 4-1/2 Inch, Sterile, Each

It does not include all types or sizes as indicated by the title nor all types which are commercially available.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:36Z
Check the source to verify that this is the current version before use.

6.3 Ordering data. Procurement documents should specify the following:

(a) Number and date of this specification.
(b) Type and size required (see 1.2).
(c) Selection of applicable levels of packaging and packing (see 5.1 and 5.2).

Custodians:

Army - MD
Navy - MS
Air Force - 03

Preparing activity:

Defense Supply Agency - DM


Project No. 6515-1686

Review activities:


Army - MD
Navy - MS
Air Force - 03

Review information is current as of the date of this document. For future coordination of changes to this document, draft circulation should be based on the information in the current DODISS.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:36Z
Check the source to verify that this is the current version before use.

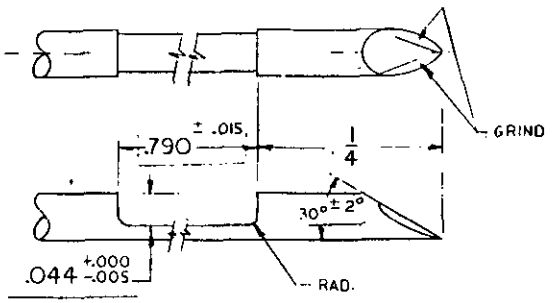


OBTURATOR TIP DETAIL

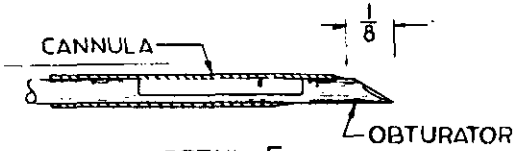

DETAIL F

ENLARGED VIEW OF TIP OF BIOPSY NEEDLE SHOWING OBTURATOR IN FULLY RETRACTED POSITION

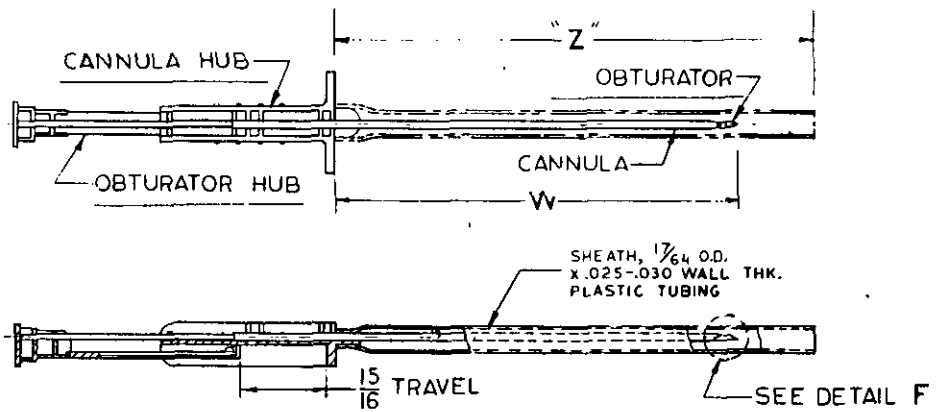

BIOPSY NEEDLE ASSEMBLY


SCHEDULE OF DIMENSIONS					
FSN	SIZE	DIM W	DIM X	DIM Y	DIM Z
6515-104-8390	6"	$6 \pm \frac{1}{8}$	$9\frac{11}{16} \pm \frac{1}{32}$	$7\frac{3}{16} \pm \frac{1}{32}$	$7\frac{1}{2}$
6515-487-9782	$4\frac{1}{2}$"	$4\frac{1}{2}$ +1/4 -1/8	$8\frac{1}{4} + \frac{1}{32}$	$5\frac{11}{16} + \frac{1}{32}$	6

NOTES:


1. UNLESS OTHERWISE SPECIFIED DIMENSIONS ARE IN INCHES AND TOLERANCES ON FRACTIONS SHALL BE ± 1/64".
2. TOLERANCES ON DIMENSIONS MARKED NOMINAL SHALL BE IN ACCORDANCE WITH ACCEPTED COMMERCIAL PRACTICE.
3. TOLERANCES INDICATED DELINEATE ACCEPTABLE EXTREME DIMENSIONS, AND ARE NOT INTENDED TO PERMIT VARIATIONS WITHIN A SINGLE INSTRUMENT WHICH WILL SACRIFICE UNIFORMITY, SYMMETRY, AND FIRST QUALITY WORKMANSHIP.

FIGURE 1

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:56Z
Check the source to verify that this is the current version before use.

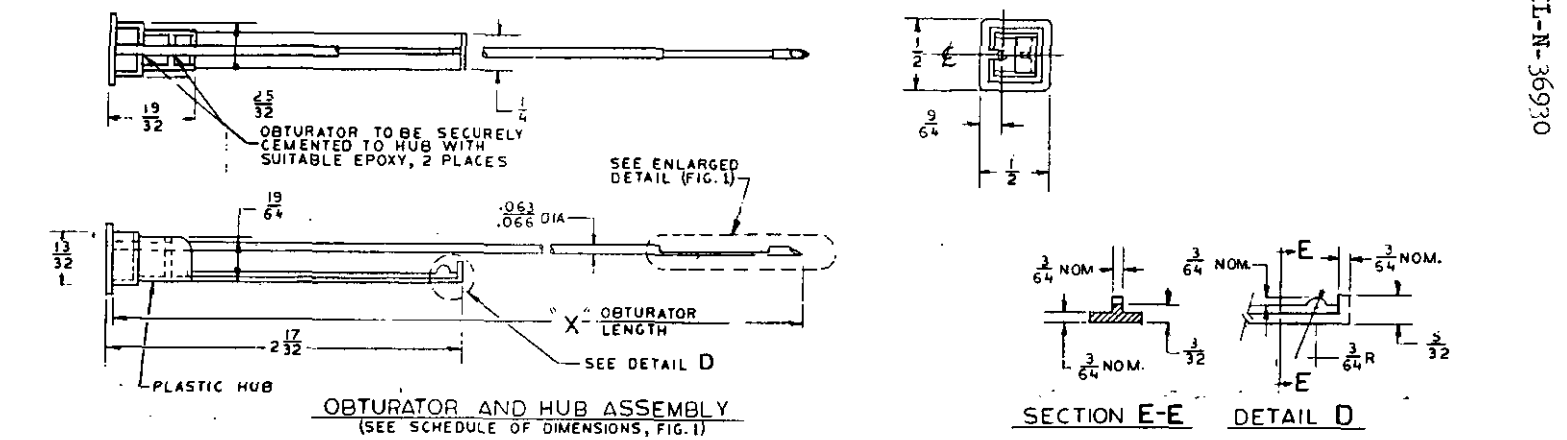

OBTURATOR AND HUB ASSEMBLY
(SEE SCHEDULE OF DIMENSIONS, FIG. 1)

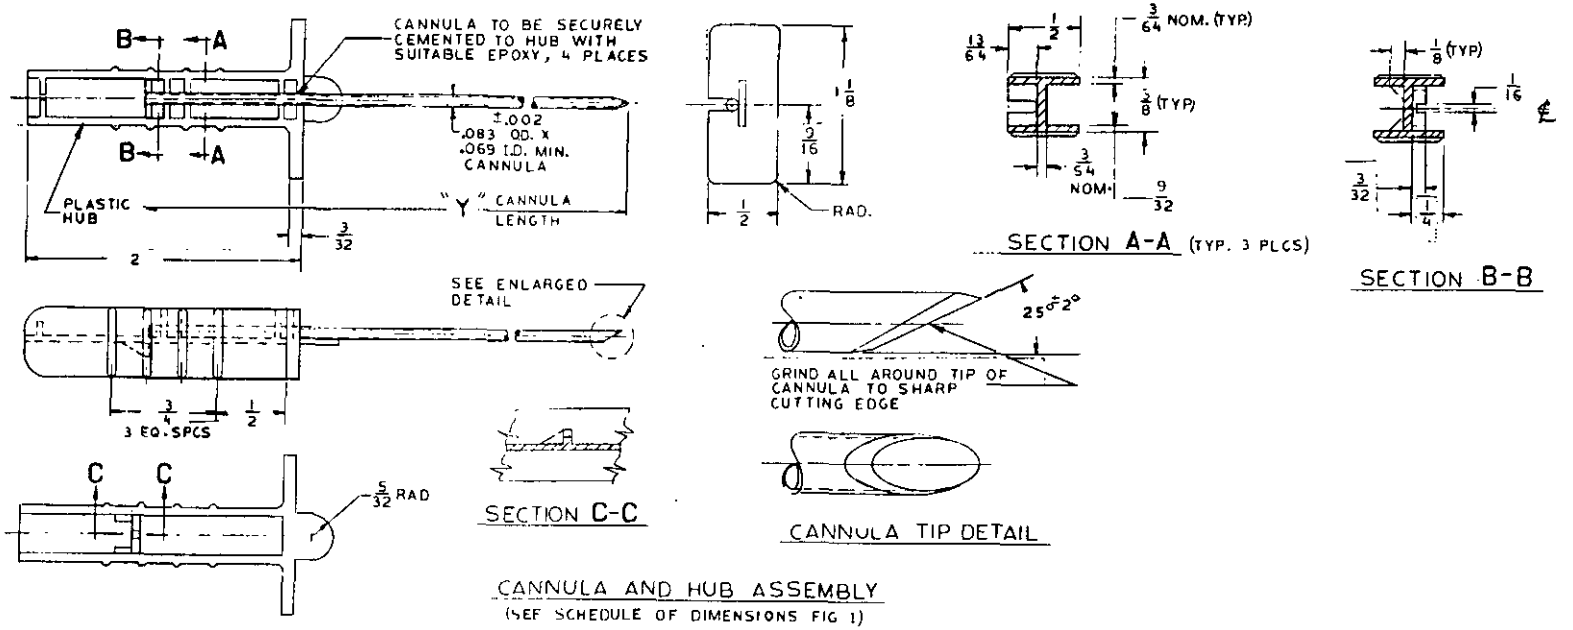

CANNULA AND HUB ASSEMBLY
(SEE SCHEDULE OF DIMENSIONS FIG 1)

FIGURE 2

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:16Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

OMB Approval
No. 22-R255

INSTRUCTIONS: The purpose of this form is to solicit beneficial comments which will help achieve procurement of suitable products at reasonable cost and minimum delay, or will otherwise enhance use of the document. DoD contractors, government activities, or manufacturers/ vendors who are prospective suppliers of the product are invited to submit comments to the government. Fold on lines on reverse side, staple in corner, and send to preparing activity. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements. Attach any pertinent data which may be of use in improving this document. If there are additional papers, attach to form and place both in an envelope addressed to preparing activity.

DOCUMENT IDENTIFIER AND TITLE

MIL-N-36930

NAME OF ORGANIZATION AND ADDRESS

CONTRACT NUMBER

MATERIAL PROCURED UNDER A

☐ DIRECT GOVERNMENT CONTRACT ☐ SUBCONTRACT

1. HAS ANY PART OF THE DOCUMENT CREATED PROBLEMS OR REQUIRED INTERPRETATION IN PROCUREMENT USE?

A. GIVE PARAGRAPH NUMBER AND WORDING.

B. RECOMMENDATIONS FOR CORRECTING THE DEFICIENCIES

2. COMMENTS ON ANY DOCUMENT REQUIREMENT CONSIDERED TOO RIGID

3. IS THE DOCUMENT RESTRICTIVE?

☐ YES ☐ NO *(If "Yes", in what way?)*

4. REMARKS

SUBMITTED BY *(Printed or typed name and address - Optional)*

TELEPHONE NO.

DATE

DD FORM 1 JAN 72 1426

REPLACES EDITION OF 1 JAN 66 WHICH MAY BE USED

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:36Z
Check the source to verify that this is the current version before use.