A-A-54292
30 November 1990

COMMERCIAL ITEM DESCRIPTION

BURS, DENTAL EXCAVATING (Tungsten Carbide)

The General Services Administration has authorized the use of this Commercial Item Description as a replacement for Federal Specification GG-B-821 and Interim Federal Specification GG-B-00821E which are cancelled.

Salient Characteristics:

This commercial item description covers excavating burs suitable for use in dental cavity preparations.

Except as noted below, the burs shall be in accordance with the latest issue of ANSI (American National Standards Institute)/ADA (American Dental Association) Specification No. 23. In case of a conflict, this document shall govern.

Types. Dental burs covered by this description shall be type II (carbide) burs.

Classes. In addition to those bur classes covered in ADA Specification No. 23 the following class will be covered by this document:

Class 2a - Straight handpiece - J-notched

Material.

Tungsten carbide. The burs shall be of two-piece construction. The head shall be fabricated from one solid piece of cemented tungsten carbide with cobalt binder.

Steel. The one-piece shank, neck and bur head base shall be fabricated from hardened and properly tempered AISI-S5 tool steel, or as an alternate, martensitic corrosion resisting steel type 420C in accordance with ASTM designation F899 with a minimum Rockwell hardness of C45. The filler metal used in joining carbide to corrosion resistant steel shall contain a minimum of 47% silver and shall have a melting range of 1290°F to 1590°F. Rockwell hardness shall be tested as specified in ASTM designation E18.

AMSC N/A FSC 6520

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:32Z
Check the source to verify that this is the current version before use.

Dimensions. Dimensions for burs not covered in ADA Specification No. 23 shall be as shown in Table 1 of this description. Shank dimensions for class 2a burs shall be in accordance with Figure 1 of this description. Class 1a, 1b, 2 and 2a shanks may have flat ends provided the edges are rounded.

Design and construction. The burs shall be suitable for use in the cavity preparation of natural dentition. The bur shall consist of a shank, a neck and a head. The joint between the head and neck shall be smoothly machined so that the resultant shape has the appearance of an integral head unit.

Increase in runout. The increase in runout shall be no greater than 0.003 inch when determined only on those samples which have been subjected to the neck strength test, and shall be performed in the manner specified for runout. The difference between the final and the initial runout shall be taken as the increase in runout.

Cutting ability. The maximum total time for cutting a brass sheet horizontally shall be as specified in Table 2 of this description for the applicable bur size number, when tested as specified herein.

Durability. The minimum total depth of 25 holes shall be as specified in Table 3 of this description for the applicable bur size number, when tested as specified herein.

Autoclaving. The entire surface area of the non-carbide portion of the bur shall be examined for evidence of corrosion after the bur is cleaned in accordance with the instructions supplied by the manufacturer and autoclaved at 270 $\pm$ 5°F and 27 $\pm$ 1 psi pressure for a minimum of 20 minutes. Corrosion present at the welded joint shall be disregarded, and shall not be cause for rejection.

Finish. The bur head shall have a finely honed finish with sharpened blades. The neck and shank of burs shall be smoothly finished. The tool steel portion of burs, when applicable shall be chromium or nickel plated. A flash gold plating shall be optional on No. 1931 and No. 1958 burs. Latch type and J-notched burs shall have latch and J-notched ends cleanly finished and free of burrs and slivers.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:32Z
Check the source to verify that this is the current version before use.

Table 1. Head and neck dimensions

USA SIZE	MIN NO. BLADES	Head DIAMETER IN.	Head DIAMETER TOL.	CARBIDE LENGTH MINIMUM TYPE II IN.	TAPER/CONE ANGLE (TOTAL BOTH SIDES) TYPE II DEGREES	Neck NECK DIAMETER MAXIMUM IN.
Round-plain blade						
1/4	6	0.019	0.003	0.012	--	0.016
Tapered fissure, long-plain blade, flat end						
169L	6	0.035	0.003	0.193	4-8	0.035
Amalgam preparation						
245	6	0.035	0.003	0.107	1-3	0.033
Inlay preparation						
271	6	0.047	0.003	0.105	4-8	0.048
Pear shape-plain blade						
1/2P	6	0.024	0.003	0.016	--	0.019
329	6	0.024	0.003	0.059	4-8	0.019
Pear shape, long-plain blade						
330L	6	0.031	0.003	0.110	4-8	0.027
Tapered fissure-crosscut blade, flat end						
699	6	0.035	0.003	0.126	4-8	0.035
703[1/]	6	0.083	0.003	0.177	4-8	0.067
Straight fissure-plain blade, dome						
1157	6	0.039	0.003	0.146	0-2	0.035
Pear-fine crosscut						
1931	6	0.039	0.003	0.059	2-4	0.030
Straight fissure-fine crosscut, dome						
1958	6	0.047	0.003	0.146	0-2	0.047

[1/] The distal head diameter of the 703 bur shall be 0.058 ± 0.002 inch.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:32Z
Check the source to verify that this is the current version before use.

Table 2. Cutting ability requirements.

USA SIZE	THICKNESS OF BRASS SHEET	DEPTH OF SETTING FOR CUT	PROJECTION OF BUR TIP THROUGH SHEET	MAXIMUM TOTAL CUTTING TIME
	IN.	IN.[2]	IN.	SECONDS
1/4	0.011	0.015	0.004	40
1/2	0.011	0.015	0.004	40
1/2P	0.011	0.015	0.004	40
2	0.011	0.022	0.011	25
4	0.020	0.034	0.014	25
4S	0.020	0.034	0.014	25
6	0.020	0.042	0.022	25
8	0.020	0.052	0.032	25
33-1/2	0.011	0.016	0.005	25
34	0.011	0.016	0.005	25
35	0.011	0.016	0.005	25
35S	0.011	0.016	0.005	25
37	0.020	0.025	0.005	50
39	0.020	0.025	0.005	50
56	0.020	0.060	0.040	50 wet[3]
57	0.020	0.060	0.040	50
168	0.011	0.051	0.040	50
169L	0.020	0.060	0.040	50 wet[3]
170L	0.020	0.060	0.040	50 wet[3]
545	0.011	0.016	0.005	25
271	0.020	0.060	0.040	50
329	0.011	0.016	0.005	25
330	0.011	0.016	0.005	25
330L	0.011	0.016	0.005	25
331L	0.020	0.060	0.040	50
556S	0.020	0.060	0.040	50

[2] The "Depth of setting for cut" indicates the depth of the bur tip below the top surface of the brass sheet. The difference between this depth and the "Thickness of brass sheet" is the "Projection of the bur tip through sheet" (distance from the bottom surface of the brass sheet downward to the tip of the bur).

[3] A lubricant or other suitable cutting fluid shall be used for the cutting test on the 56, 169L and 170L burs only.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:32Z
Check the source to verify that this is the current version before use.

Table 2. Cutting ability requirements (continued).

USA SIZE	THICKNESS OF BRASS SHEET	DEPTH OF SETTING FOR CUT	PROJECTION OF BUR TIP THROUGH SHEET	MAXIMUM TOTAL CUTTING TIME
	IN.	IN.[2]	IN.	SECONDS
557	0.020	0.060	0.040	50
558	0.020	0.060	0.040	50
558S	0.020	0.060	0.040	50
559	0.020	0.060	0.040	50
699	0.011	0.051	0.040	50
700	0.020	0.060	0.040	50
701	0.020	0.060	0.040	50
702	0.020	0.060	0.040	50
703	0.020	0.060	0.040	50
957	(Tests not applicable)			
1157	0.020	0.060	0.040	50
1931	0.011	0.016	0.005	25
1958	0.020	0.060	0.040	50

Table 3. Durability requirements.

USA BUR SIZE NUMBER	MINIMUM TOTAL DEPTH OF 25 HOLES, INCH
1/4	0.200
1/2	0.240
1/2P	0.240
2	0.400
4	0.400
4S	0.400
6	0.400
8	0.400
33-1/2	0.240
34	0.240
35	0.300
35S	0.300
37	0.400
39	0.400
56	0.325
57	0.400

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:32Z
Check the source to verify that this is the current version before use.

Table 3. Durability requirements (continued).

USA BUR SIZE NUMBER	MINIMUM TOTAL DEPTH OF 25 HOLES, INCH
168	0.300
169L	0.300
170L	0.325
245	0.300
271	0.400
329	0.300
330	0.300
330L	0.300
331L	0.300
556S	0.325
557	0.400
558	0.400
558S	0.400
559	0.400
699	0.300
700	0.300
701	0.400
702	0.400
703	0.400
957	(Tests not applicable)
1157	0.400
1931	0.300
1958	0.400

Marking. Marking of burs shall be optional. The use of a trademark is optional. The type of marking or placement of the marking shall not adversely affect or interfere with the handpiece. Markings shall be distinguishable to the unaided eye.

Instructions. Adequate and accurate instructions shall be furnished with each unit of issue on the use and care of the burs. Instructions shall also include the type of solutions, both suitable and unsuitable for cold sanitation of the burs.

Workmanship. The burs shall have uniformly cut and formed blades and shall be free from defects which detract from their appearance or may impair their intended use.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:32Z
Check the source to verify that this is the current version before use.

Unit. Package (PG). One package containing 10 individually separated burs of one type, class and size only, as specified, constitutes one unit.

Quality Assurance Provisions.

General. Quality assurance provisions shall be as specified in this document. Sections 4.1 through 4.1.2 of ADA Specification No. 23 shall not apply.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after the delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Sampling for examination. Sampling for examination shall be conducted in accordance with MIL-STD-105, with an inspection level of II and AQL (Percent defective) of 2.5. The unit of product for examination purposes shall be one bur.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:32Z
Check the source to verify that this is the current version before use.

Examination. Examination shall be as specified herein. Examination shall include, but shall not be limited to the following:

Defects

Bur size number or head shape not as specified.
Bur shank (class) not as specified.
Cut off end on shank not as shown in applicable figure.
Burs not free from defects such as chipped blades, cracks or pits.
Number of blades not as specified for the applicable bur size number.
Finish on bur not as specified.
Instructions for use inaccurate, inadequate or missing.
Welded joint of bur does not give the appearance of an integral head unit.
Packaging not as specified.

Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and as specified below. The acceptance number shall be zero for all sample sizes. The unit of product for test purposes shall be as specified below.

Test Criteria

Characteristics	Requirement	Test procedure	Inspection level	Unit of product
Hardness	Herein	Herein	S-1	1 bur
Dimensions	ADA No. 23	ADA No. 23	S-1	1 bur
Runout	ADA No. 23	ADA No. 23	S-3	1 bur
Surface roughness	ADA No. 23	ADA No. 23	S-1	1 bur
Neck strength	ADA No. 23	ADA No. 23	S-3	1 (class 4 bur)
Increase in runout	Herein	Herein	S-3	1 bur
Cutting ability	Herein	Herein	S-1	5 burs
Durability	Herein	Herein	S-1	5 burs
Autoclaving	Herein	Herein	S-1	1 bur

Tests. Tests shall be conducted to determine compliance with specification requirements. Tests not specified in this document shall be performed in accordance with the procedures specified in ADA Specification No. 23 or as otherwise specified. Where feasible, the same sample shall be used for the determination of two or more test characteristics.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:32Z
Check the source to verify that this is the current version before use.

Cutting ability.

Test material. The test material shall be cartridge brass sheet conforming to copper alloy no. C26000 of ASTM designation B36. The sheet shall have a Rockwell hardness of B40 to B65 and shall have a thickness of 0.011 inch (24 gage Brown and Sharpe) or 0.020 inch (29 gage B & S), as specified in Table 2 of this description. The sheet shall be cut into strips of suitable size for use in the test equipment as specified below.

Equipment for tests. The equipment shall consist of a precision chuck capable of holding the burs to be tested, a movable carriage for the test material, and the necessary accessories for measuring within 0.5 second the time required for the bur to cut 0.020 inch. The equipment shall be capable of applying a constant one-pound contact load between the bur and the test strip perpendicular to the bur axis.

Test procedure. A test bur and a brass sheet of the proper thickness shall be placed in the test equipment. The bur shall be positioned perpendicular to the brass strip and the relative heights adjusted as specified in Table 2 of this description. The bur shall be rotated at a speed of 4350 ± 50 revolutions per minute (rpms) and brought into contact with the edge of the brass strip. A preliminary cut equal to one-half to one bur diameter shall be made before readings are taken. The time required for the bur to cut horizontally a distance of 0.020 inch into the sheet shall be determined to ± 0.5 second. The test shall be repeated until a total of 5 burs have been tested.

Durability.

Test material. The test material shall be a crystal plate glass, a minimum of 1/8 inch thick, having a Knoop hardness of 450 to 510 with a one kilogram load.

Equipment for test. The equipment shall consist of a true-running chuck capable of holding and rotating the bur being tested, and a movable platform or carriage suitable for carrying the flat surface of a glass test block into contact with the bur at an angle of 22-1/2 ± 1/2 degrees from the axis of the bur. The equipment shall be capable of maintaining a constant contact load of one pound perpendicular to the glass surface.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:32Z
Check the source to verify that this is the current version before use.

Test procedure. A test bur shall be placed in the chuck of the test equipment and rotated at 1550 ± 50 rpms. The glass test plate shall be slowly brought into contact with the bur, and held in contact with it.

The bur shall be permitted to cut into the glass, with turpentine used as the cutting fluid. After 2000 revolutions of the bur the plate shall be moved to expose a fresh, uncut portion of flat glass surface, and the test shall be repeated until a total of 5 holes have been drilled by the test bur. The bur shall then be removed, and a second test bur inserted into the chuck. The test shall be continued until a total of 5 burs have been tested, and total of 25 holes drilled. The plate shall be removed and the depth of holes shall be measured with a sharp point on a dial gage sensitive to 0.0002 inch. (The point of the gage shall meet the requirements of ASTM designation D5).

Contractor certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producer's own drawings, specifications, standards, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Metric products. Products manufactured to metric dimensions will be considered on an equal basis with those manufactured using inch/pound units, providing they fall within the tolerances specified using conversion tables contained in the latest revision of Federal Standard No. 376, and all other requirements of this document are met. If a product is manufactured to metric dimensions and those dimensions exceed the tolerances specified in the inch/pound units, a request should be made to the contracting officer to determine if the product is acceptable. The contracting officer has the option of accepting or rejecting the product.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:32Z
Check the source to verify that this is the current version before use.

Regulatory requirement.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Federal Acquisition Regulation Subpart 23.4 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

Ordering data. Intermediate/exterior package quantities, labeling and marking must be specified in the contract and/or order.

NOTE: The following National Stock Numbers are covered by this document:

National Stock Number	Item Identification	Class	Size
6520-00-000-0064	BUR, DENTAL, EXCAVATING,	1a	957
6520-00-003-2274	Angle Handpiece, Tungsten	1a	2
6520-01-003-2263	Carbide, 10s	1a	559
6520-01-003-2264		1a	701
6520-01-003-2265		1a	702
6520-01-003-2266		1a	703
6520-01-003-2272		1a	35
6520-01-003-2273		1a	39
6520-01-003-2275		1a	4
6520-01-003-2276		1a	8
6520-01-003-2426		1a	558

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:32Z
Check the source to verify that this is the current version before use.

National Stock Number	Item Identification	Class	Size
6520-01-003-3129	BUR, DENTAL, EXCAVATING,	1a	557
6520-01-003-3138	Angle Handpiece, Tungsten	1a	700
6520-01-003-5346	Carbide, 10s (continued)	1a	37
6520-01-003-7703		1a	6
6520-01-049-0422		1a	1/2
6520-01-049-0423		1a	33-1/2
6520-01-106-3138		1a	699
6520-01-106-3139		1a	1/4
6520-01-003-2124	BUR, DENTAL, EXCAVATING,	2	703
6520-01-003-2259	Straight Handpiece,	2	558
6520-01-003-2260	Tungsten Carbide, 10s	2	559
6520-01-003-2261		2	701
6520-01-003-2262		2	702
6520-01-003-2267		2	35
6520-01-003-2268		2	37
6520-01-003-2269		2	2
6520-01-003-2270		2	4
6520-01-003-2271		2	6
6520-01-003-3131		2	8
6520-01-003-3132		2	1/2
6520-01-003-3133		2	33-1/2
6520-01-003-3134		2	557
6520-01-003-3135		2	700
6520-01-262-8685	BUR, DENTAL, EXCAVATING,	2a	702
6520-01-263-2605	Straight Handpiece,	2a	703
	J-Notched, Tungsten Carbide, 10s		
6520-01-003-2277	BUR, DENTAL, EXCAVATING,	4a	558
6520-01-003-2278	Friction Grip Angle	4a	699
6520-01-003-2280	Handpiece, Tungsten	4a	700
6520-01-003-2281	Carbide, 10s	4a	37
6520-01-003-2282		4a	4
6520-01-003-2427		4a	33-1/2
6520-01-003-2428		4a	1/4
6520-01-003-2429		4a	330
6520-01-003-3130		4a	2
6520-01-003-3136		4a	35
6520-01-003-3137		4a	6
6520-01-003-3139		4a	701
6520-01-003-3915		4a	56
6520-01-003-3916		4a	57
6520-01-003-3918		4a	34
6520-01-003-3919		4a	1/2

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:32Z
Check the source to verify that this is the current version before use.

National Stock Number	Item Identification	Class	Size
6520-01-003-4139	BUR, DENTAL, EXCAVATING,	4a	957
6520-01-003-7702	Friction Grip Angle	4a	557
6520-01-078-5684	Handpiece, Tungsten	4a	1931
6520-01-099-2318	Carbide, 10s (continued)	4a	245
6520-01-106-0098		4a	1157
6520-01-106-0099		4a	1958
6520-01-106-0100		4a	271
6520-01-137-8443		4a	328
6520-01-137-8444		4a	168
6520-01-263-2604		4a	1/2P
6520-01-003-2121	BUR, DENTAL, EXCAVATING,	4b	558S
6520-01-003-2122	Friction Grip Angle	4b	4S
6520-01-003-2123	Handpiece, Tungsten	4b	35S
6520-01-106-0097	Carbide, Short Shank, 10s	4b	556S
6520-01-003-3917	BUR, DENTAL, EXCAVATING,	4c	170L
6520-01-003-7701	Friction Grip Angle	4c	169L
6520-01-106-0931	Handpiece, Tungsten	4c	331L
6520-01-262-8683	Carbide, Long Shank, 10s	4c	330L
6520-01-221-9082	BUR, DENTAL, EXCAVATING,	4d	2
6520-01-221-9083	Friction Grip Angle	4d	4
6520-01-221-9084	Handpiece, Tungsten	4d	6
6520-01-221-9085	Carbide, Surgical Shank, 10s	4d	8

MILITARY INTERESTS:

Custodians:

Army-MD
Navy-MS
Air Force-03

PREPARING ACTIVITY:

DoD-MB

Agent:

DLA-DM

CIVIL AGENCY COORDINATING ACTIVITIES:

VA-OSS
PHS
FDA-MPQAS

PROJECT NO. 6520-2055
LOCATION: PB FLOPPY #1/CDBURSEX

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:32Z
Check the source to verify that this is the current version before use.

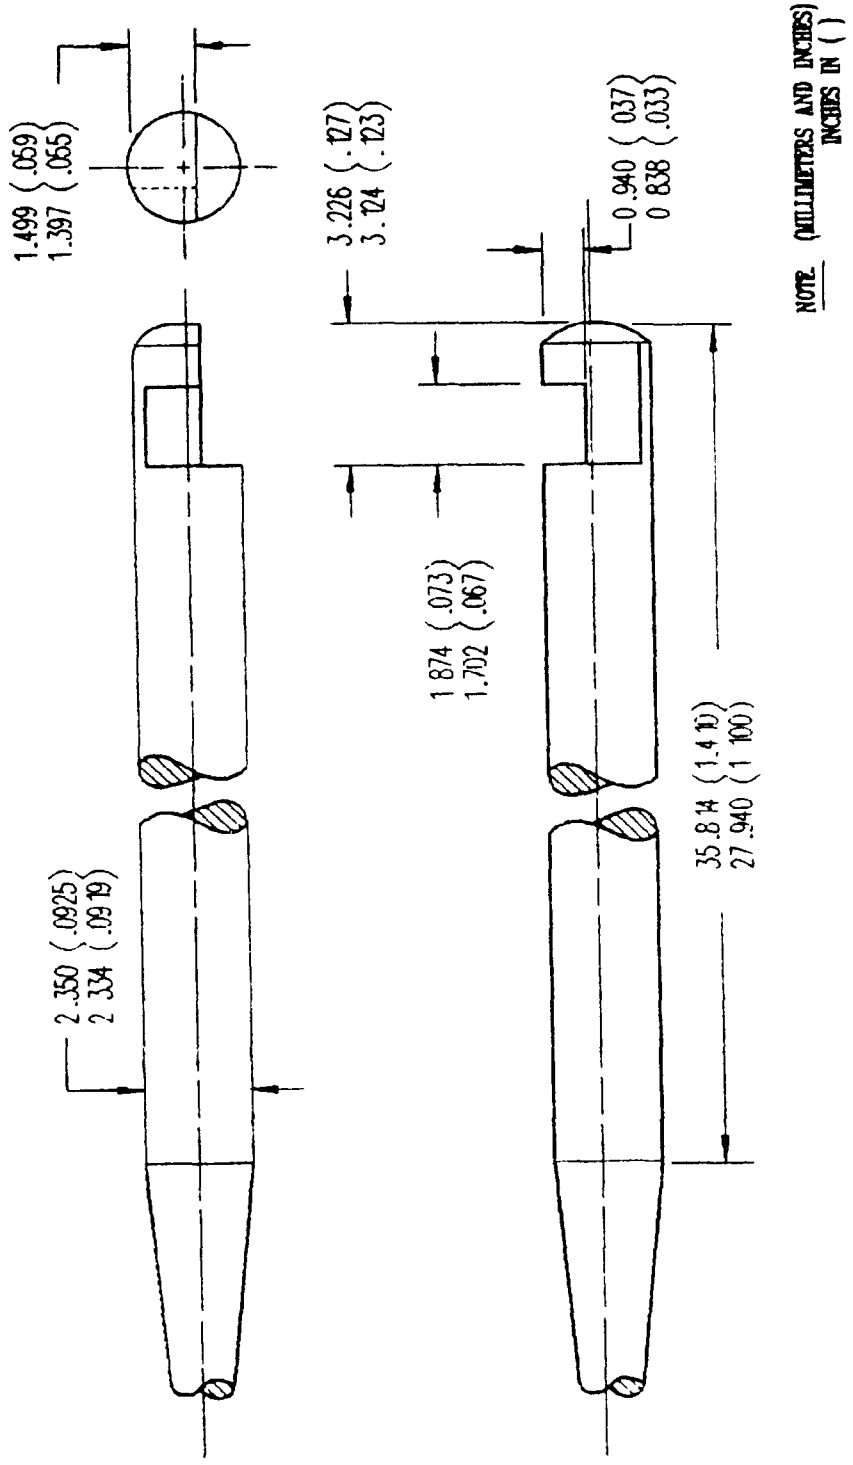


FIGURE 1. SHANK DIMENSIONS FOR CLASS 2A BURS.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:32Z
Check the source to verify that this is the current version before use.

INSTRUCTIONS: In a continuing effort to make our standardization documents better, the DoD provides this form for use in submitting comments and suggestions for improvements. All users of military standardization documents are invited to provide suggestions. This form may be detached, folded along the lines indicated, taped along the loose edge *(DO NOT STAPLE)*, and mailed. In block 5, be as specific as possible about particular problem areas such as wording which required interpretation, was too rigid, restrictive, loose, ambiguous, or was incompatible, and give proposed wording changes which would alleviate the problems. Enter in block 6 any remarks not related to a specific paragraph of the document. If block 7 is filled out, an acknowledgement will be mailed to you within 30 days to let you know that your comments were received and are being considered.

NOTE This form may not be used to request copies of documents, nor to request waivers, deviations, or clarification of specification requirements on current contracts. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document*(s)* or to amend contractual requirements.

(Fold along this line)

(Fold along this line)

DEFENSE LOGISTICS AGENCY

NO POSTAGE NECESSARY IF MAILED IN THE UNITED STATES

OFFICIAL BUSINESS
PENALTY FOR PRIVATE USE $300

BUSINESS REPLY MAIL
FIRST CLASS PERMIT NO 4966 WASHINGTON D C
POSTAGE WILL BE PAID BY THE DEFENSE LOGISTICS AGENCY

Commander
Defense Personnel Support Center
Attn: DPSC- RST
2800 South 20th Street
Philadelphia, PA 19101

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:32Z
Check the source to verify that this is the current version before use.

(TO DETACH THIS FORM, CUT ALONG THIS LINE.)

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

(See Instructions – Reverse Side)

1. DOCUMENT NUMBER	2. DOCUMENT TITLE
A-A-54292	BURS, DENTAL EXCAVATING (Tungsten Carbide)

3a. NAME OF SUBMITTING ORGANIZATION	4. TYPE OF ORGANIZATION *(Mark one)*
	☐ VENDOR
	☐ USER
b. ADDRESS *(Street, City, State, ZIP Code)*	☐ MANUFACTURER
	☐ OTHER *(Specify)* _____

5. PROBLEM AREAS

a. Paragraph Number and Wording

b. Recommended Wording

c. Reason/Rationale for Recommendation

6. REMARKS

7a. NAME OF SUBMITTER *(Last, First, MI)* – Optional	b. WORK TELEPHONE NUMBER *(Include Area Code)* – Optional
c. MAILING ADDRESS *(Street, City, State, ZIP Code)* – Optional	8. DATE OF SUBMISSION *(YYMMDD)*

DD FORM 82 MAR 1426 PREVIOUS EDITION IS OBSOLETE

Source: https://assist.dla.mil - Downloaded: 2026-10-26T09:32Z
Check the source to verify that this is the current version before use.