MILITARY SPECIFICATION

CLAMP, TEST TUBE

This specification was approved by the Departments of the Army, the Navy, and the Air Force for use of procurement services of the respective Departments.

1. SCOPE

1.1 This specification covers a test tube clamp, for use of Medical Services.

2. APPLICABLE SPECIFICATIONS, STANDARDS, DRAWINGS, AND PUBLICATIONS

2.1 The following specifications, standards, and drawing, of the issue in effect on date of invitation for bids, form a part of this specification:

SPECIFICATIONS

FEDERAL

NN-B-601 —Boxes, Wood-Cleated-Plywood, for Domestic Shipment.
NN-B-621 —Boxes, Wood, Nailed and Lock-Corner.
NN-B-631 —Boxes; Wood, Wire-bound (for Domestic Shipment).

MILITARY

JAN-P-105 —Packaging and Packing for Overseas Shipment—Boxes, Wood, Cleated, Plywood.
JAN-P-106 —Packaging and Packing for Overseas Shipment—Boxes; Wood, Nailed.
JAN-B-107 —Boxes, Wood, Wire-bound (Overseas Type).
JAN-P-120 —Packaging and Packing for Overseas Shipment—Cartons, Folding, Paperboard.
JAN-P-125 —Packaging and Packing for Overseas Shipment—Barrier-Materials, Waterproof, Flexible.
JAN-P-133 —Packaging and Packing for Overseas Shipment — Boxes, Set-Up, Paperboard.
JAN-P-140 —Packaging and Packing for Overseas Shipment — Adhesives, Water-Resistant, Case-Liner.

STANDARDS

MILITARY

MIL-STD-105 — Sampling Procedures and Tables for Inspection by Attributes.
MIL-STD-129 —Marking of Shipments.

DRAWINGS

ARMED SERVICES MEDICAL PROCUREMENT AGENCY

1306—Clamp, Test Tube.

(Reduced copy of drawing is attached as fig. 1.)

(Copies of specifications, standards, and drawings required by contractors in connection with specific procurement functions should be obtained from the procuring agency or as directed by the contracting officer.)

3. REQUIREMENTS

3.1 Material.—Material shall be of brass, approximately 0.090 inch in diameter, heavily nickel- or chrome-plated, and suitable in all respects for the purpose intended.

3.2 Style and design.—Style and design shall be in strict accordance with Drawing 1306. Test tube clamp shall be Stoddard type, and shall be constructed of one piece brass wire looped to form a hinge, two finger grips

952187-52-(500)

Source: https://assist.dla.mil -- Downloaded: 202610-16T20:38Z
Check the source to verify that this is the current version before use.

and jaws. Jaws shall be approximately 1¼ by ¾ inches in size and shall open to an extent that they will grip tubes up to 1½ inches in diameter. Overall length of clamp shall be approximately 5 inches.

3.3 Workmanship. — Workmanship shall be first class throughout. Clamps shall be free from defects which detract from their appearance or may impair their serviceability.

4. SAMPLING, INSPECTION, AND TEST PROCEDURES

4.1 Sampling.—Unless otherwise specified by the procuring activity, samples shall be submitted in accordance with instructions furnished (see 6.1). In addition, inspection at contractor's facility by inspector shall be conducted in accordance with Standard MIL-STD-105.

4.2 Inspection. — Samples shall be inspected for material, style and design, dimensions, and workmanship. (See 6.1).

4.3 Tests.—Tests shall be conducted, as necessary, to determine compliance with this specification.

5. PREPARATION FOR DELIVERY

5.1 Packaging.

5.1.1 *Unit packaging.* — One clamp, as specified, constitutes one unit. Unit packaging is not required.

5.1.2 *Intermediate packaging.* — Twelve units shall be packaged in a carton of appropriate size constructed in accordance with Specification JAN-P-120 or JAN-[illegible]. Each carton shall be adequately secured to prevent accidental opening.

5.2 Packing.

5.2.1 *For domestic shipment.* — Forty-eight intermediate cartons (576 units) shall be overpacked in an exterior container constructed in accordance with Specification NN-B-601, NN-B-621, or NN-B-631.

5.2.2 *For overseas shipment.* — Forty-eight intermediate cartons (576 units) shall be overpacked in an exterior container designed for type 2 load, and constructed in accordance with Specification JAN-P-105, JAN-P-106, or JAN-B-107. Closure and strapping shall comply with appendix of applicable specification. Each box shall be lined with a waterproof barrier (bag) conforming to Specification JAN-P-125. Closures shall be completely sealed by a continuous seam of water-resistant adhesive at least ¾ inch wide and conforming to Specification JAN-P-140.

5.2.3 *Packing variation permitted.* — If the number of units in any shipment is not the exact multiple of the number of units specified to be contained in each shipping container, the units not constituting the nearest such multiple shall be packed in an exterior container of suitable size and design and so constructed as to insure safe delivery to specified destination.

5.3 Marking.

5.3.1 *Interior packages.*—Each intermediate carton shall be marked with stock number, nomenclature, unit, quantity, and name of contractor.

5.3.2 *Shipping container.*—Shipping container shall be marked in accordance with Standard MIL-STD-129.

6. NOTES

6.1 Ordering data. — Procurement documents should specify the following:

(a) Title, number, and date of this specification.
(b) Sampling required (see 4.1).
(c) Inspection required (see 4.2).
(d) Whether packing for domestic or overseas shipment is required (see 5.2).

Source: https://assist.dla.mil -- Downloaded: 202640-16T20:38Z
Check the source to verify that this is the current version before use.

6.2 This specification covers the following item appearing in the Armed Services Catalog of Medical Materiel:

4-181-000—Clamp, Test Tube.


6.3 This specification does not include all types, classes, grades, sizes, etc., of the commodity indicated by the title of the specification, or which are commercially available, but is intended to cover the types, etc., which are normally procured to meet Military requirements.


Notice.—When Government drawings, specifications, or other data are used for any purpose other than in connection with a definitely related Government procurement operation, the United States Government thereby incurs no responsibility nor any obligation whatsoever; and the fact that the Government may have formulated, furnished, or in any way supplied the said drawings, specifications, or other data is not to be regarded by implication or otherwise as in any manner licensing the holder or any other person or corporation, or conveying any rights or permission to manufacture, use, or sell any patented invention that may in any way be related thereto.


Custodian:
Army—Medical Service

Other interest:
Army—TC
Navy—Md
Air Force.

Source: https://assist.dla.mil -- Downloaded: 2026-10-16T20:38Z
Check the source to verify that this is the current version before use.

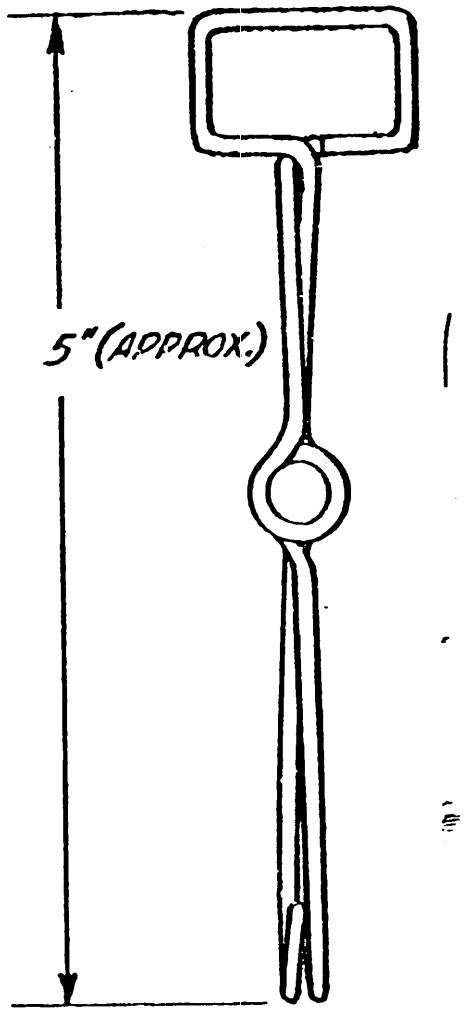

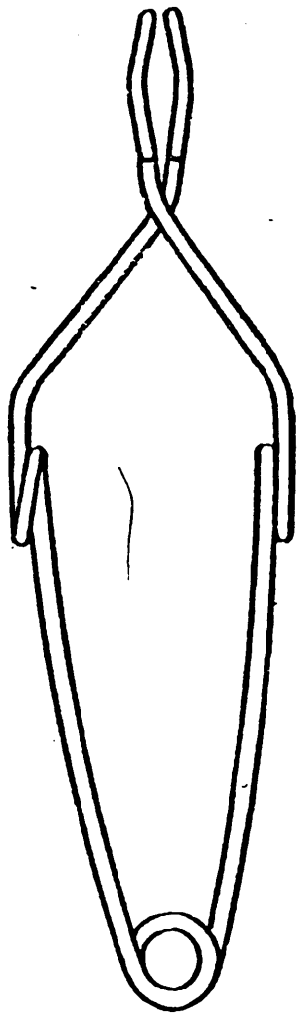

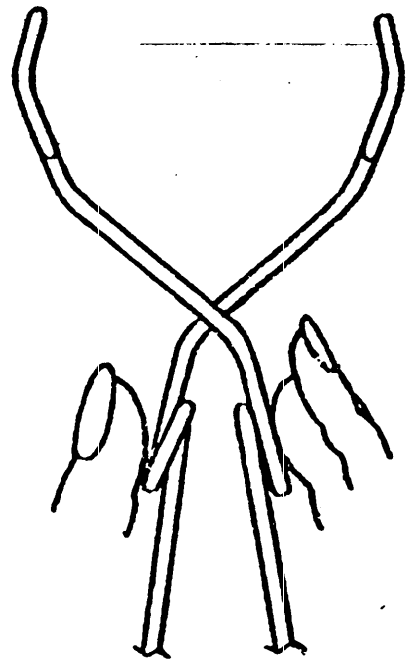

ALTERNATE POSITION OF CLAMP WHEN OPEN

MATERIAL:
NICKEL PLATED BRASS.

Source: https://assist.dla.mil -- Downloaded: 2026-01-16T20:38Z
Check the source to verify that this is the current version before use.