A-A-53224
29 September 1987

# COMMERCIAL ITEM DESCRIPTION

## SPATULA, DENTAL AND CARVER, DENTAL (Wax)

The General Services Administration has authorized the use of this commercial item description in preference to Federal Specification GG-S-598C.

This commercial item description covers double-ended spatulas and a carver suitable for dental use.

Salient characteristics:

Shall be of the following types and styles, as specified:

Type I - Spatulas
Style 1 - Beale, No. 7
Style 2 - Gritman, No. 31
Type II - Carver, Roach

The spatulas and the carvers shall be in accordance with the applicable requirements of GG-I-526, with the exceptions and with the additional requirements specified herein.

The spatulas and carvers shall be double-ended instruments of one-piece construction. The instruments shall conform to the type and style, as specified. The periphery of the blades of all operative ends shall be blended or tapered to form a carving edge, except for the spoon end of the carver. The instruments shall be suitable for use with or without heat for carving and spreading various waxes in the preparation of dental prosthetic appliances. The style and dimensions shall conform to figures 1, 2, or 3, as applicable.

Material. Spatulas and carvers shall conform to the requirements of class 4, type 420 or type 440A stainless steel.

Finish. Smooth spatula handles shall have a satin, or mirror, or bright polished finish. Those instrument handles with fillet type or notch type serrations shall have a bright finish. The operative ends and the shanks of both spatulas and the carver shall have a mirror or a bright polished finish, except for the carver, the spoon concavity may have fine hone markings.

AMSC N/A FSC 6520

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:17Z
Check the source to verify that this is the current version before use.

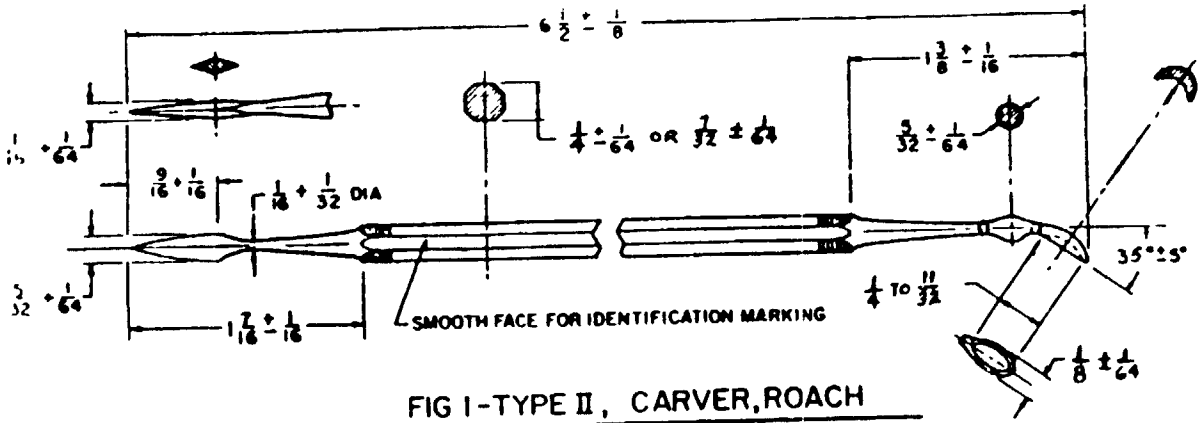



FIG 1-TYPE II, CARVER, ROACH

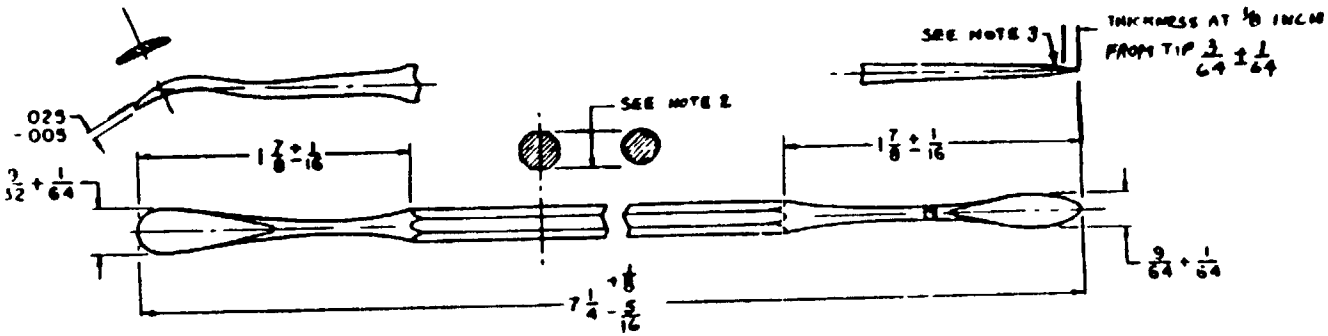



FIG 2-TYPE I, STYLE 1, SPATULA, NO 7

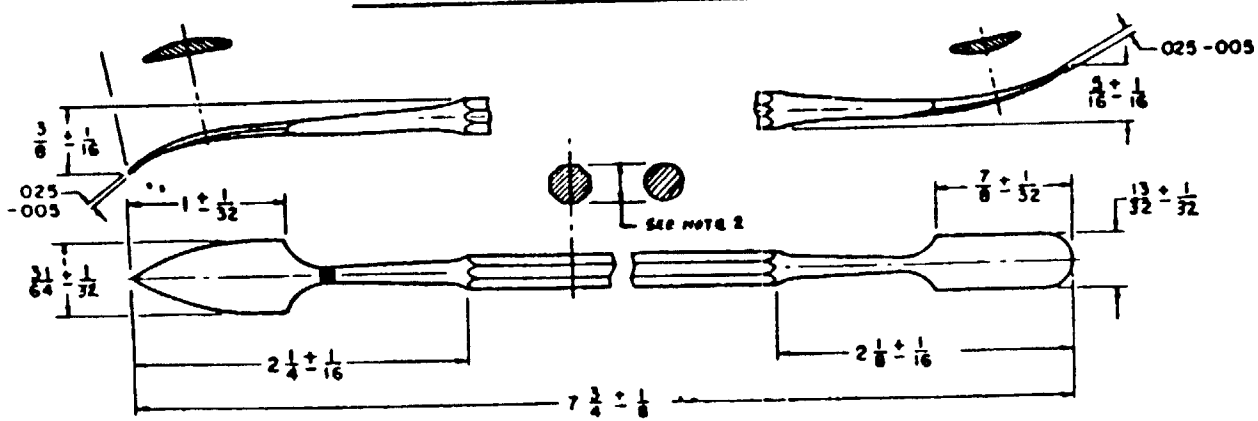



FIG 3-TYPE I, STYLE 2, SPATULA, NO 31

NOTES:

1. DIMENSIONS ARE IN INCHES
2. ACCEPTABLE HANDLE SIZES 3/16 ± 1/64, 7/32 ± 1/64 OR 1/4 ± 1/64
3. AS AN ALTERNATE, TOP FACE OF BLADE MAY BE FLAT.



Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:17Z
Check the source to verify that this is the current version before use.

Tests.

Hardness. After proper stress relieving, the Rockwell hardness of the operative ends shall be C40 to C50 for instruments fabricated from type 420 steel, and C52 to C56 for instruments fabricated from type 440A steel. Handle and shank shall be properly tempered and shall have a hardness suitable for the purpose intended. Hardness shall be tested in accordance with ASTM E18 (Rockwell) or E92 (Diamond pyramid).

Identification marking. In addition to the marking requirements of GG-I-526, each spatula shall be marked with the instrument number, and each carver shall be marked with the letters "RWC". All marking shall be legible and permanent. The word "Stainless" shall also be marked on instruments of foreign manufacture. As an alternate to the word "Stainless", the use of a registered trademark identifying the steel as stainless shall be acceptable, provided prior approval is received from the cognizant contracting officer.

Workmanship. The instruments shall be free from defects which detract from their appearance or impair their serviceability, proper functioning, and intended use. The operative ends shall be free of discolorations and course grind marks.

Unit. Each (EA). One spatula or one carver, as specified, constitutes one unit.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.



Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:17Z
Check the source to verify that this is the current version before use.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Sampling for inspection. Sampling for inspection shall be conducted in accordance with MIL-STD-105. Where feasible, the same sample shall be used for the determination of two or more inspection characteristics. The unit of product for inspection purposes shall be one instrument. Unless otherwise specified, sampling for examination shall be conducted at inspection level II, AQL 2.5, and sampling for tests (when applicable) shall be conducted at inspection level S-1, AQL 1.0.

Contractor certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Metric products. Products manufactured to metric dimensions will be considered on an equal basis with those manufactured using inch/pound units, providing they fall within the tolerance specified using conversion tables contained in the latest revision of Federal Standard No. 376, and all other requirements of this document are met. If a product is manufactured to metric dimensions and those dimensions exceed the tolerance specified in the inch/pound units, a request should be made to the contracting officer to determine if the product is acceptable. The contracting officer has the option of accepting or rejecting the product.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.



Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:17Z
Check the source to verify that this is the current version before use.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Public Law 94-580, as amended, and as implemented by Federal Acquisition Regulation Subpart 23.4 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

NOTE: The following National Stock Numbers are covered by this document.

| Stock Number | Item Identification |
|---|---|
| 6520-00-511-5550 | CARVER, DENTAL, Double-Ended, Wax, Roach. |
| 6520-00-557-1000 | SPATULA, DENTAL, Double-Ended, Beale, No. 7. |
| 6520-00-557-2000 | SPATULA, DENTAL, Double-Ended, Gritman, No. 31. |

Ordering data. Intermediate/exterior package quantities, labeling, and marking must be as specified in the contract and/or order.

MILITARY INTERESTS:

Custodians:
Army - MD
Navy - MS
Air Force - 03

Civil Agency Coordinating Activities:
VA-OSS
PHS
FDA-MPQAS

PREPARING ACTIVITY:

DoD - MB

Agent:

DLA - DM

Project No. 6520-1870

Location: NCR Disk 2

47874
05045



Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:17Z
Check the source to verify that this is the current version before use.

**INSTRUCTIONS** In a continuing effort to make our standardization documents better, the DoD provides this form for use in submitting comments and suggestions for improvements. All users of military standardization documents are invited to provide suggestions. This form may be detached, folded along the lines indicated, taped along the loose edge *(DO NOT STAPLE)*, and mailed. In block 5, be as specific as possible about particular problem areas such as wording which required interpretation, was too rigid, restrictive, loose, ambiguous or was incompatible, and give proposed wording changes which would alleviate the problems. Enter in block 6 any remarks not related to a specific paragraph of the document. If block 7 is filled out, an acknowledgement will be mailed to you within 30 days to let you know that your comments were received and are being considered.

*NOTE* This form may not be used to request copies of documents, nor to request waivers, deviations, or clarification of specification requirements on current contracts. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements.

*(Fold along this line)*

*(Fold along this line)*

DEFENSE LOGISTICS AGENCY

NO POSTAGE NECESSARY IF MAILED IN THE UNITED STATES

OFFICIAL BUSINESS
PENALTY FOR PRIVATE USE $300

**BUSINESS REPLY MAIL**
FIRST CLASS PERMIT NO 4956 WASHINGTON D C

POSTAGE WILL BE PAID BY THE DEFENSE LOGISTICS AGENCY

Commander
Defense Personnel Support Center
ATTN DPSC-ATTS
2800 South 20th Street
Philadelphia, Pennsylvania 19101-8419

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:17Z
Check the source to verify that this is the current version before use.

(TO DETACH THIS FORM, CUT ALONG THIS LINE.)

# STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

*(See Instructions – Reverse Side)*

| 1 DOCUMENT NUMBER | 2 DOCUMENT TITLE |
|---|---|
| A-A-53224 | SPATULA, DENTAL AND CARVER, DENTAL (WAX) |

| 3a. NAME OF SUBMITTING ORGANIZATION | 4 TYPE OF ORGANIZATION *(Mark one)* |
|---|---|
| | ☐ VENDOR |
| | ☐ USER |
| b. ADDRESS *(Street, City, State, ZIP Code)* | ☐ MANUFACTURER |
| | ☐ OTHER *(Specify)* |

5 PROBLEM AREAS

a. Paragraph Number and Wording

b. Recommended Wording

c. Reason/Rationale for Recommendation

6 REMARKS

| 7a. NAME OF SUBMITTER *(Last, First, MI)* – Optional | b. WORK TELEPHONE NUMBER *(Include Area Code)* – Optional |
|---|---|
| c. MAILING ADDRESS *(Street, City, State, ZIP Code)* – Optional | 8. DATE OF SUBMISSION *(YYMMDD)* |

DD FORM 82 MAR 1426 PREVIOUS EDITION IS OBSOLETE

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:17Z
Check the source to verify that this is the current version before use.