A-A-53247A
28 July 1988
SUPERSEDING
A-A-0053247(DM)
7 October 1987

COMMERCIAL ITEM DESCRIPTION

OBTURATOR, CARDIOVASCULAR TOURNIQUET (Rumel)

The General Services Administration has authorized the use of this commercial item description.

This commercial item description covers a cardiovascular tourniquet obturator suitable for use with the Rumel tourniquet.

Salient characteristics:

Style and design. Style and design of the obturator shall be in accordance with Figure 1. The style and design specified herein shall be classified as the "Rumel" design.

Materials. The obturator shall be fabricated from Type 420A corrosion-resisting steel conforming to ASTM Designation F899. As an alternate, the obturator may be fabricated from Type 4021 German stainless (corrosion-resistant) steel. This material shall comply with ASTM Designation F899, except the heat (cast) analysis results shall conform to Table I.

TABLE I

COMPOSITION OF TYPE 4021 STEEL

Elements	Compositions, %
Carbon	0.17% to 0.22%
Silicon	1.00%, Maximum
Manganese	1.00%. Maximum
Phosphorous	0.045%, Maximum
Sulfur	0.030%, Maximum
Chromium	12.00% to 14.00%
Iron	Balance

AMSC N/A FSC 6515

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:17Z
Check the source to verify that this is the current version before use.

Hardness. The obturator shall have a Rockwell Hardness C scale (HRC) of 48 to 53. As an alternate, obturators made of Type 4021 steel shall have a Rockwell Hardness C scale (HRC) of 47 to 53. The hardness shall be tested in accordance with ASTM Designation E18 or ASTM Designations E92 and E140.

Corrosion-resistance. The obturator shall pass the copper-sulphate and boil tests specified in ASTM Designation F1089.

Finish. The obturator shall have a bright overall finish. The obturator shall be passivated. Passivation shall render the obturator corrosion-resistant.

Workmanship. The obturator shall be free from feathered edges, cracks, burrs, pits, and other defects that detract from its appearance or impair its serviceability.

Unit. Each (EA). One obturator, as specified, constitutes one unit.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:17Z
Check the source to verify that this is the current version before use.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more test characteristics.

Sampling for inspection. Sampling for inspection shall be conducted in accordance with MIL-STD-105 at Level S-2, AQL 1.0%. The unit of product for inspection purposes shall be one obturator.

Contractor certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Metric products. Products manufactured to metric dimensions will be considered on an equal basis with those manufactured using inch-pound units, providing they fall within the tolerances specified using conversion tables contained in the latest revision of Federal Standard No. 376, and all other requirements of this document are met.

If a product is manufactured to metric dimensions and those dimensions exceed the tolerances specified in the inch/pound units, a request should be made to the contracting officer to determine if the product is acceptable.

The contracting officer has the option of accepting or rejecting the product.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Source: https://assist.dla.mil -- Downloaded: 202610-26T09:17Z
Check the source to verify that this is the current version before use.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Public Law 94-580 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.
NOTE: The following National Stock Number is covered by this document:

NSN	ITEM IDENTIFICATION
6515-01-139-8692	OBTURATOR, CARDIOVASCULAR TOURNIQUET, 12 Inches (30.48 cm)

Ordering data. (Intermediate/exterior package quantities and labeling and marking must be specified in the contract and/or order).

MILITARY INTERESTS:

Custodians:

Army - MD
Navy - MS
Air Force - 03

Preparing Activity:

DoD-MB

Agent:

DLA-DM


CIVIL COORDINATING ACTIVITIES:


VA-OSS
PHS
FDA-MPQAS


PGC S0082

Project No. 6515-3540

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:17Z
Check the source to verify that this is the current version before use.

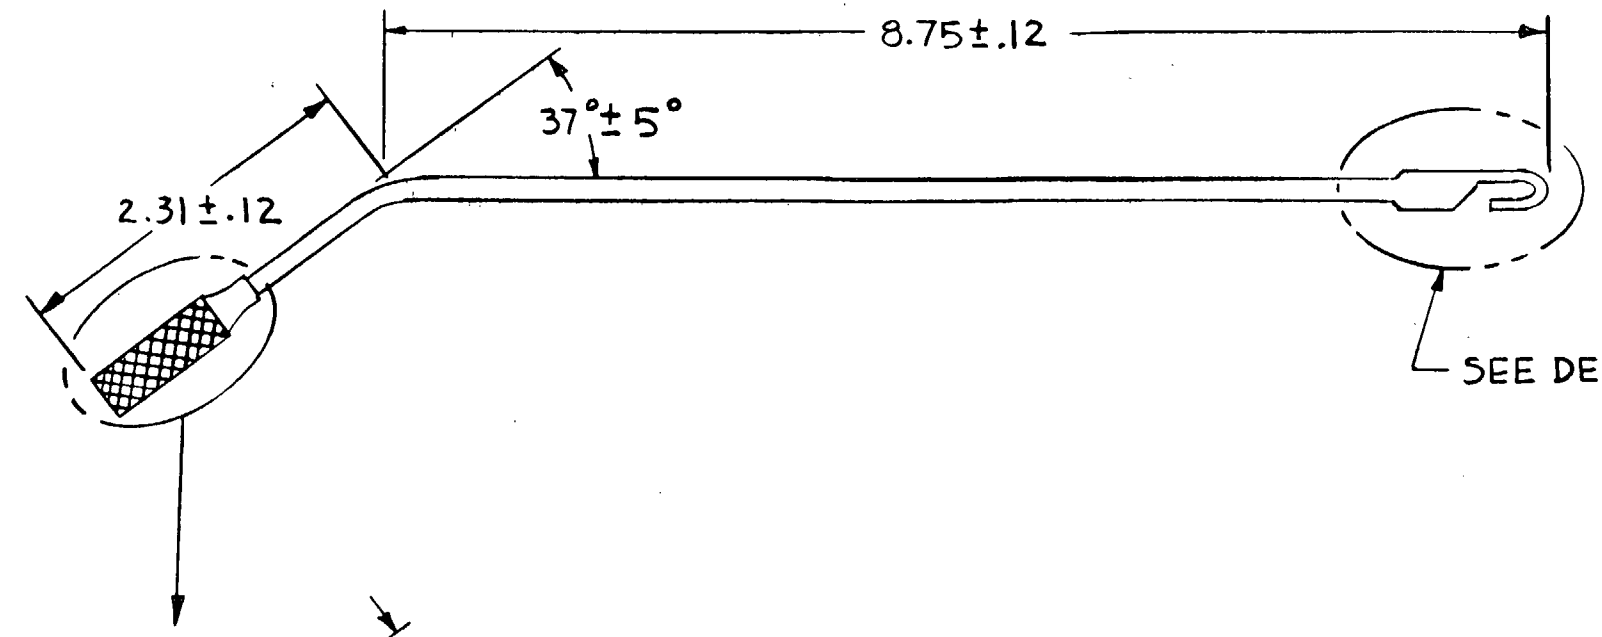

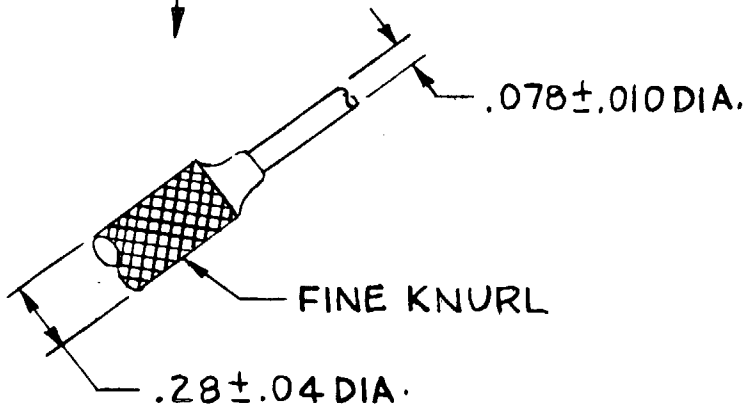

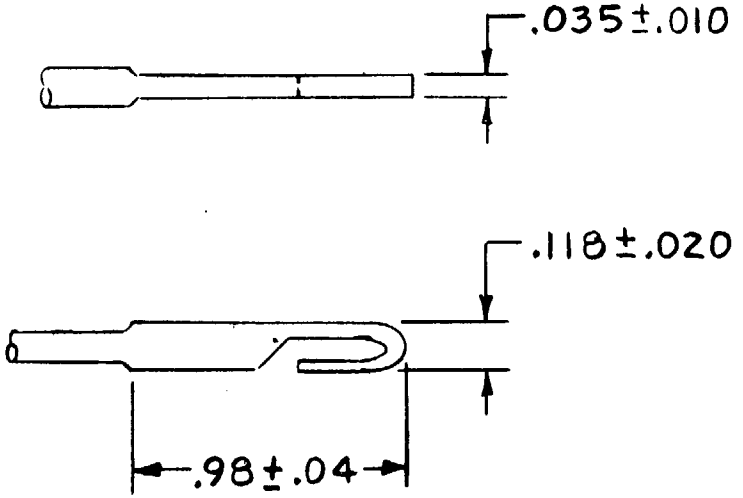

DETAIL-A

NOTE: DIMENSIONS IN INCHES

FIGURE 1 OBTURATOR, CARDIOVASCULAR TOURNIQUET (RUMEL)

☆U.S. GOVERNMENT PRINTING OFFICE: 1989 - 604-033/10105

Source: https://assist.dla.mil -- Downloaded: 2026-02-26T09:17Z
Check the source to verify that this is the current version before use.