MIL-L-37184B
25 March 1977
SUPERSEDING
MIL-L-37184A
26 June 1975 and
MIL-L-37184
23 January 1975

MILITARY SPECIFICATION

LENS BLANK, OPHTHALMIC, BIFOCAL, ONE PIECE

This specification is approved for use by all Departments and Agencies of the Department of Defense.

1. SCOPE

1.1 Scope. This specification covers semi-finished, ophthalmic one piece bifocal lens blanks of two types (see 6.1).

1.2 Classification. Lens blanks shall be of two types, as specified.

Type I - Glass lens blank.
Type II - Plastic lens blank.

2. APPLICABLE DOCUMENTS

2.1 Issues of documents. The following documents of the issue in effect on date of invitation for bids or request for proposals form a part of this specification to the extent specified herein:

SPECIFICATIONS

FEDERAL

PPP-B-585 - Boxes, Wood, Wirebound.
PPP-B-601 - Boxes, Wood, Cleated-Plywood.
PPP-B-621 - Boxes, Wood, Nailed and Lock-Corner.
PPP-B-636 - Boxes, Set-Up, Paperboard.

Beneficial comments (recommendations, additions, deletions) and any pertinent data which may be of use in improving this document should be addressed to: Hq, Defense Personnel Support Center, ATTN: Directorate of Medical Materiel, DPSC-ATT, 2800 South 20th Street, Philadelphia, PA 19101, by using the self-addressed Standardization Document Improvement Proposal (DD Form 1426) appearing at the end of this document or by letter.

FSC 6540

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:08Z
Check the source to verify that this is the current version before use.

MILITARY

MIL-L-10547 - Liners, Case, and Sheet, Overwrap; Water-Vaporproof or Waterproof, Flexible.

STANDARDS

MILITARY

MIL-STD-105 - Sampling Procedures and Tables for Inspection by Attributes.
MIL-STD-129 - Marking for Shipment and Storage.

(Copies of specifications, standards, and publications required by suppliers in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.)

2.2 Other publications. The following documents form a part of this specification to the extent specified herein. Unless otherwise indicated the issue in effect on date of invitation for bids or request for proposals shall apply.

AMERICAN NATIONAL STANDARDS INSTITUTE, INCORPORATED

ANSI Z80.1 - 1972 - American National Standard Requirements for First-Quality Prescription Ophthalmic Lenses.

(Application for copies should be addressed to the American National Standards Institute, Incorporated, 1430 Broadway, New York, NY 10018.)

AMERICAN SOCIETY FOR TESTING AND MATERIALS (ASTM) STANDARDS

D 542 - Index of Refraction of Transparent Organic Plastics.
D 785 - Rockwell Hardness of Plastics and Electrical Insulating Materials.
D 792 - Specific Gravity and Density of Plastics by Displacement.
D 1003 - Haze and Luminous Transmittance of Transparent Plastics.

(Application for copies should be addressed to the American Society for Testing and Materials, 1916 Race Street, Philadelphia, PA 19103.)

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:08Z
Check the source to verify that this is the current version before use.

U. S. DEPARTMENT OF HEALTH, EDUCATION, AND WELFARE,
FOOD AND DRUG ADMINISTRATION

Federal Food, Drug and Cosmetic Act and Regulation Promulgated Thereunder.

(Application for copies should be addressed to the Food and Drug Administration, Washington, DC 20204.)

(Technical society and technical association specifications and standards are generally available for reference from libraries. They are also distributed among technical groups and using Federal agencies.)

3. REQUIREMENTS

3.1 Material.

3.1.1 Type I. The type I lens blank shall be fabricated of high quality white ophthalmic crown glass, with an index of refraction of 1.5230 plus or minus 0.0015. The glass shall have a high degree of clearness and transparency, and shall remain clear and not discolor when exposed to ordinary sunlight.

3.1.2 Type II. The type II lens blank shall be fabricated of cast thermosetting plastic resin polymerized from allyl diglycol carbonate monomer and a catalyst with necessary additives to produce satisfactory ophthalmic lenses. The resin shall contain not less than 80 percent allyl diglycol carbonate monomer. The lens material shall conform to the physical requirements listed in table I when tested as specified in section 4. The lens material shall have a high degree of clarity and transparency. The lens blank shall remain clear and free of discoloration, as specified, when stored away from direct sunlight. Discoloration shall be determined by loss in light transmission.

TABLE I. Physical requirements.

Characteristic	Requirement
Index of refraction, 20°C, N_D	1.498 ± 0.002
Specific gravity, 25°C	1.32 ± 0.02
Barcol hardness, minimum	26 (15 seconds)
Rockwell hardness	M95 to M100 1/
Light transmission, 1/4 inch, percent, minimum	89

1/ NOTE: The Rockwell hardness shall be used as an alternate test when the Barcol hardness is not performed. Modified Rockwell hardness apparatus correlated with Barcol hardness is acceptable.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:08Z
Check the source to verify that this is the current version before use.

3.1.3 Types I and II. Both types of bifocals shall be durable and of suitable composition and hardness to give good service in use, resist the action of weather and not be easily scratched or damaged under ordinary conditions. The lens blanks shall be free of bubbles, inclusions, striae and cloudiness (see 3.5), when inspected as described in section 4.

3.2 Construction. The semifinished lens blank shall be fabricated of one of the materials specified in 3.1, according to type. The lens blank shall be a one-piece, full segment, raised ledge type bifocal. The reading segment shall extend straight across the lens. The blank shall be constructed by either grinding and polishing two curvatures on one blank, or in the case of plastic, molding two surface curvatures on the one piece blank. The front surface and body of the lens blank shall be free from any localized refractive error due to any defect which impairs the image quality when the questioned area is examined either visually or with a standard lens measuring instrument. The base curve shall be in the corrective curve form. The segment side of the blank shall be ground and polished or molded to the spherical base curve specified within a tolerance of plus or minus 0.09 diopters. (see 4.4.2).

3.2.1 Type I. The type I lens blank shall have the segment ledge located from 3 to 5 millimeters (mm) below the geometrical center of the blank. (See figure 1.) Size and shape shall be as specified in 3.3.

3.2.2 Type II. The type II lens blank shall have the segment ledge located 3 mm ± 0.5 mm below the geometric center of the blank. (See figure 2). Size and shape shall be as specified in 3.3.

3.2.3 Thickness. Each blank shall be sufficiently thick to produce the lens for which it is designated on the manufacturer's grinding chart.

3.2.4 Base curves. The front surface curve (base curve) supplied shall be such that when used in accordance with the corrected curve surfacing chart published by the manufacturer of the lens blank, the finished lens shall be in the corrected curve form (see 6.3.1) and to specified axial back vertex power within a tolerance of plus or minus 0.06 diopter. The lens blank shall be such that the finished prescription desired can be completed with tools of even multiples of 0.25 diopters only (to provide finished lens powers in 0.25 diopter increments).

3.2.5 Segment addition power. The power of the additions shall be within a tolerance of plus or minus 0.09 diopters, as specified in ANSI Standard Z80.1 - 1972.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:08Z
Check the source to verify that this is the current version before use.

3.3 Size. The type I lens blank shall be rectangular with rounded corners (see figure 1). The blank shall be a minimum of 60 mm wide and a minimum of 55 mm high through the shortest meridian. The type II blank shall be rectangular or square, with rounded corners or round (see figure 2). The blank shall be a minimum of 62 mm in the shortest and a maximum of 69 mm in the longest meridian.

3.4 Impact resistance. Both types of the bifocal raised ledge lenses in the finished stage must be capable of passing the impact resistance test required by the Department of Health, Education and Welfare, Food and Drug Administration. (See 4.1.1).

3.5 Workmanship. Workmanship shall be first class. The lens blank shall be colorless, smooth and free from blemishes (internal and external), striae, bubbles, chips, waves and other surface and internal defects which detract from their appearance or impair their serviceability.


4. QUALITY ASSURANCE PROVISIONS

4.1 Responsibility for inspection. Unless otherwise specified in the contract, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract, the contractor may use his own or any other facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspection set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

4.1.1 Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government, upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of 3 years after delivery of the supplies to which such records relate.

4.1.2 Inspection. Inspection, as used in this specification, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:08Z
Check the source to verify that this is the current version before use.

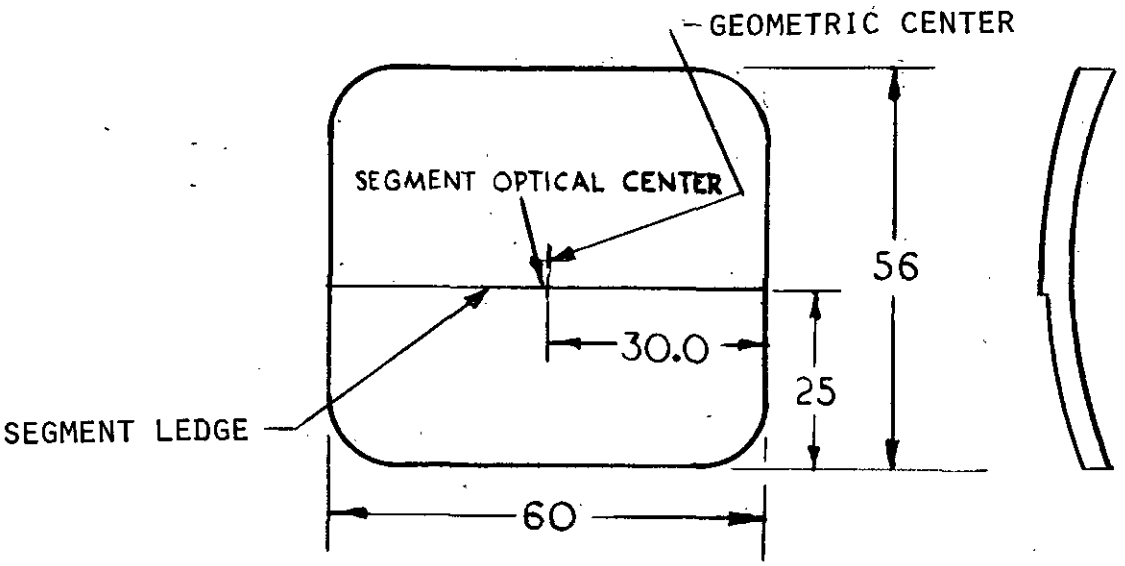


TYPE I LENS BLANK

NOTE: ALL DIMENSIONS ARE IN MM.

FIGURE 1. Type I bifocal.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:08Z
Check the source to verify that this is the current version before use.

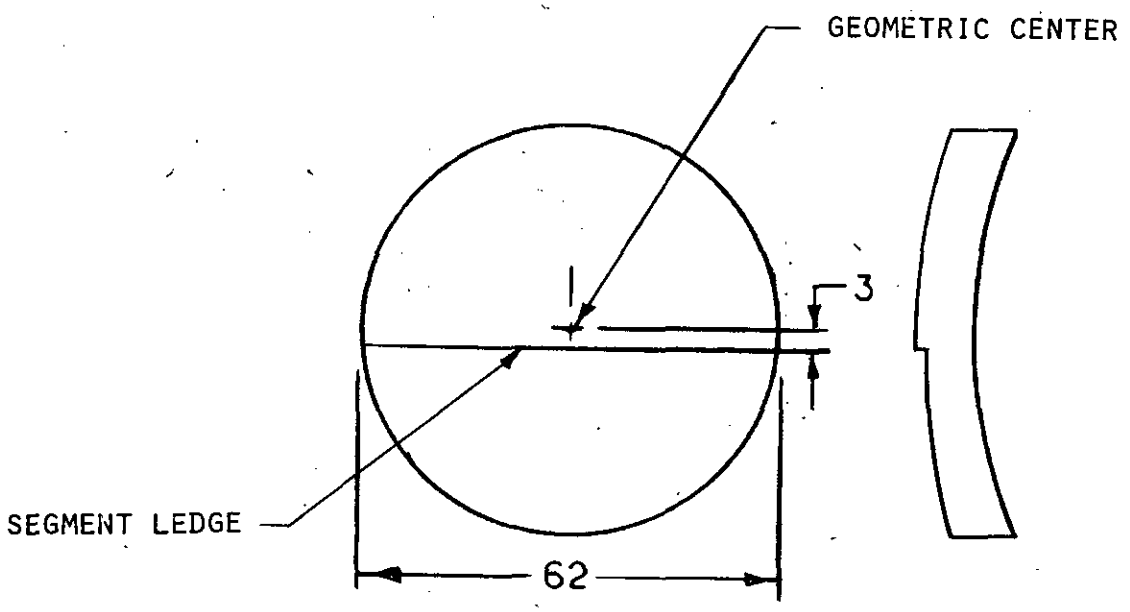

TYPE II LENS BLANK

NOTE: ALL DIMENSIONS ARE IN MM.

FIGURE 2. Type II bifocal.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:08Z
Check the source to verify that this is the current version before use.

4.1.3 Certificates of quality. Certificates of quality supplied by the manufacturer of the glass or plastic may be furnished in lieu of actual performance of such testing by the contractor, provided lot identity has been maintained and can be demonstrated to the Government. The certificate shall include the name of the contractor, the contract number, the name of the manufacturer or supplier, the National Stock Number (NSN), the name of the component/material, the lot number, the lot size, the sample size, the date of testing, the test method, individual test results, and the specification requirements.

4.2 Sampling.

4.2.1 For examination. Sampling for examination shall be conducted in accordance with MIL-STD-105, and as indicated in table II. Unit of product for examination shall be one lens.

TABLE II. Sampling criteria for examination.

Type of defect	Inspection level	AQL (percent defective)
Major	II	0.65
Minor	II	0.65
Dimensional	S-3	1.5

4.2.2 For tests. Sampling for tests shall be in accordance with MIL-STD-105 and as indicated in table III. Unit of product for test purpose shall be one lens. Where feasible, the same sample shall be used for the determination of two or more test characteristics.

TABLE III. Sampling criteria for tests.

For test	Inspection level	AQL (percent defective)
Refractive index and specific gravity (type II)	S-2	1.0
Hardness (type II)	S-1	1.0
Light transmission (type II), refractive power, addition power and surface power	S-3	1.0

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:08Z
Check the source to verify that this is the current version before use.

4.3 Examination. The lens shall be examined for compliance with specification requirements. The examination shall be conducted in accordance with but not restricted to the defects of table IV. Additional defects shall be classified in accordance with MIL-STD-105.

TABLE IV. Classification of defects.

Category	Defect
Major	
101	Defects (Pits, grayness, scratches, bubbles, striae or inclusions - located over 3 mm from any edge).
102	Wave distortion.
Minor	
201	Cloudiness or haze.
202	Jagged or sharp edges.

4.3.1 Dimensional examination. Any dimension not within the specified tolerance shall be classified as a defect.

4.3.2 Physical quality and appearance. Lens blanks shall be inspected against a dark background, in light from an open-shaded, 40 watt incandescant daylight lamp, with the lens 12 inches from the light source. No pits, scratches, grayness, watermarks, bubbles, striae, wave distortion, or inclusions 3 mm from any edge shall be acceptable. Waves found by visual inspection shall be passable if no deterioration in image quality is found when the localized area is examined with a standard lens measuring instrument. Surface defect examination shall be restricted to front surface. Discount the unfinished back surface defects that can be processed out.

4.3.3 Packaging inspection. The inspection of the unit, intermediate package, packing and marking for shipment and storage shall be in accordance with quality assurance provisions of the applicable container specification and the marking requirements of MIL-STD-129.

4.4 Tests. Tests shall be conducted to determine compliance with specification requirements.

4.4.1 Test methods. Test methods shall be as specified in table V.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:08Z
Check the source to verify that this is the current version before use.

TABLE V. Methods.

Characteristics	Requirement paragraph	Test Method
Index of refraction	3.1.1 & 3.1.2	ASTM D 542
Specific gravity	3.1.2	ASTM D 792
Barcol hardness	3.1.2	par. 4.4.1.1
Rockwell hardness	3.1.2	ASTM D 785
Light transmission	3.1.2	ASTM D 1003
Refractive powers	3.2	par. 4.4.1.2
Defects	3.5	par. 4.3.1

4.4.1.1 Barcol hardness. The Barcol hardness shall be conducted as follows:

4.4.1.1.1 Apparatus. The apparatus shall consist of the following:

(a) A Barcol Impressor manufactured by the Barber-Colman Company, Rockford, Illinois.

(b) A pressure applicating device, similar to the one shown in the diagram furnished with the instrument. This is comprised essentially of the following:

(1) Two 1/2" x 2" springs, the upper one applying the pressure to the test specimen and the lower one acting as a shock absorber. These should be so adjusted by the locking nuts that the upper spring is exerting a downward force of approximately 35 pounds (lbs.) and the lower spring an upward force of approximately 15 lbs., giving a resultant force of 20 lbs. acting downward on the test specimen.

(2) A vertical rod working freely through two sleeves. The Barcol Impressor is rigidly attached to the bottom of this rod. The rod is raised by means of the lever and is forced downward by the 20 lb. spring action.

(3) An adjustable table attached to the base of the apparatus. The plastic test specimen is placed on this table and is moved (either upward or downward) by means of the screw adjustment until the 20 lb. downward force of the Barcol needle is applied to the plastic sample. When initially setting up the apparatus, it is advisable to move the plastic test specimen to the proper position and to scribe a reference line on the moveable vertical rod at a point even with the top surface of the upper sleeve. The rod should then be raised and a second scribe line made on the rod at a point 3/32 in. below the first line. In testing specimens of varying thickness it is then only necessary to adjust the table until the upper scribe line is even with the top surface of the upper sleeve. In applying the load for the actual Barcol reading, the rod is raised until the lower scribe line is even with the upper surface of the sleeve. The rod is then quickly released.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:08Z
Check the source to verify that this is the current version before use.

4.4.1.1.2 Test specimens. Test specimens shall be lenses or flat pieces molded from lens batch. Lens should be measured on plano or nearly flat area, thickness shall be 3.0 mm or more. Flat piece shall be approximately 1 inch by 3 inches by 1/8 inch minimum thickness.

4.4.1.1.3 Conditioning. Specimens shall be conditioned for at least 24 hours at $23^{\circ} \pm 1.1^{\circ}$C. ($73.4^{\circ} \pm 2^{\circ}$ F) and 50 $\pm$ 2 percent relative humidity prior to testing.

4.4.1.1.4 Procedure.

(a) The actual testing shall be carried out in an atmosphere maintained at $23^{\circ} \pm 1.1^{\circ}$C. ($73.4^{\circ} \pm 2^{\circ}$F) and 50 $\pm$ 2 percent relative humidity.

(b) The specimen shall be placed on the adjustable table and moved into contact with the Barcol needle until the 20 lb. downward force is exerted by the spring system. (Move table unitl the upper reference mark on the adjustable vertical rod is even with the top surface of the upper sleeve of the vertical rod).

(c) Raise the adjustable rod 3/32 inch upwards by means of the lever (Raise until the lower of the two reference marks on the vertical rod is even with top surface of the upper sleeve).

(d) Move the test specimen slightly so that the Barcol needle will not contact a Barcol indentation mark or any surface irregularity. Release the lever quickly, but without jerking, and record the highest reading on the dial gage.

(e) Record the dial gage reading 15 seconds after applying the load.

(f) Repeat steps (d) and (e) until 5 separate hardness values have been obtained. Report average 15 second reading.

4.4.1.2 Refractive and addition power. Lens blanks shall be capable of being finished in accordance with the corrected curve surfacing chart supplied by the manufacturer and after finishing shall meet requirements of 3.2.4 when measured as follows: The power shall be measured with a lens measuring instrument. Using a recognized standard lens measuring instrument which gives a measure of vertex power, the bifocal addition power shall be obtained using the following procedure:

Place the segment side of the bifocal toward the light source, and take the difference between the distance and reading portion powers. The measurement through the distance portion must be made as far above the optical center of the distance portion as the measurement through the segment is below the optical center of the distance portion. The target images should be centered by the use of auxiliary prisms. The bifocal addition power shall meet the requirements specified in 3.2.5. This test need not be performed on every lot unless specified, or unless the base curve and segment curve determined by 4.4.2 do not conform.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:08Z
Check the source to verify that this is the current version before use.

4.4.2 Surface power. The surface power shall be measured with an instrument such as lens measure, a lens clock or Geneva gage when the base curve is determined by ANSI Standard Z80.1 - 1972.

5. PACKAGING

5.1 Packaging. Packaging shall be level A or C, as specified (see 6.2).

5.1.1 Unit of issue. One pair of Type I or type II lens blanks, as specified, constitutes one unit of issue.

5.1.2 Level A.

5.1.2.1 Unit package. Each lens shall be wrapped in tissue or enclosed in a suitable paper or plastic envelope or other suitable material and further packaged in snug fitting paperboard box of an appropriate design. Two individually packaged lens of one type only shall be placed together to constitute one pair.

5.1.2.2 Intermediate package. Five units (five pair) of type I or ten units (ten pair) of type II shall be packaged in a snug fitting box constructed in accordance with PPP-B-676. Closure of the box shall be adequate to prevent accidental opening.

5.1.3 Level C. Units shall be packaged in standard commercial containers of the size and kind commonly used, which will afford the degree of protection required for shipment and use of the product for its intended purpose.

5.2 Packing. Packing shall be level A, B or C, as specified (see 6.2).

5.2.1 Level A. Thirty six intermediate packages (180 Type I units or 360 Type II units) of one type only shall be packed in an exterior container designed for a type 2 load and constructed in accordance with PPP-B-585, class 3, style 3; PPP-B-601, overseas type; PPP-B-621, class 2; or PPP-B-636, class weather resistant. Closure and strapping shall be as specified in the appendix of the applicable box specification.

5.2.1.1 Case liner. Each level A wood box shall be lined with a waterproof case liner conforming to MIL-L-10547. Closure and strapping shall conform to applicable paragraph of appendix thereto. Case liner shall not be required for fiberboard boxes. Each fiberboard box shall be waterproofed in accordance with 30.4.2 of PPP-B-636.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:08Z
Check the source to verify that this is the current version before use.

5.2.2 Level B. Thirty six intermediate packages (180 Type I units or 360 Type II units) shall be packed in an exterior container designed for a type 2 load and constructed in accordance with PPP-B-585, class 1, style 3; PPP-B-601, domestic type; PPP-B-621, class 1; or PPP-B-636, class domestic. Closure shall be as specified in the appendix of the applicable box specification.

5.2.3 Level C. The subject commodity shall be packed in substantial commercial containers of the type, size, and kind commonly used for the purpose, so constructed as to insure acceptance and safe delivery by common or other carriers, at the lowest rate, to point of delivery called for in the contract or purchase order.

5.3 Marking.

5.3.1 Unit package. In addition to any commercial markings, each box shall be marked with the power, name or registered trade mark of the contractor and the month and year of manufacture.

5.3.2 Intermediate package. Each intermediate package shall be marked in accordance with MIL-STD-129. Contract or purchase order number and name of contractor shall be shown. The date of manufacture and Type II shelf life marking as specified in MIL-STD-129 shall be shown for Type II lens. Marking shall include: "STORE AT CONTROLLED ROOM TEMPERATURE 15° - 30°C (59° - 86°F)".

5.3.3 Exterior container. Exterior container shall be marked in accordance with MIL-STD-129. Marking shall include the legend: "STORE AT CONTROLLED ROOM TEMPERATURE 15° - 30°C (59° - 86°F.)". The date of manufacture and Type II Shelf Life marking shall be shown for Type II lens.

6. NOTES

6.1 Intended use. Both type I and type II, being the same design, provided both distance and reading power in the same lens with less of an "image jump" for those who require the bifocal type prescription. The lens blanks are heat treatable (type I) and naturally impact resistanct (type II) to conform to FDA regulations.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:08Z
Check the source to verify that this is the current version before use.

6.2 Ordering data. Procurement documents should specify the following:

(a) Title, number and date of this specification.
(b) Type.
(c) Base curve and addition power required.
(d) Applicable levels of packaging and packing (see 5.1 and 5.2).
(e) Applicable NSN.

6.3 Definitions.

6.3.1 Corrected curve lens. A corrected curve lens shall be one member of an integrated series of ophthalmic lenses having surface curvatures especially computed and charted, which reduce the visually important monochromatic aberrations to the least significant feasible in commercial manufacture, for at least a 60 degree vista measured on the eye side, for specified centers of rotation and object distances.

6.3.2 Power of an addition. The power of an addition is defined as the difference between the powers measured through the distance and segment portions of the blank when the segment side is placed against the stop of a recognized standard lens measuring instrument.

6.4 National Stock Number coverage. This specification is intended to cover the following items appearing in the Federal Supply Catalog:

National Stock Number	Item Identification	Specification Designation Type
6540-00-518-5035 and 6540-00-528-2744, 2749, 2752, 2817, 2842, 2843, 2844, 2847, 2848, 2850, 2853, 2857, 2870, 2970, 3016, 3183, 3187, 3270, 3296, 3341, 3479, 3500, and 3514.	LENS BLANK, OPHTHALMIC, BIFOCAL, SEMIFINISHED, White crown glass, one piece.	I
6540-00-124-9107 and 9518 thru 9524 6540-00-518-5040 6540-00-528-3515, 3533, 3559, 3665, 3854 6540-00-535-4909, 4939, 4503, 4532, 4553, 4562, 4572, 4607, 4638, 4643, 4859, 4862, 4863 and 4875 6540-00-538-6410, 6416, 6432, 6450	LENS BLANK, OPHTHALMIC, BIFOCAL, SEMIFINISHED, Plastic, one piece.	II

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:08Z
Check the source to verify that this is the current version before use.

6.5 Changes. Asterisks to indicate changes have been omitted, due to the extensiveness of the changes.

Custodians:
Army - MD
Navy - MS
Air Force - 03

Preparing activity:
Defense Logistics Agency - DM

Project Number 6540-1047

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:08Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

OMB Approval
No. 22-R255

INSTRUCTIONS: The purpose of this form is to solicit beneficial comments which will help achieve procurement of suitable products at reasonable cost and minimum delay, or will otherwise enhance use of the document. DoD contractors, government activities, or manufacturers/ vendors who are prospective suppliers of the product are invited to submit comments to the government. Fold on lines on reverse side, staple in corner, and send to preparing activity. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements. Attach any pertinent data which may be of use in improving this document. If there are additional papers, attach to form and place both in an envelope addressed to preparing activity.

DOCUMENT IDENTIFIER AND TITLE

MIL-L-37184B LENS BLANK, OPHTHALMIC, BIFOCAL, ONE PIECE

NAME OF ORGANIZATION AND ADDRESS	CONTRACT NUMBER
	MATERIAL PROCURED UNDER A ☐ DIRECT GOVERNMENT CONTRACT ☐ SUBCONTRACT

1. HAS ANY PART OF THE DOCUMENT CREATED PROBLEMS OR REQUIRED INTERPRETATION IN PROCUREMENT USE?

A. GIVE PARAGRAPH NUMBER AND WORDING.

B. RECOMMENDATIONS FOR CORRECTING THE DEFICIENCIES

2. COMMENTS ON ANY DOCUMENT REQUIREMENT CONSIDERED TOO RIGID

3. IS THE DOCUMENT RESTRICTIVE?

☐ YES ☐ NO *(If "Yes", in what way?)*

4. REMARKS

SUBMITTED BY *(Printed or typed name and address - Optional)*	TELEPHONE NO.
	DATE

DD FORM 1 JAN 72 1426 – REPLACES EDITION OF 1 JAN 66 WHICH MAY BE USED

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:08Z
Check the source to verify that this is the current version before use.