MILITARY SPECIFICATION

STOPCOCK, INTRAVENOUS THERAPY, 3-WAY, PLASTIC, DISPOSABLE

This specification is approved for use by all Departments and Agencies of the Department of Defense.

1. SCOPE

1.1 Scope. This specification covers a sterile three-way stopcock (four fluid paths) suitable for use in intravenous therapy.

2. APPLICABLE DOCUMENTS

2.1 The following documents of the issue in effect on date of invitation for bids or request for proposals, form a part of the specification to the extent specified herein:

SPECIFICATIONS

Federal

PPP-B-585	Boxes, Wood, Wirebound.
PPP-B-601	Boxes, Wood, Cleated Plywood,
PPP-B-621	Boxes, Wood, Nailed and Lock Corner.
PPP-B-636	Boxes, Shipping, Fiberboard.
PPP-T-76	Tape, Pressure-Sensitive Adhesive Paper (for Carton Sealing).
MMM-A-250	Adhesive, Water-Resistant (for Sealing Waterproofed Paper).

Military

MIL-S-36586	Sterilization Test strip set, Bacterial spore.

STANDARDS

Military

MIL-STD-105	Sampling Procedures and Tables for Inspection by Attributes.
MIL-STD-129	Marking for Shipment and Storage.

FSC 6515

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:07Z
Check the source to verify that this is the current version before use.

(Copies of specifications, and standards, required by suppliers in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.)

2.2 Other publications. The following documents form a part of this specification to the extent specified herein. Unless otherwise indicated, the issue in effect on date of invitation for bids or request for proposals shall apply.

THE UNITED STATES PHARMACOPEIAL CONVENTION, INC.

The Pharmacopeia of the United States of America (USP)

(Application for copies should be addressed to the Mack Publishing Company, Easton, PA 18042).

AMERICAN NATIONAL STANDARDS INSTITUTE INC., (ANSI)

ANSI Z70.1 Glass and Metal Luer Tapers for Medical Applications, Dimensions of

(Application for copies should be addressed to the American National Standards Institute, 1430 Broadway, NY 10018.)

U. S. DEPARTMENT OF HEALTH, EDUCATION AND WELFARE
FOOD AND DRUG ADMINISTRATION

Federal Food, Drug, and Cosmetic Act and General Regulations for its Enforcement.

(Application for copies should be addressed to Food and Drug Administration, U.S. Department of Health, Education, and Welfare, Washington, DC 20204.)

3. REQUIREMENTS

3.1 Material.

3.1.1 Plastic and rubber components. All plastic components, including end protectors, shall be fabricated from material of the best quality and suitable in all respects for the purpose intended. All material shall be sterile, safe (non-toxic) and pyrogen-free. In addition, the plastics shall meet the requirements of the USP for Class II plastics when tested as specified in 4.4.3.

3.1.2 Stopcock body and rotating plug. The stopcock body shall be fabricated from a suitable rigid plastic and the rotating plug shall be fabricated from a rigid or semi-rigid plastic. As an alternate, the rotating plug shall be fabricated from flexible natural rubber mounted to a suitable rigid plastic handle. The total combined quantity of barium, cadmium and lead for each component shall not exceed 5 parts per million (ppm) when tested as specified in 4.4.1.

NOTE: Alternate values and test procedures to those specified herein for extractable metals or heavy metals may be acceptable, providing that sufficient data equating the alternate test and test values to those specified is presented to the Government. Alternate tests and test values that meet or exceed the specified extractable metals requirement shall be acceptable.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:07Z
Check the source to verify that this is the current version before use.

3.2 Style and design. The three-way stopcock (four fluid paths) shall be a unit suitable for use in administering and controlling the direction of flow of blood and solutions for simultaneous and/or alternate intravenous therapy. All ports of the stopcock shall be covered with readily removable end protectors to maintain sterility of the fluid paths until manually removed. The stopcock shall be one of the four basic configurations as shown on Figure I.

3.2.1 Stopcock body and rotating plug. The stopcock proper shall have two arms that possess female Luer cavities and a third arm that shall possess a male Luer taper. The axis of the rotating plug shall be perpendicular to the plane of the inlet-outlet ports. The stopcock body shall be transparent or of contrasting color to the rotating plug and shall form a leakproof assembly with the rotating plug. The rotating plug shall be provided with three outwardly projecting arms which when superimposed over a body outlet port shall indicate the flow path through the stopcock. When all three rotating plug arms are superimposed over the three body ports, all fluid paths shall be flow-interconnected.


3.2.1.1 Female Luer connectors. The female Luer connectors shall be either of the Luer Lock type in accordance with Figure 3 of ANSI Standard Z70.1, or a combination of one Luer Lock connector in accordance with Figure 3 of ANSI Standard Z70.1 and one Luer Slip connector in accordance with Figure 2, female end, of ANSI Standard Z70.1. All female Luer connectors shall meet the requirements specified in 3.2.2.

3.2.1.2 Male Luer connector. The male Luer connector shall be either of the Luer Slip type or the locking collar type, (reference Figure 4 of ANSI Standard Z70.1). The external Luer taper of either type of male connector shall be in accordance with Figure 2, male end, of ANSI Standard Z70.1. The male Luer connector shall meet the requirements specified in 3.2.3.

3.2.2 Diameter and depth of female Luer connectors. The cavities of the female Luer connectors shall be tested for diameter and depth of Luer cavity as specified in 4.4.6. Connectors which do not fit the plug gage within the "GO" - "NO-GO" limits specified in 4.4.6 shall be rejected. When the cavities are fitted onto their respective gaging members, there shall be no movement of the connectors on the gages when the connectors are pressed lightly from side to side in all directions.

3.2.3 Taper of male Luer connector. The male Luer connector shall be tested for proper taper as specified in 4.4.7. Male Luer connectors which do not fit the ring gage within the "GO-NO GO" limits specified in 4.4.7, shall be rejected. In addition, when the ring gage is fitted onto the male connector, as specified in 4.4.7, there shall be no movement of the gage on the tip when the gage is pressed lightly from side to side in all directions.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:07Z
Check the source to verify that this is the current version before use.

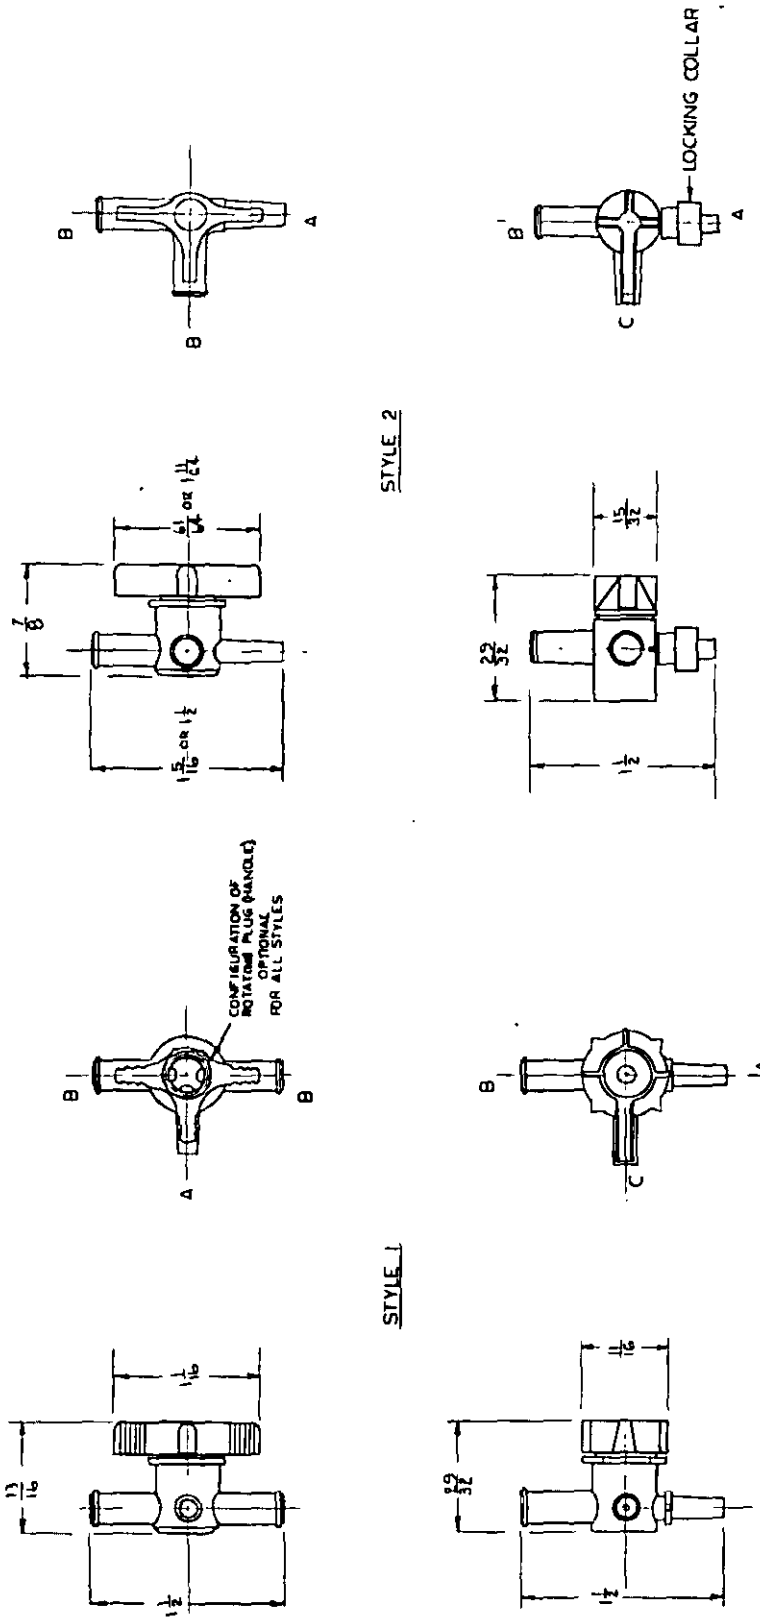

A - MALE LUER SLIP CONNECTOR IN ACCORDANCE WITH FIGURE 2, MALE END OF ANSI STD Z 70.1

B - FEMALE LUER LOCK CONNECTOR IN ACCORDANCE WITH FIGURE 3 OF ANSI STD Z 70.1. AS AN ALTERNATE THE TIPS SHALL BE EXTERNALLY THREADED TO LOCK INTO MALE LUER-LOCK CONNECTORS

C - FEMALE LUER SLIP CONNECTOR IN ACCORDANCE WITH FIGURE 2, FEMALE END OF ANSI STD Z 70.1

ALL OUTLINE DIMENSIONS SHOWN ARE FOR REFERENCES PURPOSES ONLY AND ARE IN INCHES.

FIGURE 1

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:07Z
Check the source to verify that this is the current version before use.

3.3 Sterility, safety, and freedom from pyrogens. All components of the stopcock shall be safe and pyrogen free when tested as specified in 4.4.4, and 4.4.5, respectively. The entire fluid path and end protectors shall be sterile when tested as specified in 4.4.2.

3.4 Leakage of stopcock. When tested as specified in 4.4.8, all connectors and the connection of the rotating plug and stopcock shall not show leakage exceeding the formation of one clinging drop. As an alternate, all connectors, and the connection of the rotating plug and stopcock body shall not show leakage exceeding the formation of one clinging air bubble when tested as specified in 4.4.8.1. The rotating plug shall not separate or loosen from the stopcock body during the leakage tests.

3.5 Security of assembly. When tested as specified in 4.4.9, the rotating plug shall not pull out of, or separate from, the stopcock body.

3.6 Clear passage of fluid path. The entire fluid path of the stopcock shall be clean and free from particles. Stopcocks shall be tested for clear passage of fluid path as specified in 4.4.10. Stopcocks which are sealed or constricted shall be rejected.

3.7 Sterility. The sets shall be sterile when tested with a biological indicator as specified in 4.4.2.

3.7.1 Certificate of sterility. A certificate of sterility, stating that samples from each sterilizer lot have been tested and found to be sterile, shall be submitted to the procuring activity. The certificate of sterility shall include:

a. Item identification.
b. National stock number(NSN),
c. Contract or purchase order number.
d. Sterility lot or control number.
e. Date of sterilization.
f. Quantity of product in sterilizer lot.
g. Type of sterilization (gas, radiation, heat, steam, etc.).
h. Form of biological indicator (i.e., inoculated paper spore strip or carrier, inoculated product, or inoculated simulated product).
i. Test organism(s) and population density used.
j. Test medium, incubation temperature, incubation time, and dates of tests.
k. Number of test units.
l. Statement that samples comply with sterility tests.
m. Signature of head of laboratory or a designated qualified alternate.

When inspection is made at destination, the certificate of sterility shall be submitted by the contractor to the Directorate of Medical Materiel, ATTN:

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:07Z
Check the source to verify that this is the current version before use.

3.7.1 Certificate of sterility. (cont'd)

DPSC-ATQ, Defense Personnel Support Center, 2800 South 20th Street, Philadelphia, Pa., 19101, and a copy forwarded with each shipment to the consignee. When inspection is made at source, certificate of sterility shall be furnished to the cognizant Government Quality Assurance Representative for submission to the procuring activity.

3.7.2 Sterility lot. A sterility lot is that single quantity of product subjected to the same manufacturing operation and simultaneously sterilized in the same sterilizer chamber. Each unit package shall be clearly marked with a sterility lot (control) number and date of sterilization as specified in 5.3.2. Each sterility lot shall be traceable to the pertinent manufacturing lot(s).

3.8 Certificates of freedom from pyrogens, safety and biological tests. A certificate listing all lot or control numbers shall state that representative samples from each lot or control have been tested in accordance with the methods described in the USP and found to be free from pyrogens, safe, and have passed the biological tests. This certificate shall include the specific tests performed and the test results. These certificates shall be submitted by the contractor in the manner as specified in 3.7.1.

3.9 Manufacturer's record. The manufacturer shall place a code or lot number on the immediate container or unit package which can be verified against the manufacturer's records of all tests made on sterile, pyrogen-free and nontoxic units. These records shall be made available for inspection by any duly qualified medical officer of the Armed Forces, National Institutes of Health, or any official of the Federal Food and Drug Administration. No shipment shall be made until all the tests have been completed, verified, and recorded in the permanent records of the manufacturer.

3.10 Instructions. A detailed instruction sheet for proper use of the stopcocks shall be provided with each stopcock.

3.11 Workmanship. Workmanship shall be first class throughout. Stopcocks shall be free from defects which detract from their appearance or impair their serviceability.

4. QUALITY ASSURANCE PROVISIONS

4.1 Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the supplier is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or order, the supplier may use his own or any other facilities suitable for the performance of the inspection requirements

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:07Z
Check the source to verify that this is the current version before use.

4.1 Responsibility for inspection (cont'd).

specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

4.1.1 Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government, upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of 3 years after delivery of the supplies to which such records relate.

4.1.2 Inspection. Inspection, as used in this specification, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

4.1.3 Certificates of quality. Certificates of quality, supplied by the manufacturer of the plastics and rubber used in the manufacture of the stopcocks, may be furnished in lieu of actual performance of such testing by the contractor, provided lot identity has been maintained and can be demonstrated to the Government. The Certificate shall include the name of the contractor, the contract number, the name of the manufacturer or supplier, the NSN, the Item Identification, the name of the component/material, the lot number, the lot size, the sample size the date of testing, the test method, individual test results, and the specification requirements.

4.2 Sampling.

4.2.1 For examination. Sampling for examination shall be conducted in accordance with MIL-STD-105 and as indicated in Table I. The unit of product for examination purposes shall be one stopcock.

Table I. Sampling Criteria for Examination

Type defect	Inspection level	AQL (percent defective)
Major	II	1.0
Minor	II	2.5

4.2.2 For tests.

4.2.2.1 For sterility test. Sampling for the sterility test shall be in accordance with the USP for parenteral devices and as specified in 4.4.2.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:07Z
Check the source to verify that this is the current version before use.

4.2.2.2 For pyrogen and safety tests. Sampling for pyrogen and safety tests shall be as indicated in the USP for transfusion and infusion assemblies. Samples shall be selected which are to be representative of each lot of material used in the fabrication of the stopcocks. As an alternate, sampling shall be on a sterilizer lot basis when sterilizer lots are smaller than, or equal to, production lots.

4.2.2.3 For other tests. Sampling for other tests shall be conducted in accordance with MIL-STD-105, and as indicated in Table II. The unit of product for testing purposes shall be one stopcock. Where feasible, the same sample units shall be used for the determination of two or more test characteristics.

Table II. Sampling Criteria for Tests

Component	Characteristic	Requirement	Test procedure	Inspection level	AQL
Stopcock	Material-Class II	3.1.1	4.4.3	*	**
	Extractable metals	3.1.2	4.4.1	*	**
	Diameter and depth of female Luer connectors	3.2.2	4.4.6	S-1	1.0
	Taper of male Luer connector	3.2.3	4.4.7	S-1	1.0
	Leakage test	3.4	4.4.8 or 4.4.8.1	S-1	1.0
	Security of assembly	3.5	4.4.9	S-1	1.0
	Clear passage of fluid path	3.6	4.4.10	S-1	1.0

*Sufficient samples to perform the extractable metal tests, and biological tests shall be selected from each lot and shall be representative of each batch of material used in the manufacture of the stopcocks.

**No defects permitted.

4.3 Examination.

4.3.1 Examination of stopcocks. The stopcocks shall be examined to determine compliance with all requirements contained in this specification. Examination shall be conducted as specified in Tables I and III. Examination, however, shall not be restricted to defects listed in Table III. Any stopcocks in the sample containing one or more defects shall be rejected and if the number of defective stopcocks in any sample exceeds the acceptance number for that sample, the lot represented by the sample shall be rejected.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:07Z
Check the source to verify that this is the current version before use.

Table III. Classification of Defects

Categories	Defects
Critical	None defined.
Major	
101	Stopcock not of design specified.
102	Stopcock not free from cracks, holes, pits, burrs and slivers.
103	Stopcocks not free from excessive flash.
104	Rotating plug not capable of being rotated in all positions without binding.
105	Fluid paths not protected by end protectors.
106	Stopcock not free from large imbedded particles.
107	Fluid paths obstructed or not free from foreign matter.
108	Silicone or other lubricants present on Luer connectors.
109	End protectors not hand removable.
Minor	
201	Instruction sheet missing.
202	Rotating plug and body same color.
203	Slight flashing on surfaces other than Luer.

4.3.2 Examination for preparation for delivery. An examination shall be made to determine whether the packaging, packing, and marking comply with the requirements of Section 5. Defects shall be scored as specified in Table IV. Sampling shall be in accordance with MIL-STD-105. The sample unit shall be one container fully prepared for delivery. The lot shall be the number of containers offered for inspection at one time. The inspection level shall be S-2 and the acceptable quality level shall be 4.0 defects per hundred units.

Table IV. Examination for Preparation for Delivery

Examination	Defect
Containers	Not as specified.
Quantity	Quantity in interior packages and shipping containers not as specified.
Packaging and packing materials	Any component missing or damaged.
Workmanship	Inadequate application of components, such as incomplete closure of container flaps, tape improperly applied, or containers distorted.
Markings	Omitted, incorrect, illegible, improper location, sequence, or method of application.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:07Z
Check the source to verify that this is the current version before use.

4.4 Tests. Tests shall be conducted to determine compliance with specification requirements.

4.4.1 Extractable metals. The stopcock components proper (excluding end protectors) shall be tested for extractable metals. The specimens shall be cut such that no thickness exceeds 3 millimeters (mm) and eluted for either 72 hours at 50 degrees Centigrade (^{o}C), 24 hours at 70°C, or 60 minutes at 121°C in 0.9 percent saline. Each gram of each specimen shall be covered with 5 milliliters (ml) of the menstruum (recommended amount is 10 grams of the specimen plus 50 ml of solvent). The menstruum shall be collected after agitation, at the end of the selected elution period and submitted to spectographic analysis for barium, cadmium and lead. The metals shall be reported in ppm in the eluate. A value of 1.0 ppm in the eluate shall be equivalent to extracting 1 milligram from 200 grams of test material in the elution period into 1000 ml elution menstruum.

4.4.2 Sterility test. All fluid paths, and end protectors of the stopcock shall be tested for sterility in accordance with the method specified in the USP for parenteral devices using inoculated product, inoculated simulated product, or paper spore strip (carrier). Product containing a biological indicator shall be marked or labeled so that it clearly differentiates from product intended for distribution. The incubation medium and minimum time in each case shall be soybean casein digest for 7 days for inoculated product, inoculated simulated product, or paper spore strip (carrier). The incubation temperature shall be as indicated in paragraph 4.4.2.1. The minimum number of test units, regardless of lot size, shall be 10, except for inoculated carrier which shall be 20 for Type I sterilization and 30 for Type II Sterilization including inoculated carrier and product test units.

4.4.2.1 Inoculated product or simulated product. For each type of sterilization, the organism used shall be as listed below:

Type of Sterilization	Organism	Incubation Temperature
Steam	B. stearothermophilus	55° - 65°C
Dry Heat	B. stearothermophilus, or	55° - 65°C
	B. subtilis var. niger (or globigii)	30° - 35°C
Gas	B. subtilis var. niger (or globigii)	30° - 35°C
Radiation	B. pumilus	30° - 35°C

The number of viable cells shall be sufficient to provide assurance that the product has been sterilized.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:07Z
Check the source to verify that this is the current version before use.

4.4.2.2 Inoculated carrier. Inoculated carriers (paper spore strips) if used shall be in accordance with MIL-S-36586. Other paper carriers shall be inoculated to be of equivalent resistance. The method of incubation and number of test units shall be as indicated in 4.4.2 Sterility test and 4.4.2.1 Inoculated product or simulated product. The method of sterilization will control the organism in the spore strip to be tested for as shown in 4.4.2.1 NOTE: When an inoculated carrier is chosen, product samples must also be tested as required by the USP.

4.4.2.3 Alternate method. Suppliers conducting sterility tests or designating lots in a manner other than that indicated herein shall submit proof that the alternate method provides equal assurance concerning the sterility of the product. However, all sterility tests shall be conducted using biological indicators. Requests for approval of any alternate method of testing for sterility shall be made to the Contracting Officer, and approval obtained before employment of the alternate method.

4.4.2.4 Product testing. Testing for sterility of the product after receipt by the government shall be without a biological indicator and in accordance with the USP.

4.4.3 Biological tests for class II plastics. All plastic components used in fabrication of the stopcocks shall be tested in accordance with the requirements of the USP for class II plastics.

4.4.4 Safety (toxicity test). Samples of the finished stopcock, including end protectors, shall be tested for safety in accordance with the USP for transfusion and infusion assemblies.

4.4.5 Freedom from pyrogens. Samples of the finished stopcock, including end protectors, shall be tested for freedom from pyrogens in accordance with the USP for transfusion and infusion assemblies.

4.4.6 Diameter and depth of female Luer connectors. The Luer cavities, of the female connectors shall be tested with the male Luer taper plug gage in accordance with Figure 5 of ANSI Standard Z70.1 (this gage shall be as shown in the ANSI Standard, except that it shall be constructed with a suitable fluid or pneumatic path to permit performance of the leakage test specified in 4.4.8). The female Luer cavities shall be slipped onto this gage with a straight motion, without turning or twisting the plug gage into the cavity. Once the female Luer cavity is slipped onto the gage, no additional force shall be exerted to force the plug gage into the Luer cavity. The fit of the Luer cavities onto this gage shall be tested by means of the feeler gage in accordance with Figures 5 and 6 of ANSI Standard Z70.1.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:07Z
Check the source to verify that this is the current version before use.

4.4.7 Taper of male Luer connector. The male connector shall be tested with the female Luer ring gage of Figure 7 of ANSI Standard Z70.1. The male connector shall be slipped into this gage with a straight motion, without turning or twisting the male connector into the gage. Once the male connector is slipped into the gage, no additional force shall be exerted to force the male connector into the gage.

4.4.8 Leakage test (hydrostatic method). Samples of the stopcock shall be subjected to an internal water pressure of 20 pounds per square inch gage (psig). The position of the projecting arms of the rotating plug shall be such that all stopcock ports shall be flow interconnected (all three rotating plug arms shall be superimposed over the three body ports). The modified plug gage specified in 4.4.6 shall be inserted into one of the female Luer connectors with a straight motion, without turning or twisting the plug gage into the cavity with a force not to exceed 5 pounds. The feeler gage shall be placed onto the plug gage to assure that the "GO" position is not violated. Another plug gage (not modified with a fluid or pneumatic path) in accordance with Figure 5 of ANSI Standard Z70.1 shall be inserted into the other female Luer connector with a straight motion, without turning or twisting the plug gage into the female Luer cavity with a force not to exceed 5 pounds. The feeler gage shall be placed onto this plug gage to again assure that the "GO" position is not violated.

A hypodermic needle, with the lumen sealed, shall be used to seal the male Luer connector in the following manner: The hub of the hypodermic needle shall be tested to comply with acceptable Luer cavity as specified in 4.4.6. A needle possessing a hub cavity that passes the diameter and depth of Luer cavity shall then be used to seal the male Luer connector of the stopcock.

Water shall then be internally admitted to the testing arrangement in a leakproof manner (air bubbles eliminated), with internal pressure of 20 psig applied for at least 3 minutes. The entire assembly shall be noted for leakage as specified in 3.4.

4.4.8.1 Leakage test (pneumatic method). This test shall be performed as specified in 4.4.8, except that an air pressure of 10 psig shall be applied to the testing assembly arrangement. The entire testing assembly shall be completely immersed into a suitable container of water, with air pressure applied for at least 3 minutes.

4.4.9 Security of assembly. The stopcock shall be tested for security of assembly by applying a straight force or pull of 10 pounds to the rotating plug member for a period of at least one minute with the stopcock body appropriately secured.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:07Z
Check the source to verify that this is the current version before use.

4.4.10 Clear passage test of fluid path Stopcocks shall be tested with an appropriate testing fluid applied internally to the stopcock with the stopcock placed in a horizontal position. Each path shall be tested, in turn, using testing assembly fixtures as specified in 4.4.8, except that one port shall be opened for fluid exit during the test for each path. The stopcock shall allow free passage of the testing fluid within 5 seconds after an internal pressure of 3 ± 1/2 psig has been applied to the stopcock.

5 PREPARATION FOR DELIVERY

5.1 Packaging. Packaging shall be level A or C as specified (see 6.1).

5.1.1 Level A.

5.1.1.1 Individual container. Each stopcock along with instructions shall be packaged in a sealed peel open type container of an appropriate size and capable of maintaining sterility of contents unless the container is damaged or opened. The container shall be designed with tabs to facilitate opening. The instructions may be printed on the envelope or may be inserted within the container.

5.1.1.2 Unit package. Fifty individually packaged stopcocks shall be packaged in a snug fitting box constructed in accordance with PPP-B-636, type CF, class weather-resistant. The box shall be closed by taping the top and bottom flaps with two inch wide tape conforming to PPP-T-76. Closing of bottom flaps with adhesive conforming to MMM-A-250 or metal stitches is permitted.

5.1.2 Level C. Units shall be packaged in standard commercial containers of the size and kind commonly used, which will afford the degree of protection required for shipment and use of the product for its intended purpose.

5.2 Packing. Packing shall be level A, B or C as specified (see 6.1).

5.2.1 Level A. Twelve unit packages shall be packed in an exterior container designed for a type 2 load and constructed in accordance with PPP-B-585, class 3, style 3; PPP-B-601, overseas type; PPP-B-621, class 2; or PPP-B-636, class weather-resistant. Closure and strapping shall be as specified in the appendix of the applicable box specification.

5.2.2 Level B. Twelve unit packages shall be packed in an exterior container designed for a type 2 load and constructed in accordance with PPP-B-585, class 1, style 3; PPP-B-601, domestic type; PPP-B-621, class 1; or PPP-B-636, class domestic. Closure shall be as specified in the appendix of the applicable box specification. Closure of fiberboard boxes shall conform to method II as specified in the appendix of PPP-B-636.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:07Z
Check the source to verify that this is the current version before use.

5.2.3 Level C. The subject commodity shall be packed in substantial commercial containers of the type, size, and kind commonly used for the purpose, constructed so as to insure acceptance and safe delivery by common or other carriers, at the lowest rate, to point of delivery called for in the contract or purchase order.

5.3 Marking.

5.3.1 Individual container. In addition to any commercial markings, each individual container shall be marked in accordance with the requirements of the Federal Food, Drug and Cosmetic Act. Marking shall also include the item identification, sterility lot (control) number, date of manufacture and the legend "STERILITY GUARANTEED UNLESS PACKING IS DAMAGED OR OPENED" or similar statement.

5.3.2 Unit packages. Each unit package shall be marked in accordance with MIL-STD-129. When labels are utilized, waterproofing shall be required only when applicable box is fabricated of water-resistant material. Sterility lot (control) number, contract or purchase order number and name of contractor shall be shown. The method of sterilization (G-Gas, R-Radiation, S-Steam, D-Dry Heat sterilization) shall be shown following the level of packaging and the date of packaging. Example: "A-3/75-G". Final sterilization shall be on or after indicated packaging date.

5.3.3 Exterior container. Exterior container shall be marked in accordance with MIL-STD-129. Sterility lot (control) number and the method of sterilization as specified in 5.3.2 shall also be shown.

6. NOTES

6.1 Ordering data. Procurement documents should specify the following:

(a) Title, number and date of this specification.
(b) Selection of applicable levels of packaging and packing (see 5.1 and 5.2)
(c) National Stock Number

6.2 This specification covers NSN 6515-00-926-9195 STOPCOCK, INTRAVENOUS THERAPY, 3 Way, Plastic, Disposable, 50s listed in the Federal Supply Catalog.

Custodians:
Army - MD
Navy - MS
Air Force - 03

Preparing activity:
Defense Supply Agency - DM

Project No. 6515-1917
CS

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:07Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

OMB Approval No. 22-R255

INSTRUCTIONS: *The purpose of this form* is to solicit beneficial comments which will help achieve procurement of suitable products at reasonable cost and minimum delay, or will otherwise enhance use of the document. DoD contractors, government activities, or manufacturers/ vendors who are prospective suppliers of the product are invited to submit comments to the government. Fold on lines on reverse side, staple in corner, and send to preparing activity. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements. *Attach any pertinent data which* may be of use in improving this document. If there are additional papers, attach to form and place both in an envelope addressed to preparing activity.

DOCUMENT IDENTIFIER AND TITLE: STOPCOCK, INTRAVENOUS THERAPY, 3 WAY, MIL-S-37174 PLASTIC, DISPOSABLE

NAME OF ORGANIZATION AND ADDRESS

CONTRACT NUMBER

MATERIAL PROCURED UNDER A

☐ DIRECT GOVERNMENT CONTRACT ☐ SUBCONTRACT

1. HAS ANY PART OF THE DOCUMENT CREATED PROBLEMS OR REQUIRED INTERPRETATION IN PROCUREMENT USE?

A. GIVE PARAGRAPH NUMBER AND WORDING.

B. RECOMMENDATIONS FOR CORRECTING THE DEFICIENCIES

2. COMMENTS ON ANY DOCUMENT REQUIREMENT CONSIDERED TOO RIGID

3. IS THE DOCUMENT RESTRICTIVE?

☐ YES ☐ NO *(If "Yes", in what way?)*

4. REMARKS

SUBMITTED BY *(Printed or typed name and address - Optional)*

TELEPHONE NO.

DATE

DD FORM 1 JAN 72 1426 REPLACES EDITION OF 1 JAN 68 WHICH MAY BE USED

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:07Z
Check the source to verify that this is the current version before use.

FOLD

DEFENSE PERSONNEL SUPPORT CENTER
2800 South 20th Street
Philadelphia, Pa. 19101

POSTAGE AND FEES PAID
DEFENSE SUPPLY AGENCY
DoD - 304

U.S.MAIL

OFFICIAL BUSINESS
PENALTY FOR PRIVATE USE $300

HEADQUARTERS, DEFENSE PERSONNEL SUPPORT CENTER
ATTN: DIRECTORATE OF MEDICAL MATERIEL, CODE ATT
2800 SOUTH 20TH STREET
PHILADELPHIA, PA. 19101

FOLD

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:07Z
Check the source to verify that this is the current version before use.