MILITARY SPECIFICATION

REGULATOR, OXYGEN, CHEST MOUNTED, DILUTER-DEMAND, AUTOMATIC-PRESSURE BREATHING

This specification is approved for use within the Naval Air Systems Command, Department of the Navy, and is available for use by all Departments and Agencies of the Department of Defense.

1. SCOPE

1.1 Scope. This specification covers one type of automatic-pressure breathing, diluter demand, chest mounted oxygen regulator.

2. APPLICABLE DOCUMENTS

2.1 Government documents.

2.1.1 Specifications, standards and handbooks. The following specifications, standards, and handbooks form a part of this document to the extent specified herein. Unless otherwise specified, the issues of these documents are those listed in the issue of the Department of Defense Index of Specifications and Standards (DODISS) and supplement thereto, cited in the solicitation (see 6.2).

SPECIFICATIONS

FEDERAL

BB-A-1034 - Air, Compressed, for Breathing Purposes.

Beneficial comments (recommendations, additions, deletions) and any pertinent data which may be of use in improving this document should be addressed to: Systems Engineering and Standardization Department (Code 53), Naval Air Engineering Center, Lakehurst, NJ 08733-5100, by using the self-addressed Standardization Document Improvement Proposal (DD Form 1426) appearing at the end of this document or by letter.

AMSC N/A FSC 1660
DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T00:18Z
Check the source to verify that this is the current version before use.

BB-N-411 - Nitrogen, Technical.

PPP-B-601 - Boxes, Wood, Cleated-Plywood.

PPP-B-621 - Box, Wood, Nailed and Lock Corner.

PPP-B-636 - Boxes, Shipping, Fiberboard.

PPP-B-640 - Boxes, Fiberboard, Corrugated, Triple-wall.

MILITARY

MIL-P-116 - Preservation, Methods of.

MIL-D-3464 - Desiccants, Activated, Bagged, Packaging Use and Static Dehumidification

MIL-C-5501 - Cap and Plug, Protective, Dust and Moisture Seal

MIL-C-5541 - Chemical Conversion Coatings on Aluminum and Aluminum Alloys.

MIL-P-7105 - Pipe Threads, Taper, Aeronautical National Form, Symbol ANPT, General Requirements For.

MIL-A-8625 - Anodic Coatings, for Aluminum and Aluminum Alloys.

STANDARDS

FEDERAL

FED-STD-595 - Colors.

MILITARY

MIL-STD-105 - Sampling Procedures and Tables for Inspection By Attributes.

MIL-STD-129 - Marking for Shipment and Storage.

MIL-STD-130 - Identification Marking of U.S. Military Property.

MIL-STD-889 - Dissimilar Metals.

MIL-STD-970 - Standards and Specifications, Order of Precedence for the Selection of.

MIL-STD-1189 - Standard Department of Defense Bar Code Symbology

MIL-STD-1359 - Cleaning Methods and Procedures for Breathing Oxygen Equipment.

Source: https://assist.dla.mil - Downloaded: 2026-10-21T00:18Z
Check the source to verify that this is the current version before use.

MIL-STD-2073-1A- DOD Materiel Procedures for Development and Application of Packaging Requirements

MS 27796 - Connector-Bayonet, Three Pin, Oxygen Mask

HANDBOOKS

MILITARY

MIL-HDBK-695 - Rubber Products, Recommended Shelf Life.

(Unless otherwise indicated, copies of federal and military specificaions, standards, and handbooks are available from the Standardization Document Order Desk, Bldg 4D, 700 Robbins Avenue, Philadelphia, PA 19111-5094.)

2.1.2 Other Government documents, drawings, and publications. The following other Government documents, drawings, and publications form a part of this document to the extent specified herein. Unless otherwise specified, the issues are those cited in the solicitation.

DRAWINGS

NAVAL AIR SYSTEMS COMMAND

62A116C48 - Piezometer

62A116C49 - Tube, Piezometer

62A116C50 - Ring, Piezometer

62A116C51 - Union, Piezometer

62A116E1 - Test Stand, Oxygen Systems Components

1172AS100 - Test Stand

1316AS100 - Test Stand

(Copies of drawings, required by contractors in connection with specific acquisition functions should be obtained from the contracting activity or as directed by the contracting officer.)

2.2 Non-Government publications. The following documents form a part of this document to the extent specified herein. Unless otherwise specified, the issues of the documents which are DoD adopted are those listed in the issue of the DoDISS cited in the solicitation. Unless otherwise specified, the issues of documents not listed in the DoDISS are the issues of the documents cited in the solicitation (see 6.2.).

AMERICAN SOCIETY FOR TESTING AND MATERIAL (ASTM)

ASTM D1149-78a - Rubber Deterioration - Surface Ozone Cracking in a chamber (Flat specimens)

ASTM D 3951-82 - Packaging, Commercial

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T00:18Z
Check the source to verify that this is the current version before use.

(Application for copies should be addressed to the American Society for Testing and Materials, 1916 Race Street, Philadelphia, PA 19103-1137.)

(Nongovernment standards and other publications are normally available from organizations that prepare or distribute the documents. These documents also may be available in or through libraries or other informational services.)

2.3 Order of precedence. In the event of a conflict between the text of this document and the references cited herein (except for related associated detail specifications, specification sheets or MS standards), the text of this document shall take precedence. Nothing in this document, however, supersedes applicable laws and regulations unless a specific exemption has been obtained.

3. REQUIREMENTS

3.1 Qualification. The regulators furnished under this specification shall be products which are authorized by the qualifying activity for listing on the applicable qualified products list at the time set for opening of bids (see 4.3 and 6.3).

3.2 First article. When specified (see 6.2.1e), samples shall be subjected to first article inspection (see 4.4 and 6.5).

3.3 Selection of specifications and standards. Specifications and standards for necessary commodities and services not specified herein shall be selected in accordance with MIL-STD-970.

3.4 Materials. Materials shall conform to applicable specifications and shall be as specified herein and on applicable drawings. Materials which are not covered by specifications, or which are not specifically described herein, shall be of the best quality, of the lightest practicable weight, and suitable for the purpose intended. Materials that produce toxic or corrosive substances shall not be used.

3.4.1 Metal parts. All metal parts shall be of a corrosion-resistant material or treated in such a manner as to render them adequately resistant to corrosion.

3.4.1.1 Dissimilar metals. Unless suitably protected against electrolytic corrosion, dissimilar metals shall not be used in intimate contact with each other. Dissimilar metals are defined in MIL-STD-889.

3.4.2 Nonmetallic materials. Any nonmetallic material that is adversely affected by continued use with oxygen shall not be used.

3.4.2.1 Age. Elastomer components, except silicone, shall not be more than 12 months old from the date of manufacture to the date of delivery to any Government service or to any airframe or accessory manufacturer.

3.4.2.2 Elastomer components. The elastomer components shall be composed of an ozone-resistant composition, which shall not bloom, and shall meet the specified ozone-resistance performance requirements.

3.4.2.3 Storage life. Elastomer materials shall have an expected storage life of eight years or more based on the guidelines of MIL-HDBK-695.

Source: https://assist.dla.mil Downloaded: 2026-10-21T00:18Z
Check the source to verify that this is the current version before use.

3.4.3 Protective treatment. When materials are used in the construction of the regulator that are subject to deterioration when exposed to environmental conditions likely to occur during service usage, they shall be protected against such deterioration in a manner that shall in no way prevent compliance with the performance requirements of this specification. Protective coating which might crack, chip, or scale during normal service life or under extremes of environmental conditions shall not be used.

3.5 Standard parts. MS and AN standard parts shall be used where they suit the purpose.

3.6 Design and construction. The chest mounted oxygen regulator shall be of the diluter-demand, automatic pressure breathing type. The regulator shall be designed in accordance with Figure 1 and shall not exceed the specified envelope dimensions. The regulator shall utilize a single, two-position, manual control to allow the user to select from diluter-demand to 100% oxygen and back to diluter-demand. The regulator shall be capable of delivering an adequate supply of oxygen when used under water. The regulator shall also incorporate a safety device which will automatically deliver 100% oxygen to the user if the inlet pressure should drop below 30 psi.

3.6.1 Diaphragm. The regulator shall be designed to operate by means of a loaded diaphragm. The loading mechanism shall alter the load of the diaphragm with varying altitudes. The demand diaphragm shall be fabricated of silicone compound or silicone-coated cloth which shall be approved by the procuring activity.

3.6.2 Oxygen inlet filter. The oxygen inlet shall be provided with a filter capable of preventing foreign particles, larger than 20 microns, from entering the regulator. The inlet filter shall be located upstream of the inlet port and shall in no way interfere with normal connections to the inlet of the regulator. The filter shall be installed to allow for easy removal or replacement.

3.6.3 Air port. An air port shall be provided for mixing of varying quantities of air with oxygen. The air port shall be provided with a screen, not finer than 100 mesh, nor coarser than 30 mesh, to prevent foreign particles from entering the regulator. The port shall be so located that articles of clothing cannot obstruct the opening.

3.6.4 Moisture. The design shall include provisions for preventing moisture from collecting within the regulator.

3.6.5 Plugs. All openings in the regulator shall be closed with caps or plugs to prevent foreign matter from entering the regulator during shipping and storage.

3.7 Performance.

3.7.1 Visual examination and dimensional check.

3.7.1.1 Visual examination. When visually examined as specified in 4.8.1.1, the regulator shall conform to the requirements of this specification. Table IX, Classification of Defects for Visual Examination, shall be used to classify and enumerate the defects.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T00:18Z
Check the source to verify that this is the current version before use.

3.7.1.2 Dimensional check. When dimensionally checked as specified in 4.8.1.2, the regulator shall be in accordance with Figures 1 and 2.

3.7.2 Flow characteristics. The outlet pressures of the regulator, when tested as specified in 4.8.2, shall be in accordance with the requirements in Table I.

3.7.3 Oxygen ratio. The percentage, by volume, of oxygen delivered with respect to the total oxygen-air mixture delivered, when tested as specified in 4.8.3, shall be accordance with Table II.

3.7.3.1 Low pressure safety. When tested as specified in 4.8.3.1, there shall be 98 to 100 percent oxygen delivered.

3.7.4 Noise level control. The 1/3 octave band analysis of the regulator, after test specified in 4.8.4, shall not exceed the decibel levels (db) of Table III.

3.7.5 Pressure breathing characteristics. The outlet pressure of the regulator, when tested as specified in 4.8.5, shall be in accordance with Table IV.

3.7.6 Relief valve. The relief valve, when tested as specified in 4.8.6, shall not permit a pressure greater than 27 inches of water. The relief valve leakage shall not exceed 0.01 liters per minute (lpm) after completion of the flow test.

3.7.7 Inward leakage. The inward leakage of the regulator, when tested as specified in 4.8.7, shall not exceed 0.20 lpm.

3.7.8 Overall leakage. When tested as specified in 4.8.8, there shall be no overall regulator leakage.

3.7.9 Outward leakage. The outward leakage of the regulator, when tested as specified in 4.8.9, shall not exceed 0.20 lpm. This leakage includes the allowable relief valve leakage.

3.7.10 Outlet leakage. The outlet leakage, when tested as specified in 4.8.10, shall not exceed 0.01 lpm.

3.7.11 Safety pressure. The regulator, when tested as specified in 4.8.11, shall have an outlet pressure between 0.01 and 1.5 inches of water at flows of 0, 10 and 100 lpm.

3.7.12 Overload.

3.7.12.1 Outlet. The regulator, when tested as specified in 4.8.12.1, shall operate satisfactorily.

3.7.12.2 Inlet. The regulator, when tested as specified in 4.8.12.2, shall operate satisfactorily.

3.7.13 Oxygen selector control cycling. The oxygen selector control, when tested as specified in 4.8.13, shall operate satisfactorily.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T00:18Z
Check the source to verify that this is the current version before use.

3.7.14 Oxygen selector control operating force. The oxygen selector control, when tested as specified in 4.8.14, shall require a torque of 0.5 to 3 inch-pounds or 33 ± 17 ounces to move the control in either direction.

3.7.15 High temperature. The regulator, when tested as specified in 4.8.15, shall operate satisfactorily.

3.7.16 Low temperature. The regulator, when tested as specified in 4.8.16, shall operate satisfactorily.

3.7.17 Vibration. The regulator, when tested as specified in 4.8.17, shall operate satisfactorily.

3.7.18 Acceleration. The regulator, when tested as specified in 4.8.18, shall not show any change in the normal flow of oxygen.

3.7.19 Endurance. The regulator, when tested as specified in 4.8.19, shall operate satisfactorily.

3.7.20 Underwater breathing capabilities. The regulator, when tested as specified in 4.8.20, shall be capable of delivering an adequate supply of oxygen and the subject shall be capable of breathing from the regulator while in the submerged condition.

3.7.21 Disassembly and examination. The regulator, when tested as specified in 4.8.21, shall not show any evidence of excessive deterioration or wear due to testing which might affect the regulator performance.

3.7.22 Ozone resistance. The elastomer test slabs, when tested as specified in 4.8.22, shall not show any evidence of checking, cracking or damage.

3.8 Cleanliness. The regulator shall be free of dust, dirt, objectionable odors or any other foreign matters, both internally and externally.

3.9 Interchangeability. All parts having the same manufacturer's part number shall be functionally and dimensionally interchangeable.

3.10 Weight. The weight of the oxygen regulator shall not exceed 12 ounces.

3.11 Color. The color of the regulator shall be black, approximately matching color number 37038 of FED-STD-595.

3.12 Finish. Aluminum and aluminum alloy parts shall be protected in accordance with MIL-A-8625 or MIL-C-5541.

3.13 Identification of product. The regulator shall be marked for identification in accordance with MIL-STD-130, except that the Federal Stock Number shall be omitted from the nameplate.

3.13.1 Serial numbers. Each regulator shall be identified by a serial number which will be assigned by the manufacturer. Serialization shall be by a block of consecutive numbers to cover the entire acquisition quantity. Marking shall be in accordance with 3.13.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T00:18Z
Check the source to verify that this is the current version before use.

3.14 Workmanship. The regulators shall be uniform in quality and shall be free from irregularities, defects, oil, grease, or foreign matter which could adversely affect safety, performance, reliability, or durability. The interior of the regulator shall be free from odor.

4. QUALITY ASSURANCE PROVISIONS

4.1 Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements (examinations and tests) as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any other facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

4.1.1 Responsibility for compliance. All items shall meet all requirements of Sections 3 and 5. The inspection set forth in this specification shall become a part of the contractor's overall inspection system or quality program. The absence of any inspection requirements in the specification shall not relieve the contractor of the responsibility of assuring that all products or supplies submitted to the Government for acceptance comply with all requirements of the contract. Sampling inspection as part of manufacturing operations is an acceptable practice to ascertain conformance to requirements, however, this does not authorize submission of known defective material, either indicated or actual, nor does it commit the Government to acceptance of defective material.

4.2 Classification of inspection. The inspection requirements specified herein are classified as follows:

a. Qualification inspection (see 4.3).

b. First article inspection (see 4.4).

c. Quality conformance inspection (see 4.5).

d. Quality conformance verification inspection (see 4.6).

4.3 Qualification inspection. Qualification inspection shall consist of the examinations and tests specified in Table V.

4.3.1 Qualification samples. Qualification samples shall consist of the following:

a. Four regulators.

b. Three elastomer test slabs, 6 by 6 by .075 inches, composed of the identical ozone-resistant composition and cure that was used in manufacturing the elastomer components.

c. Two sets of manufacturer's drawings in accordance with SD-6.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T00:18Z
Check the source to verify that this is the current version before use.

d. When applicable, certification from the original manufacturer that the distributor requesting qualification status is authorized to distribute the item, or to rebrand and distribute the item, as applicable.

Samples shall be forwarded to the test facility set forth in the letter of authorization to submit samples (see 6.4). The samples shall be plainly identified by securely attached durable tags marked with the following information:

Sample submitted by (name) (date) for qualification inspection in accordance with the requirements of MIL-R-29585 and number under authorization (reference authorizing letter and number. See 6.4).

4.3.2 Retention of Qualified Products Listing (QPL). The retention of qualification listings shall consist of verification every two years to determine compliance of the listed item with the requirements of this specification. Verification shall be by manufacturer's certification unless otherwise specified by the activity responsible for the QPL.

4.4 First article inspection. First article inspection shall consist of the examinations and tests specified in Table VI, Listed Sequence Mandatory. If there is no Qualified Products Listing for the part number being procured, first article testing shall consist of the tests specified in Table V.

4.4.1 First article samples. Unless otherwise specified, as soon as practicable, after the award of the contract or order, the manufacturer shall submit four regulators and three elastomer test slabs, 6 by 6 by .075 inches. The samples shall be representative of the constructions, workmanship, components, and materials to be used during production. When a manufacturer is in continuous production of these units from contract to contract, submission of further first article samples on the new contract may be waived at the discretion of the procuring activity (see 6.2.1e). Approval of the first article samples or the waiving of first article inspection does not preclude the requirements of submitting to the quality conformance inspection. The first article inspection samples shall be furnished to the Government as directed by the contracting officer (see 6.2.1f).

4.4.1.1 First article information. Upon completion of the first article inspection program, the Government activity responsible for conducting the inspection program (see 6.2.1f) shall report to the contracting officer the results of the inspection program, with appropriate recommendations.

4.4.1.2 First article sample disposition. The samples will be destroyed during the inspection program and will not be returned to the contractor.

4.5 Quality conformance inspection. Quality conformance inspection shall consist of the examinations and tests specified in Table VII (Listed Sequence Mandatory). The sampling and inspection levels and acceptance criteria shall conform to MIL-STD-105.

4.5.1 Sampling.

4.5.1.1 Inspection lot.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T00:18Z
Check the source to verify that this is the current version before use.

4.5.1.1.1 Regulator. An inspection lot size shall be expressed in units of regulators made essentially under the same conditions and from the same materials and components. The sample unit shall be one regulator.

4.5.1.1.2 Packaging. An inspection lot size shall be expressed in units of one fully prepared shipping container, containing regulators fully prepared for delivery, made from essentially the same materials and components. The sample unit shall be one shipping container, containing regulators fully prepared for delivery with the exception that it need not be sealed.

4.5.1.2 Sampling for tests and examinations of regulators. The sample size, acceptance criteria, tests, and examinations required for the regulators shall be as specified in Table VII and 4.6.

4.6 Quality conformance verification inspection. Upon successful completion of the quality conformance inspections specified in Table VII, a random sample shall be selected from each lot by the cognizant Government Quality Assurance Representive/Specialist. Sample selection shall be in accordance with MIL-STD-105, inspection level S-3; and the sample size shall be based only on the applicable sample size code letter corresponding to inspection level S-3. The samples selected shall be forwarded to the testing facility designated in the acquisition document (see 6.2.1g) for the tests and examinations listed in Table VII, listed sequence mandatory. The serial numbers of the units in the lot represented by the sample units shall be included in the data accompanying the samples to the testing facility. The Government activity responsible for conducting the Quality Conformance Verification Inspection program (see 6.2.1g) shall report the results of the tests and examinations to the designated inspection and acceptance activity specified in the acquisition document. Final acceptance of the lot from which the samples were selected shall be based upon successful completion of the inspection program by the cognizant Government Quality Assurance Representative/Specialist at the contractor's facility.

4.7 Test conditions.

4.7.1 Test gas. Unless otherwise specified, the test gas shall be nitrogen in accordance with BB-N-411, Type I, Class I, Grade B or compressed breathing air in accordance with BB-A-1034.

4.7.2 Temperature and pressure. Unless otherwise specified, tests shall be conducted at local ambient temperature and barometric pressure. Test instruments shall be calibrated or adjusted according to their required usage in conducting individual tests. Any test results obtained at conditions other than normal temperature and pressure (NTP) conditions shall be mathematically corrected to NTP conditions. NTP conditions are 29.92 inches of mercury and 70°F. In the case of pressure drop measurements, the flow setting for conducting the test shall be corrected to NTP conditions before the test is conducted.

4.7.3 Adjustment of inlet supply pressure. At the start of the operational tests, the initial static test inlet pressure of 40, 50, 70 or 120 psig applies only to zero flow conditions. When the pressure reducing regulator device is not in the same ambient conditions as the oxygen breathing regulator, means shall be provided to determine the above noted pressure at the ambient conditions of the breathing regulator. When flow is started, the

Source: https://assist.dla.mil - Downloaded: 2026-10-21T00:18Z
Check the source to verify that this is the current version before use.

inlet supply pressure shall not be allowed to drop more than 8 psig at 100 lpm ambient flow for inlet pressures of 50, 70 or 120 psig. Under no condition shall the inlet supply pressure be allowed to drop below 40 psig.

4.7.4 Orientation. The regulator shall operate as specified herein in any position in which it is mounted.

4.7.5 Piezometer assembly. The piezometer shall be connected to the mask end of the regulator as shown in Figure 3.

4.7.6 Vibratory control. If during any of the tests, the regulator vibrates, flutters, chatters, or makes noises, the regulator shall be rejected. A vibration or flutter is that condition in the regulator that causes the output flow and meter to fluctuate. Flutter dampers shall not be used to control or eliminate this condition. Flutter or vibration shall also be determined by using live subjects at various altitude conditions and shall take precedence over other types of tests when determining if flutter or vibration exists. During the subjective tests, the regulator shall be connected to an oxygen hose and mask as specified in Figure 4.

4.7.7 Test equipment.

4.7.7.1 Noise level control test set-up. Noise level control test set-up shall be in accordance with Figure 3 and the test shall be conducted in accordance with 4.8.3. The set-up shall consist of Bruel and Kjaer test equipment, or equivalent approved by the procuring activity. The equipment shall be as specified in Table VIII.

4.7.7.2 Test equipment. For qualification and quality conformance inspections, all flow and pressure tests should be performed on stand models 62A116E1, 1172AS100 or 1316AS100. Regulators, when tested on other stands, shall be capable of fulfilling all flow and pressure test requirments of this specification when tested on test stand models 62A116E1, 1172AS100 or 1316AS100.

4.8 Inspection methods.

4.8.1 Visual examination and dimensional check.

4.8.1.1 Visual examination. Every regulator shall be examined visually (for critical defects) and shall meet the requirements of 3.7.1.1.

4.8.1.2 Dimensional check. The regulators shall be dimensionally checked for conformance to the requirements of 3.7.1.2.

4.8.1.3 Packaging. Each of the fully prepared shipping containers, containing regulators selected as a sample unit from the lot shall be examined to determine that the packaging, packing, and marking conform to this specification. The classification of defects, Table X, shall be used to classify the defects found.

4.8.2 Flow characteristics. The regulator inlet shall be connected to a pressure source capable of providing the inlet pressures and conditions specified in Table I. With the regulator in the "dilute" position, the outlet pressure shall be measured as specified in 4.7.5. The regulator shall meet the requirements of 3.7.2.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T00:18Z
Check the source to verify that this is the current version before use.

4.8.3 Oxygen-ratio. The regulator oxygen selector control shall be set in the "dilute" position and the regulator inlet connected to a 40 psig pressure source. The outlet shall be connected to the piezometer assembly specified in 4.7.5. The regulator shall be subject to the outlet flows and altitudes specified in Table II. The oxygen ratio shall be determined by measuring the flow of ambient air entering the test stand altitude chamber required to stabilize the test stand altitude. The test shall then be repeated using a 120 psig inlet pressuree. THe regulator shall meet the requirements of 3.7.3.

4.8.3.1 Low pressure safety. The regulator oxygen control shall be set in the "dilute" position and the regulator connected as specified in 4.8.3. With the altitude at sea level and the inlet pressure decreased to 29 psig, the regulator shall meet the requirements of 3.7.3.1. This test shall be conducted with outlet flows of 0, 15, 50, and 100 liters per minute (lpm).

4.8.4 Noise level. The regulator shall be installed as shown in Figure 3. The regulator shall then be subjected to an ambient flow of 100 lpm at inlet pressures of 70 and 120 psig. The noise level shall be measured utilizing the specified noise level equipment (see 4.7.7.2), and shall pass the requirement specified in 3.7.4.

4.8.5 Pressure breathing characteristics. The regulator oxygen selector control shall be set in the "dilute" position and inlet pressure adjusted to 40 psig. The regulator shall be subject to the flows and altitudes specified in Table IV. This test shall be repeated with the oxygen selector control in the 100% oxygen position. These tests shall then be repeated with 120 psig inlet pressure. The regulator outlet pressure shall be measured as specified in 4.7.5 and the regulator shall meet the requirements of 3.7.5.

4.8.6 Relief valve. The regulator oxygen selector control shall be placed in the "Dilute" position and increasing pressure shall be applied to the outlet of the regulator to maintain a flow of 50 lpm for a period of 30 seconds, and the pressure shall be determined. Upon completion of the flow test, the relief valve shall be subjected to a pressure of 17 inches of water, maintained for a period of 30 seconds, and the leakage shall be determined. The relief valve shall pass the requirements specified in 3.7.6.

4.8.7 Inward leakage. With the regulator oxygen selector control set at the 100% oxygen position and the inlet port plugged, a suction of 10 inches of water shall be applied at the regulator outlet. The leakage from the regulator shall pass the requirements specified in 3.7.7.

4.8.8 Overall leakage. With the regulator oxygen selector control set in the "Diluter" position, a pressure of 120 psig shall be applied to the inlet of the regulator. The regulator leakage shall be determined by a pressure drop in a known volume or with a suitable flowmeter on the inlet side of the regulator. The regulator shall pass the requirements specified in 3.7.8.

4.8.9 Outward leakage. With the regulator oxygen selector control set in the "Diluter" position and the inlet port plugged, a pressure of 17 inches of water shall be applied to the regulator outlet through a flow metering device. The pressure shall be maintained for a minimum period of 2 minutes. The regulator shall pass the requirements specified in 3.7.9.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T00:18Z
Check the source to verify that this is the current version before use.

4.8.10 Outlet leakage. With the regulator oxygen selector control set in the "Dilute" position, a pressure of 70 psig shall be applied to the regulator inlet. The outlet leakage shall be measured using a suitable measuring device. The test shall then be repeated using a pressure of 120 psig. The regulator shall pass the requirements specified in 3.7.10.

4.8.11 Safety pressure. The regulator shall be connected to a pressure source capable of providing a pressure of 70 psig. With the oxygen selector control in the "100% oxygen" position and a inlet pressure of 70 psig, flows of 10 lpm and 100 lpm shall be drawn from the regulator outlet. The regulator outlet flow shall then be reduced to zero. The regulator shall pass the requirements specified in 3.7.11. The test shall then be repeated using inlet pressures of 40 and 120 psig at 10,000 feet.

4.8.12 Overload.

4.8.12.1 Outlet. With the regulator oxygen selector control in the "100%" position, the inlet and all other orifices shall be capped and a pressure of 27 inches of water shall be applied to the outlet of the regulator and maintained for 2 minutes. The regulator shall pass the requirements specified in 3.7.12.1.

4.8.12.2 Inlet. While maintaining a zero flow condition at sea level with the regulator oxygen selector control in the "Dilute" position, a pressure of 150 psig shall be applied to the inlet of the regulator for 3 minutes. The regulator shall pass the requirements specified in 3.7.12.2.

4.8.12.3 Verification. Upon completion of the tests specified in 4.8.12.1 and 4.8.12.2, the regulator shall be subjected to and pass the requirements of the flow characteristics, oxygen ratio and pressure breathing characteristics test.

4.8.13 Oxygen selector control cycling. The regulator shall be connected to a pressure source capable of providing a pressure of 120 psig. With an inlet pressure of 120 psig, the oxygen selector control on the regulator shall be cycled between "Dilute" and "100% oxygen" positions for a minimum of 1000 cycles at a rate of 10 cycles per minute. A cycle shall consist of changing the oxygen selector control position from "Dilute" to "100% oxygen" and back to "Dilute". The regulator shall pass the requirements specified in 3.7.13. The regulator shall then be subjected to and pass the safety pressure and the oxygen control selector operating force test.

4.8.14 Oxygen selector control operating force. The regulator shall be connected to a pressure source capable of providing a pressure of 70 psig. With a inlet pressure of 70 psig, the force required to actuate the oxygen selector control on the regulator shall be measured. The oxygen selector control operating force shall pass the requirements specified in 3.7.14.

4.8.15 High temperature. The regulator shall be conditioned at a temperature of 160° ± 5°F for 3 hours. After conditioning, and while still at this temperature, the regulator shall be subjected to the flow characteristics, oxygen ratio and the pressure breathing characteristics tests. The regulator shall then be returned to room temperature and subjected to the flow characteristics, oxygen ratio, and the pressure breathing characteristics tests. The regulator shall pass the requirements specified in 3.7.15.

Source: https://assist.dla.mil - Downloaded: 2026-10-21T00:18Z
Check the source to verify that this is the current version before use.

4.8.16 Low temperature. The regulator shall be conditioned at a temperature of -65° ± 5°F for 3 hours. After conditioning and while still at this temperature, the regulator shall be subjected to the flow characteristics, oxygen ratio and the pressure breathing characteristics tests. The regulator shall then be returned to room temperature and subjected to the flow characteristics, oxygen ratio, and the pressure breathing characteristics tests. The regulator shall pass the requirements specified in 3.7.16.

4.8.17 Vibration. The regulator shall be capped with end caps containing a minute bleed hole to relieve the buildup of pressure. A pressure of 70 ± 10 psig shall be applied to the inlet of the regulator. The regulator shall be vibrated for 3 hours at a frequency from 300 to 3000 cycles per minute, and a double amplitude of 0.018 to 0.020 inch. After vibration, the regulator shall be subjected to the pressure breathing characteristics test, oxygen-ratio test and the flow characteristics test and shall meet the values specified in Tables IV, II and I, respectively. The regulator shall then be subjected to and pass the requirements of the inward and outlet leakage tests. The regulator shall pass the requirements specified in 3.7.17.

4.8.18 Acceleration. A pressure of between 40 to 120 psig shall be applied to the inlet of the regulator and an acceleration force of 7g shall be applied to the regulator in six different directions. One force shall be applied at one time, and the forces shall be in the directions shown in Figure 5. During the application of each acceleration force, the regulator shall pass the requirements in 3.7.18.

4.8.19 Endurance. The regulator shall be subjected to 250,000 breathing cycles at a rate of 15 to 18 cycles per minute. The peak delivery rate shall be 30 lpm (NTP) flow for 90 percent of the time and 90 lpm (NTP) for 10 percent of the time. The regulator shall pass the requirements specified in 3.7.19. The regulator shall then be subjected to and pass the flow characteristics and the pressure breathing characteristics tests.

4.8.20 Underwater breathing capabilities. The regulator shall be connected to the hose and oxygen mask as specified in Figure 4. The regulator shall be positioned 2 to 4 inches below the subject's suprasternal notch. The inlet oxygen pressure shall be maintained at 50 psig. The subject shall be submerged under 16 feet of water, for 3 minutes, in both the upright and inverted positions. Under these conditions, the regulator shall pass the requirements specified in 3.7.20. At the conclusion of this test procedure, the regulator shall be dried at 120°F for three hours.

4.8.21 Disassembly and examination. At the conclusion of all the inspections, the regulator shall be disassembled and examined, and shall pass the requirements specified in 3.7.21. The regulator shall be disassembled and examined after any test, following initial pressure characteristics test, in which regulator failure indicates faulty construction.

4.8.22 Ozone-resistance (elastomer components). The three elastomer test slabs submitted for qualification inspection shall be tested for ozone resistance. The test apparatus shall be in accordance with ASTM D 1149. The test slabs shall be elongated 20 percent, placed in an ozone-free atmosphere for 24 hours, then placed in the ozone chamber. The chamber shall be adjusted

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T00:18Z
Check the source to verify that this is the current version before use.

to 100° ± 2°F and to give an exposure of ozone concentration of 120 ± 10 parts by volume of ozone per million parts by volume of air. The air-ozone velocity in the chamber shall be at least 2 feet per second. The material shall be exposed to these conditions for 60 minutes. The test slabs shall be examined under a 10X magnification and pass the requirements specified in 3.7.22.

5. PACKAGING

5.1 Preservation and packaging. Preservation and packaging shall be Level A in accordance with MIL-STD-2073-1A or commercial (see 6.2.1h).

5.1.1 Level A. The regulator shall be preserved and packaged in accordance with MIL-P-116, Sub-method IIB, using desiccant conforming to MIL-D-3464, Type II, non-dusting.

5.1.1.1 Cleaning and drying. Each regulator shall be cleaned and dried for oxygen service in accordance with the requirements of MIL-STD-1359. Immediately after cleaning and drying, all openings in the regulator shall be closed with rigid polyethylene caps and plugs conforming to MIL-C-5501 to prevent entry of dirt or foreign matter during shipment and storage.

5.1.1.2 Preservative application. Application of preservative materials, both contact preservatives and volatile corrosion inhibitor, is prohibited.

5.1.1.3 Unit packaging. Each regulator, preserved and packaged as described above, shall be placed into a container conforming to PPP-C-636, Type CF, Class Weather Resistant.

5.1.2 Commercial. The regulator shall be preserved in accordance with ASTM D 3951-82.

5.2 Packing. Packing shall be Level A, B or C, as specified in the contract or order (see 6.2.1h).

5.2.1 Level A. Each unit, packaged as specified in 5.1, shall be packed for shipment in containers confirming to PPP-B-601 or PPP-B-621, Overseas Type.

5.2.2 Level B. Each unit, packaged as specified in 5.1, shall be packed for shipment in containers conforming to PPP-B-601 or PPP-B-621, Domestic Type; fiber-board boxes conforming to PPP-B-636 or PPP-B-640, Weather Resistant may be used provided that the gross weight is not greater than the applicable specification limitation.

5.2.3 Level C. Units, packaged as specified in 5.1, shall be packed for shipment in exterior-type shipping containers conforming to rules and regulations pertaining to mode of transportation and acceptable to carrier at the lowest possible tariff rate that will ensure safe delivery. Contractor's commercial/industrial packing procedure may be used when the above criteria are met.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T00:18Z
Check the source to verify that this is the current version before use.

5.3 Marking. All unit packages and shipping containers shall be marked in accordance with MIL-STD-129, including bar code markings as specified in MIL-STD-129 and MIL-STD-1189. In addition, the following precautionary markings shall be required on each unit package and shipping container:

CAUTION

CLEANED FOR OXYGEN SERVICE

DO NOT ALLOW PETROLEUM CONTAMINANTS OF ANY KIND TO BE USED/STORED ON OR ABOUT THESE CONTAINERS.

5.4 Special requirements. All wrappings, cushioning, dunnage and containers used in preservation, packaging and packing of regulators shall be completely free of contamination by oil or grease.

6. NOTES

(This section contains information of a general or explanatory nature that may be helpful, but is not mandatory.)

6.1 Intended use. The regulator covered by this specification is intended to provide crew members breathing oxygen with dilution at altitudes up to 29,000 feet and with automatic pressure breathing at altitudes from 30,000 feet to 50,000 feet.

6.2. Acquisition requirements. Acquisition documents should specify the following:

a. Title, number and date of this specification including any amendment.

b. Issue of DODISS to be cited in the solicitation, and if required, the specific issue of individual documents referenced (see 2.1.1 and 2.2)

c. Government part number.

d. Quantity desired.

e. Whether first article inspection is waived (see 4.4.1).

f. Name and address of the first article inspection laboratory (see 4.4.1) and the name of the Government activity responsible for conducting the first article inspection program (see 4.4.1.1).

g. If required, name and address of the quality conformance verification inspection laboratory (see 4.6) and the name of the Government activity responsible for conducting the quality conformance verification inspection program (see 4.6).

h. Applicable levels of preservation, packaging, and packing (see 5.1 and 5.2); including marking requirements (see 5.3) and special requirements (see 5.4).

Source: https://assist.dla.mil Downloaded: 2026-10-21T00:18Z
Check the source to verify that this is the current version before use.

6.3 Consideration of data requirements. The following data requirements should be considered when this specification is applied on a contract. The applicable Data Item Descriptions (DID's) should be reviewed in conjunction with the specific acquisition to ensure that only essential data are requested/provided and that the DID's are tailored to reflect the requirements of the specific acquisition. To ensure correct contractual application of the data requirements, a Contract Data requirements List (DD Form 1423) must be prepared to obtain the data, except where DOD FAR Supplement 27.475-1 exempts the requirement for a DD Form 1423.

Reference paragraph	DID Number	DID Title	Suggested tailoring
4.4.1.1	DI-T-5329	First Article Inspection Report	use contractor format

The above DID's were those cleared as of the date of this specification. The current issue of DOD 5010.12-L, Acquisition Management Systems and Data Requirements Control List (AMSDL), must be researched to ensure that only current, cleared DID's are cited on the DD Form 1423.

6.4 Qualification. With respect to products requiring qualification, awards will be made only for products which are, at the time set for opening of bids, qualified for inclusion in Qualified Products List (QPL-29585) whether or not such products have actually been so listed by that date. The attention of the contractors is called to these requirements, and manufacturers are urged to arrange to have the products that they propose to offer to the Federal Government tested for qualification in order that they may be eligible to be awarded contracts of purchase orders for the products covered by this specification. The activity responsible for the Qualified Products List is Commander, Naval Air Systems Command, Washington, DC 20361; however, information pertaining to qualification of products may be obtained from the Naval Air Development Center (Code 6031), Warminster, PA 18974. Prior to submission of the samples for qualification inspection, the manufacturer shall submit a request to the Naval Air Development Center (Code 6031), indicating a date on which the samples can be forwarded and also request an authorization number to accompany the samples.

6.4.1 Documentation. When requested, the manufacturer shall make available engineering drawings and inspection reports in accordance with SD-6, 'PROVISIONS GOVERNING QUALIFICATION (Qualified Product List)'.

6.5 First article. When a first article inspection is required, the item should be a first article sample. The contracting officer should include specific instructions in acquisition documents regarding arrangements for examinations, approval of first article test results and disposition of first articles. Invitations for bids should provide that the Government reserves the right to waive the requirement for samples for first article inspection to those bidders offering a product which has been previously acquired or tested by the Government, and that bidders offering such products, who wish to rely on such production or test, must furnish evidence with the bid that prior Government approval is presently appropriate for the pending contract.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T00:18Z
Check the source to verify that this is the current version before use.

6.6 Laboratory information. The successful bidder will be furnished with the name of the quality conformance verification inspection laboratory and the Government activity responsible for conducting the inspection program at the time of award. Samples from a rejected lot shall not be resubmitted for tests and examinations, as required by 4.6, without the approval of the contracting officer.

6.7 Subject term (keyword) listings.

Gas Contaminant
Sea Level Operation
Altitude Operation
Oxygen System
Breathing Gas
Pressure Breathing
Diluter Demand
Breathing Regulator
Chest Mounted

Preparing activity:
Navy - AS

(Project 1660-N616)

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T00:18Z
Check the source to verify that this is the current version before use.

TABLE I. Flow Characteristics.

REGULATOR INLET PRESSURE (PSIG)	OUTLET FLOW (LITERS/MINUTE)	OUTLET PRESSURE (INCHES OF WATER)	ALTITUDE (1,000 FEET)
40 through 120	15 50 85 100	0 to -0.06 0 to -0.70 0 to -1.0 0 to -1.5	0,5,10,15,20,25

TABLE II. Percentage Oxygen Supplied to Total Delivered

ALTITUDE (1,000 FEET)	TOTAL OUTLET FLOW (LITERS/MINUTE)		
	15	50	100
	PERCENT OXYGEN WITH CONTROL AT "DILUTE"		
0	0 thru 100	0 thru 50	----------
5	1 thru 100	1 thru 50	----------
10	6 thru 100	6 thru 50	6 thru 65
15	14 thru 100	14 thru 60	14 thru 70
20	24 thru 100	24 thru 70	24 thru 80
25	40 thru 100	40 thru 100	40 thru 90
29	98 thru 100	98 thru 100	98 thru 100
	PERCENT OXYGEN WITH CONTROL AT 100%		
ALL ALTITUDES	98 thru 100	98 thru 100	98 thru 100

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T00:18Z
Check the source to verify that this is the current version before use.

TABLE III. Noise Level

1/3 OCTAVE BAND CENTER FREQUENCY	dba (REFERRED TO) 0.0002 dynes/cm^2
320	95
400	95
500	95
640	95
800	95
1000	95
1250	95
1600	95
2000	95
2500	95
3200	95
4000	95
5000	95
6400	95

TABLE IV. Pressure Breathing Characteristics

INLET SUPPLY PRESSURES (PSIG)	OUTLET FLOW (lpm)	ALTITUDE (FEET)	OUTLET PRESSURE (INCHES OF WATER)
40 through 120	0, 10, 100	Sea Level to 30,000 on "100%" only	0 to 1.5
40 through 120	0, 10, 50, 100	30,000	0.01 to 2.5
40 through 120		40,000	0.3 to 5.6
40 through 120		43,000	5.3 to 10.2
40 through 120		50,000	11.2 to 18.2

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T00:18Z
Check the source to verify that this is the current version before use.

TABLE V. Qualification Inspection (see 4.3)

INSPECTION	REQUIREMENT PARAGRAPH(S)	TEST METHOD PARAGRAPH(S)
Visual examination	3.7.1.1	4.8.1.1
Dimensional check	3.7.1.2	4.8.1.2
Flow characteristics	3.7.2	4.8.2
Oxygen-ratio	3.7.3	4.8.3
Low pressure safety	3.7.3.1	4.8.3.1
Pressure breathing characteristics	3.7.5	4.8.5
Relief valve	3.7.6	4.8.6
Inward leakage	3.7.7	4.8.7
Overall leakage	3.7.8	4.8.8
Outward leakage	3.7.9	4.8.9
Outlet leakage	3.7.10	4.8.10
Safety pressure	3.7.11	4.8.11
Overload, outlet	3.7.12.1	4.8.12.1
Overload, inlet	3.7.12.2	4.8.12.2
Oxygen selector control cycling	3.7.13	4.8.13
Oxygen selector control operating force	3.7.14	4.8.14
High temperature	3.7.15	4.8.15
Low temperature	3.7.16	4.8.16
Vibration	3.7.17	4.8.17
Acceleration	3.7.18	4.8.18
Endurance	3.7.19	4.8.19
Underwater breathing capabilities	3.7.20	4.8.20
Disassembly and examination	3.7.21	4.8.21
Ozone resistance	3.7.22	4.8.22
Noise level control	3.7.4	4.8.4

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T00:18Z
Check the source to verify that this is the current version before use.

TABLE VI. First Article Inspection (see 4.4)

INSPECTION	REQUIREMENT PARAGRAPH	TEST METHOD PARAGRAPH
Visual examination	3.7.1.1	4.8.1.1
Dimensional check	3.7.1.2	4.8.1.2
Overload	3.7.12	4.8.12
Flow characteristics	3.7.2	4.8.2
Oxygen-ratio	3.7.3	4.8.3
Low pressure safety	3.7.3.1	4.8.3.1
Pressure breathing characteristics	3.7.5	4.8.5
Relief valve	3.7.6	4.8.6
Inward leakage	3.7.7	4.8.7
Overall leakage	3.7.8	4.8.8
Outward leakage	3.7.9	4.8.9
Outlet leakage	3.7.10	4.8.10
Safety pressure	3.7.11	4.8.11
Oxygen selector control cycling	3.7.13	4.8.13
Oxygen selector control operating force	3.7.14	4.8.14
Noise level	3.7.4	4.8.4

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T00:18Z
Check the source to verify that this is the current version before use.

TABLE VII. Quality Conformance Inspection

INSPECTION	TEST METHOD PARAGRAPH(S)	SAMPLE SIZE	ACCEPTANCE CRITERIA
Visual examination	4.8.1.1	a. Every regulator for critical defects. b. Inspection Level II for minor defects.	a. Reject all units with any critical defect. b. An acceptable quality level of 2.5 defects per hundred units for minor defects.
Dimensional check	4.8.1.2	Inspection Level S-2 1/	Acceptance number zero rejection number 1.
Flow characteristics	4.8.2	Every regulator	Reject all defective units.
Oxygen-ratio	4.8.3	Every regulator	Reject all defective units.
Pressure breathing characteristics	4.8.5	Every regulator	Reject all defective units.
Relief valve	4.8.6	Every regulator	Reject all defective units.
Overall leakage	4.8.8	Every regulator	Reject all defective units.
Outlet leakage	4.8.10	Every regulator	Reject all defective units.
Safety pressure	4.8.11	Every regulator	Reject all defective units.
Oxygen selector operating forces	4.8.14	Inspection Level S-2 1/	Acceptance number zero rejection number 1.
Noise level	4.8.4	Every regulator	Reject all defective units.
Packaging	4.8.1.3	Inspection Level S-2 1/	Total acceptable quality level of 4.0 percent defective

1/ The sampling plan acceptance numbers shall apply collectively to all the characteristics within a stated acceptable quality level.

Source: https://assist.dla.mil - Downloaded: 2026-10-21T00:18Z
Check the source to verify that this is the current version before use.

TABLE VIII. Noise Level Control Test Equipment

DESCRIPTION	MODEL NO.
Digital Frequency Analyzer	2131
Condenser Microphone 1 inch free field	4145
Condenser Microphone Preamplifier	2619S
Graphic Level Recorder, with Voltage Control Paper Drive	2307A
Operation 2120 and 1614-10 Synchronous or Charge Cable	AQ-0035

TABLE IX. Classification of Defects for Visual Examination of the Regulator


CRITICAL	MINOR
1. Material imperfections -foreign matter embedded.	201. Marking - missing, insufficient, incorrect, illegible, or not permanent.
2. Surface - unlean, rough, misaligned, or containing cracks, nicks, or other flaws.	202. Color not as specified.
3. Any component missing, malformed, fractured, or otherwise damaged.	
4. Any component loose or otherwise not securely retained.	
5. Incorrect assembling or improper positioning or components.	
6. Any functioning part that works with difficulty.	
7. Faulty workmanship or other irregularities.	

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T00:18Z
Check the source to verify that this is the current version before use.

TABLE X. List of Defects for Preparation for Delivery

ITEM	DEFECTS
Exterior and interior markings	Missing, incorrect, incomplete, illegible; of improper size, location, sequence; or method of application; markings not the same on the interior and exterior containers.
Packaging and Packing materials	Any non-conforming component; any component missing, damaged, or otherwise defective.
Workmanship	Inadequate application of the components such as incomplete closure of the unit package, intermediate package, case liners, container flaps, loose strappings, etc.; bulging or distortion of the containers.
Exterior and interior weight or content	Number per container is more or less than required; gross or net weight exceeds the requirements; more than one type in the same container.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T00:18Z
Check the source to verify that this is the current version before use.

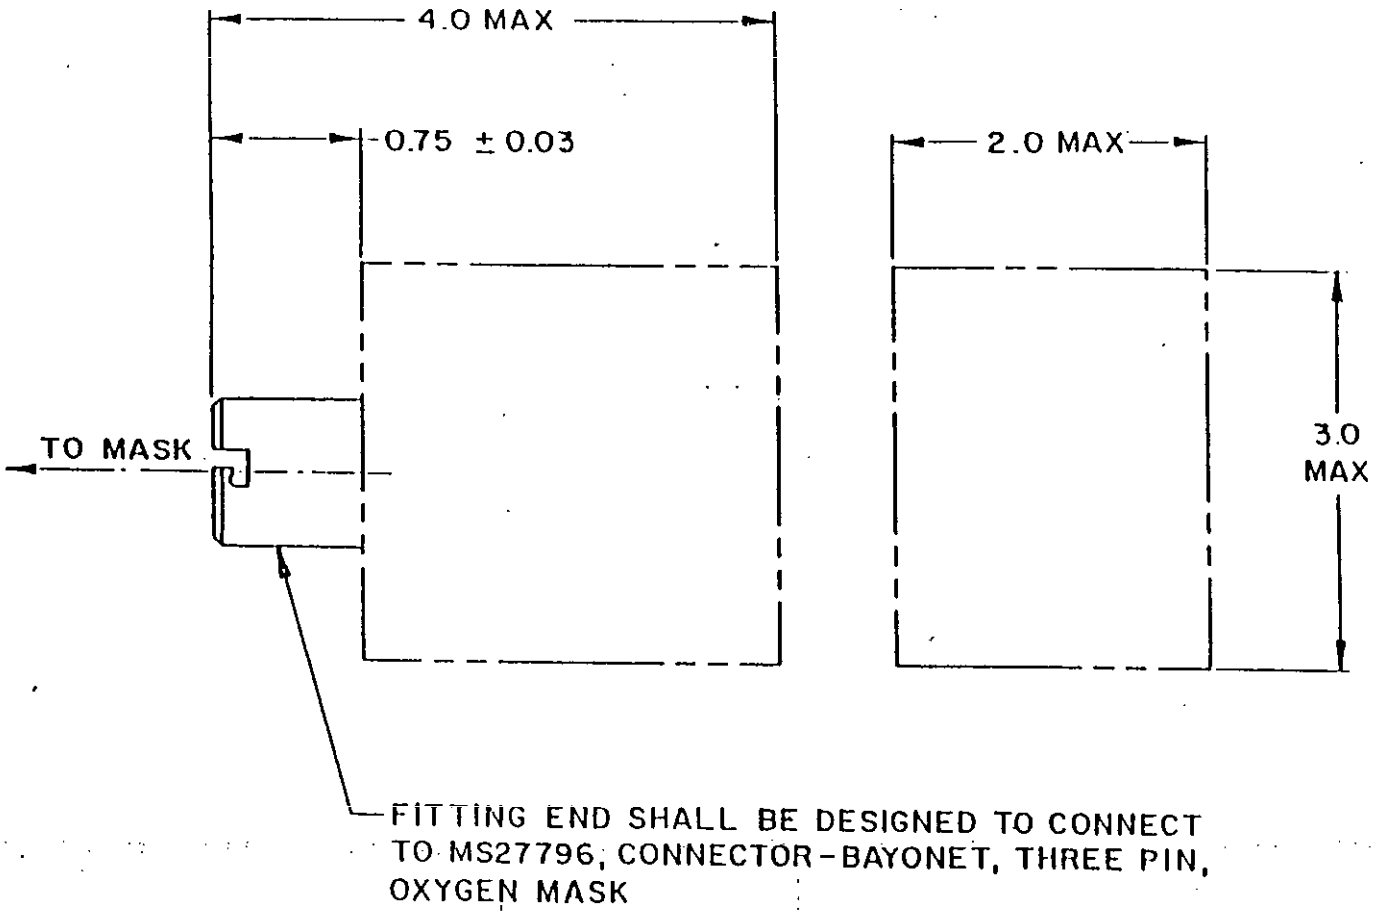

NOTES:

1. Dimensions are in inches.
2. ANPT shall be in accordance with MIL-P-7105.
3. Regulator shall include a 1/8-27 ANPT inlet fitting.
4. Envelope dimensions include all hose connecting parts.

FIGURE 1. Chest mounted regulator (envelope dimensions).

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T00:18Z
Check the source to verify that this is the current version before use.

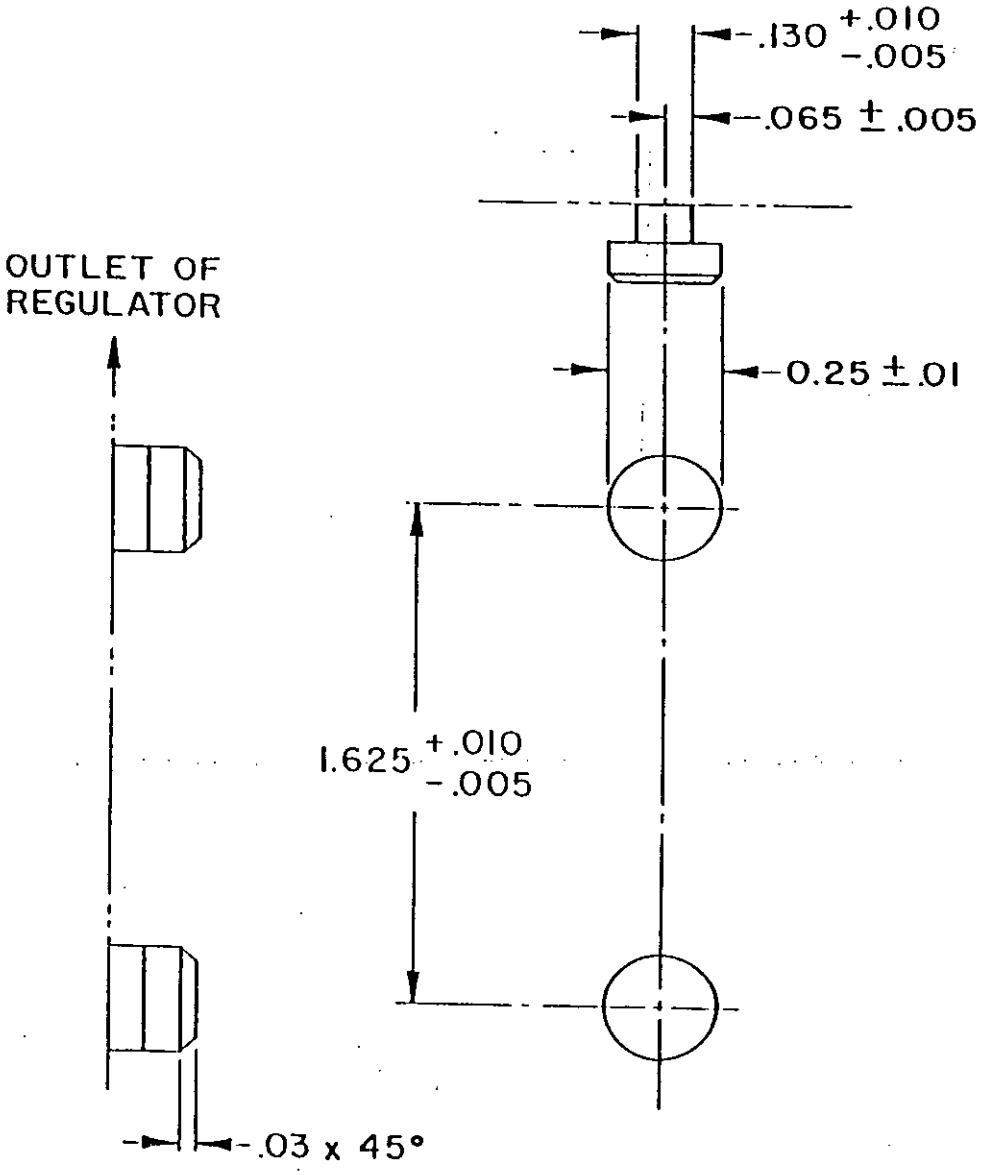


FIGURE 2. Mounting configurations.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T00:18Z
Check the source to verify that this is the current version before use.

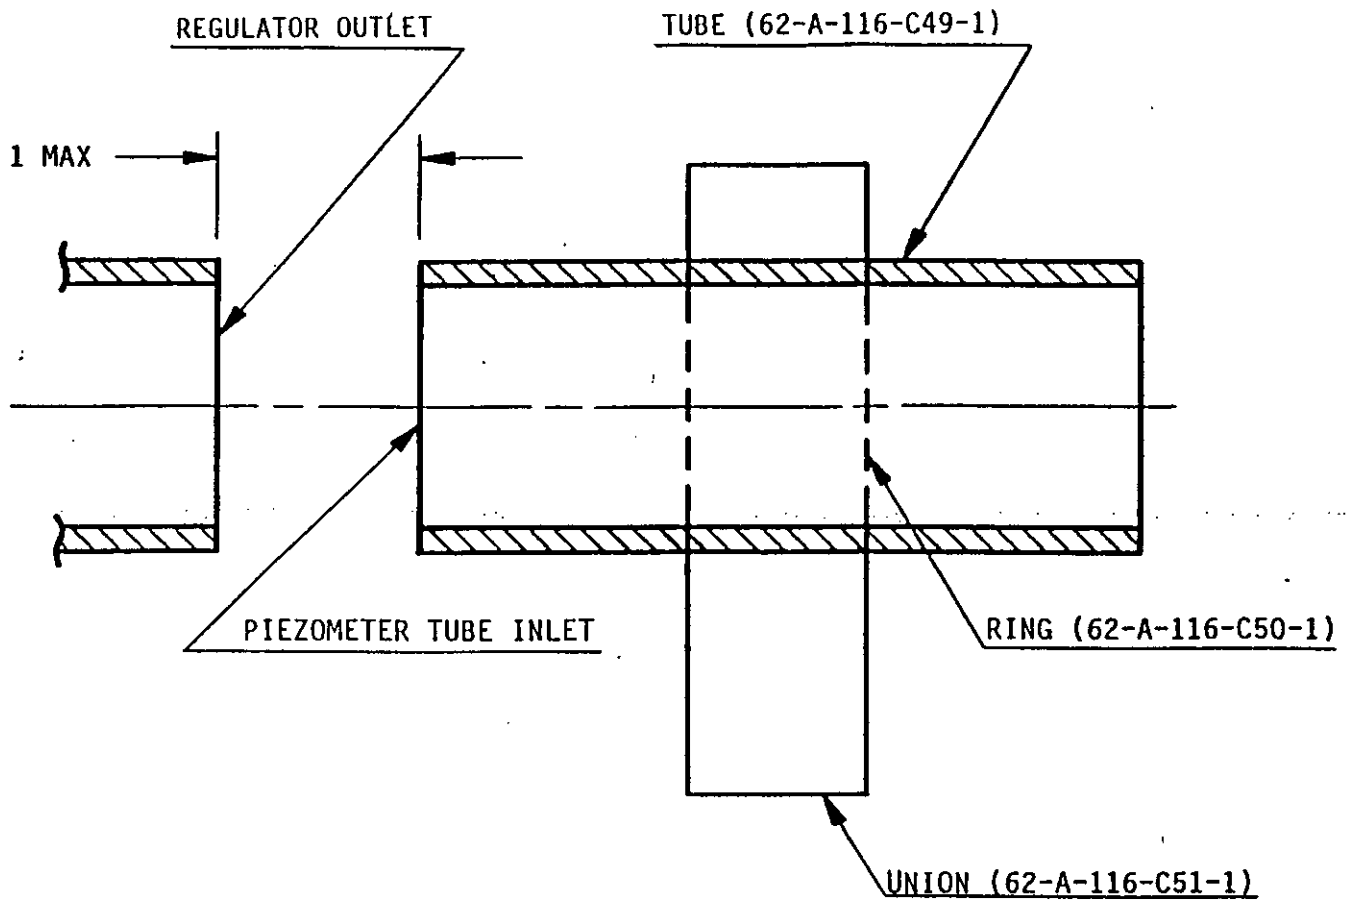


FIGURE 3. Location of Regulator outlet to piezometer (62-A-116-C48)

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T00:18Z
Check the source to verify that this is the current version before use.


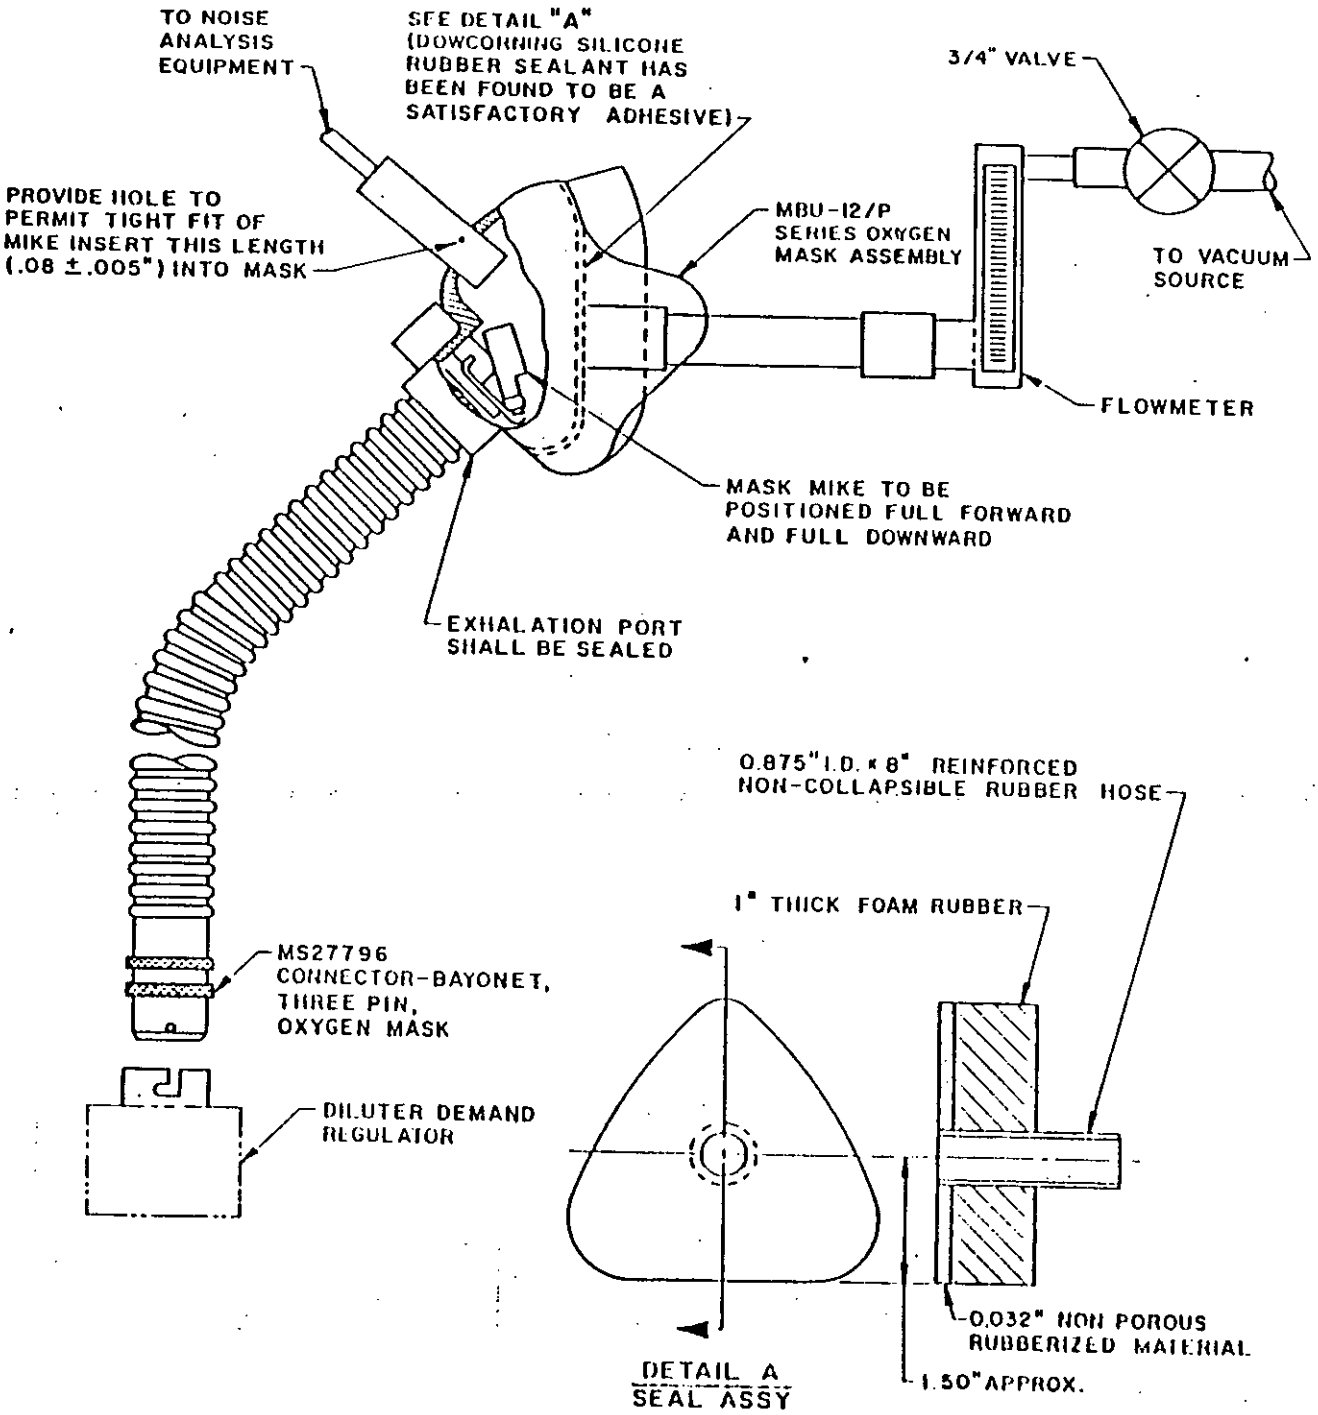


FIGURE 4. Noise level control test set-up.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T00:18Z
Check the source to verify that this is the current version before use.

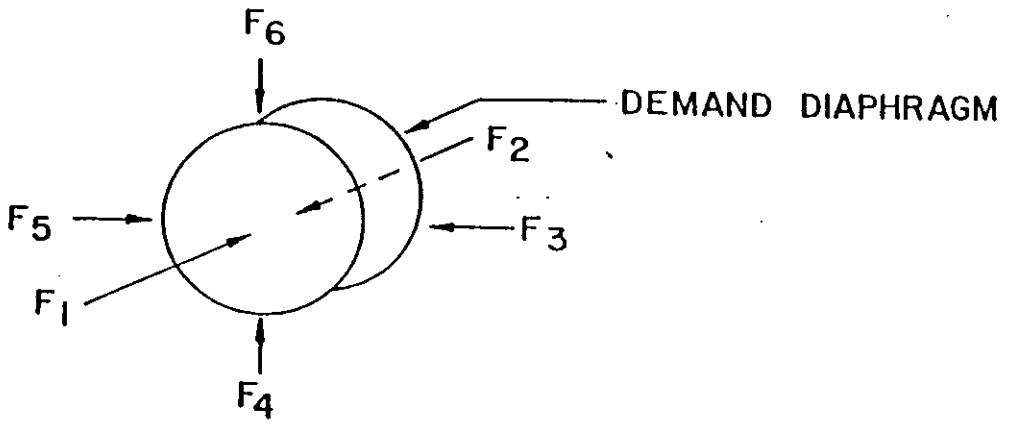

NOTES:

1. F_1 and F_2 are perpendicular to the plane of the demand diaphragm. F_3, F_4, F_5 and F_6 are parellel to the plane of the demand diaphragm.

FIGURE 5. Direction of applied forces.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T00:18Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

INSTRUCTIONS

1. The preparing activity must complete blocks 1, 2, 3, and 8. In block 1, both the document number and revision letter should be given.
2. The submitter of this form must complete blocks 4, 5, 6, and 7.
3. The preparing activity must provide a reply within 30 days from receipt of the form.

NOTE: This form may not be used to request copies of documents, nor to request waivers, or clarification of requirements on current contracts. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements.

I RECOMMEND A CHANGE:	1. DOCUMENT NUMBER	2. DOCUMENT DATE (YYMMDD)
	MIL-R-29585(AS)	91/05/15

3. DOCUMENT TITLE
REGULATOR, OXYGEN, CHEST MOUNTED, DILUTER-DEMAND, AUTOMATIC-PRESSURE BREATHING

4. NATURE OF CHANGE *(Identify paragraph number and include proposed rewrite, if possible. Attach extra sheets as needed.)*

5. REASON FOR RECOMMENDATION

6. SUBMITTER

a. NAME (Last, First, Middle Initial)	b. ORGANIZATION	
c. ADDRESS (Include Zip Code)	d. TELEPHONE (Include Area Code) (1) Commercial (2) AUTOVON (If applicable)	7. DATE SUBMITTED (YYMMDD)

8. PREPARING ACTIVITY

a. NAME	b. TELEPHONE (Include Area Code)	
Commanding Officer Naval Air Engineering Center SESD Code 5312	(1) Commercial (908) 323-1280	(2) AUTOVON 624-1280
c. ADDRESS (Include Zip Code) Lakehurst, NJ 08733-5100	IF YOU DO NOT RECEIVE A REPLY WITHIN 45 DAYS, CONTACT: Defense Quality and Standardization Office 5203 Leesburg Pike, Suite 1403, Falls Church, VA 22041-3466 Telephone (703) 756-2340 AUTOVON 289-2340	

DD Form 1426, OCT 89 — Previous editions are obsolete — 198/290

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T00:18Z
Check the source to verify that this is the current version before use.