MIL-B-36560A
5 December 1975
SUPERSEDING
MIL-B-36560
31 October 1968

MILITARY SPECIFICATION

BASSINET AND DRESSING TABLE COMBINATION, HOSPITAL

This specification is approved for use by all Departments and Agencies of the Department of Defense.

1. SCOPE

1.1 Scope. This specification covers one type of hospital bassinet and dressing table combination, corrosion-resisting steel, suitable for use in military medical facilities for the individual care of the newborn.

2. APPLICABLE DOCUMENTS

2.1 Issues of documents. The following documents of the issue in effect on date of invitation for bids or request for proposal, form a part of the specification to the extent specified herein:

SPECIFICATIONS

Federal

FF-C-77	-	Caster, Institutional Duty.
QQ-S-763	-	Steel Bars, Shapes and Forgings, Corrosion-Resisting.
PPP-B-585	-	Boxes, Wood, Wirebound.
PPP-B-601	-	Boxes, Wood, Cleated Plywood.
PPP-B-621	-	Boxes, Wood, Nailed and Lock Corner.
PPP-B-640	-	Boxes, Fiberboard, Corrugated, Triple-wall.

Military

MIL-L-10547	-	Liners, Case and Sheet, Overwrap; Water-Vaporproof or Waterproof, Flexible.

FSC 6530

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:48Z
Check the source to verify that this is the current version before use.

STANDARDS

Federal

FED-STD-66	-	Steel, Chemical Composition and Hardenability.
FED-STD-151	-	Metals, Test Methods.

Military

MIL-STD-105	-	Sampling Procedures and Tables for Inspection by Attributes.
MIL-STD-129	-	Marking for Shipment and Storage.

(Copies of specifications and standards required by suppliers in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.)

3. REQUIREMENTS

3.1 Material. The materials shall be as hereinafter specified. Materials which are not specifically described herein shall be of the highest quality throughout and suitable in all respects for the purpose intended. Material gages specified shall be considered the minimum acceptable gage. Commercial tolerances shall apply to all gages.

3.1.1 Sheet and tubing. Sheet and tubing shall be corrosion-resisting steel conforming to AISI 302 or 304 of FED-STD-66 when tested as specified in 4.4.1.

3.1.2 Rods. Rods shall be corrosion-resisting steel conforming to class 302 or 304, condition A, of QQ-S-763, when tested as specified in 4.4.1.

3.1.3 Hardware. All metal parts, other than those composed of sheet, tubing, or rods, and not otherwise specified, shall be corrosion-resisting steel, chrome over nickel plated carbon steel, anodized aluminum, bronze, or brass. Bronze or brass shall be plated with chromium over nickel.

3.1.4 Plastic. The basket shall be formed in one piece from a suitable transparent plastic such as methyl-methacrylate or polycarbonate (see 6.3).

Source: https://assist.dla.mil -- Downloaded: 202610-21T08:48Z
Check the source to verify that this is the current version before use.

3.2 Construction. The overall dimensions in the compact configuration shall be not less than 16 inches wide by 33 inches long by 35 inches high, excluding the drawer pull and the basket. The bassinet shall consist of a tubular framework designed to hold a removable plastic basket, a sliding shelf, and a side drawer in a suitably counterweighted cabinet as shown in Figures 1 and 2 or in Figure 3, or a combination thereof. The unit shall move and turn easily when wheeled over a flat surface with the shelf in the closed position.

3.2.1 Carriage frame. The frame shall be constructed of 1 inch diameter by .049 inch, No. 18 Birmingham Wire Gage (BWG), tubing, with 1/2 or 3/4 inch diameter by .049 inch (No. 18 BWG) tubing cross members. The cross tubes shall be joined to the main frame tubes by inserting them in drilled holes in the main frame and tack welding them on the underside, or expanding the cross tubes by insertion of a tapered plug to lock them to the main frame tubes. Clearance shall not exceed .010 inch at any point. As an alternate, the cross tubes shall be fully welded to the main frame tubes. The cross tubes at the top of the stand which prevent the plastic basket from sliding off of the basket support rods shall be at least 2 inches higher than the bottom of the basket. The basket support rod and upper cross-tube configuration shall be designed to provide Trendelenberg and reverse Trendelenberg positions (30^{0} to 40^{0}). The basket support rods shall be 30 inches $\pm$ 1/2 inch above the floor. Two corrosion-resisting steel channels, securely welded to the carriage frame, shall support the inner end of the sliding shelf.

3.2.2 Cabinet. The cabinet shall have overall dimensions of not less than 21-1/2 inches wide by 15 inches deep and 7 inches high and shall be mounted on the stand so that the cabinet bottom surface shall be at least 15 inches above the floor. The cabinet shall be constructed of .0375 inch, No. 20 United States Standard (U.S.S.) gage, corrosion-resisting steel. All outside corners shall be rounded.

3.2.2.1 Drawer. The cabinet shall be equipped with a drawer which shall pull out from the side. The drawer dimensions shall be not less than 20 inches wide by 14 inches deep and 5-1/2 inches high. The drawer front and interior shall be fabricated of .031 inch (No. 22 U.S.S. gage) corrosion-resisting steel sheet with all edges hemmed not less than 1/2 inch or flanged. The drawer front shall be of double pan type construction, filled with sound-deadening material, with all corner joints welded and ground smooth. Suspension for the drawer shall incorporate nylon rollers. A positive stop shall prevent inadvertent removal of the drawer, but the drawer shall be designed so that it may be removed for cleaning purposes. The drawer shall be capable of being opened to a minimum depth of 11 inches and shall close against suitable rubber bumpers. The drawer pull shall be of bronze, brass, corrosion-resisting steel, or anodized aluminum. Where bronze or brass is furnished, it shall be plated with chromium over nickel. The drawer slides and slide extensions shall be fabricated of .0375 inch (No. 20 U.S.S. gage) sheet. Drawer slides and extensions shall be corrosion-resisting steel or plated carbon steel.

Source: https://assist.dla.mil -- Downloaded: 202610-21T08:48Z
Check the source to verify that this is the current version before use.

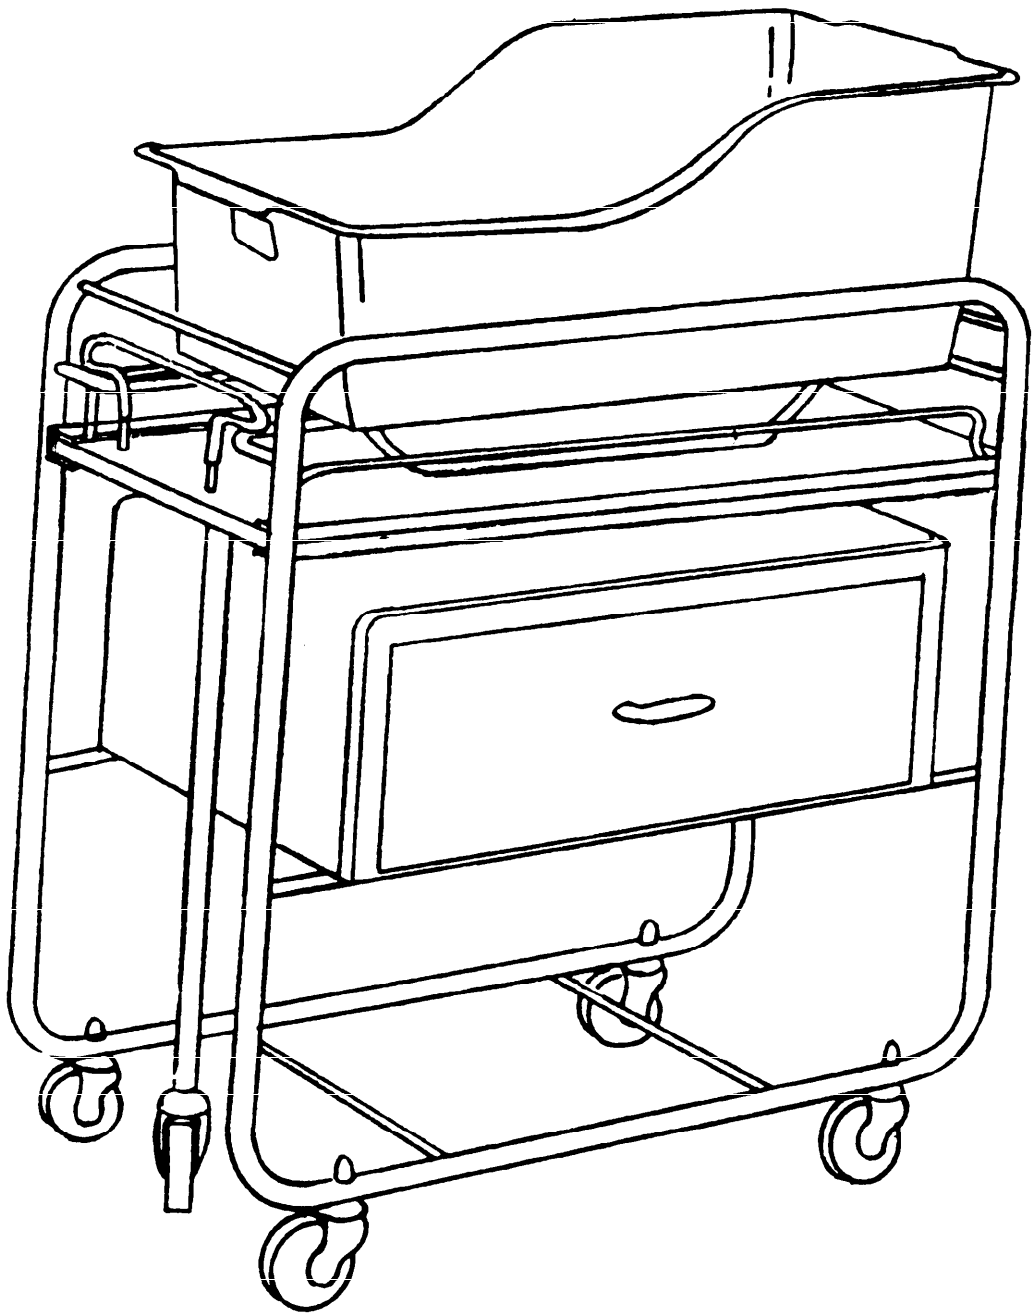


FIGURE 1. Bassinet

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:48Z
Check the source to verify that this is the current version before use.

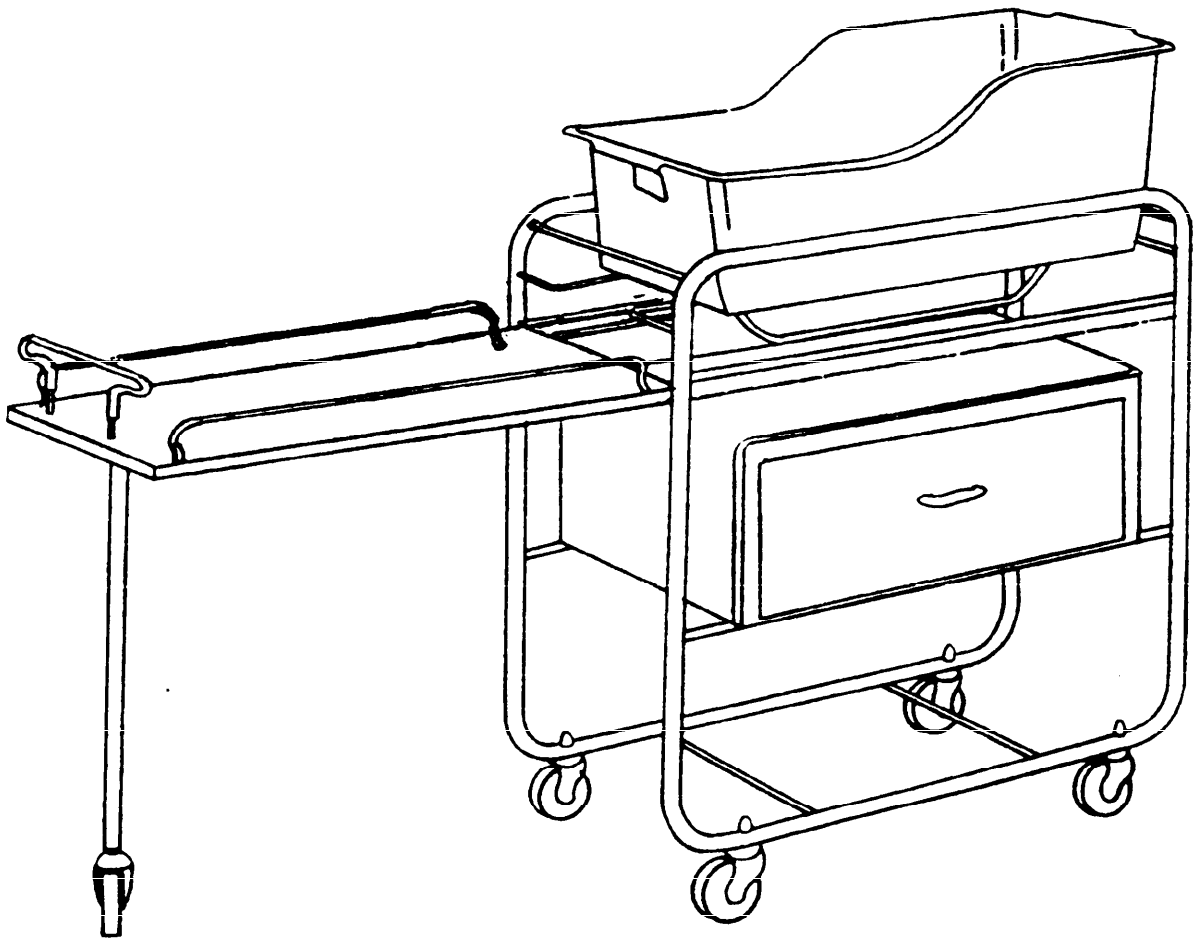


FIGURE 2. Bassinet (with tray extended).

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:48Z
Check the source to verify that this is the current version before use.

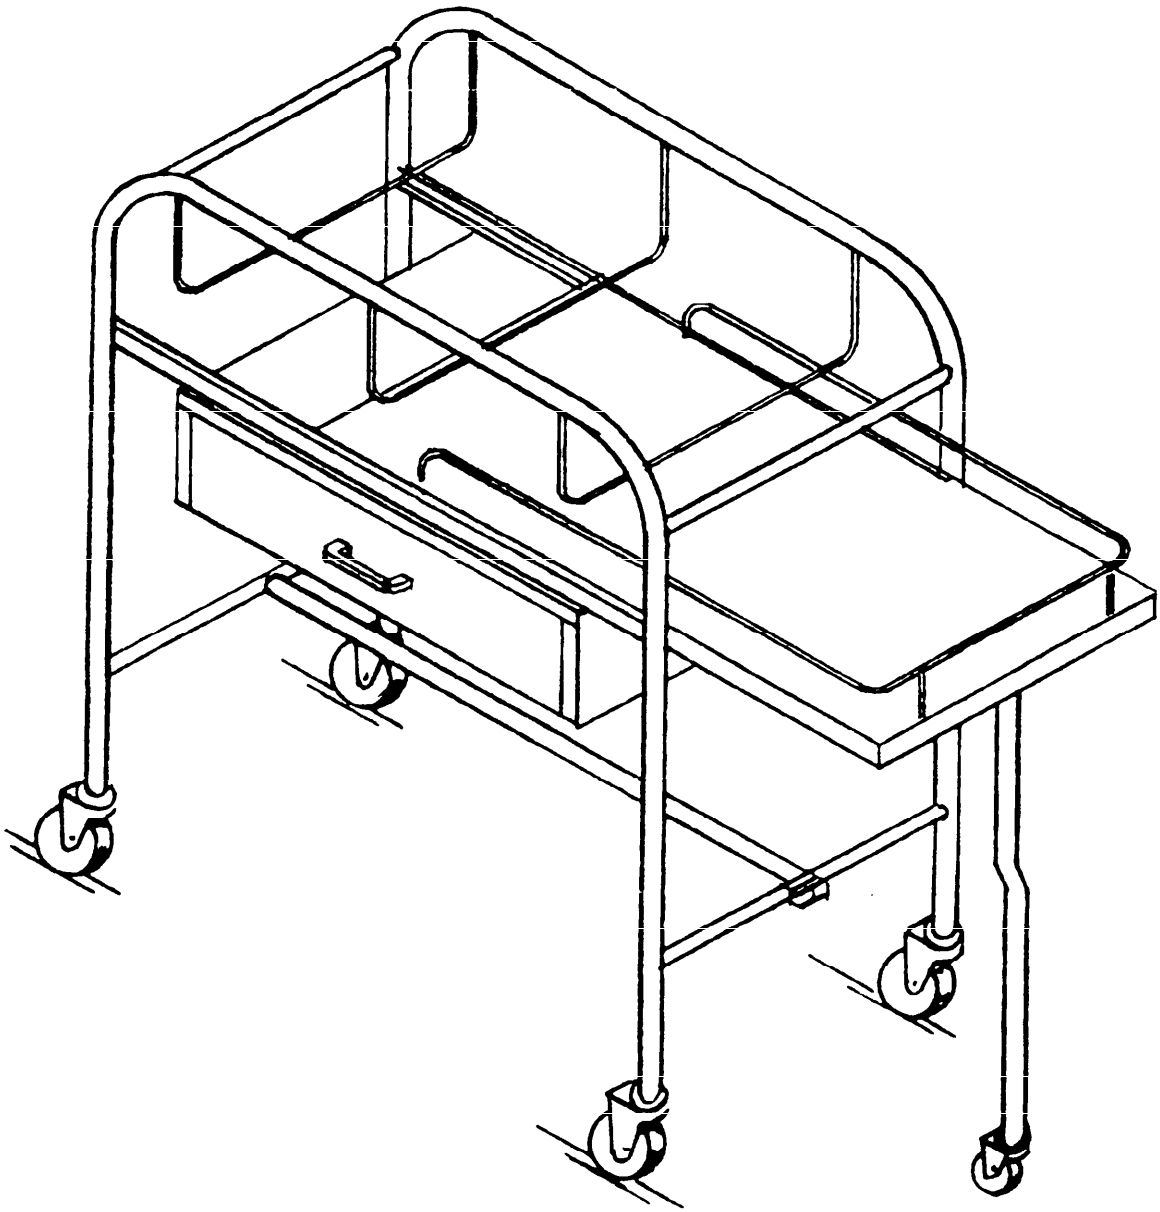


FIGURE 3. **Bassinet**.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:48Z
Check the source to verify that this is the current version before use.

3.2.3 Sliding shelf. The sliding shelf shall be fabricated of .050 inch (No. 18 U.S.S. gage) corrosion-resisting sheet steel formed into an inverted pan with the edges turned down 1 inch and fully hemmed a minimum of 1/2 inch. The hemming shall fit snugly on the underside of the shelf so that no openings or rough edges shall be present. The inner end of the shelf shall be supported by two slide blocks or rollers, fabricated of nylon, securely bolted to the shelf, which shall slide smoothly inside the support channels on the carriage frame. The outer end of the shelf shall be supported by a 1 inch, .049 wall thickness (No. 18 BWG) corrosion-resisting steel tube. The support tube shall be suitably reinforced so that it shall support the end of the shelf firmly in the open position and shall exhibit no bending or looseness after being tested as specified in 4.4.2. The support tube shall be equipped with a caster. The shelf shall lock securely in the closed position until intentionally released. The shelf shall also be held firmly in place in the open position. A shelf lock mounted on the shelf slide channel shall be acceptable. After being tested as specified in 4.4.2, the shelf shall lock securely in the closed position and be held firmly in place in the open position. The shelf shall have a guard rail on 3 sides fabricated of 1/4 inch corrosion-resisting steel rod. The guard rail shall be a minimum of 2 inches above the shelf. The top of the shelf shall be located 27 + 1/2 inches above the floor. The corners of the sliding shelf shall be filled with welding material and ground smooth. The shelf shall be not less than 14 inches wide by 29 inches long. The shelf shall extend at least 25 inches from the main frame in the open position. The shelf shall exhibit no binding or looseness after being tested as specified in 4.4.2.

3.2.4 Casters. The casters on the stand shall conform to Type II, Class B, wheel diameter 3 inches, Style b, Mounting A or T of FF-C-77. The caster on the sliding shelf support leg shall be 2 inches in diameter, ball bearing swivel type, for light duty with a soft tread composition wheel. If casters are bolted to the frame, acorn nuts shall be used.

3.2.5 Bassinet basket. The basket shall be formed in one piece of transparent plastic with intergrally molded handles on each end and shall have a vented bottom. The basket shall incorporate an identification card holder. The basket shall be intended for use with a bassinet mattress with dimensions of 27 inches long, by 13 inches wide. When tested for load as specified in 4.4.3, the basket shall suffer no permanent deformation nor any temporary deformation greater than 2 inches. When drop tested as specified in 4.4.4, the basket shall suffer no damage. Minor surface scuffs or scratches caused by the drop test shall not be cause for rejection.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:48Z
Check the source to verify that this is the current version before use.

3.3 Finish. All exposed welds, including all tubing welds, shall be ground smooth and polished to match the finish of the adjacent metal. The cabinet and drawer shall have a number 4 commercial finish. All corrosion-resisting steel tubing shall have a number 4 finish or better. All non-exposed welds shall be cleaned of flux and slag and finished with silver enamel.

3.4 Identification marking. Each bassinet shall be legibly marked with the contract or purchase order number.

3.5 Service Data. The contractor shall furnish, with each unit, two copies each of a technical manual which contains complete instructions for assembly, operation, cleaning, and maintenance and lists of component parts.

3.6 Welding. Welding shall be durable, sound in every detail and in accordance with latest practices recommended by the American Welding Society. All welds shall be produced by certified welding operators with satisfactory welding equipment using satisfactory filler metal and/or electrode where applicable to provide the best possible weld. Surfaces to be welded shall be free from grease, oil, oxides or any other foreign matter. Any cleaning method which will remove these substances and leave the surface clean is satisfactory. All weld joints shall blend into the adjacent metal in gradual, smooth curves. Beads shall be smooth and free of slag, excessive undercut, or excessive spatter. Sufficient metal shall be added to provide a suitable fillet or reinforcement unless otherwise specified. Welds shall not be oxidized. All welds shall be continuous with no visible voids, pin holes, or cracks which affect the quality, and shall have more strength than required for purpose intended.

3.7 Workmanship. Workmanship shall be first class throughout. The bassinets shall be free from defects which detract from their appearance or may impair their serviceability. Exposed metal surfaces shall be free of burs and sharp edges. Basket shall be free of rough surface, sharp edges, and flash.

4. QUALITY ASSURANCE PROVISIONS

4.1 Responsibility for inspection. Unless otherwise specified in the contract, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract, the contractor may use his own or any other facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:48Z
Check the source to verify that this is the current version before use.

4.1.1 Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government, upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of 3 years after delivery of the supplies to which such records relate.

4.1.2 Inspection. Inspection, as used in this specification, is defined as both examination (such as visual and auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

4.1.3 Certificates of quality. Certificates of quality, supplied by the manufacturer of the component or material, may be furnished in lieu of actual performance of such testing by the contractor, provided lot identity has been maintained and can be demonstrated to the Government. The Certificate shall include the name of the contractor, the contract number, the name of the manufacturer or supplier, the NSN, the Item Identification, the name of the component/material, the lot number, the lot size, the sample size, the date of testing, the test method, individual test results, and the specification requirements.

4.2 Sampling.

4.2.1 For examination. Sampling for examination shall be conducted in accordance with MIL-STD-105 and table I.

TABLE I. Sampling for examination.

	Inspection level	AQL (percent defective)
For visual examination		
Major defects	II	1.0
Total (major and minor combined)	II	4.0
For dimensional examination	S-3	2.5

4.2.2 For tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and table II. Acceptance number shall be zero for all sample sizes.

TABLE II. Sampling for tests.

Component	Characteristic	Requirement	Test procedure	Inspection level
Bassinet	Sliding action	3.2.3	4.4.2	S-2
Basket	Load strength	3.2.5	4.4.3	S-2
	Drop strength	3.2.5	4.4.4	S-2

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:48Z
Check the source to verify that this is the current version before use.

4.2.2.1 A sufficient quantity of each lot of metal used in the manufacture of the bassinet and dressing table shall be selected for composition analysis in accordance with 4.4.1.

4.3 Examination. The bassinet shall be examined to determine compliance with all requirements contained in this specification.

4.3.1 Classification of defects. Examination shall be conducted in accordance with the classification of defects listed in table III. Examination shall not be restricted to the classified possible defects listed below.

TABLE III. Classification of defects.

Categories	Defects
Major:	
101	Bassinet and dressing table combination not complete.
102	Edges and corners of component parts not free of burrs or sharpness.
103	Cabinet drawer or shelf fail to properly retract or extend from the frame of the carriage.
104	Unit fails to move and turn easily and smoothly when wheeled over a flat surface.
105	Component parts not free of cracks or ruptures.
106	Component parts in assembly not properly fitted, not securely fastened.
107	Welds not free of pits, cracks, burns, and undercutting.
108	Finish not as specified.
Minor:	
201	Surfaces of bassinet and dressing table combination not free of scratches or mars.
202	Service data missing or incomplete.
203	Identification marking not present, incomplete, or illegible.

4.3.2 Dimensional examinations. The bassinet shall be examined for defects in dimensions. Any dimension not within the tolerances specified herein shall be classified as a defect.

4.4 Tests. Tests shall be conducted to determine compliance with specification requirements.

4.4.1 Composition analysis. Tests for composition analysis shall be conducted in accordance with method 111 or 112 of FED-STD-151.

4.4.2 Shelf sliding - action test. With the bassinet on a smooth, level floor surface, the shelf shall be slid alternately into the fully-extended position and the fully-closed position for 50 complete cycles.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:48Z
Check the source to verify that this is the current version before use.

4.4.3 Basket load test. A weight of 50 pounds shall be placed in the basket. The basket shall then be lifted by the handles and held for a period of 30 seconds, supported by the handles only.

4.4.4 Basket drop test. The basket shall be dropped from a height of 24 inches onto a hard floor surface so that the point of impact shall be a bottom corner.

4.5 Examination of preparation for delivery. An examination shall be made to determine whether the packaging, packing, and marking comply with the requirements of section 5. Defects shall be scored as specified in table IV. Sampling shall be in accordance with MIL-STD-105. The sample unit shall be one container fully prepared for delivery. The lot shall be the number of containers offered for inspection at one time. The inspection level shall be S-2 and the acceptable quality level shall be 4.0 defects per hundred units.

TABLE IV. Examination of preparation for delivery.

Examination	Defects
Containers	Not as specified.
Quantity	Quantity in interior package and shipping containers not as specified.
Materials	Any component missing or damaged.
Workmanship	Inadequate application of components such as incomplete closure of container flaps, tape improperly applied, or containers distorted.
Markings	Omitted, incorrect, illegible, improper size, location, sequence, or method of application.

5. PACKAGING.

5.1 Packaging. Packaging shall be level A or C as specified (see 6.2).

5.1.1 Level A.

5.1.1.1 Unit preparation. Casters shall be removed, packaged in a bag of suitable size and design, and secured to the unit. The sliding shelf and the drawer front shall be secured to the frame. The entire unit shall be wrapped with non-corrosive paper. Wrapper shall be secured with tape. The unit shall be so wrapped as to prevent marring or abrasion of polished surfaces during transit and storage.

5.1.2 Level C. Unit shall be packaged in standard commercial containers of the size and kind commonly used, which will afford the degree of protection required for shipment and use of the product for its intended purpose.

Source: https://assist.dla.mil -- Downloaded: 202610-21T08:48Z
Check the source to verify that this is the currentversion before use.

5.2 Packing. Packing shall be level A, B, or C as specified (see 6.2).

5.2.1 Level A. Each unit shall be overboxed in an exterior container designed for a type 3 load and constructed in accordance with PPP-B-585, class 3, style 3; PPP-B-601, overseas type; PPP-B-621, class 2; or PPP-B-640, class 2, style E. Container shall be designed with suitable interior fittings or shall contain sufficient cushioning material to prevent shifting of or damage to the unit. Closure and strapping shall be as specified in the applicable box specification.

5.2.1.1 Case liner. Each level A wood box shall be lined with a waterproof case liner conforming to MIL-L-10547. Closure and sealing shall conform to applicable paragraphs of appendix thereto. Case liner shall not be required for fiberboard boxes. Each fiberboard box shall be sealed as specified in PPP-B-640.

5.2.2 Level B. Each unit shall be overboxed in an exterior container designed for a type 3 load and constructed in accordance with PPP-B-585, class 1, style 3; PPP-B-601, domestic type; PPP-B-621, class 1; or PPP-B-640, class 2, style E. Container shall be designed with suitable interior fittings or shall contain sufficient cushioning material to insure against shifting of or damage to the contents. Closure shall be as specified in the applicable box specification.

5.2.3 Level C. The subject commodity shall be packed in substantial commercial containers of the type, size, and kind commonly used for the purpose, so constructed as to insure acceptance and safe delivery by common or other carriers, at the lowest rate, to point of delivery called for in the contract or purchase order.

5.3 Marking.

5.3.1 Exterior container. Each exterior container shall be marked in accordance with MIL-STD-129.

6. NOTES

6.1 Intended use. The bassinet and dressing table shall be suitable for use in military medical facilities for the individual care of the newborn. The bassinet and dressing table shall be used with Mattress, Hospital Bassinet having National Stock Number (NSN) 6530-00-726-0459.

6.2 Ordering data. Procurement documents should specify the following:

a. Title, number, and date of this specification.
b. Selection of applicable levels of packaging and packing (see 5.1 and 5.2).

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:48Z
Check the source to verify that this is the current version before use.

6.3 Methyl-methacrylate specified in 3.1.4 is commonly known as Lucite. Polycarbonate specified in 3.1.4 is commonly known as Lexan.

6.4 This specification covers the following item appearing in the Federal Supply Catalog:

National Stock Number	Item Identification
6530-00-935-6590	BASSINET AND DRESSING TABLE COMBINATION, HOSPITAL, Corrosion-Resisting Steel, 33 by 16 by 35 inches.

6.5 Changes from previous issue. Asterisks are not used in this revision to identify changes with respect to the previous issue, due to the extensiveness of the changes.

Custodians:
Army - MD
Navy - MS
Air Force - 03

Preparing activity:
Defense Supply Agency - DSA-DM

Project No. 6530-1352
cs

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:48Z
Check the source to verify that this is the current version before use.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:48Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

OMB Approval
No. 22-R255

INSTRUCTIONS: The purpose of this form is to solicit beneficial comments which will help achieve procurement of suitable products at reasonable cost and minimum delay, or will otherwise enhance use of the document. DoD contractors, government activities, or manufacturers/vendors who are prospective suppliers of the product are invited to submit comments to the government. Fold on lines on reverse side, staple in corner, and send to preparing activity. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements. Attach any pertinent data which may be of use in improving this document. If there are additional papers, attach to form and place both in an envelope addressed to preparing activity.

DOCUMENT IDENTIFIER AND TITLE

MIL-B-36560A BASSINET AND DRESSING TABLE, COMBINATION, HOSPITAL

NAME OF ORGANIZATION AND ADDRESS

CONTRACT NUMBER

MATERIAL PROCURED UNDER A

☐ DIRECT GOVERNMENT CONTRACT ☐ SUBCONTRACT

1. HAS ANY PART OF THE DOCUMENT CREATED PROBLEMS OR REQUIRED INTERPRETATION IN PROCUREMENT USE?

A. GIVE PARAGRAPH NUMBER AND WORDING.

B. RECOMMENDATIONS FOR CORRECTING THE DEFICIENCIES

2. COMMENTS ON ANY DOCUMENT REQUIREMENT CONSIDERED TOO RIGID

3. IS THE DOCUMENT RESTRICTIVE?

☐ YES ☐ NO *(If "Yes", in what way?)*

4. REMARKS

SUBMITTED BY *(Printed or typed name and address - Optional)*

TELEPHONE NO.

DATE

DD FORM 1 JAN 72 1426

REPLACES EDITION OF 1 JAN 69 WHICH MAY BE USED

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:48Z
Check the source to verify that this is the current version before use.

FOLD

DEFENSE PERSONNEL SUPPORT CENTER
2800 South 20th Street
Philadelphia, PA. 19101

POSTAGE AND FEES PAID
DEFENSE SUPPLY AGENCY
DoD - 304

OFFICIAL BUSINESS
PENALTY FOR PRIVATE USE $300

HEADQUARTERS, DEFENSE PERSONNEL SUPPORT CENTER
ATTN: DIRECTORATE OF MEDICAL MATERIEL, CODE ATT
2800 SOUTH 20TH STREET
PHILADELPHIA, PA 19101

FOLD

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:48Z
Check the source to verify that this is the current version before use.