MIL-C-36583A
18 August 1976
SUPERSEDING
MIL-C-36583
4 August 1969

MILITARY SPECIFICATION

CATHETERS, URETHRAL, PLASTIC, DISPOSABLE, ROUND TIP, ROBINSON-NELATON

This specification is approved for use by all Departments and Agencies of the Department of Defense.

1. SCOPE

1.1 Scope. This specification covers sterile, disposable, plastic, urethral catheters of the Robinson-Nelaton design suitable for introduction into the human bladder through the urethra for the withdrawal of urine.

1.2 Classification. Catheters covered by this specification shall be of the following sizes, as specified (see 6.1):

Size 8	- 8 French (Fr.)
Size 10	- 10 Fr.
Size 12	- 12 Fr.
Size 14	- 14 Fr.
Size 16	- 16 Fr.
Size 18	- 18 Fr.

2. APPLICABLE DOCUMENTS

2.1 The following documents, of the issue in effect on date of invitation for bids or request for proposal, form a part of this specification to the extent specified herein:

Beneficial comments (recommendations, additions, deletions) and any pertient data which may be of use in improving this document should be addressed to: HQ, Defense Personnel Support Center, ATTN: Directorate of Medical Materiel, DPSC-ATT, 2800 South 20th Street, Philadelphia, PA 19101, by using the self-addressed Standardization Document Improvement Proposal (DD Form 1426) appearing at the end of this document, or by letter.

FSC 6515

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:51Z
Check the source to verify that this is the current version before use.

SPECIFICATIONS

FEDERAL

MMM-A-250	- Adhesive, Water-resistant, (For Sealing Fiberboard Boxes).
PPP-B-636	- Box, Shipping, Fiberboard.
PPP-T-76	- Tape, Pressure-Sensitive, Adhesive Paper, Water-Resistant, (For Carton Sealing).

SPECIFICATIONS

MILITARY

MIL-P-116	- Preservation, Methods of.
MIL-S-36586	- Sterilization Strip Test, Bacterial spore.

STANDARDS

MILITARY

MIL-STD-105	- Sampling Procedures and Tables for Inspection by Attributes.
MIL-STD-129	- Marking for Shipment and Storage.

(Copies of specifications, standards, and publications required by contractors in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.)

2.2 Other publications. The following documents form a part of this specification to the extent specified herein. Unless otherwise indicated, the issue in effect on date of invitation for bids or request for proposal shall apply.

UNITED STATES PHARMACOPEIAL CONVENTION, INC.

The Pharmacopeia of the United States of America (USP)

(Applications for copies should be addressed to the Mack Publishing Company, Easton, PA 18042.)

AMERICAN SOCIETY FOR TESTING AND MATERIALS (ASTM) STANDARDS

D 412 Tension Testing for Vulcanized Rubber

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:51Z
Check the source to verify that this is the current version before use.

(Application for copies should be addressed to the American Society for Testing and Materials, 1916 Race Street, Philadelphia, PA 19103).

3. REQUIREMENTS

3.1 Material. The catheters shall be fabricated from flexible, medical-grade polyvinyl chloride appropriately balanced to provide the proper degree of pliability, softness, and body to withstand the pressure of introduction into the bladder without trauma or irritation to body tissues. The plastic tubing shall meet the requirements for Class IV plastic as stated in the current Unites States Pharmacopeia (USP), when tested as specified in 4.5.1. The plastic shall contain not more than 5 parts per million (ppm) of lead, when tested as specified in 4.5.2 or alternatively, 4.5.3.

3.2 Style and design. Shall be a flexible urethral catheter of the Robinson-Nelaton design suitable for introduction into the human bladder through the urethra for withdrawal of urine. It shall have a nominal overall length of 16 inches with a rounded distal tip which may have a dimple at the tip end not exceeding .025 inch in diameter. Unless otherwise specified, the junction end shall be funnel shaped.

3.2.1 Configuration and dimensions. The configuration and dimensions of the catheter shall be in accordance with figure 1.

3.2.2 Eyes. The eyes through the wall of the catheter tube shall not overlap, and shall be staggered axially near the closed end be and be diametrically opposed to each other.

3.2.3 Color. Unless otherwise specified, the catheter shall be brick red in color.

3.3 Physical properties.

3.3.1 Breaking strength. The breaking strength of the catheters shall be as specified in table I for the appropriate size, when tested as specified in 4.5.4.

TABLE I. Breaking force

Size	8	10	12	14	16	18
Breaking strength (lb.) min.	5.0	12.0	18.0	24.0	30.0	36.0

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:51Z
Check the source to verify that this is the current version before use.

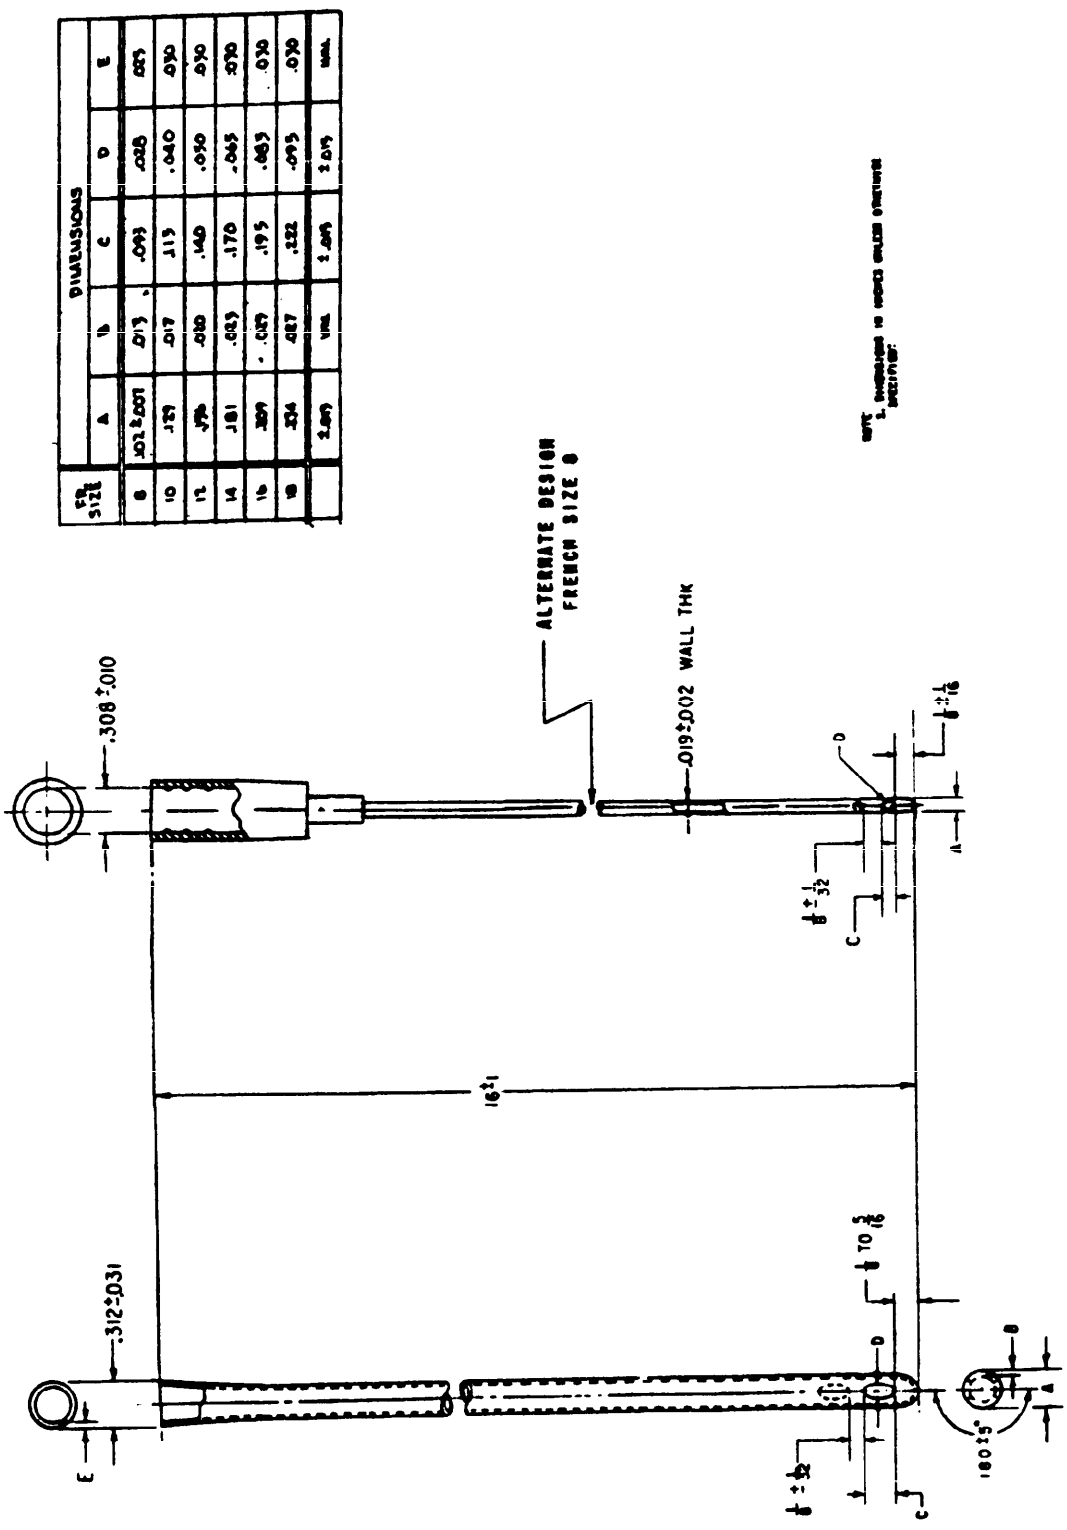


FIGURE 1. Catheter, Urethral, Plastic, Disposable, Round Tip, Robinson-Nelaton

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:51Z
Check the source to verify that this is the current version before use.

3.3.2 Elongation. The elongation of the catheters shall be 175 percent minimum, when tested as specified in 4.5.4.

3.4 Sterility. The catheters shall be sterile, when tested with a biological indicator as specified in 4.5.5.

3.4.1 Certificate of sterility. A certificate of sterility, stating that samples from each sterilizer lot have been tested and found to be sterile, shall be submitted to the procuring activity. The certificate of sterility shall include:

a. Item identification.
b. National stock number.
c. Contract or purchase order number.
d. Sterility lot or control number.
e. Date of sterilization.
f. Quantity of product in sterilizer lot.
g. Type of sterilization (gas, radiation, heat, steam, etc.).
h. Form of biological indicator (i.e., inoculated paper spore strip or carrier, inoculated product, or inoculated simulated product).
i. Test organism(s) and population density used.
j. Test medium, incubation temperature, incubation time, and dates of tests.
k. Number of test units.
l. Statement that samples comply with sterility tests.
m. Signature of head of laboratory or a designated qualified alternate.

When inspection is made at destination, the certificate of sterility shall be submitted by the contractor to the Directorate of Medical Materiel, ATTN: DPSC-ATQ Defense Personnel Support Center, 2800 South 20th Stree, Philadelphia, PA 19101, and a copy forwarded with each shipment to the consignee. When inspection is made at source, certificate of sterility shall be furnished to the cognizant Government Quality Assurance Representative for submission to the procuring activity.

3.4.2 Sterility lot. A sterility lot is that single quantity of product subjected to the same sterilizer chamber. Each unit package shall be clearly marked with a sterility lot (control) number and date of sterilization as specified in 5.3.1. Each sterility lot shall be traceable to the pertinent manufacturing lot(s).

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:51Z
Check the source to verify that this is the current version before use.

3.5 Manufacturer's record. The manufacturer shall place a code or lot number on the paper label, which can be verified against the manufacturer's records of all sterility and biological tests performed on the catheters. These records shall be made available for inspection by any duly authorized Government representative. No shipment shall be made until all tests have been completed, verified, and recorded in the permanent records of the manufacturer.

3.6 Workmanship. Workmanship shall be first class throughout. The finished catheters shall be symmetrical in shape, shall have a smoothly finished surface, and shall be free from irregularities or imperfections of any kind which detract from their appearance or which may impair their serviceability.

4. QUALITY ASSURANCE PROVISIONS

4.1 Responsibility for inspection. Unless otherwise specified in the contract, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract, the contractor may use his own or any other facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

4.1.1 Records. Records of examination and tests performed by or for the contractor shall be maintaned by the contractor and made available to the Government, upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of 3 years after delivery of the supplies to which such records relate.

4.1.2 Inspection. Inspection, as used in this specification, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

4.1.3 Certificates of quality. Certificates of quality supplied by the manufacturer of the catheters may be furnished in lieu of actural performance of such testing by the contractor, provided lot identity has been maintained and can be demonstrated to the Government. The certificate shall include the name of the contractor, the contract number, the name of the manufacturer or the component/material, the lot number, the lot size, the sample size, the date of testing, the test method, individual test results, and the specification requirements.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:51Z
Check the source to verify that this is the current version before use.

4.2 Sampling.

4.2.1 Inspection lot. The inspection lot shall be determined in accordance with MIL-STD-105.

4.2.2 Preparation for delivery. The inspection lot size shall be expressed in units of one fully prepared shipping container, containing catheters fully prepared for delivery and made from essentially the same materials and components. The sample unit shall be one fully prepared shipping container, containing instruments fully prepared for delivery, with the exception that it need not be sealed. The inspection shall be inspection Level S-2 and the Acceptable Quality Level shall be 4.0 percent defective in accordance with MIL-STD-105.

4.2.3 Sampling for visual and dimensional examination. A random sample of instruments shall be selected from each lot offered to the Government in accordance with MIL-STD-105. The Acceptable Quality Levels (AQL) shall be as indicated in table II. The unit of product shall be one forceps..

TABLE II Sampling for examination

Type of defect	Inspection level	AQL (percent defective)
Major A	II	1.0
Major B	S-4	1.0
Minor A	II	4.0
Minor B	S-2	4.0

4.2.4 For tests. Sampling for tests shall be conducted in accordance with MIL-STD-105, and as indicated in table III. Where feasible, the same sample shall be used for the determination of two or more tests characteristics. The unit of product for tests shall be one catheter.

TABLE III. Sampling for tests

Component (unit of product)	Characteristic	Requirement	Test procedure	Insp. level	AQL (percent defective)
1-catheter	Material-Class IV plastic	3.1	4.5.1.1 4.5.2 or 4.5.3	2/	
	Breaking strength	3.3.1	4.5.4	S-2	1/

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:51Z
Check the source to verify that this is the current version before use.

TABLE III. Sampling for tests (continued)

Component (unit of product)	Characteristic	Requirement	Test procedure	Insp. level	AQL (percent defective)
	Elongation	3.3.2	4.5.4	S-2	
	Sterility	3.4	4.5.5	S-2 3/	1/

1/ Acceptance number shall be zero for all sample sizes.
2/ Sufficient samples to perform the biological tests shall be selected from each lot.
3/ A minimum of ten samples shall be selected from each lot.

4.2.5 Raw material. Ten grams of each lot of plastic used in the fabrication of the catheters shall be selected for the lead test.

4.3 Examination for visual and dimensional defects. The instrument shall be examined to determine compliance with all requirements contained in this specification. Examination shall be conducted as specified in tables II and IV. Examination however, shall not be restricted to defects listed in table IV. Any in the sample containing one or more defects shall be rejected and if the number of defective instruments in any sample exceeds the acceptance number for that sample, the lot represented by the sample shall rejected.

TABLE IV. Classification of defects

Categories	Defects
Critical	None defined.
Major A	
101	Catheter not free of bloom or tackiness.
102	Inside of catheter not free of obstructing material.
103	Two eyes not staggered on opposite sides of tube wall.
104	Catheter not free of kinks.
105	Color not as specified.
Major B	
151	Angular dimension between eyes not as specified.
152	Axial dimension between eyes not as specified.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:51Z
Check the source to verify that this is the current version before use.

TABLE IV. Classification of defects (continued)

Categories	Defects
Critical	None defined.
Minor A	
201	Catheter not free of discoloration.
202	Catheter not free of pits, blisters, scratches, or crazing.
203	Catheter eye not smooth and free of flash.
Minor B	
251	Physical dimensions other than eye location not as specified.

4.4 Packaging inspection. The inspection of the preservation-packaging and interior package marking shall be in accordance with the group A and B quality conformance inspection requirements of MIL-P-116. The inspection of the packing and marking for shipment and storage shall be in accordance with the quality assurance provisions of the applicable container specification and the marking requirements of MIL-STD-129.

4.5 Tests. Tests shall be conducted to determine compliance with specification requirements.

4.5.1 Biological tests. The catheters shall be tested in accordance with the requirements of the current edition of the USP for class IV plastic.

4.5.1.1 Animal implantation test. Samples of the catheters shall be tested in accordance with the method given in the current edition of the USP for Implantation Test for class IV plastic, except for the changes which follows: Last paragraph, second line, after "72 hours" add "and not to exceed 144 hours". Last paragraph, third and fourth sentences, delete entirely and substitute: "The tissues surrounding the implants shall be examined, both grossly and microscopically, by a pathologist certified by the American Board of Pathology or the American College of Veterinary Pathologists."

4.5.2 Test for lead. Ten grams of plastic shall be taken, ignited to char, and then further ignited in a muffler at 700° C. to a white ash. The ash shall be boiled in 15 milliliters (ml) of 10 percent by volume of concentrated nitric acid (specific gravity of 1.4, chemically pure or analytical reagent grade), filtered into a volumetric flask and made up to 100 ml. An aliquot

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:51Z
Check the source to verify that this is the current version before use.

portion, equivalent to one gram of sample, shall be taken and placed in a separator. The dithizone test for lead, as given in the current edition of the Pharmacopeia of the Unites States, shall be applied using a control of 5 ppm or 12 ppm of lead solution as given in the USP test. If the sample solution is darker than the limit, smaller aliquots shall be used until the color of the control is matched by the sample solution and the concentration of lead in ppm is determined.

4.5.3 Alternate test for lead. Accurately weigh a 5-gram sample into a 1-oz. Vycor crucible. Reduce to ash in a muffle furnace at 650°C for eight hours. Let cool to room temperature and add 15 ml of 1:1 hydrochloric acid. Bring to a boil on a hot plate, allow to boil for 2 to 3 minutes, remove, let cool, and filter through Whatman #2 filter paper into a 50-ml volumetric flask. Rinse the residue on the filter with deionised water and dilute to 50 ml. Prepare standard lead solutions of 1, 2 and 5 ppm lead. Determine the absorbances of these solutions at the 283 millimicron wave length using a Hollow Cathode Pb lamp and a 10x scale expansion on a spectrophotometer, such as the Perkin-Elmer Model 303 Atomic Absorption Spectrophotometer. Determine the absorbance of the sample solutions using the same conditions as with the standards.

Calculation:

$$\frac{A \times F \times \text{dilution} = \text{ppm lead}}{W}$$

A = Absorbance

F = Factor = $\frac{\text{(Concentration standard in ppm Pb)}}{\text{absorbance}}$ 1/

W = Sample weight in grams

1/ The three standards are averaged to give ppm/unit A.

4.5.4 Physical properties tests. The breaking strength and percentage elongation of the catheters shall be tested in accordance with ASTM Method D 412 at a speed of separation of 20 ± 2 inches per minute.

4.5.5 Sterility test. The catheter shall be tested for sterility in accordance with the method specified in the USP for non-parenteral devices using inoculated product, inoculated simulated product, or paper spore strip (carrier). Product containing a biological indicator shall be marked or labeled so that it clearly differentiates it from product intended for distribution. The incubation medium and minimum time in each case shall be soybean casein digest for 7 days for inoculated product, inoculated simulated product, or paper spore strip (carrier). The incubation temperature shall be as indicated in paragraph 4.5.5.1. The minimum number of test units, regardless of

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:51Z
Check the source to verify that this is the current version before use.

lot size, shall be 10, except for inoculated carrier which shall be 20 for Type I Sterilization and 30 for Type II Sterilization including inoculated carrier and product test units. The inspection level shall be as indicated in table IV. Sampling for Tests.

4.5.5.1 Inoculated product or simulated product. For each type of sterilization the organism used shall be as listed below:

Type of Sterilization	Organism	Temperature
Steam	B. stearothermophilus	55° - 65°C
Dry Heat	B. stearothermophilus, or	55° - 65°C
	B. subtilis var. niger (or globigii)	30° - 35°C
Gas	B. subtilis var. niger (or globigii)	30° - 35°C
Radiation	B. pumilus	30° - 35°C

The number of viable cells shall be sufficient to provide assurance that the product has been sterilized.

4.5.5.2 Inoculated carrier. Inoculated carriers (paper spore strips) if used shall be in accordance with MIL-S-36586. Other paper carriers shall be inoculated to be of equivalent resistance. The method of incubation and number of test units shall be as indicated in 4.5.5 Sterility test and 4.5.5.1 Inoculated product or simulated product. The method of sterilization will control the organism in the spore strip to be tested for as shown in 4.5.5.1.
NOTE: When an inoculated carrier is chosen, product samples must also be tested as required by the USP.

4.5.5.3 Alternate method. Suppliers conducting sterility tests or designating lots in a manner other than that indicated herein shall submit proof that the alternate method provides equal assurance concerning the sterility of the product. However, all sterility tests shall be conducted using biological indicators. Request for approval of any alternate method of testing for sterility shall be made to the Contracting Officer, and approval obtained before employment of the alternate method on a government contract.

4.5.5.4 Product testing. Testing for sterility of the product after receipt by the government shall be without a biological indicator and in accordance with the USP.

Source: https://assist.dla.mil -- Downloaded: 202610-21T08:51Z
Check the source to verify that this is the current version before use.

5. PACKAGING

5.1 Preservation-packaging. Preservation-packaging shall be level A or C, as specified (see 6.1).

5.1.1 Unit of issue. One package containing one hundred individually packaged catheters, as specified, constitutes one unit of issue.

5.1.2 Level A.

5.1.2.1 Cleaning. Catheters shall be cleaned in accordance with MIL-P-116, process C-1.

5.1.2.2 Drying. Catheters shall be dried in accordance with MIL-P-116.

5.1.2.3 Preservative application. Preservatives shall not be applied to catheters.

5.1.2.4 Individual package. Each catheter shall be packaged sterile in a sealed, peel open type container of an appropriate size and capable of maintaining sterility of contents unless damaged or opened. The envelope shall be designed with tabs to facilitate opening.

5.1.2.5 Unit package. One hundred individually packaged catheters of one size only shall be packaged in a box conforming to PPP-B-636, class weather-resistant. The box shall be closed by taping the top and bottom flaps with 2 inch wide tape conforming to PPP-T-76. Closing of the bottom flaps with adhesive conforming to MMM-A-250 or metal stitches is permitted.

5.1.3 Level C. Catheters shall be clean, dry, and individually packaged sterile. The individually packaged catheters shall be further packaged in a manner that will afford adequate protection against deterioration and physical damage during shipment from the supply source to the first receiving activity.

5.2 Packing. Packing shall be level A, B or C, as specified (see 6.1).

5.2.1 Level A. Four unit packages containing catheters of one size only shall be packed in an exterior container designed for a type 2 load and conforming to PPP-B-636, class weather-resistant. Closure, strapping and waterproofing shall be as specified in the appendix of the box specification.

5.2.2 Level B. Four unit packages containing catheters of one size only shall be packed in an exterior container designed for a type 2 load and conforming to PPP-B-636, class domestic. Closure shall be as specified in the appendix of the box specification.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:51Z
Check the source to verify that this is the current version before use.

5.2.3 Level C. The packaged catheters shall be packed in shipping containers in a manner that will afford adequate protection against damage during direct shipment from the supply source to the first receiving activity. These packs shall conform to the applicable carrier rules and regulations.

5.3 Marking.

5.3.1 Individual package. In addition to any commercial markings, each individual package shall be marked in accordance with the requirements of the Federal Food, Drug and Cosmetic Act. Marking shall include the item identification, size, length, name and address of the manufacturer, sterility lot or control number and the legends:

"STERILITY GUARANTEED UNLESS PACKAGE IS DAMAGED OR OPENED" and "DISPOSABLE" or similar statements.

5.3.2 Unit package. Each unit package shall be marked in accordance with MIL-STD-129 and the requirements of the Federal Food, Drug and Cosmetic Act. Sterility lot (control) number, French size, contract or purchase order number, and name of contractor shall be shown. In addition, the method of sterilization (G-Gas, R-Radiation, S-Steam, C-Cold, D-Dry Heat Sterilization) shall be shown following the level of packaging and the date of packaging. Example "A-2/76-G". Final sterilization shall be on or after indicated packaging date.

5.3.3 Exterior container. Exterior container shall be marked in accordance with MIL-STD-129. Sterility lot or control number and method of sterilization as specified in 5.3.2 shall be shown.

6. NOTES

6.1 Ordering data. Purchasers should exercise any desired options specified herein, and the procurement documents should specify the following:

(a) Title, number and date of this specification.

(b) Size required (see 1.2).

(c) Applicable levels of packaging and packing, (see 5.1 and 5.2).

(d) Applicable NSN.

Source: https://assist.dla.mil -- Downloaded: 202610-21T08:51Z
Check the source to verify that this is the current version before use.

6.2 National Stock Number Coverage. This specification is intended to cover the following items appearing in the Federal Supply Catalog:

NSN	Item Identification	Size
6515-00-145-0011	CATHETER, URETHRAL, Plastic, Disposable, Round Tip, Robinson-Nelaton, 8 Fr., 100s	8
6515-00-400-3399	CATHETER, URETHRAL, Plastic, Disposable, Round Tip, Robinson-Nelaton, 10 Fr., 100s	10
6515-00-400-3401	CATHETER, URETHRAL, Plastic, Disposable, Round Tip, Robinson-Nelaton, 12 Fr., 100s	12
6515-00-400-5465	CATHETER, URETHRAL, Plastic, Disposable, Round Tip, Robinson-Nelaton, 14 Fr., 100s	14
6515-00-400-5466	CATHETER, URETHRAL, Plastic Disposable, Round Tip, Robinson-Nelaton, 16 Fr., 100s	16
6515-00-400-5467	CATHETER, URETHRAL, Plastic, Disposable, Round Tip, Robinson-Nelaton, 18 Fr., 100s	18

6.3 This specification does not include all types, classes, grades, sizes, etc., of the commodity indicated by the title of this specification, or which are commercially available, but is intended to cover the types, etc., which are normally procured to meet Military requirements.

6.4 Changes from previous issue. Asterisks are not used in this revision to identify changes with respect to the previous issue, due to the extensiveness of the changes.

Custodians:
Army - MD
Navy - MS
Air Force - 03

Preparing activity:
Defense Supply Agency - DM

Project No. 6515-1982

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:51Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

OMB Approval
No. 22-R255

INSTRUCTIONS: The purpose of this form is to solicit beneficial comments which will help achieve procurement of suitable products at reasonable cost and minimum delay, or will otherwise enhance use of the document. DoD contractors, government activities, or manufacturers/vendors who are prospective suppliers of the product are invited to submit comments to the government. Fold on lines on reverse side, staple in corner, and send to preparing activity. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements. Attach any pertinent data which may be of use in improving this document. If there are additional papers, attach to form and place both in an envelope addressed to preparing activity.

DOCUMENT IDENTIFIER AND TITLE

MIL-C-36583A CATHETER, URETHRAL, PLASTIC, Disposable, Round Tip, Robinson-Nelaton

NAME OF ORGANIZATION AND ADDRESS

CONTRACT NUMBER

MATERIAL PROCURED UNDER A

☐ DIRECT GOVERNMENT CONTRACT ☐ SUBCONTRACT

1. HAS ANY PART OF THE DOCUMENT CREATED PROBLEMS OR REQUIRED INTERPRETATION IN PROCUREMENT USE?
   A. GIVE PARAGRAPH NUMBER AND WORDING.

   B. RECOMMENDATIONS FOR CORRECTING THE DEFICIENCIES

2. COMMENTS ON ANY DOCUMENT REQUIREMENT CONSIDERED TOO RIGID

3. IS THE DOCUMENT RESTRICTIVE?

   ☐ YES ☐ NO *(If "Yes", in what way?)*

4. REMARKS

SUBMITTED BY *(Printed or typed name and address - Optional)*

TELEPHONE NO.

DATE

DD FORM 1 JAN 72 1426

REPLACES EDITION OF 1 JAN 66 WHICH MAY BE USED

Source: https://assist.dla.mil -- Downloaded: 202640-21T08:51Z
Check the source to verify that this is the current version before use.

FOLD

DEFENSE PERSONNEL SUPPORT CENTER
2800 South 20th Street
Philadelphia, PA 19101

POSTAGE AND FEES PAID
DEFENSE SUPPLY AGENCY
DoD - 304

OFFICIAL BUSINESS
PENALTY FOR PRIVATE USE $300

HEADQUARTERS, DEFENSE PERSONNEL SUPPORT CENTER
ATTN: DIRECTORATE OF MEDICAL MATERIEL, CODE ATT
2800 SOUTH 20TH STREET
PHILADELPHIA, PA 19101

FOLD

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:51Z
Check the source to verify that this is the current version before use.