MIL-M-6482D
17 February 1970
Superseding
MIL-M-6482C
28 August 1967

MILITARY SPECIFICATION

MASK ASSEMBLIES, OXYGEN, PRESSURE BREATHING

This specification is mandatory for use by all Departments and Agencies of the Department of Defense.

1. SCOPE

1.1 Scope - This specification covers pressure breathing oxygen mask assemblies, with and without suspension harness, furnished in small, medium, and large sizes.

1.2 Classification - Mask assemblies shall be of the following types, as specified (see 6.2).

Type I - Mask assembly (without suspension harness)
Type II - Mask assembly (with suspension harness)

2. APPLICABLE DOCUMENTS

2.1 The following documents, of the issue in effect on date of invitation for bids or request for proposal, form a part of this specification to the extent specified herein.

SPECIFICATIONS

Federal

L-P-378	Plastic Film (Polyethylene Thin Gage)
V-T-295	Thread, Nylon
QQ-A-200/3	Aluminum Alloy Bar, Rod, Shapes, and Tube, Extruded, 2024
QQ-A-225/3	Aluminum Alloy Bar, Rod, and Wire, 2011

FSC 1660

Source: https://assist.dla.mil -- Downloaded: 202610-17T07:05Z
Check the source to verify that this is the current version before use.

SPECIFICATIONS

Federal (Continued)

QQ-B-613	Brass, Leaded and Non-Leaded, Plate Rolled Bar, Sheet and Strip
QQ-S-698	Steel, Sheet and Strip, Low Carbon
QQ-S-777	Steel, Carbon, Strip, Cold-Rolled, Untempered Spring
UU-P-553	Paper, Wrapping, Tissue
UU-T-106	Tape, Pressure-Sensitive Adhesive, Masking, Paper
CCC-T-191	Textile Test Methods
PPP-B-601	Box, Wood, Cleated-Plywood
PPP-B-636	Box, Fiberboard

Military

MIL-P-79	Plastic, Rods and Tubes, Thermosetting, Laminated
MIL-P-116	Preservation, Methods of
MIL-B-543	Buckles, Tongueless and Web Strap
MIL-C-5040	Cord, Nylon
MIL-W-5625	Webbing, Textile, Nylon, Tubular

Source: https://assist.dla.mil -- Downloaded: 202640-17T07:05Z
Check the source to verify that this is the current version before use.

SPECIFICATIONS

Military (Continued)

MIL-C-5646	Cloth, Cotton, Airplane
MIL-D-6055	Drums, Metal Reusable, Shipping and Storage (Cap. From 88 To 510 Cubic Inches)
MIL-R-6891	Rubber, Anodic
MIL-S-7720	Steel, Corrosion-Resistant (18-8) Bars, and Forging Stock (For Aircraft Applications)
MIL-S-18729	Steel Plate, Sheet, and Strip, Alloy, 4130, Aircraft Quality
MIL-V-21701	Valve, Oxygen Mask, Inlet Check
MIL-F-22191	Films, Transparent, Flexible, Heat Sealing, For Packaging Applications
MIL-H-22486	Hose Assemblies, Oxygen Mask to Connector
MIL-O-27210	Oxygen, Aviator's Breathing, Liquid and Gas
MIL-V-81552	Valve, Exhalation, Oxygen Mask, Pressure Compensating, with Safety Relief

STANDARDS

Federal

FED-STD-595	Colors
FED-STD-601	Rubber; Sampling and Testing (Test method)
FED-STD-751	Stitches, Seams and Stitching

Military

MIL-STD-105	Sampling Procedures and Tables for Inspection by Attributes
MIL-STD-129	Marking for Shipment and Storage

Source: https://assist.dla.mil -- Downloaded: 202640-17T07:05Z
Check the source to verify that this is the current version before use.

STANDARDS

Military (Continued)

MIL-STD-130	Identification Marking of U.S. Military Property
MIL-STD-143	Specifications and Standards, Order of Precedence for the Selection of
MIL-STD-	Visual Examination of Mask Blanks
MS22001	Mask, Oxygen, Pressure Breathing
MS22016	Connector, Oxygen Mask Hose, Type MC-3A
MS22064	Clamp, Oxygen Hose
MS24347	Drums, Metal-Shipping and Storage
MS27796	Connector-Bayonet, Three Pin, Oxygen Mask
MS33586	Metals, Definition of Dissimilar
MS90339	Hose Assembly, Oxygen Mask to Connector

Air Force - Navy Aeronautical

AN227	Fasteners - Snap and Curtain

DRAWINGS

Aerospace Crew Equipment Department

ACEL 570	Yoke, A13A Oxygen Mask, Modified Suspension
ACEL 32D1317	Index, Personal Hoses, Mask Mounted Regulator to Disconnect
ACEL 33D1101	Oxygen Mask Retention Release Assembly

(Copies of specifications, standards, drawings, and publications required by suppliers in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.)

2.2 Other publications - The following documents form a part of this specification to the extent specified herein. Unless otherwise indicated, the issue in effect on date of invitation for bids or request for proposal shall apply.

American Society for Testing Materials Standard

D1149	Method of Test for Accelerated Ozone Cracking of Vulcanized Rubber

Source: https://assist.dla.mil -- Downloaded: 2026-10-17T07:05Z
Check the source to verify that this is the current version before use.

(Application for copies should be addressed to the American Society for Testing Materials, 1916 Race Street, Philadelphia, Pennsylvania 19103.)

3. REQUIREMENTS

3.1 Qualification - The mask assembly furnished under this specification shall be a product which has been inspected, and passed the qualification inspections specified herein, and has been listed on or approved for listing on the applicable qualified products list.

3.2 First article - The mask assembly furnished under this specification shall be a product which has been inspected and passed the first article inspection specified herein.

3.3 Selection of specifications and standards - Specifications and standards for necessary commodities and services not specified herein shall be selected in accordance with MIL-STD-143.

3.4 Materials - Materials shall conform to applicable specifications and shall be as specified herein and on applicable drawings. Materials which are not covered by specifications, or which are not specifically described herein, shall be of the best quality, of the lightest practicable weight, and suitable for the purpose intended.

3.4.1 Metal parts - All metal parts shall be of a corrosion resistance material or treated in a manner to render them adequately resistant to corrosion.

3.4.1.1 Dissimilar metals - Unless suitably protected against electrolytic corrosion, dissimilar metals shall not be used in intimate contact with each other. Dissimilar metals are defined in MS33586.

3.4.2 Nonmetallic materials - Any nonmetallic material that is adversely affected by continued use with oxygen shall not be used.

3.4.2.1 Age - Elastomer components, except silicone, shall not be more than 12 months old from the cure date of manufacture to the date of delivery to any Government Service or to any airframe or accessory manufacturer. The month and year the elastomer components were cured shall be stamped with a suitable ink or molded on all parts where such marking is practical. When figures are used, they shall be at least 3/32 inch.

3.4.2.2 Elastomer components - The elastomer components shall be composed of an ozone resistant composition, which shall not bloom, and shall meet the specified ozone-resistance performance requirements.

Source: https://assist.dla.mil -- Downloaded: 202640-17T07:05Z
Check the source to verify that this is the current version before use.

3.4.2.3 Webbing (Type II) - The nylon webbing used for construction of the suspension harness shall be 3/4-inch wide conforming to MIL-W-5625, except that the outer marker thread shall be the same color as the rest of the webbing. The dyed webbing shall have a fastness to perspiration of at least good when tested in accordance with CCC-T-191.

3.4.3 Protective treatment - When materials are used in the construction of the mask assembly that are subject to deterioration when exposed to environmental conditions likely to occur during service usage, they shall be protected against such deterioration in a manner that will in no way prevent compliance with the performance requirements of this specification. Protective coating which might crack, chip, or scale during normal service life or under extremes of environmental conditions shall not be used.

3.5 Design - The design and construction of the mask assemblies shall be in accordance with applicable figures specified herein. The mask assembly shall consist of the following:

Mask
Inlet check valves
Exhalation valve
Clamp
Insert, phenolic (Type I)

3.5.1 Mask - The mask shall be constructed in accordance with applicable figures of this specification and MS22001.

3.5.1.1 Dimensions -

3.5.1.1.1 Facial fit - The dimensions of the mask relative to facial fit shall conform to Figure 3.

3.5.1.1.2 Fixed dimensions - The fixed dimensions of the mask shall be in accordance with Figure 4. All dimensions not specifically defined herein shall be approved by the Procuring Service prior to acceptance of the masks.

3.5.1.2 Microphone pocket - The mask shall have an integrally constructed microphone pocket conforming to Figure 5.

3.5.1.2.1 Lead-in tube - The microphone pocket shall contain a 3/16-inch diameter lead-in tube, with an allowable wall thickness of 3/32-inch, for the microphone cable. The lead-in tube shall be centrally located in its portion of the molding with a minimum wall thickness of 3/32 inch around the opening. A rubber plug shall be provided for the lead-in tube opening.

Source: https://assist.dla.mil -- Downloaded: 2026-10-17T07:05Z
Check the source to verify that this is the current version before use.

3.5.1.2.2 Cable guide (Type II) - A removable cable guide, as shown in Figure 6, shall be attached to the mask over the common inlet duct.

3.5.1.3 Suspension lugs (Type II) -

3.5.1.3.1 Lower lugs - Two lower suspension lugs conforming to Figure 7, shall be molded into the mask. A hole, 1/4-inch maximum by 1/8-inch maximum shall be punched in the center of each lug, with the longer side of the hole parallel to and adjacent to the flange of the lug. The cloth reinforcements in the finished lugs shall be completely embedded in the rubber of the molding.

3.5.1.3.2 Upper lugs - Two upper suspension lugs shall be molded into the mask at the locations shown in Figure 2. The lugs shall be approximately 7/8-inch long and 1/8-inch thick. An incision approximately 5/8-inch long shall be so located in each lug that the incision is at least 1/8-inch from the outside edge of the lug at all points. The ends of the incision shall be rounded to prevent tearing. The upper lugs shall not be reinforced.

3.5.1.4 Inlet ducts - Two inlet ducts shall be formed in the mask. Each duct shall have a cross-sectional area of not less than 0.2 square inch.

3.5.1.4.1 Inlet ports - Each inlet duct shall terminate in an inlet port having an opening to the interior of the mask. Dimensions of this opening shall conform to those shown in Figure 4, Section A-A.

3.5.1.4.2 Common inlet tube - The two inlet ducts shall be joined at the chin of the mask to form a common inlet tube. The common inlet tube shall have an inside diameter of 3/4-inch.

3.5.1.4.2.1 Inlet insert (Type I) - The inlet tube shall be furnished with a 3/4-inch long plastic tubing insert conforming to MIL-P-79, Type PBE. The insert shall have an outside diameter of 3/4-inch with a wall thickness of 0.050 $\pm$ 0.005 inch.

3.5.1.4.2.2 Inlet insert (Type II) - A metal insert conforming to Figure 8 shall be attached to the common inlet tube.

3.5.2 Inlet check valve - An inlet check valve assembly, conforming to MIL-V-21701, shall be inserted in each inlet orifice of the mask facepiece.

3.5.3 Exhalation valve - An exhalation valve, conforming to MIL-V-81552, shall be inserted in the expiratory chamber as shown in Figure 9 with the protuberance on the exhalation valve inserted through the floor of the expiratory chamber.

Source: https://assist.dla.mil -- Downloaded: 202640-17T07:05Z
Check the source to verify that this is the current version before use.

3.5.4 Delivery hose -

3.5.4.1 Type I - When specified, delivery hoses conforming to MIL-H-22486 and MS90339-1 or MS90339-2 shall be furnished with the mask assembly (see 6.2 and 6.3) and attached to the mask assembly by a clamp specified in 3.5.5.

3.5.4.2 Type II - The mask shall be furnished with a corrugated delivery hose, conforming to Figure 10.

3.5.4.2.1 Delivery hose length-limiting cord - A nylon cord and snap assembly conforming to Figure 11 shall be installed inside the delivery hose by attaching the nylon loop to the cross-bar of the metal tubing insert specified in 3.5.1.4.2.2. This attachment is made at the mask end of the delivery hose while the metal snap is attached to the cross-bar of the connector-bayonet specified in 3.5.6.2 and located at the lower end of the mask delivery hose.

3.5.5 Clamp - The delivery hose shall be attached to the mask by means of a hose clamp conforming to MS22064-18.

3.5.6 Connector -

3.5.6.1 Type I - When specified, a connector conforming to MS22016 shall be furnished with the mask assembly (see 6.2 and 6.3) and the connector shall be attached to the free end of the delivery hose by a clamp specified in 3.5.5.

3.5.6.2 Type II - A connector conforming to MS27796 shall be attached to the free end of the delivery hose by a clamp specified in 3.5.5.

3.5.7 Suspension harness (Type II) - A suspension harness consisting of green nylon webbing straps and hardware shall be attached to the mask as shown on MS22001. Sewing shall be accomplished with nylon thread conforming to V-T-295, type I or II, class 1, color sage green No. 1511, size FF. Stitching shall be type 301 in accordance with Federal Standard 751, 7 to 11 stitches per inch. All stitching shall be backstitched not less than 1/2 inch. All strap ends shall be seared to prevent fraying.

3.5.7.1 Straps - Straps shall be as specified herein or as shown on MS22001, as applicable.

Source: https://assist.dla.mil -- Downloaded: 202610-17T07:05Z
Check the source to verify that this is the current version before use.

3.5.7.1.1 Strap, right side - The right side hook strap shall be a 10-3/8 ± 1/8 inch length of webbing. The middle of this strap shall be sewn into a 7-7/8 ± 1/16 inch length of webbing, doubled on itself and sewn to form a two-layer mask hook strap as shown on MS22001.

3.5.7.1.2 Strap, nose - A buckle conforming to Figure 12 shall be sewn on each end of a 5-1/8 ± 1/16 inch length of webbing for the nose piece strap shown on MS22001.

3.5.7.1.3 Strap, left side - The left side snap fastener strap shall be a 10-3/8 ± 1/8 inch length of webbing. One end of the strap shall be inserted through the snap fastener component, leaving the snap fastener component approximately in the middle of the strap as shown on MS22001.

3.5.7.1.4 Assembly to mask - The nose piece strap shall be inserted through the two upper lugs of the mask and assembled as shown on MS22001. One end of the right and left side straps shall be attached to the buckles on either end of the nose strap. The bar, adapter, and buckle assembly shall be inserted through the lower lug of the mask. The free ends of the right and left straps shall be attached to the bar adapter, and buckle assembly as shown on MS22001.

3.5.7.2 Hardware - The buckles, snap fastener components, bar adapter and buckle assemblies and mask hook shall conform to Figures 12, 13, 14, and 15 respectively. In addition to the hardware installed on the mask, a helmet hook conforming to Figure 16, and six screws round-head, brass, 3/8, No. 3-56, right hand thread shall be furnished with each mask.

3.5.7.3 Nosepiece - A green plastic nosepiece, acceptable to the Procuring Service, shall be assembled on the face piece of the mask as shown on MS22001.

3.6 Performance -

3.6.1 Low temperature pliability - The mask assembly, when tested as specified in 4.7.2, shall be pliable and suitable for use and there shall be no apparent increase in the rigidity of the mask assembly.

3.6.2 Low temperature starting delay - The mask assembly, when tested as specified in 4.7.3, shall function immediately.

3.6.3 High and low temperature operation - The mask assembly, when tested as specified in 4.7.4, shall function properly. The mask assembly shall not become detached nor shall there be any failure of components.

Source: https://assist.dla.mil -- Downloaded: 2026-10-17T07:05Z
Check the source to verify that this is the current version before use.

3.6.4 High and low temperature storage - The mask assembly, when tested as specified in 4.7.5, shall not be gummy or tacky.

3.6.5 Mask leakage - The inboard mask leakage, when tested as specified in 4.7.6, shall not exceed 0.1 liter per minute.

3.6.6 Inlet check valve installation (low suction) - The total leakage through the inlet check valve, when tested as specified in 4.7.7, shall not exceed 50 milliliters per minute.

3.6.7 Inlet check valve installation (high suction) - The total leakage through the inlet check valve, when tested as specified in 4.7.8, shall not exceed 300 milliliters per minute.

3.6.8 Exhalation valve installation - The exhalation valve, when tested as specified in 4.7.9, shall open at a pressure between 15 and 20 millimeters of mercury in the inlet tube.

3.6.9 Odor - The odor of the mask assembly shall be considered objectionable, when tested as specified in 4.7.10, if so judged by two or more test personnel.

3.6.10 Delivery hose (Type II) -

3.6.10.1 Delivery hose leakage - The delivery hose, when tested as specified in 4.7.11.1, shall not leak.

3.6.10.2 Delivery hose stretch - The delivery hose, when tested as specified in 4.7.11.2, shall not break or be adversely affected.

3.6.11 Exhalation port icing - The exhalation port of the mask assembly, when tested as specified in 4.7.12, shall be capable of being freed of ice by manual manipulation.

3.6.12 Lug strength (Type II) - The lower mask lugs, when tested as specified in 4.7.13, shall not show any evidence of damage to the mask assembly or fasteners.

3.6.13 Disassembly and examination - The mask assembly, when tested as specified in 4.7.14, shall not show any evidence of excessive deterioration or wear due to testing which might affect the mask assembly performance.

Source: https://assist.dla.mil -- Downloaded: 202610-17T07:05Z
Check the source to verify that this is the current version before use.

3.6.14 Material composition tests -

3.6.14.1 Physical property tests (elastomer components) - The elastomer components of the mask assembly, when tested as specified in 4.7.15.1, shall pass the specified physical property requirements.

3.6.14.2 Ozone-resistance (elastomer components) - The elastomer components of the mask, when tested as specified in 4.7.15.2, shall not show any evidence of checking, cracking, or damage.

3.6.15 Resiliency test - The elastomer sample, when tested as specified in 4.7.16, shall pass the Bashore value specified in Table III.

3.7 Interchangeability - All parts having the same manufacturer's part number shall be functionally and dimensionally interchangeable.

3.8 Color - The color of the mask, webbing, and the delivery hose shall be medium green, approximately matching color number 34079 of FED-STD-595.

3.9 Identification of product - The mask assemblies shall be marked for identification in accordance with MIL-STD-130 except that the Federal Stock Number shall be omitted from the nameplate. The following special marking shall be added: MS Part No., Size.

3.10 Marking -

3.10.1 Mask - The word "SILICONE" shall be molded, either recessed or by relief, into all masks that are manufactured of silicone rubber. The marking shall in no way have an adverse affect in the functioning of the oxygen mask. The lettering size shall be within the height range of 3/16 to 3/4 inch.

3.10.2 Hose - The words "MASK END" shall be molded into the mask end of the hose as shown in Figure 10. The date of manufacture (month and year) shall be molded or stamped on one end of the hose. The letter and number characters shall be least 3/32 inch high.

3.11 Workmanship - The mask assemblies shall be uniform in quality and shall be free from defects which could adversely affect safety, performance, reliability, or durability. The faceblank inner and outer surfaces shall be smooth and free from imperfections. The elastomeric material shall be compact and free from holes and bubbles.

Source: https://assist.dla.mil -- Downloaded: 2026-10-17T07:05Z
Check the source to verify that this is the current version before use.

4. QUALITY ASSURANCE PROVISIONS

4.1 Responsibility for inspection - Unless otherwise specified in the contract or purchase order, the supplier is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or order, the supplier may use his own or any other facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

4.2 Classification of inspection - The examination and testing of the mask assemblies shall be classified as follows:

(a) Qualification inspection - Qualification inspection consists of examinations and tests performed on samples submitted for approval as qualified products.

(b) First article inspection - First article inspection consists of examinations and tests performed on samples which are representative of the production item after award of a contract to determine that the production item meets the requirements of this specification.

(c) Quality conformance inspection - Quality conformance inspection consists of examinations and tests performed on individual products or lots to determine conformance of the products or lots with the requirements set forth in this specification.

4.3 Qualification inspection - Qualification inspection shall consist of all the examinations and tests of this specification.

4.3.1 Qualification samples - Qualification samples shall consist of one mask assembly of each type and size, less hose assembly, for which qualification is required, and six elastomer tests slabs, 6 by 6 by 0.075 inches, composed of the identical ozone-resistant composition and cure that was used in manufacturing the elastomer components. Samples shall be forwarded to the Supply Officer, Naval Air Development Center, Johnsville, Warminster, Pennsylvania 18974, Attention: Director Aerospace Crew Equipment Department. The samples shall

Source: https://assist.dla.mil -- Downloaded: 202610-17T07:05Z
Check the source to verify that this is the current version before use.

be plainly identified by securely attached durable tags marked with the following information:

Sample submitted by (name) (date) for qualification inspection in accordance with the requirements of MIL-M-6482D, Type _____, Size _____, and number under authorization (reference authorizing letter and number, see 6.5).

4.4 First article inspection - First article inspection shall consist of the following examinations and tests:

Visual examination
Dimensions
Low temperature pliability
Mask leakage
Inlet check valve installation (low suction)
Inlet check valve installation (high suction)
Exhalation valve installation
Delivery hose stretch (Type II)
Lug strength (Type II)

4.4.1 First article samples -

4.4.1.1 Applicable to the Naval Air Systems Command - Unless otherwise specified, as soon as practicable after award of a contract or order, the manufacturer shall submit one mask assembly of each size. The samples shall be representative of the construction, workmanship, components, and materials to be used during production. When a contractor is in continuous production of these masks from contract to contract, submission of further first article samples on the new contract may be waived at the discretion of the procuring activity (see 6.2). Approval of the first article samples or the waiving of the first article inspection does not preclude the requirements of submitting to the quality conformance inspection. The first article samples shall be forwarded to the Government as directed by the contracting officer (see 6.2).

4.4.1.1.1 Upon completion of the first article inspection, all the applicable inspection reports and when applicable, recommendations and comments pertinent for use in monitoring production will be forwarded to the cognizant Government activity. One approved mask assembly will be returned to the manufacturer for use in monitoring production. The remaining samples will be consumed or destroyed in the first article inspection and shall not be considered as part of the quantity to be delivered under contract.

Source: https://assist.dla.mil -- Downloaded: 202640-17T07:05Z
Check the source to verify that this is the current version before use.

4.4.1.2 Applicable to the Army - For purchases by the Army, the quantity and kind of samples, the name and address of the first article inspection activity and other pertinent information (see 4.4.1.1 and 4.4.1.1.1 for information) shall be as specified (see 6.2).

4.5 Quality conformance inspection - The sampling and inspection levels shall conform to MIL-STD-105. Quality conformance inspection shall consist of the following examinations and tests:

Visual examination
Dimensions
Low temperature pliability
Mask leakage
Inlet check valve installation (low suction)
Exhalation valve installation
Delivery hose stretch (Type II)
Preparation for Delivery

4.5.1 Sampling -

4.5.1.1 Inspection lot -

4.5.1.1.1 Mask assembly - An inspection lot size shall be expressed in units of one mask assembly made under essentially the same conditions and from the same materials and components. The sample unit shall be one mask assembly.

4.5.1.1.2 Preparation for delivery - An inspection lot size shall be expressed in units of one fully prepared shipping container, containing mask assemblies of one size, fully prepared for delivery from essentially the same materials and components. The sample unit shall be one shipping container, containing mask assemblies of one size, fully prepared for delivery with the exception that it need not be sealed.

4.5.1.2 Sampling for tests and examinations of the mask assemblies - the sample size, acceptance criteria, tests, and examinations required for the mask assemblies shall be as specified in Table I.

4.6 Test conditions -

4.6.1 Gas - Unless otherwise specified, the gas used in testing the mask assemblies shall be oxygen conforming to MIL-O-27210, Type I.

Source: https://assist.dla.mil -- Downloaded: 2026-10-17T07:05Z
Check the source to verify that this is the current version before use.

TABLE I

SAMPLE SIZE, ACCEPTANCE CRITERIA, TESTS, AND EXAMINATION OF THE MASK ASSEMBLIES

Inspection	Method	Sample Size	Acceptance Criteria 1/
Visual Examination (See classification of defects)	4.7.1.1	Every mask assembly	Reject all units with any major defect. An acceptable quality level of 4.0 defects per hundred units for minor defects.
Dimensions	4.7.1.1.1	Inspection Level S-2	An acceptable quality level of 2.5 defects per 100 units.
Low Temperature Pliability	4.7.2	Inspection Level S-2	An acceptable quality level of 2.5 defects per 100 units.
Mask Leakage	4.7.6	Every mask assembly	Reject all defective units.
Inlet Check Valve Installation (Low Suction)	4.7.7	Every mask assembly	Reject all defective units.
Exhalation Valve Installation	4.7.9	Every mask assembly	Reject all defective units.
Delivery Hose Stretch (Type II) 2/	4.7.11.2	Inspection Level S-2	An acceptable quality level of 2.5 defects per 100 units.
Preparation for Delivery	4.7.1.2	Inspection Level S-2	Total acceptable quality level of 4.0 percent defective.

1/ The sampling plan acceptance numbers shall apply collectively to all the characteristics within a stated acceptable quality level.

2/ This is a destructive test (see 6.2).

Source: https://assist.dla.mil -- Downloaded: 202640-17T07:05Z
Check the source to verify that this is the current version before use.

4.6.2 Temperature and pressure - Unless otherwise specified, tests shall be conducted at local ambient temperatures and barometric pressure. Corrections shall be made to provide agreement with the temperature and pressure calibration of the instrument. Inspection data provided by any instrument not calibrated to normal temperature and pressure (NTP) conditions shall be corrected to determine NTP requirements. NTP conditions are 29.92 inches of mercury and 70°F.

4.6.3 Test equipment -

4.6.3.1 Resiliency test - Test shall be performed on a Bashore Resiliometer, Precision Scientific Company Catalog No. TS 15100 or equivalent.

4.7 Inspection methods -

4.7.1 Visual examination -

4.7.1.1 Mask assembly - Every mask assembly shall be examined visually to determine conformance to this specification and applicable drawings. The classification of defects, MIL-STD-1349 , shall be used to classify the defects found.

NOTE: Reference standards have been established to define the type and category (major or minor) of each defect. Defects of a magnitude greater than the established reference standards shall be cause for rejection. Reference standards (photographs of defects) shall be used by successful bidders to determine compliance with requirements. The reference standards (photographs of defects) form a part of MIL-STD-1349.

4.7.1.1.1 Dimensions - The mask assembly shall be checked dimensionally to determine conformance to the dimensions specified herein.

4.7.1.2 Preparation for delivery - Each of the fully prepared shipping containers, containing mask assemblies of one size, selected as a sample unit from the lot shall be examined to determine that the packaging, packing, and marking conform to this specification. The classification of defects, Table II, shall be used to classify the defects found.

4.7.2 Low temperature pliability - The mask assembly shall be conditioned at -65 ± 5°F for one hour. While at this temperature, the mask assembly shall be worn by a subject or simulated mechanically for determining pliability and suitability for use. The mask assembly shall pass the requirements specified in 3.6.1.

Source: https://assist.dla.mil -- Downloaded: 202640-17T07:05Z
Check the source to verify that this is the currentversion before use.

TABLE II

LIST OF DEFECTS FOR PREPARATION FOR DELIVERY

ITEM	DEFECTS
Exterior and interior markings	Missing, incorrect, incomplete, illegible; of improper size, location, sequence; or method of application; markings not the same on the interior and exterior containers.
Packaging and Packing materials	Any non-conforming component; any component missing, damaged, or otherwise defective.
Workmanship	Inadequate application of the components such as incomplete closure of the unit package, intermediate package, container flaps, loose strappings, etc.; bulging or distortion of the containers.
Exterior and interior weight or content	Number per container is more or less than required; gross or net weight exceeds the requirements; more than one type or size in the same container.

4.7.3 Low temperature starting delay - The mask assembly shall be conditioned at -40 ± 5°F for 2 hours. While at this temperature, the mask assembly shall be worn by a subject or simulated mechanically to determine the time required for the mask to start operating. The mask assembly shall pass the requirements specified in 3.6.2.

4.7.4 High and low temperature operation - The mask assembly shall be placed in an atmosphere maintained at temperatures of +160 ± 5°F and -40 ± 5°F and having a wind velocity of not less than 15 miles per hour for a period of not less than three hours. After each exposure, the mask assembly shall pass the requirements specified in 3.6.3.

4.7.5 High and low temperature storage - The mask assembly shall be placed in an atmosphere maintained at temperatures of +160 ± 5°F and -65 ± 5°F for a period of not less than 50 hours. After each exposure, the mask assembly shall pass the requirements specified in 3.6.4.

Source: https://assist.dla.mil -- Downloaded: 202640-17T07:05Z
Check the source to verify that this is the current version before use.

4.7.6 Mask leakage - In order that equal suction may be applied to both sides of the exhalation valve, a suitable obstruction shall be inserted in the inhalation check valve assembly to hold the valve open during this test. After blocking the inhalation check valve as described, each mask shall be fitted to a suitable facsimile of a head of the proper size for the mask to provide a comfortable snug fit against the face and to simulate service conditions. The free end of the mask tubing shall be plugged, and a suction of 25 millimeters of mercury shall be applied within the face piece of the mask. The mask shall pass the requirements specified in 3.6.5.

4.7.7 Inlet check valve installation (low suction) - Inlet check valves shall be completely dry throughout the following tests. The mask inlet check valves shall be inspected for imperfect seating of the flapper on the seat and for any leaks around the valve seat by applying and maintaining a suction of 1 inch of water at the free end of the delivery tube. A suitable means shall be used to prevent collapse of the hose if necessary. The mask shall pass the requirements specified in 3.6.6.

4.7.8 Inlet check valve installation (high suction) - Repeat the above test using a suction of 25 millimeters of mercury. The mask shall pass the requirements specified in 3.6.7.

4.7.9 Exhalation valve installation - Each mask shall be fitted to a suitable facsimile of a head of the proper size for the mask to provide a comfortable snug fit against the face and to simulate service conditions. All suction and pressure from previous tests shall be exhausted. A pressure of 20 millimeters of mercury shall be applied at the mask tubing. The pressure at the mask tubing shall than be gradually reduced, causing the inlet check valves to close, and causing a pressure differential to be applied across the exhalation valve. The exhalation valve shall pass the requirements specified in 3.6.8.

4.7.10 Odor - The mask shall be worn by six subjects in a manner that will prevent exterior odors from influencing the test. The mask shall pass the requirements specified in 3.6.9.

4.7.11 Delivery hose (Type II) -

4.7.11.1 Delivery hose leakage - One end of the delivery hose shall be plugged and an air pressure of three pounds per square inch applied to the other end. The hose shall be immersed just under the surface of water. The delivery hose shall pass the requirements specified in 3.6.10.1.

Source: https://assist.dla.mil -- Downloaded: 2026-10-17T07:05Z
Check the source to verify that this is the current version before use.

4.7.11.2 Delivery hose stretch - One end of the hose shall be attached to a fitting simulating the mask connection. The other end shall be connected to a fitting simulating a connector conforming to MS27796. Clamps for the connections shall be the type specified herein. One of the end connections shall be attached to a support. A weight of 63 ± 1 pounds shall be attached in the other connection so as to exert a straight pull on the hose for a period of 3 ± 2 seconds. The hose shall pass the requirements specified in 3.6.10.2.

4.7.12 Exhalation port icing - The mask assembly shall be subjected to respiration while exposed to atmospheric conditions that will cause water to collect in the exhalation port and channel. The mask shall then be exposed to a temperature that will cause the water to freeze. After the water is completely frozen, the mask shall be manually massaged and manipulated to remove the ice. The mask assembly shall pass the requirements specified in 3.6.11.

4.7.13 Lug strength (Type II) - With the bar, buckle and adapter assembly attached to the lower lug, a dead weight of 35 pounds shall be attached to the fastener. The mask shall be held in different positions to determine adequacy of lug strength in different directions. The lower lugs shall pass the requirements specified in 3.6.12.

4.7.14 Disassembly and examination - At the conclusion of all the inspections, the mask assembly shall be disassembled and examined. The mask assembly shall pass the requirements specified in 3.6.13. The mask assembly shall be disassembled and examined after any test in which mask assembly failure indicates faulty construction.

4.7.15 Material composition tests -

4.7.15.1 Physical property tests (elastomer components) - Three of the six elastomer test slabs submitted for qualification inspection (see 4.3.1) shall be tested in accordance with the following procedures in the FED TEST METHOD STD. NO. 601 and shall meet the physical property requirements specified in Table III.

4.7.15.2 Ozone resistance test (elastomer components) - Three of the six test slabs submitted for qualification inspection (see 4.3.1) shall be tested for ozone resistance. The test apparatus shall be in accordance with ASTM Method No. D 1149. The test slabs shall be elongated 20 percent, placed in an ozone-free atmosphere for 24 hours, then placed in the ozone chamber. The

Source: https://assist.dla.mil -- Downloaded: 2026-10-17T07:05Z
Check the source to verify that this is the current version before use.

chamber shall be adjusted to 100 ± 2°F and to give an exposure of ozone concentration of 120 ± 10 parts by volume of ozone per million parts by volume of air. The air-ozone velocity in the chamber shall be at least 2 feet per second. The material shall be exposed to these conditions for 60 minutes. The test slabs shall be examined under 10X magnification and shall pass the requirements specified in 3.6.14.2.

TABLE III

Property	Method	Requirement
Original		
Modulus (100% Elongation), psi	4131	100 min. - 200 max.
Tear Resistance (Type B die), minimum lb/in	4211	130
Tensile Strength, minimum psi	4111	1000
Ultimate Elongation, percent minimum	4121	600
Shore Durometer Hardness	3021	47 ± 5
Tension Set, percent maximum	4411	15
Specific Gravity, Hydrostatic, maximum	14011	1.20
Bashore Value, percent minimum	-----	40
Accelerated aging at 212 ± 5°F for 72 hours		
Tensile Strength, percent loss, maximum	7221	15
Ultimate Elongation, percent loss, maximum	7221	15
Compression Set (30 percent deflection), percent maximum	3311	35

4.7.16 Resiliency test - The elastomer sample shall be 1/2 inch thick (one piece or piled up) by 1-1/4 inch diameter. The test shall be conducted on an instrument specified in 4.6.3.1 and shall be performed in the following manner:

1. Level the instrument by means of two leveling screws on front of base.

2. Raise the 1 ounce plunger to top of plunger guide rod by holding plunger lightly between thumb and index finger.

Source: https://assist.dla.mil -- Downloaded: 2026-10-17T07:05Z
Check the source to verify that this is the current version before use.

3. Release the two locking knobs and raise the resilience scale to a height sufficient to accommodate the sample.

4. Place center of sample directly under the plunger guide and lower the resilience scale, allowing its full weight to rest upon the sample. Re-tighten the two locking knobs.

5. Release the plunger by exerting a slight pressure against the plunger release rod. Plunger must slide freely on guide rod.

6. Obtain reading by observing the number immediately behind the top of the plunger at the peak of rebound.

7. Disregard the first three readings and average the next three rebounds as the resilience reading.

The elastomer sample shall pass the requirements specified in 3.6.15.

1/ The following precautions shall be taken in conducting the above test procedure:

1. Whenever it is necessary to test samples of less than 1/4 inch total thickness, place a piece of brass 1/4 inch x 1-1/4 inch diameter under the sample, making sure that it rests flat.

2. Samples as thin as 1/8 inch should be used for comparative testing only.

3. Always keep a sample of rubber under the stabilizer when instrument is not in use to avoid damage to plunger.

4. Do not attempt to lift plunger with one finger or do not apply any side pressure on plunger guide rod. Side pressure on the plunger guide rod may cause permanent deflection and hinder free fall of the plunger.

5. Do not oil any part of this instrument.

5. PREPARATION FOR DELIVERY

5.1 Packaging - Packaging shall be level A or C as specified in the contract or order (see 6.2).

Source: https://assist.dla.mil -- Downloaded: 202610-17T07:05Z
Check the source to verify that this is the current version before use.

5.1.1 Level A - Each mask shall be cleaned and packaged in accordance with MIL-P-116, Method IA-5(X). Each mask, appropriately cleaned, shall have the facepiece filled with tissue paper conforming to UU-P-553, type I, grade A, class 1 or 2 to support the flexible portion thereof in a manner that will preclude deformation. The mask, neatly arranged, shall be placed within a snug .002 inch polyethylene bag, material conforming to L-P-378, type I or MIL-F-22191, type III. The affixing hardware, i.e., helmet hook, mask hook, buckle, etc., shall be suitably wrapped/bagged, tape sealed and placed within the polyethylene bag. The open end of the polyethylene bag shall be tape sealed with pressure sensitive tape conforming to UU-T-106 or equivalent. The continuous line marking requirement of MIL-F-22191, paragraph 3.4.1, is not mandatory. Prior to or during the closure operation, the excess air within the bag shall be expelled. The metal container required to accomplish the unit package shall conform to MIL-D-6055, MS24347-6.

5.1.2 Level C - Each mask shall be cleaned and packaged in a manner that will afford it the degree of protection necessary to prevent physical damage or deterioration during transit from the supply source to the first receiving activity. The contractor's commercial practice may be utilized when it conforms to the criteria stated herein.

5.1.3 Intermediate packaging - Unless otherwise specified, unit containers shall be afforded intermediate packaging. Each intermediate container shall be horizontally and vertically partitioned, with full height of the container, half slotted style, double face corrugated fiberboard pads which shall be fitted together in a manner that will accommodate six unit containers and accomplish a close fit. The intermediate container shall conform to PPP-B-636, domestic class. The container closure and sealing shall be accomplished in accordance with the procedures in the appendix to the specification.

5.2 Packing - Packing shall be Level A, B, or C as specified in the contract or order (see 6.2).

5.2.1 Level A - Masks packaged as specified in 5.1.1 and 5.1.3 shall be packed for export shipment in shipping containers conforming to PPP-B-601, weather resistant class. The plywood boxes shall be surface treated in accordance with the requirements of PPP-B-601. Unless otherwise authorized the gross weight of each packed shipping container shall not exceed 200 pounds. Insofar as practicable shipping containers shall contain masks of one size only, the contents shall effect a close fit, contain identical

Source: https://assist.dla.mil -- Downloaded: 2026-10-17T07:05Z
Check the source to verify that this is the current version before use.

quantities and be of uniform configuration. The containers shall be secured, sealed and strapped in accordance with the procedures specified in the appendix of the applicable specification.

5.2.2 Level B - Unless otherwise specified by the procuring activity, masks packaged in accordance with 5.1.1 and 5.1.3 need not be packed for domestic (continental U. S.) shipment and storage. When packing is specified by the procuring activity, the masks shall be packed for shipment in the same manner specified in 5.2.1 except that fiberboard containers conforming to PPP-B-636, Class-Weather Resistant V3c or V3s shall be utilized. The weight limitation of fiberboard containers (PPP-B-636) shall be in accordance with table I.

5.2.3 Level C - Masks, packaged as specified in 5.1, shall be packed in a manner to insure carrier acceptance and safe delivery at destination at the lowest transportation rate for such supplies. Containers shall be in accordance with rules or regulations of carriers applicable to the mode of transportation.

5.3 Marking - All unit, intermediate and shipping containers shall be marked in accordance with MIL-STD-129. The date of cure/manufacture and the contract or order number shall be indicated on all unit and intermediate containers. When the intermediate container also serves as the shipper, marking shall indicate Level B Packing.

5.3.1 Precautionary marking - The following precautionary marking shall appear on each unit package:

"CAUTION: DO NOT ALLOW CONTAMINANTS OF ANY KIND TO BE USED ON OR ABOUT THE MASK ASSEMBLIES"

5.3.1.1 Additional marking - In addition, the following shall be marked on all packages and containers:

"STORE MASKS AT TEMPERATURES OF
32 TO 80 DEGREES FAHRENHEIT"

6. NOTES

6.1 Intended use - The oxygen masks described by this specification are for use in dispensing gaseous oxygen from pressure demand regulators to aviators engaged in high altitude flying and for use with constant flow systems such as portable oxygen sources used by personnel parachuting from high altitudes.

Source: https://assist.dla.mil -- Downloaded: 2026-10-17T07:05Z
Check the source to verify that this is the current version before use.

6.2 Ordering data - Procurement documents should specify the following:

(a) Title, number, and date of this specification.

(b) Type of mask required (see 1.2).

(c) Whether delivery hoses and connectors should be furnished with the mask assembly (see 3.5.4.1 and 3.5.6.1).

(d) Items of data required (see 6.4).

(e) Whether first article inspection is required for Naval Air Systems Command purchases and where the samples should be delivered (see 4.4.1.1).

(f) First article information for Army purchases (see 4.4.1.2).

(g) Selection of applicable levels of preservation, packaging and packing required (see 5.1 and 5.2).

(h) Applicable methods of cleaning and preservation.

(i) Samples subjected to destructive test are not to be considered or shipped as part of the contract or order (see Table I).

6.3 Components necessary for final application will vary as listed below:

6.3.1 Hoses -

Mask mounted regulator system - Hoses in accordance with ACEL Drawing 32D1317
Chest mounted regulator - Hoses in accordance with MS90339-1
Diluter demand regulator - Hoses in accordance with MS90339-1 or -2 with MS22016 connector.

6.3.2 Retention systems - Retention systems shall be in accordance with ACEL drawings 570 or 33D1101.

Source: https://assist.dla.mil -- Downloaded: 2026-10-17T07:05Z
Check the source to verify that this is the current version before use.

6.4 Data - For the information of Contractors and Contracting Officers, any of the data specified in applicable documents listed in Section 2 of this specification or referenced lower-tier documents need not be prepared for the Government and shall not be furnished to the Government unless specified in the contract or order. The data to be furnished shall be listed on DD Form 1423 (Contractor Data Requirements List), which shall be attached to and made a part of the contract or order. NAVAIR Form 4200/25 (Drawings, Lists, and Specifications Required) shall be attached where applicable.

6.5 With respect to products requiring qualification, awards will be made only for products which are at the time set for opening of bids, qualified for inclusion in the applicable Qualified Products List whether or not such products have actually been so listed by that date. The attention of suppliers is called to this requirement, and manufacturers are urged to arrange to have the products that they propose to offer to the Federal Government tested for qualification in order that they may be eligible to be awarded contracts or orders for the products covered by this specification. The activity responsible for the Qualified Products List is the Commander, Naval Air Systems Command, Department of the Navy, Washington, D.C. 20360; however, authorization for qualification of products shall be obtained from the Commanding Officer, Naval Air Development Center, Johnsville, Warminster, Pennsylvania 18974, Attention: Director, Aerospace Crew Equipment Department. Prior to submission of the samples for qualification inspection, the manufacturer shall submit a request to the Aerospace Crew Equipment Department indicating a date on which the samples can be forwarded and also request an authorization number to accompany the samples.

6.5.1 When requested, the manufacturer shall submit engineering drawings and inspection reports in accordance with SD-6, Provisions Governing Qualification.

Custodians:

Army - AV
Navy - AS

Preparing Acitvity:

Navy - AS

Project No. (1660-0068)

Review Activities:

Army - AV and GL
Navy - AS

NOTICE: Review/user information is current as of the date of this document. For future coordination of changes to this document, draft circulation should be based on the information in the current DODISS.

Source: https://assist.dla.mil -- Downloaded: 202640-17T07:05Z
Check the source to verify that this is the currentversion before use.

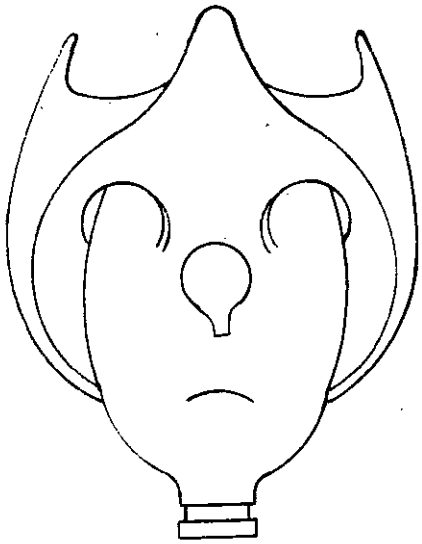


FIGURE 1. FRONT VIEW (TYPE I)


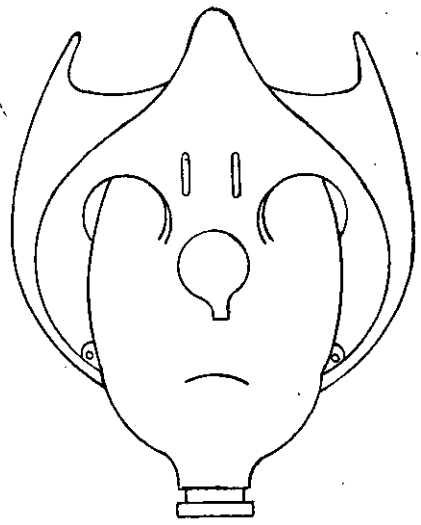


FIGURE 2. FRONT VIEW WITHOUT HARNESS (TYPE II)

Source: https://assist.dla.mil -- Downloaded: 2026-10-17T07:05Z
Check the source to verify that this is the current version before use.

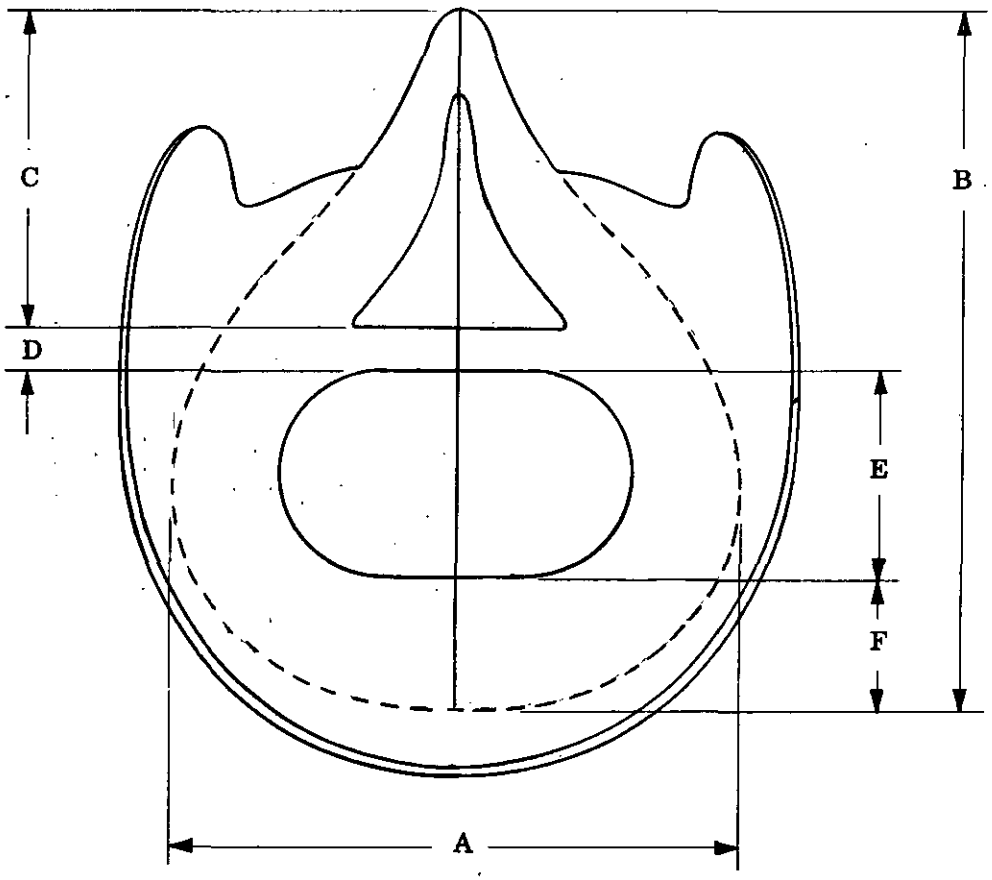


DIMENSIONS	TOLERANCE PLUS OR MINUS	LARGE	MEDIUM	SMALL
A	1/16	4-1/16	3-15/16	3-5/8
B	1/16	5-1/16	4-5/8	4-1/4
C	1/16	2-5/16	2-3/16	2-3/16
D	1/32	3/8	1/4	1/4
E	1/16	1-3/8	1-3/8	1-5/32
F	1/16	1	13/16	5/8

DIMENSIONS IN INCHES

FIGURE 3. FACIAL DIMENSIONS RELATIVE TO SIZE


Source: https://assist.dla.mil -- Downloaded: 2026-10-17T07:05Z
Check the source to verify that this is the current version before use.

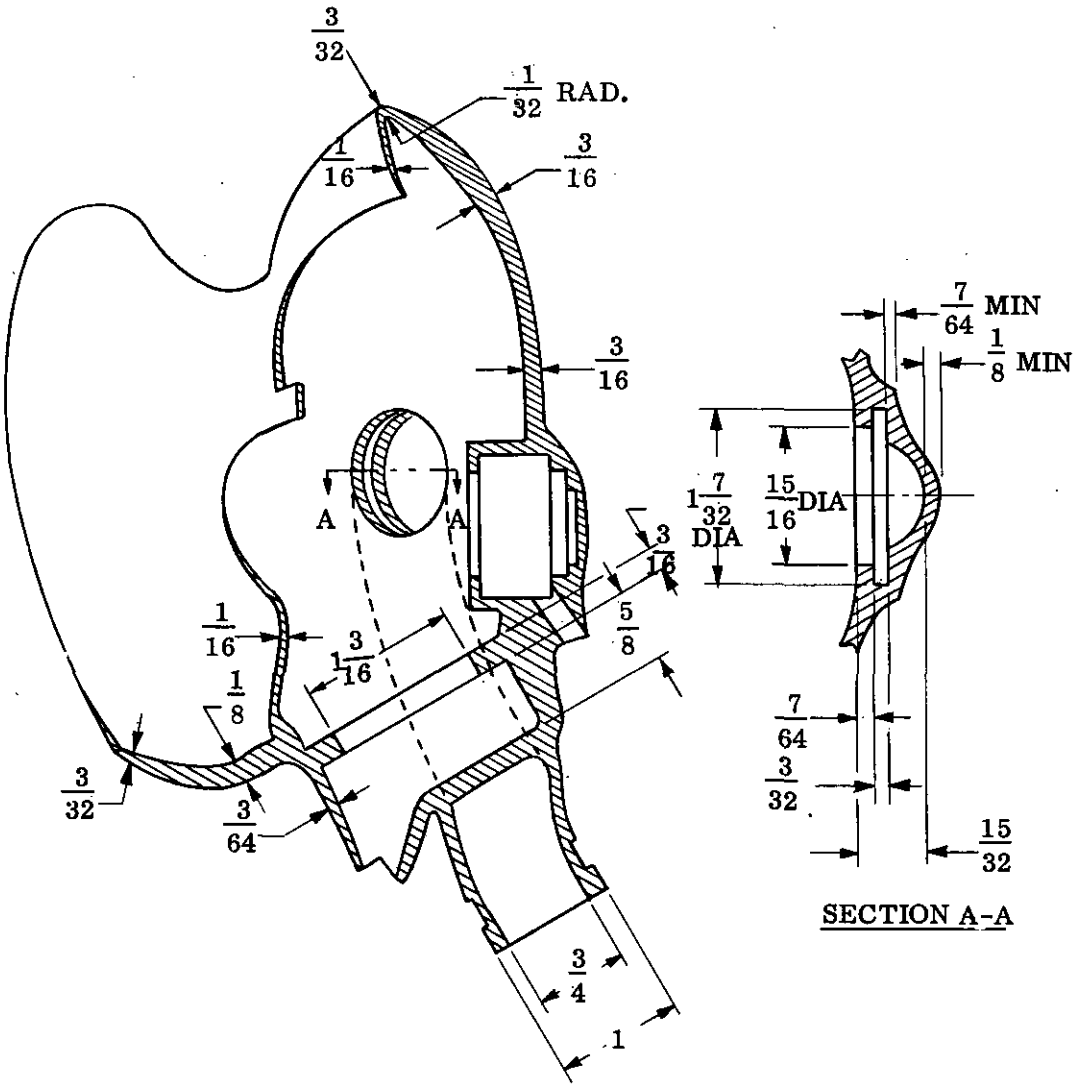

DIMENSIONS IN INCHES. UNLESS OTHERWISE SPECIFIED, TOLERANCES: FRACTIONS ± 1/32.

FIGURE 4. FIXED MASK DIMENSIONS


Source: https://assist.dla.mil -- Downloaded: 2026-10-17T07:05Z
Check the source to verify that this is the current version before use.

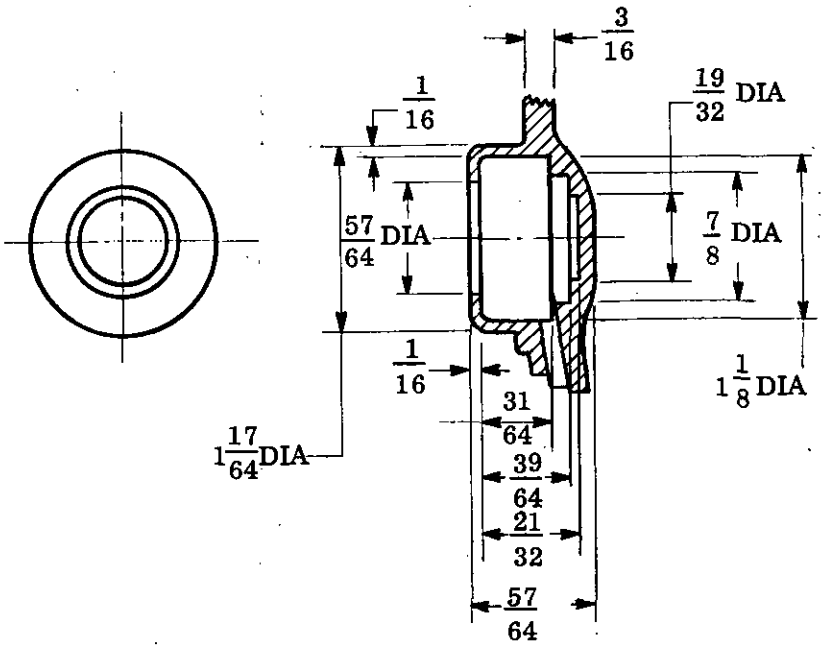

DIMENSIONS IN INCHES. UNLESS OTHERWISE SPECIFIED, TOLERANCES: FRACTIONS ± 1/64

FIGURE 5. MICROPHONE POCKET

Source: https://assist.dla.mil -- Downloaded: 2026-10-17T07:05Z
Check the source to verify that this is the current version before use.

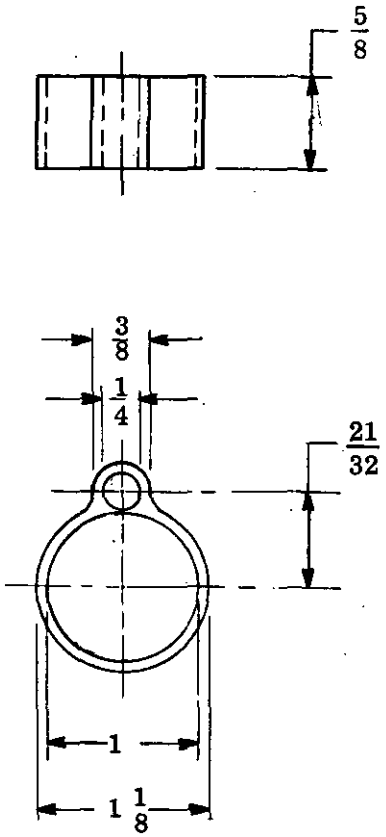


MATERIAL: RUBBER, MIL-R-6891 OR COMPRESSION MOLDED RUBBER USED IN FACEPEICE.

DIMENSIONS IN INCHES. UNLESS OTHERWISE SPECIFIED, TOLERANCES: FRACTIONS ± 1/64

FIGURE 6. MICROPHONE CABLE GUIDE (TYPE II)

Source: https://assist.dla.mil -- Downloaded: 2026-10-17T07:05Z
Check the source to verify that this is the current version before use.

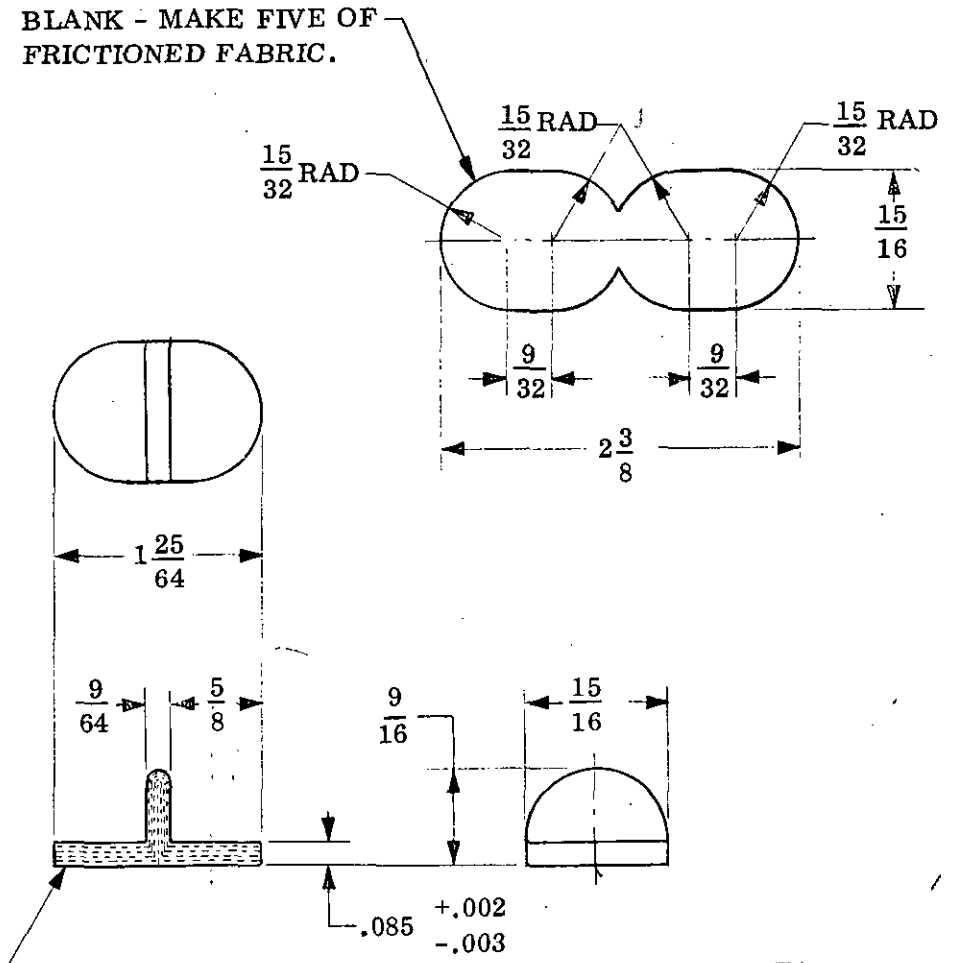


MATERIAL: BASE CLOTH CONFORMING TO MIL-C-5646.

DIMENSIONS IN INCHES. UNLESS OTHERWISE SPECIFIED, TOLERANCES: FRACTIONS ± 1/64.

FIGURE 7. LUG - LOWER (TYPE II)

Source: https://assist.dla.mil -- Downloaded: 202610-17T07:05Z
Check the source to verify that this is the current version before use.

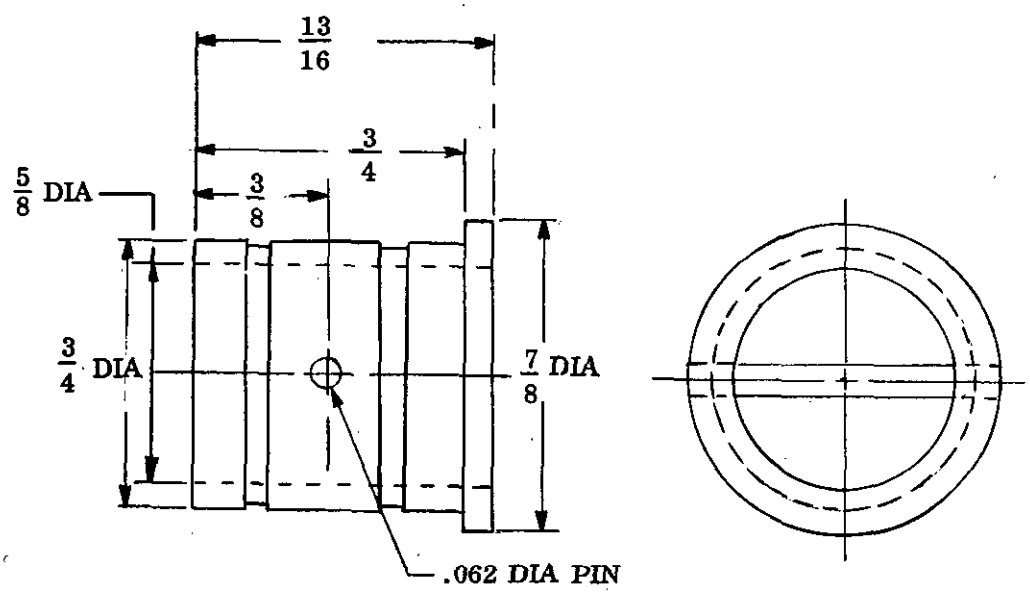

MATERIAL: INSERT, AL ALLOY, QQ-A-200/3, TEMPER T-4 OR QQ-A-225/3 T-4.
PIN, STEEL, MIL-S-7720, COMP 302, COND B OR COMMERCIAL PROD. EQUAL TO AND INTERCHANGEABLE WITH ROLL PIN, 79-018-078-0750, ELASTIC STOP-NUT CORP, UNION, NEW JERSEY

DIMENSIONS IN INCHES. UNLESS OTHERWISE SPECIFIED, TOLERANCES: DECIMALS ± 0.005, FRACTIONS ± 1/64.

FIGURE 8. METAL TUBING INSERT (TYPE II)

Source: https://assist.dla.mil -- Downloaded: 202610-17T07:05Z
Check the source to verify that this is the current version before use.


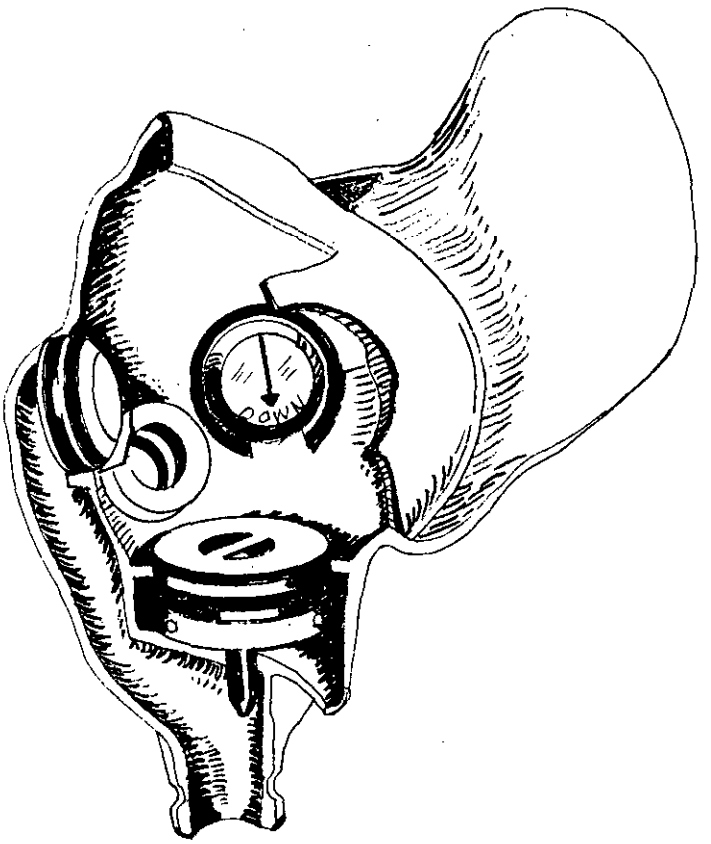


FIGURE 9. VALVE INSTALLATION


Source: https://assist.dla.mil -- Downloaded: 202640-17T07:05Z
Check the source to verify that this is the current version before use.

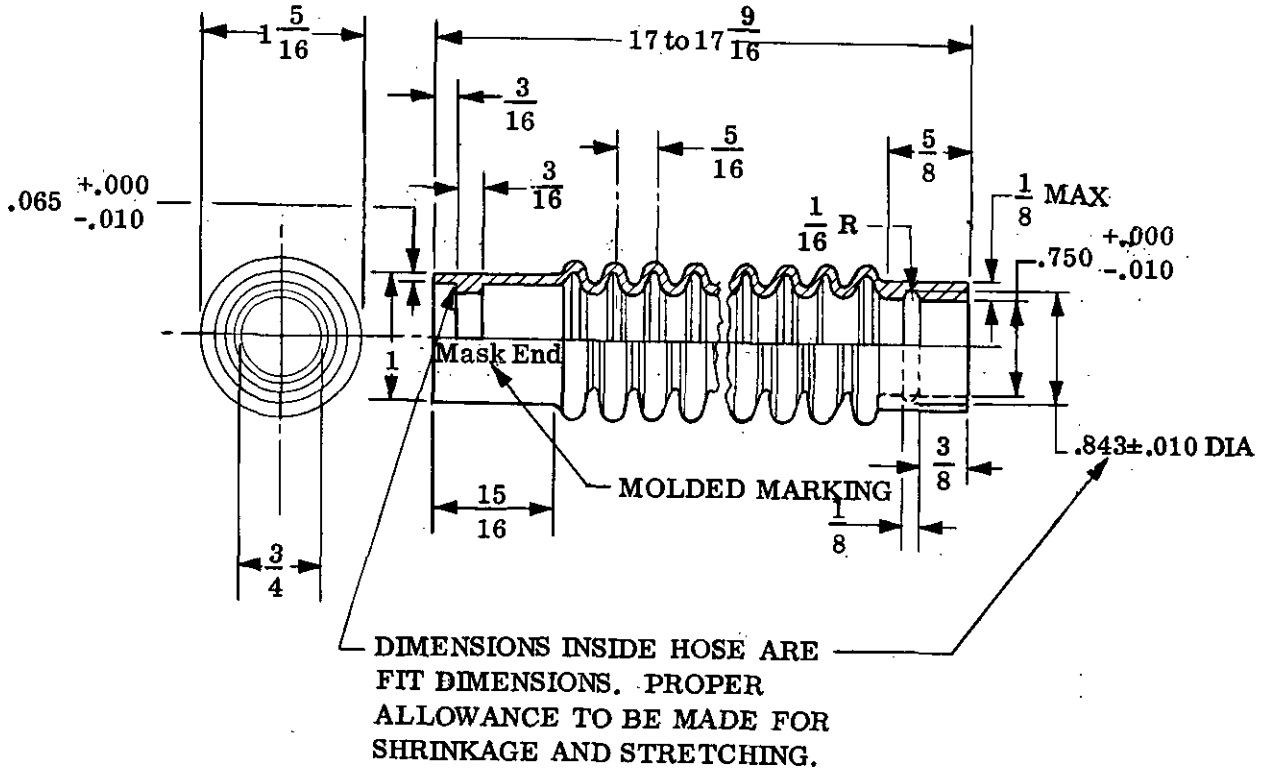

DIMENSIONS IN INCHES. UNLESS OTHERWISE SPECIFIED, TOLERANCES: FRACTIONS ± 1/16.

FIGURE 10. DELIVERY HOSE (TYPE II)

Source: https://assist.dla.mil -- Downloaded: 202610-17T07:05Z
Check the source to verify that this is the currenversion before use.

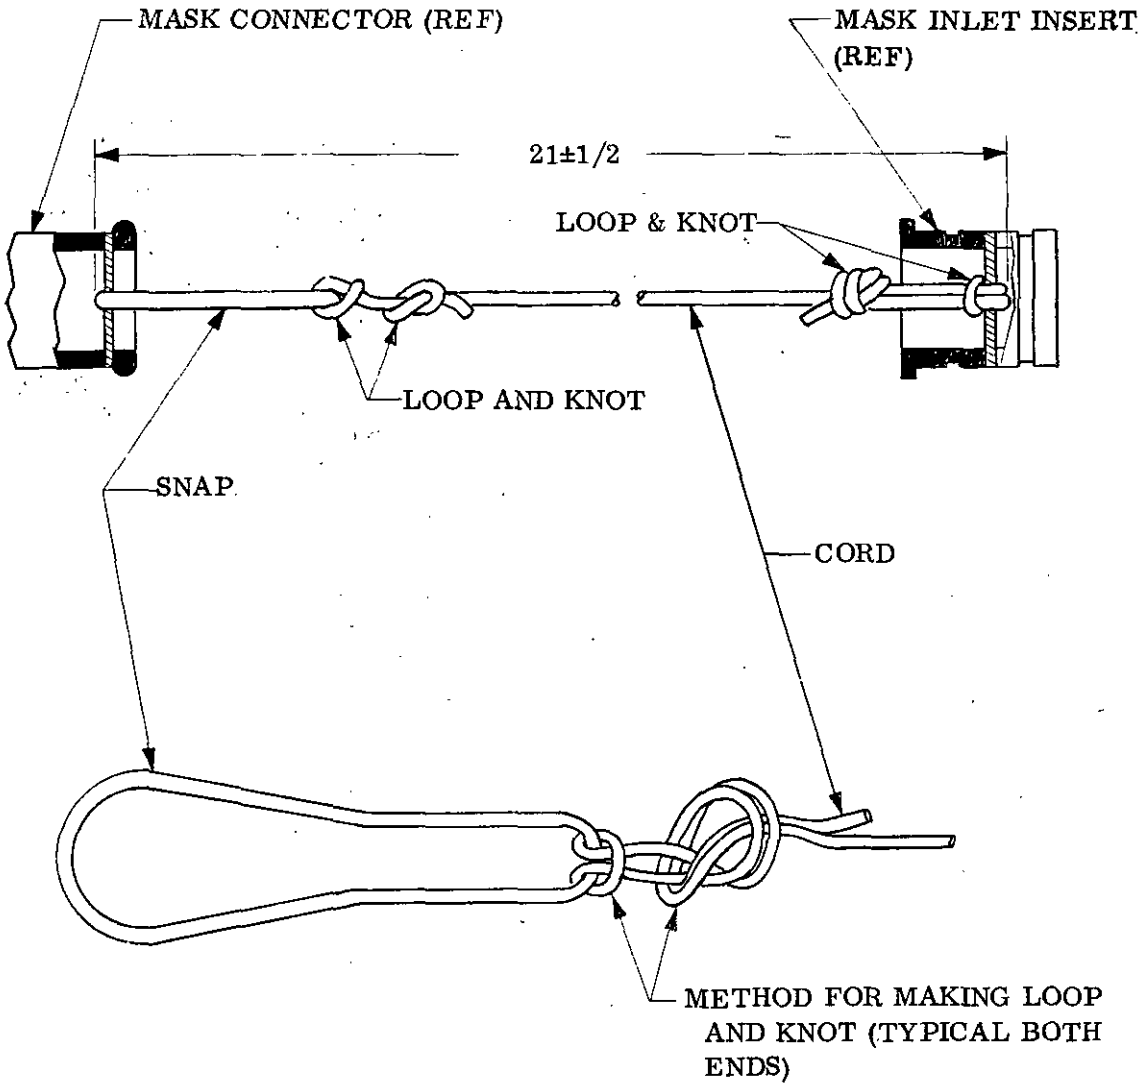


MATERIAL: SNAP, COMMERCIAL PRODUCT MUST BE EQUAL TO AND INTERCHANGEABLE WITH McMAHON, 110 LB TEST, SIZE 2/0, LENGTH 1-3/16, MARINE SPECIALTY MFG. CO. 1223 WESTERN AVE, SEATTLE, WASHINGTON OR EQUIVALENT. CORD, NYLON, MIL-C-5040, TYPE 1A, 100 LB TEST.

DIMENSIONS IN INCHES, UNLESS OTHERWISE SPECIFIED, TOLERANCES FRACTIONS ± 1/16.

FIGURE 11. DELIVERY HOSE LIMITING CORD (TYPE II)


Source: https://assist.dla.mil -- Downloaded: 202640-17T07:05Z
Check the source to verify that this is the current version before use.

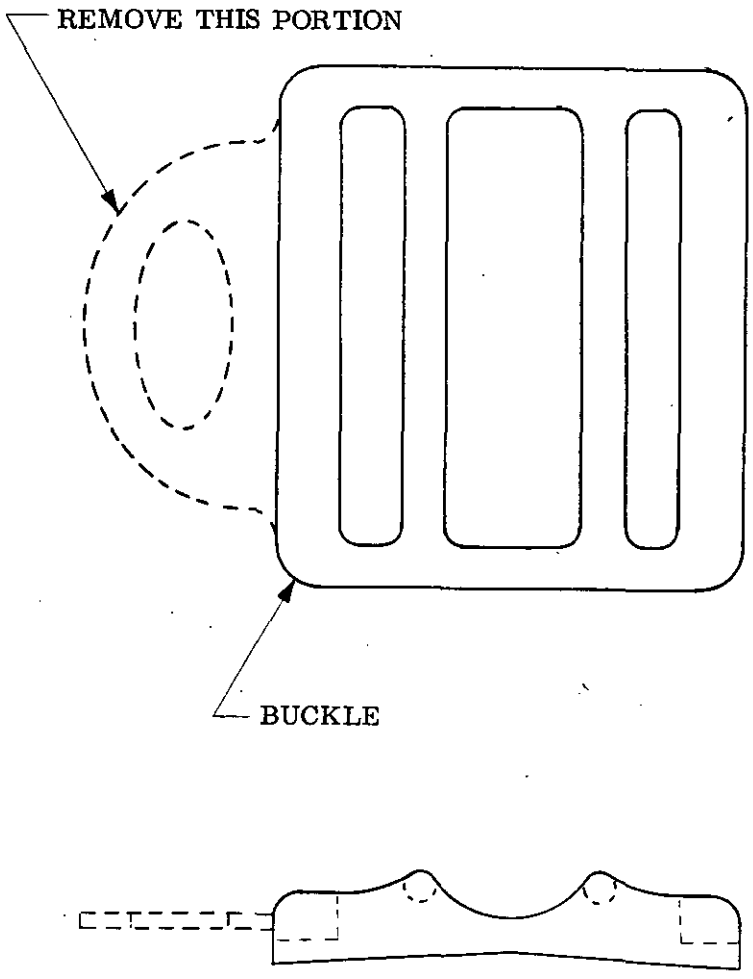

MATERIAL: BUCKLE, 3/4, TONGULESS, DOUBLE BAR, MIL-B-543, TYPE II, STYLE 2, CLASS 1. ALTER IN ACCORDANCE WITH THIS DRAWING.

FIGURE 12. BUCKLE (TYPE II)

Source: https://assist.dla.mil -- Downloaded: 2026-10-17T07:05Z
Check the source to verify that this is the current version before use.

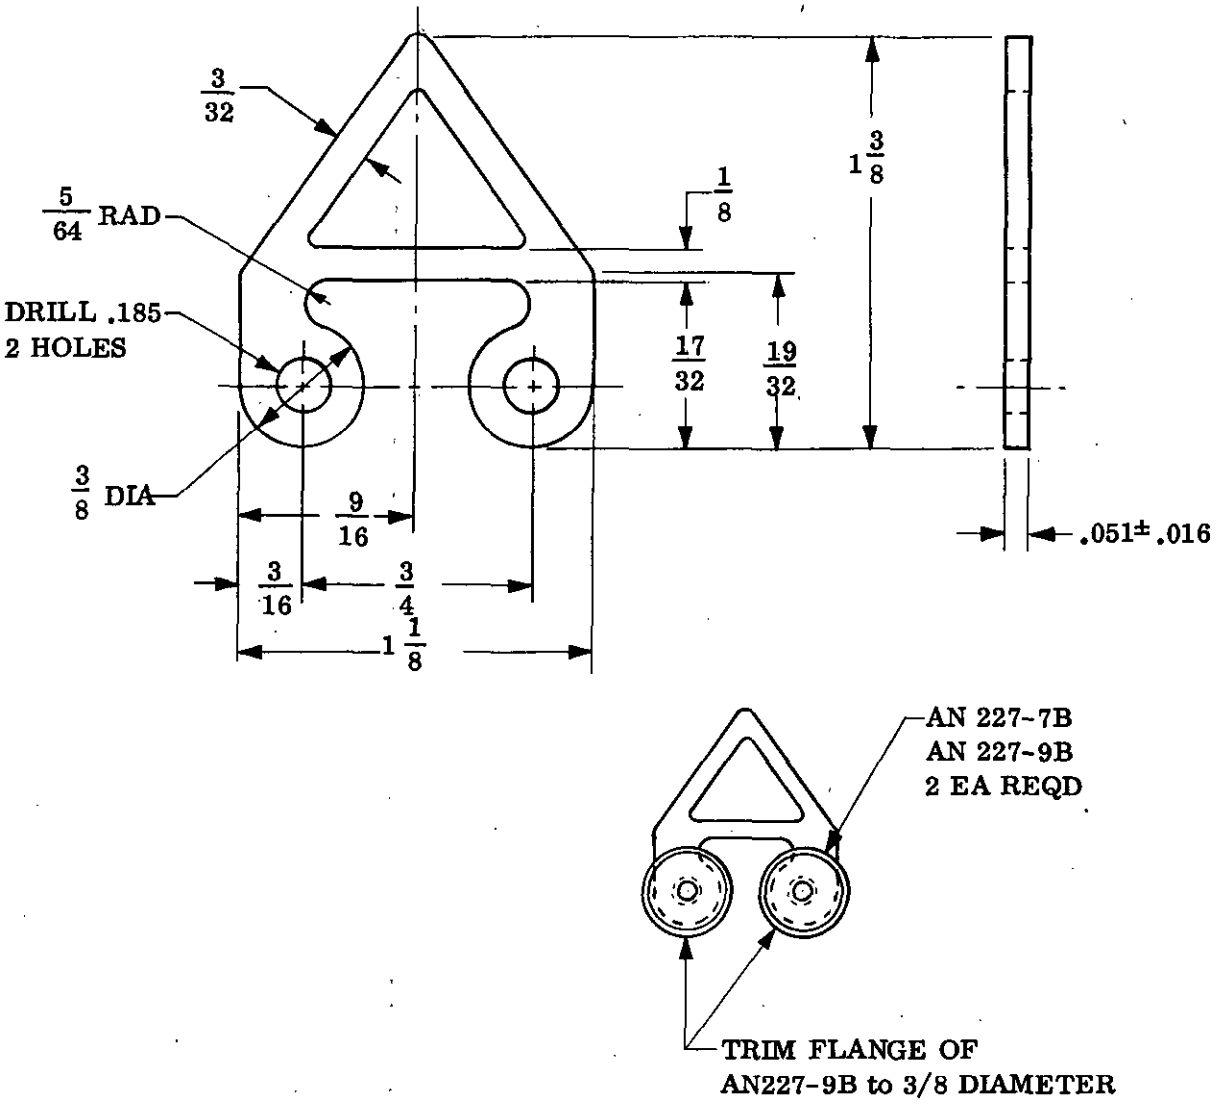

MATERIAL: BRASS, QQ-B-613, COMP, C, 1/2 HARD OR STEEL QQ-S-698, COND 2.


FINISH: BLACK OXIDE

REMOVE ALL BURRS AND SHARP EDGES

DIMENSIONS IN INCHES. UNLESS OTHERWISE SPECIFIED, TOLERANCES: FRACTIONS ± 1/64

FIGURE 13. SNAP FASTENER COMPONENT (TYPE II)


Source: https://assist.dla.mil -- Downloaded: 202640-17T07:05Z
Check the source to verify that this is the current version before use.

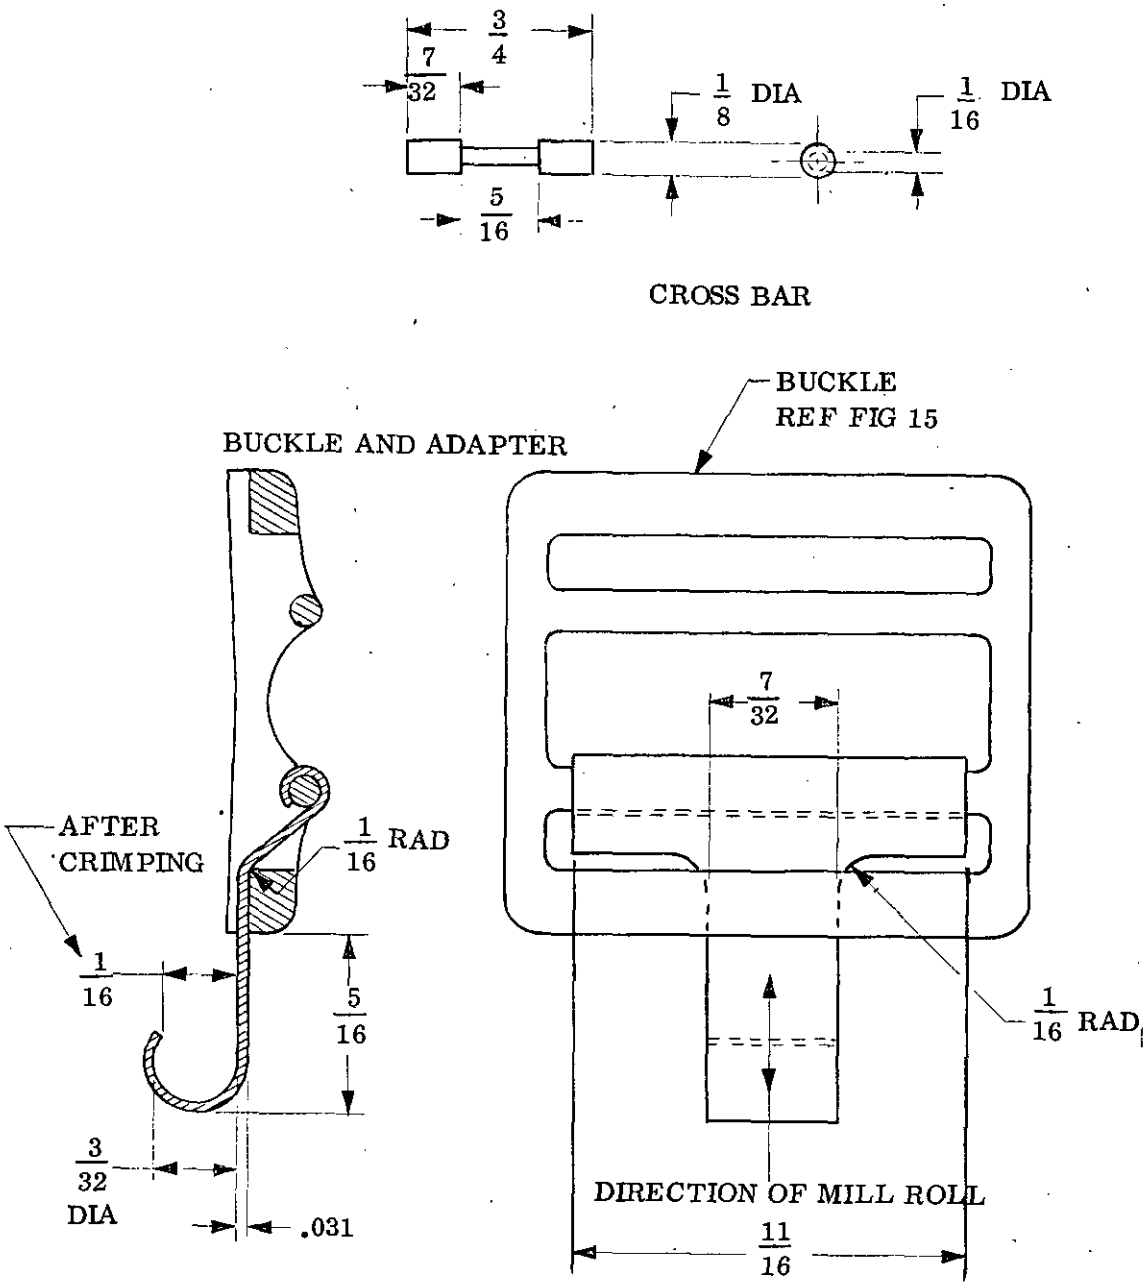

MATERIAL: STEEL, MIL-S-18729 COND. A
FINISH: BLACK OXIDE
DIMENSIONS IN INCHES. UNLESS OTHERWISE SPECIFIED, TOLERANCES:
FRACTIONS ±1 /64

FIGURE 14. BAR, ADAPTER AND BUCKLE ASSEMBLY (TYPE II)

Source: https://assist.dla.mil -- Downloaded: 2026-10-17T07:05Z
Check the source to verify that this is the current version before use.

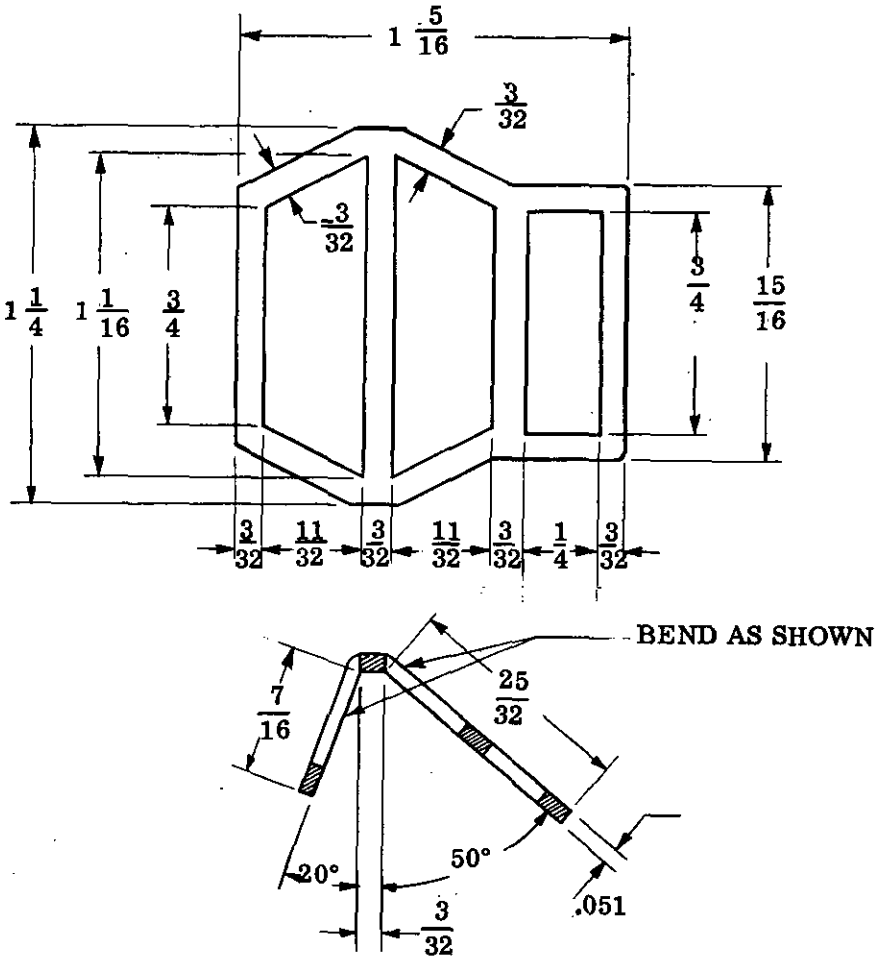


MATERIAL: BRASS, SPEC: QQ-B-613, COMP C, HALFHARD
FINISH: BLACK OXIDE

REMOVE ALL BURRS & SHARP EDGES.
DIMENSIONS IN INCHES. UNLESS OTHERWISE SPECIFIED, TOLERANCES:
ANGLES ±1°, DECIMALS ±0.005, FRACTIONS ±1/64

FIGURE 15. MASK HOOK (TYPE II)

Source: https://assist.dla.mil -- Downloaded: 202610-17T07:05Z
Check the source to verify that this is the current version before use.

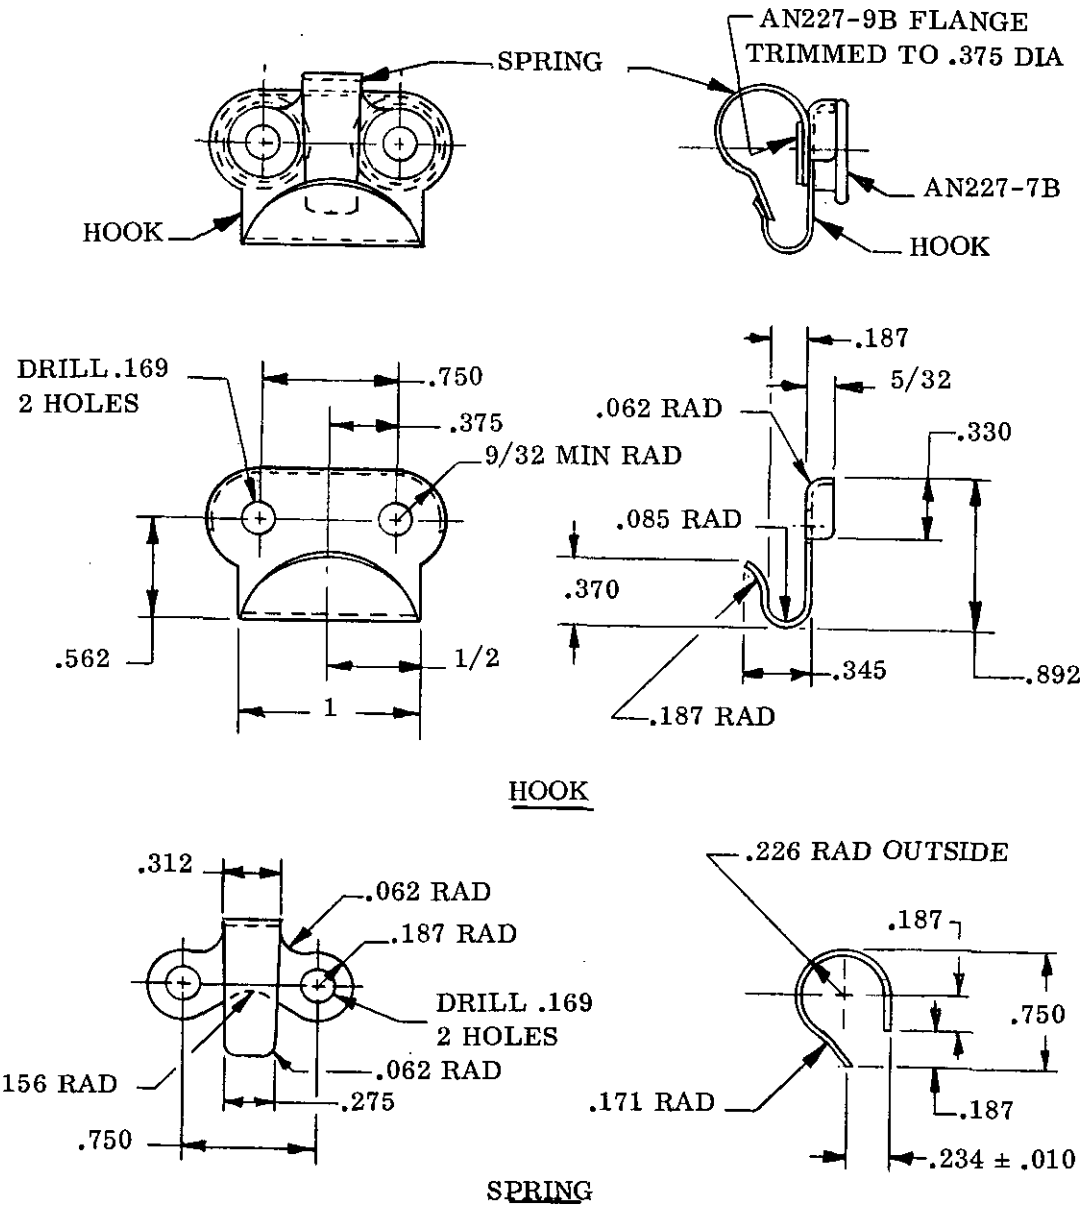

MATERIAL: HOOK, BRASS QQ-B-613, COMP C, 1/2 HARD.
SPRING, STEEL QQ-S-777, COND A. AFTER FORMING SPRING, METAL MUST BE HARDENED AND TEMPERED TO SPRING TENSION.
FINISH: BLACK OXIDE
REMOVE ALL BURRS AND SHARP EDGES.
DIMENSIONS IN INCHES. UNLESS OTHERWISE SPECIFIED, TOLERANCES: DECIMALS ±.005, FRACTIONS ±1/64

FIGURE 16. HELMET HOOK (TYPE II)

Source: https://assist.dla.mil -- Downloaded: 202640-17T07:05Z
Check the source to verify that this is the current version before use.

INDEX

CONTENTS	PARAGRAPH	PAGE
APPLICABLE DOCUMENTS	2	1
CLASSIFICATION	1.2	1
CLASSIFICATION OF DEFECTS		
Preparation for delivery	Table II	17
CLASSIFICATION OF INSPECTION	4.2	12
First article inspection	4.2 (b)	12
Qualification inspection	4.2 (a)	12
Quality conformance inspection	4.2 (c)	12
COLOR	3.8	11
DATA	6.4	25
DESIGN AND CONSTRUCTION	3.5	6
Clamp	3.5.5	8
Connector	3.5.6	8
Type I	3.5.6.1	8
Type II	3.5.6.2	8
Delivery hose	3.5.4	8
Type I	3.5.4.1	8
Type II	3.5.4.2	8
Delivery hose length-limiting cord	3.5.4.2.1	8
Exhalation valve	3.5.3	7
Inlet check valve	3.5.2	7
Mask	3.5.1	6
Dimensions	3.5.1.1	6
Facial fit	3.5.1.1.1	6
Fixed dimensions	3.5.1.1.2	6
Inlet ducts	3.5.1.4	7
Common inlet tube	3.5.1.4.2	7
Inlet insert (Type I)	3.5.1.4.2.1	7
Inlet insert (Type II)	3.5.1.4.2.2	7
Inlet port	3.5.1.4.1	7

Source: https://assist.dla.mil -- Downloaded: 202610-17T07:05Z
Check the source to verify that this is the current version before use.

INDEX (Continued)

CONTENTS	PARAGRAPH	PAGE
Microphone pocket	3.5.1.2	6
Cable guide (Type II)	3.5.1.2.2	7
Lead-in tube	3.5.1.2.1	6
Suspension lugs (Type II)	3.5.1.3	7
Lower lugs	3.5.1.3.1	7
Upper lugs	3.5.1.3.2	7
Suspension harness (Type II)	3.5.7	8
Hardware	3.5.7.2	9
Nosepiece	3.5.7.3	9
Straps	3.5.7.1	8
Assembly to mask	3.5.7.1.4	9
Strap, left side	3.5.7.1.3	9
Strap, nose	3.5.7.1.2	9
Strap, right side	3.5.7.1.1	9
FIGURES (1 to 16)		26 to 40
FIRST ARTICLE		
Inspection	4.4	13
Samples	4.4.1	13
Applicable to the Army	4.4.1.2	14
Applicable to the Naval Air Systems Command	4.4.1.1	13
Information	4.4.1.1.1	13
Requirements	3.2	5
IDENTIFICATION OF PRODUCT	3.9	11
INSPECTION METHODS	4.7	16
Delivery hose (Type II)	4.7.11	18
Delivery hose leakage	4.7.11.1	18
Delivery hose stretch	4.7.11.2	19
Disassembly and examination	4.7.14	19
Exhalation port icing	4.7.12	19
Exhalation valve installation	4.7.9	18
High and low temperature operation	4.7.4	17
High and low temperature storage	4.7.5	17
Inlet check valve installation (high suction)	4.7.8	18
Inlet check valve installation (low suction)	4.7.7	18

Source: https://assist.dla.mil -- Downloaded: 2026-10-17T07:05Z
Check the source to verify that this is the current version before use.

INDEX (Continued)

CONTENTS	PARAGRAPH	PAGE
Low temperature pliability	4.7.2	16
Low temperature starting delay	4.7.3	17
Lug strength (Type II)	4.7.13	19
Mask leakage	4.7.6	18
Material composition tests	4.7.15	19
Ozone resistance test (elastomer components)	4.7.15.2	19
Physical property tests (elastomer components)	4.7.15.1	19
Odor	4.7.10	18
Visual examination	4.7.1	16
Mask assembly	4.7.1.1	16
Dimensions	4.7.1.1.1	16
Preparation for delivery	4.7.1.2	16
INTENDED USE	6.1	23
INTERCHANGEABILITY	3.7	11
MATERIALS	3.4	5
Metal parts	3.4.1	5
Dissimilar metals	3.4.1.1	5
Nonmetallic material	3.4.2	5
Age	3.4.2.1	5
Elastomer components	3.4.2.2	5
Webbing (Type II)	3.4.2.3	6
Protective treatment	3.4.3	6
ORDERING DATA	6.2	24
PERFORMANCE	3.6	9
Delivery hose (Type II)	3.6.10.	10
Delivery hose leakage	3.6.10.1	10
Delivery hose stretch	3.6.10.2	10
Disassembly and examination	3.6.13	10
Exhalation port icing	3.6.11	10
Exhalation valve installation	3.6.8	10
High and low temperature operation	3.6.3	9
High and low temperature storage	3.6.4	10
Inlet check valve installation (high suction)	3.6.7	10
Inlet check valve installation (low suction)	3.6.6	10

Source: https://assist.dla.mil -- Downloaded: 202640-17T07:05Z
Check the source to verify that this is the current version before use.

INDEX (Continued)

CONTENTS	PARAGRAPH	PAGE
Low temperature pliability	3.6.1	9
Low temperature starting delay	3.6.2	9
Lug strength (Type II)	3.6.12	10
Mask leakage	3.6.5	10
Material composition tests	3.6.14	11
Ozone resistance (elastomer components)	3.6.14.2	11
Physical property tests (elastomer components)	3.6.14.1	11
Odor	3.6.9	10
PREPARATION FOR DELIVERY	5	21
Marking	5.3	23
Precautionary marking	5.3.1	23
Additional marking	5.3.1.1	23
Packaging	5.1	21
Intermediate	5.1.3	22
Level A	5.1.1	22
Level C	5.1.2	22
Packing	5.2	22
Level A	5.2.1	22
Level B	5.2.2	23
Level C	5.2.3	23
QUALIFICATION		
Information	6.5	25
Inspection	4.3	12
Samples	4.3.1	12
Requirements	3.1	5
QUALITY CONFORMANCE		
Inspection	4.5	14
Sampling	4.5.1	14
Inspection lot	4.5.1.1	14
Mask assembly	4.5.1.1.1	14
Preparation for delivery	4.5.1.1.2	14
Sampling for tests and examination of the mask assemblies	4.5.1.2	14

Source: https://assist.dla.mil -- Downloaded: 202610-17T07:05Z
Check the source to verify that this is the current version before use.

INDEX (Continued)

CONTENTS	PARAGRAPH	PAGE
Sample size, acceptance criteria, tests, and examination of the mask assemblies	Table I	15
RESPONSIBILITY FOR INSPECTION	4.1	12
SCOPE	1.1	1
SELECTION OF SPECIFICATIONS AND STANDARDS	3.3	5
TEST CONDITIONS	4.6	14
Gas	4.6.1	14
Temperature and pressure	4.6.2	16
WORKMANSHIP	3.11	11

☆U.S. GOVERNMENT PRINTING OFFICE:1970-433-693/8624

Source: https://assist.dla.mil -- Downloaded: 202610-17T07:05Z
Check the source to verify that this is the current version before use.

SPECIFICATION ANALYSIS SHEET

Form Approved
Budget Bureau No. 119-R004

INSTRUCTIONS

This sheet is to be filled out by personnel either Government or contractor, involved in the use of the specification in procurement of products for ultimate use by the Department of Defense. This sheet is provided for obtaining information on the use of this specification which will insure that suitable products can be procured with a minimum amount of delay and at the least cost. Comments and the return of this form will be appreciated. Fold on lines on reverse side, staple in corner, and send to preparing activity *(as indicated on reverse hereof)*.

SPECIFICATION MIL-M-6482D MASK ASSEMBLIES, OXYGEN, PRESSURE BREATHING

ORGANIZATION *(Of submitter)* | CITY AND STATE

CONTRACT NO. | QUANTITY OF ITEMS PROCURED | DOLLAR AMOUNT $

MATERIAL PROCURED UNDER A

☐ DIRECT GOVERNMENT CONTRACT ☐ SUBCONTRACT

1. HAS ANY PART OF THE SPECIFICATION CREATED PROBLEMS OR REQUIRED INTERPRETATION IN PROCUREMENT USE?

A. GIVE PARAGRAPH NUMBER AND WORDING.

B. RECOMMENDATIONS FOR CORRECTING THE DEFICIENCIES.

2. COMMENTS ON ANY SPECIFICATION REQUIREMENT CONSIDERED TOO RIGID

3. IS THE SPECIFICATION RESTRICTIVE?

☐ YES ☐ NO IF "YES", IN WHAT WAY?

4. REMARKS *(Attach any pertinent data which may be of use in improving this specification. If there are additional papers, attach to form and place both in an envelope addressed to preparing activity)*

SUBMITTED BY *(Printed or typed name and activity)* | DATE

DD, FORM 1426 APR 63 REPLACES NAVSHIPS FORM 4063, WHICH IS OBSOLETE C-8079

Source: https://assist.dla.mil -- Downloaded: 2026-10-17T07:05Z
Check the source to verify that this is the current version before use.