A-A-54306
17 December 1990

COMMERCIAL ITEM DESCRIPTION

PERIOSTEOTOME

The General Services Administration has authorized the use of this commercial item description as a replacement for Military Specification MIL-P-36976, which is cancelled

This commercial item description covers a costal periosteotome of the Alexander-Farabeuf design suitable for incision and detachment of the periosteum of the ribs during surgical procedures

Salient characteristics:

General The periosteotome shall be of the Alexander-Farabeuf style

Material The blade and shank shall be fabricated from Class 4 martensitic corrosion-resisting steel The handle shall be fabricated of brass having chromium over nickel plating As an alternate, the handle may be fabricated from Class 4 martensitic, or Class 3 austenitic corrosion-resistant steel The Class 3 and 4 steels shall be in accordance with ASTM Designation F899

Hardness The blade and shank shall have a Rockwell hardness C scale (HRC) of 50 min when tested in accordance with ASTM Designation E18 or E92 whichever is applicable Conversion of Vickers hardness values shall be in accordance with ASTM Designation E140

Style, design, and dimensions The periosteotome shall be in accordance with Figure 1

Finish The periosteotome shall have a mirror, or mirror and satin finish

Passivation The periosteotome shall be properly stress relieved and passivated.

AMSC N/A FSC 6515
DISTRIBUTION STATEMENT A Approved for public release, distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:32Z
Check the source to verify that this is the current version before use.

Corrosion resistance The periosteotome shall show no evidence of corrosion or plating of copper when tested in accordance with ASTM Designation F1089

Identification marking and labeling The periosteotome shall be legibly marked with the contractor's name or trademark and the word 'stainless' Foreign manufactured periosteotomes shall bear the name of the country of origin

Workmanship The periosteotome shall be free from burrs, cracks, sharp edges, scale, corrosion or other defects which detract from its appearance or impair its serviceability

Product Quality Level

Visual and dimensional examination The periosteotome shall be examined to verify that design, construction and workmanship are in accordance with applicable requirements

Materials The supplier shall be responsible for performing tests to assure that materials are in accordance with specification requirements

Unit Each (EA) One periosteotome, as specified, constitutes one unit

QUALITY ASSURANCE PROVISIONS

Responsibility for inspection Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein Except otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements

Records Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:32Z
Check the source to verify that this is the current version before use.

Inspection Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means and chemical properties) of the item

Sampling for examination Sampling for examination shall be conducted in accordance with MIL-STD-105, and as specified herein Unit of product for examination purposes shall be one periosteotome Sampling shall be Inspection level II with an acceptable quality level (AQL) of 1 0

Examination Examination shall be conducted to determine compliance with specification requirements

Sampling for tests Sampling for tests shall be conducted in accordance with MIL-STD-105 and as specified herein The unit of product for test purposes shall be one periosteotome Sampling shall be inspection level S-2 with an AQL of 1 0

Tests Tests shall be conducted to determine compliance with specification requirements Where feasible, the same sample shall be used for the determination of two or more text characteristics

Contractor certification The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producers'own drawings, specifications, standards, and quality assurance practices The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract

Metric products Products manufactured to metric dimensions will be considered on an equal basis with those manufactured using inch-pound units, providing they fall within the tolerances specified using conversion tables contained in the latest revision of Federal Standard No 376, and all other requirements of this document are met

If a product is manufactured to metric dimensions and those dimensions exceed the tolerances specified in the inch/pound units, a request should be made to the contracting officer to determine if the product is acceptable.

The contracting officer has the option of accepting or rejecting the product

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:32Z
Check the source to verify that this is the current version before use.

Regulatory requirements

Federal Food, Drug, and Cosmetic Act If the product covered by this document has been determined by the U S Food and Drug Administration to be under its jurisdiction , the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug Cosmetic Act as amended, and regulations promulgated thereunder In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal State, and local statutes, ordinances, and regulations

Recovered materials The offeror/contractor is encouraged to use recovered material in accordance with Federal Acquisition Regulation Subpart 23 4 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc , involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and /or order

NOTE The following National Stock Number is covered by this document·

NSN	ITEM IDENTIFICATION
6515-00-355-3300	Periosteotome, Alexander-Farabeuf

Ordering data (Intermediate/exterior package quantities and labeling and marking must be specified in the contract and/or order)

MILITARY INTERESTS

Custodians·

Army - MD
Navy - MS
Air Force - 03

Preparing Activity

DoD-MB

Agent

DLA-DM


Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:32Z
Check the source to verify that this is the current version before use.

CIVIL AGENCY COORDINATING ACTIVITIES

VA-OSS
PHS
FDA-MPQAS

Project No 6515-4866

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:32Z
Check the source to verify that this is the current version before use.

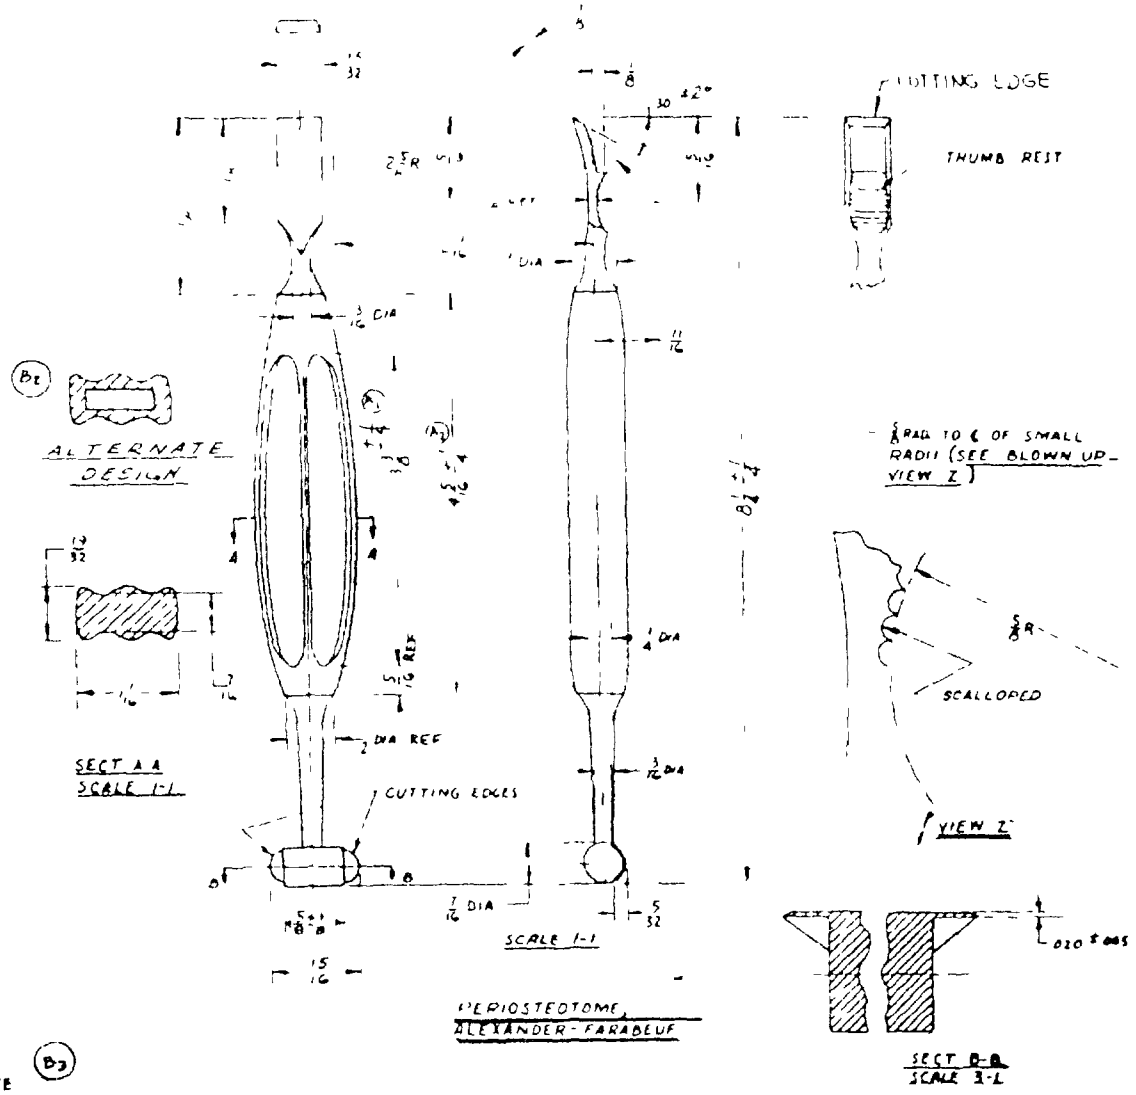

NOTE

TOLERANCES INDICATED DELINEATE ACCEPTABLE EXTREME DIMENSIONS, AND ARE NOT INTENDED TO PERMIT VARIATIONS WITHIN A SINGLE INSTRUMENT WHICH WILL SACRIFICE UNIFORMITY, SYMMETRY AND FIRST QUALITY WORKMANSHIP

DIMENSIONS ARE IN INCHES.
UNLESS OTHERWISE SPECIFIED
TOLERANCES ON FRACTIONS ± 1/32

FIGURE 1

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:32Z
Check the source to verify that this is the current version before use.

INSTRUCTIONS. In a continuing effort to make our standardization documents better, the DoD provides this form for use in submitting comments and suggestions for improvements. All users of military standardization documents are invited to provide suggestions. This form may be detached, folded along the lines indicated, taped along the loose edge *(DO NOT STAPLE)*, and mailed. In block 5, be as specific as possible about particular problem areas such as wording which required interpretation, was too rigid, restrictive, loose, ambiguous, or was incompatible, and give proposed wording changes which would alleviate the problems. Enter in block 6 any remarks not related to a specific paragraph of the document. If block 7 is filled out, an acknowledgement will be mailed to you within 30 days to let you know that your comments were received and are being considered.

NOTE. This form may not be used to request copies of documents, nor to request waivers, deviations, or clarification of specification requirements on current contracts. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements.

(Fold along this line)

(Fold along this line)

NO POSTAGE NECESSARY IF MAILED IN THE UNITED STATES

OFFICIAL BUSINESS
PENALTY FOR PRIVATE USE $300

BUSINESS REPLY MAIL
FIRST CLASS PERMIT NO 4966 Alexandria, VA

POSTAGE WILL BE PAID BY

Commander
Defense Personnel Support Center
ATTN DPSC-WQE
2800 South 20th Street
Philadelphia, Pennsylvania 19101-8419

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:32Z
Check the source to verify that this is the current version before use.

(TO DETACH THIS FORM, CUT ALONG THIS LINE.)

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

(See Instructions - Reverse Side)

1 DOCUMENT NUMBER	2 DOCUMENT TITLE
A-A-54306	PERIOSTEOTOME

3a. NAME OF SUBMITTING ORGANIZATION	4 TYPE OF ORGANIZATION *(Mark one)*
	☐ VENDOR
b ADDRESS *(Street, City State ZIP Code)*	☐ USER
	☐ MANUFACTURER
	☐ OTHER *(Specify)* _____

5 PROBLEM AREAS

a. Paragraph Number and Wording

b. Recommended Wording

c. Reason/Rationale for Recommendation

6 REMARKS

7a NAME OF SUBMITTER *(Last First MI)* – Optional	b WORK TELEPHONE NUMBER *(Include Area Code)* – Optional
c MAILING ADDRESS *(Street City State, ZIP Code)* – Optional	8 DATE OF SUBMISSION (YYMMDD)

DD Form 1426

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:32Z
Check the source to verify that this is the current version before use.