A-A-54315
11 January 1991

COMMERCIAL ITEM DESCRIPTION

CATHETERS, UMBILICAL

The General Services Administration has authorized the use of this commercial item description as a replacement for Military Specification MIL-C-37063 (1), which is cancelled.

This commercial item description covers sterile, umbilical catheters suitable for insertion into the umbilical arteries or veins of neonates for measuring blood pressure, blood chemistry, blood volume, and for administering venous infusions and exchange transfusions.

Salient characteristics:

General. This specification covers the following sizes of umbilical catheters:

Size 1	3.5 Fr.
Size 2	5 Fr
Size 3	8 Fr.

Material. The umbilical catheters shall be made of clear, transparent plastic and be suitably soft for vascular insertion without injury. The catheters shall be sterile, non-pyrogenic, and conform to USP Class IV plastics requirements. Lead content shall not exceed 5 ppm.

Style, design and dimensions. The umbilical catheters shall be 15 inches long have a radiopaque line along its length, and be marked at the 5, 10, and 15 centimeter distances from the distal end. All surfaces shall be smooth. The distal end shall have an open tip with no lateral eyes. The proximal end shall form a tight, leak-proof fit with a male Luer connector in accordance with ANSI/HIMA MD70.1. The catheters shall be in accordance with Figure 1.

Performance. The umbilical catheters shall demonstrate breaking strengths of 2.5 lbs., 6.0 lbs , and 8.0 lbs., minimum, for the 3.5 Fr, 5 Fr, and 8.0 Fr catheter sizes respectively. Catheters shall also have a Shore Durometer Hardness and ultimate elongation of 85 + 5 (Shore A, 10 seconds) and 200% respectively. Units shall be shown to be free of foreign matter when tested as specified herein

AMSC N/A FSC 6515

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:32Z
Check the source to verify that this is the current version before use.

Sterility. The umbilical catheters shall be sterile in accordance with the USP, or AAMI requirements. Sterility assurance level shall be 0.000001.

Breaking strength. The breaking strength of the catheter and suction tubing shall be determined in accordance with ASTM Designation D412

Ultimate elongation. The ultimate elongation of the catheter and suction tubing shall be determined in accordance with ASTM Designation D412.

Suitability. The plastic catheter tubing of the unit shall be suitable in accordance with the United States Pharmacopeia (USP) for Class IV plastics.

Safety and freedom from pyrogens. The catheters shall be safe and free from pyrogens in accordance with the USP.

Freedom from foreign matter. The inside of the vial and lumen of tubes shall be viewed from a distance of 14 inches without magnification. Illumination of units shall be twin, 15 watt cool-white fluorescent tubes.

Workmanship. The umbilical catheters shall be processed in such a manner as to be uniform and free from defects which affect life, performance, utility, or appearance.

Product Quality Level

Visual and dimensional examination. Shall be examined to verify that design, construction and workmanship are in accordance with applicable requirements.

Materials. The supplier shall be responsible for performing tests to assure that materials are in accordance with requirements specified.

Unit. Package (PG). One package containing 10 individually packaged sterile catheters, as specified, constitutes one unit. The individual package shall be sealed, peel open type container capable of maintaining sterility of contents unless package is damaged or opened.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:32Z
Check the source to verify that this is the current version before use.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Examination. The umbilical catheters shall be examined to determine compliance with all requirements contained in this specification.

Sampling for examination. Sampling for examination shall be conducted in accordance with MIL-STD-105. The inspection level shall be II with an AQL of 1.0 (percent defective). The unit of product for examination purposes shall be one catheter.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more test characteristics.

Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and as specified herein. The unit of product for test purposes shall be one catheter. Inspection level shall be S-2 with an AQL of 1.0 (percent defective).

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:32Z
Check the source to verify that this is the current version before use.

Contractor certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Metric products. Products manufactured to metric dimensions will be considered on an equal basis with those manufactured using inch pound units, providing they fall within the tolerances specified using conversion tables contained in the latest revision of Federal Standard No. 376, and all other requirements of this document are met.

If a product is manufactured to metric dimensions and those dimensions exceed the tolerances specified in the inch/pound units, a request should be made to the contracting officer to determine if the product is acceptable.

The contracting officer has the option of accepting or rejecting the product.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Federal Acquisition Regulation Subpart 23.4 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:32Z
Check the source to verify that this is the current version before use.

NOTE: The following National Stock Numbers their respective Item Identifications and Sizes are covered by this document:

NSN	ITEM IDENTIFICATION	SIZE
6515-00-133-5877	CATHETER, UMBILICAL, Polyvinyl Chloride, Disposable, 5 Fr 10s	2
6515-00-360-5162	CATHETER, UMBILICAL Polyvinyl Chloride, Disposable, 3-1/2 Fr 10s	1
6515-00-360-5163	CATHETER, UMBILICAL, Polyvinyl Chloride, Disposable, 8 Fr, 10s	3

Ordering data (intermediate/exterior package guarantees and labeling and marking must be specified in the contract and/or order).

MILITARY INTERESTS:

Custodians:

Army - MD
Navy - MS
Air Force - 03

Preparing Activity:

DoD-MB

Agent:


DLA-DM

CIVIL AGENCY COORDINATING ACTIVITIES:

VA-OSS
PHS
FDA-MPQAS

Project No. 6515-4248

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:32Z
Check the source to verify that this is the current version before use.

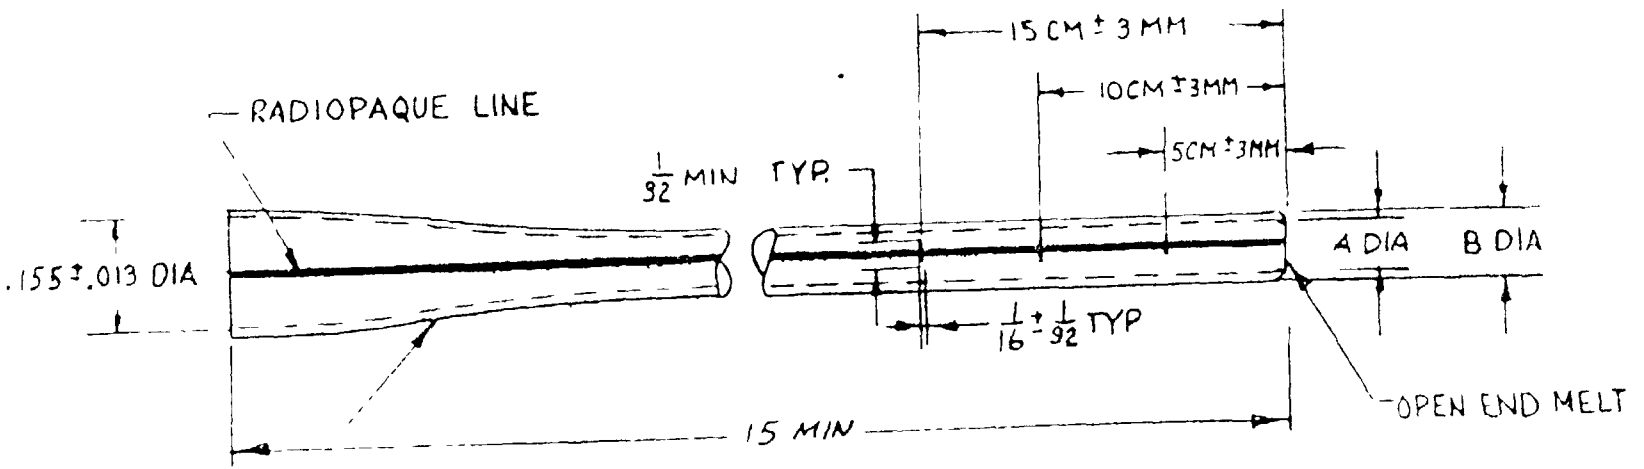

DIMENSIONS ARE IN INCHES, UNLESS OTHERWISE STATED.

NSN	SIZE	DIMENSIONS	A ±.013	B ± .01
6515-00-360-5162	A	3½ FR	.025	.043
6515-00-133 5877	B	5 FR.	.037	.063
6515-00-360-5163	C	8 FR.	068	.102

CATHETER, UMBILICAL, POLYVINYL CHLORIDE, DISPOSABLE

FIGURE 1

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:32Z
Check the source to verify that this is the current version before use.

INSTRUCTIONS In a continuing effort to make our standardization documents better, the DoD provides this form for use in submitting comments and suggestions for improvements. All users of military standardization documents are invited to provide suggestions. This form may be detached, folded along the lines indicated, taped along the loose edge *(DO NOT STAPLE)*, and mailed. In block 5, be as specific as possible about particular problem areas such as wording which required interpretation, was too rigid, restrictive, loose, ambiguous, or was incompatible, and give proposed wording changes which would alleviate the problems. Enter in block 6 any remarks not related to a specific paragraph of the document. If block 7 is filled out, an acknowledgement will be mailed to you within 30 days to let you know that your comments were received and are being considered.

NOTE This form may not be used to request copies of documents, nor to request waivers, deviations, or clarification of specification requirements on current contracts. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements.

(Fold along this line)

(Fold along this line)

NO POSTAGE NECESSARY IF MAILED IN THE UNITED STATES

OFFICIAL BUSINESS
PENALTY FOR PRIVATE USE $300

BUSINESS REPLY MAIL
FIRST CLASS PERMIT NO 4966 Alexandria, VA

POSTAGE WILL BE PAID BY

Commander
Defense Personnel Support Center
ATTN: DPSC-MSTE
2800 South 20th Street
Philadelphia, Pennsylvania 19101-8419

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:32Z
Check the source to verify that this is the current version before use.

(TO DETACH THIS FORM, CUT ALONG THIS LINE.)

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

(See Instructions – Reverse Side)

1 DOCUMENT NUMBER	2 DOCUMENT TITLE
A-A-54315	CATHETERS, UMBILICAL

3a NAME OF SUBMITTING ORGANIZATION

b ADDRESS *(Street, City, State, ZIP Code)*

4 TYPE OF ORGANIZATION *(Mark one)*

- ☐ VENDOR
- ☐ USER
- ☐ MANUFACTURER
- ☐ OTHER *(Specify)* _____

5 PROBLEM AREAS

a. Paragraph Number and Wording

b. Recommended Wording

c. Reason/Rationale for Recommendation

6 REMARKS

7a NAME OF SUBMITTER *(Last, First, MI)* – Optional	b WORK TELEPHONE NUMBER *(Include Area Code)* – Optional
c MAILING ADDRESS *(Street, City, State, ZIP Code)* – Optional	8 DATE OF SUBMISSION *(YYMMDD)*

DD FORM 1426 PREVIOUS EDITION IS OBSOLETE

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:32Z
Check the source to verify that this is the current version before use.