[METRIC]
A-A-54322
4 February 1991

COMMERCIAL ITEM DESCRIPTION

BROACH, PULP CANAL, BARBED, STERILE

The General Services Administration has authorized the use of this Commercial Item Description as a replacement for Military Specification MIL-B-42027 which is cancelled.

Salient Characteristics:

This commercial item description covers sterile barbed pulp canal broaches designed for use in extirpating pulpal tissue and debridement of pulp canals during endodontic procedures.

General. Except as noted below, the broaches shall be in accordance with ANSI (American National Standards Institute)/ADA (American Dental Association) No. 63 for type I barbed broaches. In case of a conflict, this document shall govern.

Classification. The barbed pulp canal broaches shall be furnished in the following sizes, as specified.

Size XF - Extra Fine
Size M - Medium
Size C - Coarse

Material. The operative end of the broach shall be fabricated from Class 3 corrosion-resistant steel type 301 or 302 with a minimum tensile strength of 1715 MPa when tested as specified herein. The steel shall be in accordance with ASTM F899. The handle shall be fabricated from rigid plastic.

Style, and design. Barbed broaches shall be of two-piece construction, consisting of an operative end (working end, neck, and shank) and a handle. The barbed broaches shall be for use in extirpating pulpal tissue and debridement of pulp canals during endodontic procedures. The broaches shall be straight. The full diameter of the wire shall be present over the entire length of the shank portion of the broach. The barbs shall be properly cut to a depth of 10 to 15 percent of the diameter of the working end. The cross section of each barb shall increase parabolically from the tip to the base of the barb.

AMSC N/A FSC 6520

DISTRIBUTION STATEMENT A: Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:32Z
Check the source to verify that this is the current version before use.

Broaches shall be tapered for their full working length, with barbs arranged in uniformly spaced helical rows, projecting from the working end.

The shape of the tip shall be optional. The style and design of the broaches shall in accordance with Figure 1.

Handles. In addition to the requirements of ADA 63, the handle shall meet the following requirements. The handles shall be designed to provide proper finger-gripping. The handles shall be longitudinally serrated or shall have cross cut serrations. The entire handle shall be serrated or as an alternate only the finger-gripping portion shall be serrated.

Sterility. Sterility shall be in accordance with the USP or AAMI guidelines with a Sterility Assurance level of 1×10^{-6}.

Corrosion resistance. The broaches shall show no evidence of corrosion when tested in accordance with ASTM 1089.

Finish. The barbed section of the broach shall have a bright and smoothly cut finish. The broach shall be free from burrs, scales, rough areas and grid marks.

Identification marking. The handles shall be color coded in accordance with ADA 63.

Workmanship. The broaches shall be free from any defects that may detract from their appearance or impair their serviceability, proper functioning or intended use.

Unit. Package (PG). One package containing thirty sterile broaches, as specified, constitutes one unit. Each broach shall be compartmentalized and sealed to allow individual usage without contamination of the remainder.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:32Z
Check the source to verify that this is the current version before use.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after the delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Certificates of quality. Certificates of quality, supplied by the manufacturer of the materials, may be furnished in lieu of actual performance of such testing by the contractor, provided lot identity has been maintained and can be demonstrated to the Government.

Sampling for examination. Sampling for examination shall be conducted in accordance with MIL-STD-105, with an inspection level of II with an AQL of 2.5 (percent defective). The unit of product for examination purposes shall be one broach.

Examination. Examination shall be conducted to determine compliance with specification requirements.

Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105, with an inspection level of S-2, with an AQL of 1.0 (percent defective). The unit of product for test purposes shall be one broach.

Tensile strength. Tensile strength shall be performed in a tension tester on a 20 cm sample of steel stock used to produce the broaches.

Diameter. The broach diameter at the tip, 3 mm and 10.5 mm from the tip shall be measured.

Contractor certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producer's own drawings, specifications, standards, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:32Z
Check the source to verify that this is the current version before use.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Federal Acquisition Regulation Subpart 23.4 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment for the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling marking shall be as specified in the contract and/or order.

NOTE: The following National Stock Numbers are covered by this document:

National Stock Number	Item Identification
6520-01-221-9089	BROACH, PULP CANAL, BARBED, Medium, Straight, 30: Sterile
6520-01-221-9090	BROACH, PULP CANAL, BARBED, Coarse, Straight, 30: Sterile
6520-01-222-9974	BROACH, PULP CANAL, BARBED, Extra-fine, Straight, 30: Sterile

Ordering data. Intermediate/exterior package quantities, labeling, and marking must be specified in the contract and/or order.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:32Z
Check the source to verify that this is the current version before use.

MILITARY INTERESTS:

Custodians:

Army-MD
Navy-MS
Air Force-03

PREPARING ACTIVITY:

DoD-MB

Agent:


DLA-DM

CIVIL AGENCY COORDINATING ACTIVITIES:

VA-OSS
PHS
FDA-MPQAS


PROJECT NO. 6520-2274
LOCATION: Word/BROACH1

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:32Z
Check the source to verify that this is the current version before use.

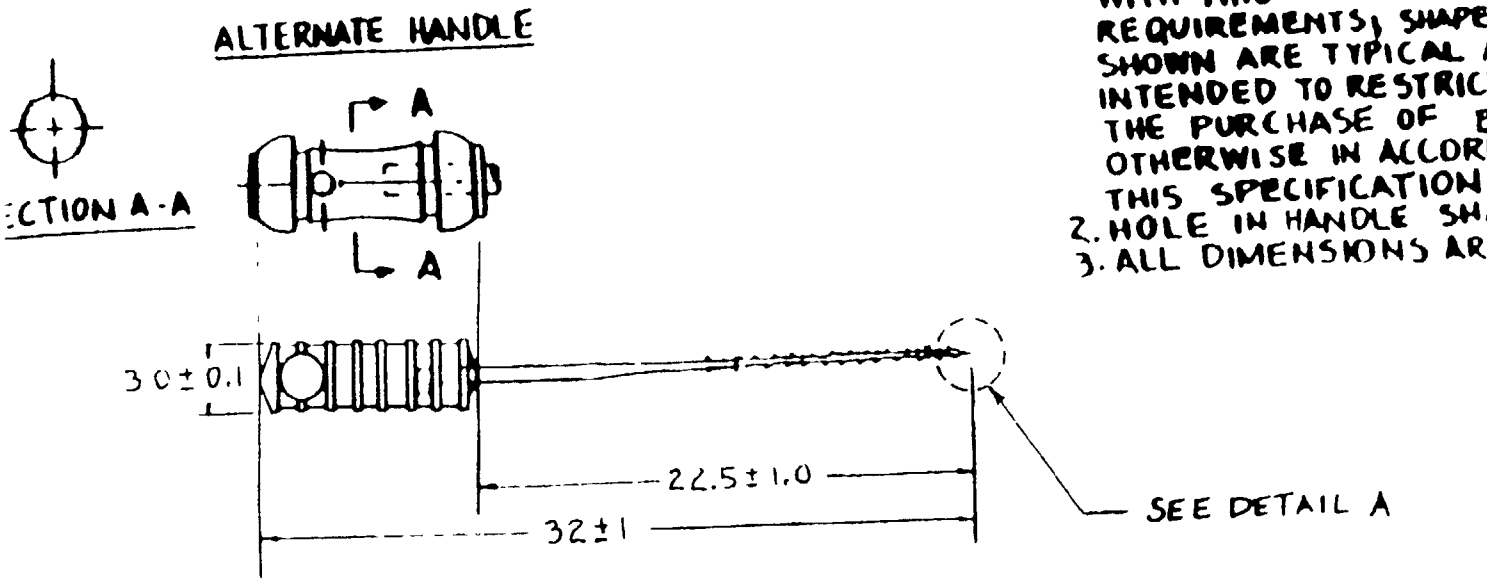

NOTES:

1. HANDLES SHALL BE IN ACCORDANCE WITH THIS FIGURE FOR DIMENSIONAL REQUIREMENTS; SHAPE OF HANDLES SHOWN ARE TYPICAL AND ARE NOT INTENDED TO RESTRICT OR PRECLUDE THE PURCHASE OF BROACHES WHICH ARE OTHERWISE IN ACCORDANCE WITH THIS SPECIFICATION.
2. HOLE IN HANDLE SHALL BE OPTIONAL.
3. ALL DIMENSIONS ARE IN MILLIMETERS.

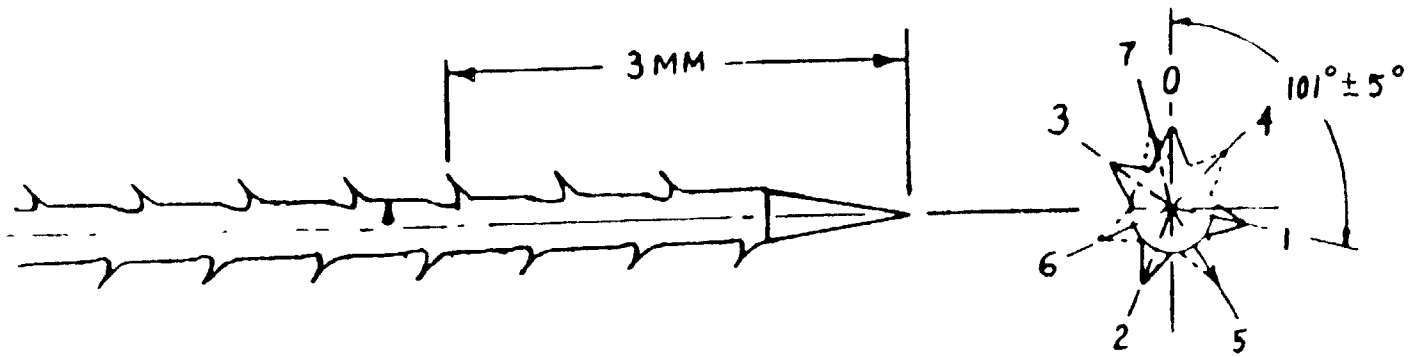

DETAIL A
(ENLARGED)

NOTE:

BARB DISTANCE IS 101° WITH A STEADY SPIRAL INCLINATION OF 0.9 MM REF. BY 360° IN SEQUENCE 1 THRU 7 AS SHOWN.

FIGURE 1 BROACH, PULP CANAL, BARBED, STERILE

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:32Z
Check the source to verify that this is the current version before use.

INSTRUCTIONS: In a continuing effort to make our standardization documents better, the DoD provides this form for use in ~~writing comments and suggestions for improvements. All users of military standardization documents are invited to provide~~ ~~sions.~~ This form may be detached, folded along the lines indicated, taped along the loose edge *(DO NOT STAPLE)*, and mailed. In block 5, be as specific as possible about particular problem areas such as wording which required interpretation, was too rigid, restrictive, loose, ambiguous, or was incompatible, and give proposed wording changes which would alleviate the problems. Enter in block 6 any remarks not related to a specific paragraph of the document. If block 7 is filled out, an acknowledgement will be mailed to you within 30 days to let you know that your comments were received and are being considered.

NOTE: This form may not be used to request copies of documents, nor to request waivers, deviations, or clarification of specification requirements on current contracts. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document*(s)* or to amend contractual requirements.

(Fold along this line)

(Fold along this line)

DEFENSE LOGISTICS AGENCY

NO POSTAGE NECESSARY IF MAILED IN THE UNITED STATES

OFFICIAL BUSINESS
PENALTY FOR PRIVATE USE $300

BUSINESS REPLY MAIL
FIRST CLASS PERMIT NO. 4966 WASHINGTON D C

POSTAGE WILL BE PAID BY THE DEFENSE LOGISTICS AGENCY

Commander
Defense Personnel Support Center
Attn: DPSC-MSTE
2800 South 20th Street
Philadelphia, PA 19101

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:32Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

(See Instructions – Reverse Side)

1. DOCUMENT NUMBER	2. DOCUMENT TITLE
A-A-54322	BROACH, PULP CANAL, BARBED, STERILE

3a. NAME OF SUBMITTING ORGANIZATION

4. TYPE OF ORGANIZATION *(Mark one)*

- ☐ VENDOR
- ☐ USER
- ☐ MANUFACTURER
- ☐ OTHER *(Specify)*: _____

b. ADDRESS *(Street, City, State, ZIP Code)*

5. PROBLEM AREAS

a. Paragraph Number and Wording

b. Recommended Wording

c. Reason/Rationale for Recommendation

6. REMARKS

7a. NAME OF SUBMITTER *(Last, First, MI)* – Optional	b. WORK TELEPHONE NUMBER *(Include Area Code)* – Optional
c. MAILING ADDRESS *(Street, City, State, ZIP Code)* – Optional	8. DATE OF SUBMISSION *(YYMMDD)*

(TO DETACH THIS FORM, CUT ALONG THIS LINE.)

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:32Z
Check the source to verify that this is the current version before use.