COMMERCIAL ITEM DESCRIPTION

BATH, WATER, DENTAL IMPRESSION COMPOUND

The General Services Administration has authorized the use of this Commercial Item Description as a replacement for Federal Specification GG-B-140D, which is cancelled.

This Commercial Item Description covers an electrically heated, thermostatically controlled water bath and compatible insert pan, suitable for use with dental impression materials.
This commercial item description covers the following types:

Type 1: Complete Unit
Type 2: Replacement Insert Pan only

Salient characteristics:

Material. The enclosure, removable insert pan, cover, shell, and lifting platform shall be fabricated of AISI Type 302 or 304 stainless sheet steel. The perforated rack shall be fabricated of black synthetic rubber with a Shore Durometer Hardness of B-75 to B-85. All water bath components shall be corrosion-resistant. The lifting platform shall be fabricated of corrosion-resistant steel or chromium over nickel plated brass.

Style, design, and dimensions. Each complete Type 1 water bath shall be nominally composed of an enclosure, inner shell, thermostatically controlled heating element (adjustable thermostat), main on/off switch, pilot light, removable insert pan with a compatible cover, a removable rubber rack, a lifting platform, and two cloth covers which fit over the platform.

The bottom of the water bath shall be equipped with a heat shield which limits the bottom surface temperature of the unit to 150°F when operated on a black nonreflective surface, at the boiling setting, with the insert pan filled to operating level. The water bath shall be equipped with a temperature dial which is calibrated in increments of 20°F in the range from 100°F to boiling. A reference line which clearly indicates one extreme position of the thermostat shall be provided on the dial.

AMSC N/A FSC 6520
DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:32Z
Check the source to verify that this is the current version before use.

The removable insert pan shall be in accordance with Figure 1 herein, be compatible for use with the water bath and shall have a ribbed bottom for reinforcement and preventing concavity. The insert pan cover shall be dome-shaped with a reverse draw and a plastic knob for lifting. Each removable insert pan shall be formed from one piece of stainless steel, with a rolled flattened bead on the top edge to provide a finger grip for removal. The pan shall have a telescopic fit into the tubular shell of the water bath, shall be readily removable, and shall have full surface to surface contact with the heating element when placed in position. The stainless steel cover for the insert pan shall be of one-piece construction, having an outer diameter of 6-3/8 inches.

The lifting platform shall be a 4-3/4 inch diameter ring raised 1-1/2 inches above the surface it is placed on. A vertical handle shall be provided with a plastic knob for lifting the platform out of the tank. Two cloth covers which fit over the ring of the platform, shall be provided for suspending articles in the water bath.

Each perforated rubber rack shall have three compartments: one 3/4 inch wide x 5/8 inch deep and perforated, to accommodate tubes of hydrocolloid, one 5/8 inch deep and perforated, to accommodate syringes ready for use, and one 2-1/2 inch deep non-perforated tempering bath with a 3/16 inch minimum side wall thickness, designed to receive the filled impression tray.

All tolerances on dimensions shall be ± 5% unless otherwise specified, provided neither fit nor function is sacrificed.

Construction. Water bath construction shall be such that a stainless steel enclosure surrounds a tubular shell. The top and bottom of the water bath shall contain openings which allow the tubular shell to fit into them. There shall be an insulating dead air space of at least one inch between the side enclosure and the tubular shell. The shell shall have a thermostat mounted on a vertical wall. Two pair of slots shall be provided on the circumference of the shell. The shell material between the slots shall hold the tank against the thermostat. The thermostat shall be enclosed in a stainless steel case located on the front side of the unit. Heating element construction shall be immersion, disk, or sheathed ring type.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:32Z
Check the source to verify that this is the current version before use.

A hinge shall be secured to the back of the bath cover and to the top of the unit to permit three resting positions for the cover: in place on the tank, in a nearly vertical position, and cover tilted all the way over to permit removal of the pan from the unit.

Electrical characteristics. The water bath shall require an input of 115 VAC, 50/60 Hz. The heating element shall have a minimum capacity of 270 W. The heating system shall be capable of reaching the power level of 300 W ± 10%. The heating element shall be rated to provide a uniform temperature. The main switch, pilot light, electrical cord, and power plug shall be UL approved. Line cord shall be 3 conductor type and at least 6 feet in length with a 3 blade plug attached to one end.

Identification marking. Each water bath shall permanently and legibly exhibit the model number, voltage, power rating, serial number, and the name or registered trademark of the manufacturer. Markings shall be permanently and legibly printed or depressed with typewriter characters on the Type 1 water bath, or a pressure sensitive name tape permanently affixed thereto. Marking of the replacement insert pan shall be optional.

Performance. The water bath shall exhibit no signs of electrical, thermal, or mechanical deterioration after being subjected to 23 hours of continuous operation at 300 W and 200°F, followed by one hour of operation with the thermostat set for boiling. The water bath temperature shall rise to boiling at a rate which is in accordance with manufacturer's specifications. Altitude above sea level shall be considered in determining thermostat setting necessary in the upper temperature range to produce a water boiling condition. The thermostat shall control the temperature of the water bath (when filled with water to the operating level) within 2°F of any selected temperature in the range from 100°F to 212°F after the temperature has stabilized. Temperature dial calibration shall be accurate to ± 5% within the temperature range from 100°F to 212°F.

Service data. Each Type 1 water bath shall be supplied with two copies each of operating, maintenance, and service manuals, and parts list. Service manuals must include complete calibration procedures.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:32Z
Check the source to verify that this is the current version before use.

Finish. All inside and outside surfaces of platform, removable insert pan and cover, and exposed surface of the inner shell shall have a No. 4 finish. As alternates, the interior surface of the insert pan may be electropolished, and the exposed surface of the inner shell may have a No. 2B finish. All surfaces shall be smooth and free of sharp edges.

Workmanship. Water baths and insert pans shall be free from defects which may detract from their appearance or impair their serviceability.

Unit. Each. (EA).

Type 1. The water bath, a replacement insert pan, a perforated rubber rack, a cover for the insert pan, a lifting platform, and 2 cloth covers which fit over the platform, as specified shall constitute one unit.

Type 2. Each replacement insert pan, without an accompanying water bath, as specified, constitutes one unit.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after the delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:32Z
Check the source to verify that this is the current version before use.

Sampling for examination. Sampling for examination shall be conducted in accordance with MIL-STD-105. Where feasible, the same sample shall be used for the determination of two or more examination characteristics. The unit of product for examination purposes shall be one Type 1 water bath or one Type 2 insert pan, unless otherwise specified. Sampling for examination shall be conducted at inspection level II, except dimensions shall be examined at inspection level S-1, all with an AQL of 2.5 (percent defective).

Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 at inspection level S-2, with an acceptance number of zero for all sample sizes, except dielectric strength and performance tests shall be tested at an inspection level of 100%. Where feasible, the same sample shall be used for the determination of two or more test characteristics. The unit of product for test purposes shall be one complete Type 1 water bath, or one Type 2 insert pan.

Tests. Tests shall be conducted to determine compliance with specification requirements.

Metric products. Products manufactured to metric dimensions will be considered on an equal basis with those manufactured using inch/pound units, providing they fall within the tolerances specified using conversion tables contained in the latest revision of Federal Standard No. 376, and all other requirements of this document are met. If a product is manufactured to metric dimensions and those dimensions exceed the tolerances specified in the inch/pound units, a request should be made to the contracting officer to determine if the product is acceptable. The contracting officer has the option of accepting or rejecting the product.

Contractor certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producer's own drawings, specifications, standards, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:32Z
Check the source to verify that this is the current version before use.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Federal Acquisition Regulation Subpart 23.4 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

NOTE: The following National Stock Numbers are covered by this document:

National Stock Number	Item Identification
6520-00-535-7100	BATH, WATER, DENTAL IMPRESSION MATERIAL, THERMOSTATICALLY-CONTROLLED, 115V, 50/60 Hz
6520-00-145-0114	PAN, WATER BATH, DENTAL IMPRESSION MATERIAL, CORROSION-RESISTING STEEL

Ordering data. Intermediate/exterior package quantities, labeling, and marking must be specified in the contract and/or order.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:32Z
Check the source to verify that this is the current version before use.

MILITARY INTERESTS

Custodians:

Army-MD
Navy-MS
Air Force-03

PREPARING ACTIVITY:

DoD-MB

Agent:


DLA-DM

CIVIL AGENCY COORDINATING ACTIVITIES:

VA-OSS
PHS
FDA-MPQAS

PROJECT NO. 6520-2381
LOCATION: Word/BATH.DOC

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:32Z
Check the source to verify that this is the current version before use.

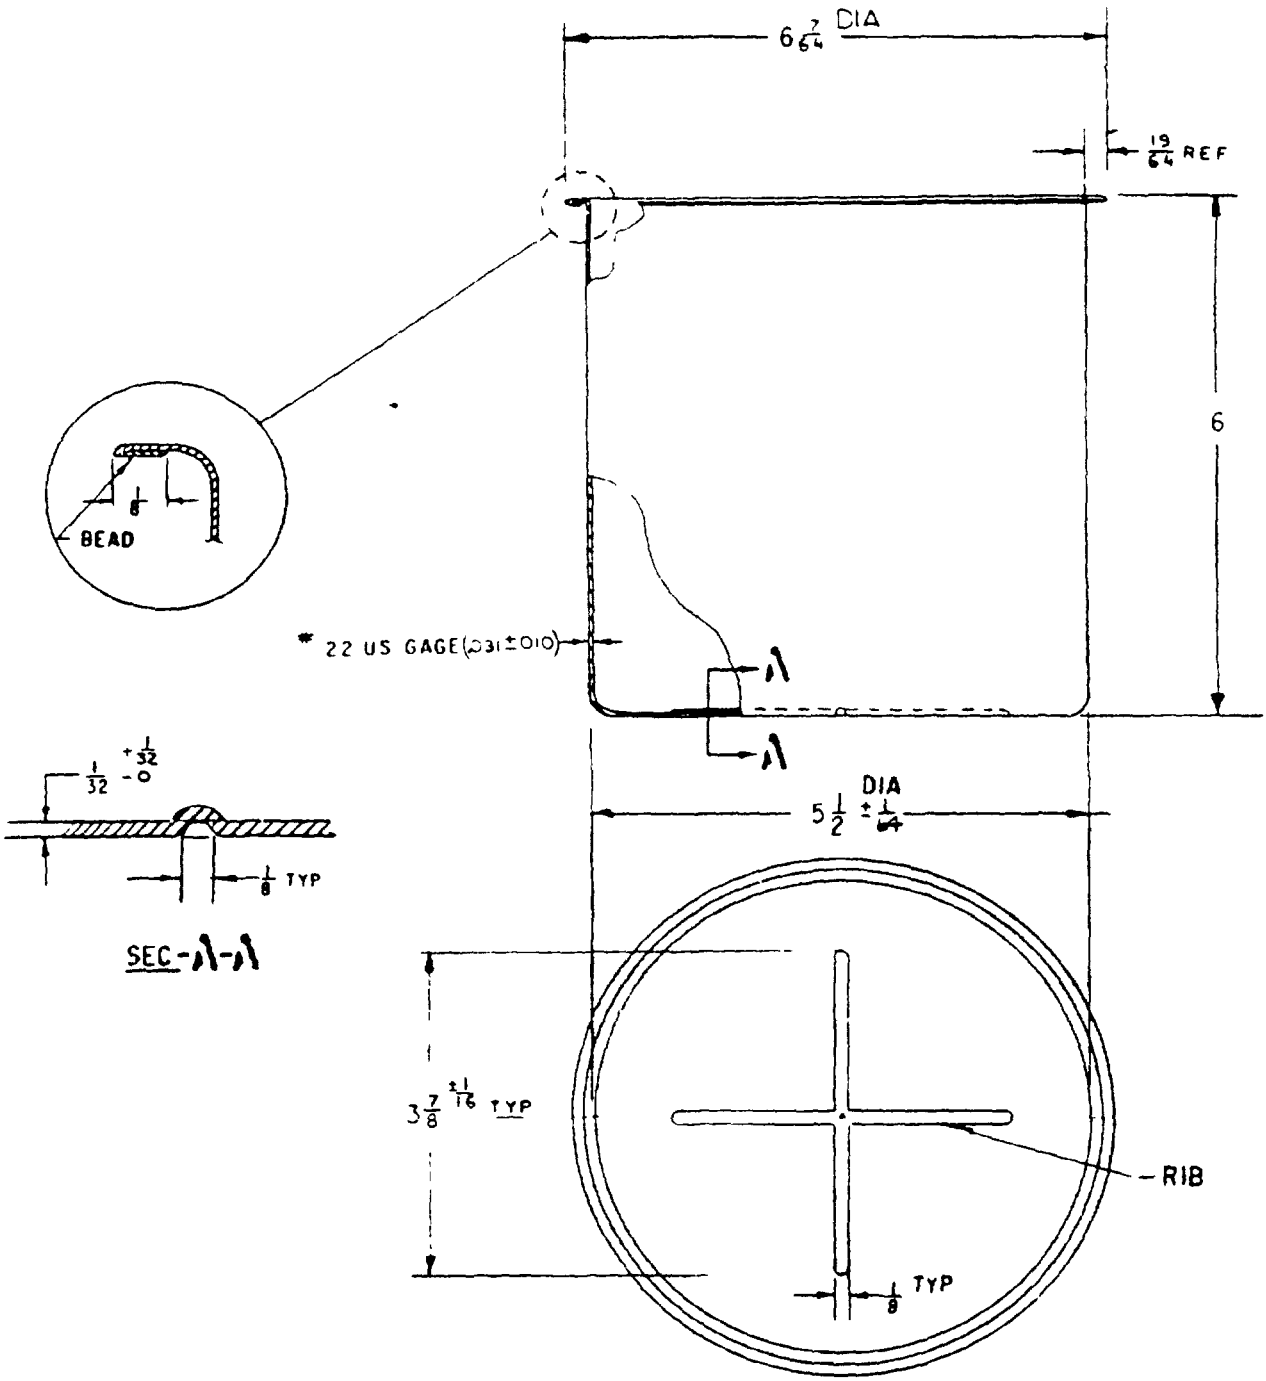

NOTE

1. ALL EDGES SHALL BE ROUNDED
2. UNLESS OTHERWISE SPECIFIED, ALL DIMENSIONS ARE IN INCHES AND TOLERANCES SHALL BE ± 1/32

BOTTOM VIEW

FIGURE 1

INSERT PAN, WATER BATH

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:32Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

INSTRUCTIONS

1. The preparing activity must complete blocks 1, 2, 3, and 8. In block 1, both the document number and revision letter should be given.
2. The submitter of this form must complete blocks 4, 5, 6, and 7.
3. The preparing activity must provide a reply within 30 days from receipt of the form.

NOTE: This form may not be used to request copies of documents, nor to request waivers, or clarification of requirements on current contracts. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements.

I. RECOMMEND A CHANGE:	1. DOCUMENT NUMBER A-A-54345	2. DOCUMENT DATE (YYMMDD) 15 February 1991

3. DOCUMENT TITLE
BATH, WATER, DENTAL IMPRESSION COMPOUND

4. NATURE OF CHANGE (Identify paragraph number and include proposed rewrite, if possible. Attach extra sheets as needed.)

5. REASON FOR RECOMMENDATION

6. SUBMITTER

a. NAME (Last, First, Middle Initial)	b. ORGANIZATION	
c. ADDRESS (Include Zip Code)	d. TELEPHONE (Include Area Code) (1) Commercial (2) AUTOVON (If applicable)	7. DATE SUBMITTED (YYMMDD)

8. PREPARING ACTIVITY

a. NAME Defense Personnel Support Center	b. TELEPHONE (Include Area Code) (1) Commercial: (215)737-2870 (2) AUTOVON: 444-2870
c. ADDRESS (Include Zip Code) ATTN: DPSC-MSTE 2800 S. 20th Street Philadelphia, PA 19101	IF YOU DO NOT RECEIVE A REPLY WITHIN 45 DAYS, CONTACT: Defense Quality and Standardization Office 5203 Leesburg Pike, Suite 1403, Falls Church, VA 22041-3466 Telephone (703) 756-2340 AUTOVON 289-2340

DD Form 1426, OCT 89 — Previous editions are obsolete — 198/290

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:32Z
Check the source to verify that this is the current version before use.