A-A-53583
29 July 1988

COMMERCIAL ITEM DESCRIPTION

MOUNT, RADIOGRAPHIC FILM, DENTAL

The General Services Administration has authorized the use of this Commercial Item Description in preference to Interim Federal Specification G-M-00656.

This Commercial Item Description covers an open-window cardboard or plastic mount, suitable for use in filing dental x-ray films.

Salient characteristics:

The dental radiographic film mount shall be one of the following two types:

Type I - Capable of mounting fourteen 1-1/4 inch by 1-5/8 inch (3.18 cm by 4.12 cm) number 2 standard periapical dental films and two 1-1/16 inch by 2-1/8 inch (2.7 cm by 5.4 cm) number 3 bitewing dental films.

Type II - Capable of mounting two 1-1/16 inch by 2-1/8 inch (2.7 cm by 5.4 cm) number 3 bitewing dental films.

The film mount shall be fabricated of either three layers of paper stock, or two layers of paper stock, glued together with a strong, durable, adhesive.

Paper stock used in the fabrication of the three-layer dental mount shall have the following minimum values:

1. Thickness of 0.009 inch (.23 mm).
2. Basis weight (1000 sheets 22-1/2 inch by 28-1/2 inch (57.15 cm by 72.39 cm)) of 158 pounds.
3. Bursting strength of 60 pounds per square inch.

Paper stock used in the fabrication of the two-layer dental mount shall have the following minimum values:

AMSC N/A FSC 6525

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:21Z
Check the source to verify that this is the current version before use.

1. Thickness of 0.0135 inch (.34 mm).
2. Basis weight of 225 pounds.
3. Bursting strength of 100 pounds per square inch.

As an alternate, the mount may be of equivalent plastic construction.

Type I Mount - Design and construction.

The type I mount shall have nominal dimensional of 13-1/4 inches by 5-3/16 inches. The mount shall be scored so that it shall be possible to fold the mount to approximately one-third of its open size, and so that folding shall not cause breaks in the paper stock. Placement of windows in each approximate one-third section shall be as follows (see figures 1 or 3):

Each of the outer sections shall have five windows - four to accommodate 1-1/4 by 1-5/8 inch (3.18 by 4.12 cm) film and one to accommodate 1-1/16 by 2-1/8 inch (2.7 by 5.4 cm) film. The five windows shall be symetrically placed so that two windows for 1-1/4 by 1-5/8 inch film shall be side by side in the upper portion of the section, two windows for 1-1/4 by 1-5/8 inch film shall be side by side in the lower portion of the section, and the window for the 1-1/16 by 2-1/8 inch film shall be in the center of the section. The long axis of all the windows shall be parallel to the long axis of the mount.

The center section shall have six windows to accommodate 1-1/4 by 1-5/8 inch (3.18 by 4.12 cm) film. Three of the windows shall be placed side by side in the upper portion of the section and aligned with three windows placed in the lower portion. The side by side placement shall be symetrical with reference to the width of the section. The long axis of all the windows shall be perpendicular to the long axis of the mount.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:21Z
Check the source to verify that this is the current version before use.

The front panel shall be smooth throughout and imprinted as follows:

a. In top margin:

NAME_____SER. NO._____

RANK OR RATE_____DATE_____

b. In the bottom margin:

ACTIVITY_____

Under each window for 1-1/4 by 1-5/8 inch (3.18 cm by 4.12 cm) film, shall be as follows: (clockwise, starting at upper left, for each section)

Left end section: "Upper Molar Area, Bicuspid Area, Bicuspid Area, Lower Molar Area".
Center Section: "Cuspid Area, Incisor Area, Cuspid Area, Cuspid Area, Incisor Area, Cuspid Area".
Right end section: "Bicuspid Area, Upper Molar Area, Lower Molar Area, Bicuspid Area".

Type II Mount - Design and construction.

The type II mount shall have nominal dimensions of 5-3/8 inches by 2-15/16 inches (13.78 cm by 7.55 cm). The two windows shall be symetrically placed, side by side, with the long axis of the windows parallel to the long axis of the mount. The mount shall permit insertion of the film in the back panel (see figure 2).

The front panel shall be smooth throughout and imprinted as follows:

a. In top margin:

NAME_____SER. NO._____

RANK OR RATE_____DATE_____

b. In the bottom margin:

ACTIVITY_____

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:21Z
Check the source to verify that this is the current version before use.

Both type I and type II mount windows shall be cleanly cut with rounded corners, free of ragged edges, with no marginal separations. They shall be constructed to permit easy insertion of film in the back panel, to secure holding of the film and to allow full viewing of the film. Slots for film insertion may be either at the right or the left for the horizontal windows and either at the top or the bottom for vertical windows.

Both type I and type II mounts shall be free of oil, grease, dirt, and other contamination.

Workmanship. The dental radiographic film mount shall be free from defects which detract from its appearance or impair its serviceability.

Unit. Package (PG). One package containing twenty-five film mounts of one type only, as specified, constitutes one unit.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:21Z
Check the source to verify that this is the current version before use.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more test characteristics.

Sampling for examination. Sampling for examination shall be conducted in accordance with MIL-STD-105, with an AQL of 1.0 (percent defective) and an inspection level of II. The unit of product for examination purposes shall be one dental radiographic film mount as specified in this description.

Defects.

Material not as specified.

Placement of windows not in accordance with applicable figure.

Mount not scored.

Separation of paper layers because of insufficient glue.

Identification marking missing, illegible, or incomplete.

Windows do not have rounded corners and smooth edges.

Mount not free of tears or rough edges.

Mount not free of oil, grease, dirt, or other contamination.

Sampling for tests. Sampling for tests including dimensional test, shall be conducted in accordance with MIL-STD-105, with an AQL of 2.5 (percent defective) and an inspection level of S-3. The unit of product for test purposes shall be one dental radiographic film mount.

Tests

Film Insertion Test. Films, of the sizes specified for type I and type II mounts, shall be tried for fit in the film mounts. For the type I mount, not less than six windows shall have the sample films inserted. For type II mounts, at least one window shall have the sample film inserted. Any film difficult to insert, or not securely held by mount, shall constitute a defect.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:21Z
Check the source to verify that this is the current version before use.

Thickness test. The paper to be tested shall be a single sheet of paper not less than 2 inches by 2 inches (51 mm by 51 mm) and free from wrinkles and creases.

After calibration of a suitable micrometer by means of an accepted method, the paper specimen shall be clamped between the faces of the micrometer under a steady pressure of 7.0 to 9.0 pounds per square inch (0.40 to 0.63 kg per square cm). A thickness less than 0.009 inch (three-layer mount) or 0.0135 inch (two-layer mount) shall constitute a defect.

Basis Weight Test. The paper specimen to be tested shall consist of 10 sheets of 22-1/2 inches by 28-1/2 inches (57.15 cm by 72.39 cm) paper.

The weight of the 10 paper sheet specimen shall be determined by a suitable method. The weight of 1000 sheets shall than be calculated. A 1000 sheet weight less than 158 pounds (three-layer mount) or 225 pounds (two-layer mount) shall constitute a defect.

Metric products. Products manufactured to metric dimensions will be considered on an equal basis with those manufactured using inch-pound units, providing they fall within the tolerances specified using conversion tables contained in the latest revision of Federal Standard 376, and all other requirements of this document are met.

If a product is manufactured to metric dimensions and those dimensions exceed the tolerances specified in the inch/pound units, a request should be made to the contracting officer to determine if the product is acceptable.

The contracting officer has the option of accepting or rejecting the product.

Contractor certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:21Z
Check the source to verify that this is the current version before use.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Public Law 94-580, as amended, and as implemented by Federal Acquisition Regulation Subpart 23.4 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

NOTE: The following National Stock Numbers are covered by this document:

6525-00-817-2363 (Type I)
6525-00-817-2364 (Type II)

Ordering data. Intermediate/exterior package quantities, labeling, and marking must be specified in the contract and/or order.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:21Z
Check the source to verify that this is the current version before use.

A-A-53583

MILITARY INTERESTS:

Custodians:

Army - MD
Navy - MS
Air Force - 03

PREPARING ACTIVITY:

DoD - MB

Agent:

DLA-DM

CIVIL AGENCY COORDINATING ACTIVITIES:

VA-OSS
PHS
FDA-MPQAS

Project No. 6525-1242

PGC 05108

Location: CID/DENTAL/MOUNT/FILM/H13-32

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:21Z
Check the source to verify that this is the current version before use.

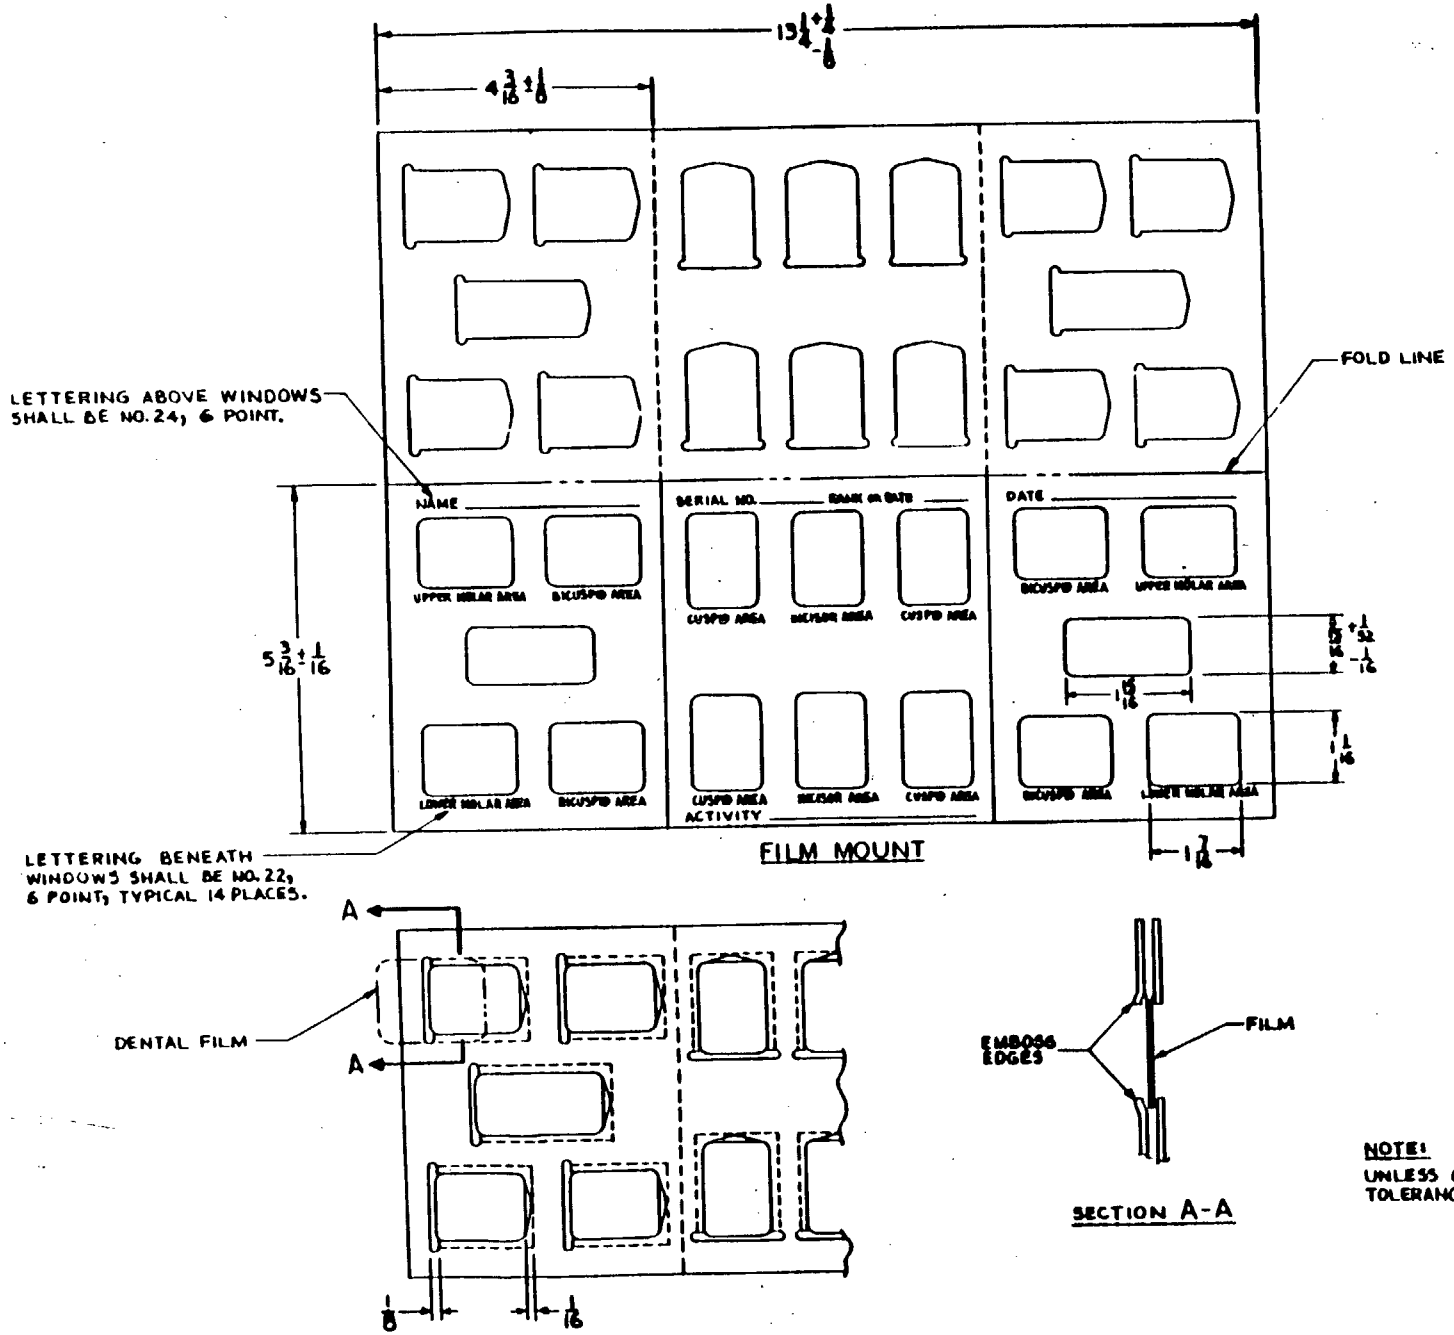


FIGURE 1. Mount, Radiographic Film, Dental

Source: https://assist.dla.mil - Downloaded: 2026/10-26T09:21Z
Check the source to verify that this is the current version before use.

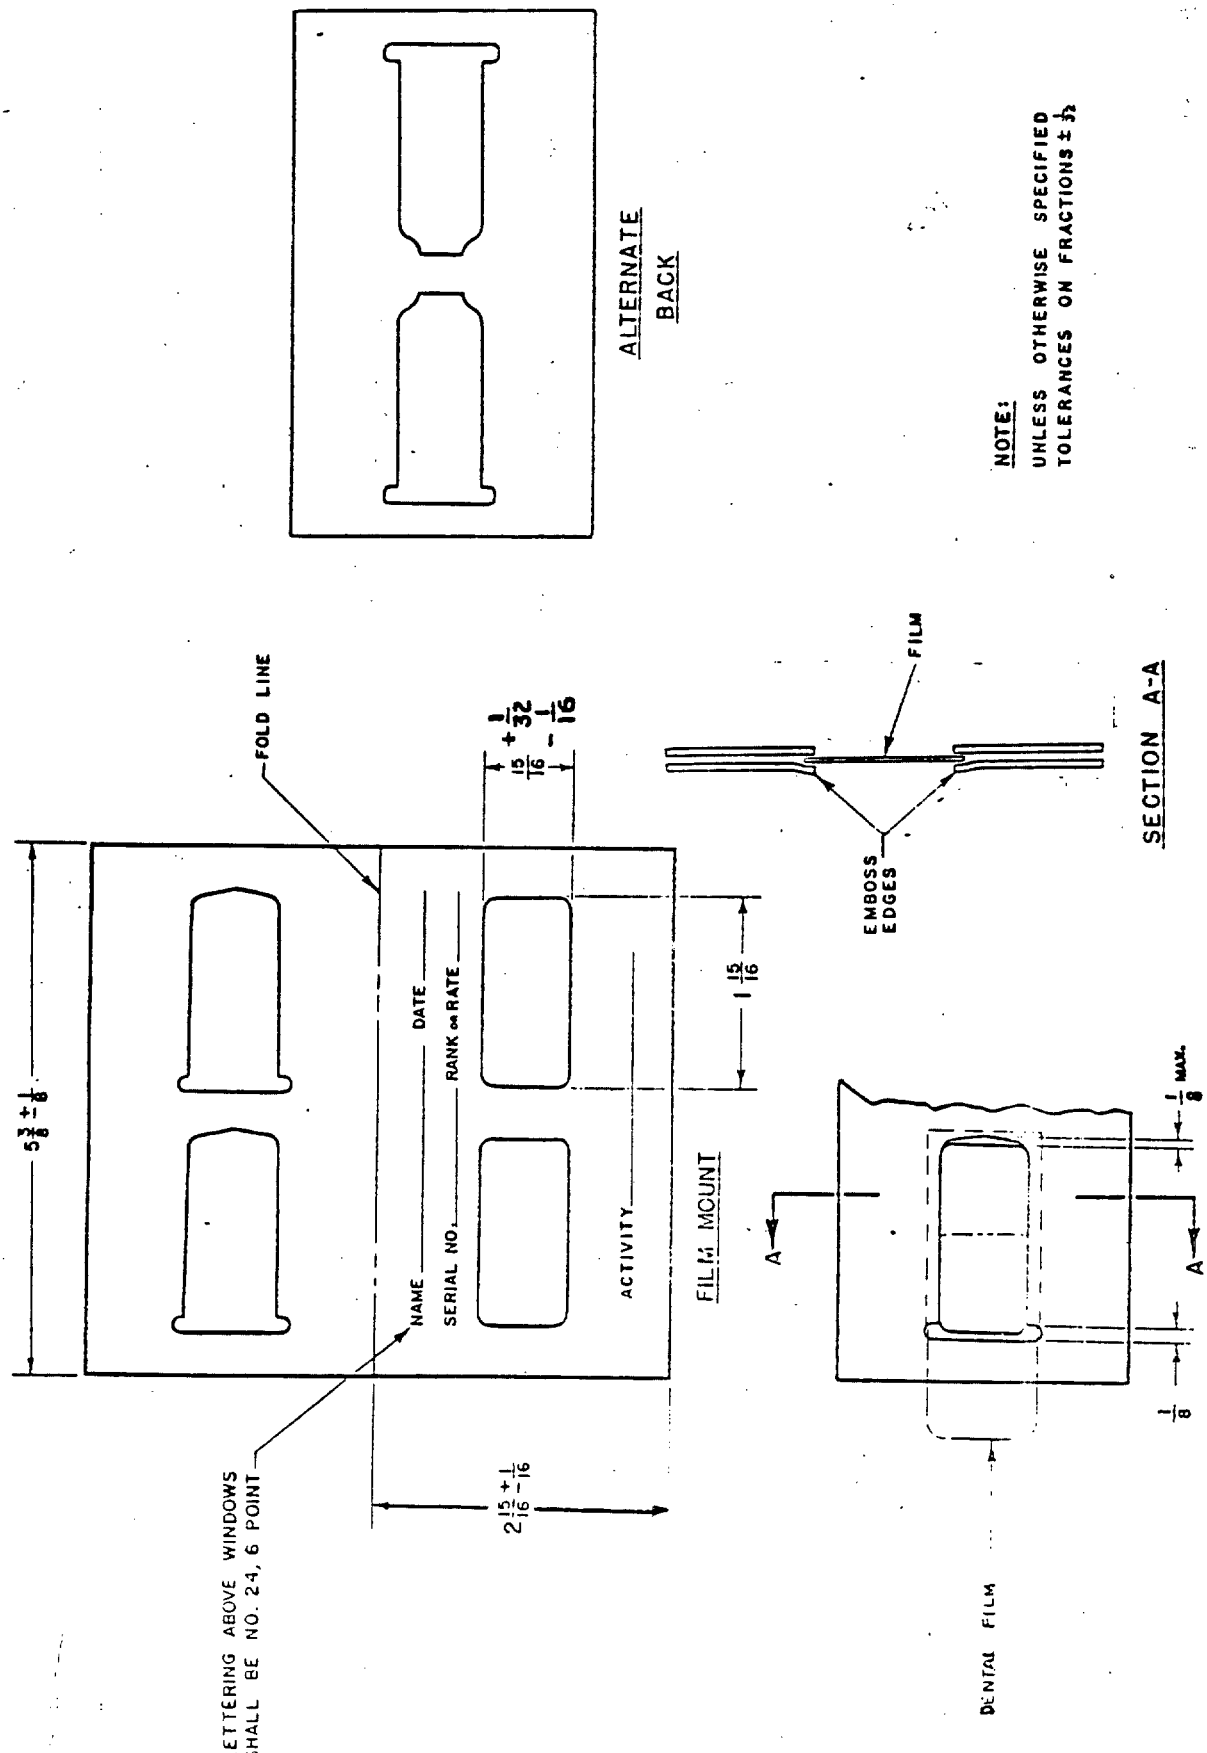


FIGURE 2. Mount, Radiographic Film, Dental

Source: https://assist.dla.mil -- Downloaded: 202610-26T09:21Z
Check the source to verify that this is the current version before use.

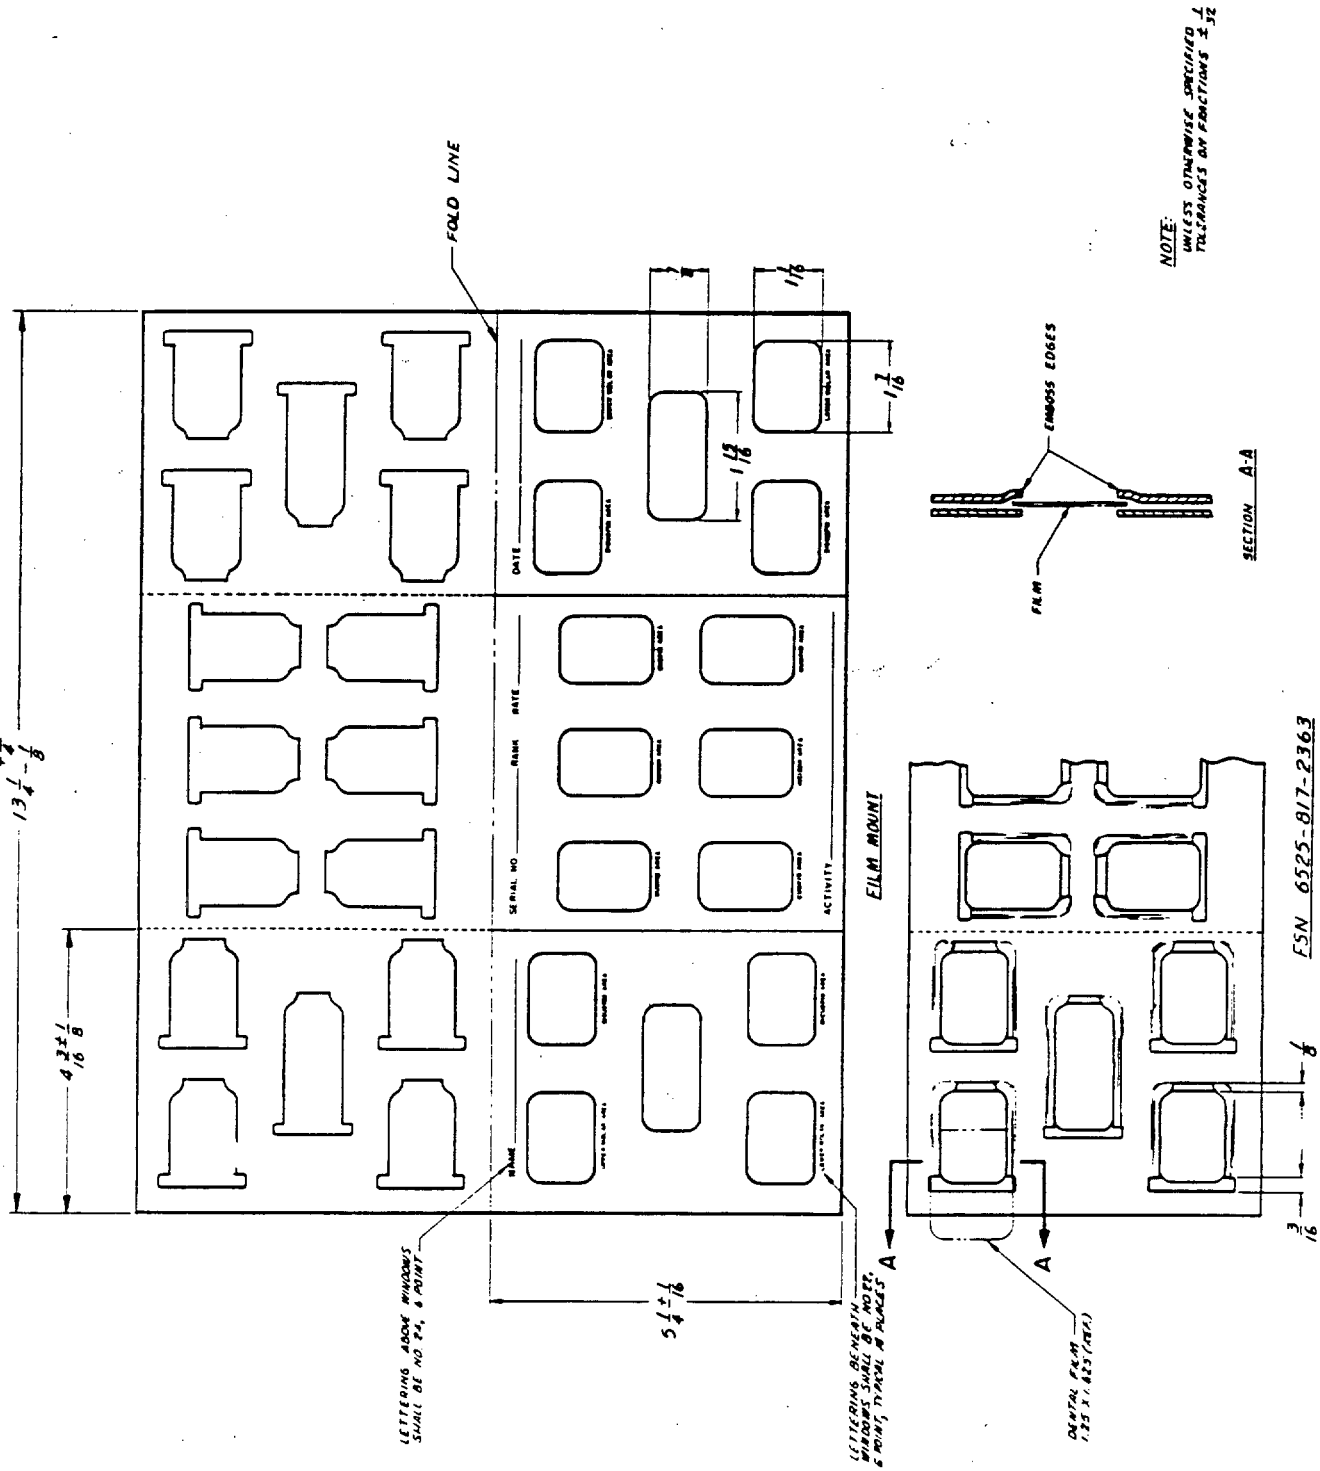


FIGURE 3. Mount, Radiographic Film, Dental

FSN 6525-817-2363

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:21Z
Check the source to verify that this is the current version before use.