A-A-53585
29 July 1988

COMMERCIAL ITEM DESCRIPTION

TANK, INSERT, X-RAY FILM PROCESSING

The General Services Administration has authorized the use of this Commercial Item Description as a replacement for Military Specification MIL-T-36213 which is cancelled.

This Commercial Item Description covers a lightweight, stainless steel insert tank suitable for field use in an x-ray film processing master tank.

Salient characteristics:

The x-ray processing insert tank shall be suitable for field use in an x-ray film processing master tank and shall be supplied in the following types:

Type I	15 gallon capacity tank with legs.
Type II	5 gallon capacity tank with ledge-support bars instead of legs.

The insert tank shall be fabricated from American Iron and Steel Institute (AISI) Type 316 corrosion-resisting steel. The Type I tank shall be 0.050 inch (No. 18, United States Standard Gage) thick. The Type II tank shall be 0.025 inch (No. 24, United States Standard Gage) thick.


The design and dimensions of the Type I tank shall be as shown in figure 1 with drain location, neoprene drain plug, and neoprene tipped legs. The design and dimensions of the Type II tank shall be as shown in figure 2 with drain location and neoprene drain plug.

The insert tank shall be of rigid, durable, leakproof construction. The outside surface of the tank shall not distort more than 0.015 inch per linear inch of the surface when hydrostatically tested for rigidity. When tested for capacity, the volume of water required to fill the insert tank to a level of one inch below the top shall be between 100 percent and 103 percent of rated capacity. Finish shall be Commercial Standard No. 2B.

AMSC N/A FSC 6525

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:21Z
Check the source to verify that this is the current version before use.

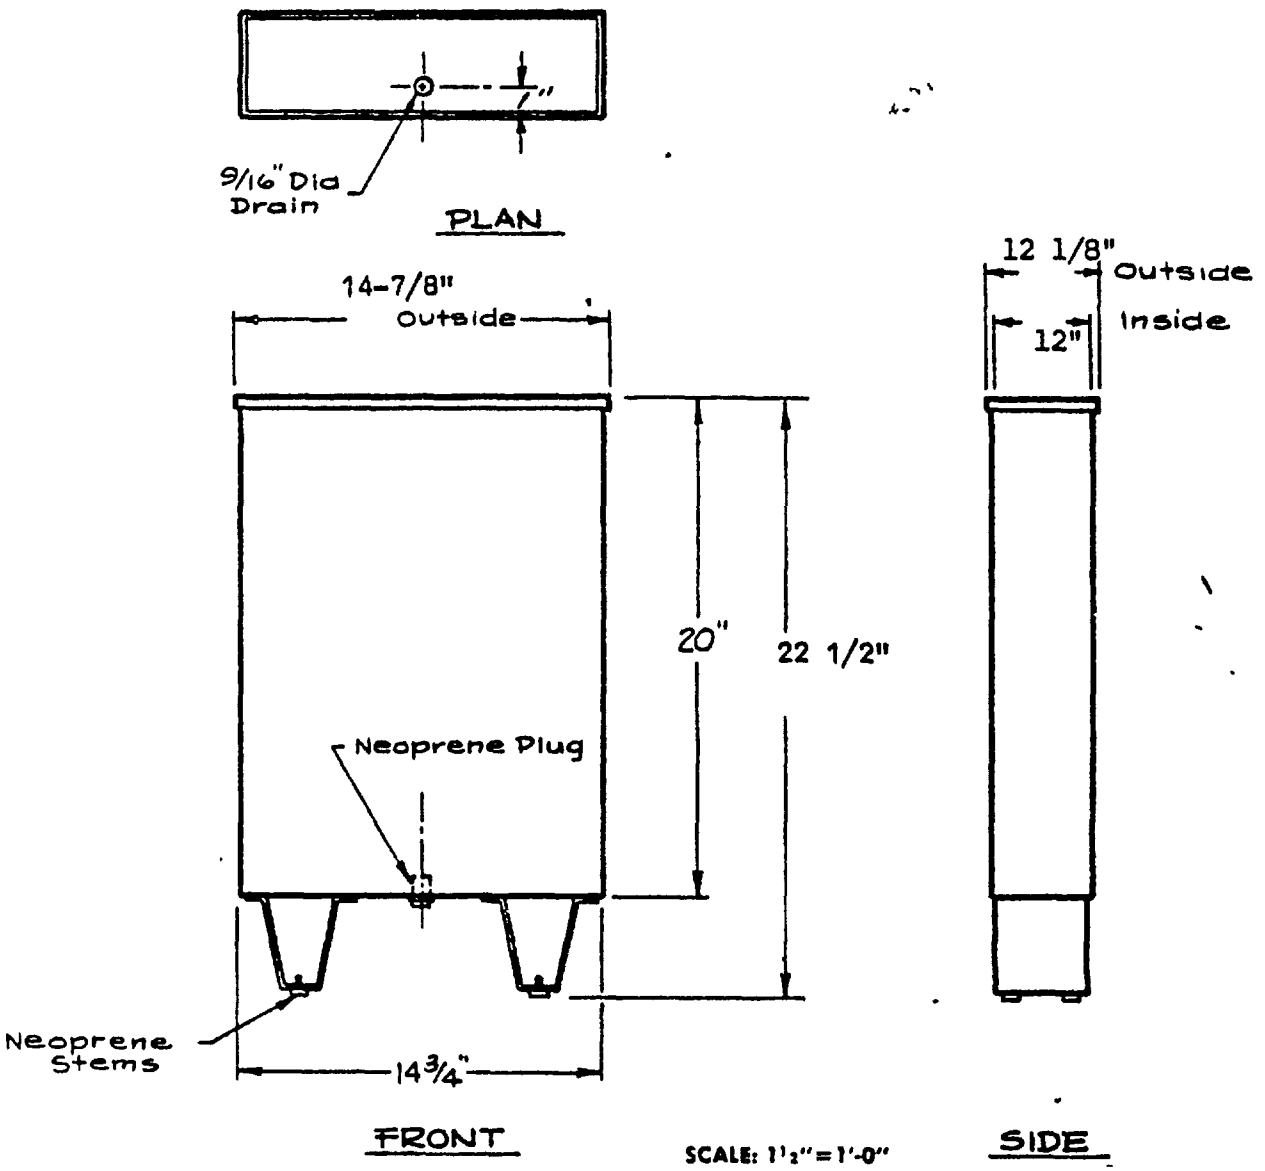


NOTES

1. 18 gauge stainless steel, type 316, heliarc welded seams.
2. Drain with neoprene plug.
3. Neoprene stems on bottom of legs.

FIGURE 1. X-ray film processing tank insert - 15 gallon capacity

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:21Z
Check the source to verify that this is the current version before use.

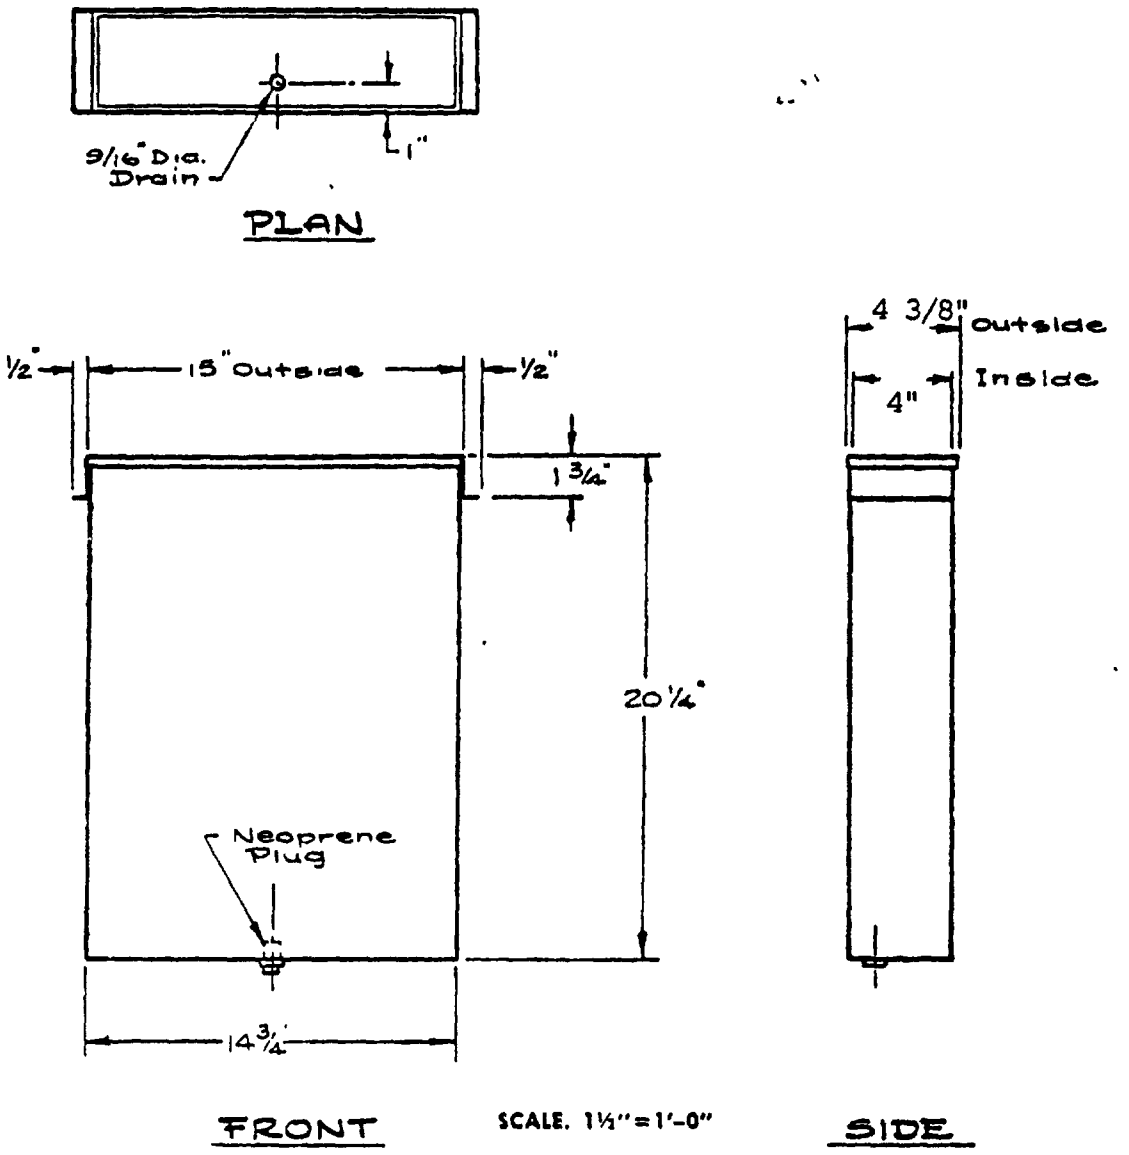

NOTES
1. 24 gauge, type 316 stainless steel, hellarc welded.
2. Drain with neoprene plug.

FIGURE 2. X-ray film processing tank insert - 5 gallon capacity.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:21Z
Check the source to verify that this is the current version before use.

All welding shall be according to standard practice. Complete penetration of corner welds shall be accomplished to provide a sound weld and to eliminate the crevice between the two welded sheets. Where welding rod is used, it shall be Type 316 stainless steel, and the resultant weld shall be ground and polished smooth to remove all pits, discontinuities, flux, scale, and laps. Spot welds shall be smoothly dressed to blend with adjacent surfaces. The tank shall pass the tests for leakage and corrosion resistance.

After fabrication, as a final treatment, the tank shall be passivated or pickled by complete immersion into a bath of nitric acid or a mixture of nitric and hydrofluoric acid of proper concentration and temperature. Slight etching shall be permitted on the number 2B finish as a result of the passivation or pickling process to remove contamination and discoloration. Following the passivation or pickling treatment, the tank shall be thoroughly washed with water until all traces of the acid solution have been removed, and shall then be dried.

The tank shall be free of oil, grease, dirt, or other contamination. Exposed edges shall be free of burrs or sharpness. All interior surfaces shall be smooth and free of pits, protruding ridges, and other defects.

Workmanship. The x-ray film processing insert tank shall be free from defects which detract from its appearance or impair its serviceability.

Unit. Each (EA). One tank, as specified, constitutes one unit.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:21Z
Check the source to verify that this is the current version before use.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more test characteristics.

Sampling for examination. Sampling for examination shall be conducted in accordance with MIL-STD-105, with an AQL of 1.0 (percent defective) and an inspection level of II. The unit of product for examination purposes shall be one x-ray film processing insert tank as specified in this description.

Defects.

Tank not AISI Type 316 corrosion-resisting steel.

Tank not correct United States Standard Gage.

Tank design does not conform to figure 1 or figure 2.

Tank does not have drain or neoprene drain plug.

Welds not ground and polished smooth to remove all pits, discontinuities, flux, scale, and laps.

Welds not smoothly dressed to blend with adjacent surfaces.

Exposed edges of tank not free of burrs or sharpness.

Interior surfaces of tank not smooth and free of pits, protruding ridges, and other defects.

Tank not free of oil, grease, dirt, or other defects.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:21Z
Check the source to verify that this is the current version before use.

Sampling for tests. Sampling for tests including dimensional test shall be conducted in accordance with MIL-STD-105, with an AQL of 2.5 (percent defective) and an inspection level of S-1. The unit of product for test purposes shall be one x-ray film processing insert tank.

Tests

Hydrostatic test for rigidity. The tank under test shall be placed on a flat surface. The camber of each outside surface shall be measured by the use of a straight edge applied horizontally, vertically, and diagonally across the center of each side. Fill the tank with water. Remeasure the chamber. Check for leakage. Distortion of the tank more than 0.015 inch per linear inch of the surface or any evidence of leakage shall constitute a defect.

Tank leakage test. All welds on the tank shall be coated on the outside with a fluorescent penetrant suspended in oil. The welds shall be viewed from the inside of the tank under ultraviolet light in a darkroom for indications of porosity and breaks in the welds. Any evidence of leakage shall constitute a defect.

Corrosion resistance test. A 3-5 percent salt solution maintained at 140°F. shall be allowed to stand in the tank for 48 hours. The tank shall be observed for evidence of corrosion. Any evidence of corrosion shall consititute a defect.

Capacity test. Measurement to determine capacity of the insert tank shall be made as follows, in the order listed.

a. Place the insert tank into a larger tank or within a master tank.
b. From a premeasured volume of water (at approximately 70°F) equal to the rated capacity of the insert tank, pour approximately 80 percent into the insert tank.
c. Fill the larger or master tank with water to a level approximately one inch below the top of the insert tank.
d. Add the balance of the premeasured volume of water (in "b" above) to the insert tank.
e. Measure the distance from the top to the water level in the insert tank.
f. Pour an additional volume of water into the insert tank equal to three percent of its capacity.
g. Repeat measurement made in "e" above.
h. Analyze measurements obtained in "e" and "g" above to determine whether the one inch water level below the top of the tank occurs between 100 percent and 103 percent of rated capacity. Any deficiency in capacity shall constitute a defect.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:21Z
Check the source to verify that this is the current version before use.

Metric products. Products manufactured to metric dimensions will be considered on an equal basis with those manufactured using inch-pound units, providing they fall within the tolerances specified using conversion tables contained in the latest revision of Federal Standard 376, and all other requirements of this document are met.

If a product is manufactured to metric dimensions and those dimensions exceed the tolerances specified in the inch/pound units, a request should be made to the contracting officer to determine if the product is acceptable.

The contracting officer has the option of accepting or rejecting the product.

Contractor certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Public Law 94-580, as amended, and as implemented by Federal Acquisition Regulation Subpart 23.4 to the maximum extent practical.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:21Z
Check the source to verify that this is the current version before use.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

NOTE: The following National Stock Numbers are covered by this document:

6525-00-604-2160 (Type 1)
6525-00-616-7679 (Type 2)

Note: 1. NSN 6525-00-604-2160 shall be suitable for use with NSN 6525-00-616-7651, Processing unit, x-ray film, 2 compartment, with rear panel.

2. NSN 6525-00-616-7679 shall be suitable for use with NSN 6525-00-616-7400, Tank, master, x-ray film processing, refrigerated, single compartment.

Ordering data. Intermediate/exterior package quantities, labeling, and marking must be specified in the contract and/or order.

MILITARY INTERESTS:

Custodians:

Army - MD
Navy - MS
Air Force - 03

PREPARING ACTIVITY:

DoD - MB

Agent:

DLA-DM

CIVIL AGENCY COORDINATING ACTIVITIES:

VA-OSS
PHS
FDA-MPQAS

Project No. 6525-1235

PGC 60391
05373

Location: CID/TANK/INSERT/H13-32

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:21Z
Check the source to verify that this is the current version before use.

STRUCTIONS. In a continuing effort to make our standardization documents better, the DoD provides this form for use in ›mitting comments and suggestions for improvements. All users of military standardization documents are invited to provide ¡gestions. This form may be detached, folded along the lines indicated, taped along the loose edge *(DO NOT STAPLE)*, and ¡led. In block 5, be as specific as possible about particular problem areas such as wording which required interpretation, was › rigid, restrictive, loose, ambiguous, or was incompatible, and give proposed wording changes which would alleviate the ›blems. Enter in block 6 any remarks not related to a specific paragraph of the document. If block 7 is filled out, an .nowledgement will be mailed to you within 30 days to let you know that your comments were received and are being ısidered.

'TE. This form may not be used to request copies of documents, nor to request waivers, deviations, or clarification of cification requirements on current contracts. Comments submitted on this form do not constitute or imply authorization waive any portion of the referenced document*(s)* or to amend contractual requirements.

(Fold along this line)

(Fold along this line)

NSE LOGISTICS AGENCY

ICIAL BUSINESS
ALTY FOR PRIVATE USE $300

NO POSTAGE NECESSARY IF MAILED IN THE UNITED STATES

BUSINESS REPLY MAIL
FIRST CLASS PERMIT NO 4966 WASHINGTON D C

POSTAGE WILL BE PAID BY THE DEFENSE LOGISTICS AGENCY

Commander
Defense Personnel Support Center
ATTN: DPSC- RSTE
2800 South 20th Street
Philadelphia, Pennsylvania 19101-8419

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:21Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

(See Instructions – Reverse Side)

1. DOCUMENT NUMBER	2. DOCUMENT TITLE
A-A-53585	TANK, INSERT, X-RAY FILM PROCESSING

3a. NAME OF SUBMITTING ORGANIZATION	4. TYPE OF ORGANIZATION *(Mark one)*
	☐ VENDOR
	☐ USER
b. ADDRESS *(Street, City, State, ZIP Code)*	☐ MANUFACTURER
	☐ OTHER *(Specify)*:

5. PROBLEM AREAS

a. Paragraph Number and Wording:

b. Recommended Wording.

c. Reason/Rationale for Recommendation

6. REMARKS

7a. NAME OF SUBMITTER *(Last, First, MI)* – Optional	b. WORK TELEPHONE NUMBER *(Include Area Code)* – Optional
c. MAILING ADDRESS *(Street, City, State, ZIP Code)* – Optional	8. DATE OF SUBMISSION *(YYMMDD)*

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:21Z
Check the source to verify that this is the current version before use.