MILITARY SPECIFICATION

COVER, SURGICAL INSTRUMENT STAND,
BAG TYPE

1. SCOPE

1.1 This specification covers a suitable bag type protective cover for use with an adjustable, surgical instrument stand (see 6.1).

2. APPLICABLE DOCUMENTS

2.1 The following documents of the issue in effect on date of invitation for bids or request for proposal, form a part of this specification to the extent specified herein:

SPECIFICATIONS

V-T-276	Thread, Cotton.
CCC-C-461	Cloth, Uniform Twill, Cotton.
CCC-T-191	Textile Test Methods.
DDD-L-20	Label, for Clothing, Equipage, and Tentage, (General Use).
DDD-T-86	Tape, Textile, Cotton, General Purpose, (Unbleached, Bleached or Dyed).
PPP-B-585	Boxes, Wood, Wirebound.
PPP-B-601	Boxes, Wood, Cleated-Plywood.
PPP-B-621	Boxes, Wood, Nailed and Lock-Corner.
PPP-B-636	Box, Fiberboard.

Military

MIL-L-10547	Liners, Case, and Sheet, Overwrap; Water-Vaporproof or Waterproof, Flexible.

STANDARDS

Military

MIL-STD-105	Sampling Procedures and Tables for Inspection by Attributes.
MIL-STD-129	Marking for Shipment and Storage.

FSC 6530

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:31Z
Check the source to verify that this is the current version before use.

(Copies of specifications and standards required by suppliers in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.)

2.2 Other publication. The following document forms a part of this specification to the extent specified herein. Unless otherwise indicated, the issue in effect on date of invitation for bids or request for proposal shall apply.

MUNSELL COLOR COMPANY

Munsell Color Company Color Book.

(Application for copies of Munsell color standards should be addressed to the Munsell Color Company, 10 East Franklin Street, Baltimore, Md.)

3. REQUIREMENTS

3.1 Materials.

3.1.1 Cloth, cotton. The basic material used in the fabrication of the cover shall be a cotton uniform twill cloth conforming to type IV of CCC-C-461.

3.1.2 Thread, cotton. The cotton thread used for stitching and seaming shall conform to type IA3, 3-ply, ticket No. 50 of V-T-276.

3.1.3 Color. The cotton uniform twill cloth and the thread shall be vat-dyed to a uniform grayish green shade identified in the Munsell Color Company Book as follows:

Hue	8BG to 2B
Value	5.0 to 6.0
Chroma	1.5 to 2.5

The color shall be approximately identified as 10BG 5.6/2.0 , although its hue, value, and chroma may fall within the ranges listed above.

3.1.4 Tape. Tape shall conform to DDD-T-86, and shall be type I, class 1, 1/2 inch wide.

3.2 Construction. The cover shall be constructed as shown on figure 1, with one end open. Not more than four pieces of cloth shall be used in fabricating the cover. Each piece shall be at least the full length or full width of the cover, as applicable, in one dimension, and not less than 9 inches in the other (finished dimensions). All raw edges shall be turned under and stitched, or they shall be enclosed by binding tape and stitched. Stitching shall be 12 to 16 stitches per inch. After fabrication, the cover shall be turned inside out, so that the hem and seams or binding tape are on the inside.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:31Z
Check the source to verify that this is the current version before use.

3.3 Identification marking. The cover shall be marked on the inside of the cover 1/2 to 1 inch below the hem, using type III or IV markings as specified in DDD-L-20. Markings shall be fast to laundering. Markings shall include the following:

Stock number.
Item identification.
Contractor's name or registered trademark.
Contract number.

Letters shall be at least 1/8 inch high.

3.4 Workmanship. The finished cover shall conform to the quality of product established by this specification. The occurrence of defects shall not exceed the limits set by the applicable acceptable quality levels.

4. QUALITY ASSURANCE PROVISIONS

4.1 Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the supplier is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified, the supplier may utilize his own facilities or any commercial laboratory acceptable to the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

4.2 Inspection for acceptance. Inspection shall be conducted in accordance with MIL-STD-105, except where otherwise indicated hereinafter.

4.2.1 Inspection of components. An inspection (examination and testing) of components shall be made in accordance with the quality assurance provisions contained in the applicable subsidiary specifications referenced herein to the extent applicable, except that this specification shall govern in the event of conflict.

4.2.2 Inspection of the end item. An examination shall be made on the finished cover for visual and dimensional defects.

4.2.2.1 Examination for visual defects. The defects found during this examination shall be classified in accordance with the defects listed in 4.2.2.2 and 4.2.2.3. The sample unit for this examination shall be one cover. The lot size shall be expressed in units of one cover. The sample size shall be selected in accordance with inspection level II of MIL-STD-105. The acceptable quality levels shall be as specified below:

Major	2.5 defects per 100 units
Total (major and minor)	6.5 defects per 100 units

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:31Z
Check the source to verify that this is the current version before use.

4.2.2.2 Classification of defects.

	MAJOR	MINOR
Material defects and damages:		
a. Holes or seriously weakening defects such as smashes, floats, loose and weakening slubs, etc., expected to develop into a hole.	X	
b. Heavy shade bars, unsightly slubs, etc., or any defect affecting appearance on the outside.	X	
c. Needle chews which may develop into a hole, scissors, or knife cuts, tears, mends, or burns.	X	
Shaded parts:		
Any part noticeably shaded.	X	
Cleanness:		
a. Spots or stains of a permanent nature.	X	
b. Thread ends not trimmed, loose threads, and removable spots or stains not removed.		X
Component and assembly:		
a. Any defect of component or assembly.	X	
b. Any component part or required operation omitted.	X	
c. Length of any piece less than full width or full length of the cover, as applicable.	X	
d. Width of any piece less than 9 inches.	X	
Cutting:		
a. Component part not cut in conformance with those shown on figure 1.	X	
b. More than four pieces used to fabricate the cover.	X	
Seams and stitching:		
a. Seams puckered, twisted, or pleated, affecting appearance.	X	
b. Thread breaks.		X
c. Gauge of stitching: Irregular, i.e., unevenly gauged or not uniformly gauged, affecting appearance.		X

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:31Z
Check the source to verify that this is the current version before use.

	MAJOR	MINOR
d. Open seam more than 1/4 inch.	X	
e. Hem less than 3/4 inch or more than 1 inch.		X
f. Raw edges more than 1/4 inch.		X
g. Raw edges of cloth exposed.	X	
h. Less than 12 or more than 16 stitches per inch.		X
Identification marking:		
a. Not accomplished as specified.	X	
b. Missing, incorrect, or illegible.		X

4.2.2.3 Examination for dimensional defects. During this examination, any measurement deviating from the nominal dimension and tolerance specified on figure 1 shall be scored as a size measurement defect. The sample unit for this examination shall be one cover. The lot size shall be expressed in units of one cover. The sample size shall be in accordance with inspection level S-3 of MIL-STD-105. The acceptable quality level shall be 4.0 (one class) defects per 100 units.

4.3 Tests. All required testing shall be conducted in accordance with the test requirements contained in the subsidiary specifications as listed in 2.1, and in accordance with the test methods prescribed in CCC-T-191.

5. PREPARATION FOR DELIVERY

5.1 Packaging.

5.1.1 Unit of issue. One (1) bag, as specified, constitutes one unit of issue.

5.1.2 Packaging quantities. The number of units of issue indicated in table I shall be packaged in each unit, intermediate, and exterior container, as applicable, for the required level of protection specified in the procurement document.

Table I. Packaging quantities

Unit package	Intermediate package	Exterior container
1 unit	12 units	24 units

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:31Z
Check the source to verify that this is the current version before use.

5.1.2.1 Packing variation permitted. If the required number of units to be shipped is less than the number of units specified to be overpacked in an exterior container, such units shall be packed in an exterior container of suitable size and design, acceptable to a common carrier, which shall insure safe delivery to destination.

5.1.3 Level A.

5.1.3.1 Unit package. Each unit shall be neatly folded and packaged compactly in a polyethylene bag of appropriate size and design. Closure of bag shall be effected by heat sealing.

5.1.3.2 Intermediate package. Intermediate package shall be a box of appropriate size and design constructed in accordance with PPP-B-636, type CF, class domestic. Closure of box shall be adequate to prevent spillage of contents under normal handling.

5.2 Packing.

5.2.1 Level A.

5.2.1.1 Exterior container. Exterior container shall be designed for type 2 load, and constructed in accordance with PPP-B-585, style 3, for class 3 use; PPP-B-601, table II, using type III, class 1 plywood; PPP-B-621, table III; or PPP-B-636, type CF, class weather-resistant.

5.2.1.2 Case liner. Each level A wood box shall be lined with a waterproof case liner conforming to MIL-L-10547. Closure and sealing shall conform to applicable paragraphs of appendix thereto. Case liner shall not be required for fiberboard boxes.

5.2.1.3 Closure. Closure of wood boxes shall be in accordance with appendix of applicable box specification. Closure of each fiberboard box shall be as specified in the appendix of PPP-B-636. In addition, waterproofing shall be as specified in 30.4 of PPP-B-636.

5.2.1.4 Strapping. Strapping, when required, shall be in accordance with appendix of applicable box specification.

NOTE: Strapping shall not be required for shipments forwarded to a receiving activity within the continental limits of the United States for storage and redistribution.

5.2.2 Level B.

5.2.2.1 Exterior container. Exterior container shall conform to PPP-B-601, table I, using type III, class 1 plywood; or shall be designed for type 2 load, and constructed in accordance with PPP-B-585, style 3, for class 2 use; PPP-B-621, table I; or PPP-B-636, type CF, class domestic. Closure of fiberboard boxes shall be in accordance with method I of appendix to box specification

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:31Z
Check the source to verify that this is the current version before use.

5.3 Marking.

5.3.1 Interior packages. Each unit package and each intermediate package shall be marked in accordance with MIL-STD-129. When labels are utilized, waterproofing shall be required only when applicable carton is fabricated of water-resistant material. Contract or purchase order number and name of contractor shall be shown. Unit package markings shall be printed directly on the bag, or on a label inserted within the bag in such a manner as to permit ready identification.

5.3.2 Exterior container. Exterior container shall be marked in accordance with MIL-STD-129.

6. NOTES

6.1 Intended use: The cover, surgical instrument stand, bag type, is intended for use with FSNs 6530-708-1590, Stand, Surgical Instrument, Adjustable, Corrosion-Resisting Steel, and 6530-551-8681, Stand, Surgical Instrument, Adjustable, Steel, Olive Drab Enameled, Field.

6.2 Ordering data. Procurement documents should specify the following:

(a) Number and date of this specification.
(b) Selection of applicable levels of packing (see 5.2).

6.2 This specification does not include all types, classes, grades, sizes, etc., of the commodity indicated by the title of this specification, or which are commercially available, but is intended to cover the types, etc., which are normally procured to meet Military requirements.


Custodians:
Army - MD
Navy - MS
Air Force - 03

Review activities:
Army - MD
Navy - MS
Air Force - 03

Preparing activity:
Defense Supply Agency - DM

Review information is current as of the date of this document. For future coordination of changes to this document, draft circulation should be based on the information in the current DODISS.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:31Z
Check the source to verify that this is the current version before use.

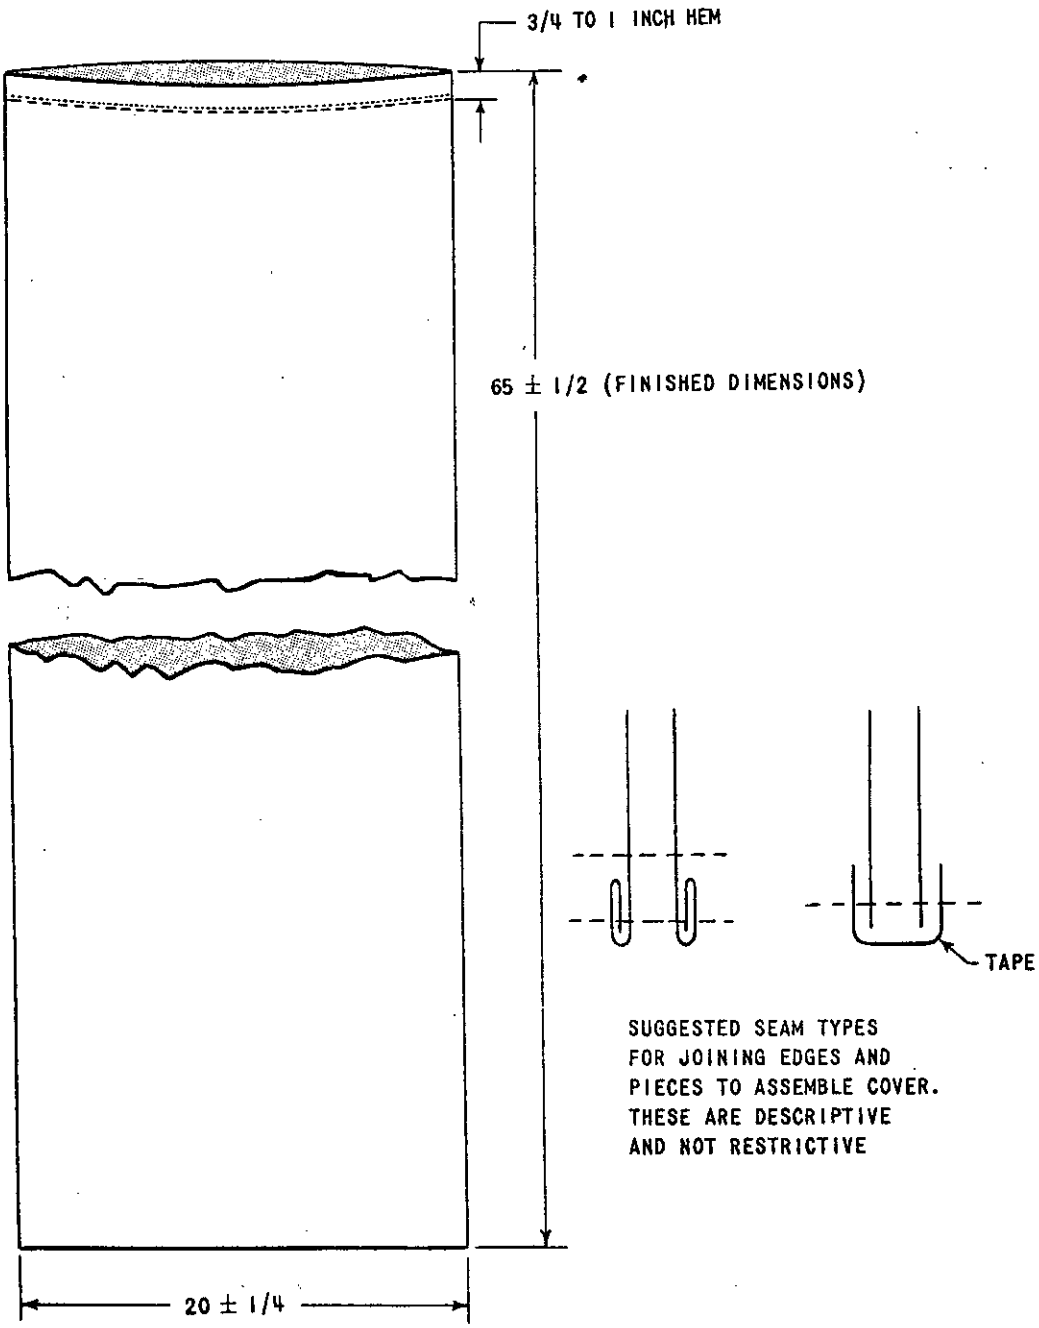

COVER, SURGICAL INSTRUMENT STAND
6530-890-2026

FIGURE 1

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:31Z
Check the source to verify that this is the current version before use.

SPECIFICATION ANALYSIS SHEET

Form Approved
Budget Bureau No. 119-R004

INSTRUCTIONS

This sheet is to be filled out by personnel either Government or contractor, involved in the use of the specification in procurement of products for ultimate use by the Department of Defense. This sheet is provided for obtaining information on the use of this specification which will insure that suitable products can be procured with a minimum amount of delay and at the least cost. Comments and the return of this form will be appreciated. Fold on lines on reverse side, staple in corner, and send to preparing activity *(as indicated on reverse hereof)*.

SPECIFICATION MIL-C-36398(DM), COVER, SURGICAL INSTRUMENT STAND, BAG TYPE
DATED 25 FEBRUARY 1965

ORGANIZATION *(Of submitter)*	CITY AND STATE

CONTRACT NO.	QUANTITY OF ITEMS PROCURED	DOLLAR AMOUNT
		$

MATERIAL PROCURED UNDER A

☐ DIRECT GOVERNMENT CONTRACT ☐ SUBCONTRACT

1. HAS ANY PART OF THE SPECIFICATION CREATED PROBLEMS OR REQUIRED INTERPRETATION IN PROCUREMENT USE?

A. GIVE PARAGRAPH NUMBER AND WORDING.

B. RECOMMENDATIONS FOR CORRECTING THE DEFICIENCIES.

2. COMMENTS ON ANY SPECIFICATION REQUIREMENT CONSIDERED TOO RIGID

3. IS THE SPECIFICATION RESTRICTIVE?

☐ YES ☐ NO IF "YES", IN WHAT WAY?

4. REMARKS *(Attach any pertinent data which may be of use in improving this specification. If there are additional papers, attach to form and place both in an envelope addressed to preparing activity)*

SUBMITTED BY *(Printed or typed name and activity)*	DATE

3ND PPSO 12502

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:31Z
Check the source to verify that this is the current version before use.

CAUTION

NOTICE TO BIDDERS/OFFERORS

DO NOT CONDITION OR BASE YOUR BID/OFFER ON ANY CURRENT PROCUREMENT ON THE INFORMATION SUBMITTED ON THIS FORM SINCE ANY CHANGES OR DELETIONS IN THE SPECIFICATIONS MAY RENDER YOUR BID/OFFER NON-RESPONSIVE IN WHICH CASE IT CANNOT BE CONSIDERED FOR AWARD.

FOLD UNDER

DEFENSE SUPPLY AGENCY
DEFENSE MEDICAL SUPPLY CENTER
3RD AVENUE AND 29TH STREET
BROOKLYN, N.Y., 11232

OFFICIAL BUSINESS

POSTAGE FEES PAID
DEFENSE SUPPLY AGENCY

DEFENSE SUPPLY AGENCY

DEFENSE MEDICAL SUPPLY CENTER

ATTN: DIRECTORATE OF TECHNICAL OPERATIONS (CODE TM5)

3RD AVENUE AND 29TH STREET

BROOKLYN, N.Y., 11232

FOLD

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:31Z
Check the source to verify that this is the current version before use.