MIL-P-36403B
26 July 1967
SUPERSEDING
MIL-P-36403A
22 September 1965

MILITARY SPECIFICATION

PAD, DENTAL RUBBER DAM

This specification is mandatory for use by all Departments and Agencies of the Department of Defense.

1. SCOPE.

1.1 Scope. This specification covers a disposable pad suitable for use during dental operative procedures involving the use of a rubber dam.

2. APPLICABLE DOCUMENTS

2.1 The following documents of the issue in effect on date of invitation for bids or request for proposal, form a part of this specification to the extent specified herein:

SPECIFICATIONS

Federal

CCC-T-191	Textile Test Methods.
PPP-B-585	Boxes, Wood, Wirebound.
PPP-B-601	Boxes, Wood, Cleated-Plywood.
PPP-B-621	Boxes, Wood, Nailed and Lock-Corner.
PPP-B-636	Box, Fiberboard.

Military

MIL-L-10547	Liners, Case, and Sheet, Overwrap; Water-Vaporproof or Waterproof, Flexible.

STANDARDS

Military

MIL-STD-105	Sampling Procedures and Tables for Inspection by Attributes.
MIL-STD-129	Marking for Shipment and Storage.

FSC 6520

Source: https://assist.dla.mil -- Downloaded: 202610-21T08:32Z
Check the source to verify that this is the current version before use.

(Copies of specifications and standards required by suppliers in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.)

3. REQUIREMENTS.

3.1 Material. The pad shall be fabricated from a plain weave, soft-filled, double-napped cotton flannelette of high commercial quality, suitable in every respect to serve the intended purpose.

3.2 Style, design, and dimensions. The pad shall be a disposable, protective, absorbent pad suitable for protecting the patient's face from irritation by a rubber dam or saliva during dental operative procedures involving use of the dam. The pad shall be in accordance with Figure 1 for style, design, and dimensions. The pad shall be cut on a bias and shall have clean-cut edges to minimize marginal threading. A pre-cut hole shall serve as a suitable mouth opening.

3.3 Physical properties. The finished cloth shall conform to the physical properties specified in 3.3.1 through 3.3.3.

3.3.1 Fiber identification. Pads shall be of the material specified in 3.1, when determined as specified in 4.4.1.

3.3.2 Weight per square yard. The weight per square yard shall be a minimum of 3.25 ounces and a maximum of 3.75 ounces, when determined as specified in 4.4.2.


3.3.3 Yarns per inch. The warp shall contain a minimum of 42 yarns per inch and the filling shall contain a minimum of 40 yarns per inch, when determined as specified in 4.4.3.

3.4 Color. Color of the pad shall be white.

3.5 Odor. Pads shall be free from objectionable odor.

3.6 Workmanship. Workmanship shall be first class throughout. Pads shall be free from defects (such as tears or cuts) which detract from their appearance or may impair their serviceability.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:32Z
Check the source to verify that this is the current version before use.

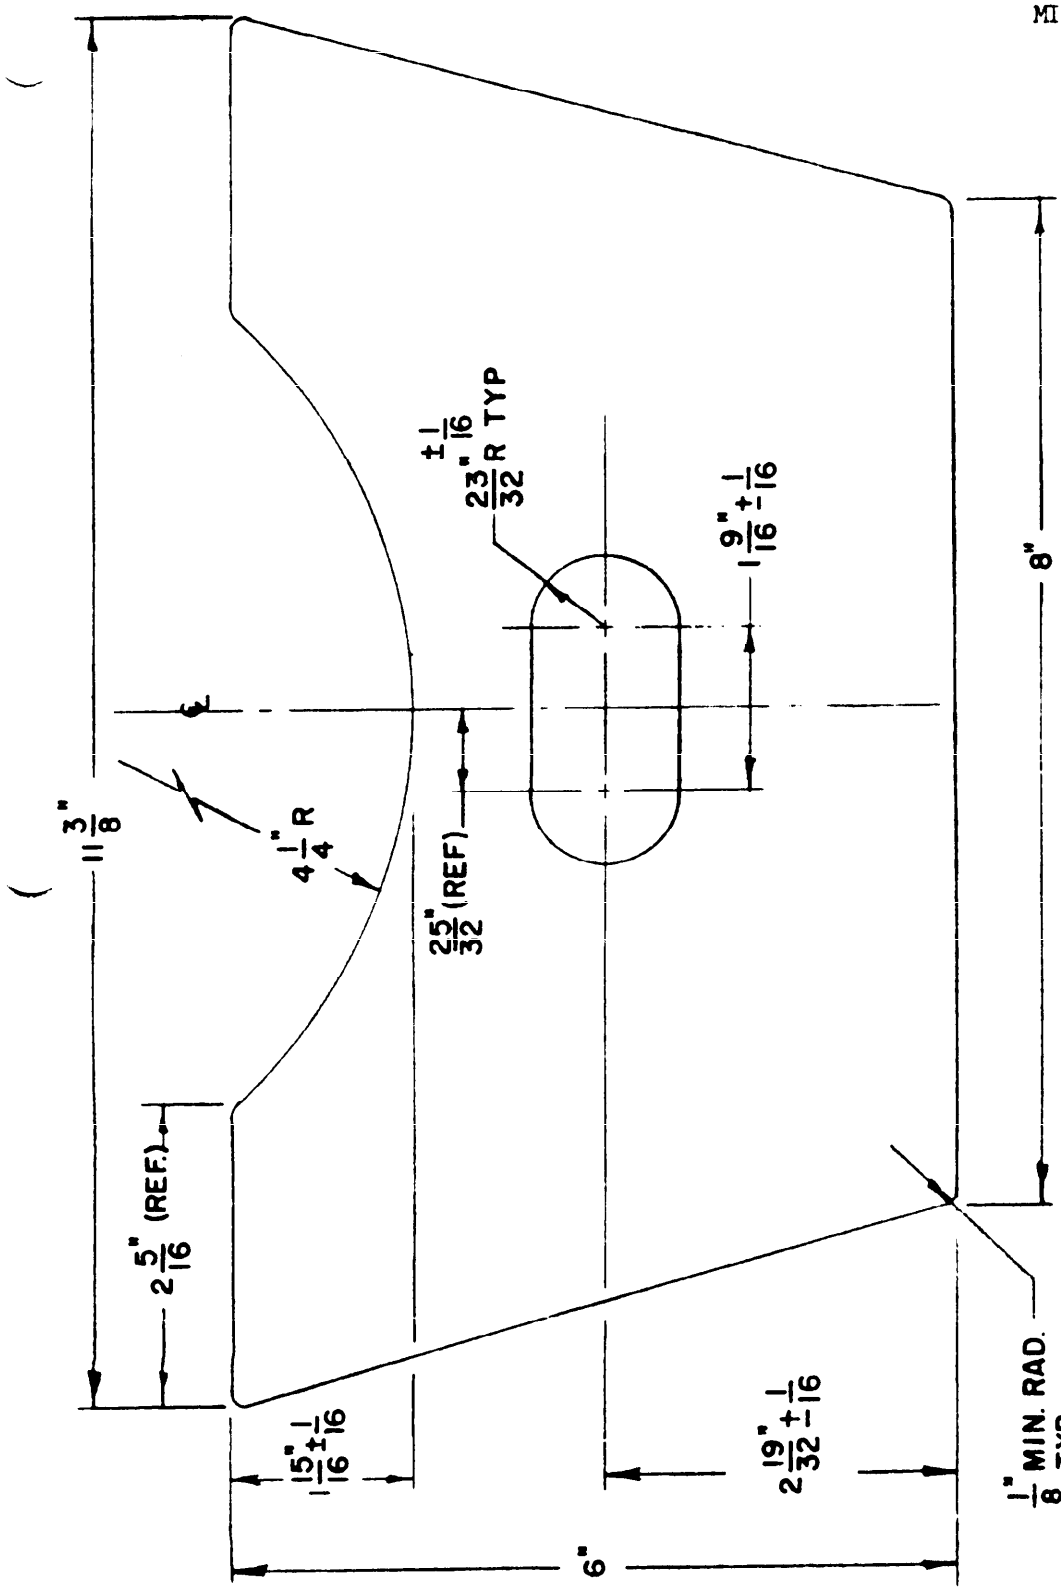

TOLERANCE FOR ALL DIMENSIONS ± 1/4" EXCEPT WHERE SHOWN OTHERWISE.
ROUND ALL SHARP EDGES.

FIGURE 1 PAD, DENTAL RUBBER DAM

Source: https://assist.dla.mil -- Downloaded: 202610-21T08:32Z
Check the source to verify that this is the current version before use.

4. QUALITY ASSURANCE PROVISIONS.

4.1 Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the supplier is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified, the supplier may utilize his own facilities or any commercial laboratory acceptable to the Government. The Government reserves the right to perform any of the inspections set forth in the specification, where such inspections are deemed necessary to assure that supplies and services conform to prescribed requirements.

4.1.1 Inspection. Inspection, as used in this specification, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties).

4.1.2 Certificates of quality. When available, certificates of quality, supplied by the manufacturer of the component or material, listing the specified test method and test results obtained, may be furnished in lieu of actual performance of such testing by the contractor.

4.2 Sampling.

4.2.1 For examination. Sampling for examination shall be conducted in accordance with MIL-STD-105. The inspection levels and the acceptable quality levels (AQL's) shall be as indicated in table I.

Table I. Examination Criteria

Type defect	Inspection level	AQL (Percent defective)
Classification of defects:		
Major	II	2.5
Minor	II	4.0
Dimensional	S-2	4.0

Source: https://assist.dla.mil -- Downloaded: 202610-21T08:32Z
Check the source to verify that this is the currentversion before use.

4.2.2 For tests. Sampling for tests shall be conducted as follows. One sample unit from each lot of raw flannelette shall be tested. The sample unit shall be of sufficient size to perform completely all the tests on the specimens required in the referenced test methods of table II.

Table II. Test Criteria

Characteristic	Requirement	Test Method
Fiber identification	3.3.1	4.4.1
Weight per square yard	3.3.2	4.4.2
Yarns per inch	3.3.3	4.4.3

4.3 Examination. The pads shall be examined to determine compliance with specification requirements.

4.3.1 Classification of defects. Examination shall be conducted in accordance with the following classification of defects, but not restricted thereto.

Table III. Classification of Defects

Category	Defect
Major:	
101	Pad not cut on a bias.
102	Weave other than plain.
103	Excess marginal threading, edges not clean-cut.
104	Pad not soft, or is noticeably irritating to face.
105	Pad not double napped.
106	Pad torn or cut.
Minor:	
201	Color other than white.
202	Pad not clean, or not free from foreign matter.
203	Pad not absorbent.
204	Pad has objectionable odor.
205	Packing, packaging, or marking not as specified.

Source: https://assist.dla.mil -- Downloaded: 202610-21T08:32Z
Check the source to verify that this is the current version before use.

4.3.2 Dimensional examination. The pads shall be examined for dimensional defects. Any dimension not within the tolerances specified in Figure 1 shall be classified as a defect.

4.4 Tests.

4.4.1 Fiber identification. Identification of the fiber of the pad shall be made in accordance with Method 1200 of CCC-T-191.

4.4.2 Weight per square yard. The weight per square yard shall be determined in accordance with Method 5041.1 of CCC-T-191.

4.4.3 Yarns per inch. The yarns per inch shall be determined in accordance with Method 5050.2 of CCC-T-191.

5. PREPARATION FOR DELIVERY.

5.1 Packaging.

5.1.1 Unit of issue. One box (50 pads), as specified, constitutes one unit of issue.

5.1.2 Packaging quantities. The number of units of issue indicated in table IV shall be packaged in each unit and exterior container, as applicable, for the required level of protection specified in the procurement document.

Table IV. Packaging Quantities

Unit package	Intermediate package	Exterior container
1 unit	Not required	24 units

5.1.2.1 Packing variation permitted. If the required number of units in the entire shipment is less than the number of units specified to be overpacked in an exterior container, such units shall be packed in an exterior container of suitable size and design, acceptable to a common carrier, which shall insure safe delivery to destination.

5.1.3 Level A.

5.1.3.1 Unit package. Each unit shall be packaged in a carton of suitable size and design. Closure of carton shall be adequate to prevent spilling of contents under normal handling.

Source: https://assist.dla.mil -- Downloaded: 202640-21T08:32Z
Check the source to verify that this is the currentversion before use.

5.2 Packing.

5.2.1 Level A.

5.2.1.1 Exterior container. Exterior container shall be designed for type 2 load, and constructed in accordance with PPP-B-585, style 3, for class 3 use; PPP-B-601, table II, using type I, class 1 plywood; PPP-B-621, table III; or PPP-B-636, type CF, class weather-resistant. Closure and strapping shall be in accordance with appendix of applicable box specification.

5.2.1.2 Case liner. Each level A wood box shall be lined with a waterproof case liner conforming to MIL-L-10547. Closure and sealing shall conform to applicable paragraphs of appendix thereto. Case liner shall not be required for fiberboard boxes.

NOTE: Strapping shall not be required for shipments forwarded to a receiving activity within the continental limits of the United States for storage and redistribution.

5.2.2 Level B.

5.2.2.1 Exterior container. Exterior container shall conform to PPP-B-601, table I, using type III, class 1 plywood; or shall be designed for type 2 load, and constructed in accordance with PPP-B-585, style 3, for class 2 use; PPP-B-621, table I; or PPP-B-636, type CF, class domestic and method I closure shall be utilized.

5.3 Marking.

5.3.1 Interior packages. Each unit package shall be marked in accordance with MIL-STD-129. When labels are utilized, waterproofing shall be required only when applicable carton is fabricated of water-resistant material. Contract or purchase order number and name of contractor shall be shown.

5.3.2 Exterior container. Exterior container shall be marked in accordance with MIL-STD-129.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:32Z
Check the source to verify that this is the current version before use.

6. NOTES.

6.1 Ordering data. Procurement documents should specify the following:

(a) Number and date of this specification.
(b) Selection of applicable levels of packaging and packing (See 5.1 and 5.2).

6.2 This specification does not include all types, classes, grades, or sizes of the commodity indicated by the title of this specification, or which are commercially available, but is intended to cover the types which are normally procured to meet Military requirements.

Custodians:
Army - MD
Navy - MS
Air Force - 03

Preparing activity:
Defense Supply Agency - DM

Review activities:
Army - MD
Navy - MS
Air Force - 03

Review information is current as of the date of this document. For future coordination of changes to this document, draft circulation should be based on the information in the current DODISS.

Category N.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:32Z
Check the source to verify that this is the current version before use.

SPECIFICATION ANALYSIS SHEET

Form Approved
Budget Bureau No. 22-R255

INSTRUCTIONS: This sheet is to be filled out by personnel, either Government or contractor, involved in the use of the specification in procurement of products for ultimate use by the Department of Defense. This sheet is provided for obtaining information on the use of this specification which will insure that suitable products can be procured with a minimum amount of delay and at the least cost. Comments and the return of this form will be appreciated. Fold on lines on reverse side, staple in corner, and send to preparing activity. Comments and suggestions submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or serve to amend contractual requirements.

SPECIFICATION

MIL-P-36403B

ORGANIZATION

CITY AND STATE

CONTRACT NUMBER

MATERIAL PROCURED UNDER A

☐ DIRECT GOVERNMENT CONTRACT ☐ SUBCONTRACT

1. HAS ANY PART OF THE SPECIFICATION CREATED PROBLEMS OR REQUIRED INTERPRETATION IN PROCUREMENT USE?

A. GIVE PARAGRAPH NUMBER AND WORDING.

B. RECOMMENDATIONS FOR CORRECTING THE DEFICIENCIES

2. COMMENTS ON ANY SPECIFICATION REQUIREMENT CONSIDERED TOO RIGID

3. IS THE SPECIFICATION RESTRICTIVE?

☐ YES ☐ NO *(If "yes", in what way?)*

4. REMARKS *(Attach any pertinent data which may be of use in improving this specification. If there are additional papers, attach to form and place both in an envelope addressed to preparing activity)*

SUBMITTED BY *(Printed or typed name and activity - Optional)*

DATE

DD FORM 1 JAN 88 1426

REPLACES EDITION OF 1 OCT 84, WHICH MAY BE USED.

Source: https://assist.dla.mil -- Downloaded: 202610-21T08:32Z
Check the source to verify that this is the current version before use.

CAUTION

NOTICE TO BIDDERS/OFFERORS

DO NOT CONDITION OR BASE YOUR BID/OFFER ON ANY CURRENT PROCUREMENT ON THE INFORMATION SUBMITTED ON THIS FORM SINCE ANY CHANGES OR DELETIONS IN THE SPECIFICATIONS MAY RENDER YOUR BID/OFFER NON-RESPONSIVE IN WHICH CASE IT CANNOT BE CONSIDERED FOR AWARD.

Fold

DEFENSE PERSONNEL SUPPORT CENTER
2800 SOUTH 20TH STREET
PHILADELPHIA, PA. 19101

DEFENSE SUPPLY AGENCY
OFFICIAL BUSINESS

POSTAGE AND FEES PAID
DEFENSE SUPPLY AGENCY

HEADQUARTERS, DEFENSE PERSONNEL SUPPORT CENTER
ATTN: DIRECTORATE OF MEDICAL MATERIEL
2800 SOUTH 20TH STREET
PHILADELPHIA, PA. 19101

Fold

DPSC FORM 2418
AUG 68

Source: https://assist.dla.mil -- Downloaded: 202610-21T08:32Z
Check the source to verify that this is the current version before use.