MIL-S-36366A
27 November 1972
SUPERSEDING
MIL-S-36366(DM)
2 January 1965

MILITARY SPECIFICATION

STERILIZER, SURGICAL INSTRUMENT

1. SCOPE

1.1 This specification covers a portable, dry heat sterilizer suitable for sterilizing dental and surgical instruments.

2. APPLICABLE DOCUMENTS

2.1 The following documents of the issue in effect on date of invitation for bids or request for proposal, form a part of this specification to the extent specified herein.

SPECIFICATIONS

Federal

QQ-A-250/1	Aluminum Alloy 1100, Plate and Sheet.
QQ-A-250/2	Aluminum Alloy 3003, Plate and Sheet.
QQ-A-250/8	Aluminum Alloy 5052, Plate and Sheet.
PPP-B-585	Boxes, Wood, Wirebound.
PPP-B-601	Boxes, Wood, Cleated-Plywood.
PPP-B-621	Boxes, Wood, Nailed and Lock-Corner.
PPP-B-636	Box, Fiberboard.

Military

MIL-M-7290	Manual Technical Commercial Equipment
MIL-A-8625	Anodic Coatings, for Aluminum and Aluminum Alloys.
MIL-L-10547	Liners, Case, and Sheet, Overwrap; Water-Vaporproof or Waterproof, Flexible.

STANDARDS

Federal

Fed. Std. No. 66 Steel: Chemical Composition and Hardenability.
Fed. Test Method Std. No. 151 Metals, Test Methods.

FSC 6530

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:28Z
Check the source to verify that this is the current version before use.

Military

MIL-STD-105	Sampling Procedures and Tables for Inspection by Attributes.
MIL-STD-129	Marking for Shipment and Storage.

(Copies of specifications and standards required by suppliers in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.)

UNDERWRITERS' LABORATORIES, INC.

Underwriters' Laboratories Standard:

UL 544 Standard for Medical and Dental Equipment.

(Underwriters' Laboratories Standards are available from the Underwriters' Laboratories, Inc., Walt Whitman Road, Melville, L. I., N. Y. 11749 207 East Ohio Street, Chicago, Ill. 60611, and 1655 Scott Boulevard, Santa Clara, Calif. 95050)

American National Standards Institute (ANSI)

C73.11 Plugs and Receptacles - General Purpose.
125 Volts, 15 Amperes, 2 Pole, 3 Wire, Grounding Type.

Applications for copies should be addressed to American National Standards Institute, 1430 Broadway, New York, N. Y. 10018.

3. REQUIREMENTS

3.1 Fire and casuality hazards.

3.1.1 The contractor shall submit proof, prior to delivery, that the items to be delivered under the contract conform to the applicable requirements of UL 544. Proof shall consist of one of the following:

A. UL label or UL listing of the product, provided the contractor agrees to have Underwriters' Laboratories, Inc. forward a copy of the UL report directly to the Contracting Officer, upon the latter's request.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:28Z
Check the source to verify that this is the current version before use.

B. Laboratory report from a qualified independent laboratory. If an independent laboratory is used, it must be adequately equipped and competent to determine compliance with UL standards. The qualification of such laboratory shall be determined by the Government which reserves the right to require a facilities report and to conduct a facilities survey. Any laboratory report submitted shall include actual test methods, data taken, and results of tests. Detailed findings of examinations necessary to determine compliance shall also be included. The test report shall also have a section that describes the test sample items with the test sample. This section shall be supplemented with construction information such as materials used, spacings between electrical components, types of bushings, photographs, wiring diagrams, sketches, and parts list, all appropriately identified. Compliance with this paragraph does not excuse compliance with all other requirements of the contract and specifications.

3.2 Material.

3.2.1 Corrosion-resisting steel. Corrosion-resisting steel used in the fabrication of the sterilizer shall conform to the requirements for chemical composition for 300 series of Fed. Std. No. 66.

3.2.2 Aluminum. Aluminum sheet used in the fabrication of the instrument trays shall be alloy 1100 of QQ-A-250/1 alloy 3003 of QQ-A-250/2, or alloy 5052 of QQ-A-250/8.

3.2.3 Plastic. The door handle, Knobs and other plastic parts shall be of heat-resistant phenol formaldehyde, plastic.

3.2.4 Heating elements. The heating elements used shall consist of resistance wire insulated by a suitable filler in a corrosion-resisting steel or aluminum sheath. Aluminum sheath shall be alloy 3003.

3.2.5 Heat insulation. The heat insulation material used shall be glass fiber.

3.2.6 Hardware. Nuts, bolts, screws, and other hardware shall be made of corrosion-resisting steel.

3.3 Construction. The sterilizer shall conform to Figure 1 for style and design. Material gages specified herein are minimum. Commercial tolerances shall apply to all gages.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:28Z
Check the source to verify that this is the current version before use.

3.3.1 Housing. The housing shall be fabricated of corrosion-resisting steel sheet 0.025 inch (No. 24, Unites States Standard (U.S.S.) gage) thick, minimum. The overall dimensions of the housing shall not exceed 16-1/4 inches by 10-3/4 inches by 11-3/8 inches. The housing shall be provided with a removable back cover plate to permit easy accessibility to the internal components. The housing shall be mounted on 1-inch diameter rubber or plastic feet or buttons, not less than 1/2 inch high, located at each corner. A removable bracket shall be secured to the front of the housing to support the scale end of the angle thermometer. A recessed, removable cover plate shall be secured to the side of the shell by screws and shall have a cutout to accomodate the shaft of the thermostat.

3.3.2 Sterilizing chamber. The sterilizing chamber shall be fabricated of 0.025 inch (No. 24 U.S.S. gage) thick minimum corrosion-resisting steel sheet. The chamber shall be attached to the inner frame of the housing shell with screws and a supporting strap. The inside dimensions of the chamber shall be a minimum of 12-1/4 inches long, 5-1/4 inches high and 7-1/4 inches wide. The opening shall be the full width and height of the chamber. Two angle-shaped tray supports shall be provided on each side of the chamber. The roof of the inner chamber shall have an inverted cup in which the bulb of the thermometer shall be located.

3.3.3 Door assembly. The door shall be fabricated of corrosion-resisting steel sheet 0.025 inch (No. 24, U.S.S. gage) thick. The door shall have a handle at the top and be securely attached to a continuous piano hinge at the bottom. The door panel shall be 14 inches by 6-3/4 inches, nominal dimensions. The door panel shall have a minimum of 1/2 inch thick pan securely attached to the inside surface. The pan shall fit snugly without binding into the opening of the sterilizing chamber, and shall be filled with glass fiber insulation. The top and side edges of the door panel shall be hemmed and bent at right angles providing a flange to which the door pan shall be attached. The bottom edge of the door panel shall be hemmed and bent out at an angle such that the door is supported in a horizontal position when open. The top and side edges of the door panel shall fit flush against the housing, and shall be faced with a felt gasket held in place with heat-resistant adhesive. A magnetic sensitive strip shall be secured to the door with heat-resistant adhesive, and shall be oriented to make contact with the magnetic door lock when the door is closed. Adhesive for the gasket and magnetic sensitive strip shall not dry out when tested as specified in 4.4.2.

3.4 Components.

3.4.1 Heating element. Two tubular heating elements shall be provided. The heating elements shall be located in the inner chamber of the sterilizer. Each element shall cover one side of the chamber and part of the bottom. The elements shall be separated from the wall and bottom of the chamber by ceramic bushings, except the element along the side closest to the thermostat shall be clamped directly to the chamber wall without ceramic bushings.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:28Z
Check the source to verify that this is the current version before use.

3.4.2 Timer switch. A timer switch shall be provided and shall be secured to the front panel of the housing as shown in Figure 1. The timer shall have a minimum range of 0 to 120 minutes automatic operation and shall be accurate to within ± 3 minutes when tested as specified in 4.4.1. A dial plate shall be provided to indicate a minimum time setting of 2 hours and to permit the operator to select, by controlling the shaft position of the timer switch, either the "HOLD" position for continuous operation or automatic time operation for the desired duration.

3.4.3 Lampholder. A lampholder with pilot light shall be provided to indicate operation of the sterilizer. The lampholder shall be mounted to the housing and shall be located as shown in Figure 1. The pilot light shall be activated by the timer switch. As an alternate, an additional pilot light indicating thermostat activation shall be acceptable.

3.4.4 Thermostat. A thermostat shall be provided and shall be securely attached to the chamber shell. A calibrated knob shall be supplied with the thermostat to select the desired temperature. The thermostat shall be adjustable by means of the adjustment knob and shall control the average chamber temperature to ± 3 degrees (Fahrenheit) as indicated on the unit thermometer at 320 degrees (F) and at 360 degrees (F) for at least 2 hours each when tested as specified in 4.4.1.

3.4.5 Magnetic door lock. A magnetic door lock shall be located on the front panel as shown in Figure 1. The lock shall hold the door assembly in closed position by contact with a magnetic strip on the door.

3.4.6 Thermometer. A mercury-type thermometer having a range of 100° F. to 400° F. shall be provided. Minimum graduations shall be at 10° F. intervals. The thermometer shall have an accuracy of ± 2-1/2° F.

3.4.7 Power supply cord. Each sterilizer shall be equipped with a three conductor power cord. A strain relief bushing shall be provided where the cord enters the sterilizer. The cord shall be equipped with a plug suitable for use with receptacles specified in ANSI C73.11, for Caps and Receptacles, 125 Volts, 15 Amperes, 2-Pole, 3-Wire Grounding Type. The cord shall withstand a 35 pound pull when tested as specified in 4.4.5.

3.4.8 Instrument trays. Three aluminum trays shall be supplied. Two of the trays shall be suitable for holding instruments, and shall have inside dimensions of 10 ± 1/8 inches long, 6-1/4 ± 1/8 inches wide, and 3/4 + 1/8 - 3/16 inches high. The two long sides shall have 1/4 inch hems. The two ends shall be flanged one at right angles for 1/2 inch. The bottoms of the trays shall be perforated with 3/16 inch diameter holes located on 7/16 inch centers. The two trays shall be capable of being easily inserted and removed from the chamber. The third tray shall be nonperforated, shall be suitable for holding needles and shall have minimum inside dimensions of 4-7/8 inches long, 1-7/16 inches wide and 1/2 inch high.

Source: https://assist.dla.mil -- Downloaded: 202640-21T08:28Z
Check the source to verify that this is the current version before use.

3.4.9 Instrument tray handle. A handle, similar to that shown in Figure 1, suitable for insertion and removal of instrument trays, shall be provided. The handle shall be designed to permit handling of the instrument trays without direct contact by the operator.

3.5 Design and performance. The sterilizer shall be designed for operation on 115 volts, 60 cycle alternating current. When starting at an ambient temperature of 72° F., the sterilizer shall reach an operating temperature of 320° F. in not more than 15 minutes. Test shall be conducted as specified in 4.4.1. The average temperature of the petrolatum shall not exceed 20 degrees (F) more than nor 5 degrees (F) less than average temperature indicated on the unit thermometer when tested as specified in 4.4.1.

3.5.1 Electrical input. The measured input of the sterilizer shall be not more than 105 percent of its marked rating. Tests shall be conducted as specified in 4.4.1.

3.5.2 Temperature rise. The temperature of the following parts shall not exceed the maximum temperatures specified below when tested as specified in 4.4.2.

Location	Temperature Degrees Centigrade (C.)
Supply cord inside unit at bushing	50
Supply cord at separation of conductors	76
Supply cord conductor at splice	76
Phenolic body of timer switch	82
Phenolic body of lampholder	94
Supporting surface under center	67
Supporting surface under foot mounting screws	46
Sterilizer compartment floor at center	190
Phenolic knob on thermostat control	65

3.5.3 Dielectric strength. There shall be no electrical breakdown when the sterilizer is subjected to the dielectric strength test specified in 4.4.3.

3.6 Weight. The sterilizer unit shall weigh not more than 15 pounds.

3.7 Finish. All corrosion-resisting steel surfaces shall have a uniform No. 4 commer ial finish. The aluminum trays shall be anodized in accordance with MIL-A-8625, Type II, Class 1.

3.8 Identification marking. Each unit shall be legibly and permanently marked in an inconspicuous location with the following information:

Federal stock number.
Manufacturer's name or registered trademark.
Contract or purchase order number.
U.S.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:28Z
Check the source to verify that this is the current version before use.

Nameplates shall be a minimum of 0.020 inch thick. In addition, the model number, serial number, and electrical characteristics shall appear. Marking secured by adhesives shall not be used.

3.9 Service Data. The contractor shall furnish, with each unit, two copies each of a technical manual which contains complete instructions for installation, operation, and maintenance and lists of compoenent parts. The manual shall comply with the requirements of MIL-M-7298. As soon as practicable after award of the contract or purchase order, the contractor shall furnish to the Contracting Officer, via the cognizant Government inspector, two preliminary copies of his proposed technical manual for review and comment by the Directorate of Medical Materiel, Defense Personnel Support Center. The preliminary manuals shall be submitted sufficiently early to permit adequate review by the Directorate of Medical Materiel, Defense Personnel Support Center (based on a maximum period of 30 days for such review) and to allow incorporation by the contractor of any required revisions and corrections in the final manual without delaying delivery under the contract, or purchase order. In addition, the contractor shall furnish 15 copies of the approved technical manual to the Contracting Officer for distribution. Should the supplier have furnished acceptable manuals for the identical item within two years preceding the date of the contract and propose to furnish manuals identical with those previously accepted, then the requirements for review of drafts and submission of 15 additional copies may be waived upon requests to the Contracting Officer, Waiver of submission of drafts and submission of 15 additional copies shall be at the option of the Government.

3.10 Workmanship. Workmanship shall be first class throughout. The sterilizers shall be free from defects which detract from their appearance or may impair their serviceability.

4. QUALITY ASSURANCE PROVISIONS

4.1 Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the supplier is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or order, the supplier may use his own or any other facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Source: https://assist.dla.mil -- Downloaded: 202610-21T08:28Z
Check the source to verify that this is the current version before use.

4.1.1 Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government, upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of 3 years after delivery of the supplies to which such records relate.

4.1.2 Inspection. Inspection, as used in this specification, is defined as both examination (such as visual, and auditory, investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

4.1.3 Certificates of quality. Certificates of quality, supplied by the manufacturers of the steel and aluminum may be furnished in lieu of actual performance of such testing by the contractor, provided lot identity has been maintained and can be demonstrated to the Government. The Certificates shall include the name of the contractor, the contract number, the name of the manufacturer or supplier, the FSN, the Item Identification, the name of the component or material, the lot number, the lot size, the sample size, the date of testing, the test method, individual test results, and the specification requirements.

4.2 Classification of Inspections.

4.2.1 For examination. Sampling for examination shall be conducted in accordance with MIL-STD-105, and Table I.

Table I

	Inspection level	AQL (defects per hundred units)
For visual examination		
Major defects	II	1.0
Minor defects	II	4.0
For dimensional examination	S-3	2.5

4.2.2 For tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and Table II.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:28Z
Check the source to verify that this is the current version before use.

Table II

Characteristic	Requirement	Test procedure	Inspection level
Adhesive heat resistance	3.3.3	4.4.2	*
Strain relief	3.4.7	4.4.5	S-2
Temperature rise	3.5.2	4.4.2	*
Dielectric strength	3.5.3	4.4.3	100%
Performance			
Input	3.5.1	4.4.1	S-2
Timer switch	3.4.2	4.4.1	S-2
Thermometer	3.4.6	4.4.1	S-2
Time to reach 320° F.	3.5	4.4.1	S-2
Thermostat accuracy	3.4.4	4.4.1	S-2

* One unit shall be tested from each lot.

4.2.3 Raw materials. Four ounces of each lot of metal used in the construction of the sterilizer shall be selected for chemical analysis.

4.3 Examination. The sterilizers shall be examined to determine compliance with all requirements contained in this specification.

4.3.1 Classification of defects. Examination shall be conducted in accordance with the following classification of defects:

Table III
Categories and defects*

Major	
101	Any component missing, broken, or otherwise unusable.
102	Exposed edges not free of burs and sharpness.
103	Door does not open and close freely.
104	Thermometer does not have minimum range specified.
105	Timer does not have minimum range specified.
106	Door does not fit chamber opening snugly without binding.
107	Magnetic door lock does not operate properly.
Minor A	
201	Instruction plate not permanently secured to sterilizer.
202	Finish scratched, marred, or otherwise defective.
203	Sterilizer does not rest evenly on flat surface.
204	Outside surfaces not No. 4 finish.
205	Trays not fitting smoothly on supports.
206	Nameplate missing, incomplete, or illegible.
207	Service data missing or does not include all specified information.
208	Instrument tray handle not capable of handling trays.

Source: https://assist.dla.mil -- Downloaded: 202640-21T08:28Z
Check the source to verify that this is the currentversion before use.

Minor B
251 Any dimension not within tolerance specified.

* Examination shall not be restricted to the classified possible defects listed above.

4.4 Tests. Tests shall be conducted to determine compliance with specification requirements.

4.4.1 Performance. Test shall be performed at an ambient room temperature between 68 and 80 degrees F. Suspend one thermocouple, No. 24 American Wire Gage (AWG) or smaller, in the center of a corrosion resisting steel or glass jar filled to within 1/2 inch of the top with petrolatum. Container shall be approximately 3 inches high by 3 inches in diameter and shall be placed on the bottom shelf with the top shelf removed. The sterilizer shall then be connected to a 115 volt 60 Hertz power source with a voltmeter and ammeter in the circuit. Set the thermostat for maximum control and set the timer to the hold position and begin to measure, the time required to reach 320 degrees F. as shown by the thermometer mounted on the unit. The chamber temperature shall be stabilized at 320 degrees F. by means of the thermostat control. The thermocouple readings shall be taken and recorded at 5 minute intervals for a period of 2 hours following stabilization at 320 degrees F. As an alternate, the thermocouple readings shall be continuously recorded. Following this period, the thermostat shall be adjusted until the chamber temperature as indicated by the thermometer on the sterilizer stabilizes at 360 degrees F. Thermocouple readings shall be taken and recorded every 5 minutes for a minimum of 2 hours. The report shall include:

a. Input current.
b. Time to reach 320 degrees F. on unit thermometer.
c. The average temperature of the thermocouple during stabliization at 320 degrees F. and 360 degrees F.
d. The swing of the unit thermometer during stabilization.

4.4.2 Temperature rise. The bottom mountings of the sterilizer shall be removed and the sterilizer shall be placed on a soft wood surface covered with a double layer of tissue paper. The thermostat shall be set to the maximum heat position. Thermocouples, consisting of wires not larger than No. 24 American Wire Gage (AWG) shall be connected at specific locations within the sterilizer. The sterilizer shall be connected to a 115 volt, 60 Hertz power source. The ambient temperature shall be 25 $\pm$ 5 degrees Centigrade. Measurements shall be taken when constant temperatures are obtained.

4.4.3 Dielectric strength. The sterilizer shall be connected to a 115 volt, 60 Hertz power source, the thermostat control shall be set to the maximum position and the timer set for a minimum of 5 minutes operation. During this period it should be observed if the timer activates and deactivates the heaters and indicator lights. Immediately following operation, while the unit is still in the heated condition, the unit shall be subjected to a gradually increasing 60 Hertz potential of from 0 to 1000 volts applied between live and dead metal parts. The voltage shall be maintained at 1000 volts for 1 minute.

Source: https://assist.dla.mil -- Downloaded: 202610-21T08:28Z
Check the source to verify that this is the current version before use.

4.4.4 Chemical composition. Tests for chemical analysis shall be conducted in accordance with method 111.2 or 112.2 of Fed. Test Method Std. No. 151.

4.4.5 Strain relief. The power supply cord shall be tested in accordance with UL 544.

5. PREPARATION FOR DELIVERY.

5.1 Packaging.

5.1.1 Unit of issue. One (1) sterilizer, as specified, constitutes one unit of issue.

5.1.2 Packaging quantities. The number of units of issue indicated in table IV shall be packaged in each unit, intermediate, and exterior container, as applicable, for the required level of protection specified in the procurement document.

Table IV. Packaging Quantities

Unit package	Intermediate package	Exterior container
1 unit	Not required	2 units

5.1.2.1 Packing variation permitted. If the required number of units to be shipped is less than the number of units specified to be overpacked in an exterior container, such units shall be packed in an exterior container of suitable size and design, acceptable to a common carrier, which shall insure safe delivery to destination.

5.1.3 Level A.

5.1.3.1 Unit package. Each sterilizer shall be wrapped with kraft paper or other suitable anticorrosive material and packaged in a box of appropriate size constructed in accordance with PPP-B-636, type CF, class domestic. The box shall be designed with suitable interior fittings or shall contain sufficient cushioning material to insure against shifting of or damage to the contents. Closure shall conform to method I as specified in the appendix of the box specification.

5.1.4 Level C. Units shall be packaged in standard commercial containers of the size and kind commonly used, which will afford the degree of protection required for shipment and use of the product for its intended purpose within the continental limits of the United States of America.

Source: https://assist.dla.mil -- Downloaded: 202610-21T08:28Z
Check the source to verify that this is the currentversion before use.

5.2 Packing.

5.2.1 Level A.

5.2.1.1 Exterior container. Exterior container shall be designed for type 2 load, and constructed in accordance with PPP-B-585, style 3, for class 3 use; PPP-B-601, overseas type; PPP-B-621, class 2 or PPP-B-636, type CF, class weather-resistant, grade V3c. Fiberboard boxes shall conform to the special requirements specified in Table II of PPP-B-636.

5.2.1.2 Case liner. Each level A wood box shall be lined with a waterproof case liner conforming to MIL-L-10547. Closure and sealing shall conform to applicable paragraphs of appendix thereto. Case liner shall not be required for fiberboard boxes.

5.2.1.3 Closure. Closure of wood boxes shall be in accordance with appendix of applicable box specification. Closure of each fiberboard box shall be as specified in the appendix, and waterproofing shall conform with 30.4, of PPP-B-636.

5.2.1.4 Strapping. Strapping, when required, shall be in accordance with appendix of applicable box specification.

NOTE: Strapping shall not be required for shipments forwarded to a receiving activity within the continental limits of the United States for storage and redistribution.

5.2.2 Level B.

5.2.2.1 Exterior container. Exterior container shall be designed for a type 2 load and constructed in accordance with PPP-B-585, class 1, style 3; PPP-B-601, domestic type; PPP-B-621, class 1; or PPP-B-636, type CF, class domestic. Fiberboard boxes shall conform to the special requirements as specified in table I of PPP-B-636. Closure shall be as specified in the appendix of the applicable box specification. Closure of fiberboard boxes shall conform to Method II as specified in PPP-B-636.

5.2.3 Level C. The subject commodity shall be packed in substantial commercial containers of the type, size, and kind commonly used for the purpose, so constructed as to insure acceptance and safe delivery by common or other carriers, at the lowest rate, to point of delivery called for in the contract or purchase order.

5.3 Marking.

5.3.1 Interior package. Each unit package shall be marked in accordance with MIL-STD-129. When labels are utilized, waterproofing shall be required only when applicable carton is fabricated of water-resistant material. Contract or purchase order number and name of contractor shall be shown. Commercial markings, when utilized, shall be acceptable provided that there shall be no interference with the intended purpose of the markings herein specified.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:28Z
Check the source to verify that this is the current version before use.

5.3.2 Exterior container. Exterior container shall be marked in accordance with MIL-STD-129.

6. NOTES

6.1 Intended use. Item is intended for use as a dry heat sterilizer for sterilizing dental and surgical instruments.

6.2 Ordering data. Procurement documents should specify the following:

(a) Number and date of this specification
(b) Selection of applicable levels of packaging and packing. (see 5.1 and 5.2).

6.3 This specification covers the following item appearing in the Federal Supply Catalog:

Federal Stock Number	Item Identification
6530-962-9965	STERILIZER, SURGICAL INSTRUMENT, Dry Heat Type, Electrically Heated, Corrosion-Resisting Metal, 11-1/2 by 6-1/2 by 5 inches, 110 Volt 60 Cycle, AC.

6.4 This specification does not include all types, classes, grades, and sizes of the commodity indicated by the title of this specification, or which are commercially available, but is intended to cover the types, etc., which are normally procured to meet Military requirements.

6.5 "The margins of this specification are marked with an asterisk to indicate where changes (additions, modifications, corrections, deletions) from the previous issue were made. This was done as a convenience only and the Government assumes no liability whatsoever for any inaccuracies in these notations. Bidders and contractors are cautioned to evaluate the requirements of this document based on the entire content irrecpective of the marginal notations and relationship to the last previous issue."

Custodians:
Army - MD
Navy - MS
Air Force - 03

Review activities:
Army - MD
Navy - MS
Air Force - 03

Preparing activity:
Defense Supply Agency - DM

Project No. 6530-1260

Review information is current as of the date of this document. For future coordination of changes to this document, draft circulation should be based on the information in the current DODISS.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:28Z
Check the source to verify that this is the current version before use.

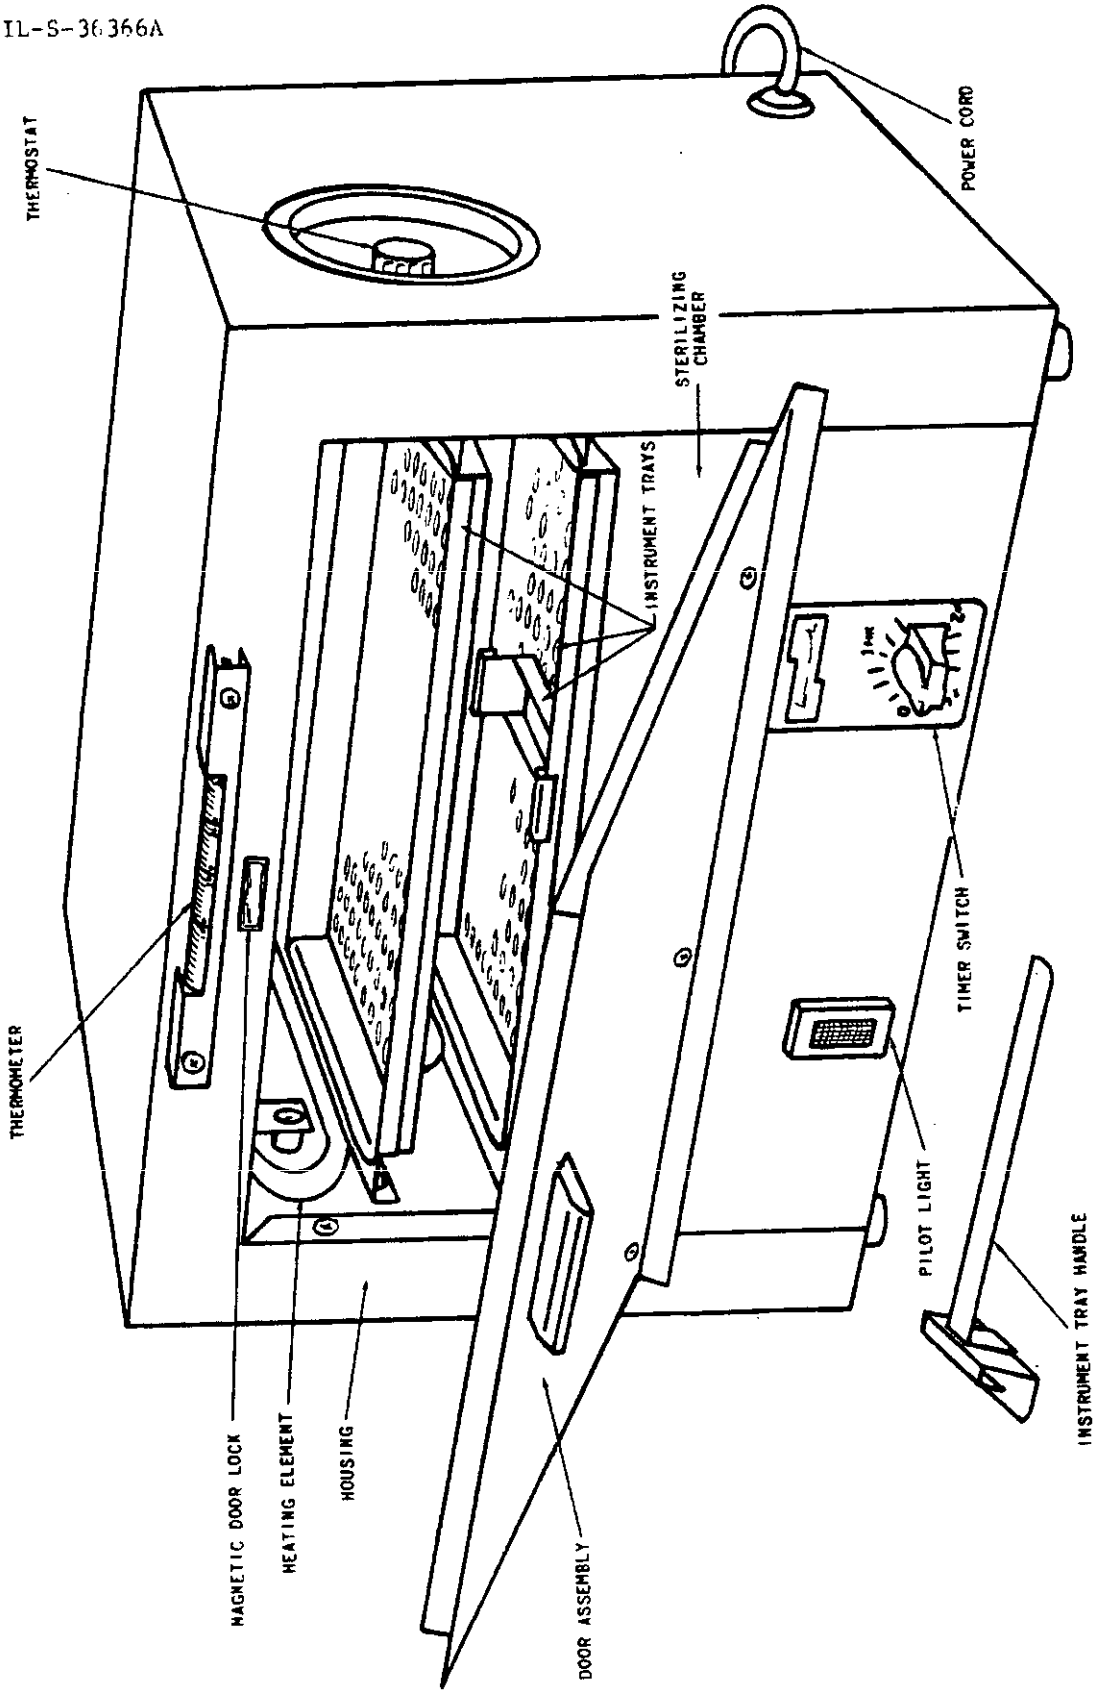


Figure 1

Source: https://assist.dla.mil -- Downloaded: 202610-21T08:28Z
Check the source to verify that this is the current version before use.

FOLD

DEFENSE PERSONNEL SUPPORT CENTER
2800 South 20th Street
Philadelphia, Pa. 19101

Defense Supply Agency

OFFICIAL BUSINESS
PENALTY FOR PRIVATE USE $300

POSTAGE AND FEES PAID
DEFENSE SUPPLY AGENCY
DoD - 304

U.S. MAIL

HEADQUARTERS, DEFENSE PERSONNEL SUPPORT CENTER
ATTN: DIRECTORATE OF MEDICAL MATERIEL, CODE ATT
2800 SOUTH 20TH STREET
PHILADELPHIA, PA. 19101

FOLD

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:28Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

OMB Approval
No. 22-R255

INSTRUCTIONS: The purpose of this form is to solicit beneficial comments which will help achieve procurement of suitable products at reasonable cost and minimum delay, or will otherwise enhance use of the document. DoD contractors, government activities, or manufacturers/vendors who are prospective suppliers of the product are invited to submit comments to the government. Fold on lines on reverse side, staple in corner, and send to preparing activity. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements. Attach any pertinent data which may be of use in improving this document. If there are additional papers, attach to form and place both in an envelope addressed to preparing activity.

DOCUMENT IDENTIFIER AND TITLE

MIL-S-36366A

NAME OF ORGANIZATION AND ADDRESS

CONTRACT NUMBER

MATERIAL PROCURED UNDER A

☐ DIRECT GOVERNMENT CONTRACT ☐ SUBCONTRACT

1. HAS ANY PART OF THE DOCUMENT CREATED PROBLEMS OR REQUIRED INTERPRETATION IN PROCUREMENT USE?

A. GIVE PARAGRAPH NUMBER AND WORDING.

B. RECOMMENDATIONS FOR CORRECTING THE DEFICIENCIES

2. COMMENTS ON ANY DOCUMENT REQUIREMENT CONSIDERED TOO RIGID

3. IS THE DOCUMENT RESTRICTIVE?

☐ YES ☐ NO *(If "Yes", in what way?)*

4. REMARKS

SUBMITTED BY *(Printed or typed name and address - Optional)*

TELEPHONE NO.

DATE

DD FORM 1 JAN 72 1426 REPLACES EDITION OF 1 JAN 66 WHICH MAY BE USED

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:28Z
Check the source to verify that this is the current version before use.