MIL-V-36372B
29 June 1977
SUPERSEDING
MIL-V-36372A
17 July 1973

MILITARY SPECIFICATION

VIBRATOR, DENTAL MOLDING, 115 VOLT, 60 HERTZ

This specification is approved for use by all Departments and Agencies of the Department of Defense.

1. SCOPE

1.1 Scope. This specification covers an electro-mechanical vibrator, suitable for use in prosthetic procedures.

2. APPLICABLE DOCUMENTS

2.1 Issues of documents. The following documents of the issue in effect on date of invitation for bids or request for proposals form a part of this specification to the extent specified herein.

SPECIFICATIONS

FEDERAL

PPP-B-585 - Boxes, Wood, Wirebound.
PPP-B-601 - Boxes, Wood, Cleated-plywood.
PPP-B-621 - Boxes, Wood, Nailed and Lock-corner.
PPP-B-636 - Box, Fiberboard.

MILITARY

MIL-P-116 - Methods of Preservation.
MIL-L-10547 - Liners, Case and Sheet, Overwrap; Water-Vaporproof or Waterproof, Flexible.

Beneficial comments (recommendations, additions, deletions) and any pertinent data which may be of use in improving this document should be addressed to: Headquarters, Defense Personnel Support Center, ATTN: Directorate of Medical Materiel, Code ATT, 2800 South 20th Street, Philadelphia, Pa. 19101, by using the self-addressed Standardization Document Improvement Proposal (DD Form 1426) appearing at the end of this document or by letter.

FSC 6520

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:29Z
Check the source to verify that this is the current version before use.

STANDARDS

FEDERAL

FED-STD-151 - Metal, Test Methods.

MILITARY

MIL-STD-105 - Sampling Procedures and Tables for Inspection by Attributes.
MIL-STD-129 - Marking for Shipment and Storage.

(Copies of specifications, standards, drawings, and publications required by contractors in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.)

2.2 Other publications. The following documents form a part of this specification to the extent specified herein. Unless otherwise indicated, the issue in effect on date of invitation for bids or request for proposals shall apply.

AMERICAN NATIONAL STANDARDS INSTITUTE, INC. (ANSI)

C73.11 - Dimensions of Plugs and Receptacles, General Purpose, 125 Volts, 15 Amperes, 2 Pole, 3 Wire, Grounding Type.

(Applications for copies should be addressed to the American National Standards Institute, Inc., 1430 Broadway, New York, NY 10018.)

UNDERWRITERS' LABORATORIES, INC.

UL1262 - Standard for Safety, Laboratory Equipment.

(Application for copies should be addressed to the Underwriters' Laboratories, Inc., 1285 Walt Whitman Road, Melville, L.I., NY, 11746; 207 E. Ohio Street, Chicago, Illinois, 60611; or 1655 Scott Blvd., Santa Clara, Calif. 95050.)

AMERICAN SOCIETY FOR TESTING AND MATERIALS (ASTM)

D790 - Standard Methods of Test for Flexual Properties of Plastic.

D2240 - Standard Method of Test for Indentation Hardness of Rubber and Plastics by Means of a Durometer.

(Application for copies should be addressed to the American Society for Testing and Materials, 1916 Race Street, Philadelphia, PA 19103.)

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:29Z
Check the source to verify that this is the current version before use.

3. REQUIREMENTS

3.1 Fire and casualty hazards.

3.1.1 The contractor shall submit proof, prior to delivery, that the items to be delivered under the contract conform to the applicable requirements of Underwriters' Laboratories, Inc. (U.L.) Standard of Safety 1262. Proof shall consist of one of the following:

A. U.L. label affixed to the product, provided the contractor agrees to have Underwriters' Laboratories, Inc. forward a copy of the U.L. report directly to the Contracting Officer, upon the latter's request.

B. Laboratory report from a nationally recognized independent laboratory. If an independent laboratory is used, it must be adequately equipped and competent to determine compliance with U.L. standards. The Government reserves the right to require a facilities report and to conduct a facilities survey. Any laboratory report submitted shall include actual test methods, data taken, and results of tests. Detailed findings of examinations necessary to determine compliance shall also be included. The test report shall also have a section that describes the test sample in such a way that the report can be used to insure identity of production items with the test sample. This section shall be supplemented with construction information such as materials used, spacings between electrical components, types of bushings, photographs, wiring diagrams, sketches, and parts list, all appropriately identified. Compliance with this paragraph does not excuse compliance with all other requirements of the contract and specifications.

3.2 Material. Materials shall conform to the applicable specifications and requirements specified herein. Materials not specifically designated shall be of high commercial quality throughout, and shall be entirely suitable for the purpose intended.

3.3 Design and construction. The vibrator shall be an electrically operated unit suitable for use in dental prosthetic laboratories for packing gypsum materials. The vibrator shall consist essentially of a table top with rubber deck, two leaf springs, base assembly cover with controls assembly, and a magnet assembly consisting of an armature, core and coil. The table top and armature shall be bolted to the leaf springs which in turn shall be bolted to the base assembly. When the coil is energized, the armature and table top shall be pulled down sharply deflecting the leaf springs. When the coil is de-energized, the springs, armature and table top shall be returned for the next cycle. This cycle shall be repeated 3600 times per minute thus providing vibration to the table top. The cover and control assembly shall consist of a line switch, rheostat and rectifier with their necessary electrical connections. The vibrator shall be capable of continuously vibrating a 10 pound load on the table. The displacement of the table shall be continuously variable from 0.010 to 0.060 $\pm$ 0.010 inch

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:29Z
Check the source to verify that this is the current version before use.

by the use of the rheostat when tested as specified in 4.5.1. The vibrator shall operate on 115 volts, 60 Hertz with a power consumption of 20 to 40 watts. The outline and dimensions shall be in accordance with figure 1. The constructon shall be in accordance with figure 2. The vibrator shall consist of high quality components rated for continuous duty at maximum output of vibrator. The vibrator shall be equipped with four rubber isolators to prevent transfer of vibration to supporting surface.

3.3.1 Base. The base shall be fabricated of gray cast iron having machined surfaces which provide parallel seating of the leaf springs. The base shall have adequate cross sectional area to prevent deformation and cracking due to the vibratory forces. The base shall be of sufficient weight to prevent slipping and creeping during operation. The rubber isolators shall be secured to the base.

3.3.1.1 Base cover. The base cover shall be fabricated of aluminum alloy having a thickness of 0.051 to 0.063 inch.

3.3.2 Top cover. The top cover shall be fabricated of aluminum alloy having a thickness of 0.051 to 0.063 inch.

3.3.2.1 Deck. The deck shall be fabricated of chloroprene rubber having a hardness (durometer) of 60 to 65 when tested as specified in 4.5.2. The deck shall have four ribs, on top surface, 1/4 ± 1/16 inch high. The ribs shall be molded as an integral part of the deck along each side and ends to hold the work on the deck. The ribs shall be separated at the corners to permit spillage to be easily removed from deck surface.

3.3.3 Springs. The springs shall be 9-ply fiberglass reinforced epoxy laminate having a flexure strength (modulus of rupture) of 90,000 pounds per square inch (psi) when tested as specified in 4.5.3. The springs shall have a modulus of elasticity of 3×10^6 psi when tested as specified in 4.5.4. The spring shall measure 3 ± 1/16 inches wide, 7 3/4 ± 1/8 inches long, and 1/8 ± 1/64 inch thick.

3.3.4 Electrical components. The control components shall consist of a power switch, a rectifier, a wirewound rheostat, and an electro-magnetic coil. The circuit wiring shall be a minimum 18 AWG, type TEW C.S.A., 105° C appliance wire, UL type 1015, thermoplastic cover, 600 volts. All wire ends shall be terminated in crimp type, eyelet terminal connectors.

3.3.4.1 Power switch. The power switch shall be a double pole, single throw, snap-action switch, rated at 15 amperes, 125 volts, AC. Provisions shall be provided to indicate the position, "ON" or "OFF", of the switch.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:29Z
Check the source to verify that this is the current version before use.

3.3.4.2 Rheostat. The rheostat shall be wire wound, continuous duty, rated 50 watts (minimum) at 115 volts, 60 Hz. The rheostat shall be equipped with screw type terminals with brass screws and nuts. The rheostat shall be equipped with a pointer type knob and an indicator bezel evenly divided from "1" to "10" to indicate the amplitude setting.

3.3.4.3 Coil. The coil shall be wound with a film covered bondable type magnet wire. The finished coil shall be potted in epoxy. The coil shall be provided with two flexible, stranded, single conductor leads with thermoplastic insulation. The encapsulated coil shall be entirely protected from moisture. The completed coil shall have a resistance of 12 ohms and designed to operate on 115 volts, 60 Hz current.

3.3.4.4 Rectifier. The rectifier shall be a silicon diode rectifier having a peak inverse voltage of 400 volts and a continuous current rating of 3 amperes. The rectifier shall be suitable for half wave rectification of 115 volts, 60 Hz current (see 6.4).

3.3.5 Air gap. The vibrator shall be equipped with a device for adjusting the air gap between the two poles (the armature and the core). The adjusting device shall be accessible from the outside of the case and shall be equipped with a locking screw for securing the proper setting. The pole faces shall not strike when tested as specified in 4.5.5.

3.3.6 Power cord. The power cord shall be a 3-conductor, Underwriters' Laboratories type SJO having a minimum gage of 18 AWG. The power cable shall be equipped with a 125 volt, 15 ampere, 2-pole, 3-wire grounding type plug in accordance with American National Standards Institute (ANSI) Standard C73.11. The power cord shall have a minimum length of 6 feet. A strain relief shall be provided where the power cord enters the base. The terminal connections inside the housing shall show no evidence of strain when tested as specified in 4.5.6.

3.3.7 Weight. The weight of the vibrator assembly shall be 21 $\pm$ 2 pounds.

3.4 Finish. The cast base, base cover and top cover shall be painted with a suitable and durable epoxy gray enamel. The magnet core, magnet armature, and spring clamping bars shall be treated with a black oxide finish. All hardware shall be suitably plated to resist corrosion.

3.5 Operational test. The vibrator shall operate without failure or overheating when tested as specified in 4.5.7.

3.6 Dielectric withstand. The vibrator shall be capable of withstanding, without breakdown, a potential of 1240 volts, 60 Hertz when tested as specified in 4.5.8.

Source: https://assist.dla.mil -- Downloaded: 20261O-21T08:29Z
Check the source to verify that this is the current version before use.

3.7 Excessive current. The vibrator shall not draw more than 1.0 ampere, and shall have a table displacement of 0.035 to 0.040 inch when tested under the load and rheostat setting specified in 4.5.9.

3.8 Identification marking. Each vibrator shall be permanently and legibly marked with the name or registered trademark of the manufacturer, model designation, serial numbers, and electrical characteristics, such as voltage, frequency and amperage.

3.9 Service data. The contractor shall furnish, with each unit, two copies each of a technical manual which contains complete instructions for installation, operation, and maintenance and lists of component parts. The manual shall comply with the requirements of MIL-M-7298. As soon as practicable after award of the contract or purchase order, the contractor shall furnish to the Contracting Officer two preliminary copies of his proposed technical manual for review and comment by the Directorate of Medical Materiel, Defense Personnel Support Center. The preliminary manuals shall be submitted sufficiently early to permit adequate review by the Directorate of Medical Materiel, Defense Personnel Support Center (based on a maximum period of 30 days for such review) and to allow incorporation by the contractor of any required revisions and corrections in the final manual without delaying delivery under the contract, or purchase order. In addition, the Contractor shall furnish 15 copies of the approved technical manual to the Contracting Officer for distribution. Should the supplier have furnished acceptable manuals for the identical item within two years preceding the date of the contract and propose to furnish manuals identical with those previously accepted, then the requirements for review of drafts and submission of 15 additional copies may be waived upon request to the Contracting Officer. Waiver of submission of drafts and submission of 15 additional copies shall be at the option of the Government.

3.10 Workmanship. Workmanship shall be first class throughout. Vibrators shall be free from defects which detract from their appearance or impair their serviceability.

4. QUALITY ASSURANCE PROVISIONS

4.1 Responsibility for inspection. Unless otherwise specified in the contract, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract, the contractor may use his own or any other facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Source: https://assist.dla.mil -- Downloaded: 202610-21T08:29Z
Check the source to verify that this is the currentversion before use.

4.1.1 Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government, upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

4.1.2 Inspection. Inspection, as used in this specification, is defined as both examination (such as visual and auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

4.1.3 Certificates of quality. Certificates of quality, supplied by the manufacturer of the materials may be furnished in lieu of actual performance of such testing by the contractor, provided lot identity has been maintained and can be demonstrated to the Government. The certificate shall include the name of the contractor, the contract number, the name of the manufacturer or supplier, the NSN, the Item Identification, the name of the component/material, the lot number, the lot size, the sample size, the date of testing, the test method, individual test results, and the specification requirements.

4.2 Sampling.

4.2.1 For examination. Sampling for examination shall be conducted in accordance with MIL-STD-105, and as indicated in table I. The unit of product for examination purposes shall be one vibrator.

TABLE I. Sampling for examination.

Type defect	Inspection level	AQL (percent defective)
Major	S-2	1.0
Minor	S-2	2.5

4.2.2 For tests. Sampling for tests shall be conducted in accordance with MIL-STD-105, and as indicated in table II, except that the acceptance number shall be zero for all sample sizes. Where feasible, the same sample unit shall be used for the determination of two or more test characteristics. The unit of product for test purposes shall be one vibrator.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:29Z
Check the source to verify that this is the current version before use.

TABLE II. Sampling for tests.

Characteristic	Requirement	Test procedure	Inspection level
Displacement of table	3.3	4.5.1	100%
Hardness of deck	3.3.2.1	4.5.2	S-2
Flexure strength	3.3.3	4.5.3	1/
Modulus of elasticity	3.3.3	4.5.4	1/
Air gap-pole faces	3.3.5	4.4.5	S-2
Power cord strain	3.3.6	4.5.6	S-2
Operational test	3.5	4.5.7	S-1
Dielectric withstand	3.6	4.5.8	100%
Excessive current	3.7	4.5.9	100%

1/ In accordance with ASTM-D790.

4.3 Examination.

4.3.1 Vibrator. The vibrator shall be examined to determine compliance with all requirements specified herein. Examination shall be conducted as specified in tables I and III. Examination, however, shall not be restricted to defects listed in table III.

TABLE III. Classification of defects.

Classification	Defect
Major:	
101	Housing not free of cracks.
102	Base not free of cracks.
103	Power switch inoperative.
104	Amplitude control inoperative.
105	Metal parts not free of corrosion.
Minor:	
201	Service data missing, incomplete, incorrect or illegible.
202	Markings not complete, correct, legible or permanent.
203	Housing not free of scratches or other surface imperfections.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:29Z
Check the source to verify that this is the current version before use.

4.3.2 Dimensional examination. The vibrator shall be examined for defects in dimensions. Any dimensions not within the tolerances specified herein shall be classified as a defect.

4.4 Packaging inspection. The inspection of the preservation-packaging shall be in accordance with the group A and B quality conformance inspection requirements of MIL-P-116. The inspection of the packing and marking for shipment and storage shall be in accordance with the quality assurance provisions of the applicable container specification and the marking requirements of MIL-STD-129.

4.5 Tests. Tests shall be conducted to determine compliance with specification requirements.

4.5.1 Displacement of table. A displacement sticker conforming to figure 3 shall be applied at the center of a long side of the chloroprene deck. The sticker shall be positioned so that a bisector of the "V" shall be parallel to the horizontal surface of the deck. A box, capable of fitting within the ribs of the deck, shall be filled with 5 pounds of sand and placed centrally on the deck. The rheostat shall be placed on the lowest and highest indicating positions. The displacement shall be read at the apex of the "V" when set at these positions. The vibrator shall meet the requirements specified in 3.3.

4.5.2 Hardness of deck. The hardness (durometer) of the deck shall be determined in accordance with ASTM-D2240 using Shore A durometer.

4.5.3 Flexure strength. The flexure strength of the spring material shall be determined in accordance with ASTM-D790.

4.5.4 Modulus of elasticity. The modulus of elasticity of the spring material shall be determined in accordance with ASTM-D790.

4.5.5 Air gap. A 10 pound load shall be centrally positioned on the deck within the deck ribs, and the vibrator operated for 10 minutes with the rheostat setting at maximum.

4.5.6 Power cord strain. Power cord strain shall be tested in accordance with UL1262.

4.5.7 Operational test. A 5 pound load shall be centrally positioned on the deck within the deck ribs and the vibrator operated at 25 percent over the rated voltage at 3/4 rheostat setting for a period of 72 hours.

4.5.8 Dielectric withstand. A slowly rising potential, from 0 to 1240 volts, 60 Hertz, shall be applied between live and dead metal parts. This potential shall be maintained at maximum for one minute. There shall be no evidence of breakdown.

Source: https://assist.dla.mil -- Downloaded: 202610-21T08:29Z
Check the source to verify that this is the currentversion before use.

4.5.9 Excessive current. A 10 pound load shall be centrally positioned on the deck within the deck ribs. The vibrator shall be connected to a 115 volt, 60 Hertz source. The power switch shall be turned on and the rheostat shall be set at maximum. The vibrator shall meet the requirements specified in 3.7. The displacement of the table shall be determined as specified in 4.5.1.

5. PACKAGING

5.1 Preservation-packaging. Preservation-packaging shall be level A or C, as specified (see 6.2).

5.1.1 Level A.

5.1.1.1 Cleaning, drying and preservative. Each vibrator shall be thoroughly cleaned and dried in accordance with the applicable method as outlined in MIL-P-116. Preservative shall not be applied.

5.1.1.2 Unit packaging. Each vibrator shall be wrapped in neutral tissue or other suitable anticorrosive material. Each vibrator shall be further packaged in accordance with MIL-P-116, method 1C-2.

5.1.2 Level C. Vibrators shall be clean and individually packaged in a manner that will afford adequate protection against corrosion, deterioration and physical damage during shipment from supply source to the first receving activity.

5.2 Packing. Packing shall be level A, B or C as specified (see 6.2).

5.2.1 Level A. Two (2) vibrators shall be packed in an exterior container designed for a type 2 load and constructed in accordance with PPP-B-585, class 3, style 3; PPP-B-601, overseas type; PPP-B-621, class 2 or PPP-B-636, class weather-resistant. Closure and strapping shall be as specified in the appendix of the applicable box specification.

5.2.2 Level B. Two (2) vibrators shall be packed in an exterior container designed for a type 2 load and constructed in accordance with PPP-B-585, class 1, style 3; PPP-B-601, domestic type; PPP-B-621, class 1; or PPP-B-636, class domestic. Closure shall be as specified in the appendix of the box specification.

5.2.3 Level C. The packaged vibrators shall be packed in shipping containers in a manner that will afford adequate protection against damage during direct shipment from the supply source to the first receiving activity. These packs shall conform to the applicable carrier rules and regulations.

5.3 Marking. Each unit and exterior container shall be marked as specified in MIL-STD-129.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:29Z
Check the source to verify that this is the current version before use.

6. NOTES

6.1 Intended use. The vibrator covered by this specification is intended to be used for packing gypsum materials in military dental prosthetic laboratories.

6.2 Ordering data. Purchasers should select the preferred options permitted herein and include the following information in procurement documents.

a. Title, number, and date of this specification.
b. National stock number (NSN).
c. Applicable levels of packaging and packing, (see 5.1 and 5.2).

6.3 This specification covers the following item appearing in the Federal Supply Catalog:

National Stock Number	Item Identification
6520-00-962-2106	VIBRATOR, DENTAL, MOLDING, 115 volt, 60 Hertz

6.4 A suitable rectifier would be JEDEC No. 1N3965 or JEDEC No. 1N2244.

Custodians:
Army - MD
Navy - MS
Air Force - 03

Review activity:
DoD - MB

Preparing activity:
DLA-DM

Project No. 6520-1443

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:29Z
Check the source to verify that this is the current version before use.


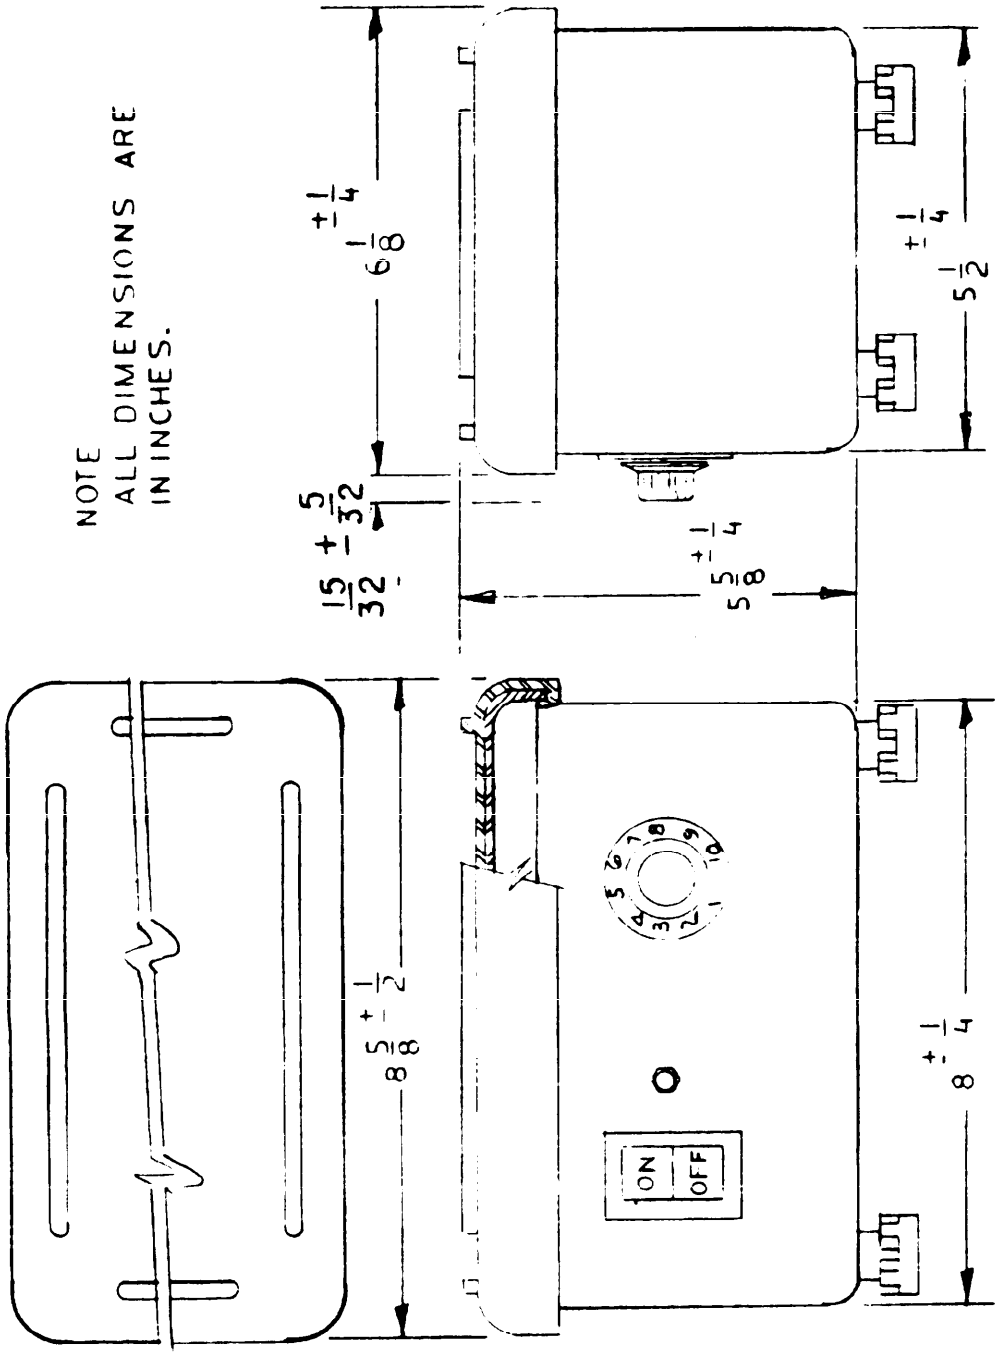


FIGURE 1. Outline and overall dimensions.

Source: https://assist.dla.mil -- Downloaded: 202610-21T08:29Z
Check the source to verify that this is the current version before use.

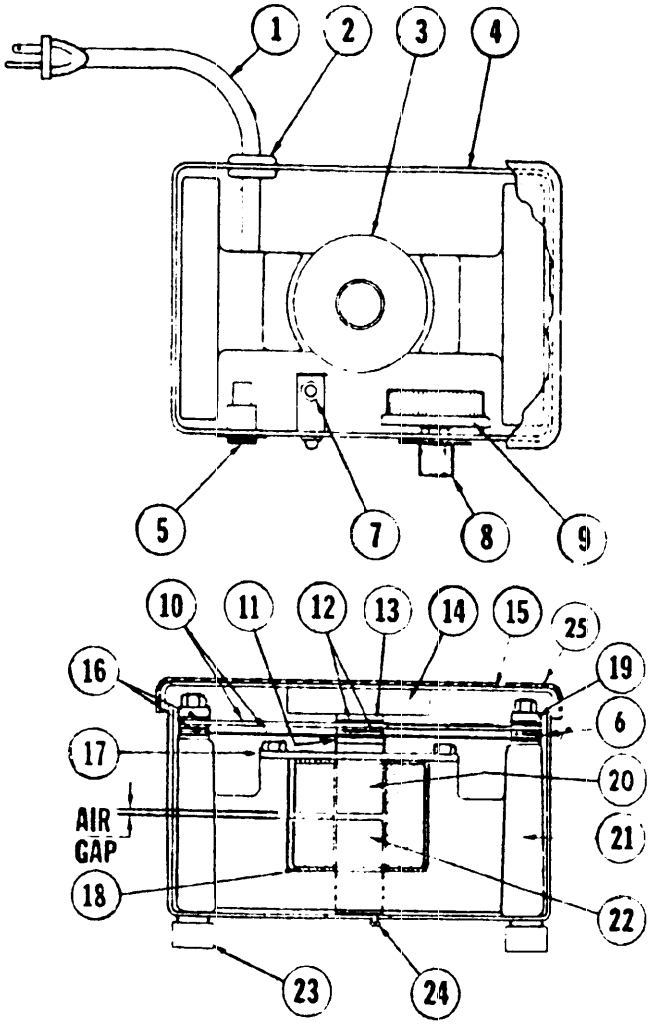

Item No.	Nomenclature
1.	Cable
2.	Strain Relief
3.	Coil Assembly
4.	Base Cover
5.	Switch
6.	Spacer
7.	Rectifier
8.	Knob
9.	Rheostat
10.	Leaf Spring
11.	Mounting Bar-Armature
12.	Spacers
13.	Spacer
14.	Cover Support
15.	Top Cover
16.	Spacers
17.	Coil Clamp
18	Coil Washers
19.	Spring Clamps
20.	Armature
21.	Base
22.	Core
23.	Rubber Feet
24.	Core Locking Screw
25.	Rubber Deck

FIGURE 2. Vibrator, dental molding.

Source: https://assist.dla.mil -- Downloaded: 2026/10-21T08:29Z
Check the source to verify that this is the current version before use.




FIGURE 3. Displacement sticker.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:29Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

OMB Approval
No. 22-R255

INSTRUCTIONS: The purpose of this form is to solicit beneficial comments which will help achieve procurement of suitable products at reasonable cost and minimum delay, or will otherwise enhance use of the document. DoD contractors, government activities, or manufacturers/vendors who are prospective suppliers of the product are invited to submit comments to the government. Fold on lines on reverse side, staple in corner, and send to preparing activity. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements. Attach any pertinent data which may be of use in improving this document. If there are additional papers, attach to form and place both in an envelope addressed to preparing activity.

DOCUMENT IDENTIFIER AND TITLE
MIL-V-36372B VIBRATOR, DENTAL MOLDING, 115 VOLT, 60 HERTZ

NAME OF ORGANIZATION AND ADDRESS	CONTRACT NUMBER
	MATERIAL PROCURED UNDER A ☐ DIRECT GOVERNMENT CONTRACT ☐ SUBCONTRACT

1. HAS ANY PART OF THE DOCUMENT CREATED PROBLEMS OR REQUIRED INTERPRETATION IN PROCUREMENT USE?
   A. GIVE PARAGRAPH NUMBER AND WORDING.

   B. RECOMMENDATIONS FOR CORRECTING THE DEFICIENCIES

2. COMMENTS ON ANY DOCUMENT REQUIREMENT CONSIDERED TOO RIGID

3. IS THE DOCUMENT RESTRICTIVE?
   ☐ YES ☐ NO *(If "Yes", in what way?)*

4. REMARKS

SUBMITTED BY *(Printed or typed name and address - Optional)*	TELEPHONE NO.
	DATE

DD FORM 1 JAN 72 1426 REPLACES EDITION OF 1 JAN 68 WHICH MAY BE USED

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:29Z
Check the source to verify that this is the current version before use.

FOLD

DEFENSE PERSONNEL SUPPORT CENTER
2800 SOUTH 20TH STREET
PHILADELPHIA, PA. 19101

POSTAGE AND FEES PAID
DEFENSE SUPPLY AGENCY
DoD - 304



OFFICIAL BUSINESS
PENALTY FOR PRIVATE USE $300

HEADQUARTERS, DEFENSE PERSONNEL SUPPORT CENTER
ATTN: DIRECTORATE OF MEDICAL MATERIEL, CODE ATT
2800 SOUTH 20TH STREET
PHILADELPHIA, PA. 19101

FOLD

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:29Z
Check the source to verify that this is the current version before use.