FED. SUP CLASS
6640



MS36199-1

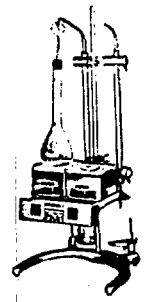

MS36199-2

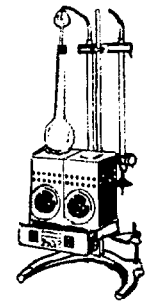

MS36199-1

PART NUMBER	W IN. (mm)	D IN. (mm)	H IN. (mm)	HEAT CONTROL TYPE
MS36199-1	12 (305)	14 (356)	36 (914)	Single Heat
MS36199-2	12 (305)	14 (356)	36 (914)	Rheostat
MS36199-3	12 (305)	14 (356)	36 (914)	Autotransformer

MATERIAL: Frame, cast aluminum and formed steel; base, case iron; support rod, nickel plated steel; manifold, tubular copper; condenser, pure block tin; cooling tank, stainless steel; flask support, cast aluminum. Refractories shall be porcelain or other suitable material.

DESIGN: The apparatus shall accommodate two flasks, 500 and 800 ml capacity. The electrical heaters shall be nichrome wound type with 3-prong line cords. Part numbers -1 and -2 are 120V, AC/DC, 1.1 KW and Part number -3 is 120V, 50/60 Hz, 1.5 KW. The heater controls shall be as follows:

-1 Fixed, 550 watts
-2 Adjustable, 110 to 550 watts
-3 Adjustable, 0 to 750 watts

FINISH: All metal parts shall have a baked enamel finish.

NOTES:
1. Furnish complete except glassware.
2. Items that vary in design but which otherwise conform to the requirements herein are considered one interchangeable Military Standard item.

USER ACTIVITIES:

REVIEWER ACTIVITIES: Army, MD
Navy, AS, OS, YD

APPROVED 7 FEB 80 REVISED

This military standard is approved for use by all Departments and Agencies of the Department of Defense. Selection for all new engineering and design applications and for repetitive use shall be made from this document.

P.A.	INTERNATIONAL INTEREST	TITLE	MILITARY STANDARD
EA		DISTILLING APPARATUS, LABORATORY KJELDAHL, NITROGEN DETERMINATION twin-unit, electric	MS36199
Other Cust MS 99			
Procurement Specifications GG-D-465A	SUPERSEDES:		SHEET 1 OF 1

DD FORM 1 MAY 73 672 (COORDINATED) PREVIOUS EDITIONS OF THIS FORM ARE OBSOLETE

Project Number 6640-0780
DATE

☆U.S. GOVERNMENT PRINTING OFFICE: 1980—603-121/1044

Source: https://assist.dla.mil -- Downloaded: 2026-10-23T17:36Z
Check the source to verify that this is the current version before use.