MILITARY SPECIFICATION

CEMENT, ZINC OXIDE AND POLYACRYLIC ACID, DENTAL

This specification is mandatory for use by all Departments and Agencies of the Department of Defense.

1. SCOPE

1.1 This specification covers zinc polycarboxylate cement suitable for use as a luting agent for crowns, bridges, inlays, space maintainers, and orthodontic bands.

2. APPLICABLE DOCUMENTS

2.1 Specifications and standards. The following documents of the issue in effect on date of invitation for bids or request for proposal, form a part of the specification to the extent specified herein:

SPECIFICATIONS

Federal

PPP-B-566	Box, Folding, Paperboard.
PPP-B-585	Box, Wood, Wirebound.
PPP-B-601	Box, Wood, Cleated-plywood.
PPP-B-621	Box, Wood, Nailed and Lock-corner.
PPP-B-636	Box, Fiberboard.
PPP-B-676	Box, Setup.
PPP-C-186	Container, Packaging and Packing for Drugs, Chemicals and Pharmaceuticals.

FSC 6520

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:29Z
Check the source to verify that this is the current version before use.

Military

MIL-L-10547	Liners, Case, and Sheet, Overwrap; Water-Vaporproof Or Waterproof, Flexible.

STANDARDS

Military

MIL-STD-105	Sampling Procedures and Tables for Inspection by Attributes.
MIL-STD-129	Marking for Shipment and Storage.

(Copies of specifications and standards required by suppliers in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.)

2.2 Other publication. The following documents form a part of this specification to the extent specified herein. Unless otherwise indicated, the issue in effect on date of invitation for bids or request for proposal shall apply.

THE UNITED STATES PHARMACOPEIAL CONVENTION, INC.

The Pharmacopeia of the United States of America

(Application for copies should be addressed to the Mack Publishing Company, Easton, Pa. 18042).

AMERICAN PHARMACEUTICAL ASSOCIATION

National Formulary

(Application for copies should be addressed to the Mack Publishing Company, Easton, Pa. 18042).

AMERICAN CHEMICAL SOCIETY SPECIFICATIONS

Reagent Chemicals

(Application for copies should be addressed to the American Chemical Society, 1155 16th Street, N. W., Washington, D. C. 20036).

Source: https://assist.dla.mil -- Downloaded: 2026l0-21T09:29Z
Check the source to verify that this is the currentversion before use.

3. REQUIREMENTS

3.1 Material. The zinc polycarboxylate cement shall be composed essentially of a zinc oxide-magnesium oxide powder and polycarboxylate copolymer (consisting of copolymer of acrylic acid and one or more polycarboxylic acids) liquid. The zinc oxide and magnesium oxide shall be in accordance with the tests, standards, and requirements of the Pharmacopeia of the United States of America (U.S.P.), including any supplements or revisions thereto. Any ingredients entering into the cement which are not included in the U.S.P. or National Formulary (N.F.) shall be of high quality throughout and shall be suitable for the purpose intended.

3.2 Description. The zinc polycarboxylate dental cement shall consist of the following:

one 90-gram bottle of powder
one 60-gram dropper bottle of liquid
one powder measuring scoop
one mixing pad
one set of instructions

The zinc polycarboxylate dental cement shall be suitable for use as a luting agent for the final cementation of dental crowns, inlays, bridges, space maintainers, and orthodontic bands.

3.2.1 Powder. The powder shall be homogeneous throughout, free of extraneous material, and shall contain no fillers such as quartz. A minimum of 90 grams shall be supplied in each bottle.

3.2.2 Liquid. The liquid component shall be water-clear, and shall be colorless to pale yellow. The liquid shall be free from deposits or sediment. A minimum of 60 grams shall be supplied in each bottle.

3.3 Physical properties (except adhesion and color). The zinc polycarboxylate cement shall conform to the physical properties listed in table I when tested as specified in 4.4.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:29Z
Check the source to verify that this is the current version before use.

Table I. Physical properties

Working time (minutes)	1 1/2 (minimum)
Setting time at 37° C. (minutes)	5 - 9
Setting time at 25° C. (minutes)	8 - 15
Film thickness (microns)	25 (maximum)
Ultimate compressive strength (pounds per square inch)	8000 - 9600
Diametral tensile strength (pounds per square inch)	550 - 900
Solubility and disintegration (percent)	0.2 maximum
Arsenic content (percent)	0.0002 maximum

3.3.1 Color of set cement. The set cement shall be light beige or buff in color.

3.3.2 Certificates of adhesion. Cement shall adhere to both tooth and button after undergoing the adhesion (button tensile) test as specified in 4.4.2. The contractor shall submit to the procuring activity, a copy of the original certification, that the lots or batches offered to the Government were composed of the same formula and manufactured identically as the production lot or batch originally tested for adhesion.

3.4 Toxicity. The manufacturer shall furnish prior to delivery a statement directly to the Directorate of Medical Materiel (Code ATTS-2), Defense Personnel Support Center, 2800 South 20th Street, Philadelphia, Pa. 19101, that the zinc polycarboxylate, when clinically tested and used according to manufacturer's instructions has no toxic effect on a normal healthy person and produces a lower average pulpal response than zinc phosphate dental cement.

3.5 Instructions. Instructions for use included in the immediate container shall consist of the following as a minimum requirement:

(a) Powder/liquid ratio in terms of number of scoops of powder to number of drops of liquid, and also in terms of grams of powder to grams of liquid. Recommended powder/liquid ratio of 1.5 grams of powder to 1.0 gram of liquid. Ratio for thinner mixes may be included.

(b) Working time relative to powder/liquid ratio(s).

(c) Procedure of mixing including note that metal spatula shall be used.

(d) Mixing time.

(e) Preparation of tooth surface prior to application.

Source: https://assist.dla.mil -- Downloaded: 202610-21T09:29Z
Check the source to verify that this is the current version before use.

3.6 Immediate container. Immediate container of zinc polycarboxylate cement shall consist of a bottle of powder, a bottle of liquid, set of directions, mixing pad and measuring scoop. The zinc polycarboxylate powder and liquid components shall each be furnished in properly sealed polyethylene containers suitable for preserving the physical properties of the components without contaminating the contents. Bottle for powder shall conform to PPP-C-186 with the exception of a polypropylene screw cap closure instead of a phenol resin screw cap. Bottle for liquid shall be an ophthalmic polyethylene squeeze type with drop dispensing plug. Bottle shall have a 1/16-inch diameter orifice sealed by a threaded plastic screw cap and shall conform to PPP-C-186. Immediate container labeling for each component shall include lot or control number. The immediate containers and all components shall be compatible and shall not interact physically or chemically with the powder or liquid.

3.7 Delivery schedule. Not more than 3 months shall have elapsed from the date of manufacture of the pulp protector to the date of delivery to the Government.

3.8 Lot or control number. Each unit package shall bear a lot or control number, consisting of a series of numbers or letters, or both, established by the manufacturer to record production and control of the product.

3.9 Stability. Cement shall conform to the requirements of this specification for no less than two years from date of delivery to the Government when stored in a cool, dry, place (59 degrees Fahrenheit (° F.) to 86° F.).

3.10 Workmanship. Workmanship shall be first class throughout. Zinc polycarboxylate cement shall be free from defects which may detract from its appearance or impair its serviceability.

4. QUALITY ASSURANCE PROVISIONS

4.1 Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the supplier is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or order, the supplier may use his own or any other facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in this specification where such inspections are deemed necessary to assure that supplies and services conform to prescribed requirements.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:29Z
Check the source to verify that this is the current version before use.

4.1.1 Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government, upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of 3 years after delivery of the supplies to which such records relate.

4.1.2 Inspection. Inspection, as used in this specification, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

4.1.3 Certificates of quality. Certificates of quality, supplied by the manufacturer of the packaging and raw materials, may be furnished in lieu of actual performance of such testing by the contractor, provided lot identity has been maintained and can be demonstrated to the Government. The Certificate shall include the name of the contractor, the contract number, the name of the manufacturer or supplier, the FSN, the Item Identification, the name of the material, the lot number, the lot size, the sample size, the date of testing, the test method, individual test results, and the specification requirements.

4.2 Quality conformance inspection. Quality conformance inspection shall consist of all examinations specified in 4.3 and tests specified in 4.4.1 through 4.4.9, and shall apply to those samples selected in accordance with 4.2.1 and 4.2.2.

4.2.1 Sampling for examination. Sampling for examination shall be conducted in accordance with MIL-STD-105. The inspection levels and acceptable quality levels (AQL's) shall be as indicated in table II. Unit of product for examination purposes shall be one package (unit of issue).

Table II. Inspection and acceptable quality levels.

Type defect	Inspection level	AQL (Percent defective)
Major	S-2	2.5
Minor	S-2	4.0

Source: https://assist.dla.mil -- Downloaded: 202610-21T09:29Z
Check the source to verify that this is the current version before use.

4.2.2 Sampling tests. Sampling for tests shall be conducted in accordance with table III. Unit of product for test purposes shall be unit of issue (one package).

Table III. Tests

Characteristic	Requirement	Test procedure	Units of product to be tested per lot or batch number	Number of determinations per unit of product
Working time	3.3	4.4.4	1	2
Setting time (37° C.)	3.3	4.4.6	1	2
Setting time (25° C.)	3.3	4.4.5	1	2
Film thickness	3.3	4.4.7	1	2
Ultimate compressive strength	3.3	4.4.8	1	5
Diametral tensile strength	3.3	4.4.3	1	5
Solubility and disintegration	3.3	4.4.9	1	2
Arsenic content	3.3	4.4.10	1	1

4.3 Examination. Zinc polycarboxylate cement shall be examined for defects, including, but not limited to, those listed in table IV.

Table IV. Classification of defects

Categories	Defects
Major	
101	Minimum weight of powder and liquid not as specified. 1/
102	All components not present in package.
103	Powder not homogeneous or free of extraneous material. 1/
104	Color not as specified.
105	Bottle for powder does not have screwcap closure.
106	Bottle for liquid not squeeze type.
107	Loose caps, broken bottles, leaks, etc. present.
Minor	
201	Lot or control number not present on each immediate container.
202	Instructions missing, incorrect, incomplete, or illegible.
203	Packaging and packing not as specified.
204	Marking not as specified.

1/ In process examination may be employed for this defect.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:29Z
Check the source to verify that this is the current version before use.

4.4 Tests.

4.4.1 Preparation of specimens. Test specimens shall be prepared in the following manner for tests in 4.4.2 through 4.4.10:

Prepare all test specimens at a temperature of 23 ± 2 degrees Centigrade (° C.), (73.4 ± 3.6° F.) and at a relative humidity of between 50 ± 10 percent. Weigh 1.5 grams (gm.) powder and 1.0 gm. liquid on a glass mixing slab approximately 150 millimeters (mm.) by 75 mm. Spread the liquid with a corrosion-resisting steel spatula and draw the powder into the liquid without dividing into portions. Mix for 30 to 35 seconds to a smooth consistency by a combination of circular and linear motion.

4.4.2 Adhesion. An extracted human tooth that has been kept moist until testing and a stainless steel orthodontic lingual button shall be used. The tooth shall be mounted in dental stone with the labial surface positioned on a plane with the top surface of the mounting ring and stone. The test tooth surface shall be prepared by polishing with a pumice-water slurry using a dental handpiece at a slow speed. Specimens shall be rinsed with water followed by a scrubbing with an alcohol-soaked cotton swab. The button shall be cemented onto the tooth (care being taken to achieve a uniform film thickness). The moist specimens shall be stored at 37.0 ± 0.5° C. for 3 hours prior to testing. The button and tooth shall then be separated by using an adhesion test frame apparatus. This apparatus shall consist of keyed aluminum clamps affixed to the top of the crosshead of an Instron in such a manner as to permit easy centering of the test button under the lifting hook suspended from the tensile load cell. The lifting hook shall be connected to the load cell through a short length of flexible steel chain in order to compensate for minor variations in orientation (this provides that the applied force is as nearly pure tensile as possible). The button shall then be lifted off the tooth using the Instron apparatus. Cement should be present on both tooth and button without either being completely clean.

4.4.3 Diametral tensile strength. Prepare specimens as for compressive strength. Measure and record diameter and length of specimen just before testing. Pad each side of the specimen with sheet polyethylene approximately 1 to 2 mils. thick and load at a crosshead speed of 0.02 inch per minute.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:29Z
Check the source to verify that this is the current version before use.

Calculate tensile strength as follows:

$$\text{Tensile Strength} = \frac{2P}{3.14\ DL}$$

Where P is load in pounds at fracture

D is diameter of specimen in inches

L is length of specimen in inches

Report average of 5 specimens to the nearest 100 pounds per square inch (p.s.i.) or 7 kilograms per square centimeter (Kg/cm^2).

4.4.4 Working time. Test for working time shall be performed as follows:

Gather the material on the plate in a small area, touch the material with the tip (1/2 inch) of the spatula blade, raise the blade 1-1/2 to 2 inches above the mixing plate and hold in this position to allow the material to flow downward. Repeat the gathering and test for flow each 30 seconds until the material ceases to flow and starts to become rubbery and stringy. Report the average of two tests to the nearest 30 seconds.

4.4.5 Setting time at 25° C. Test for setting time at 25° C. shall be performed as follows:

Place a brass ring (approx. 10 mm. inside diameter, 13 mm. outside diameter and 5 mm. high) on a glass plate and slightly overfill the ring with the mixed cement. Strike off the excess material flush with the ring top. At six minutes from the start of mixing carefully lower the tip of the standard Gilmore needle vertically to the surface of the cement for a 5-second period (the Gilmore needle weighs 454 gm. and has an end 1.06 mm. in diameter). Repeat at 30 second intervals, and, as the setting time approaches, as indicated by the failure of the needle to make a perceptible circle on the cement, remove the glass and make final judgment of setting time on the cement surface which was in contact with glass. The time from beginning of mix to the time of failure to indent the surface of the cement is recorded as the setting time. Report the average of two tests to the nearest 30 seconds.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:29Z
Check the source to verify that this is the current version before use.

4.4.6 Setting time at 37° C. Test for setting time at 37° C. shall be performed as follows:

Slightly overfill a brass ring resting on a glass plate as for setting time at 25° C. but do not strike off the excess. At 2 minutes from start of mix place ring in humidor at 37.0 ± 0.5° C. Check for setting time with the Gilmore needle at 30 second intervals for 5 second periods. Make initial checks near the outer edge of the specimen, keeping the center for checking when very close to the setting time. Gilmore needle should be held in a straight, vertical position during test. Record setting time to nearest 30 seconds as that time from start of mix when only a slight depression is made by the needle. Report the average of 2 tests to the nearest 30 seconds.

4.4.7 Film thickness. Test for film thickness shall be performed as follows:

Place a portion of mixed cement (about 6 mm. square) between 2 flat, smooth glass plates of uniform thickness and approximately 2 cm. square. One and one-half minutes from start of mix apply a load of 15 Kgs. (33 lbs.) to the glass plates in a plastometer. At 10 minutes from start of mix, remove the load and measure the thickness of the glass sandwich with a toolmaker's micrometer. Measure to the nearest 0.00005 inch. The difference in thickness of the two plates with and without the specimen between them is the film thickness.

Report the average of two tests to the nearest .00005 inch or nearest micron.

4.4.8 Ultimate compressive strength (24 hours). The test for ultimate compressive strength shall be preformed as follows:

The mold used to form the specimens is shown in figure 1. Place a 32 mm. by 32 mm. by 6 mm. lucite block with a centrally located 13-mm. diameter hole on a similar block minus the hole. Lubricate the inner surface of the mold shown in figure 1 with a 3 percent solution of microcrystalline wax in benzene. Fill the lucite cavity with the mixed cement. At one minute from start of mix, press the metal mold into the cement to fill the inside of the mold. A slight back and forth rotation of the mold will aid in filling the mold. Cover the surface of the cement in the mold with a lucite block similar to the one on the bottom and clamp the assembly in a "C" clamp. At 2 minutes from start of mix place the mold in a covered container in the humidor at 37.0 ± 0.5° C. The container atmosphere is at 100 percent relative humidity. Remove the mold from the container at 1 hour from start of mix. Remove "C" clamp and top and bottom plates, leaving the middle block attached to the metal mold as an aid to finishing the ends of the specimen. Place the mold in a beaker of water at 37.0 ± 0.5° C. Sand the ends of the specimen with wet 400A wet-dry paper immersed in water to make the specimen ends parallel. Push the specimen out of the mold with a nylon rod and place it in a covered bottle of distilled water kept in the humidor at 37.0 ± 0.5° C. until 24 hours from start of mix.

Determine compressive strength at 0.02 inch per minute crosshead speed.

Report average of 5 specimens to the nearest 100 psi (or 7 Kg/cm^2).

Source: https://assist.dla.mil -- Downloaded: 202610-21T09:29Z
Check the source to verify that this is the current version before use.

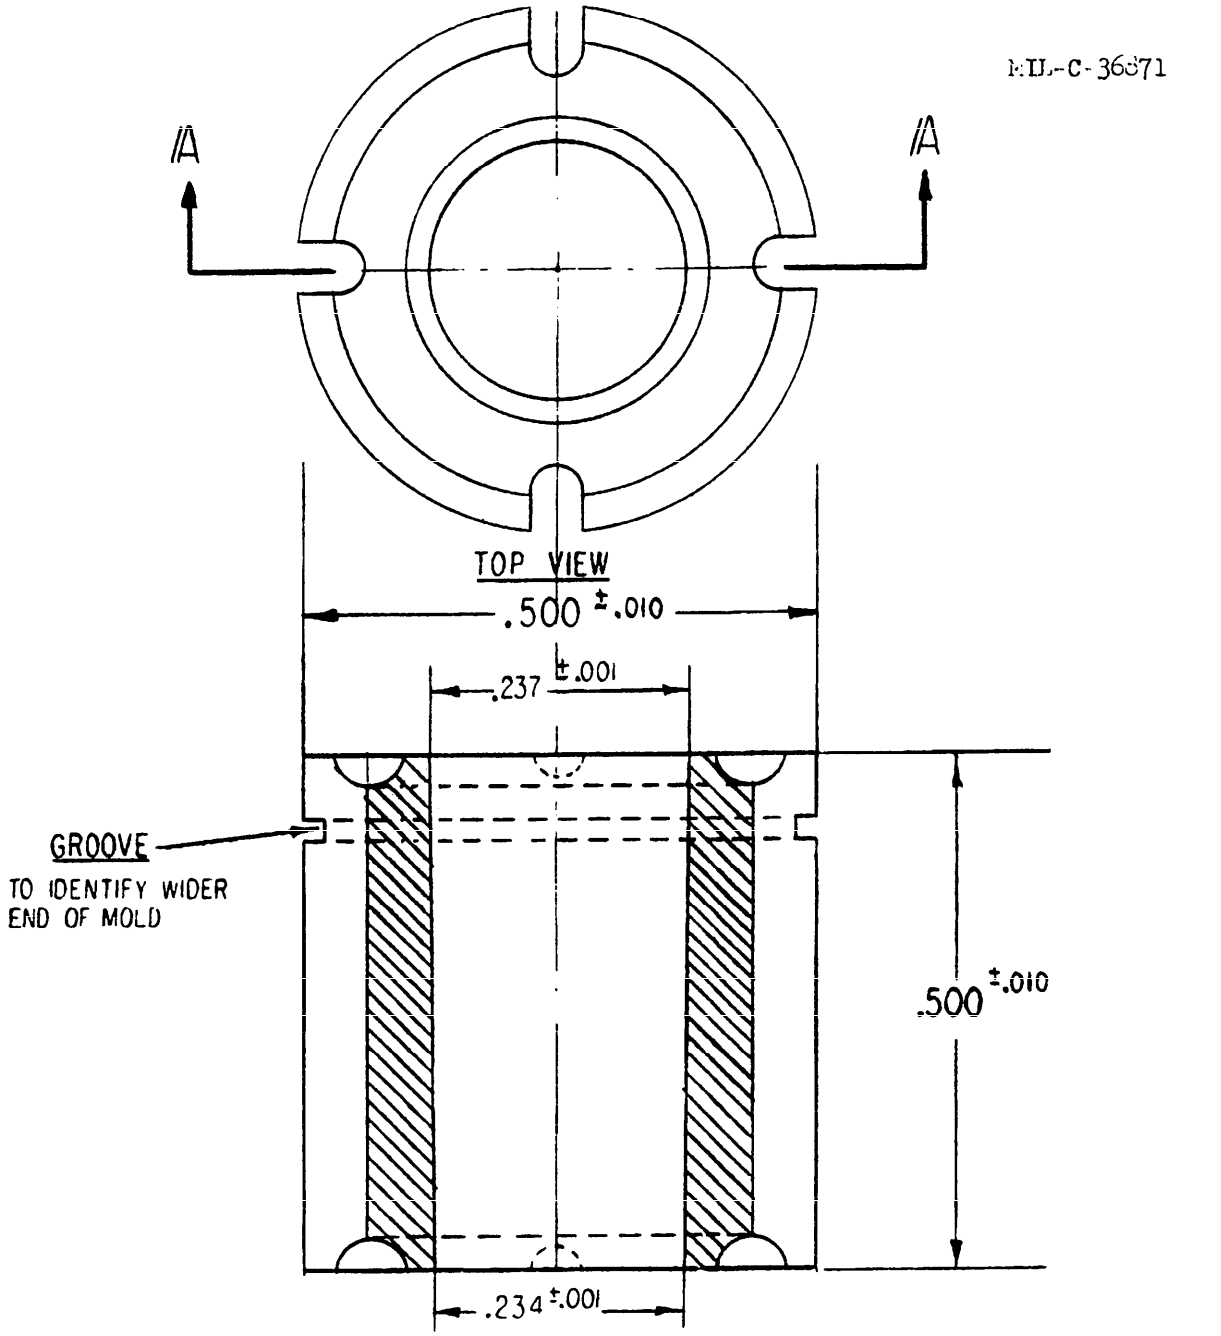


FIGURE 1

MOLD

FOR COMPRESSIVE STRENGTH SPECIMEN

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:29Z
Check the source to verify that this is the current version before use.

4.4.9 Solubility and disintegration. The test for solubility and disintegration shall be performed as follows:

Place a split stainless steel ring (20 mm. inside diameter and 1.5 mm. thick) on a thin sheet of polyethylene on a flat stainless steel plate. Transfer one-half ml. of cement to the ring, insert a piece of fine stainless steel wire into the cement as a holder, and press the cement into the ring with another plate faced with a polyethylene sheet. Two minutes after the mix is started place the assembly into a humidor at 37.0 ± 0.5° C. and 100 percent relative humidity. Prepare 2 specimens.

After 1 hour place the specimens in a tared weighing bottle (see figure 2), which has been heated to constant weight at 150 ± 5° C., with a cover and weigh to the nearest .01 gm. (The tared weighing bottle alone should have been weighed to the nearest 0.2 milligram [mg.]). Immediately after weighing, add 50 milliliters (ml.) distilled water to the bottle, cover and place in an oven or humidor at 37.0 ± 0.5° C. for 23 hours. At the end of this period no crystal growth on the specimen should be present. Evaporate the water from the bottle below 100° C. and finally dry the bottle at 150 ± 5° C. to constant weight, weighing to the nearest 0.2 mg. After heating to 150 ± 5° C. bottles must be cooled to room temperature in a $CaSO_4$ or Silica-gel desiccator for 20-30 mins. before weighing.

The difference between the final and initial weights of the bottle, divided by the weight of the two specimens minus the wires, times 100, gives the percentage of disintegration.

Report the average of two such tests to the nearest 0.1 percent.

4.4.10 Arsenic content. The arsenic content test shall be performed as follows:

Make a standard size mix of cement and press it between 2 glass plates approximately 50 mm. square. Remove from the glass after 15 minutes and store in a dry air-tight container for 24 hours. Grind in a mortar to pass a 200 mesh sieve. Digest one gram of the sample in 100 ml. distilled water on a steam bath for 1 hour. Filter and use the filtrate in the Gutzeit test for arsenic conforming to that designated in Reagent Chemicals, American Chemical Society Specifications.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:29Z
Check the source to verify that this is the current version before use.

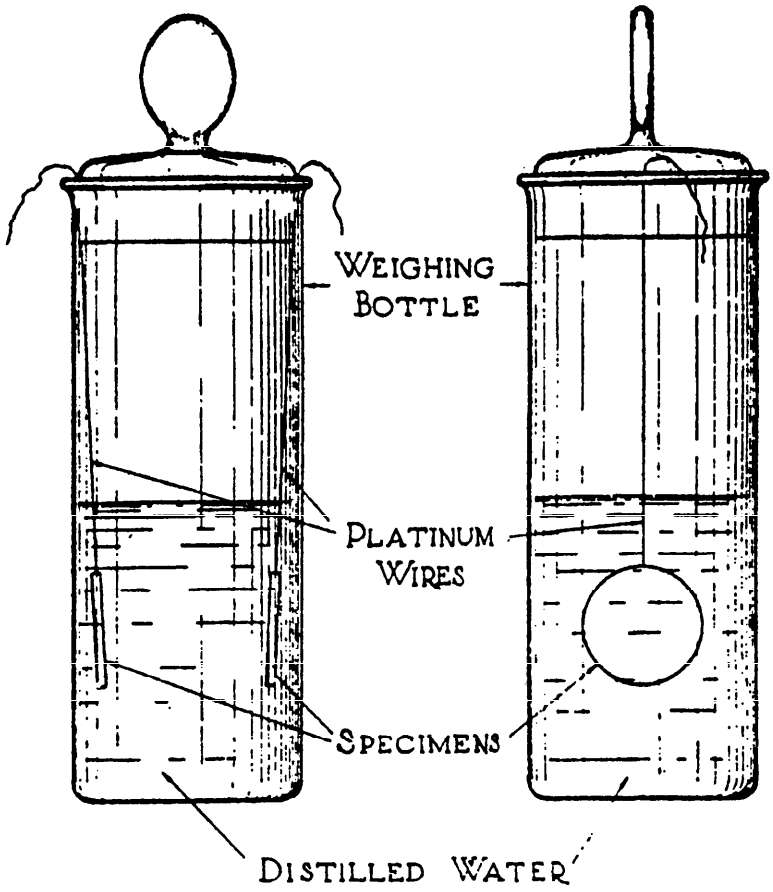


FIGURE 2. *–Weighing bottle containing solubility specimens*

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:29Z
Check the source to verify that this is the current version before use.

5. PREPARATION FOR DELIVERY

5.1 Packaging.

5.1.1 Unit of issue. One package containing one bottle of powder, one bottle of liquid, one scoop, one mixing pad, and one set of instructions, as specified, constitutes one unit of issue.

5.1.2 Packaging quantities. The number of units of issue indicated in table V shall be packaged in each unit, intermediate, and exterior container, as applicable, for the required level of protection specified in the procurement document.

Table V. Packaging Quantities

Unit package	Intermediate package	Exterior container
1 unit	6 units	96 units

5.1.2.1 Packing variation permitted. If the required number of units in the entire shipment is less than the number of units specified to be overpacked in an exterior container, such units may be packed in an exterior container of suitable size and design, acceptable to a common carrier, which shall insure safe delivery to destination.

5.1.3 Level A.

5.1.3.1 Unit package. Unit package shall be a box of appropriate size and design constructed in accordance with PPP-B-566 or PPP-B-676, except commercial colors will be acceptable, or PPP-B-636, type CF, class domestic. Closure shall be adequate to prevent accidental opening under normal handling.

5.1.3.2 Intermediate package. Intermediate package shall be a box of appropriate size and design constructed in accordance with PPP-B-636, type CF, class domestic or PPP-B-676 except that commercial colors are acceptable. Closure shall be adequate to prevent spilling of contents under normal handling.

5.1.4 Level C. Units shall be packaged in standard commercial containers of the size and kind commonly used, which will afford the degree of protection required for shipment and use of the product for its intended purpose.

Source: https://assist.dla.mil -- Downloaded: 202610-21T09:29Z
Check the source to verify that this is the current version before use.

5.2 Packing.

5.2.1 Level A.

5.2.1.1 Exterior container. Exterior container shall be designed for a type 2 load and constructed in accordance with PPP-B-585, class 3, style 3; PPP-B-601, overseas type; PPP-B-621, class 2; or PPP-B-636, class weather-resistant, grade V3c. Fiberboard boxes shall conform to the special requirements specified in PPP-B-636.

5.2.1.2 Case liner. Each level A wood box shall be lined with a waterproof case liner conforming to MIL-L-10547. Closure and sealing shall conform to applicable paragraphs of appendix thereto. Case liner shall not be required for fiberboard boxes.

5.2.1.3 Closure. Closure of wood boxes shall be in accordance with appendix of applicable box specification. Closure of each fiberboard box shall be as specified in the appendix, and waterproofing shall conform with 30.4 of PPP-B-636.

5.2.1.4 Strapping. Strapping, when required, shall be in accordance with appendix of applicable box specification.

NOTE: Strapping shall not be required for shipments forwarded to a receiving activity within the continental limits of the United States for storage and redistribution.

5.2.2 Level B.

5.2.2.1 Exterior container. Exterior container shall be designed for a type 2 load and constructed in accordance with PPP-B-585, class 1, style 3; PPP-B-601, domestic type; PPP-B-621, class 1; or PPP-B-636, class domestic. Closure shall be as specified in the appendix of the applicable box specification. Fiberboard box shall be closed by method II of PPP-B-636. Fiberboard boxes shall conform to special requirements as specified in PPP-B-636.

5.2.3 Level C. The subject commodity shall be packed in substantial commercial containers of the type, size, and kind commonly used for the purpose, so constructed as to insure acceptance and safe delivery by common or other carriers, at the lowest rate, to point of delivery called for in the contract or purchase order.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:29Z
Check the source to verify that this is the current version before use.

5.3 Marking.

5.3.1 Interior packages. Each unit package, and each intermediate package shall be marked in accordance with MIL-STD-129. When labels are utilized, waterproofing shall be required only when applicable carton is fabricated of water-resistant material. Contract or purchase order number and name of contractor shall be shown.

5.3.2 Exterior container. Exterior container shall be marked in accordance with MIL-STD-129.

6. NOTES

6.1 Ordering data. Procurement documents should specify the following:

(a) Title, number, and date of this specification.
(b) Selection of applicable levels of packaging and packing (see 5.1 and 5.2).

6.2 Limitations. This specification does not cover all types, classes, grades, styles, or sizes of the commodity indicated by the title of this specification, or those which are commercially available, but is intended to cover those items which are normally procured to meet Military requirements.

6.3 Federal stock number (FSN) coverage. This specification includes the requirements of FSN 6520-141-0420, CEMENT, ZINC OXIDE AND POLYACRYLIC ACID, DENTAL.

Custodians:
Army - MD
Navy - MS
Air Force - 03

Review activities:
Army - MD
Navy - MS
Air Force - 03

Preparing activity:
Defense Supply Agency - DM

Project No. 6520-1325

Review information is current as of the date of this document. For future coordination of changes to this document, draft circulation should be based on the information in the current DODISS.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:29Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

OMB Approval
No. 22-R255

INSTRUCTIONS: The purpose of this form is to solicit beneficial comments which will help achieve procurement of suitable products at reasonable cost and minimum delay, or will otherwise enhance use of the document. DoD contractors, government activities, or manufacturers/ vendors who are prospective suppliers of the product are invited to submit comments to the government. Fold on lines on reverse side, staple in corner, and send to preparing activity. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements. Attach any pertinent data which may be of use in improving this document. If there are additional papers, attach to form and place both in an envelope addressed to preparing activity.

DOCUMENT IDENTIFIER AND TITLE
MIL-C-36871

NAME OF ORGANIZATION AND ADDRESS

CONTRACT NUMBER

MATERIAL PROCURED UNDER A
☐ DIRECT GOVERNMENT CONTRACT ☐ SUBCONTRACT

1. HAS ANY PART OF THE DOCUMENT CREATED PROBLEMS OR REQUIRED INTERPRETATION IN PROCUREMENT USE?
   A. GIVE PARAGRAPH NUMBER AND WORDING.

   B. RECOMMENDATIONS FOR CORRECTING THE DEFICIENCIES

2. COMMENTS ON ANY DOCUMENT REQUIREMENT CONSIDERED TOO RIGID

3. IS THE DOCUMENT RESTRICTIVE?
   ☐ YES ☐ NO *(If "Yes", in what way?)*

4. REMARKS

SUBMITTED BY *(Printed or typed name and address - Optional)*

TELEPHONE NO.

DATE

DD FORM 1 JAN 72 1426 REPLACES EDITION OF 1 JAN 66 WHICH MAY BE USED

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:29Z
Check the source to verify that this is the current version before use.

FOLD

POSTAGE AND FEES PAID
DEFENSE SUPPLY AGENCY
DOD-304



OFFICIAL BUSINESS
PENALTY FOR PRIVATE USE $300

FOLD

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:29Z
Check the source to verify that this is the current version before use.