MILITARY SPECIFICATION

STRIPPER, BLOOD BAG TUBING,

ROLLER TYPE

This specification is approved for use by all Departments and Agencies of the Department of Defense.

1. SCOPE

1.1 This specification covers a stripping device basically involving two opposing rollers used for "stripping" unanticoagulated blood in the donor tube of a blood bag so that it can be mixed with the anticoagulant solution.

2. APPLICABLE DOCUMENTS

2.1 The following documents of the issue in effect on date of invitation for bids or request for proposals, form a part of this specification to the extent specified herein:

SPECIFICATIONS

Federal

PPP-B-585	Box, Wood, Wirebound.
PPP-B-601	Box, Wood, Cleated-plywood.
PPP-B-621	Box, Wood, Nailed and Lock-corner.
PPP-B-636	Box, Fiberboard.
PPP-B-676	Box, Set-up.

Military

MIL-P-116	Preservation, Methods of.
MIL-L-10547	Liners, Case and Sheet Overwrap; Water-Vaporproof or Waterproof, Flexible.

FSC 6515

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:30Z
Check the source to verify that this is the current version before use.

STANDARDS

Military

MIL-STD-105	Sampling Procedures and Tables for Inspection by Attributes.
MIL-STD-129	Marking for Shipment and Storage.

(Copies of specifications and standards required by suppliers in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.)

2.2 Other publications. The following documents form a part of this specification to the extent specified herein. Unless otherwise indicated the issue in effect on date of invitation for bids or request for proposals shall apply.

AMERICAN SOCIETY FOR TESTING AND MATERIALS (ASTM)

ASTM Standard E 18	Rockwell Hardness and Rockwell Superficial Hardness of Metallic Materials.

(Application for copies should be addressed to American Society for Testing and Materials, 1903 Race Street, Philadelphia, Pa. 19103.)

3. REQUIREMENTS

3.1 Material.

3.1.1 Handle-jaw. The handle-jaw members of the pliers shall be made of martensitic stainless steel or chromium over nickel plated forged steel. The latter shall have a hardness of Rc 38 to 48.

3.1.2 Rollers and roller pins. Shall be made of martensitic stainless steel having a hardness of Rc 32 to 38.

3.1.3 Joint pin. The joint pin (rivet) shall have a hardness of Rc 30 to 40.

3.1.4 Handle insulation. The handles shall be insulated with an encasement of polyvinyl chloride plastisol.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:30Z
Check the source to verify that this is the current version before use.

3.2 Design, style and construction. The stripper shall be similar to that shown in Figure 1. The stripper shall be properly proportioned in all parts so as to be strong, durable, and easy to use. In the fully open position, there shall be a 3/4-inch distance between the rollers. The rollers shall be parallel to each other in the closed position. The rollers shall rotate freely to minimize friction between the blood bag tube and the rollers. The clearance between the rollers in the closed position shall be 0.030 to 0.035 inch and controlled by a set screw.

3.3 Stripping test. The stripper shall be capable of compressing the donor tube of standard blood bags when tested as described in 4.4.3. The stripper shall be suitable for use with standard blood bags Federal Stock Numbers 6515-926-4766, 6515-926-4767, 6515-079-9483, 6515-079-9510, and 6515-079-9530.

3.4 Deflection and set. The deflection under load and permanent set of the handles for the stripper shall not exceed the values shown herein when subjected to the load test specified in 4.4.2:

Deflection under load, maximum	Permanent set maximum
0.95 inch	0.03 inch

3.6 Joint. The stripper shall have either a lap or, as an alternate, a box joint. There shall be no excessive sidewise movement, play or other indication of looseness of the two halves of the stripper when the stripper is open or closed. Opening and closing of the jaws shall easily be accomplished with one hand.

3.7 Marking. The stripper shall be marked in a legible and permanent manner with the manufacturer's name or trademark of such known character that the source of manufacture may be readily determined.

3.8 Workmanship. Workmanship shall be first class throughout. Strippers shall be free from defects which detract from their appearance or may impair their serviceability.

4. QUALITY ASSURANCE PROVISIONS

4.1 Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the supplier is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or order, the supplier may use his own or any other facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:30Z
Check the source to verify that this is the current version before use.

4.1.1 Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government, upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of 3 years after delivery of the supplies to which such records relate.

4.1.2 Inspection. Inspection, as used in this specification, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

4.1.3 Certificates of quality. Certificates of quality, supplied by the manufacturer of the martensitic stainless steel or the chromium over nickel plated forged steel, may be furnished in lieu of actual performance of such testing by the contractor, provided lot identity has been maintained and can be demonstrated to the Government. The certificate shall include the name of the contractor, the contract number, the name of the manufacturer or supplier, the FSN, the item identification, the name of the component/material, the lot number, the lot size, the sample size, the date of testing, the test method, individual test results, and the specification requirements.

4.2 Sampling.

4.2.1 For examination. Sampling for examination shall be conducted in accordance with MIL-STD-105. The inspection levels and acceptable quality levels shall be as indicated in Table I.

Table I. Sampling for Examination

Type of defect	Inspection level	AQL (percent defective)*
Major	S-2	1.0
Minor	S-2	2.5

* If acceptance number is not exceeded, lot shall be accepted. If rejection number is equalled or exceeded, the lot shall be rejected.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:30Z
Check the source to verify that this is the current version before use.

4.2.2 For tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and as indicated in Table II.

Table II. Sampling for Tests

Characteristic	Requirement	Test procedure	Inspection level	AQL (percent defective)
Hardness	3.1.1, 3.1.2, 3.1.3	4.4.1	S-1	1.5
Stripping	3.3	4.4.3	S-1	1.5
Deflection and set	3.4	4.4.2	S-1	1.5

4.3 Examination. The stripper shall be examined to determine compliance with specification requirements. Examination shall be conducted in accordance with Tables I and III. Examination shall include but not be limited to the defects listed in Table III.

Table III. Classification of Defects

Categories	Defects
Major	
101	Rollers do not rotate freely.
102	Clearance between rollers not present with jaws closed.
103	Rollers are not parallel in closed position.
104	Rollers are not smooth and free from burrs.
105	Plating (as applicable) not adherent, smooth, continuous, free from pits, blisters, nodules and other defects affecting protective value.
106	Stripper not in accordance with Figure.
107	Dimensions not as specified for distance between rollers in open position and in closed position (see 3.2).
108	Jaw action not proper (see 3.6).
Minor	
201	Stripper is not free of foreign matter.
202	Marking on stripper not as required (see 3.7).

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:30Z
Check the source to verify that this is the current version before use.

4.4 Tests. Tests shall be conducted to determine compliance with specification requirements.

4.4.1 Hardness. The hardness of all strippers shall be the mean value of three or more determinations taken in an area. ASTM Standard E 18 shall be used. The insulation shall be stripped wherever necessary before making the hardness determinations. If reliable readings cannot be obtained on the finished stripper because of difficulty in supporting the test sample and maintaining the test surface level at the point of indentation, a suitable fixture shall be employed for clamping or properly supporting the sample under test. Hardness determinations for handles shall be taken approximately midway between the rivet and the end of the handles. The hardness of rivets or bolts shall be determined on the assembled tool. All other hardness determinations shall be made on a Rockwell tester, using the Rockwell "C" scale or a suitable equivalent scale on the Rockwell testing machines.

4.4.2 Handle-load tests. The sample stripper under test shall be supported in a manner suitable for applying the load properly and determining the deflection and permanent set of handles. The insulation shall be stripped wherever necessary. A platform scale may be used for making load tests. The opposing surfaces of the jaws shall be in normal horizontal position, with the head resting on a support or guide. The lower handle shall rest on a suitable fixed knife-edge support at the point of maximum handle curvature (the center of handle bow). A 400 inch-pound load shall be applied through a knife edge to the upper handle at the point of maximum handle curvature (the center of handle bow) and in line with the lower handle support. Test loads applied to the handle shall be calculated by dividing the test load specified herein by the distance in inches between the center of the rivet and the line of action of the load. A steel insert 1/8-inch thick is placed between the jaws. It shall have a Rockwell C number of not less than 40. The width of the flat steel insert shall be at least equal to that of the jaws. The method of determining the amount of deflection under load and the permanent set shall be that of marking the extreme ends of the handles with light centerpunch marks and measuring the distance between the marks by means of a divider and scale. After an initial application of a load of approximately 5 pounds, the distance between the punch marks shall be measured with the load still applied. The difference between the initial measurement and the measurement after the test load has been reduced to approximately 5 pounds, shall be the permanent set. If necessary, the extreme ends of the handles may be ground to obtain a surface suitable for making the centerpunch marks. Load and deflection tests may be made on a universal testing machine, a suitably equipped platform scale or a specially calibrated testing device employing dead weights. If the deflection under load or the permanent set is in excess of the maximum value specified herein, or if the handles or jaws break, crack, chip, or spread under load, or if the rivet shows signs of weakness, the sample shall be rejected.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:30Z
Check the source to verify that this is the current version before use.

4.4.3 Stripping. The donor tube of standard blood bags shall be compressed flat by the rollers as the stripper is run along it for a minimum distance of 24 inches. The compressive action shall be observed along the edge of the donor tube as the stripper proceeds along its length.

5. PREPARATION FOR DELIVERY

5.1 Packaging.

5.1.1 Unit of issue. One stripper, as specified, constitutes one unit of issue.

5.1.2 Packaging quantities. The number of units of issue indicated in Table IV shall be packaged in each unit, intermediate, and exterior container, as applicable, for the required level of protection specified in the procurement document.

Table IV. Packaging Quantities

Unit package	Intermediate package	Exterior container
1 unit	12 units	144 units

5.1.2.1 Packing variation permitted. If the required number of units in the entire shipment is less than the number of units specified to be overpacked in an exterior container, such units may be packed in an exterior container of suitable size and design, acceptable to a common carrier, which shall insure safe delivery to destination.

5.1.3 Level A.

5.1.3.1 Cleaning and drying. Each unit shall be thoroughly cleaned and dried in accordance with the applicable method as outlined in MIL-P-116.

5.1.3.2 Preservative. Not required.

5.1.3.3 Intimate wrap. Each unit shall be wrapped in neutral tissue or other suitable anticorrosive material.

5.1.3.4 Unit package. Each unit shall be packaged in accordance with MIL-P-116, method IC-1 or IC-2.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:30Z
Check the source to verify that this is the current version before use.

5.1.3.5 Intermediate package. Intermediate package shall be a box of appropriate size and design constructed in accordance with PPP-B-636, type CF, class domestic or PPP-B-676 except that commercial colors are acceptable. Closure shall be adequate to prevent spilling of contents under normal handling.

5.1.4 Level C. Units shall be packaged in standard commercial containers of the size and kind commonly used, which will afford the degree of protection required for shipment and use of the product for its intended purpose.

5.2 Packing.

5.2.1 Level A.

5.2.1.1 Exterior container. Exterior container shall be designed for a type 2 load and constructed in accordance with PPP-B-585, class 3, style 3; PPP-B-601, overseas type; PPP-B-621, class 2; or PPP-B-636, class weather-resistant. Fiberboard boxes shall conform to the special requirements as specified in PPP-B-636.

5.2.1.2 Case liner. Each level A wood box shall be lined with a waterproof case liner conforming to MIL-L-10547. Closure and sealing shall conform to applicable paragraphs of appendix thereto. Case liner shall not be required for fiberboard boxes.

5.2.1.3 Closure. Closure of wood boxes shall be in accordance with appendix of applicable box specification. Closure of each fiberboard box shall be as specified in the appendix, and waterproofing shall conform with 30.4 of PPP-B-636.

5.2.1.4 Strapping. Strapping, when required, shall be in accordance with appendix of applicable box specification.

NOTE: Strapping shall not be required for shipments forwarded to a receiving activity within the continental limits of the United States for storage and redistribution.

5.2.2 Level B.

5.2.2.1 Exterior container. Exterior container shall be designed for a type 2 load and constructed in accordance with PPP-B-585, class 1, style 3; PPP-B-601, domestic type; PPP-B-621, class 1; or PPP-B-636, class domestic. Closure shall be as specified in the appendix of the applicable box specification. Fiberboard box shall be closed by method II of PPP-B-636. Fiberboard boxes shall conform to special requriements specified in PPP-B-636.

5.2.3 Level C. The subject commodity shall be packed in substantial commercial containers of the type, size, and kind commonly used for the purpose, so constructed as to insure acceptance and safe delivery by common or other carriers, at the lowest rate, to point of delivery called for in the contract or purchase order.

Source: https://assist.dla.mil -- Downloaded: 202610-21T09:30Z
Check the source to verify that this is the currentversion before use.

5.3 Marking.

5.3.1 Interior packages. Each unit package, and each intermediate package shall be marked in accordance with MIL-STD-129. When labels are utilized, waterproofing shall be required only when applicable carton is fabricated of water-resistant material. Contract or purchase order number and name of contractor shall be shown.

5.3.2 Exterior container. Exterior container shall be marked in accordance with MIL-STD-129.

6. NOTES

6.1 Ordering data. Purchasers should exercise any desired options offered herein, and the procurement documents should specify the following:

(a) Title, number, and date of this specification.
(b) Selection of applicable levels of packaging and packing (see 5.1 and 5.2).
(c) Federal stock number.

6.2 This specification is intended to cover the following item appearing in the Federal Supply Catalog:

Federal Stock No.	Item Identification
6515-075-6526	STRIPPER, BLOOD BAG TUBING, Roller Type

It does not include all types or sizes as indicated by the title nor all types which are commercially available.

6.3 Supersession data. This specification includes requirements of Purchase Description No. 1, dated 13 March 1972.

Custodians:
Army - MD
Navy - MS
Air Force - 03


Review activities:
Army - MD
Navy - MS
Air Force - 03

Preparing activity:
Defense Supply Agency - DM

Project No. 6515-1659

Review information is current as of the date of this document. For future coordination of changes to this document, draft circulation should be based on the information in the current DODISS.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:30Z
Check the source to verify that this is the current version before use.

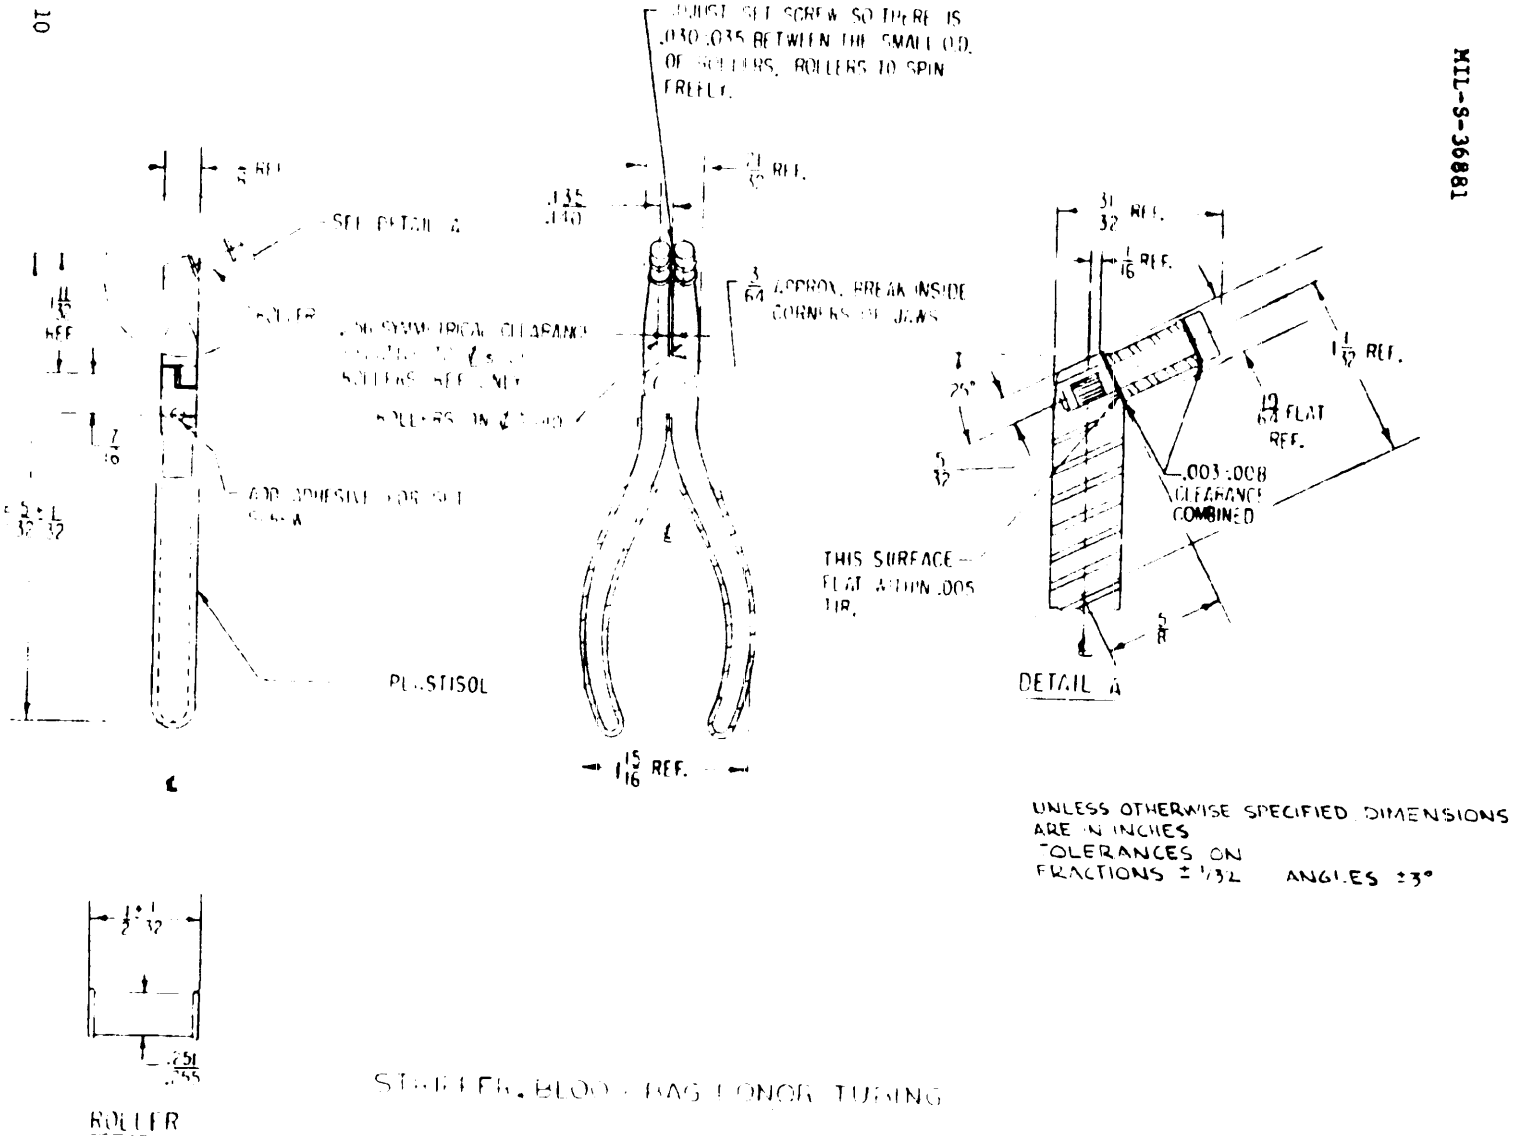

STEERER, BLOOD BAG DONOR TUBING

FIGURE 1

Source: https://assist.dla.mil -- Downloaded: 2026-02-21T09:30Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

OMB Approval
No. 22-R255

INSTRUCTIONS: The purpose of this form is to solicit beneficial comments which will help achieve procurement of suitable products at reasonable cost and minimum delay, or will otherwise enhance use of the document. DoD contractors, government activities, or manufacturers/vendors who are prospective suppliers of the product are invited to submit comments to the government. Fold on lines on reverse side, staple in corner, and send to preparing activity. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements. Attach any pertinent data which may be of use in improving this document. If there are additional papers, attach to form and place both in an envelope addressed to preparing activity.

DOCUMENT IDENTIFIER AND TITLE

MIL-S-36881

NAME OF ORGANIZATION AND ADDRESS

CONTRACT NUMBER

MATERIAL PROCURED UNDER A

☐ DIRECT GOVERNMENT CONTRACT ☐ SUBCONTRACT

1. HAS ANY PART OF THE DOCUMENT CREATED PROBLEMS OR REQUIRED INTERPRETATION IN PROCUREMENT USE?

A. GIVE PARAGRAPH NUMBER AND WORDING.

B. RECOMMENDATIONS FOR CORRECTING THE DEFICIENCIES

2. COMMENTS ON ANY DOCUMENT REQUIREMENT CONSIDERED TOO RIGID

3. IS THE DOCUMENT RESTRICTIVE?

☐ YES ☐ NO *(If "Yes", in what way?)*

4. REMARKS

SUBMITTED BY *(Printed or typed name and address - Optional)*

TELEPHONE NO.

DATE

DD FORM 1 JAN 72 1426

REPLACES EDITION OF 1 JAN 66 WHICH MAY BE USED

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:30Z
Check the source to verify that this is the current version before use.

FOLD

DEFENSE PERSONNEL SUPPORT CENTER
2800 South 20th Street
Philadelphia, Pa. 19101

Defense Supply Agency

OFFICIAL BUSINESS
PENALTY FOR PRIVATE USE $300

POSTAGE AND FEES PAID
DEFENSE SUPPLY AGENCY
DoD - 304

U.S. MAIL

HEADQUARTERS, DEFENSE PERSONNEL SUPPORT CENTER
ATTN: DIRECTORATE OF MEDICAL MATERIEL, CODE ATT
2800 SOUTH 20TH STREET
PHILADELPHIA, PA. 19101

FOLD

Source: https://assist.dla.mil -- Downloaded: 202640-21T09:30Z
Check the source to verify that this is the current version before use.