A-A-53515
2 June 1988

COMMERCIAL ITEM DESCRIPTION

CATHETER KIT, PACING, TRANSVENOUS (Bipolar)

The General Services Administration has authorized the use of this commercial item description.

This commercial item description covers a bipolar transvenous pacing catheter kit suitable for insertion of a catheter into the right ventricle for endocardial pacing.

Salient characteristics:

General. The catheter kit shall consist of a 5 French catheter whose usable length is 90 cm, a percutaneous introducer assembly, a 3 cc disposable syringe, and an ECG adapter. The catheter shall have a single lumen and a balloon with a nominal inflation capacity of 1.3 cc. The balloon shall be located between 2 bipolar electrodes spaced 1 cm apart at the distal tip of the catheter. The catheter shall have a balloon inflation valve at the proximal end. The percutaneous introducer assembly shall be 6 Fr I.D. and contain a needle, guide wire, tapered vessel dilator and insertion sheath. The needle shall be 18 gauge thin-wall, 2-3/4 inches long and the guide wire shall be 40 cm X .035 inches diameter with 3 cm flexible tip. The ECG Adapter shall be compatible on the distal end with .080 inch standard pin electrode connector and on the proximal end to male "V" lead size .125 to .150 inches.

AMSC N/A FSC 6515

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:20Z
Check the source to verify that this is the current version before use.

Style, design and dimensions. The balloon inflation valve shall be Luer lock in accordance with ANSI/HIMA MD70.1. The catheter, vessel dilator, and insertion sheath shall be radiopaque in accordance with ASTM Designation F640. The catheter shall have the following design features:

Effective length	90 to 105 cm
Catheter size	5 Fr, color coded
Diameter of deflated balloon	5 to 6 Fr
Diameter of inflated balloon	8 to 10 mm
Balloon volume	0.75 to 1.30 cc
Electrode material	Stainless steel or platinum
Electrode spacing	1.0 to 2.5 cm
Electrode pin dimensions	0.40 in. x 0.08 in. dia.,
Markings	Every 10 cm
Balloon deflation time	5 seconds, maximum

The shape and style of the catheter shall be in accordance with Figure 1.

Material. The catheter tubing and the hub of the insertion sheath shall be polyvinylchloride (PVC). The vessel dilator and insertion sheath shall be polytetrafluoroethylene (PTFE) or fluorinated ethylene propylene (FEP). The needle and guide wire shall fabricated from an austenitic stainless steel in accordance with ASTM Designation F899. The catheter, vessel dilator, and insertion sheath shall meet the requirements of the USP for Class IV plastics.

Sterility. The catheter kit shall be sterile in accordance with USP or AAMI guidelines.

Toxicity and pyrogenicity. The catheter kit shall be non-toxic and non-pyrogenic in accordance with the USP.

Shelf life. At least 12 months shelf life shall remain at the time of delivery to the Government.

Instructions. The catheter kit shall include detailed instructions for use.

Workmanship. The catheter kit shall be processed in such a manner as to be uniform and free from defects which affect life, utility, or appearance.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:20Z
Check the source to verify that this is the current version before use.

Product Quality Level.

Visual and dimensional examination. Shall be examined to verify that design, construction and workmanship are in accordance with applicable requirements.

Materials. The supplier shall be responsible for performing tests to assure that materials are in accordance with requirements specified.

Unit. Each (EA). One catheter kit, as specified constitutes one unit. The kit shall be packaged sterile in a sealed, peel-open type container capable of maintaining the sterility of the contents unless the package is damaged or opened.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Examination. The catheter kit shall be examined to determine compliance with specification requirements.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more test characteristics.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:20Z
Check the source to verify that this is the current version before use.

Certificate of biocompatibility. A certificate of compliance, stipulating offered items meet the requirements specified herein, shall be acceptable, provided that the contractor has supplied acceptable items to the Government within the past three years, and that there has been no changes to materials, formulation and methods of processing. The certificate shall include the current contract testing, the test method and results, the name and title of the person evaluating test results, and a statement to the effect that material formulation and processing has not changed since the test were p

Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and as specified herein. The unit of product for test purposes shall be one catheter kit. Sampling shall be S-1 and AQL 1.0.

Contractor certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Metric products. Products manufactured to metric dimensions will be considered on an equal basis with those manufactured using inch-pound units, providing they fall within the tolerances specified using conversion tables contained in the latest revision of Federal Standard No. 376, and all other requirements of this document are met.

If a product is manufactured to metric dimensions and those dimensions exceed the tolerances specified in the inch/pound units, a request should be made to the contracting officer to determine if the product is acceptable.

The contracting officer has the option of accepting or rejecting the product.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:20Z
Check the source to verify that this is the current version before use.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Public Law 94-580 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

NOTE: The following National Stock Number is covered by this document:

NSN	ITEM IDENTIFICATION
6515-01-166-9008	CATHETER KIT, PACING, TRANSVENOUS With Bipolar, Swan-Ganz, 5 Fr, 90 cm Catheter

Ordering data (Intermediate/exterior packaging quantities and labeling and marking must be specified in the contract and/or order).

MILITARY INTERESTS:

Custodians:

Army - MD
Navy - MS
Air Force - 03

Preparing Activity:

DoD-MB

Agent:

DLA-DM

CIVIL AGENCY COORDINATING ACTIVITIES:

VA-OSS
PHS
FDA-MPQAS

PGC 50980

Project No. 6515-4250

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:20Z
Check the source to verify that this is the current version before use.

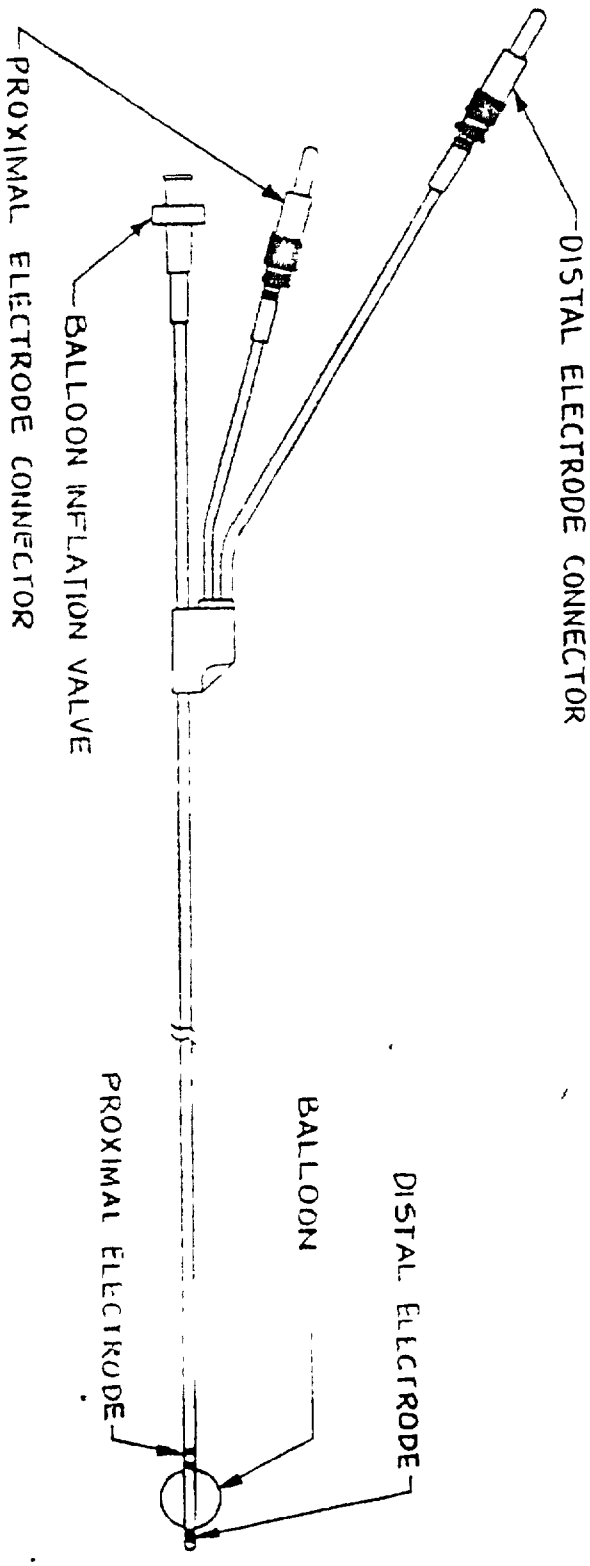


FIGURE 1 CATHETER KIT, PACING TRANSVENOUS

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:20Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

(See Instructions – Reverse Side)

1 DOCUMENT NUMBER	2 DOCUMENT TITLE
A-A-53515	CATHETER KIT, PACING, TRANSVENOUS (Bipolar)

3a NAME OF SUBMITTING ORGANIZATION	4 TYPE OF ORGANIZATION *(Mark one)*
	☐ VENDOR
	☐ USER
b ADDRESS *(Street, City, State, ZIP Code)*	☐ MANUFACTURER
	☐ OTHER *(Specify)*:

5 PROBLEM AREAS

a Paragraph Number and Wording

b Recommended Wording

c Reason/Rationale for Recommendation

6 REMARKS

7a NAME OF SUBMITTER *(Last, First, MI)* – Optional	b WORK TELEPHONE NUMBER *(Include Area Code)* – Optional
c MAILING ADDRESS *(Street, City, State, ZIP Code)* – Optional	8 DATE OF SUBMISSION *(YYMMDD)*

DD FORM 1426 MAR

PREVIOUS EDITION IS OBSOLETE

(TO DETACH THIS FORM, CUT ALONG THIS LINE.)

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:20Z
Check the source to verify that this is the current version before use.

(Fold along this line)

NO POSTAGE NECESSARY IF MAILED IN THE UNITED STATES

OFFICIAL BUSINESS
PENALTY FOR PRIVATE USE $300

BUSINESS REPLY MAIL
FIRST CLASS PERMIT NO 4966 Alexandria, VA

POSTAGE WILL BE PAID BY

Commander
Defense Personnel Support Center
ATTN DPSC-RSTE
2800 South 20th Street
Philadelphia, Pennsylvania 19101-8419

INSTRUCTIONS In a continuing effort to make our standardization documents better, the DoD provides this form for use in submitting comments and suggestions for improvements. All users of military standardization documents are invited to provide suggestions. This form may be detached, folded along the lines indicated, taped along the loose edge (*DO NOT STAPLE*), and mailed. In block 5, be as specific as possible about particular problem areas such as wording which required interpretation, was too rigid, restrictive, loose, ambiguous, or was incompatible, and give proposed wording changes which would alleviate the problems. Enter in block 6 any remarks not related to a specific paragraph of the document. If block 7 is filled out, an acknowledgement will be mailed to you within 30 days to let you know that your comments were received and are being considered.

NOTE. This form may not be used to request copies of documents, nor to request waivers, deviations or clarification of specification requirements on current contracts. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced documents, or to amend contractual requirements.

(Fold along this line)

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:20Z
Check the source to verify that this is the current version before use.