A-A-53519
6 June 1988

COMMERCIAL ITEM DESCRIPTION

HANDLE, BONE CUTTING SAW (Gigli)

The General Services Administration has authorized the use of this Commercial Item Description as a replacement for Military Specification MIL-H-37020, dated 12 December 1973, which is cancelled.

This commercial item description covers a Gigli bone cutting saw handle used with a conductor and wire saw suitable for use in neurosurgery.

Salient characteristics:

General. The handle shall be a Gigli bone cutting saw handle for use with a conductor and wire saw (See Note 2).

Material. The handle shall be fabricated from Class 3 austenitic corrosion-resisting steel, or Class 4 martensitic corrosion-resisting steel in accordance with American Society for Testing and Materials (ASTM) Designation F899.

Hardness. The handle shall have a Rockwell Hardness B Scale (HRB) of 75 to 105. As an alternate, the handle shall have a Rockwell Hardness C Scale (HRC) of 40 to 45. The hardness shall be tested in accordance with ASTM Designations E18 or E92. Conversion of hardness values shall be in accordance with ASTM Designation E140.

Style, design and dimensions. The handle shall be in accordance with Figures 1 or 2 for style, design and dimensions.

Passivation. The handle shall be properly passivated.

Finish. The finish of the handle shall be satin or mirror.

Resistance to corrosion. The handle shall show no signs of corrosion when tested in accordance with ASTM Designation F1089.

AMSC N/A FSC 6515

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:20Z
Check the source to verify that this is the current version before use.

Identification markings. The handle shall bear the contractor's name or registered trademark and the word "stainless". Handles of foreign manufacture shall bear the name of the country of origin.

Workmanship. The handle shall be free from defects which detract from its appearance or impair its serviceability.

Product Quality Level.

Visual and dimensional examination. Shall be examined to verify that design, construction and workmanship are in accordance with applicable requirements.

Materials. The supplier shall be responsible for performing tests to assure that materials are in accordance with requirements specified.

Unit. Each (EA). One handle, as specified, constitutes one unit.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:20Z
Check the source to verify that this is the current version before use.

Sampling for examination. Sampling for examination shall be conducted in accordance with MIL-STD-105, with an AQL of 1.0 (percent defective) and an inspection level of II. The unit of product for sampling purposes shall be one handle.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more test characteristics.

Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105, as specified herein. The unit of product for test purposes shall be one handle. AQL shall be 1.0 (percent defective) with an inspection level of S-2.

Contractor certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Public Law 94-580, as amended, and as implemented by Federal Acquisition Regulation Subpart 23.4 to the maximum extent practical.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:20Z
Check the source to verify that this is the current version before use.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

NOTE 1: The following National Stock Number is covered by this document:

NSN	ITEM IDENTIFICATION
6515-00-363-2400	HANDLE, BONE CUTTING WIRE SAW, Gigli

NOTE 2: The Gigli bone cutting wire saw handle is intended to be used with a Bailey bone cutting wire saw conductor, NSN 6515-00-363-2300, and a 20 inch bone cutting wire saw, NSN 6515-00-363-2700, to form a Gigli bone saw.

Ordering data. (Intermediate/exterior package quantities, labeling, and marking must be specified in the contract and/or order).

MILITARY INTERESTS:

Custodians:

Army - MD
Navy - MS
Air Force - 03

PREPARING ACTIVITY:

DoD - MB

Agent:

DLA-DM


CIVIL AGENCY COORDINATING ACTIVITIES:

VA-OSS
PES
FDA-MPQAS

PGC 45580

Project No. 6515-3946

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:20Z
Check the source to verify that this is the current version before use.

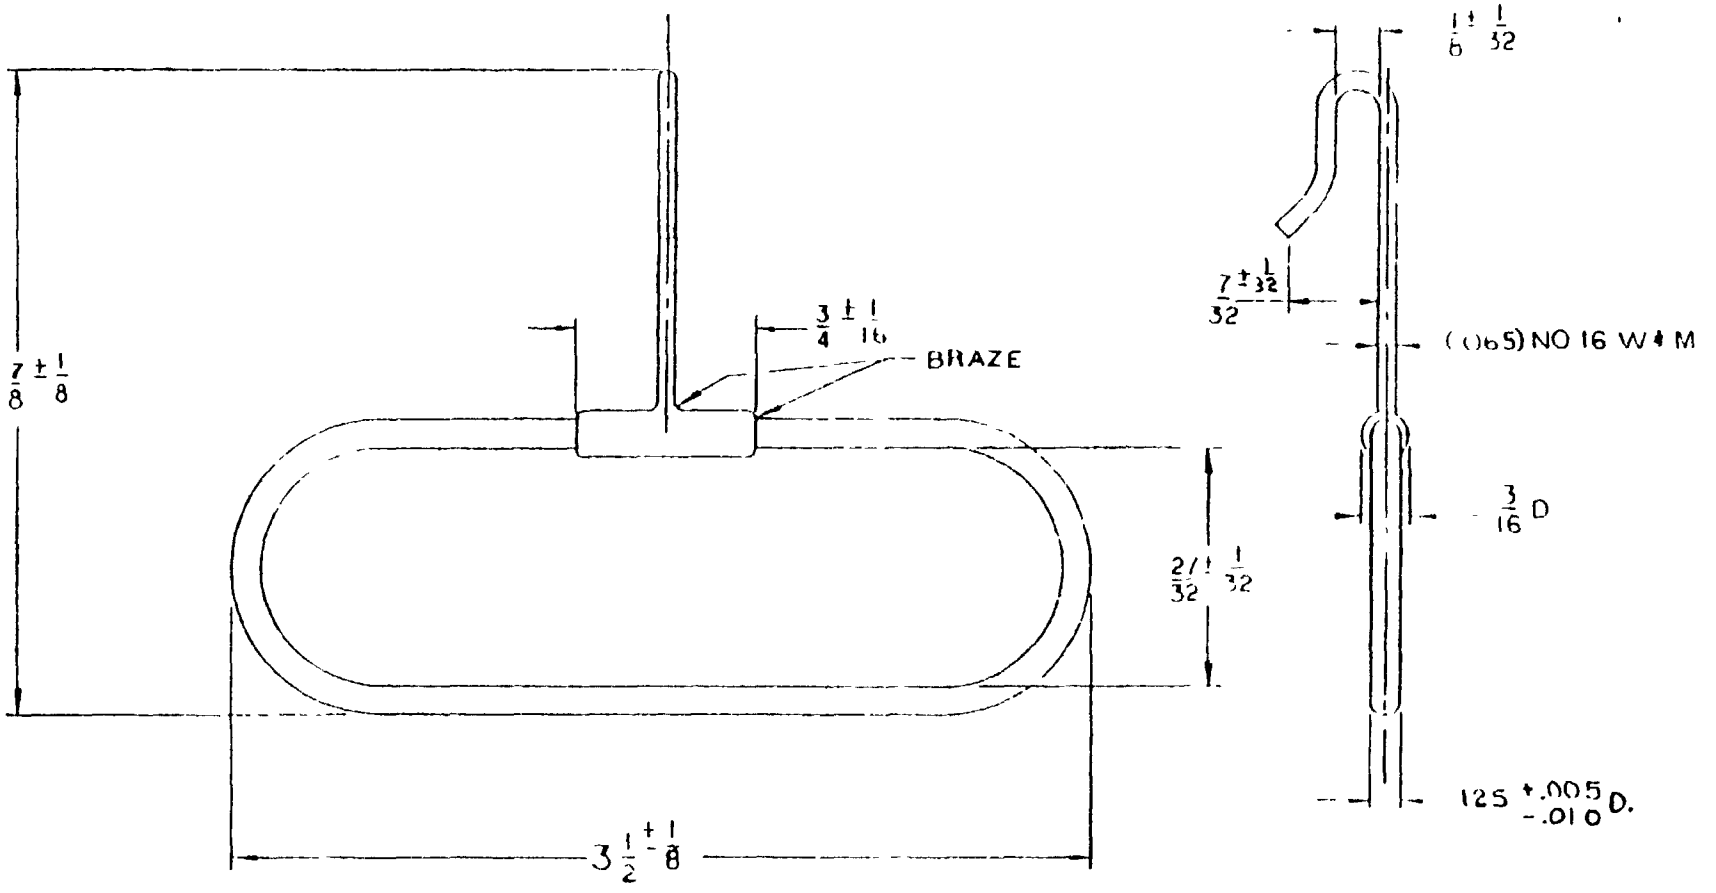

NSN 6515-00-363-2400


STYLE I

HANDLE, BONE CUTTING WIRE SAW, GIGLI

FIG. 1

Unless Otherwise Specified
Dimensions Are In Inches

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:20Z
Check the source to verify that this is the current version before use.

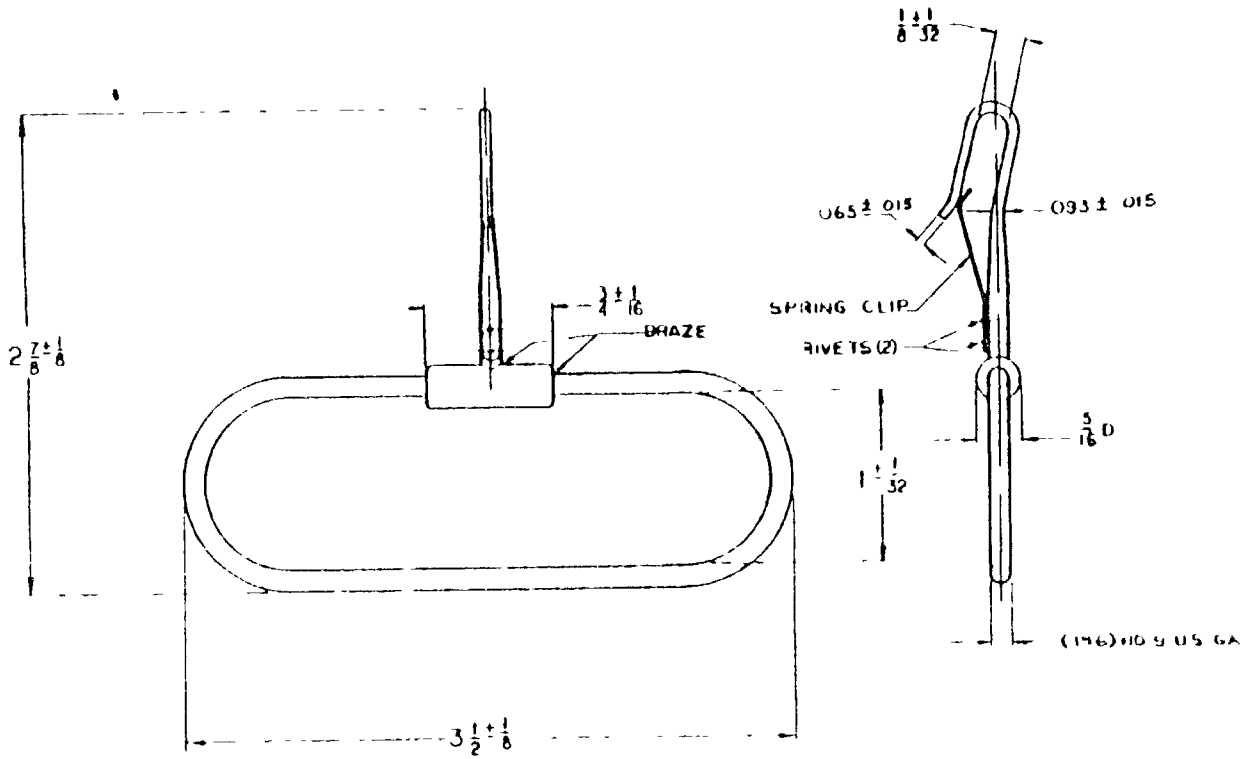

(1)

NSN 6515-00-363-2400

STYLE II (2)

20620

(3)

DEFENSE PERSONNEL SUPPORT CENTER
DIR OF MEDICAL MATERIEL PHILA PA

HANDLE, BONE CUTTING WIRE SAW, GIGLI

FIG 2

UNLESS OTHERWISE SPECIFIED
DIMENSIONS ARE IN INCHES

A-A-53519

Source: https://assist.dla.mil -- Downloaded: 2026/10-26T09:20Z
Check the source to verify that this is the current version before use.

INSTRUCTIONS: In a continuing effort to make our standardization documents better, the DoD provides this form for use in submitting comments and suggestions for improvements. All users of military standardization documents are invited to provide suggestions. This form may be detached, folded along the lines indicated, taped along the loose edge *(DO NOT STAPLE)*, and mailed. In block 5, be as specific as possible about particular problem areas such as wording which required interpretation, was too rigid, restrictive, loose, ambiguous, or was incompatible, and give proposed wording changes which would alleviate the problems. Enter in block 6 any remarks not related to a specific paragraph of the document. If block 7 is filled out, an acknowledgement will be mailed to you within 30 days to let you know that your comments were received and are being considered.

NOTE. This form may not be used to request copies of documents, nor to request waivers, deviations, or clarification of specification requirements on current contracts. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements.

(Fold along this line)

(Fold along this line)

NO POSTAGE NECESSARY IF MAILED IN THE UNITED STATES

OFFICIAL BUSINESS
PENALTY FOR PRIVATE USE $300

BUSINESS REPLY MAIL
FIRST CLASS PERMIT NO 4966 Alexandria, VA

POSTAGE WILL BE PAID BY

Commander
Defense Personnel Support Center
ATTN: DPSC-RSTE
2800 South 20th Street
Philadelphia, Pennsylvania 19101-8419

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:20Z
Check the source to verify that this is the current version before use.

(TO DETACH THIS FORM, CUT ALONG THIS LINE.)

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

(See Instructions – Reverse Side)

1. DOCUMENT NUMBER	2. DOCUMENT TITLE
A-A-53519	HANDLE, BONE, CUTTING SAW (Gigli)

3a. NAME OF SUBMITTING ORGANIZATION	4. TYPE OF ORGANIZATION *(Mark one)*
	☐ VENDOR
	☐ USER
b. ADDRESS *(Street, City, State, ZIP Code)*	☐ MANUFACTURER
	☐ OTHER *(Specify)*:

5. PROBLEM AREAS

a. Paragraph Number and Wording

b. Recommended Wording

c. Reason/Rationale for Recommendation

6. REMARKS

7a. NAME OF SUBMITTER *(Last, First, MI)* – Optional	b. WORK TELEPHONE NUMBER *(Include Area Code)* – Optional
c. MAILING ADDRESS *(Street, City, State, ZIP Code)* – Optional	8. DATE OF SUBMISSION *(YYMMDD)*

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:202
Check the source to verify that this is the current version before use.