A-A-53540
27 June 1988

COMMERCIAL ITEM DESCRIPTION

CALIPER, EYE, CASTROVIEJO

The General Services Administration has authorized the use of this commercial item description as a replacement for Federal Specification GG-C-106A which is cancelled.

This commercial item description covers an eye caliper of the Castroviejo design, for use in measuring distances on the eyeball.

Salient characteristics:

General.

The caliper shall conform to style, design and dimensions in accordance with Figure 1. It shall be spring loaded to make it in open position normally. A knurled adjustment knob shall be able to be held the pointer in a set position. The pointer tips shall be sharp and remain sharp after repeated uses.

Material. The shanks (including points) shall be fabricated from class 4 corrosion resistant steel in accordance with American Society for Testing and Materials (ASTM) F899. The scale shall be made of similar material, or as an alternate, class 3 corrosion resistant steel will be acceptable. The spring shall be made of class 3 material, tempered for the purpose intended. The remainder of the instrument (pivot screw, knob and stud) shall be class 4 material, or steel having chromium content of 17.5% max, carbon content of 0.10 to 0.17%, and sulfur content of 0.45% max.

Hardness. The Rockwell hardness of the shanks shall be C40 to C50. Other parts shall be hardened for durability.

Characteristics. The scale shall be calibrated from 0 to 20 millimeters (mm) in 1 mm intervals. The 0, 5, 10, 15 and 20 mm graduation marks shall be identified. The graduation marks and numerals shall be permanently marked.

Accuracy of the caliper shall be within $\pm$ 0.5 millimeter (mm) over the range of 1 mm to 20 mm.

AMSC N/A FSC 6540

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:21Z
Check the source to verify that this is the current version before use.

Finish. The finished caliper shall have mirror finish, except the scale shall be satin.

Corrosion resistance. No signs of corrosion or plating of copper shall show when tested for corrosion resistance as specified in Quality Assurance Provisions.

Tests. Corrosion resistance, hardness and performance shall be tested as specified under Quality Assurance Provisions.

Identification mark. The caliper shall be stamped with manufacturer's name or trademark, in addition to the word "stainless".

Workmanship. The caliper shall be free from defects which detract from its appearance or impair its serviceability.

Product Quality Level.

Visual and dimensional examination. Contractor shall be examined to verify that design, construction and workmanship are in accordance with applicable requirements.

Materials. The contractor shall be responsible for performing tests to assure that materials are in accordance with requirements specified.

Unit. Each (EA). One caliper, as specified, constitutes one unit.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract of purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:21Z
Check the source to verify that this is the current version before use.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more test characteristics.

Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and as follows. For accuracy, the Inspection level shall be S-1 and 1.0% AQL (percent defective). For corrosion resistance and hardness, the Inspection level shall be S-2 and 1.0% AQL (percent defective). The unit of product for examination purposes shall be one caliper.

Certificates of quality. Certificates of quality, supplied by the manufacturer of the materials, may be furnished in lieu of actual performance of composition testing by the contractor, provided lot identity has been maintained and can be demonstrated to the Government. The certificate shall include the name of the contractor, the contract number, the name of the manufacturer or supplier, the NSN, the item identification, the name of the component/material, the lot number, the lot size, the test method, and the test results.

Chemical analysis. In the absence of certificates of quality, the chemical analysis of the material used in the fabrication of the caliper shall be performed by the contractor.

Hardness test. Hardness shall be determined in accordance with ASTM E18 or ASTM E92. Conversion of Vickers hardness values into Rockwell hardness values shall be in accordance with ASTM E140.

Accuracy test. Set the points of the caliper to 20 mm using a precision scale. Read the caliper scale and record the reading. Repeat the above but set the caliper points to 10 mm. Both readings of the caliper shall meet the accuracy specified.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:21Z
Check the source to verify that this is the current version before use.

Corrosion tests. Sample of the instrument shall pass the Copper sulfate test and Boil test specified in ASTM F1089-Standard Test Method for Corrosion of Surgical Instruments.

Contractor certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Metric Products. Products manufactured to metric dimensions will be considered on an equal basis with those manufactured using inch-pound units, providing they fall within the tolerances specified using conversion tables contained in the latest revision of Federal Standard No. 376, and all other requirements of this document are met.

If a product is manufactured to metric dimensions and those dimensions exceed the tolerances specified in the inch/pound units, a request should be made to the contracting officer to determine if the product is acceptable.

The contracting officer has the option of accepting of rejecting the product.

Regulatory requirements.

Federal Food, Drug, and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use the covered material in accordance with Public Law 94-580 to the maximum extent practical.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:21Z
Check the source to verify that this is the current version before use.

Preservation, packaging, packing, labeling and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

NOTE: The following National Stock Number is covered by this document:

NSN	ITEM IDENTIFICATION
6540-00-299-9497	CALIPER, EYE, CASTROVIEJO

Ordering data. (Intermediate/exterior package quantities, labeling, and marking must be specified in the contract and/or order).

MILITARY INTERESTS:

Custodians:

ARMY - MD
NAVY - MS
AIR FORCE - 03

PREPARING ACTIVITY:

DoD-MB

Agent:


DLA-DM

CIVIL AGENCY COORDINATING ACTIVITIES:

VA-OSS
PHS
FDA-MPQAS
GSA

Project No. 6540-1198

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:21Z
Check the source to verify that this is the current version before use.

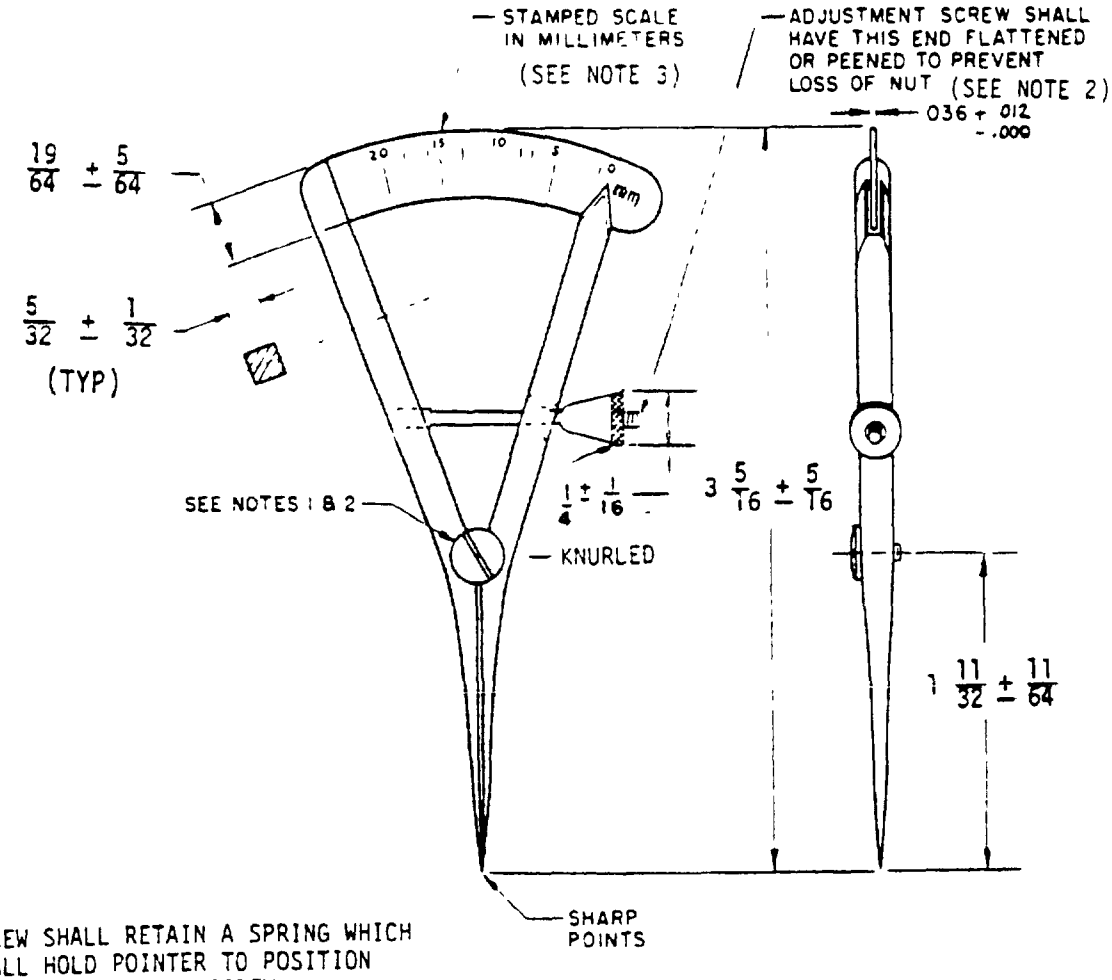

NOTES

1 SCREW SHALL RETAIN A SPRING WHICH SHALL HOLD POINTER TO POSITION SET BY ADJUSTMENT SCREW.
2 SCREW SHALL NOT BIND OR LOOSEN DURING USE. SCREW LOCK SHALL BE TIGHT ENOUGH TO PREVENT WOBBLING OF POINTS.
3 AS AN OPTION THE SCALE MAY APPEAR ON BOTH SIDES

ALL DIMENSIONS ARE IN INCHES.

6540-00-299-9497

FIGURE 1. Eye caliper, Castroviejo.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:21Z
Check the source to verify that this is the current version before use.

INSTRUCTIONS In a continuing effort to make our standardization documents better, the DoD provides this form for use in submitting comments and suggestions for improvements. All users of military standardization documents are invited to provide suggestions. This form may be detached, folded along the lines indicated, taped along the loose edge *(DO NOT STAPLE)*, and mailed. In block 5, be as specific as possible about particular problem areas such as wording which required interpretation, was too rigid, restrictive, loose, ambiguous, or was incompatible, and give proposed wording changes which would alleviate the problems. Enter in block 6 any remarks not related to a specific paragraph of the document. If block 7 is filled out, an acknowledgement will be mailed to you within 30 days to let you know that your comments were received and are being considered.

NOTE This form may not be used to request copies of documents, nor to request waivers, deviations, or clarification of specification requirements on current contracts. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements.

(Fold along this line)

(Fold along this line)

DEFENSE LOGISTICS AGENCY

NO POSTAGE NECESSARY IF MAILED IN THE UNITED STATES

OFFICIAL BUSINESS
PENALTY FOR PRIVATE USE $300

BUSINESS REPLY MAIL
FIRST CLASS PERMIT NO 4966 WASHINGTON D C

POSTAGE WILL BE PAID BY THE DEFENSE LOGISTICS AGENCY

Commander
Defense Personnel Support Center
ATTN: DPSC-STE
2800 South 20th Street
Philadelphia, Pennsylvania 19101-8419

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:21Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

(See Instructions – Reverse Side)

1 DOCUMENT NUMBER	2 DOCUMENT TITLE
A-A-53540	CALIPER, EYE, CASTROVIEJO

3a. NAME OF SUBMITTING ORGANIZATION	4 TYPE OF ORGANIZATION *(Mark one)*
	☐ VENDOR
	☐ USER
b ADDRESS *(Street City State ZIP Code)*	☐ MANUFACTURER
	☐ OTHER *(Specify)*

5 PROBLEM AREAS

a. Paragraph Number and Wording

b Recommended Wording

c Reason/Rationale for Recommendation

6 REMARKS

7a NAME OF SUBMITTER *(Last First, MI)* – Optional	b WORK TELEPHONE NUMBER *(Include Area Code)* – Optional
c MAILING ADDRESS *(Street City State ZIP Code)* – Optional	8 DATE OF SUBMISSION *(YYMMDD)*

DD FORM 92 MAR 1426 PREVIOUS EDITION IS OBSOLETE

Source: https://assist.dla.mil – Downloaded: 2026-10-26T09:21Z
Check the source to verify that this is the current version before use.