A-A-53560
30 June 1988

COMMERCIAL ITEM DESCRIPTION

CANNULA BRONCHIAL (Holinger)

The General Services Administration has authorized the use of this commercial item description.

This commercial item description covers an aspirating cannula of the Holinger design suitable for the aspiration of bronchial secretions through a Holinger bronchoscope.

Salient characteristics:

Material. The cannula shall be manufactured from monel (nickel-copper-molybdenum alloy). As an alternate, the cannula may be manufactured from Class 3 austenitic corrosion-resistant steel in accordance with American Society for Testing and Materials (ASTM) Standard F899.

Style and design. The cannula shall be in accordance with Figure 1 with two eyes on diametrically opposite sides of the tube.

Passivation (steel cannulas only). The cannula shall be properly passivated.

Finish. The finish shall be mirror or satin.

Workmanship. The cannula shall be free from burrs, slivers, grind and tool marks, or any defects which affect their appearance or utility.

Product Quality Level.

Visual and dimensional examination. Shall be examined to verify that design, construction and workmanship are in accordance with applicable requirements.

Materials. The supplier shall be responsible for performing tests to assure that materials are in accordance with requirements specified.

AMSC N/A FSC 6515

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:21Z
Check the source to verify that this is the current version before use.

Unit. Each 24 cannulae, as specified, constitutes one unit.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures, and testing (determination by technical means of physical and chemical properties) of the item.

Examination. The cannulas shall be examined to determine compliance with all requirements contained in this specification. Sampling for examination shall be conducted in accordance with MIL-STD-105, sampling level S-2, AQL 1.5 (percent defective).

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more test characteristics.

Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and as specified herein. The unit of product for test purposes shall be one cannula. Inspection level shall be S-1 with an AQL of 1.0, except for chemical composition.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:21Z
Check the source to verify that this is the current version before use.

Corrosion-resistant test. Cannulas manufactured from monel shall be tested for resistance to corrosion in accordance with the Resistance to Salt Spray Test of Federal Specification GG-I-526.

Cannulas manufactured from steel shall be tested for resistance to corrosion in accordance with the Resistance to Boil Test of ASTM Test Method F1089.

Composition test. In the absence of certificates of quality, a sufficient amount of raw material shall be tested for chemical composition as to be representative of the lot (or raw material). The acceptance number for composition shall be zero (0).

Certificates of quality. Certificates of quality, supplied by the manufacturer of the materials, may be furnished in lieu of actual performance of composition testing by the contractor, provided lot identity has been maintained and can be demonstrated to the Government. The certificate shall include the name of the contractor, the contract number, the name of the manufacturer, or supplier, the NSN, the item identification, the name of the component material, the lot number, the lot size, the test method, and the test results.

Contractor certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producers' own drawings, specification, standard, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers with the requirements of the Federal Food, Drug and Cosmetic Act as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials The offeror/contractor is encouraged to use recovered material in accordance with Public Law 94-580 to the maximum extent practical.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:21Z
Check the source to verify that this is the current version before use.

A-A-50560

Preservation, packaging, packing, labeling and marking. Unless otherwise specified, preservation, packaging and packing shall be to a degree of protection to preclude damage to contents and its contents incident under normal shipping conditions handling, etc., in the supplier's facility to the receiving activity, plus requirements for reuse of containers shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and or order.

NOTE. The following National Stock Number is covered by this document:

NSN	ITEM IDENTIFICATION
6515-01-360-0781	Cannula, Endotracheal, Rubber 12 French

Ordering data: Intermediate/exterior package quantities and labeling and marking must be specified in the contract and or order.

Military Departments:

Preparing Activity:

Army - MD
Navy - MC
Air Force - 99

Agent:

DLA-DM

CIVIL AGENCY COORDINATING ACTIVITIES:

VA-OSS
PHS
FDA-MPOAS

PSC 6505

Project No. 6515-0746

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:21Z
Check the source to verify that this is the current version before use.

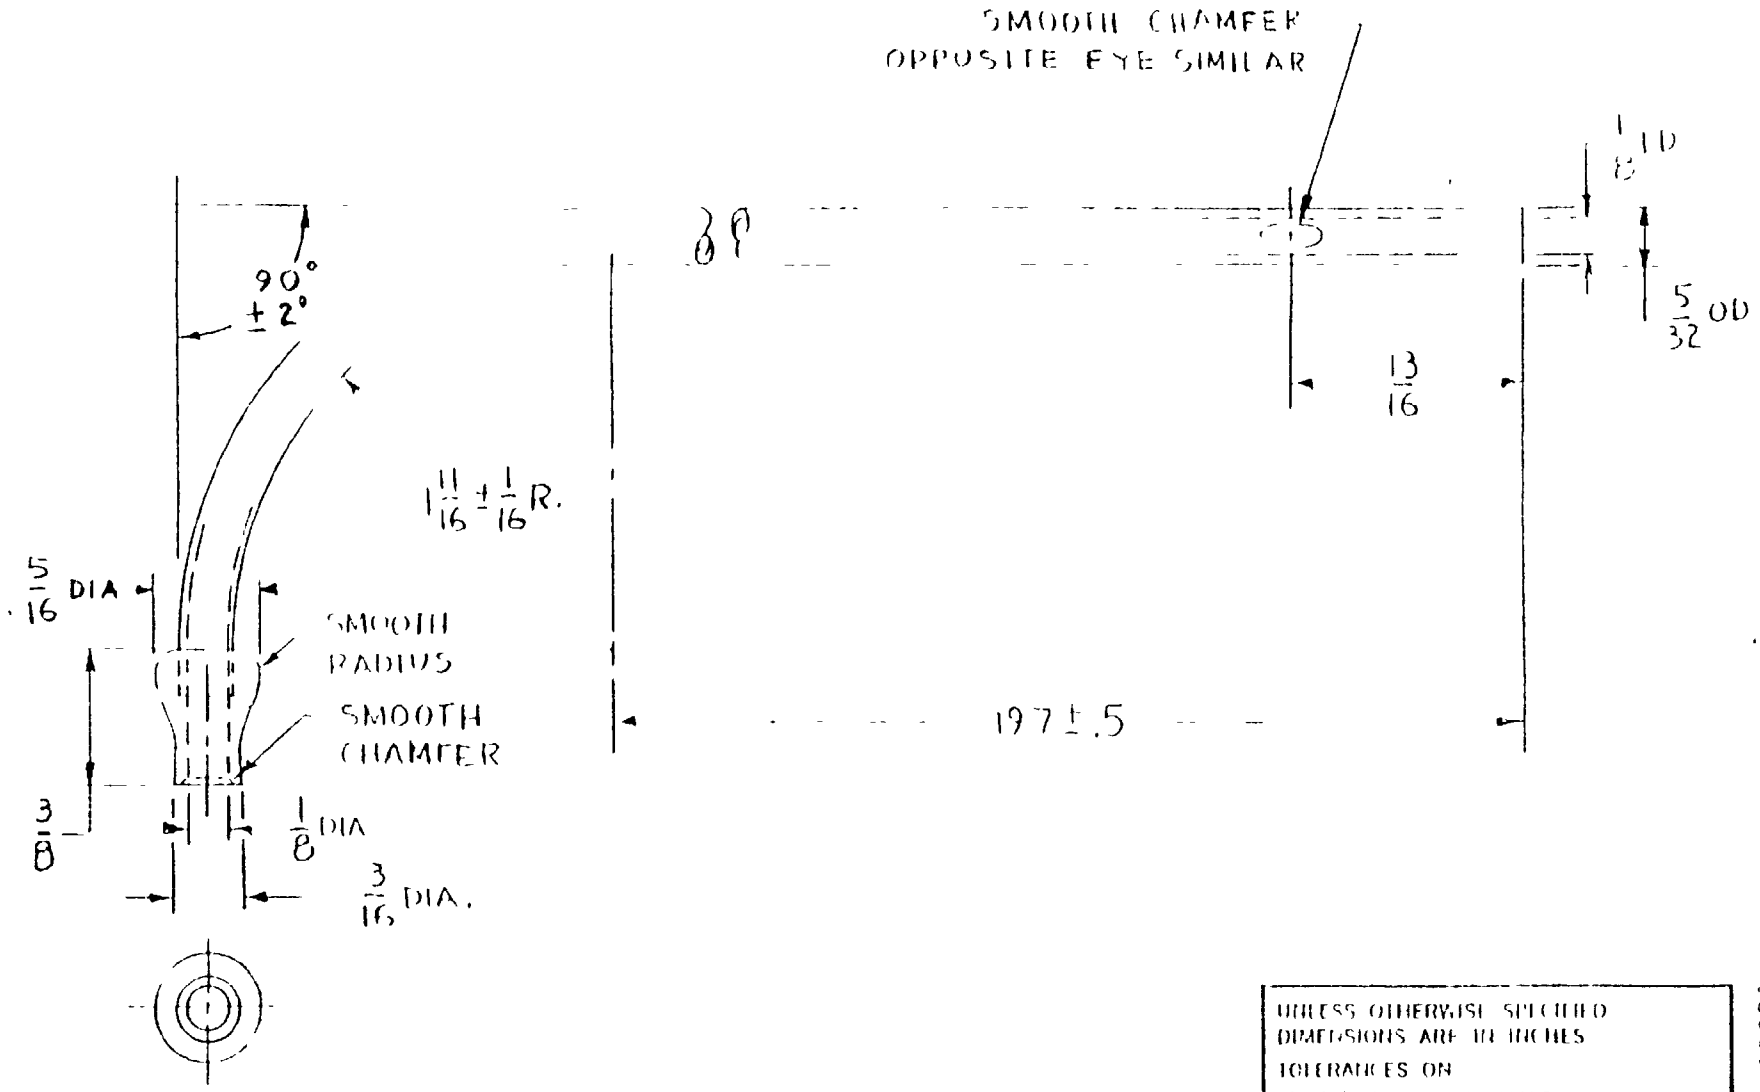


FIGURE 1. CANNULA, BRONCHIAL, HOLINGER

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:21Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

(See Instructions - Reverse Side)

1. DOCUMENT NUMBER	2. DOCUMENT TITLE
A-A-53560	CANNULA, BRONCHIAL (Bolinger)

3. NAME OF SUBMITTING ORGANIZATION	4. TYPE OF ORGANIZATION (Mark one)
	☐ VENDOR
	☐ USER
5. ADDRESS (Street, City, State, ZIP Code)	☐ MANUFACTURER
	☐ OTHER (Specify)

5. PROBLEM AREAS

a. Paragraph Number and Wording

b. Recommended Wording

c. Reason/Rationale for Recommendation

6. REMARKS

7a. NAME OF SUBMITTER (Last, First, MI) – Optional	b. WORK TELEPHONE NUMBER (Include Area Code) – Optional
c. MAILING ADDRESS (Street, City, State, ZIP Code) – Optional	8. DATE OF SUBMISSION (YYMMDD)

(FOLD ON THIS LINE)

(FOLD ON THIS LINE)

DD FORM 1426

Source: https://assist.dla.mil -- Downloaded: 2020-10-26T00:21Z
Check the source to verify that this is the current version before use.

NSTRUCTIONS In a continuing effort to make our standardization documents better he DoD provides this orm for use in ubmitting comments and suggestions or improvements All users of military standardization documents are invited to provide uggestions This orm may be detached olded along the lines indicated taped along the loose edge DO NOT STAPLE, and mailed In block 5 be as specific as possible about particular problem areas such as wording which required interpretation, was oo rigid restrictive oose ambiguous, or was incompatible and give proposed wording changes which would alleviate the problems Enter n block any remarks not related to a specific paragraph of he document If block is filled out an cknowledgement will be mailed to you within 30 days to let you know that our comments were received and are being onsidered

NOTE This form may not be used to request copies of documents nor to request waivers deviations or clarification of pecific government requirements on current contracts Comments submitted on this form do not constitute or imply authorization o waive any portion of the referenced document or to amend contractual requirements

Fold along this line

Fold along this line

NO POSTAGE NECESSARY IF MAILED IN THE UNITED STATES

FIRST CLASS PERMIT NO. 966 Alexandria, VA

BUSINESS REPLY MAIL

POSTAGE WILL BE PAID BY

Commander
Defense Personnel Support Center
ATTN: DPSC-PSTS
2800 South 20th Street

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:21Z
Check the source to verify that this is the current version before use.