
FED. SUP CLASS
6630

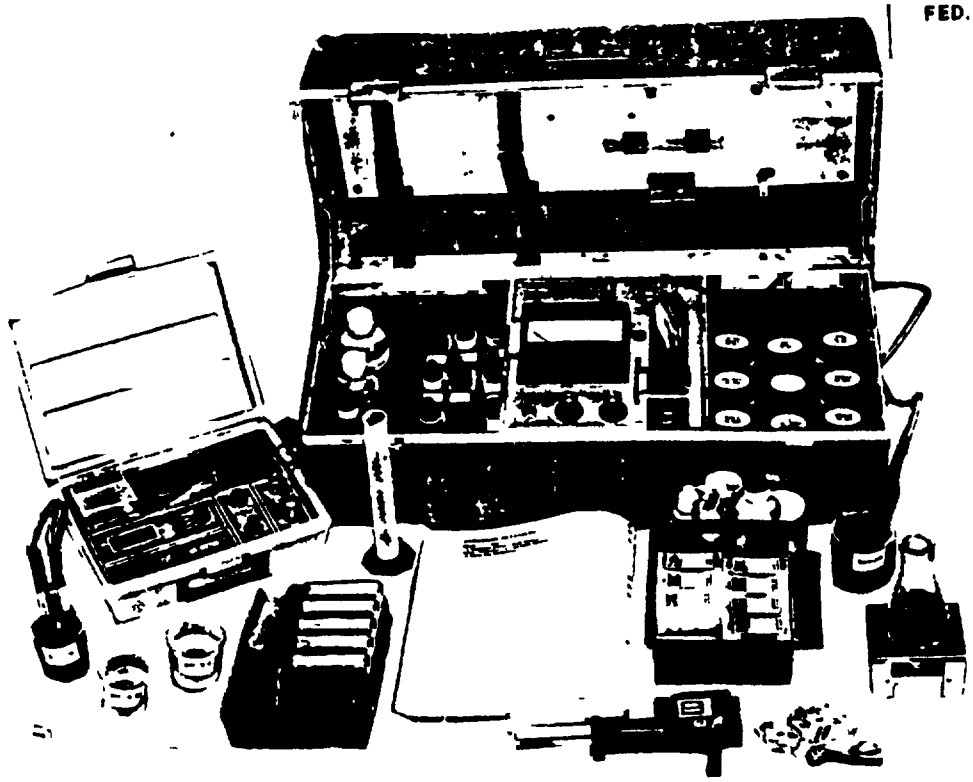

USER ACTIVITIES ARMY - CE

REVIEWER ACTIVITIES ARMY - ER, ME
AIR FORCE -

PART NUMBER	NET WEIGHT	SPECIALIZED EQUIPMENT
MS36551-1	16 1 kg	Spectrophotometer, Digital Titrator With Titration Cartridges
MS36557-2	16 6 kg	Spectrophotometer, Digital Titrator With Titration Cartridges, Conductivity Meter
MS36557-3	17 0 kg	Spectrophotometer, Digital Titrator With Titration Cartridges, Conductivity Meter, Digital pH Meter
MS36557-4	16 0 kg	pH Electrode, Colormeter Digital Titrator With Titration Cartridges, 120-240V Battery Eliminator

MATERIAL: Carrying case shall be of ABS (acrylonitrile-butadiene-styrene) plastic in accordance with Federal Specification L-P-1183B

DESIGN Each set shall contain all the chemical paraphernalia, glassware, and batteries required for conducting the analytical water test, including a comprehensive instruction manual

APPROVED 19 February 68 REVISED (A) 18 FEB 1971

This military standard is approved for use by all Departments and Agencies of the Department of Defense. Selection for all new engineering and design applications and for repetitive use shall be made from this document

(A) ENTIRE STANDARD REVISED

P A	EA	INTERNATIONAL INTEREST	TITLE	MILITARY STANDARD
Other Cust	MS 99		WATER QUALITY CONTROL SET	MS36557
Procurement Specifications	NONE	SUPERSEDES:		SHEET 1 OF 2

PROJECT NUMBER 6630-0194

DD FORM 1 MAY 73 672 (COORDINATED) PREVIOUS EDITIONS OF THIS FORM ARE OBSOLETE

REVISION DATE

Source: https://assist.dla.mil -- Downloaded: 2026-10-23T17:43Z
Check the source to verify that this is the current version before use.

FED SUP CLASS
6630

Each set shall have a digital titrator with three delivery tubes and titration cartridges for acidity, alkalinity, carbon dioxide, chloride, dissolved oxygen and hardness tests.

MS36557-1, -2, -3 sets shall have a spectrophotometer with a photometric accuracy of ± 2.5 mm and a wavelength range of 400 - 700 mm and a band pass less than 17 mm

MS36557-2 and -3 sets shall have a conductivity meter with ranges of 0-2, 0-20, 0-200, 0-2000, 0-20,000 μ siemens/cm (μ mhos), an accuracy of ± 2% of full scale and an automatic temperature compensation of 0-100°C.

MS36557-3 sets shall have a digital pH meter with automatic temperature compensation of 0-100°C, a range of 0-14 pH with pH accuracy of ± 0.01 unit, ± 1 digit, mv: ± 0.1% of full scale and powered by one 9V battery.

PURPOSE: For use in conducting water and wastewater testing.

NOTE:
1. Items differing from this Military Standard by minor variations in design or dimensions are considered standard under this document, provided such variations do not affect performance and are not in conflict with the material requirements as specified herein.

2 Referenced document shall be of the issue in effect on date of invitations for bids

REVISED

APPROVED

This military standard is approved for use by all Departments and Agencies of the Department of Defense. Selection for all new engineering and design applications and for repetitive use shall be made from this document

P A	INTERNATIONAL INTEREST	TITLE	MILITARY STANDARD
Other Cust		WATER QUALITY CONTROL SET	MS 36557
Procurement Specifications	SUPERSEDES:		SHEET 2 OF 2

DD FORM 672 (COORDINATED) PREVIOUS EDITIONS OF THIS FORM ARE OBSOLETE DATE

Source: https://assist.dla.mil - Downloaded: 2026-10-23T11:43Z
Check the source to verify that this is the current version before use.