INCH-POUND

A-A-53072A
12 February 1993
SUPERSEDING
A-A-0053072(DM)
15 July 1987

COMMERCIAL ITEM DESCRIPTION

BRONCHOSCOPE, FIBER OPTIC, HOLINGER

The General Services Administration has authorized the use of this Commercial Item Description as a replacement for Military Specification MIL-B-36893A which is cancelled.

This commercial item description covers fiber optic bronchoscopes, of the Holinger design, suitable for use in bronchoscopy and anesthesiology.

Salient characteristics:

Classification. The bronchoscopes shall be supplied in the following sizes:

Type I - 3.5 mm diameter lumen by 25 cm long
Type II - 9 mm diameter lumen by 40 cm long

General. Shall be a fiber optic bronchoscope of the Holinger design, suitable for use in bronchoscopy and anesthesiology when used with fiber optic endoscopic instrument light, 115 volt, 60 Hz, AC and fiber optic endoscopic instrument cable, 72 inches long. (See Notes).

The instrument shall be supplied with an oval-shaped fiber optic light carrier that will disperse illumination when assembled into the light carrier channel of the instrument and assembled to the fiber optic endoscopic instrument light and cable specified above.

Style, design and dimensions. The fiber optic bronchoscope shall be in accordance with Figure 1 for style, design and dimensions.

AMSC N/A FSC 6515
DISTRIBUTION STATEMENT A: Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:15Z
Check the source to verify that this is the current version before use.

The bronchoscope shall have a smooth distal tip to provide maximum visibility and ease of instrument insertion. The instrument shall have an air tube assembly, with a 15 millimeter (mm) tracheal connector secured to the air tube. The air tube shall be permanently secured to the main tube proper. The 15 mm connector shall have a standard external taper in accordance with Figure 2 of ANSI Standard Z79.2 to accept standard tracheal tubes for anesthesiology and aspiration procedures. The handle of the bronchoscope shall be permanently secured to the main tube and shall have an external taper at the proximal end which will accommodate an interchangeable window plug to provide a closed system for administering anesthesia.

The fiber optic light carrier shall be of the bayonet type that shall be readily inserted into the light carrier channel and positioned into place by a slot in the instrument handle. The light carrier channel shall be permanently secured to the main tube and shall be completely sealed at the outer surface of the distal end. Open slots shall be on both sides of the main tube at the distal end. When the light carrier is inserted into the light carrier channel, the lumen of the instrument shall not be decreased in size.

Material. The main tube, light carrier channel, and light carrier housing shall be manufactured from unplated nickel-copper alloy (Monel) of composition in accordance with American Society for Testing and Materials (ASTM) Standard B165. As an alternate, the distal tip of the main tube may be manufactured from UNS C75200 nickel-silver of composition in accordance with ASTM Standard B122, and the tip silver-brazed to the main tube.

The handle, air tube assembly, bayonet connector, window plug housing, window plug cap, and spacers shall be manufactured from austenitic corrosion-resistant steel in accordance with ASTM Standard F899. As an alternate, these componenets may be manufactured from Monel of composition in accordance with ASTM B164 or ASTM B165.

The window of the window plug assembly shall be manufactured from clear polycarbonate. The sealing washers of the window plug assembly shall be manufactured from polytetrafluoroethylene (Teflon).

The light carrier shall be filled with fiberoptic glass fibers which transmit illumination.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:15Z
Check the source to verify that this is the current version before use.

Finish. All surfaces of the instrument and components shall have a uniform and smooth finish. Exterior surfaces shall be polished. The finish shall be free from burrs, pits, cracks, holes, rough areas, corrosion, or sharp edges. The edges of the side eyes shall be rounded or chamfered.

Passivation. Corrosion-resistant steel components shall be properly passivated.

Identification marking and labeling. The bronchoscope shall be legibly and permanently marked with name of the manufacturer or registered trademark, size designation and date of manufacturing (year, month). The light carrier shall be permanently marked with the nominal length in centimeters.

Workmanship. The bronchoscope shall be free from defects which detract from its appearance or impair its serviceability.

Unit. EACH (EA). One bronchoscope of the size specified, constitutes one unit.

QUALITY ASSURANCE PROVISIONS.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspection are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:15Z
Check the source to verify that this is the current version before use.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Sampling for examination. Sampling for examination shall be conducted in accordance with MIL-STD-105 and as specified herein. Unit of product for examination purposes shall be one bronchoscope as specified. Sampling shall be inspection level II with an Acceptable Quality Level (AQL) of 1.0.

Examination. Examination shall be conducted to determine compliance with specification requirements.

Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and as specified herein. Unit of product for test purposes shall be one bronchoscope. Sampling shall be inspection level S-2 with an AQL of 1.0.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for determination of two or more test characteristics.

Metric products. Products manufactured to metric dimensions will be considered on an equal basis with those manufactured using inch-pound units, providing they fall within the tolerance specified using conversion tables contained in the latest revision of Federal Standard No. 376, and all other requirements of this document are met.

If a product is manufactured to metric dimensions and those dimensions exceed the tolerances specified in the inch-pound units, a request should be made to the contracting officer to determine if the product is acceptable.

The contracting officer has the option of accepting or rejecting the product.

Contractor certification. The contractor shall certify and maintain substantiating evidence that the product offered meets the salient characteristics of this Commercial Item Description, and that the product conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:15Z
Check the source to verify that this is the current version before use.

Regulatory requirements.

Federal Food, Drug, and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Federal Acquisition Regulation Subpart 23.4 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

Ordering data. Intermediate/exterior package quantities and labeling and marking must be specified in the contract and/or order.

NOTE 1: The cable, fiber optic and light, fiber optic described under salient characteristics are standardized items and carry National Stock Number 6515-00-104-8434 and 6515-00-104-8520 respectively.

NOTE 2: The following National Stock Numbers, Item Identifications and their respective Types are covered by this document:

NATIONAL STOCK NUMBER	ITEM IDENTIFICATION	TYPE
6515-00-890-3518	BRONCHOSCOPE, FIBER OPTIC, HOLINGER, 3.5 mm by 25 cm	I
6515-01-187-7777	BRONCHOSCOPE, FIBER OPTIC, HOLINGER, 9 mm by 40 cm	II

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:15Z
Check the source to verify that this is the current version before use.

A-A-53072A

MILITARY INTERESTS:

Custodians:

Army - MD
Navy - MS
Air Force - 03

Preparing Activity:

DoD-MB

Agent:


DLA-DM

CIVIL AGENCY COORDINATING ACTIVITIES:

VA-OSS
USPHS
FDA-MPQAS

Project Number: 6515-5445
Location: c:\word\doc\eric\bronccid

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:15Z
Check the source to verify that this is the current version before use.

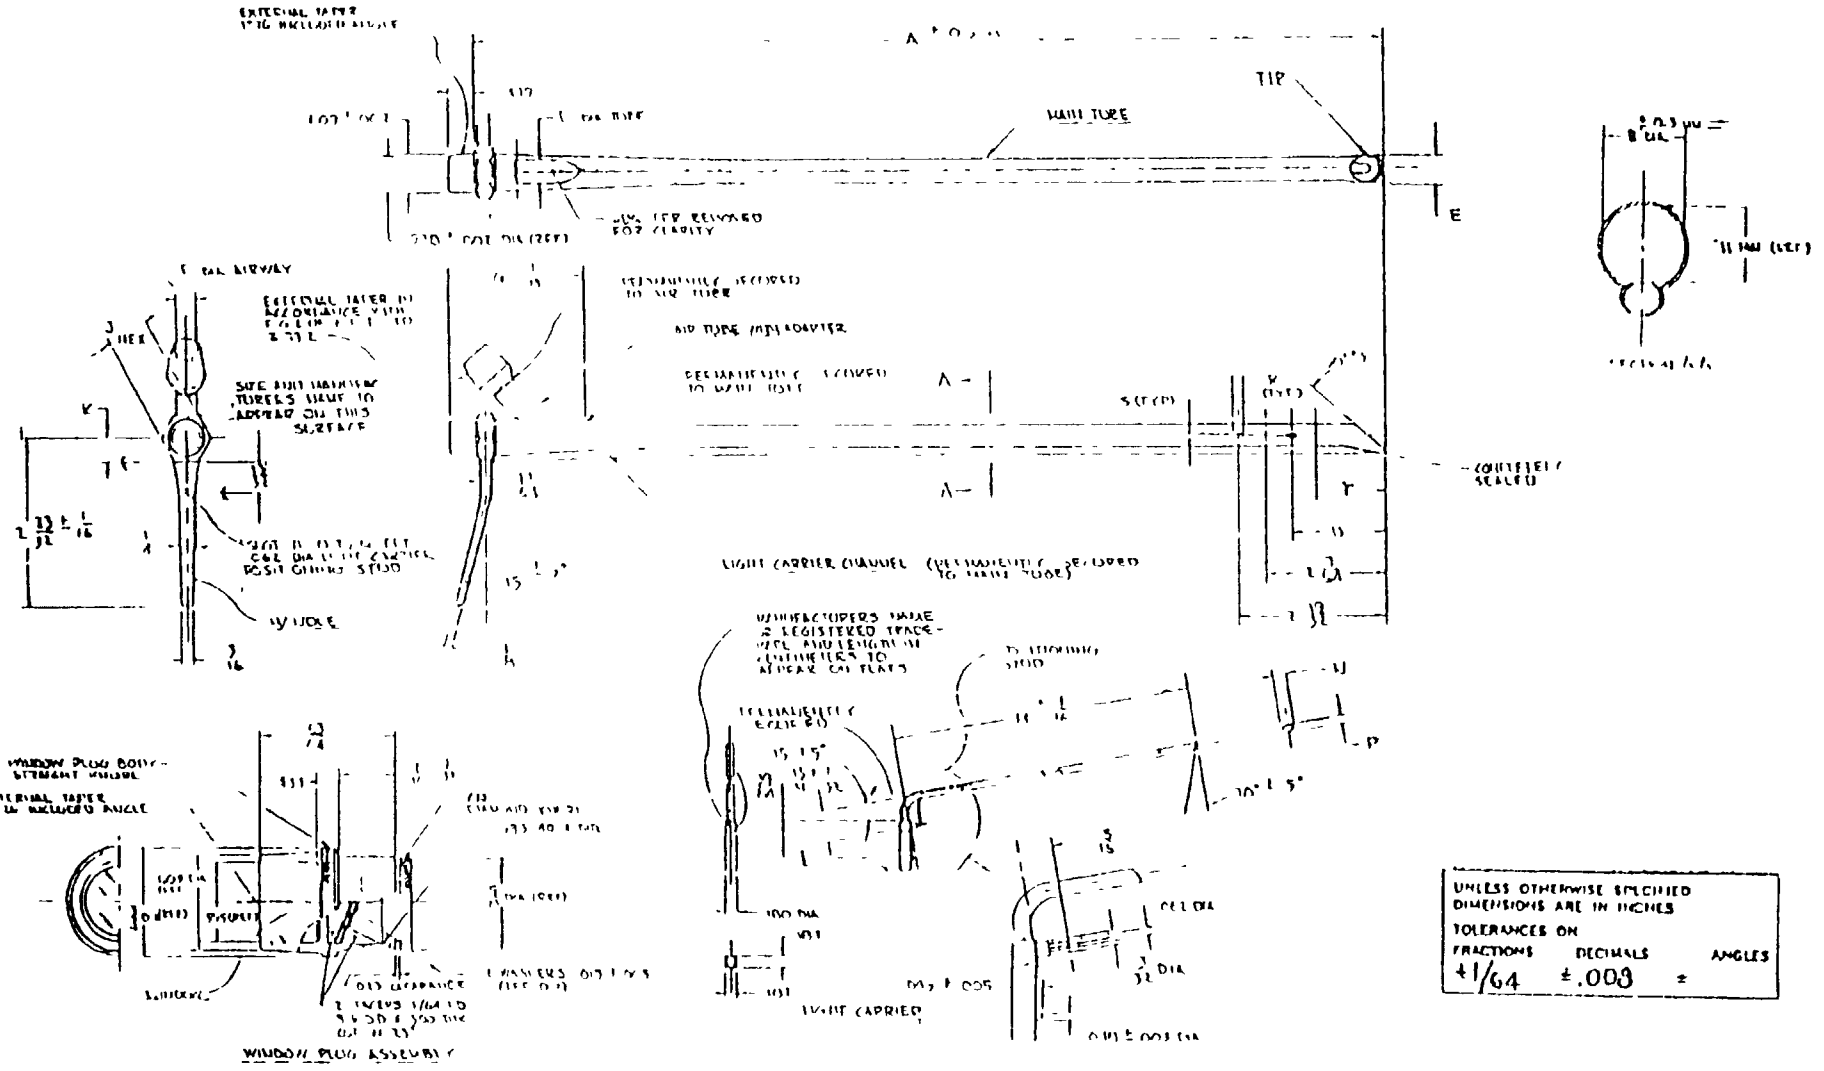

NSN	TYPE	SIZE	A	B	C	D	E	F	G	H	J	K	L	M	N	P	R	S
6515-00-890-3518	I	3.5 MM X 25 CM	25 CM	3.5 MM	1-1/8	1.9/16	.240	9/32	2.3/32	3.0 MM	1/16	3/8	.316	9.9/16	.090	.065	7/64	1/16
6515-01-187-7777	II	9 MM X 40 CM	40 CM	9.0 MM	1.15/64	1.2.1/32	.445	1/32	2.7/16	8.5 MM	3/4	27/64	.305	15	.150	.097	1/64	3/32

A-A-53072A

FIGURE 1. BRONCHOSCOPE, FIBER OPTIC, HOLDING

Source: https://assist.dla.mil - Downloaded: 2026-10-26T09:15Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

INSTRUCTIONS

1. The preparing activity must complete blocks 1, 2, 3, and 8. In block 1, both the document number and revision letter should be given.
2. The submitter of this form must complete blocks 4, 5, 6, and 7.
3. The preparing activity must provide a reply within 30 days from receipt of the form.

NOTE: This form may not be used to request copies of documents, nor to request waivers, or clarification of requirements on current contracts. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements.

I RECOMMEND A CHANGE:	1. DOCUMENT NUMBER	2. DOCUMENT DATE (YYMMDD)
	A-A-53072A	12 February 1993

3. DOCUMENT TITLE
BRONCHOSCOPE, FIBER OPTIC, HOLINGER

4. NATURE OF CHANGE (*Identify paragraph number and include proposed rewrite, if possible. Attach extra sheets as needed.*)

5. REASON FOR RECOMMENDATION

6. SUBMITTER

a. NAME (Last, First, Middle initial)	b. ORGANIZATION	
c. ADDRESS (Include Zip Code)	d. TELEPHONE (Include Area Code) (1) Commercial (2) AUTOVON (If applicable)	7. DATE SUBMITTED (YYMMDD)

8. PREPARING ACTIVITY

a. NAME	b. TELEPHONE (Include Area Code) (1) Commercial	(2) AUTOVON
Defense Personnel Support Center ATTN: DPSC-MSE	(215)7372870	444-2870
c. ADDRESS (Include Zip Code) 2800 South 20th Street Philadelphia, PA 19145	IF YOU DO NOT RECEIVE A REPLY WITHIN 45 DAYS, CONTACT Defense Quality and Standardization Office 5203 Leesburg Pike, Suite 1403, Falls Church, VA 22041-3466 Telephone (703) 756-2340 AUTOVON 289-2340	

DD Form 1426, OCT 89 — *Previous editions are obsolete*

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:15Z
Check the source to verify that this is the current version before use.