A-A-53102
28 July 1987

COMMERCIAL ITEM DESCRIPTION

ADAPTER, HYPODERMIC NEEDLE-TO-TUBING

The General Services Administration has authorized the use of this commercial item description.

This commercial item description covers one type of hypodermic needle-to-tubing adapter.

Salient characteristics:

Style and design. Style and design of the adapter shall conform to Figure 1. The adapter shall contain a hose-end, a knurled finger grip, and a male Luer Slip that conforms to ANSI/HIMA MD70.1.

Dimensions. The adapter shall pass the test listed in ANSI/HIMA MD70.1.

Performance. The adapter shall effect a leak-tight connection between 1/8 inch I.D. rubber tubing and a hypodermic needle that has a female Luer-Slip hub. When tubing is connected, the tubing-to-adapter connection shall not separate under a 2 lb. tensile load. The adapter shall pass the leak test specified in ANSI/HIMA MD70.1. Prior to testing, rubber tubing shall be secured to the adapter's hose-end and closed with a suitable pinch-clamp.

Materials. The adapter shall be fabricated from properly tempered Type 260, 270, or 360 brass conforming to GG-I-526.

Finish. The adapter shall be nickel plated or chromium-over-nickel plated. The plated adapter shall have a smooth, uniform finish.

Corrosion-resistance. The adapter shall pass the boil and salt-spray tests specified in GG-I-526. For the salt spray test, the exterior of the adapter shall be the significant surface.

AMSC N/A FSC 6515

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:15Z
Check the source to verify that this is the current version before use.

Workmanship. The adapter shall be free from nicks, dents, burrs sharp edges, corrosion, flaking or peeling plating, and any other defects that detract from its appearance or impair its serviceability. The adapter shall be supplied clean.

Unit. Each (EA). One adapter, as specified, constitutes one unit.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more test characteristics.

Sampling for inspection. Sampling for inspection shall be conducted in accordance with MIL-STD-105 at Level II, AQL (Acceptable Quality Level) 1.0 percent. The unit of product for test purposes shall be one adapter.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:15Z
Check the source to verify that this is the current version before use.

Contractor certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Public Law 94-580 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

NOTE: The following National Stock Number is covered by this document:

NSN	ITEM IDENTIFICATION
6515-00-300-0500	ADAPTER, HYPODERMIC NEEDLE-to-TUBING, Brass:

Ordering data. (Intermediate/exterior package quantities and labeling and marking must be specified in the contract and/or order.)

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:15Z
Check the source to verify that this is the current version before use.

COMMERCIAL ITEM DESCRIPTION A-A-53102

MILITARY INTERESTS:

Custodians:

Army - MD
Navy - MS
Air Force - 03

Civil Coordinating Activity:

VA-OSS
PHS
FDA-MPQAS

Preparing Activity:

DoD-MB


Agent:

DLA-DM

PGC 44997

Project No. 6515-3585

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:15Z
Check the source to verify that this is the current version before use.

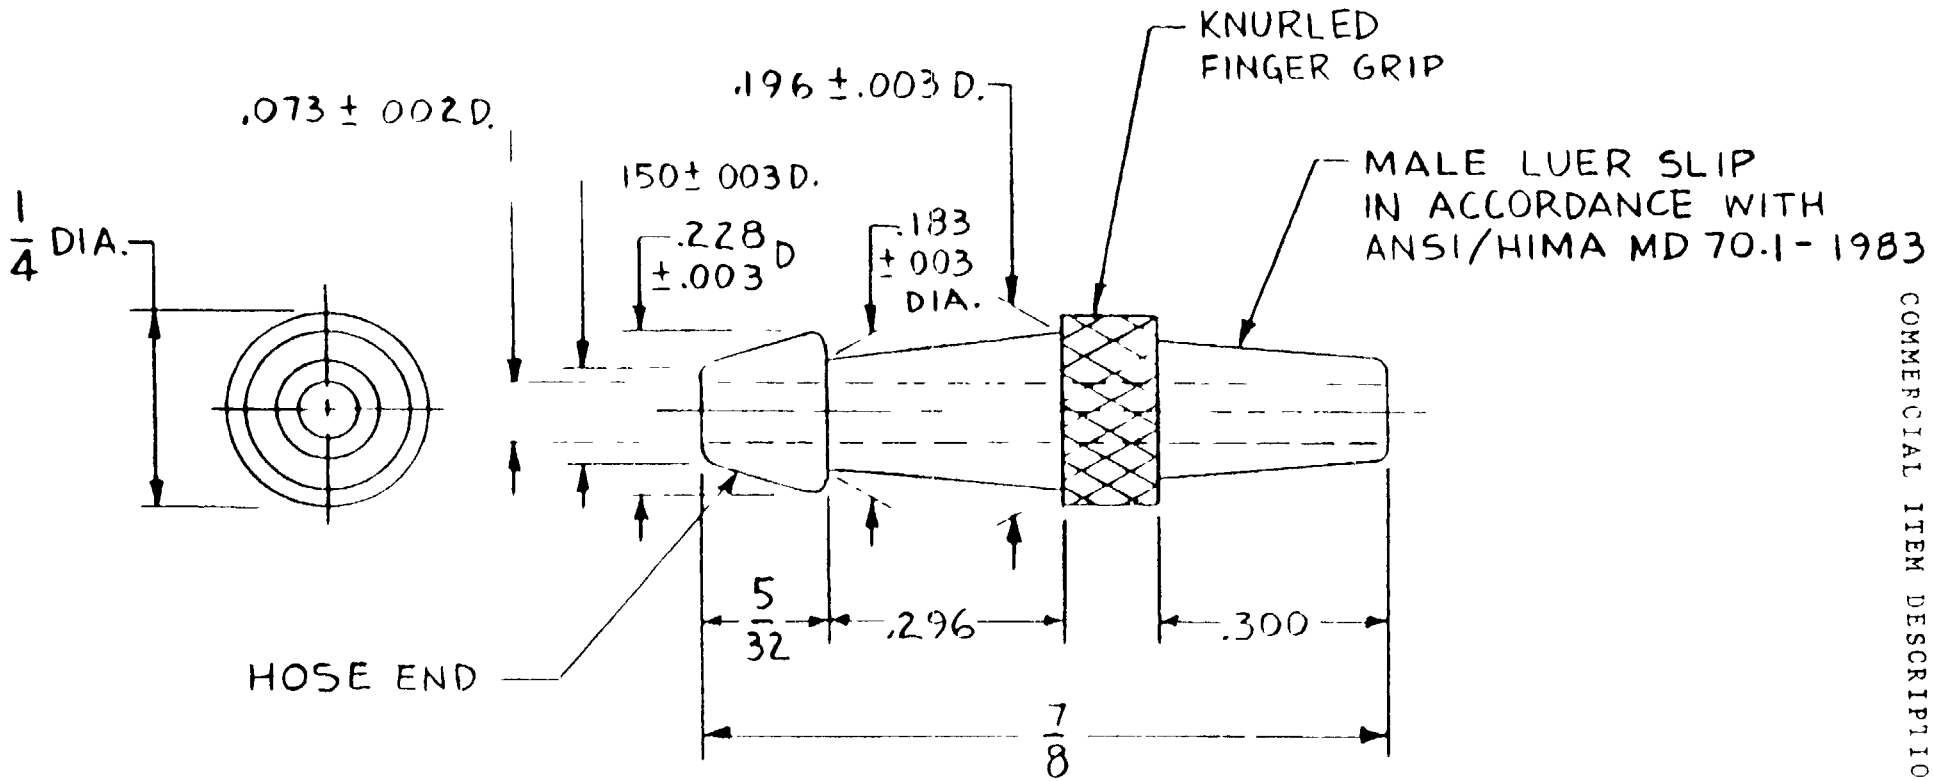

UNLESS OTHERWISE SPECIFIED DIMENSIONS ARE IN INCHES		
TOLERANCES ON		
FRACTIONS	DECIMALS	ANGLES
± 1/32	± .005	±

COMMERCIAL ITEM DESCRIPTION A-A-53102

FIGURE 1 ADAPTER, HYPODERMIC NEEDLE TO TUBING, BRASS

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:15Z
Check the source to verify that this is the current version before use.

INSTRUCTIONS In a continuing effort to make our standardization documents better, the DoD provides this form for use in submitting comments and suggestions for improvements. All users of military standardization documents are invited to provide suggestions. This form may be detached, folded along the lines indicated, taped along the loose edge *(DO NOT STAPLE)* and mailed. In block 5, be as specific as possible about particular problem areas such as wording which required interpretation, was too rigid, restrictive, loose, ambiguous, or was incompatible, and give proposed wording changes which would alleviate the problems. Enter in block 6 any remarks not related to a specific paragraph of the document. If block 7 is filled out, an acknowledgement will be mailed to you within 30 days to let you know that your comments were received and are being considered.

NOTE This form may not be used to request copies of documents, nor to request waivers, deviations, or clarification of specification requirements on current contracts. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements.

(Fold along this line)

(Fold along this line)

DEFENSE LOGISTICS AGENCY

NO POSTAGE NECESSARY IF MAILED IN THE UNITED STATES

OFFICIAL BUSINESS
PENALTY FOR PRIVATE USE $300

BUSINESS REPLY MAIL
FIRST CLASS PERMIT NO. 4966 WASHINGTON, D.C.

POSTAGE WILL BE PAID BY THE DEFENSE LOGISTICS AGENCY

Commander
Defense Personnel Support Center
ATTN: DPSC-[illegible]
2800 South 20th Street
Philadelphia, PA 19101-8419

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:15Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

(See Instructions – Reverse Side)

1. DOCUMENT NUMBER	2. DOCUMENT TITLE
A-A-53102	ADAPTER, HYPODERMIC NEEDLE-TO-TUBING

3a. NAME OF SUBMITTING ORGANIZATION	4. TYPE OF ORGANIZATION *(Mark one)*
	☐ VENDOR
	☐ USER
b. ADDRESS *(Street, City, State, ZIP Code)*	☐ MANUFACTURER
	☐ OTHER *(Specify)*

5. PROBLEM AREAS

a. Paragraph Number and Wording

b. Recommended Wording

c. Reason/Rationale for Recommendation

6. REMARKS

7a. NAME OF SUBMITTER *(Last, First, MI – Optional)*	b. WORK TELEPHONE NUMBER *(Include Area Code) – Optional*
c. MAILING ADDRESS *(Street, City, State, ZIP Code) – Optional*	8. DATE OF SUBMISSION *(YYMMDD)*

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:15Z
Check the source to verify that this is the current version before use.