A-A-53103A
9 July 1990
SUPERSEDING
A-A-0053103(DM)
30 July 1987

COMMERCIAL ITEM DESCRIPTION

SYRINGE, ASPIRATING

The General Services Administration has authorized the use of this commercial item description.

This commercial item description covers a sterile, disposable, aspirating syringe suitable for the aspirating of mucous from the nose and mouth of premature and newborn infants.

Salient characteristics:

General. The syringe shall be a sterile, disposable aspirating syringe.

Syringes shall be Type I or II as specified (See Note):

Type
I
II

Material. The syringe shall be manufactured entirely from flexible polyvinyl chloride. The syringe shall meet the requirements for Class II plastics as stated in the United States Pharmacopeia (USP).

Style and design. The syringe shall have a tapered tip. The syringe shall have molded flanges designed to provide a secure grip. The tapered tip shall be free from any restrictions or occlusions. The syringe shall meet the dimensional requirements of Figure 1.

AMSC N/A FSC 6515
DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:15Z
Check the source to verify that this is the current version before use.

Physical properties. The polyvinyl chloride used in the manufacture of the syringe shall have the properties shown in Table 1. A sufficient amount of the raw material, which is representative of the lot or batch, shall be used as a sample for testing.

TABLE I

Property	Value	Test Method
Tensile strength, break	1100-1400 psi	ASTM D638
Elongation %, break	450-500	ASTM D638
Tensile modulus 100%	350-400 psi	ASTM D638
Hardness (shore durometer)	55-63A	ASTM D2240

Hardness. Using ASTM Designation D2240, the gage reading shall be made 10 seconds after application of the instrument.

Vacuum test. When tested as specified, the syringe shall draw a vacuum of not less than 760 mm of mercury. Manually evacuate the syringe by compressing the top of the syringe until it touches the opposite wall. Connect the syringe to a mercury manometer and release the syringe. Take the reading once the manometer reaches equilibrium. The vacuum suction pressure shall be not less than 760 mm of mercury.

Accelerated aging test. Preheat an air oven to 140° +\- 4°F prior to placing the sample in the oven. The sample shall be placed in the oven for seven days. The appearance of the sample before and after the aging test shall be noted. The physical properties listed in Table I shall not decrease by more than 25 percent due to the aging test. The vacuum suction pressure shall not be less than 760 mm of mercury as a result of the aging test. The physical properties of the representative polyvinyl chloride sample shall be established prior to performing the accelerated aging test.

Sterilization, safety and freedom from pyrogens. The syringe shall be sterile, free from pyrogens and safe. The syringe shall be tested for sterility, freedom from pyrogens and safety in accordance with the USP.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:15Z
Check the source to verify that this is the current version before use.

Certificates of biocompatiblity. A certificate of compliance, stipulating that offered item meet the biocompatibility test, shall be acceptable, provided that the contractor has supplied acceptable items to the Government within the past three years and that there have been no changes to material formulation and the method of processing since actual testing was performed. The certificate shall include the date the testing was performed, the test method and results, the name and title of the person evaluating the results, the current contract, contract number and NSN, a statement certifying, that the material processing and formulation have not changed since the time that biocompatibility was performed and the signature and title of the person making the certification.

Minimum full time test. Completely aspirate and discharge the syringe with water continously for 10 cycles. On the tenth cycle measure the time to aspirate the syringe. The maximum time required to fill the syringe on the tenth aspiration shall be 2.5 seconds for 2oz. syringe and 3.6 seconds for 3oz. syringes.

Workmanship. The aspirating syringe set shall be free from defects which detract from its appearance or impair its serviceability.

Unit. Package (PG). One package containing fifty syringes of one size only constitutes one unit. Each syringe shall be packaged sterile in s sealed peel-open type container capable of maintaining sterility of contents unless package is damaged or opened.

QUALITY ASSURANCE PROVISIONS.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:15Z
Check the source to verify that this is the current version before use.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means and chemical properties) of the item.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more text characteristics.

Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and as specified herein. The unit of product for test purposes shall be one aspirating syringe. Sampling shall be S-2, AQL 2.5.

Metric products. Products manufactured to metric dimensions will be considered on an equal basis with those manufactured using inch-pound units, providing they fall within the tolerances specified using conversion tables contained in the leastest revision of Federal Standard No. 376, and all other requirements of this document are met.

If a product is manufactured to metric dimensions and those dimensions exceed the tolerances specified in the inch/pound units, a request should be made to the contracting officer to determine if the product is acceptable.

The contracting officer has the option of accepting or rejecting the product.

Contractor certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producers'own drawings, specifications, standards, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:15Z
Check the source to verify that this is the current version before use.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statues, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Federal Acquisition Regulation Subpart 23.4 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

NOTE: The following National Stock Numbers are covered by this document:

NSN	ITEM IDENTIFICATION	TYPE
6515-01-198-0181	SYRINGE, ASPIRATING, Disposable, Plastic, Ear and Ulcer Type, 2 oz.	I
6515-01-256-9688	SYRINGE, ASPIRATING, Newborn Infant, Bulb Type, 3 oz.	II

Ordering data (Intermediate/exterior packaging quantities and labeling and marking must be specified in the contract and/or order).

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:15Z
Check the source to verify that this is the current version before use.

A-A-53103A

MILITARY INTERESTS:

Custodians:

Army - MD
Navy - MS
Air Force - 03

Preparing Activity:

DoD-MB

Agent:


DLA-DM

CIVIL AGENCY COORDINATING ACTIVITIES:

VA-OSS
PHS
FDA-MPQAS

Project No. 6515-4752

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:15Z
Check the source to verify that this is the current version before use.

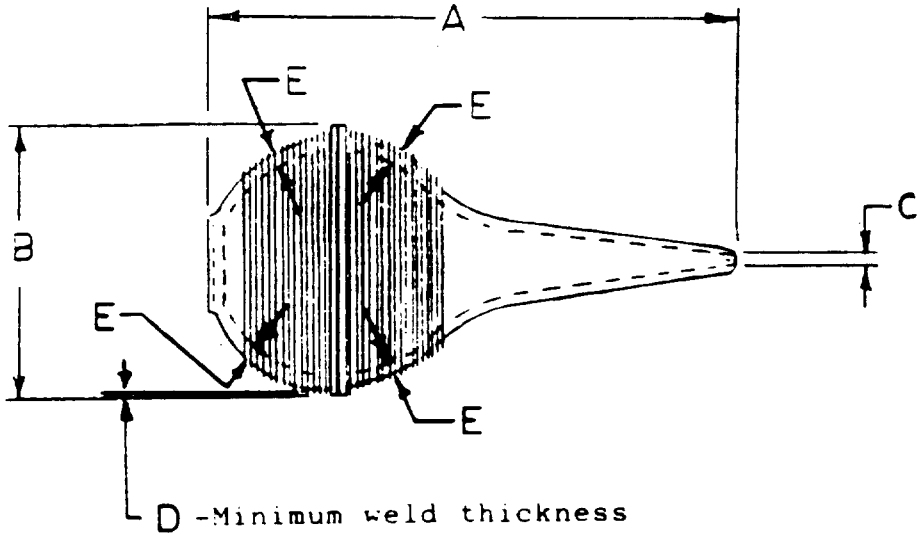

TYPE	NSN	"A" DIM. ± .03	"B" DIM. ± .03	"C" DIM. ± .005	"D" DIM. (Min.)	"E" DIM. ± .005
I	6515-01-198-0181	4.27	2.22	.116	.13	.090
II	6515-01-256-9688	4.95	2.68	.124	.11	.121

Notes:
1. All dimensions are in inches.

FIGURE 1 SYRINGE, ASPIRATING

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:15Z
Check the source to verify that this is the current version before use.