A-A-53105
31 August 1987

# COMMERCIAL ITEM DESCRIPTION

## HOLDER, RADIOGRAPHIC FILM EXPOSURE

The General Services Administration has authorized the use of this commercial item description.

This commercial item description covers an x-ray film exposure holder for use in x-ray procedures.

Salient characteristics:

The radiographic film exposure holder shall be suitable for holding medical x-ray film of the following nominal sizes during exposure:

Size 1 - 8 inches by 10 inches

Size 2 - 10 inches by 12 inches

The holder shall have an outer cover fabricated from one-piece, nonwoven cover stock, with new cotton-rag fibers for a base. The cover shall be impregnated with latex and coated with pyroxylin. The outer cover shall be black and shall be impervious to moisture and stains.

The holder shall have an envelope or insert fabricated from a base stock of a dyed, purified, alpha-cellulose fiber blended with latex and coated with pyroxylin. The envelope shall be black.

The holder shall have a lead backing made of a commercial lead foil having a thickness of not less than 0.004 inch and not more than 0.006 inch. One side of the lead foil shall have suitable backing for resilience.

AMSC N/A FSC 6525

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:15Z
Check the source to verify that this is the current version before use.

The holder construction shall be as illustrated in figure 1. The holder shall consist of an outer cover, an insert or film-holding envelope, and a sheet of lead foil. The holder shall be rectangular in shape and shall be folded in half. Both halves shall be capable of being opened and closed without causing tears or deterioration at the crease in the fold. One side of the outer covering shall be marked "tube side", with a double coated tape. The tape shall hold the insert securely in place, and shall be removable to allow the insert to be replaced, if necessary. The insert shall be creased and folded, and with suitable overlapping shall make a light-tight holder for the film. The lead backing shall be attached to the inside front cover, opposite the envelope on the "tube side". The lead backing shall be secured with a double-coated tape to facilitate easy removal and replacement. The dimensions of the holders in the closed position shall be as follows:

| | Length | Width |
|---|---|---|
| Size 1 - | 10-1/2 inches $^{+1/8\ inch}_{-1/16\ inch}$ | 8-1/2 inches $^{+1/8\ inch}_{-1/16\ inch}$ |
| Size 2 - | 12-1/2 inches $^{+1/8\ inch}_{-1/16\ inch}$ | 10-1/2 inches $^{+1/8\ inch}_{-1/16\ inch}$ |

Each holder shall be permanently and legibly marked with the following information:

a) Manufactures's name or registered trademark.
b) National Stock Number.
c) Contract or purchase order number.
d) Size.
e) The letters U.S.
f) "Tube side".

The proper size radiographic film shall fit flatly and evenly into the film envelope.

All component parts of the holder shall be smoothly, evenly and securely cemented together. The components shall be free of visible cuts or ruptures.

The holder shall be free of bends, rough edges, scuffs, scratches, or dirty areas.

Workmanship. The radiographic film exposure holder shall be free from defects which detract from its appearance or impair its serviceability.



Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:15Z
Check the source to verify that this is the current version before use.

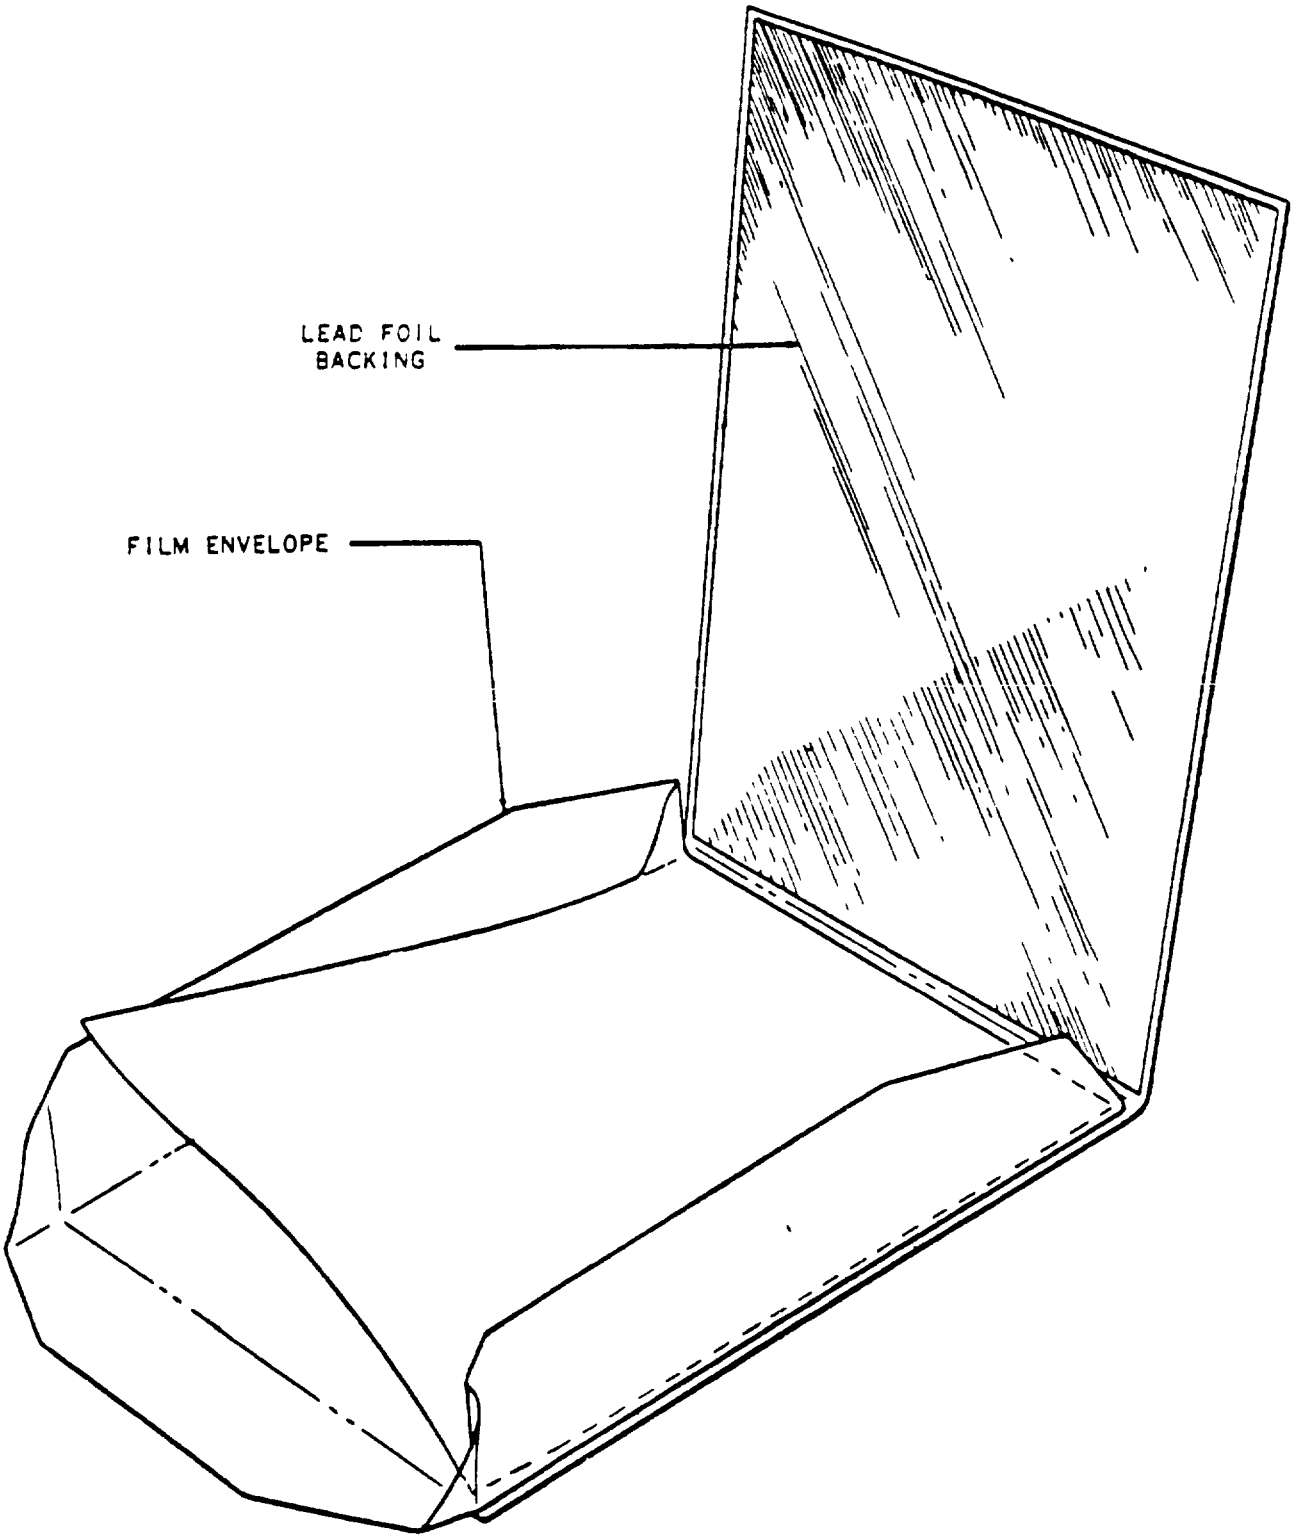



**Figure 1 Radiographic Film Exposure Holder**



Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:15Z
Check the source to verify that this is the current version before use.

Unit. Each (EA). One radiographic film exposure holder, as specified, constitutes one unit.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more test characteristics.

Sampling. Sampling for examination shall be conducted in accordance with MIL-STD-105 and table I. The unit of product for sampling purposes shall be two radiographic film exposure holders as specified in this description.

TABLE I. Sampling for examination.

| | Inspection level | AQL (defects per hundred units) |
|---|---|---|
| For visual examination | | |
| Major defects | II | 1.0 |
| Total defects (Major and minor combined) | II | 4.0 |
| For dimensional examination | S-1 | 2.5 |



Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:15Z
Check the source to verify that this is the current version before use.

Examination. The film exposure holder shall be examined to determine compliance with all requirements contained in this specification.

Classification of defects. Examination shall be conducted in accordance with the classification of defects listed in table II. Examination shall not be restricted to the classified possible defects below.

TABLE II. Classification of Defects.

| Classification | Defect |
|---|---|
| Major | |
| 101 | Any component part missing or unusable. |
| 102 | Envelope not made of correct material. |
| 103 | Envelope not black. |
| 104 | Lead foil thickness not between 0.004 inch and 0.006 inch. |
| 105 | Envelope outer covering not marked "tube side" correctly. |
| 106 | Envelope torn or punctured. |
| Minor | |
| 201 | Envelope not marked as specified (markings other than "tube side"). |
| 202 | Envelope not free of bends, rough edges, scuffs, scratches, or dirty areas. |

Dimensional Examination. The radiographic film exposure holder shall be examined for defects in dimensions. Any dimension not within the specifications herein shall be classified as a defect.

Contractor certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.



Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:15Z
Check the source to verify that this is the current version before use.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Public Law 94-580, as amended, and as implemented by Federal Acquisition Regulation Subpart 23.4 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

NOTE: The following National Stock Numbers are covered by this document:

6525-00-903-8168 (Size 1)
6525-00-903-8172 (Size 2)

Ordering data. Intermediate/exterior package quantities, labeling, and marking must be specified in the contract and/or order.



Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:15Z
Check the source to verify that this is the current version before use.

MILITARY INTERESTS:

Custodians:

Army - MD
Navy - MS
Air Force - 03

PREPARING ACTIVITY:

DoD - MB

Agent:

DLA-DM

CIVIL AGENCY COORDINATING ACTIVITIES:

VA-OSS
PHS
FDA-MPQAS

Project No. 6525-1205

PGC 05106

Location: CID/HOLDER/H13-16



Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:15Z
Check the source to verify that this is the current version before use.

**INSTRUCTIONS:** In a continuing effort to make our standardization documents better, the DoD provides this form for use in submitting comments and suggestions for improvements. All users of military standardization documents are invited to provide suggestions. This form may be detached, folded along the lines indicated, taped along the loose edge *(DO NOT STAPLE)*, and mailed. In block 5, be as specific as possible about particular problem areas such as wording which required interpretation, was too rigid, restrictive, loose, ambiguous, or was incompatible, and give proposed wording changes which would alleviate the problems. Enter in block 6 any remarks not related to a specific paragraph of the document. If block 7 is filled out, an acknowledgement will be mailed to you within 30 days to let you know that your comments were received and are being considered.

*NOTE* This form may not be used to request copies of documents, nor to request waivers, deviations, or clarification of specification requirements on current contracts. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements.

*(Fold along this line)*

*(Fold along this line)*

DEFENSE LOGISTICS AGENCY

NO POSTAGE NECESSARY IF MAILED IN THE UNITED STATES

OFFICIAL BUSINESS
PENALTY FOR PRIVATE USE $300

**BUSINESS REPLY MAIL**
FIRST CLASS PERMIT NO 4068 WASHINGTON D C

POSTAGE WILL BE PAID BY THE DEFENSE LOGISTICS AGENCY

Commander
Defense Personnel Support Center
Attn: DPSC-RSTS
2800 South 20th Street
Philadelphia, PA 19101

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:15Z
Check the source to verify that this is the current version before use.

# STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

*(See Instructions - Reverse Side)*

| 1. DOCUMENT NUMBER | 2. DOCUMENT TITLE |
|---|---|
| A-A 53105 | Holder, Radiographic Film exposure |

| 3a. NAME OF SUBMITTING ORGANIZATION | 4. TYPE OF ORGANIZATION *(Mark one)* |
|---|---|
| | ☐ VENDOR<br>☐ USER<br>☐ MANUFACTURER<br>☐ OTHER *(Specify)* |
| b. ADDRESS *(Street, City, State, ZIP Code)* | |

5. PROBLEM AREAS

a. Paragraph Number and Wording

b. Recommended Wording

c. Reason/Rationale for Recommendation

6. REMARKS

| 7a. NAME OF SUBMITTER *(Last, First, MI)* - Optional | b. WORK TELEPHONE NUMBER *(Include Area Code)* - Optional |
|---|---|
| c. MAILING ADDRESS *(Street, City, State, ZIP Code)* - Optional | 8. DATE OF SUBMISSION *(YYMMDD)* |

DD FORM 82 MAR 1426 PREVIOUS EDITION IS OBSOLETE

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:15Z
Check the source to verify that this is the current version before use.