FEDERAL SPECIFICATION

CHISELS, DENTURE-TRIMMING, LABORATORY

This specification was approved by the Director, Bureau of Federal Supply, for the use of all departments and establishments of the Government.

1. CLASSIFICATION

1.1 Type and classes. — Laboratory denture-trimming chisels covered by this specification shall be of one type and of the following classes, as specified:

Class 1.—With curved shank.
Class 2.—With straight shank.

1.2 Shapes.—The chisels shall be of the shapes shown in figure 1, as specified.

2. APPLICABLE SPECIFICATIONS

2.1 The following Federal Specification, of the issue in effect on date of invitation for bids, forms a part of this specification:

GG–I–526—Instruments, Dental and Surgical; General Specifications.

(Copies of Federal specifications and the Federal Specifications Index may be obtained upon application, accompanied by postal note, money order, coupon, or cash, to the Superintendent of Documents, Government Printing Office, Washington 25, D.C. Prices may be obtained from the Superintendent of Documents.)

2.2 Specifications and other publications applicable only to individual departments are listed in section 7.

3. REQUIREMENTS

3.1 Materials.

3.1.1 *Carbon steel.*—The carbon steel shall conform to the requirements of Federal Specification GG–I–526, class 1, composition E, except that no plating will be required.

3.1.2 *Wood.* — The wood shall be close-grained hardwood.

3.2 Blades and shanks. — The blades and shanks of the chisels shall be of steel. The blades shall be not less than $\frac{1}{20}$ inch in thickness, with the width at the widest part $\frac{9}{32} \pm \frac{1}{32}$ inch. The cutting edge shall be properly shaped, ground to a beveled edge, and sharpened. The shanks shall be $\frac{5}{32} \pm \frac{1}{32}$ inch in diameter. The end of that portion of the shank which is embedded in the handle shall be flattened to approximately $\frac{1}{20}$ inch in thickness by approximately $\frac{1}{8}$ inch in width for a distance of $\frac{1}{4}$ inch from the end, to prevent the blade from turning within the handle.

3.3 Identification marking. — Each chisel shall be legibly and permanently marked on the blade end near the handle with the name or registered trade-mark of the manufacturer.

3.4 Class 1 chisels.

3.4.1 *Design.*—Class 1 chisels shall have curved shanks and mushroom-shaped handles of the general designs shown in figure 1, with the differences in beveling as indicated in shapes A, B, and C.

3.4.2 *Handle.* — The handle for class 1 chisels shall be of close-grained hardwood or other suitable material. It shall be of mushroom shape with flattened side; the mushroom end shall be $1\frac{1}{8} \pm \frac{1}{8}$ inches in diameter. The handle shall be securely attached to the shank and shall have a $\frac{1}{4}$-inch ferrule attached to the distal end. The length of the handle, including ferrule, shall be $2\frac{1}{4} \pm \frac{1}{4}$ inches.

850844—49—(3)

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:50Z
Check the source to verify that this is the current version before use.

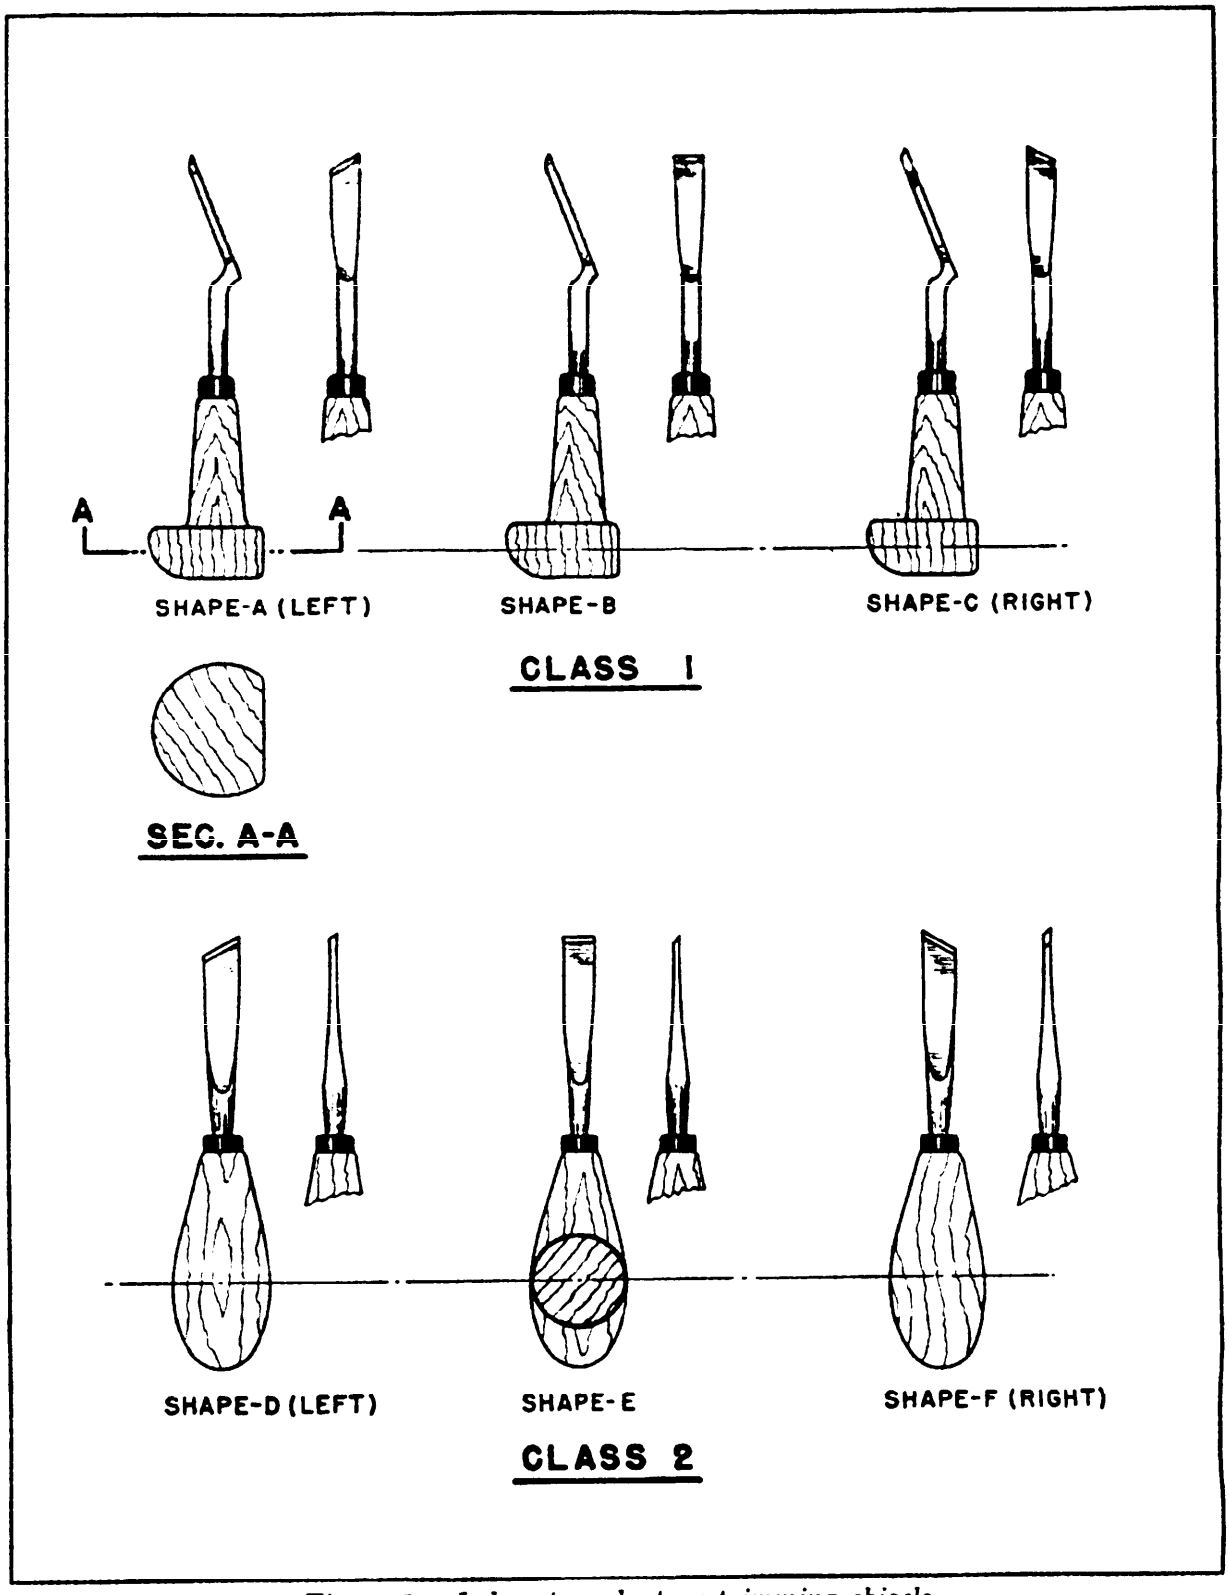


Figure 1.—*Laboratory denture-trimming chisels.*

Source: https://assist.dla.mil -- Downloaded: 202610-26T11:50Z
Check the source to verify that this is the current version before use.

3.4.3 *Over-all length.*—The over-all length of the chisel, including the handle, shall be $4\frac{1}{8} \pm \frac{1}{8}$ inches.

3.5 Class 2 chisels.

3.5.1 *Design.*—Class 2 chisels shall have straight shanks and handles of the general designs shown in figure 1, with the differences in beveling as shown in shapes D, E, and F.

3.5.2 *Handle.* — The handle for class 2 chisels shall be of close-grained hardwood or other suitable material. It shall be well-proportioned and of suitable shape to provide a comfortable hand grip. The handle shall be securely attached to the shank and shall have a ¼-inch ferrule attached to the distal end. The length of the handle, including ferrule, shall be $3\frac{1}{4} \pm \frac{1}{4}$ inches. The diameter of the handle at the largest part shall be approximately $^{23}/_{32}$ inch.

3.5.3 *Over-all length.*—The over-all length of the chisel, including the handle, shall be $5 \pm \frac{1}{2}$ inches.

3.6 **Workmanship.** — Blades and shanks shall be symmetrically made, smoothly and properly finished and polished. Handles shall be smoothly finished. Chisels shall be free from defects which detract from their appearance or which may impair their serviceability.

4. SAMPLING, INSPECTION, AND TEST PROCEDURES

4.1 **Sampling.**—Unless otherwise specified, one chisel of each class and shape shall be taken at random from each lot of 100, or fraction thereof, delivered.

4.2 **Inspection.**—Each sample shall be inspected for material, design, class, shape, construction, dimensions, workmanship, packaging, packing, and marking.

4.3 Tests.

4.3.1 *Carbon steel.*—Tests for hardness of steel shall be made in accordance with the applicable requirements of Federal Specification GG–I–526.

5. PREPARATION FOR DELIVERY

5.1 **Packaging.** — Unless otherwise specified, each chisel shall be packaged in accordance with accepted commercial practice.

5.2 **Packing.** — The subject commodity shall be prepared for shipment to permit acceptance by carrier for transportation at the lowest applicable rate, and to afford maximum protection from normal hazards of transportation.

5.3 Marking.

5.3.1 *Packages.* — Unless otherwise specified, packages shall be marked with the name, class, and shape of the commodity, the quantity contained therein, and the names of the contractor and manufacturer.

5.3.2 *Shipping containers.*—Unless otherwise specified, shipping containers shall be marked with the name, class, and shape of the commodity as defined by the contract or order under which the shipment is made, the quantity contained therein, the name of the contractor, the number of the contract or order, the name and address of the consignee, and the gross weight.

6. NOTES

6.1 **Ordering data.** — Purchasers should specify the class and shape of chisels required, and should exercise any desired options offered herein. (See 1.1, 1.2, 4.1, 5.1, 5.3, and 7.2.5.)

6.2 This specification covers the following items listed in the Army-Navy Catalog of Medical Materiel:

5–147–550 — Chisel, laboratory, left bevel.

5–148–050 — Chisel, laboratory, right bevel.

Source: https://assist.dla.mil -- Downloaded: 202610-26T11:50Z
Check the source to verify that this is the current version before use.

6.3 It is believed that this specification adequately describes the characteristics necessary to secure the desired material, and that normally no samples will be necessary prior to award to determine compliance with this specification. If, for any particular purpose samples with bids are necessary, they should be specifically asked for in the invitation for bids, and the particular purpose to be served by the bid sample should be definitely stated, the specification to apply in all other respects.

6.4 This specification does not include all types, classes, grades, sizes, etc., of the commodity indicated by the title of the specification, or which are commercially available, but is intended to cover the types, etc., which are suitable for Federal Government requirements.

Patent notice.—When Government drawings, specifications, or other data are used for any purpose other than in connection with a definitely related Government procurement operation, the United States Government thereby incurs no responsibility nor any obligation whatsoever; and the fact that the Government may have formulated, furnished, or in any way supplied the said drawings, specifications, or other data, is not to be regarded by implication or otherwise as in any manner licensing the holder or any other person or corporation, or conveying any rights or permission to manufacture, use, or sell any patented invention that may in any way be related thereto.

7. DEPARTMENTAL REQUIREMENTS

7.1 The following specifications and other publications, of the issues in effect on date of invitation for bids, and special requirements, form a part of this specification for purchases made under this specification by the respective departments.

7.2 Army, Navy, and Air Force.

7.2.1 *Applicable specifications and other publications.*—

Federal Specifications:

NN-B-601—Boxes; Wood, Cleated, Plywood, for Domestic Shipment.

NN-B-621 — Boxes; Wood, Nailed and Lock-Corner.

NN-B-631 — Boxes; Wood, Wirebound, for Domestic Shipment.

Military Specifications:

JAN-P-105—Packaging and Packing for Overseas Shipment — Boxes, Wood, Cleated, Plywood.

JAN-P-106—Packaging and Packing for Overseas Shipment — Boxes; Wood, Nailed.

JAN-B-107—Boxes, Wood, Wirebound (Overseas Type).

JAN-P-116—Packaging and Packing for Overseas Shipment — Preservation, Methods of.

JAN-P-120—Packaging and Packing for Overseas Shipment—Cartons, Folding, Paperboard.

JAN-B-121—Barrier-Materials, Greaseproof.

JAN-P-125—Packaging and Packing for Overseas Shipment — Barrier-Materials, Waterproof, Flexible.

JAN-P-133—Packaging and Packing for Overseas Shipment — Boxes; Set-Up, Paperboard.

JAN-P-140—Packaging and Packing for Overseas Shipment — Adhesives, Water-Resistant, Case-Liner.

U. S. Army Specifications:

94-40645—Marking, Exterior, Domestic and Export Shipments by Contractors.[1]

100-2—Standard Specification for Marking Shipments by Contractors.[2]

Navy Department Specifications:

General Specifications for Inspection of Material.[3]

52C18 — Compound, Rust-Preventive, Thin-Film (Polar Type).

Bureau of Supplies and Accounts Publication:

Navy Shipment Marking Handbook.[3]

[1] Applicable only to Air Force purchases.
[2] Applicable only to Army purchases.
[3] Applicable only to Navy purchases.

Source: https://assist.dla.mil -- Downloaded: 202610-26T11:50Z
Check the source to verify that this is the current version before use.

(Copies of specifications required for Army purchases may be obtained upon application to the procuring agency. Both the title and identifying symbol or number should be stipulated when requesting copies.

(Copies of Federal and Military specifications required for Navy purchases, Navy Department specifications, and the Navy Shipment Marking Handbook may be obtained without cost upon application to the Bureau of Supplies and Accounts, Department of the Navy, Washington 25, D. C., except that Naval activities should make application to Supply Officer in Command, Naval Supply Center, Norfolk 11, Virginia. Both the title and identifying symbol or number should be stipulated when requesting copies of specifications.

(Copies of specifications required for Air Force purchases may be obtained upon application to the Commanding General, Air Matériel Command, Wright-Patterson Air Force Base, Dayton, Ohio. Both the title and identifying symbol or number should be stipulated when requesting copies.)

7.2.2 *Cleaning, preservation, and packaging.*

7.2.2.1 *Cleaning.* — Each chisel shall be thoroughly cleaned in accordance with the applicable method outlined in appendix I of Military Specification JAN–P–116.

7.2.2.2 *Preservation.*—Each chisel shall be dipped in rust-preventive, thin-film compound (polar type) conforming to grade III of Navy Department Specification 52C18. Sufficient time (not less than 1 hour) shall be allowed for the compound to set before the unit is wrapped.

7.2.2.3 *Packaging.*

7.2.2.3.1 *Unit packages.*—One chisel of the class and shape specified in the invitation for bids, contract, or order constitutes one unit. Each unit shall be completely wrapped in greaseproof paper conforming to the requirements for grade A of Military Specification JAN–B–121, and packaged in a carton or box of appropriate size conforming to the requirements of Military Specification JAN–P–120 or JAN–P–133. Cartons shall contain sufficient cushioning material to prevent shifting and breakage. The greaseproof wrapper and carton shall be adequately secured to prevent accidental opening.

7.2.2.3.2 *Intermediate packages.*—Twelve units, packaged as specified in 7.2.2.3.1, shall be packaged in a carton of appropriate size and design or shall be completely wrapped in kraft paper of suitable weight. Carton or wrapping shall be adequately secured to prevent accidental opening.

7.2.3 *Packing.*

7.2.3.1 *Domestic.* — Twenty-four intermediate packages (288 units) shall be packed in a shipping container conforming to the requirements of Federal Specification NN–B–601, NN–B–621, or NN–B–631.

7.2.3.2 *Overseas.*—Twenty-four intermediate packages (288 units) shall be packed in a shipping container designed for type 2 load and conforming to the requirements of Military Specification JAN–P–105, JAN–P–106, or JAN–B–107. Closure and strapping shall conform to the requirements of the appendix to the applicable box specification. Each shipping container shall be lined with a sealed waterproof bag, or its equivalent, made from material conforming to the requirements of Military Specification JAN–P–125, for case liners; seams and closures shall be sealed with water-resistant adhesive conforming to the requirements of Military Specification JAN–P–140.

7.2.3.3 *Packing variation permitted.* — If the number of units in any shipment is not the exact multiple of the number of units specified to be contained in each shipping container, the units not constituting the nearest such multiple shall be packed in a shipping container of suitable size and design, so constructed as to insure safe delivery to specified destination.

7.2.4 *Marking.*

7.2.4.1 *Packages.*—Each unit package and each intermediate package shall be marked

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:50Z
Check the source to verify that this is the current version before use.

with the stock number, nomenclature, class, shape, unit, quantity, and the name of the contractor. When the contractor is not the manufacturer, the name of the manufacturer shall also appear.

7.2.4.2 *Shipping containers.*—In addition to the marking specified in 5.3, shipping containers for the Army shall be marked in accordance with the requirements of U. S. Army Specification 100-2; for the Navy, in accordance with the Navy Shipment Marking Handbook; and for the Air Force, in accordance with U. S. Army Specification 94-40645.

7.2.5 *Ordering data* — Requests, requisitions, schedules, and contracts or orders should specify the following: (a) Domestic or overseas packing and marking of shipping containers (see 7.2.3 and 7.2.4); (b) Army, Navy, or Air Force marking of shipping containers (see 7.2.4.2).

NAVY: MS

This specification is a part of Section IV, Part 5, of the Federal Standard Stock Catalog.

For sale by the Superintendent of Documents, Washington 25, D. C. Price 5 cents.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:50Z
Check the source to verify that this is the current version before use.