GG-N-00195B (DSA-DM)
Interim Amendment-3 (DSA-DM)
August 15, 1974
SUPERSEDING
Int. Amendment-2 (DSA-DM)
April 9, 1974 and
Amendment-1
November 7, 1972

FEDERAL SPECIFICATION

NEEDLE, HYPODERMIC, BLOOD COLLECTING, DOUBLE-POINTED, DISPOSABLE, 20 GAUGE

This interim amendment was developed by the Defense Personnel Support Center, 2800 South 20th Street, Philadelphia, PA 19101, based upon currently available technical information. It is recommended that Federal agencies use it in procurement and forward recommendations for changes to the preparing activity at the address shown above. The General Services Administration has authorized the use of this interim amendment as a valid exception to Federal specification GG-N-00195B (DSA-DM).

Page 3

* 3.2.1 Cannula. Delete last sentence and substitute: "Venipuncture point shall be in accordance with GG-N-196, paragraph D-2, except for dimensions which shall be in accordance with Figures 1 and 2."

Page 7

Table II. Under Inspection level for sterility, delete "*" and insert "S-4". Also, delete the asterisked paragraph immediately below Table II.

Page 9

4.4.5 Deformation. Delete and substitute:

"4.4.5 Deformation. Needle shall be subjected to autoclaving for 20 minutes at 15 pounds pressure and 121°C."

FSC 6515

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:49Z
Check the source to verify that this is the current version before use.

Page 13

5.3.2.2 Unit package. Line 10 following "sterile", insert "or similar statement".

Page 16

* Figure 1. Delete venipuncture needle bevel of ".164 ± .016" and substitute ".164 + .039, -.016".

Page 17

* Delete and destroy present page 17, Figure 1, and insert attached page 17, Figure 2. Delete venipuncture needle bevel of ".164 ± .016" and substitute ".164 + .039, -.016".

The margins of this specification are marked with an asterisk to indicate where changes (additions, modifications, corrections, deletions) from the previous issue were made. This was done as a convenience only and the Government assumes no liability whatsoever for any inaccuracies in these notations. Bidders and contractors are cautioned to evaluate the requirements of this document based on the entire content irrespective of the marginal notations and relationship to the last previous issue.

Custodians:
Army - MD
Navy - MS
Air Force - 03

Review activities:
Army - MD
Navy - MS
Air Force - 03

Preparing activity:
Defense Supply Agency - DM

Project No. 6515-1854

Source: https://assist.dla.mil -- Downloaded: 202640-26T11:49Z
Check the source to verify that this is the current version before use.

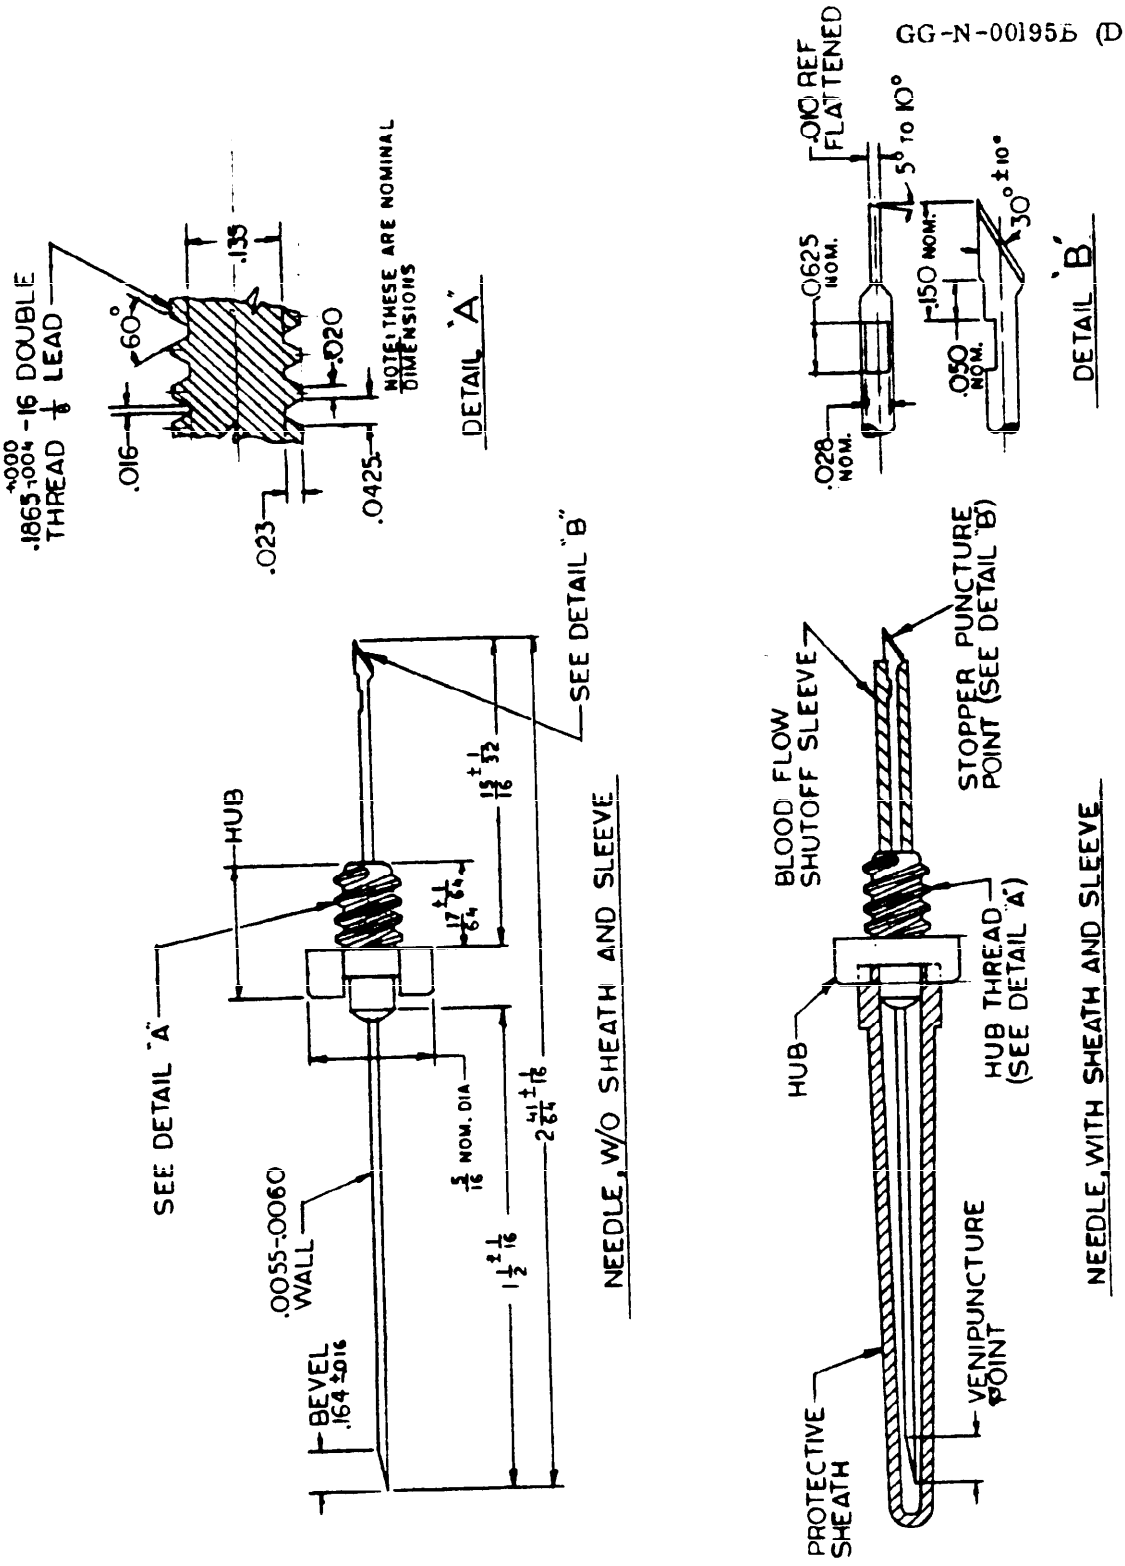


FIGURE 2 - NEEDLE, TYPE II
(WITH SHUTOFF SLEEVE)

Source: https://assist.dla.mil -- Downloaded: 202610-26T11:49Z
Check the source to verify that this is the currentversion before use.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:49Z
Check the source to verify that this is the current version before use.