GG-S-167A
November 17, 1978
SUPERSEDING
GG-S-167
October 13, 1961

FEDERAL SPECIFICATION

SCISSORS, EYE, (IRIS, STRABISMUS, ENUCLEATION AND TENOTOMY)

This specification was approved by the Commissioner, Federal Supply Service, General Services Administration, for the use of all Federal agencies.

1. SCOPE AND CLASSIFICATION

1.1 Scope. This specification covers iris, strabismus, enucleation, and tenotomy scissors for use in surgical procedures on the eye.

1.2 Classification. The eye scissors shall be of the following types and classes as specified (see 6.2).

Type I. Iris.

Class 1. - Straight, 4-1/4 inches.
Class 2. - Full Curved, 4-1/4 inches.
Class 3. - Angular, 4-1/2 inches.

Type II. Strabismus, 4-1/4 inches.

Type III. Tenotomy.

Class 1. - Straight, 4-1/4 inches.
Class 2. - Curved, 4-1/4 inches.

Type IV. Enucleation, 5 inches.

2. APPLICABLE DOCUMENTS

2.1 The following documents, of the issue in effect on date of invitation for bid or request for proposal form a part of this specification to the extent specified herein:

FSC 6515

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:49Z
Check the source to verify that this is the current version before use.

Federal Specifications:

GG-I-526	- Instrument, Dental and Surgical, General Specifications.
ZZ-R-690	- Rubber Dam, Dental.
PPP-B-566	- Boxes, Folding, Paperboard.
PPP-B-636	- Boxes, Shipping, Fiberboard.
PPP-B-676	- Boxes, Setup.

Federal Standards:

Fed. Std. No. 123 - Marking for Shipment (Civil Agencies).

(Activities outside the Federal Government may obtain copies of Federal Specifications, Standards, and Handbooks as outlined under General Information in the Index of Federal Specifications and Standards and at the prices indicated in the Index. The Index, which includes cumulative monthly supplements as issued, is for sale on a subscription basis by the Superintendent of Documents, US Government Printing Office, Washington, DC 20402.

(Single copies of this specification and other Federal Specifications required by activities outside the Federal Government for bidding purposes are available without charge from Business Service Centers at the General Services Administration Regional Offices in Boston, New York, Philadelphia, PA, Washington, DC, Atlanta, Chicago, Kansas City, MO, Fort Worth, Denver, Houston, San Francisco, Los Angeles, and Seattle.

(Federal Government activities may obtain copies of Federal Specifications, Standards, and Handbooks and the Index of Federal Specifications and Standards from established distribution points in their agencies.)

Military Specifications:

MIL-P-116 - Preservation, Methods of.

Military Standards:

MIL-STD-105	- Sampling Procedures and Tables for Inspection by Attributes.
MIL-STD-129	- Marking for Shipment and Storage.

(Copies of Military specifications, standards, and drawings required by contractors in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.)

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:49Z
Check the source to verify that this is the current version before use.

2.2 Other publications. The following documents form a part of this specification to the extent specified herein. Unless otherwise indicated, the issue in effect on date of invitation for bid or request for proposal shall apply.

American Society for Testing and Materials (ASTM).

ASTM E 18	- Rockwell Hardness and Rockwell Superficial Hardness of Metallic Materials.
ASTM E 92	- Vickers Hardness of Metallic Materials.
ASTM E 140	- Standard Hardness Conversion Tables for Metals.

(Application for copies should be addressed to the American Society for Testing and Materials, 1916 Race Street, Philadelphia, PA 19103.)

(Technical society and technical association specifications and standards are generally available for reference from libraries. They are also distributed among technical groups and using Federal agencies.)

3. REQUIREMENTS

3.1 General requirements. The eye scissors shall be in accordance with the applicable requirements of GG-I-526, and as specified herein.

3.2 Material. The eye scissors shall be fabricated from class 4, type 420 material in accordance with the requirements of GG-I-526 except that the carbon content shall be 0.30 percent minimum. As an alternate, the chromium content shall be 12 to 15 percent and the phosphorus content shall be 0.045 percent maximum.

3.3 Hardness. After proper stress relieving the eye scissors shall exhibit a Rockwell hardness of C50 to C55, except for the screw, when tested as specified in 4.4.1.

3.4 Style, designs and dimensions. The eye scissors shall be of the style, design and dimensions specified herein. All types and classes shall be suitable for fine surgical procedures of the eye.

3.4.1 Type I. The type I eye scissors shall consist of the following classes:

3.4.1.1 Class 1. The class 1 scissors shall have straight, sharp pointed blades. The style, design and dimensions shall be in accordance with figure 1.

3.4.1.2 Class 2. The class 2 scissors shall have curved, sharp pointed blades. The style, design and dimensions shall be in accordance with figure 1.

3.4.1.3 Class 3. The class 3 scissors shall have angular, probe tipped blades. The style, design and dimensions shall be in accordance with figure 2.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:49Z
Check the source to verify that this is the current version before use.

3.4.2 Type II. The type II scissors shall be of one type and class. The type II scissors shall have straight blades with slightly radiused tips. The style, design and dimensions shall be in accordance with figure 3.

3.4.3 Type III. The type III scissors shall consist of the following classes.

3.4.3.1 Class 1. The class 1 scissors shall be tenotomy scissors of the Stevens design, having straight blades with blunt tips. The style, design and dimensions shall be in accordance with figure 4.

3.4.3.2 Class 2. The class 2 scissors shall be tenotomy scissors of the Stevens design having curved blades with blunt tips. The style, design and dimensions shall be in accordance with figure 4.

3.4.4 Type IV. The type IV scissors shall be of one type and class. The scissors shall have curved blades with blunt tips. The style, design and dimensions shall be in accordance with figure 5.

3.5 Finish. The scissors shall have a mirror finish except for the inside of the blades which shall be crocus.

3.5.1 Passivation. The entire scissors shall be properly passivated.

3.6 Scissors performance. The scissors, when tested as specified in 4.4.2, shall cut a continuous length of the test material for the minimum length indicated in table I for the appropriate type and class. The cutting requirement shall apply to the entire length of cut specified including the tips.

TABLE I. Length of cut

Type	Class	Length of cut (inches)
I	1	3/8
I	2	3/8
I	3	1/2
II	-	1/2
III	1	3/8
III	2	3/8
IV	-	1

3.7 Identification. In addition to GG-I-526 requirements, scissors of foreign manufacture shall also be marked "stainless".

3.8. Dimensional tolerances. Unless otherwise specified, the tolerance for the linear dimensions specified in figures 1 through 5 shall be plus or minus 1/64 inch.

3.9 Workmanship. The scissors shall be free from cracks, burrs, pits, rough areas, scale and corrosion and any other defects which detract from their appearance or impair their serviceability.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:49Z
Check the source to verify that this is the current version before use.

4. QUALITY ASSURANCE PROVISIONS

4.1 Responsibility for inspection. Unless otherwise specified in the contract, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract, the contractor may use his own or any other facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

4.1.1 Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government, upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

4.1.2 Inspection. Inspection, as used in this specification, is defined as both examination (such as visual and auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

4.1.3 Certificates of quality. Certificates of quality, supplied by the manufacturer of the martensitic steel, may be furnished in lieu of actual performance of such testing by the contractor, provided lot identity has been maintained and can be demonstrated to the Government. The certificate shall include the name of the contractor, the contract number, the name of the manufacturer or supplier, the National Stock Number (NSN), the item identification, the name of the component/material, the lot number, the lot size, the sample size, the date of testing, the test method, individual test results, and the specification requirements.

4.2 Sampling.

4.2.1 For examination. Sampling for examination shall be conducted in accordance with MIL-STD-105 and as indicated in table II. The unit of product for examination purposes shall be one eye scissors.

TABLE II. Sampling for examination

Type defect	Inspection level	AQL (percent defective)
Major	II	1.0
Minor	II	2.5

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:49Z
Check the source to verify that this is the current version before use.

4.2.2 For tests. Sampling for test shall be conducted in accordance with MIL-STD-105 and as indicated in table III. The unit of product for test purposes shall be one eye scissors. Where feasible, the same sample unit shall be used for the determination of two or more test characteristics.

TABLE III. Sampling for tests

Component	Characteristics	Requirement	Test procedure	Inspection level	AQL (percent defective)
Eye scissors	Hardness	3.3	4.4.1	S-2	1.5
	Dimensions	3.4	-	S-2	2.5
	Copper sulfate test	GG-I-526	GG-I-526	S-2	1.0
	Boil test	GG-I-526	GG-I-526	S-2	1.0
	Performance	3.6	4.4.2	II	1.0

4.2.3 Composition analysis. A sufficient quantity of each lot of metal used in the manufacture of the eye scissors shall be selected for composition analysis in accordance with GG-I-526.

4.3 Examination.

4.3.1 Eye scissors. The eye scissors shall be examined to determine compliance with specification requirements. Examination shall be conducted in accordance with tables II and IV. Examination, however, shall not be restricted to defects listed in table IV.

TABLE IV. Classification of defects

Categories	Defects
Critical	None defined.
Major:	
101	Scissors not type or class specified.
102	Cutting action of scissors not free of excessive stiffness.
103	Screw in lock not permanently set.
104	Cutting edges not free of nicks, feathers, or burrs.
105	Surfaces of scissors not free of pits, corrosion, discoloration, or plating.
106	Scissors not free of cracks.
107	Scissors surfaces not free of burrs, sharpness (except cutting edges) or roughness.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:49Z
Check the source to verify that this is the current version before use.

TABLE IV. Classification of defects (Cont'd)

Categories	Defects
Minor:	
201	Finish not mirror and crocus as specified.
202	Finish not free of course grind marks or excessive scratched surface areas.
203	Identification marking not permanent, legible or complete.

4.3.2 Examination of preparation for delivery. An examination shall be made to determine compliance with the packaging, packing and marking requirements of section 5. Defects shall be scored as specified in table V. Sampling shall be in accordance with MIL-STD-105. The sample unit shall be one container fully prepared for delivery. The lot shall be the number of containers offered for inspection at one time. The inspection level shall be S-2 with an AQL of 4.0 expressed in terms of percent defective.

TABLE V. Examination of preparation for delivery

Examine	Defect
Contents	Not as specified.
Container	Not as specified.
Marking	Omitted; incorrect; illegible; improper size, location, sequence or method of application.
Material	Component missing or damaged.
Workmanship	Bulging or distortion of containers.

4.3.2.1 Examination of closure, waterproofing and banding of container. When the container is required to comply with PPP-B-566, PPP-B-636, or PPP-B-676 the examination for defects in closure, waterproofing or banding shall be in accordance with the appendix of the appropriate box specification.

4.4 Tests. Tests shall be conducted to determine compliance with specification requirements.

4.4.1 Hardness test. Hardness shall be determined in accordance with ASTM E 18 or ASTM E 92. Conversion of Vickers hardness values into Rockwell values shall be in accordance with ASTM E 140.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:49Z
Check the source to verify that this is the current version before use.

4.4.2 Scissors performance test. The test material shall be dental rubber dam type I, size 1, per ZZ-R-690. Scissors to be tested shall be cleaned prior to test. Three separate, consecutive tests shall be performed with each scissors. Each test shall consist of making one cut through one thickness of rubber dam. Each cut shall be made using the scissors in the normal manner, i.e., with the examiner's fingers in the finger rings of the instrument, except that no lateral pressure shall be exerted.

5. PREPARATION FOR DELIVERY

5.1 Preservation-packaging. Preservation-packaging shall be level A or C as specified (see 6.2).

5.1.1 Level A.

5.1.1.1 Cleaning. Scissors shall be cleaned in accordance with MIL-P-116, process C-1.

5.1.1.2 Drying. Scissors shall be dried in accordance with MIL-P-116.

5.1.1.3 Preservative application. Preservatives shall not be used.

5.1.1.4 Unit packaging. Each pair of scissors shall be packaged in accordance with MIL-P-116, method IC-1.

5.1.1.5 Intermediate package. Six unit packages containing scissors of one type and class only shall be packaged in a box conforming to PPP-B-566, or PPP-B-676. Closure shall be as specified in the appendix of the applicable box specification.

5.1.2 Level C. Scissor shall be clean, dry and individually packaged in a manner that will afford adequate protection against corrosion, deterioration and physical damage during shipment from the supply source to the first receiving activity.

5.2 Packing. Packing shall be level A, B or C as specified (see 6.2).

5.2.1 Level A. Forty-eight intermediate packages (288 units) containing scissors of one type and class only shall be packed in a shipping container designed for a type 2 load and conforming to PPP-B-636, class weather-resistant. Closure, banding and waterproofing shall be as specified in the box specification.

5.2.2 Level B. Forty-eight intermediate packages (288 units) shall be packed in a shipping container designed for a type 2 load and conforming to PPP-B-636, class domestic. Closure shall be as specified in the appendix of the box specification.

5.2.3 Level C. The packaged scissors shall be packed in a manner that will afford adequate protection against damage during direct shipment from the supply source to the first receiving activity. These packs shall conform to the applicable carrier's rules and regulations.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:49Z
Check the source to verify that this is the current version before use.

5.3 Marking.

5.3.1 Interior packages. Each unit and intermediate package shall be marked as specified in MIL-STD-129. Contract or purchase order number and name of contractor shall be shown.

5.3.2 Exterior container. Exterior containers shall be marked as specified in MIL-STD-129.

6. NOTES

6.1 Intended use. The scissors covered by this specification are intended for use in fine surgical operative procedures.

6.2 Ordering data. The procurement document should specify the following:


(a) Title, number, and date of this specification.
(b) Type and class (see 1.2).
(c) Selection of applicable levels of packaging and packing (see 5.1 and 5.2).
(d) If marking shall be in accordance with Fed. Std. 123 or MIL-STD-129 (see 5.3).
(e) National stock number (NSN).

6.3 National stock number. This specification covers the following items appearing in the Federal Supply Catalog:

National stock number	Item identification
6515-00-364-2800	SCISSORS, Enucleation, Curved, 5 inch.
6515-00-364-4200	SCISSORS, Iris, Angular, 4-1/2 inch.
6515-00-364-4600	SCISSORS, Iris, Full Curved, 4-1/4 inch.
6515-00-364-4800	SCISSORS, Iris, Straight, 4-1/4 inch.
6515-00-365-5200	SCISSORS, Strabismus, Straight, 4-1/4 inch.
6515-00-365-6200	SCISSORS, Tenotomy, Curved, Stevens, 4-1/4 inch.
6515-00-365-6300	SCISSORS, Tenotomy, Straight, Stevens, 4-1/4 inch.

6.4 Changes from previous issue. Asterisks are not used in this revision to identify changes with respect to previous issue due to the extensiveness of the changes.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:49Z
Check the source to verify that this is the current version before use.

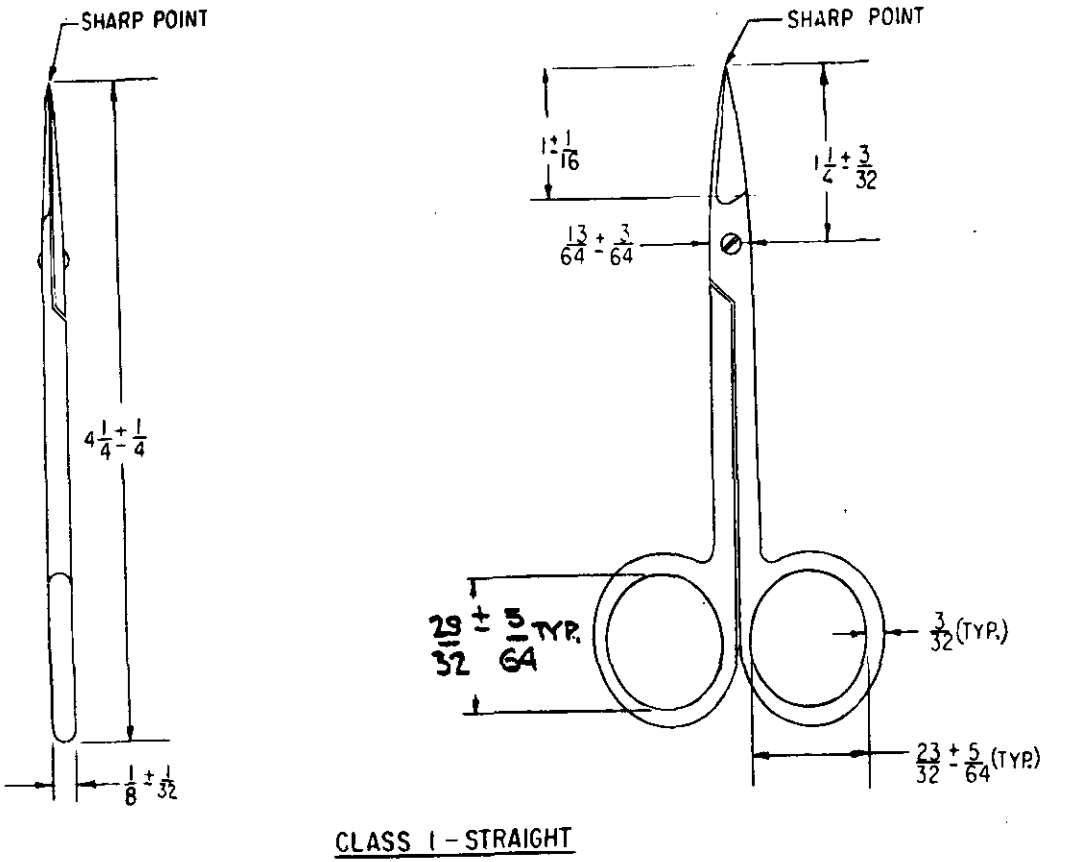


CLASS 1 – STRAIGHT


CLASS 2 - CURVED

NOTE
ALL DIMENSION ARE IN INCHES.

FIGURE 1. Scissors, iris.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:49Z
Check the source to verify that this is the current version before use.

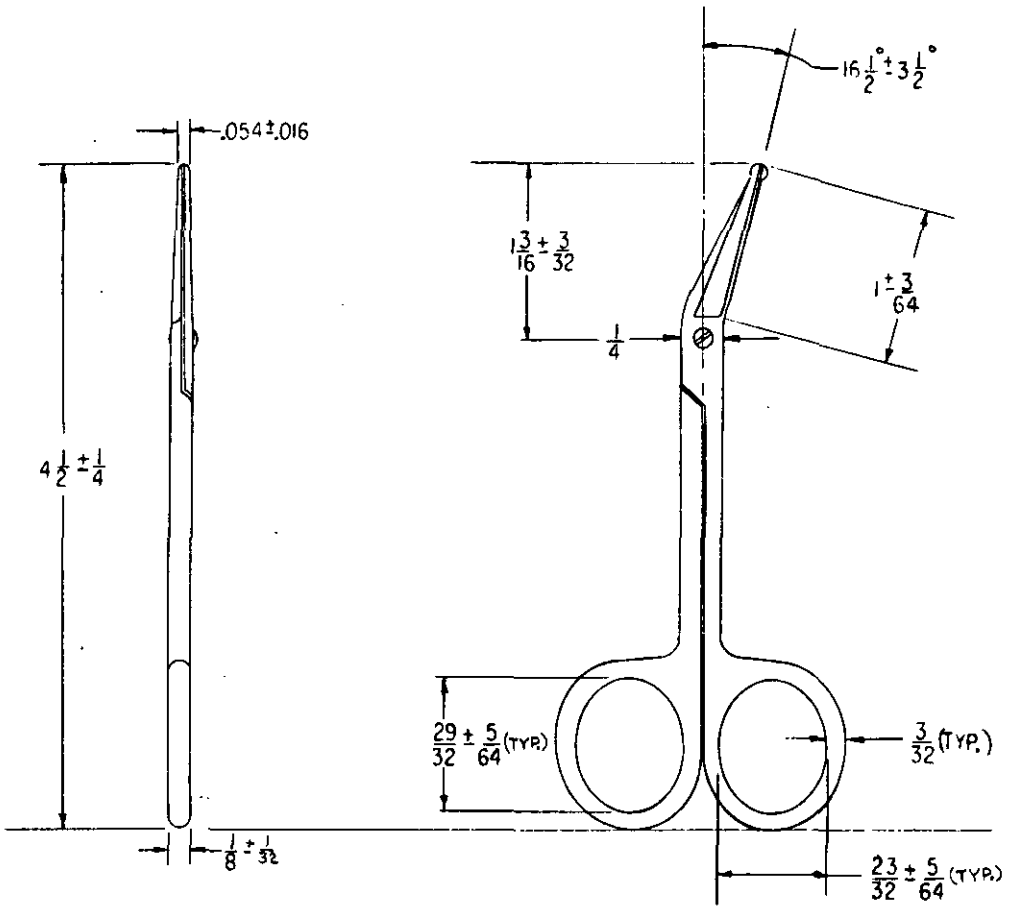


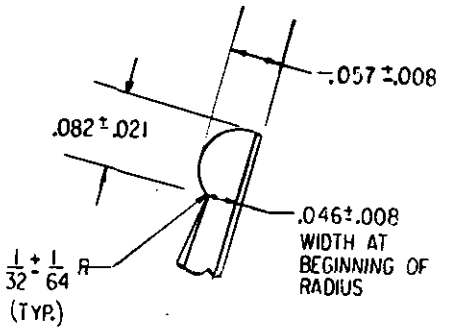

DETAIL A

PROBE

TYPICAL BOTH BLADES

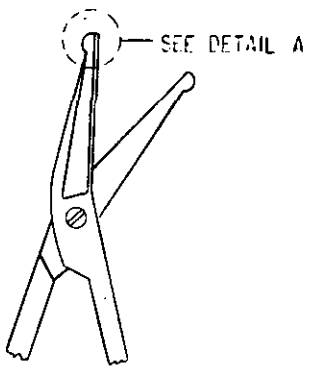


NOTE

ALL DIMENSIONS ARE IN INCHES.

FIGURE 2. Scissors, iris, angular.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T14:49Z
Check the source to verify that this is the current version before use.

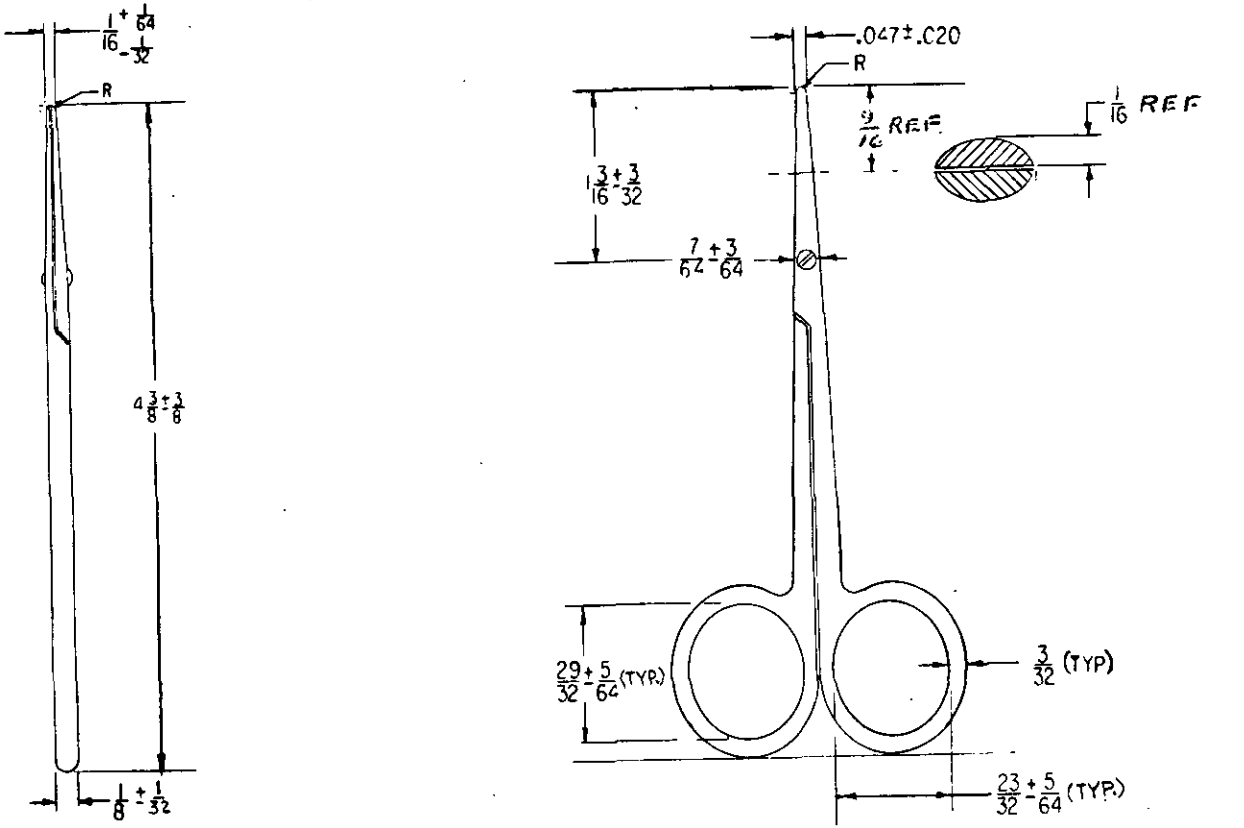

NOTE:
ALL DIMENSION ARE IN INCHES.

FIGURE 3. Scissors, strabismus, straight.

Source: https://assist.dla.mil - Downloaded: 2026-10-20T14:49:49Z
Check the source to verify that this is the current version before use.

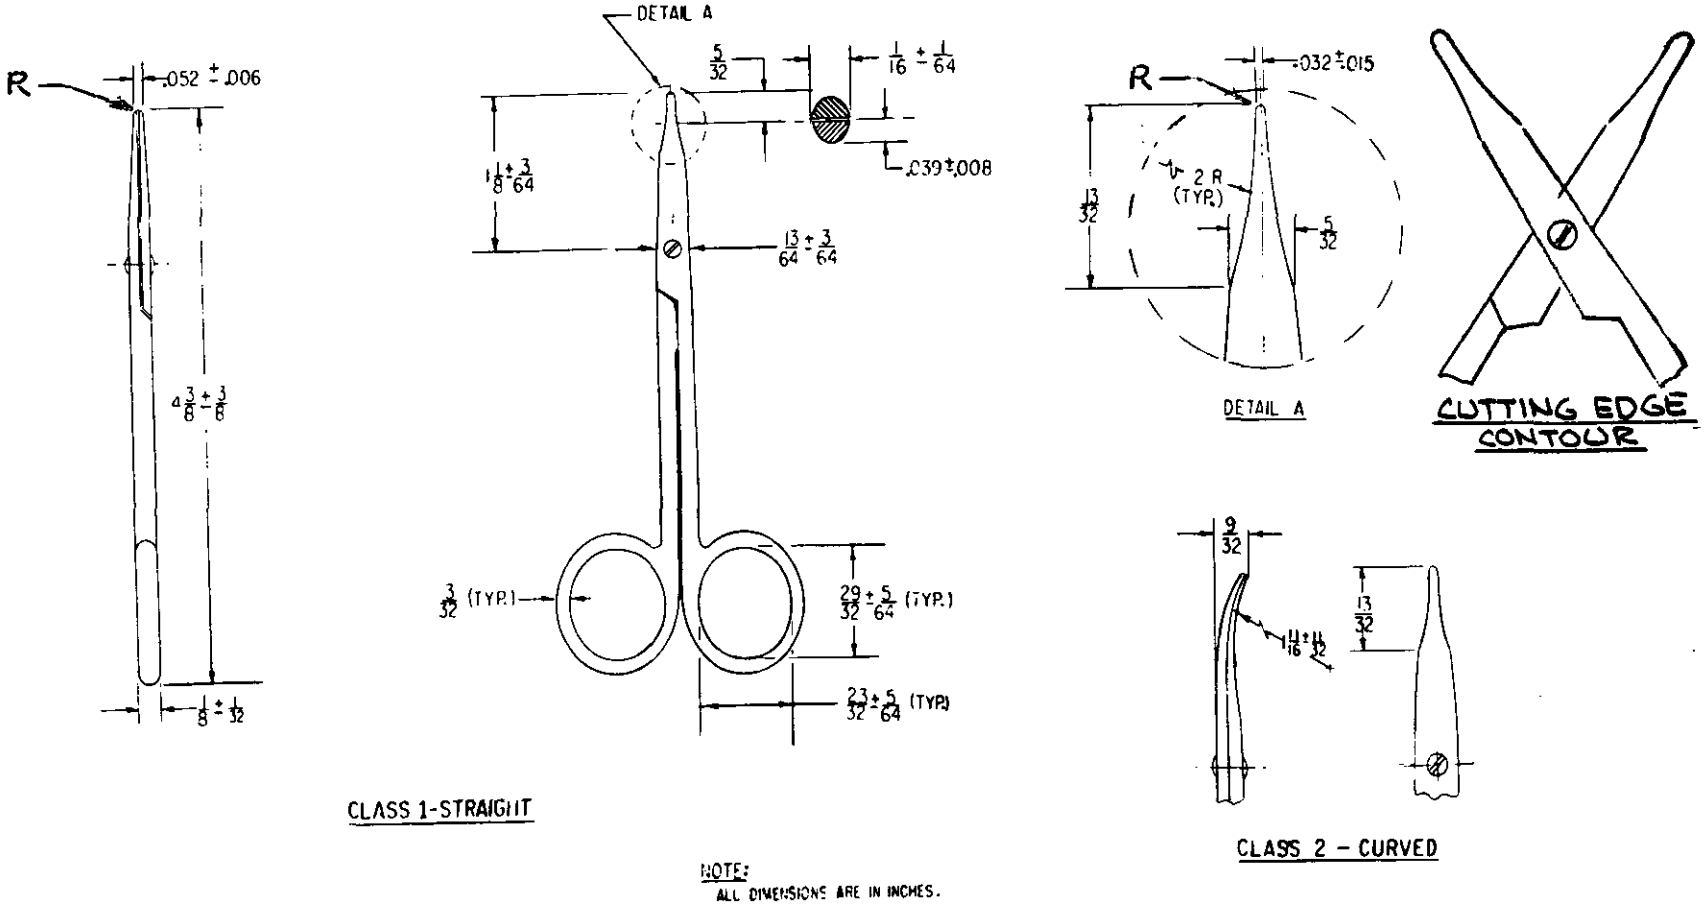


FIGURE 4. Scissors, tenotomy, Stevens.

GG-S-167A

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:49Z
Check the source to verify that this is the current version before use.

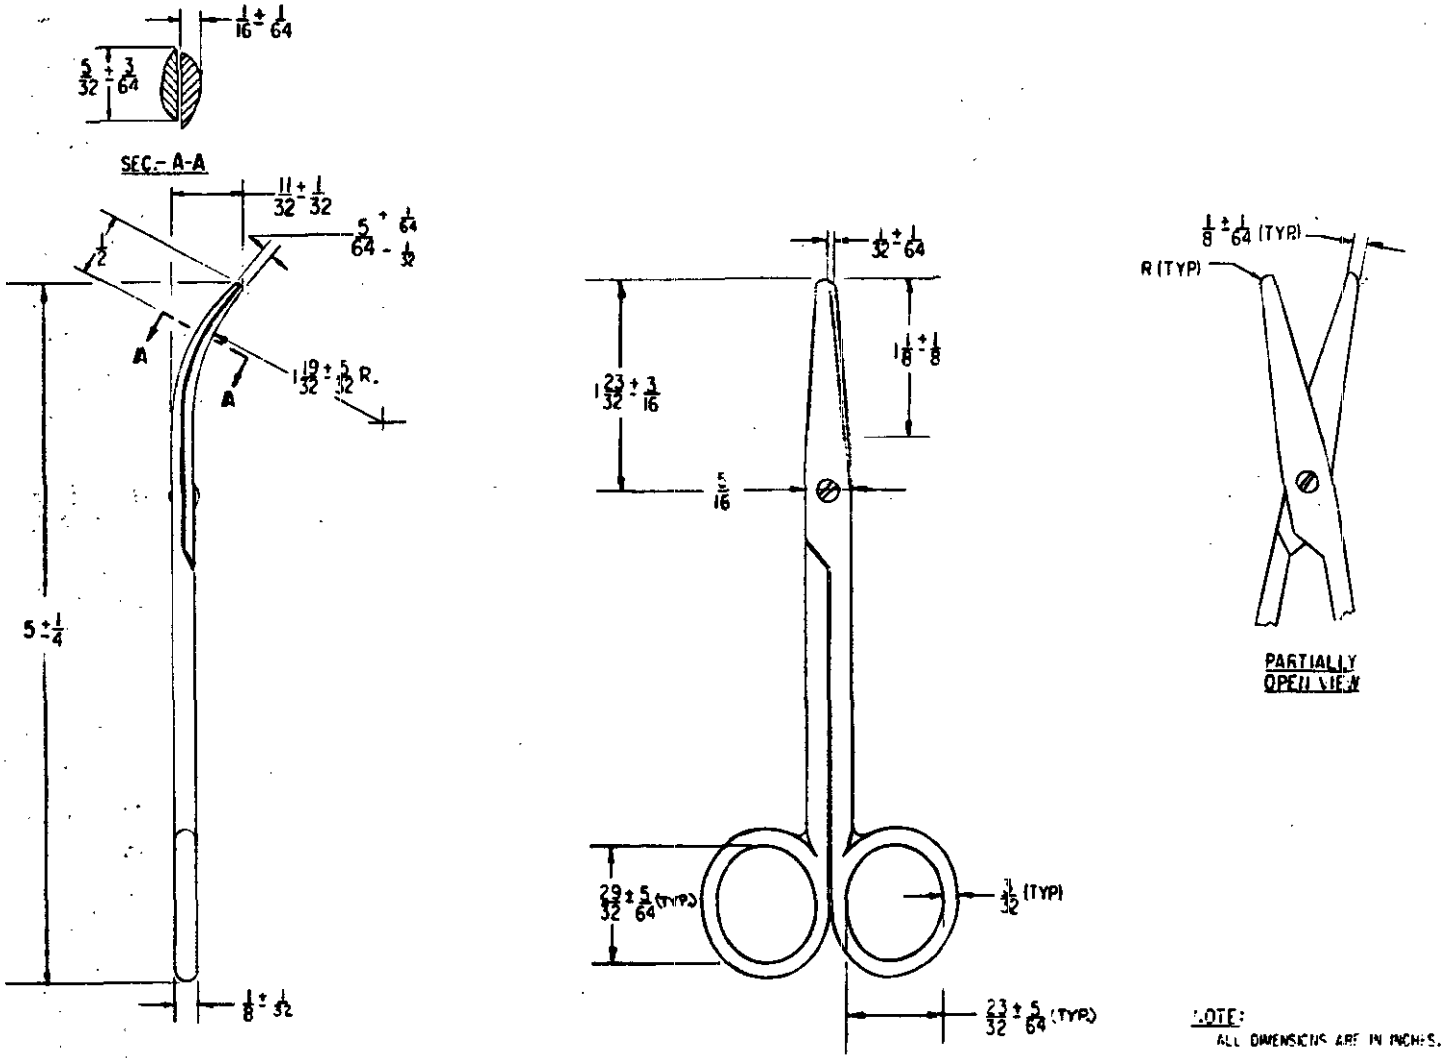


FIGURE 5. Scissors, enucleation, curved.

Source: https://assist.dla.mil -- Downloaded: 2026-10-30 15:49:49
Check the source to verify that this is the current version before use.

MILITARY CUSTODIANS:
Army - MD
Navy - MS
Air Force - 03

Review activity:
DoD - MB

Preparing activity:
DLA-DM

Civil Agency Coordinating Activities:
GSA-FSS
HEW-HSM
VA-DMS

Project No. 6515-2059

Orders for this publication are to be placed with the General Services Administration, acting as an agent for the Superintendent of Documents. See Section 2 of this specification to obtain extra copies of documents referenced herein.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:49Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

INSTRUCTIONS: This form is provided to solicit beneficial comments which may improve this document and enhance its use. DoD contractors, government activities, manufacturers, vendors, or other prospective users of the document are invited to submit comments to the government. Fold on lines on reverse side, staple in corner, and send to preparing activity. Attach any pertinent data which may be of use in improving this document. If there are additional papers, attach to form and place both in an envelope addressed to preparing activity. A response will be provided to the submitter, when name and address is provided, within 30 days indicating that the 1426 was received and when any appropriate action on it will be completed.
NOTE: This form shall not be used to submit requests for waivers, deviations or clarification of specification requirements on current contracts. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements.

DOCUMENT IDENTIFIER *(Number)* AND TITLE

GG-S-167A SCISSORS, EYE, (IRIS, STRABISMUS, ENUCLEATION AND TENOTOMY)

NAME OF ORGANIZATION AND ADDRESS OF SUBMITTER

☐ VENDOR ☐ USER ☐ MANUFACTURER

1. ☐ HAS ANY PART OF THE DOCUMENT CREATED PROBLEMS OR REQUIRED INTERPRETATION IN PROCUREMENT USE? ☐ IS ANY PART OF IT TOO RIGID, RESTRICTIVE, LOOSE OR AMBIGUOUS? PLEASE EXPLAIN BELOW.

A. GIVE PARAGRAPH NUMBER AND WORDING

B. RECOMMENDED WORDING CHANGE

C. REASON FOR RECOMMENDED CHANGE(S)

2. REMARKS

SUBMITTED BY *(Printed or typed name and address — Optional)*

TELEPHONE NO.

DATE

DD FORM 1 OCT 76 1426

EDITION OF 1 JAN 72 WILL BE USED UNTIL EXHAUSTED.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:49Z
Check the source to verify that this is the current version before use.